

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120325\
 Data File : PS032585.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2025 14:10
 Operator : AR\AJ
 Sample : Q3733-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 15:18:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120325.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 03 13:46:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.021	7.383	305.6E6	239.6E6	55.322	44.700
Target Compounds							
1) T	Dalapon	0.000	2.472	0	1835.3E6	N.D.	251.452
2) T	3,5-DICHL...	6.234	6.385	7165422	32388690	<MDL	5.302 #
5) T	DICAMBA	7.200	7.569	241.8E6	35853670	10.881	1.807 #
6) T	MCP	7.318f	7.665	1729848	11430386	<MDL	<MDL #
7) T	MCPA	7.524	7.908	223.1E6	135.1E6	13.799	8.135 #
8) T	DICHLORPROP	7.874	8.318f	39550776	202.0E6	7.338	40.659 #
9) T	2,4-D	8.104f	8.629	96714071	14918727	15.840	2.656 #
10) T	Pentachlo...	8.398	9.127f	105.8E6	42310237	1.443	<MDL #
11) T	2,4,5-TP ...	9.011f	9.492	4508.1E6	1121.2E6	134.916	39.083 #
13) T	2,4-DB	9.858	10.463	68312294	309.0E6	21.901	75.850 #
14) T	DINOSEB	10.985	10.858	1311.3E6	273.8E6	47.552	15.140 #
15) T	Picloram	0.000	11.980	0	139.4E6	N.D.	3.874
16) T	DCPA	11.267f	0.000	1799.5E6	0	44.912	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120325\
Data File : PS032585.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2025 14:10
Operator : AR\AJ
Sample : Q3733-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 15:18:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120325.M
Quant Title : 8080.M
QLast Update : Wed Dec 03 13:46:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

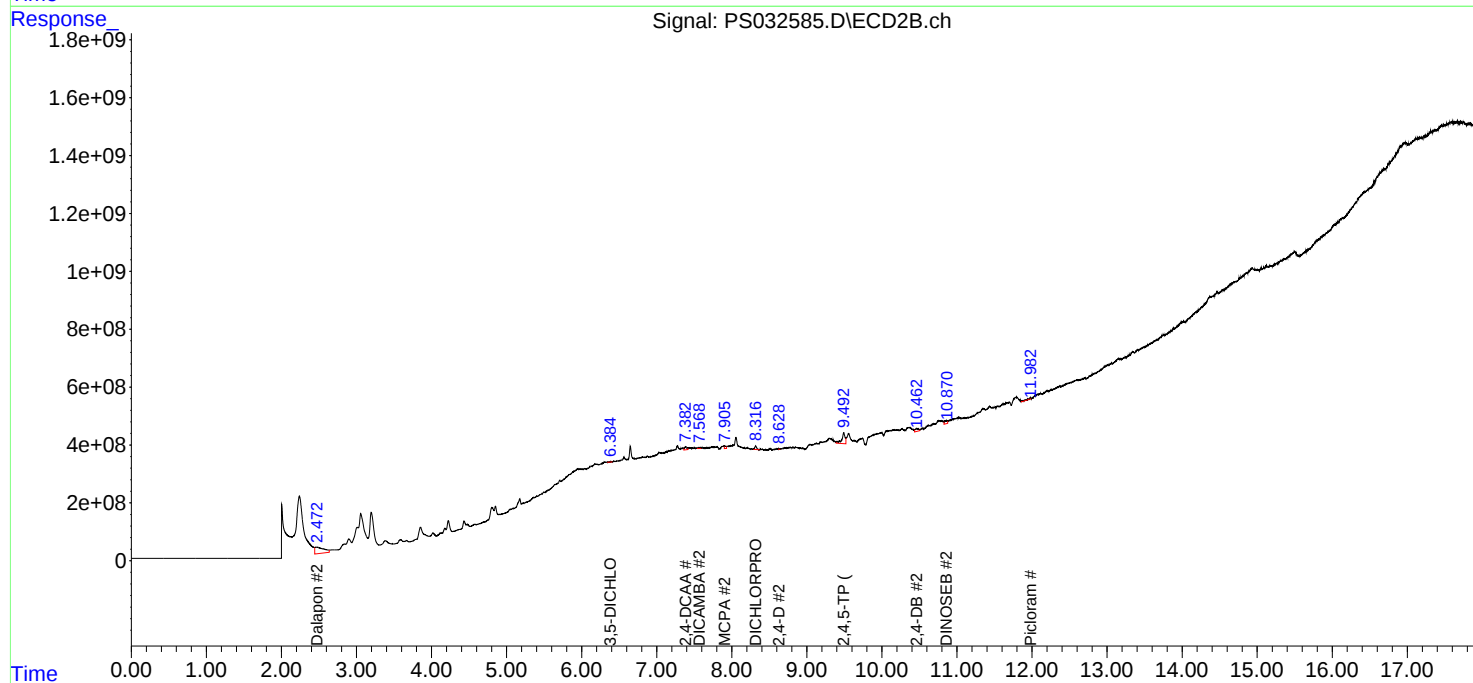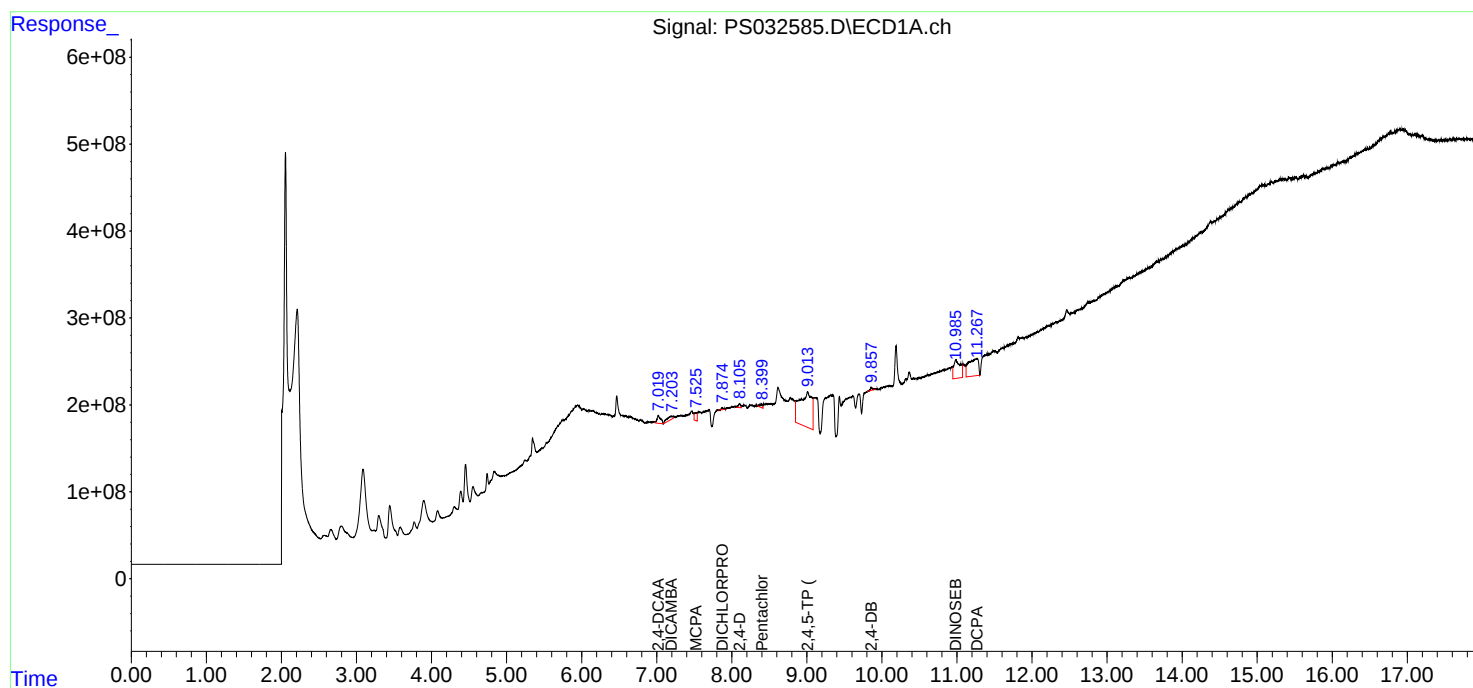


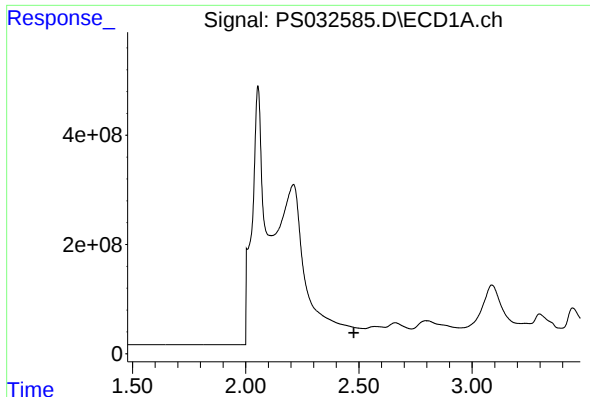

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.478 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

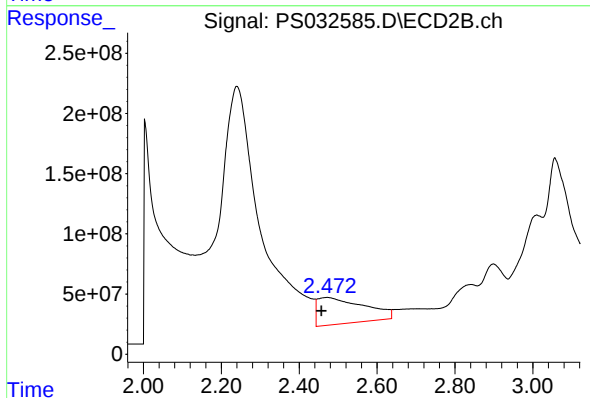


#1 Dalapon

R.T.: 2.472 min
Delta R.T.: 0.015 min
Response: 1835330519
Conc: 251.45 ng/ml

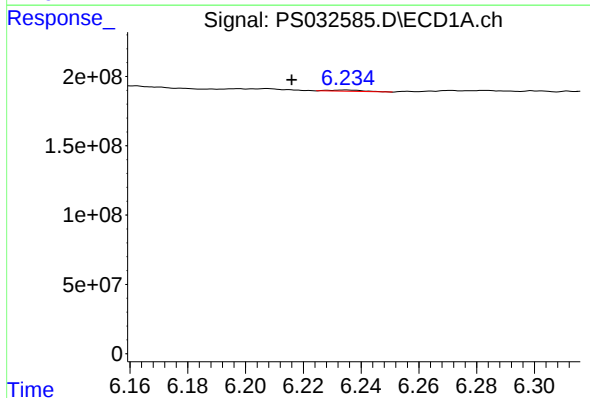


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.234 min
Delta R.T.: 0.018 min
Response: 7165422
Conc: N.D.

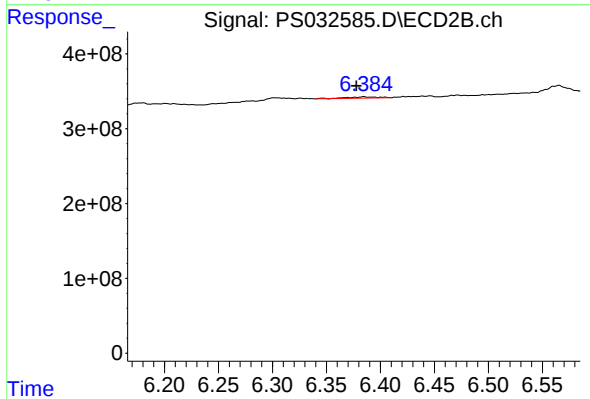

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.385 min
Delta R.T.: 0.007 min
Response: 32388690
Conc: 5.30 ng/ml

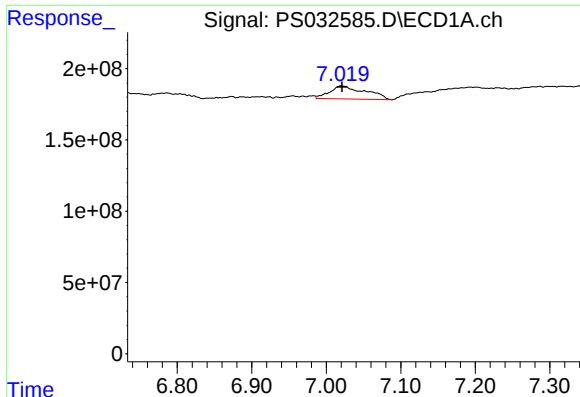

#4 2,4-DCAA


R.T.: 7.021 min
Delta R.T.: 0.000 min
Response: 305578691
Conc: 55.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

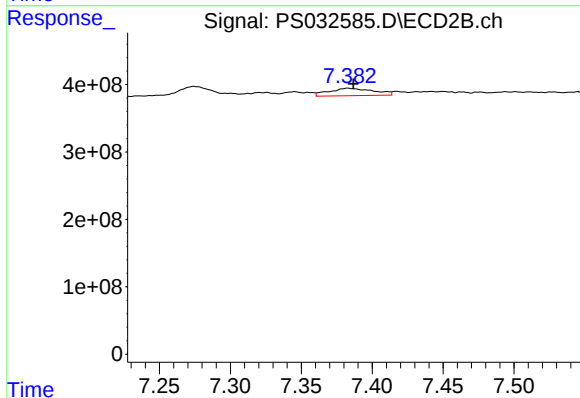


#4 2,4-DCAA

R.T.: 7.383 min
Delta R.T.: -0.003 min
Response: 239647936
Conc: 44.70 ng/ml

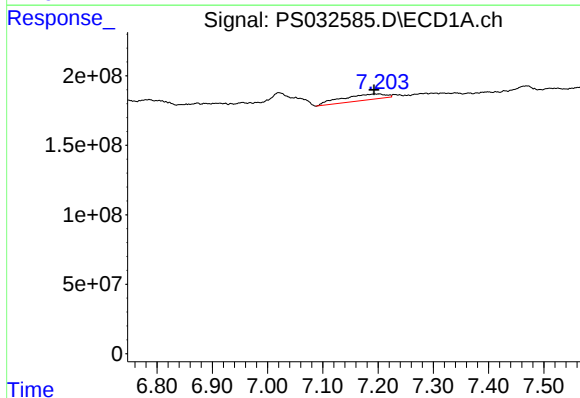


#5 DICAMBA

R.T.: 7.200 min
Delta R.T.: 0.007 min
Response: 241754267
Conc: 10.88 ng/ml

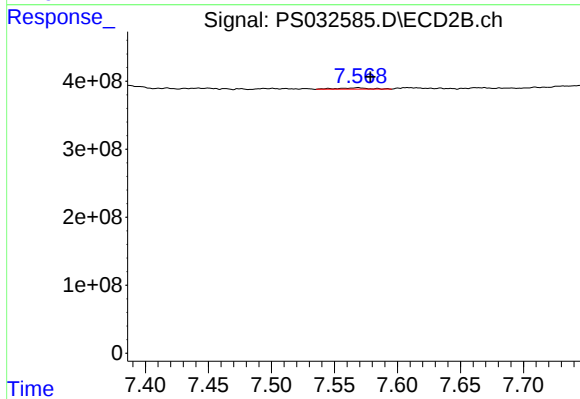

#5 DICAMBA


R.T.: 7.569 min
Delta R.T.: -0.010 min
Response: 35853670
Conc: 1.81 ng/ml

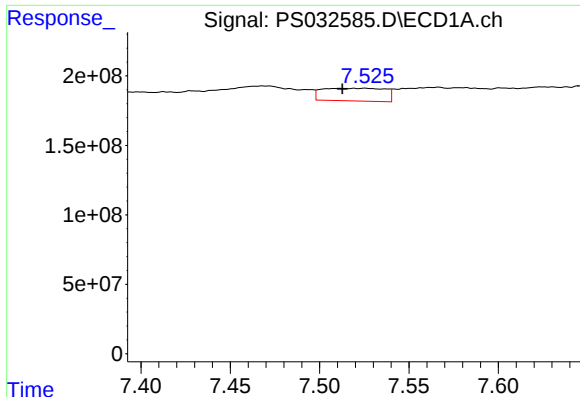

#7 MCPA


R.T.: 7.524 min
Delta R.T.: 0.011 min
Response: 223118190
Conc: 13.80 ug/ml

Instrument :
ECD_S
ClientSampleId :

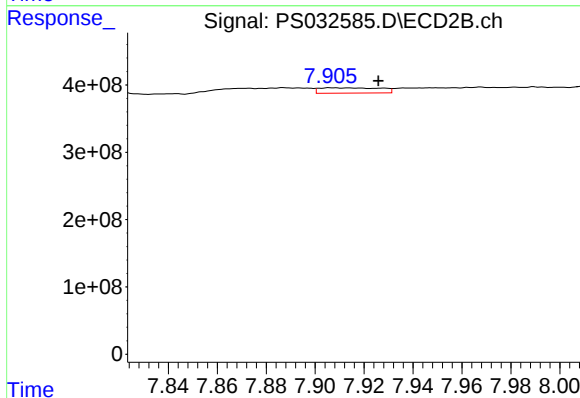


#7 MCPA

R.T.: 7.908 min
Delta R.T.: -0.018 min
Response: 135087638
Conc: 8.14 ug/ml

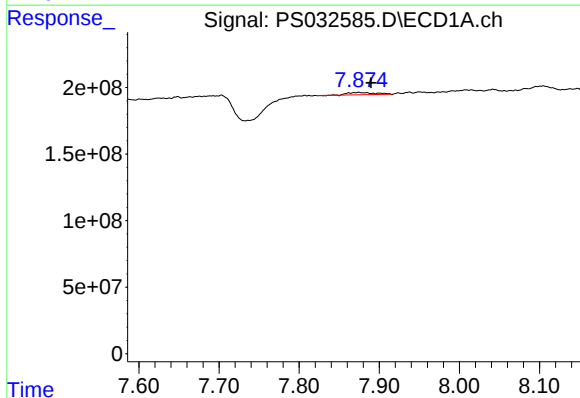


#8 DICHLORPROP

R.T.: 7.874 min
Delta R.T.: -0.016 min
Response: 39550776
Conc: 7.34 ng/ml

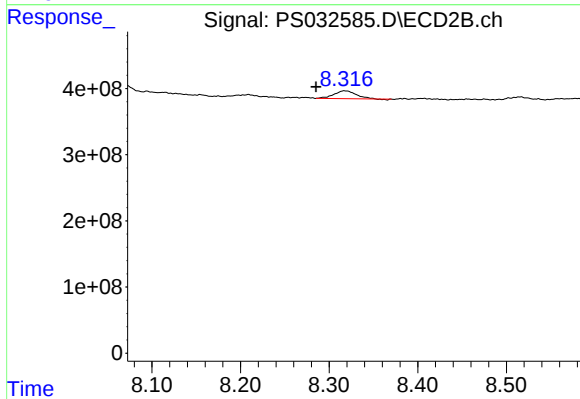

#8 DICHLORPROP


R.T.: 8.318 min
Delta R.T.: 0.032 min
Response: 201987095
Conc: 40.66 ng/ml

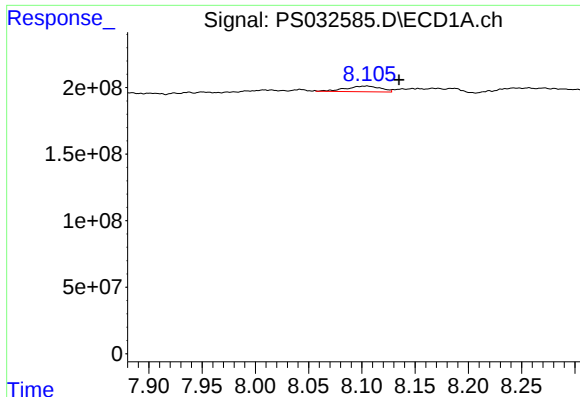

#9 2,4-D


R.T.: 8.104 min
Delta R.T.: -0.031 min
Response: 96714071
Conc: 15.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

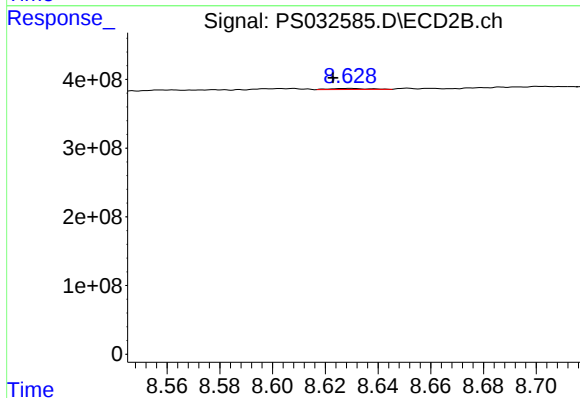


#9 2,4-D

R.T.: 8.629 min
Delta R.T.: 0.006 min
Response: 14918727
Conc: 2.66 ng/ml

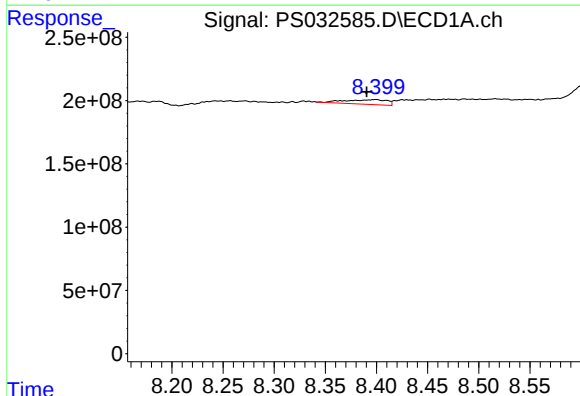


#10 Pentachlorophenol

R.T.: 8.398 min
Delta R.T.: 0.008 min
Response: 105823589
Conc: 1.44 ng/ml

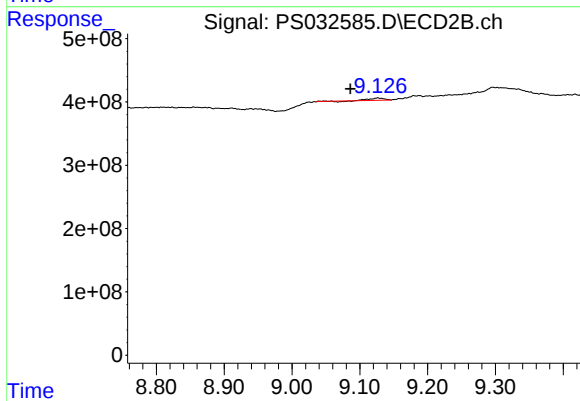

#10 Pentachlorophenol


R.T.: 9.127 min
Delta R.T.: 0.041 min
Response: 42310237
Conc: N.D.

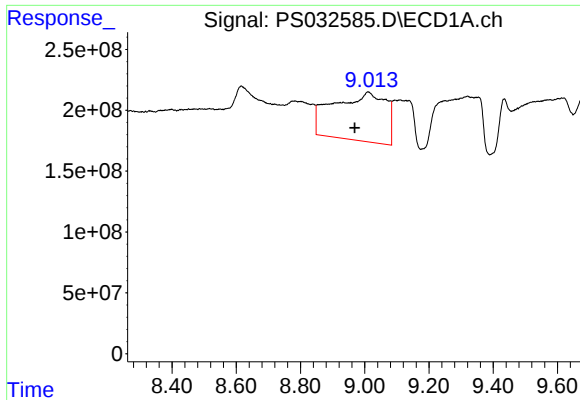

#11 2,4,5-TP (SILVEX)


R.T.: 9.011 min
Delta R.T.: 0.042 min
Response: 4508130155
Conc: 134.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

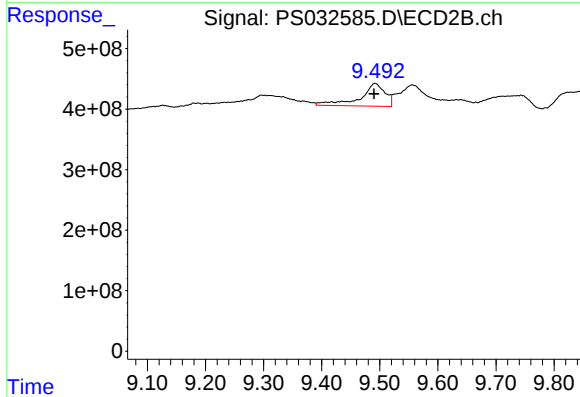


#11 2,4,5-TP (SILVEX)

R.T.: 9.492 min
Delta R.T.: 0.002 min
Response: 1121229504
Conc: 39.08 ng/ml

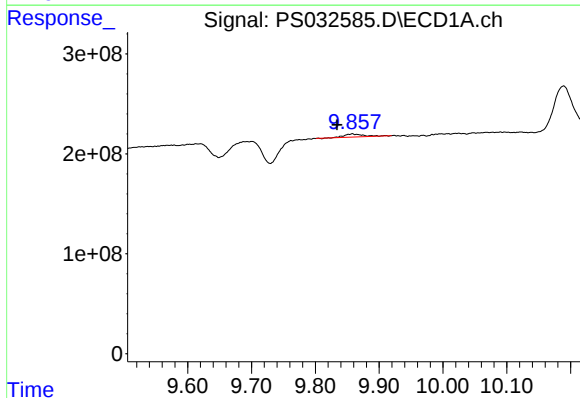


#13 2,4-DB

R.T.: 9.858 min
Delta R.T.: 0.024 min
Response: 68312294
Conc: 21.90 ng/ml

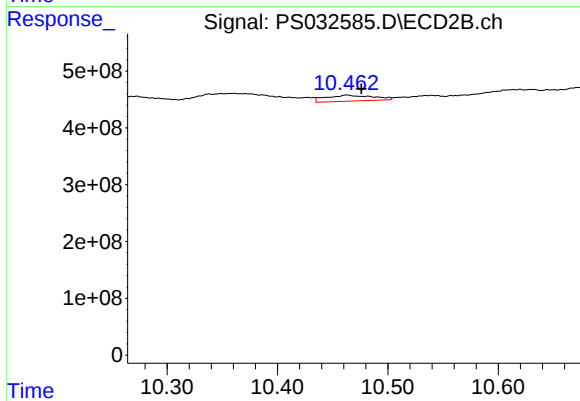

#13 2,4-DB


R.T.: 10.463 min
Delta R.T.: -0.013 min
Response: 308977882
Conc: 75.85 ng/ml

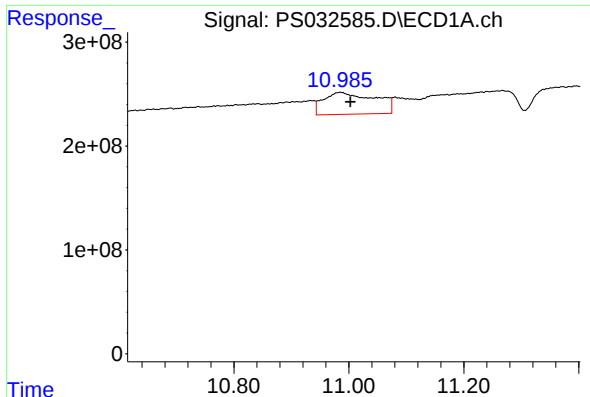

#14 DINOSEB


R.T.: 10.985 min
Delta R.T.: -0.018 min
Response: 1311290154
Conc: 47.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

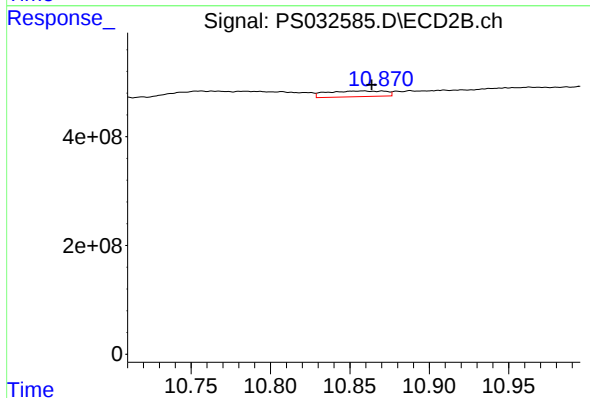


#14 DINOSEB

R.T.: 10.858 min
Delta R.T.: -0.006 min
Response: 273798214
Conc: 15.14 ng/ml

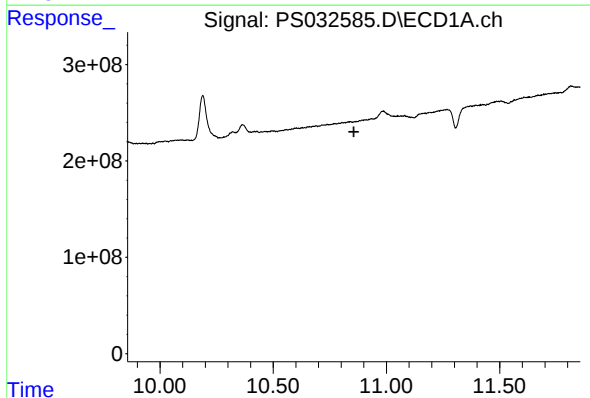


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.856 min
Response: 0
Conc: N.D.

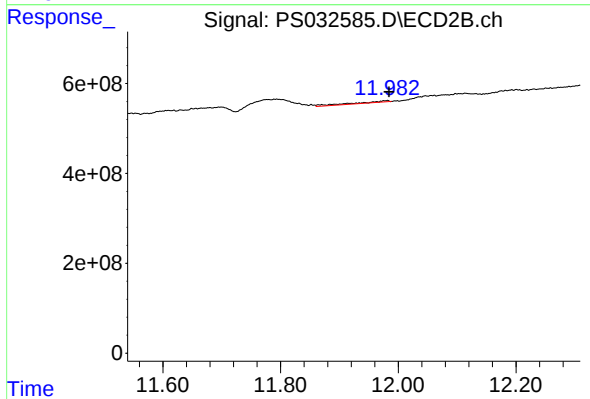

#15 Picloram


R.T.: 11.980 min
Delta R.T.: -0.004 min
Response: 139444220
Conc: 3.87 ng/ml

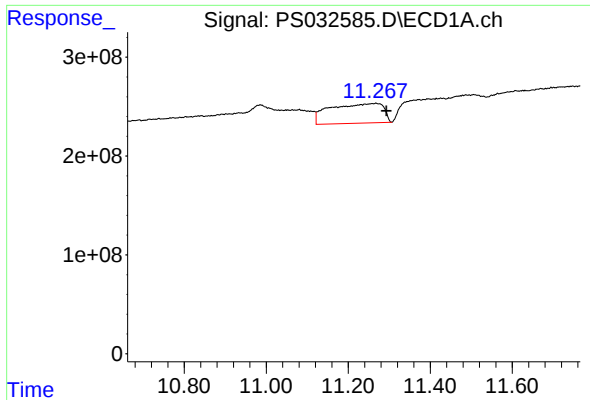

#16 DCPA

R.T.: 11.267 min
Delta R.T.: -0.026 min
Response: 1799487894
Conc: 44.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

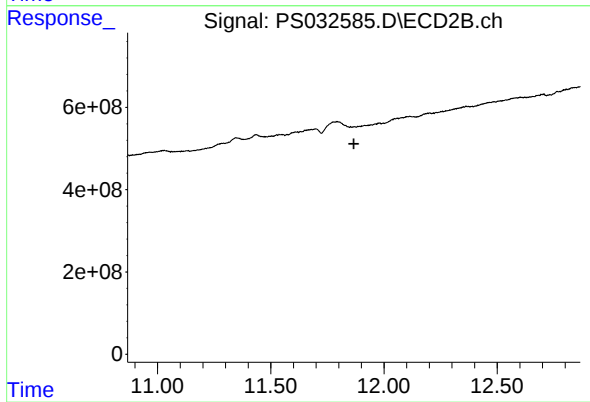

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.867 min
Response: 0
Conc: N.D.