

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120325\
 Data File : PS032604.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Dec 2025 22:11
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 01:04:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120325.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 03 13:46:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.012	7.381	1835.6E6	1561.4E6	332.320	291.235
Target Compounds							
2) T	3,5-DICHL...	6.229	6.397	4233235	3490192	<MDL	<MDL #
3) T	4-Nitroph...	6.902f	6.970	-1280591	2910078	N.D.	1.218
6) T	MCP	7.387	0.000	493560	0	<MDL	N.D. #
7) T	MCPA	7.505	7.900f	18895573	5622674	1.169	<MDL #
8) T	DICHLORPROP	0.000	8.269	0	1540510	N.D.	<MDL
9) T	2,4-D	0.000	8.613	0	3764676	N.D.	<MDL
10) T	Pentachlo...	0.000	9.085	0	6389612	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	9.491	0	9169381	N.D.	<MDL
13) T	2,4-DB	0.000	10.452	0	182.2E6	N.D.	44.717
14) T	DINOSEB	0.000	10.861	0	379.2E6	N.D.	20.970



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120325\
Data File : PS032604.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Dec 2025 22:11
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 01:04:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120325.M
Quant Title : 8080.M
QLast Update : Wed Dec 03 13:46:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

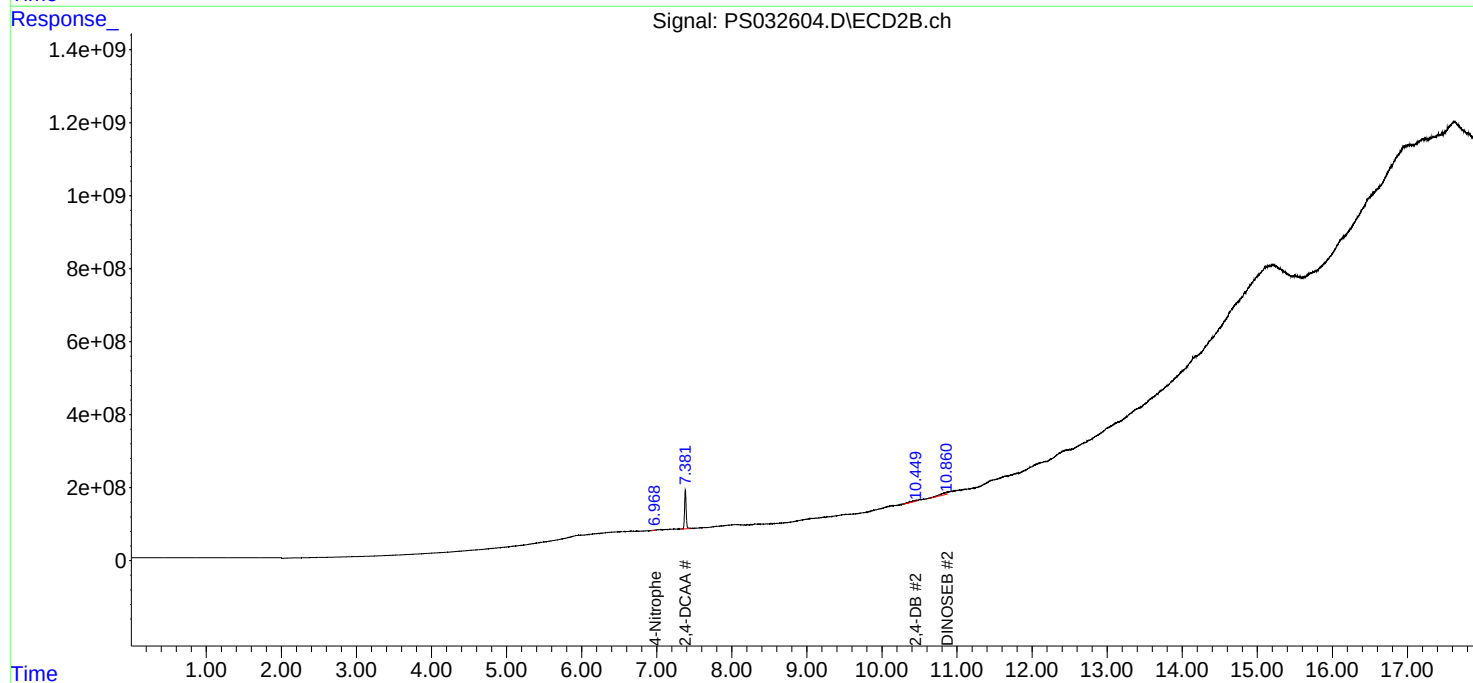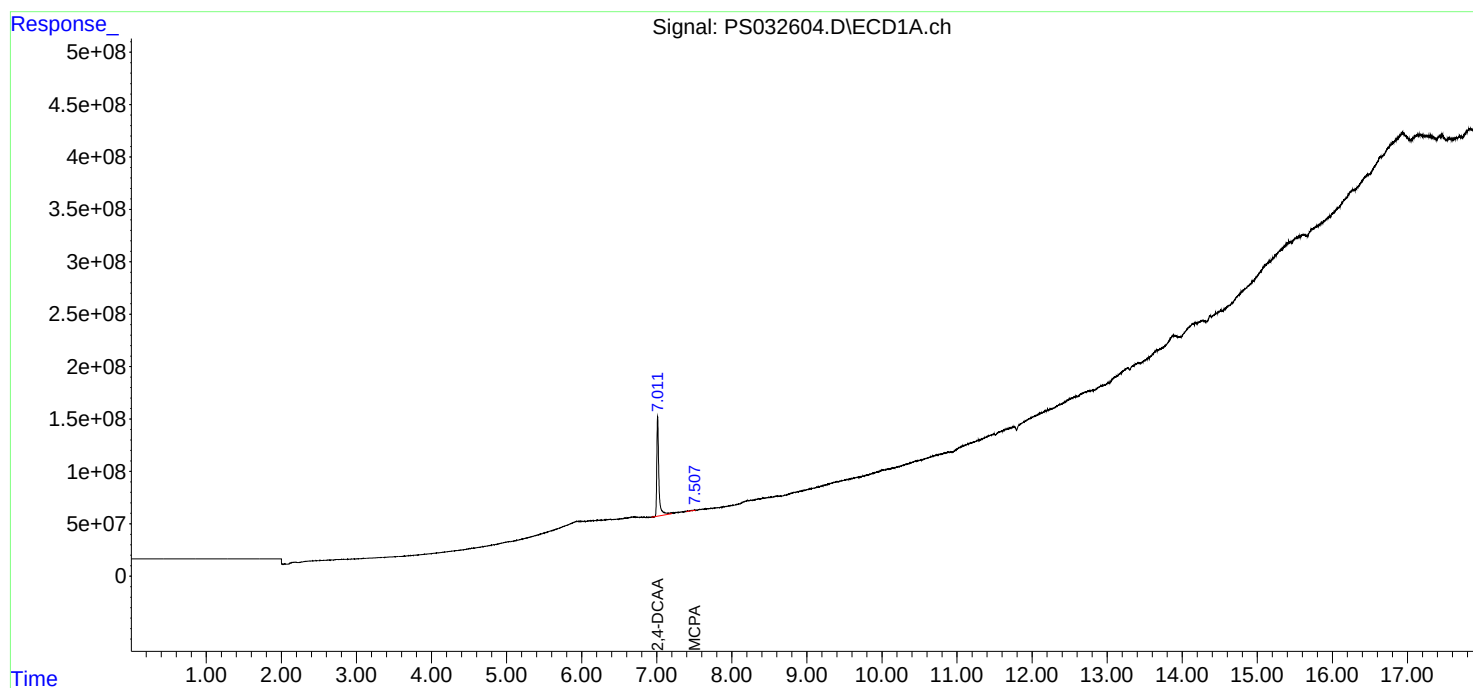


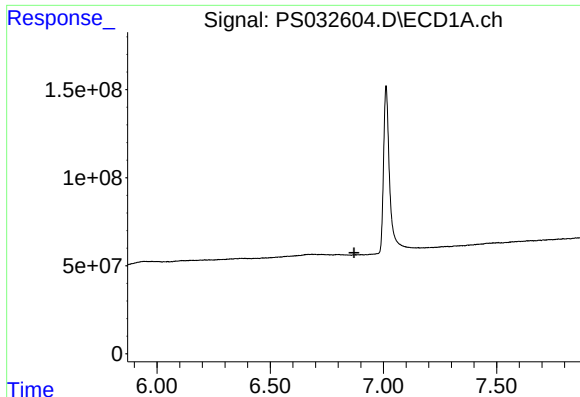

#3 4-Nitrophenol


R.T.: 6.902 min
Delta R.T.: 0.032 min
Response: -1280591
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

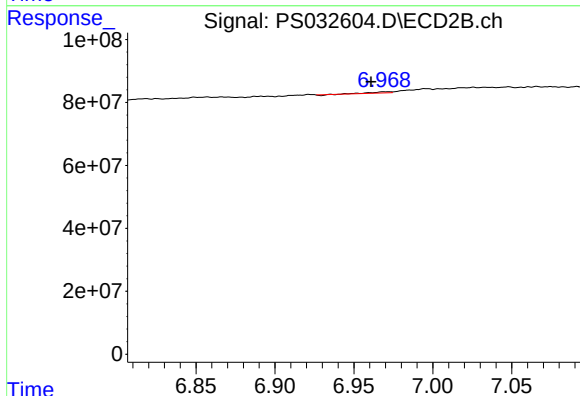


#3 4-Nitrophenol

R.T.: 6.970 min
Delta R.T.: 0.009 min
Response: 2910078
Conc: 1.22 ng/ml

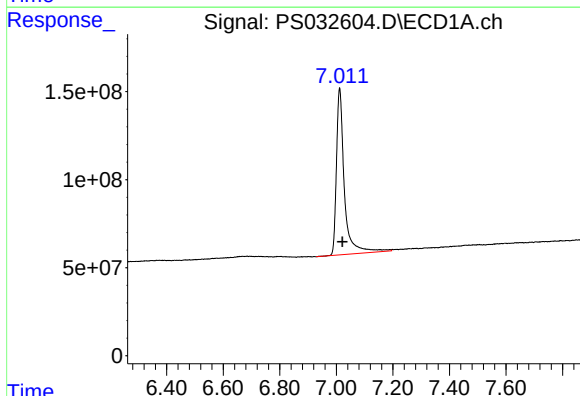


#4 2,4-DCAA

R.T.: 7.012 min
Delta R.T.: -0.010 min
Response: 1835618692
Conc: 332.32 ng/ml

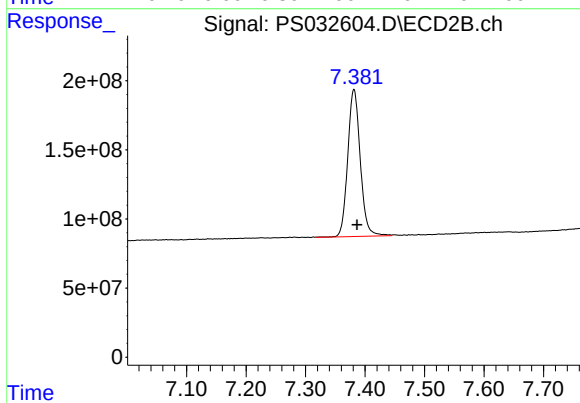

#4 2,4-DCAA


R.T.: 7.381 min
Delta R.T.: -0.005 min
Response: 1561370949
Conc: 291.23 ng/ml

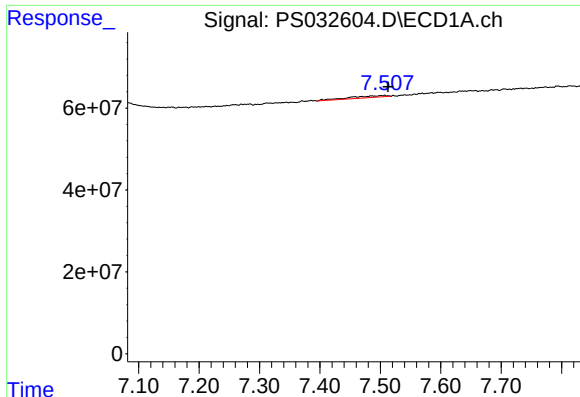

#7 MCPA


R.T.: 7.505 min
Delta R.T.: -0.007 min
Response: 18895573
Conc: 1.17 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

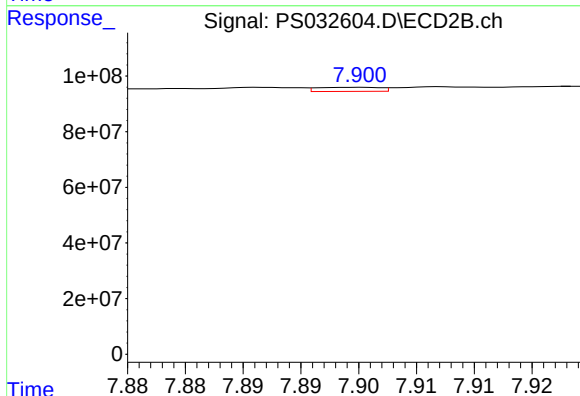


#7 MCPA

R.T.: 7.900 min
Delta R.T.: -0.026 min
Response: 5622674
Conc: N.D.

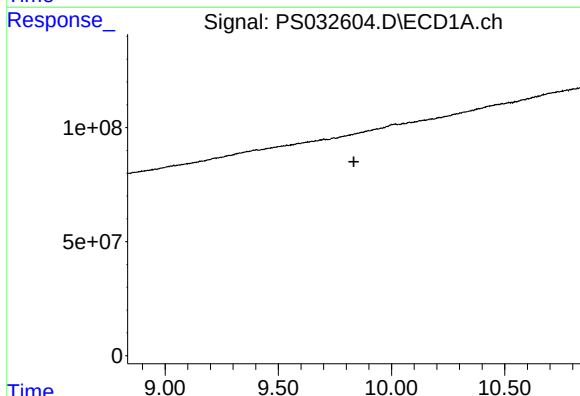


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.834 min
Response: 0
Conc: N.D.

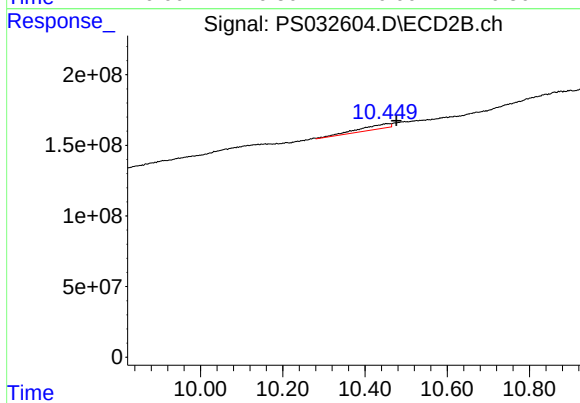

#13 2,4-DB


R.T.: 10.452 min
Delta R.T.: -0.024 min
Response: 182158532
Conc: 44.72 ng/ml

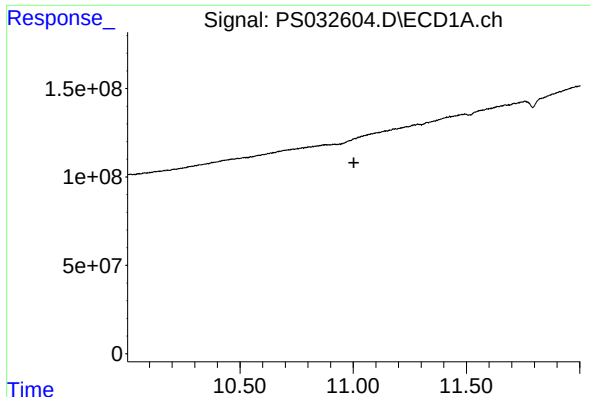

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

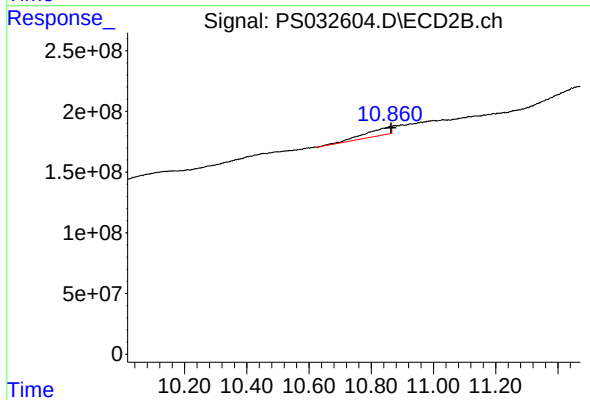

#14 DINOSEB

R.T.: 10.861 min
Delta R.T.: -0.003 min
Response: 379230382
Conc: 20.97 ng/ml