

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120419\
 Data File : PS007903.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2019 12:02
 Operator : SM\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 04:31:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:27:41 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.454	5.180	1189.7E6	593.0E6	750.000	750.000
Target Compounds							
1) T	Dalapon	2.038	1.748	1417.0E6	817.4E6	682.500	682.500
2) T	3,5-DICHL...	4.830	4.489	1499.3E6	740.9E6	697.500	697.500
3) T	4-Nitroph...	5.307	4.870	518.3E6	305.4E6	682.500	682.500
5) T	DICAMBA	5.602	5.304	4088.0E6	2067.8E6	705.000	705.000
6) T	MCPD	5.754	5.389	297.1E6	152.0E6	70.500	70.500
7) T	MCPA	5.885	5.563	431.6E6	224.5E6	69.750	69.750
8) T	DICHLORPROP	6.225	5.832	1034.4E6	507.6E6	705.000	705.000
9) T	2,4-D	6.440	6.101	1149.9E6	633.2E6	705.000	705.000
10) T	Pentachlo...	6.695	6.463	15808.1E6	7955.3E6	712.500	712.500
11) T	2,4,5-TP ...	7.228	6.826	6155.4E6	3143.2E6	712.500	712.500
12) T	2,4,5-T	7.500	7.184	6687.2E6	2987.8E6	712.500	712.500
13) T	2,4-DB	8.027	7.668	905.1E6	400.0E6	712.500	712.500
14) T	DINOSEB	9.107	7.974	4932.2E6	2371.0E6	705.000	705.000
15) T	Picloram	8.943	8.909	9269.8E6	4678.6E6	712.500	712.500
16) T	DCPA	9.379	8.866	8012.2E6	4208.5E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120419\
Data File : PS007903.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2019 12:02
Operator : SM\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 04:31:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:27:41 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

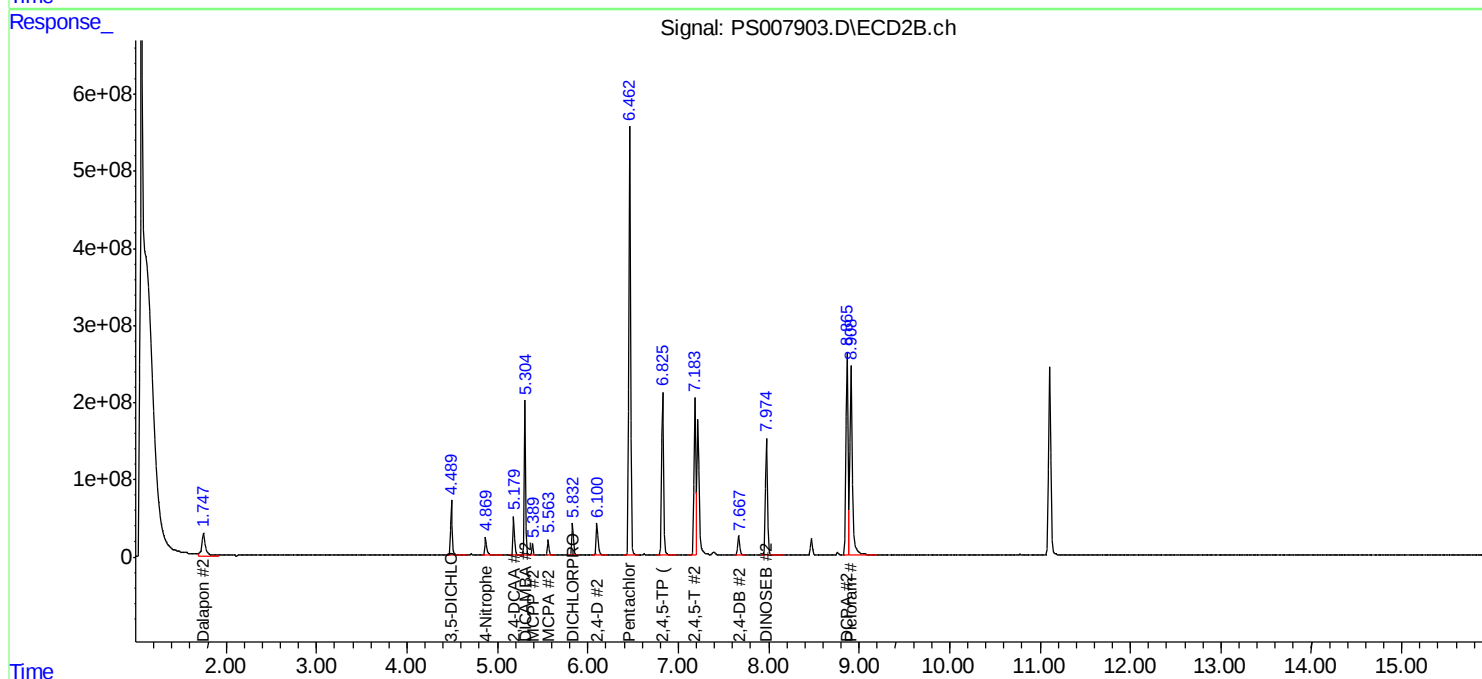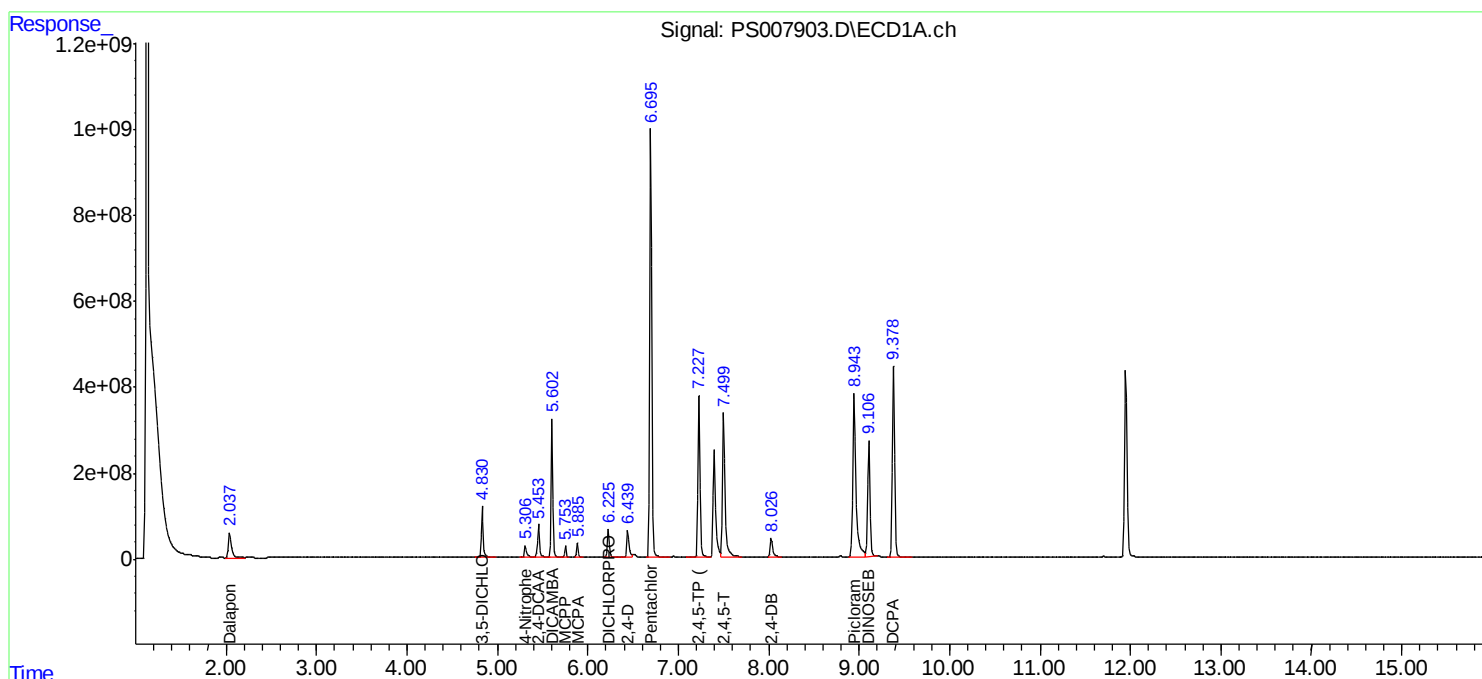


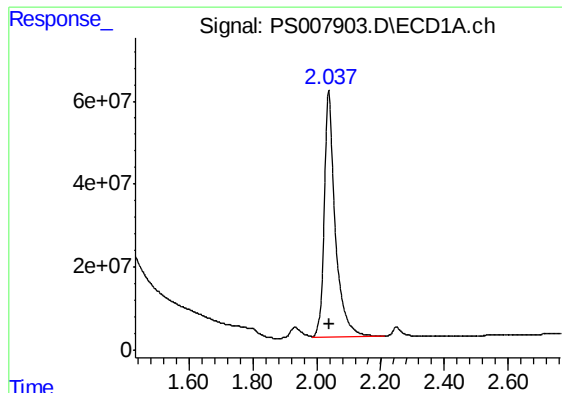

#1 Dalapon


R.T.: 2.038 min
Delta R.T.: 0.000 min
Response: 1417016057
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

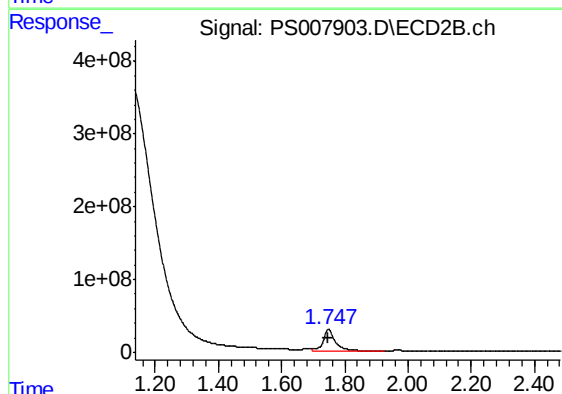


#1 Dalapon

R.T.: 1.748 min
Delta R.T.: 0.000 min
Response: 817394544
Conc: 682.50 ng/ml

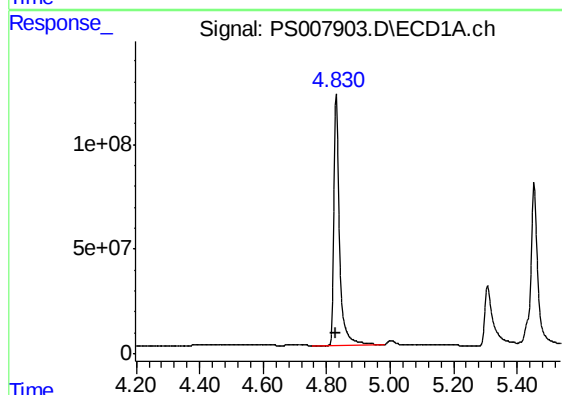


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.830 min
Delta R.T.: 0.000 min
Response: 1499284145
Conc: 697.50 ng/ml

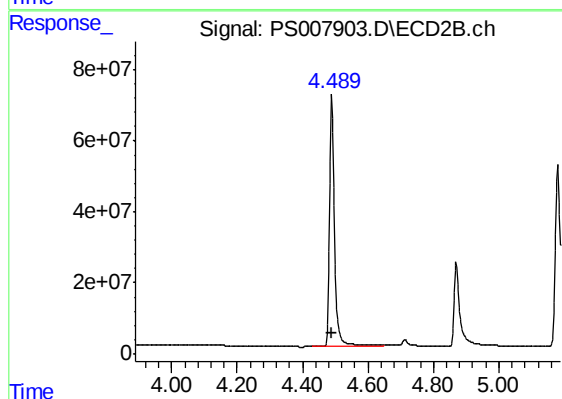

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.489 min
Delta R.T.: 0.000 min
Response: 740916008
Conc: 697.50 ng/ml

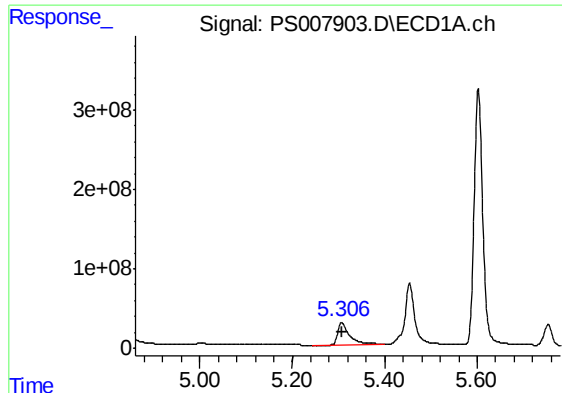

#3 4-Nitrophenol


R.T.: 5.307 min
Delta R.T.: 0.000 min
Response: 518262555
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

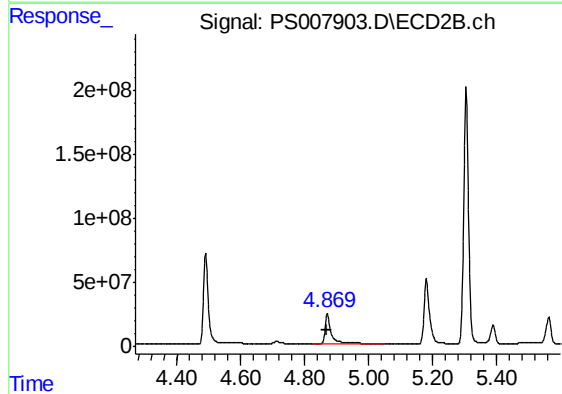


#3 4-Nitrophenol

R.T.: 4.870 min
Delta R.T.: 0.000 min
Response: 305353920
Conc: 682.50 ng/ml

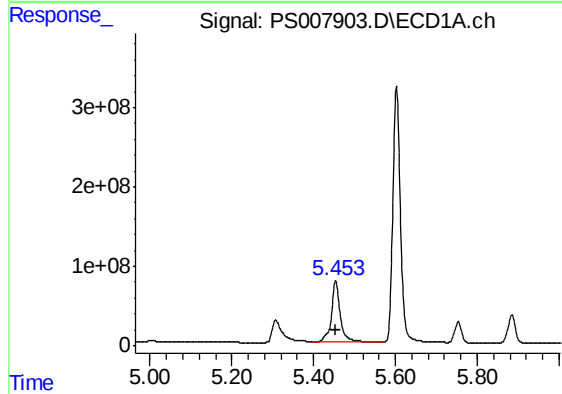


#4 2,4-DCAA

R.T.: 5.454 min
Delta R.T.: 0.000 min
Response: 1189682319
Conc: 750.00 ng/ml

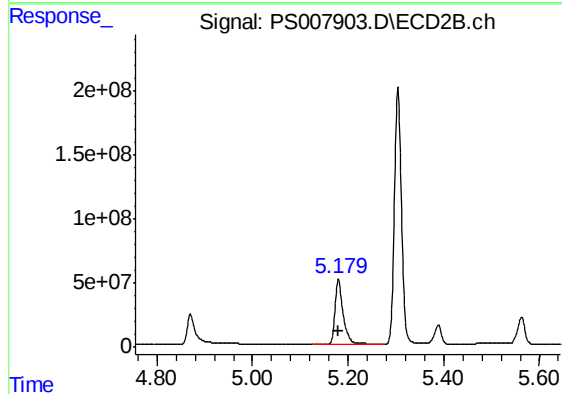

#4 2,4-DCAA


R.T.: 5.180 min
Delta R.T.: 0.000 min
Response: 592995847
Conc: 750.00 ng/ml

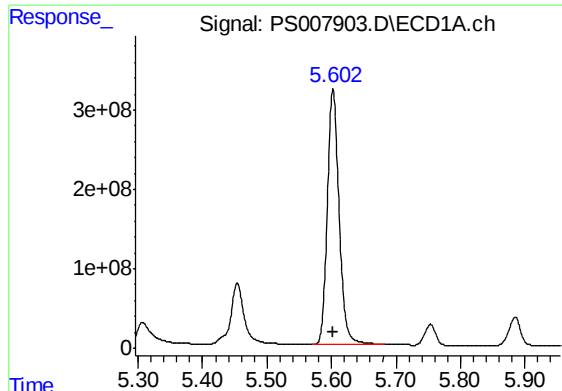

#5 DICAMBA


R.T.: 5.602 min
Delta R.T.: 0.000 min
Response: 4088023343
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

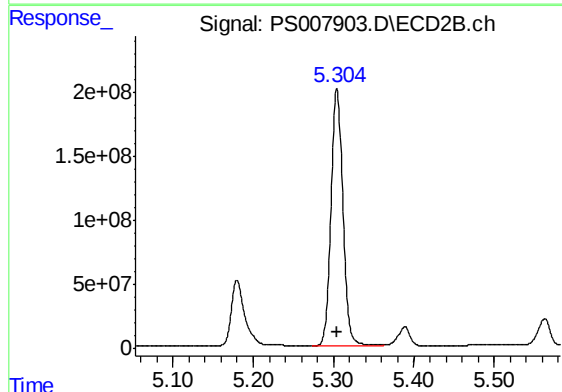


#5 DICAMBA

R.T.: 5.304 min
Delta R.T.: 0.000 min
Response: 2067796815
Conc: 705.00 ng/ml

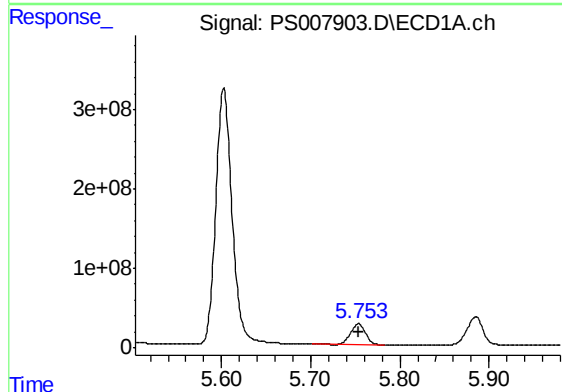


#6 MCPP

R.T.: 5.754 min
Delta R.T.: 0.000 min
Response: 297078016
Conc: 70.50 ug/ml

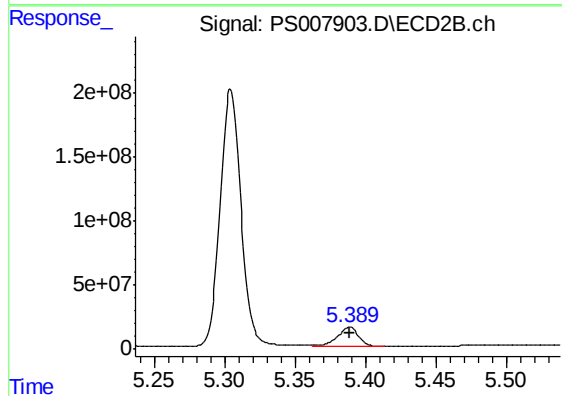

#6 MCPP


R.T.: 5.389 min
Delta R.T.: 0.000 min
Response: 152006140
Conc: 70.50 ug/ml

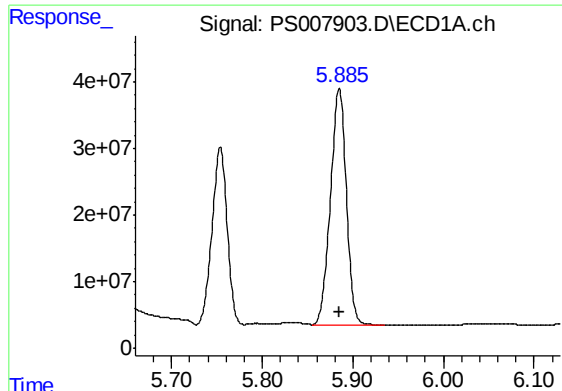

#7 MCPA


R.T.: 5.885 min
Delta R.T.: 0.000 min
Response: 431551316
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

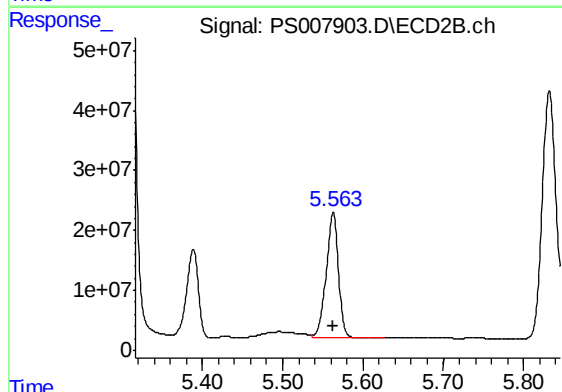


#7 MCPA

R.T.: 5.563 min
Delta R.T.: 0.000 min
Response: 224532836
Conc: 69.75 ug/ml

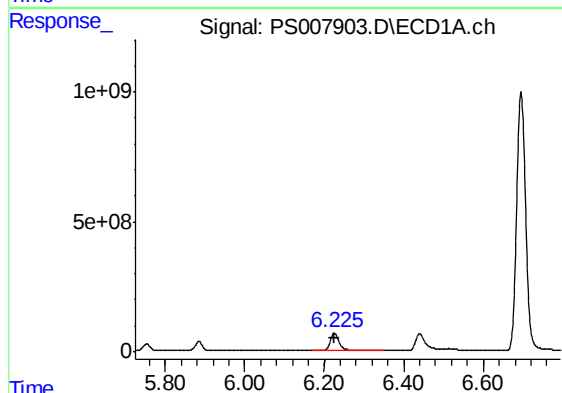


#8 DICHLORPROP

R.T.: 6.225 min
Delta R.T.: 0.000 min
Response: 1034413968
Conc: 705.00 ng/ml

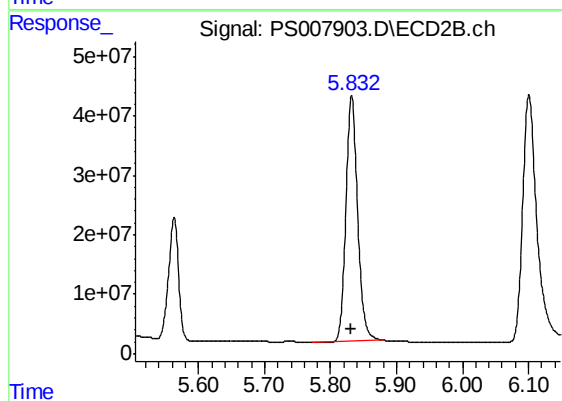

#8 DICHLORPROP


R.T.: 5.832 min
Delta R.T.: 0.000 min
Response: 507554713
Conc: 705.00 ng/ml

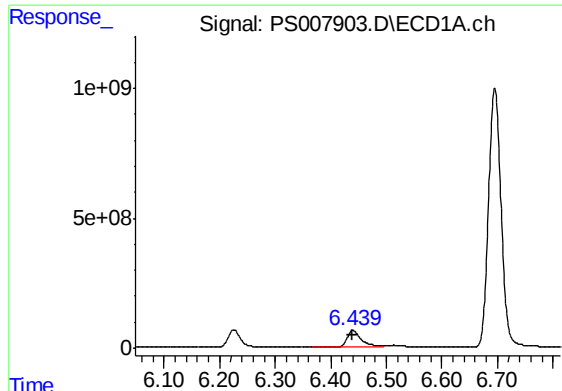

#9 2,4-D


R.T.: 6.440 min
Delta R.T.: 0.000 min
Response: 1149924714
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

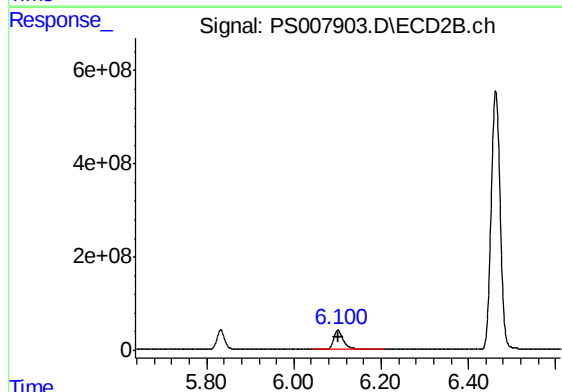


#9 2,4-D

R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 633249433
Conc: 705.00 ng/ml

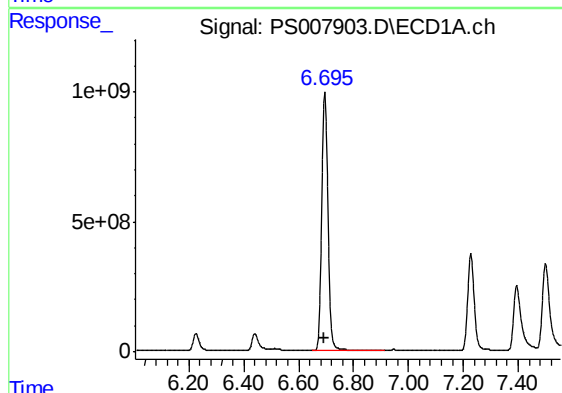


#10 Pentachlorophenol

R.T.: 6.695 min
Delta R.T.: 0.000 min
Response: 15808050274
Conc: 712.50 ng/ml

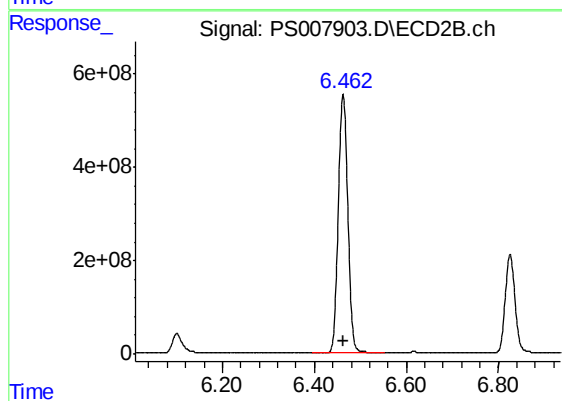

#10 Pentachlorophenol


R.T.: 6.463 min
Delta R.T.: 0.000 min
Response: 7955327155
Conc: 712.50 ng/ml

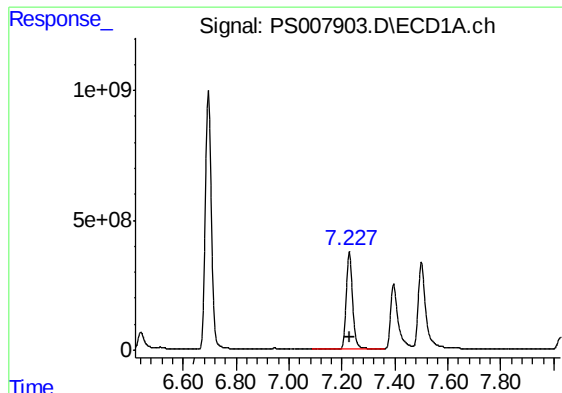

#11 2,4,5-TP (SILVEX)


R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 6155442021
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

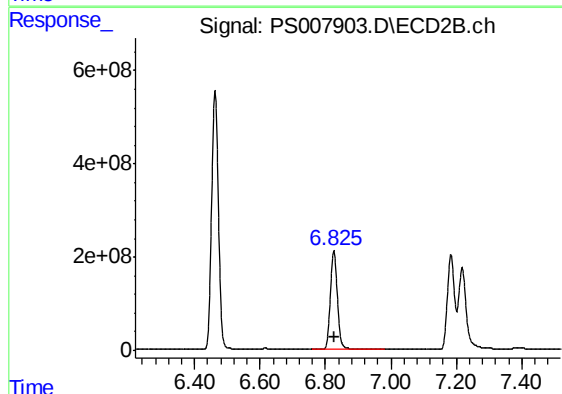


#11 2,4,5-TP (SILVEX)

R.T.: 6.826 min
Delta R.T.: 0.000 min
Response: 3143239582
Conc: 712.50 ng/ml

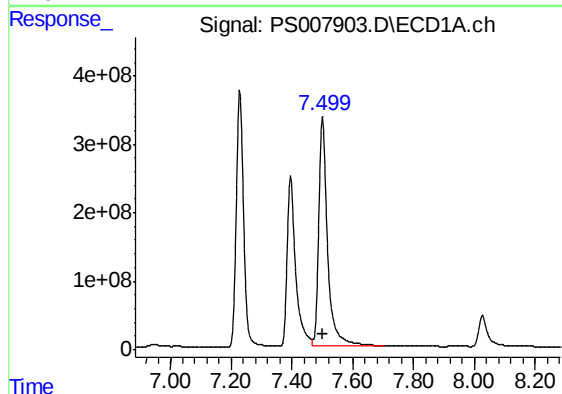


#12 2,4,5-T

R.T.: 7.500 min
Delta R.T.: 0.000 min
Response: 6687237539
Conc: 712.50 ng/ml

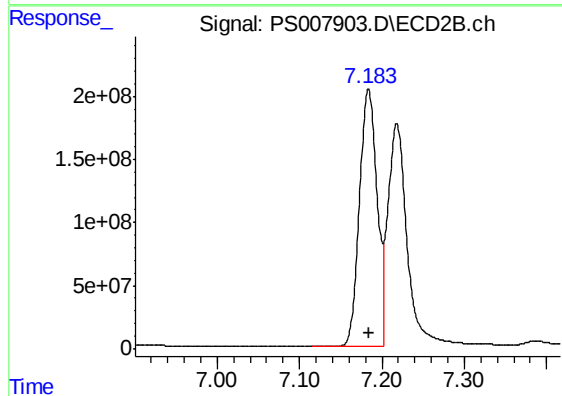

#12 2,4,5-T


R.T.: 7.184 min
Delta R.T.: 0.000 min
Response: 2987777213
Conc: 712.50 ng/ml

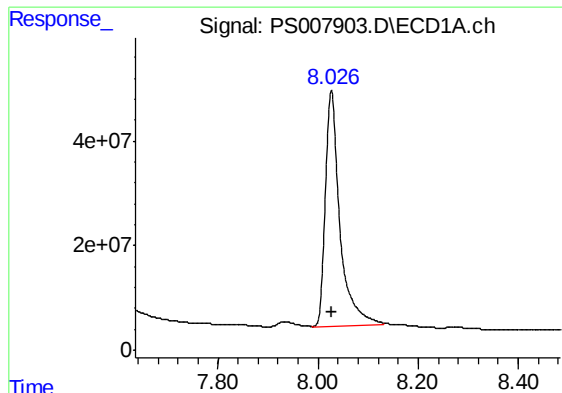

#13 2,4-DB


R.T.: 8.027 min
Delta R.T.: 0.000 min
Response: 905081297
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

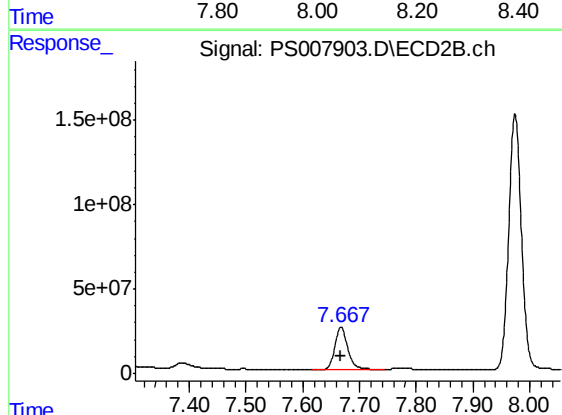


#13 2,4-DB

R.T.: 7.668 min
Delta R.T.: 0.000 min
Response: 400005761
Conc: 712.50 ng/ml

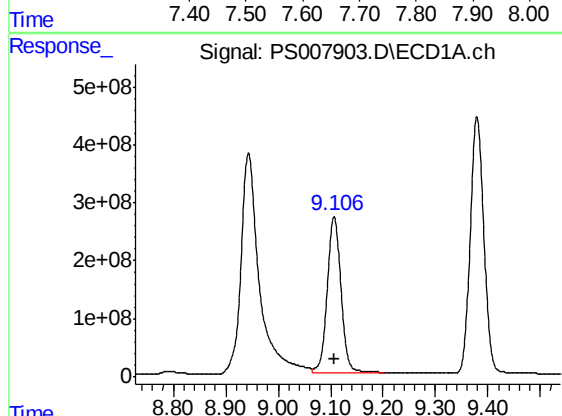


#14 DINOSEB

R.T.: 9.107 min
Delta R.T.: 0.000 min
Response: 4932172748
Conc: 705.00 ng/ml

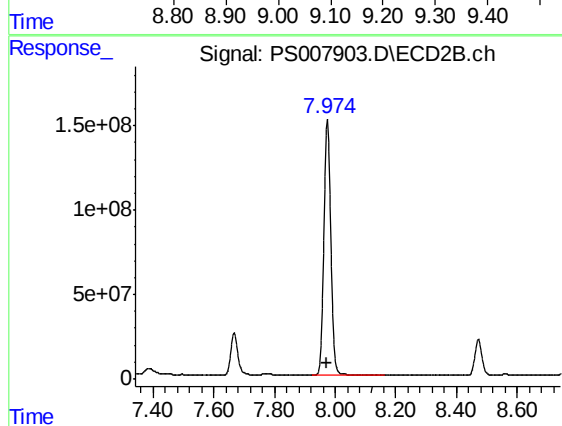

#14 DINOSEB


R.T.: 7.974 min
Delta R.T.: 0.000 min
Response: 2371034501
Conc: 705.00 ng/ml

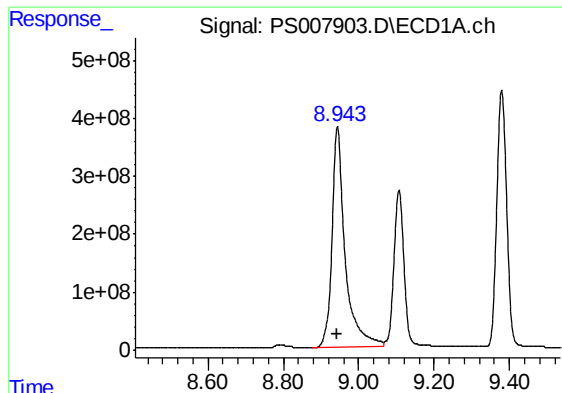

#15 Picloram


R.T.: 8.943 min
Delta R.T.: 0.000 min
Response: 9269758546
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

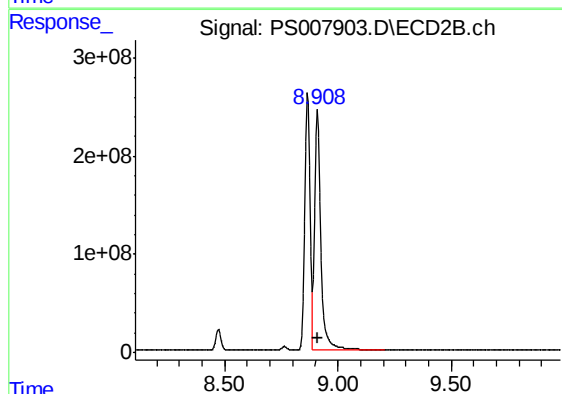


#15 Picloram

R.T.: 8.909 min
Delta R.T.: 0.000 min
Response: 4678626391
Conc: 712.50 ng/ml

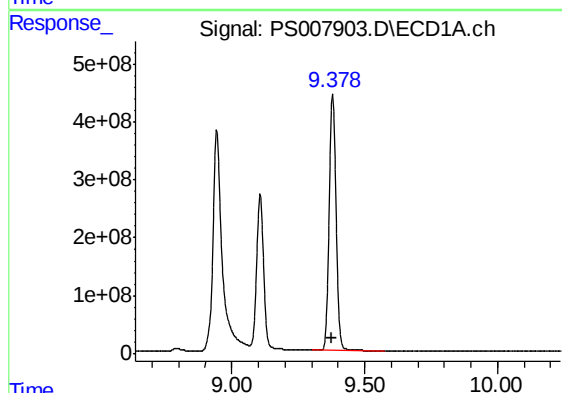

#16 DCPA

R.T.: 9.379 min
Delta R.T.: 0.000 min
Response: 8012210781
Conc: 720.00 ng/ml

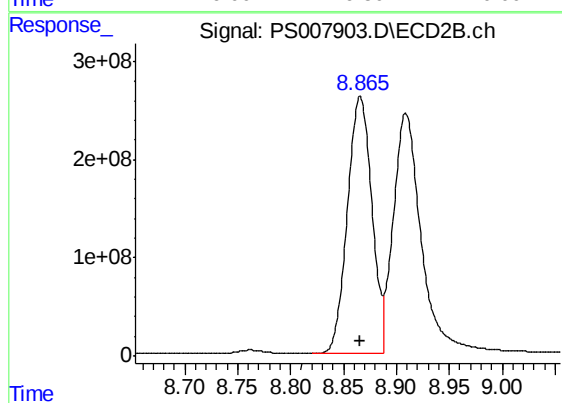

#16 DCPA

R.T.: 8.866 min
Delta R.T.: 0.000 min
Response: 4208538520
Conc: 720.00 ng/ml