

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120424\
 Data File : PS028688.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2024 09:20
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 23:25:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	2.671f	0.000	23025764	0	7.935	N.D.	#
3) T	4-Nitroph...	7.011	0.000	3748686	0	2.181	N.D.	#
5) T	DICAMBA	0.000	7.918	0	4964550	N.D.	<MDL	
7) T	MCPA	0.000	8.246f	0	9150817	N.D.	1.475	
8) T	DICHLORPROP	8.146f	8.686f	834487	2284768	<MDL	1.429	#
11) T	2,4,5-TP ...	9.227	9.873	167810	14357605	<MDL	1.505	#
12) T	2,4,5-T	9.524	10.289	4330562	5066731	<MDL	<MDL	#
13) T	2,4-DB	10.099	0.000	566486	0	<MDL	N.D.	#
15) T	Picloram	11.121	12.330	35173178	11592134	1.183	<MDL	#
16) T	DCPA	11.589	12.330f	3859786	11592134	<MDL	1.045	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120424\
Data File : PS028688.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2024 09:20
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 23:25:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

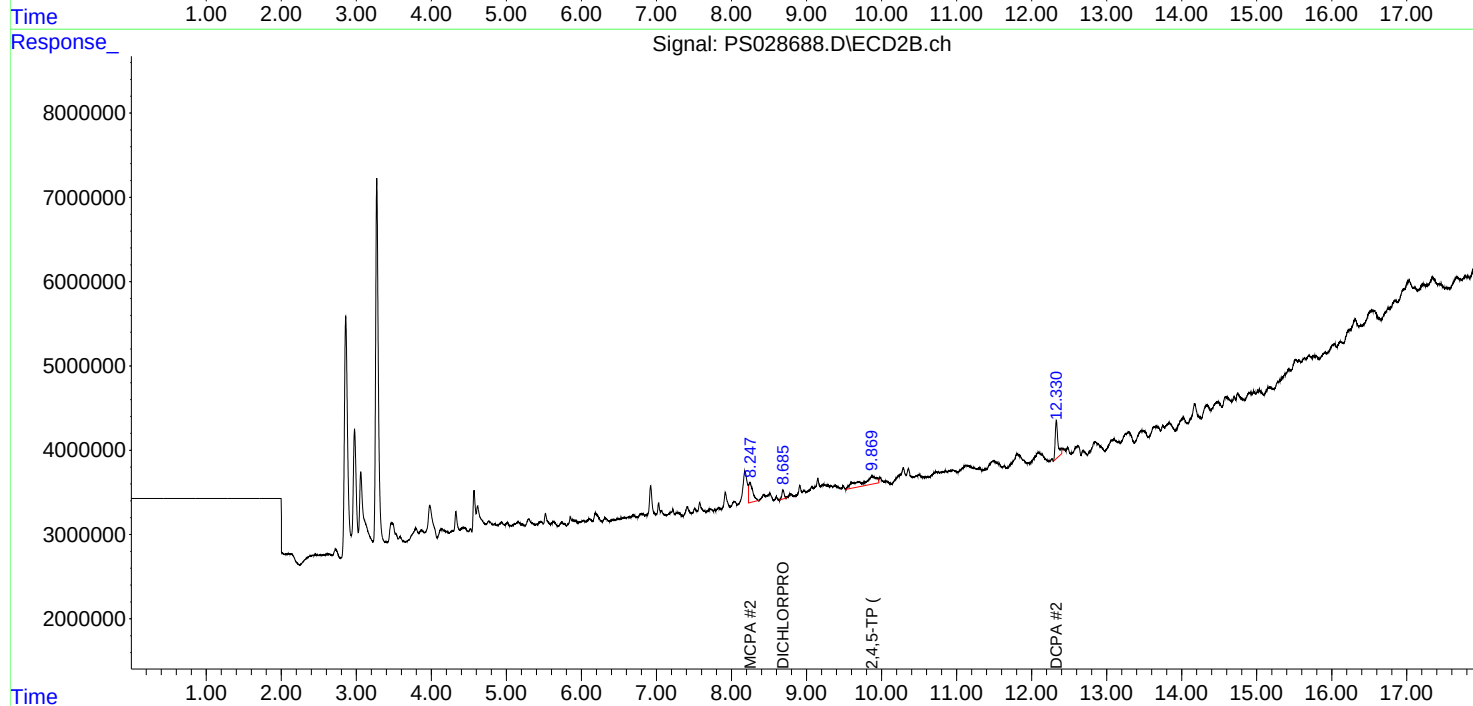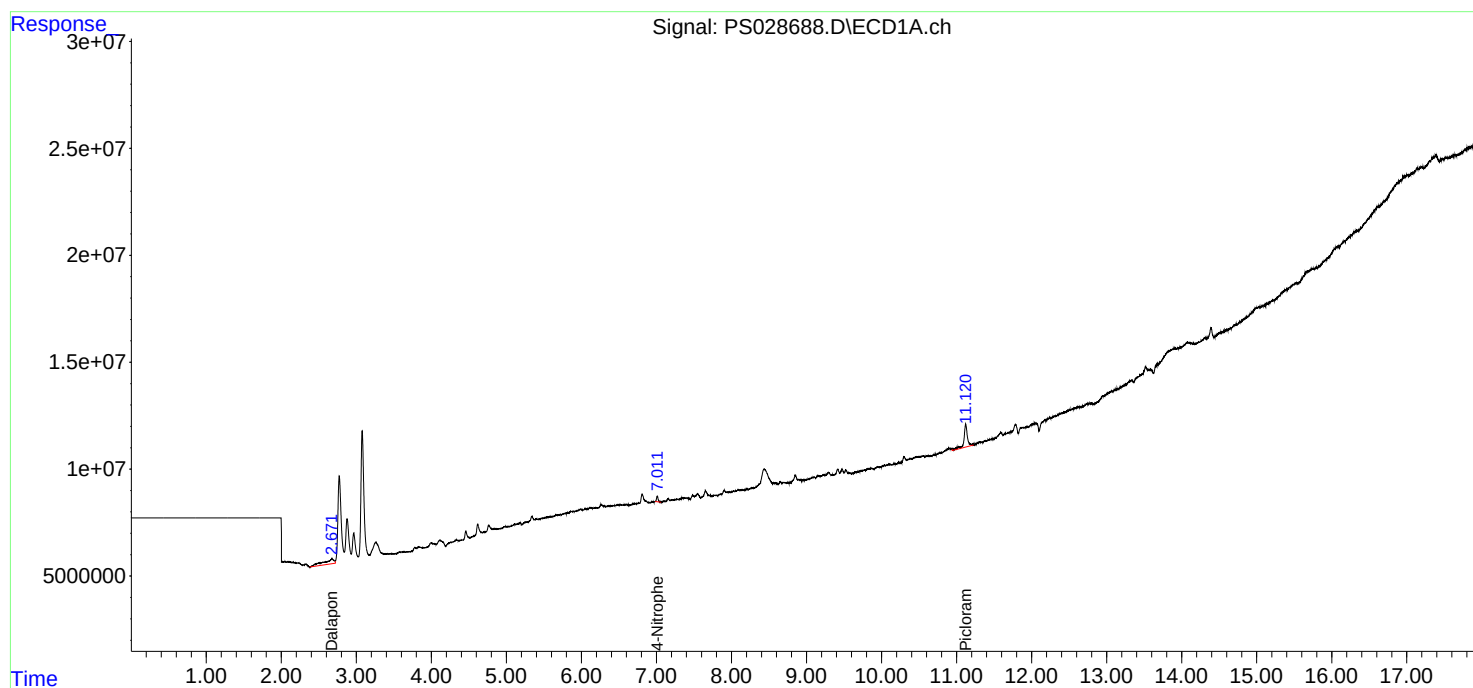


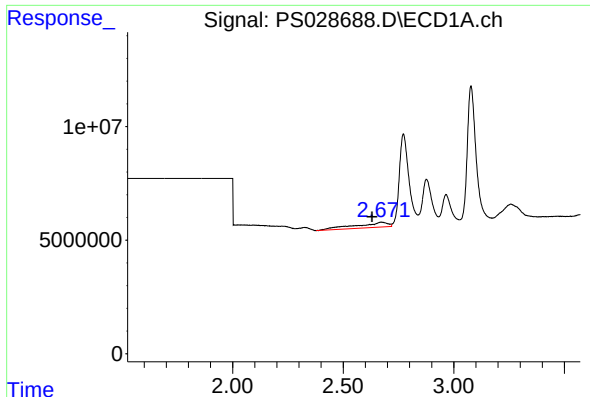

#1 Dalapon


R.T.: 2.671 min
Delta R.T.: 0.041 min
Response: 23025764
Conc: 7.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

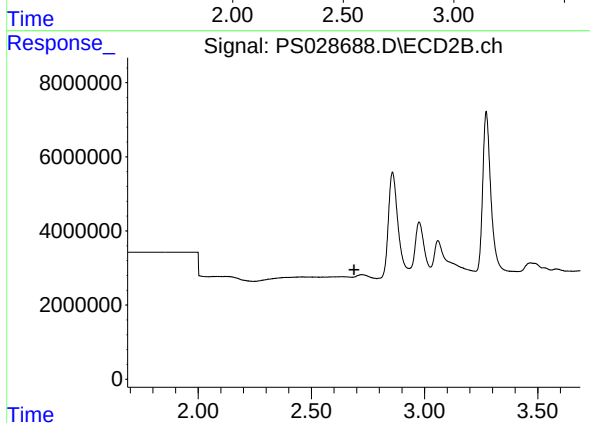


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.688 min
Response: 0
Conc: N.D.

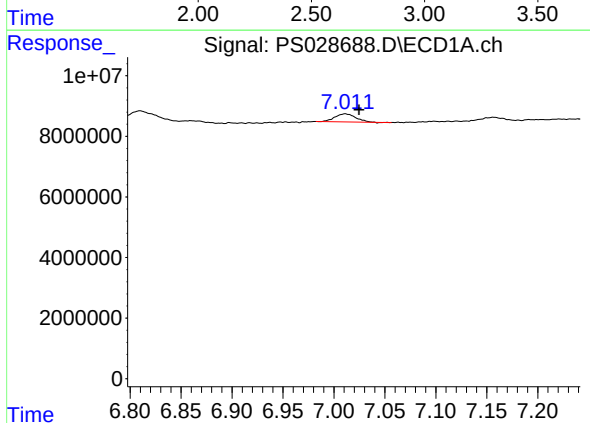


#3 4-Nitrophenol

R.T.: 7.011 min
Delta R.T.: -0.013 min
Response: 3748686
Conc: 2.18 ng/ml

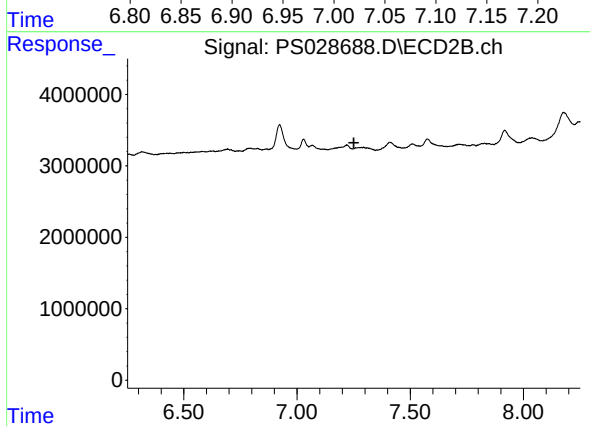

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.251 min
Response: 0
Conc: N.D.

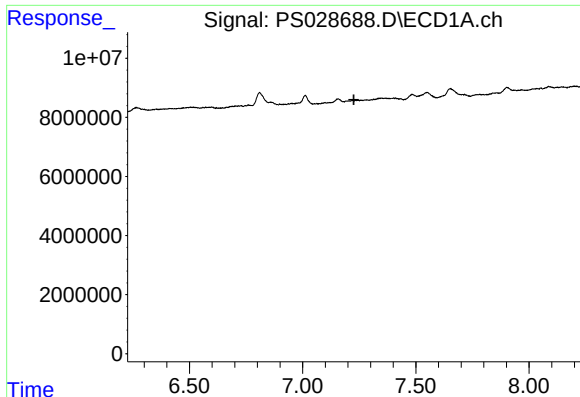

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.226 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

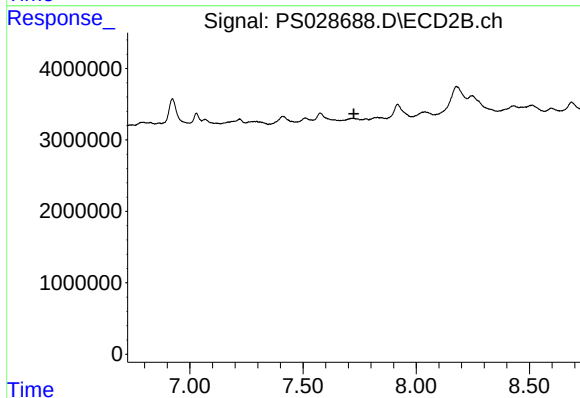


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.725 min
Response: 0
Conc: N.D.

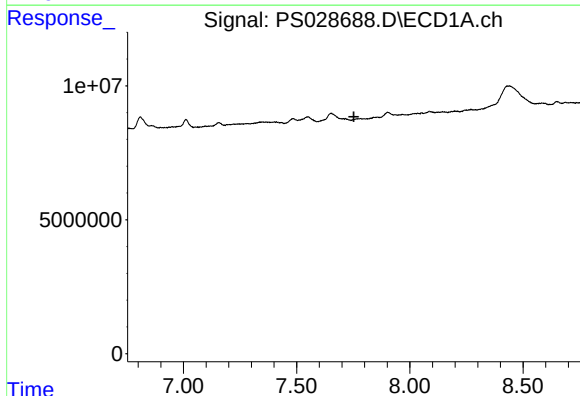


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.753 min
Response: 0
Conc: N.D.

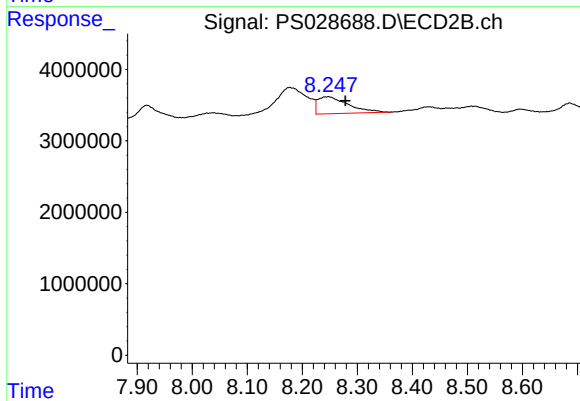

#7 MCPA


R.T.: 8.246 min
Delta R.T.: -0.032 min
Response: 9150817
Conc: 1.47 ug/ml

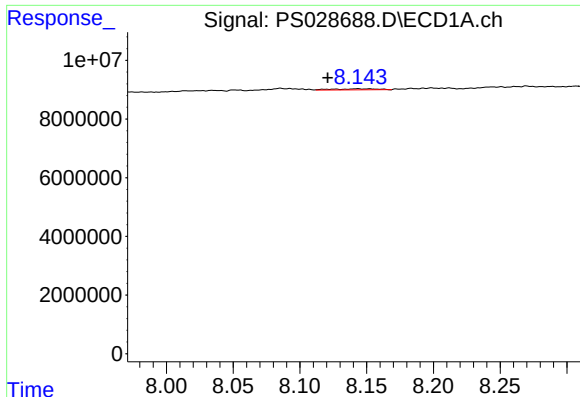

#8 DICHLORPROP


R.T.: 8.146 min
Delta R.T.: 0.026 min
Response: 834487
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

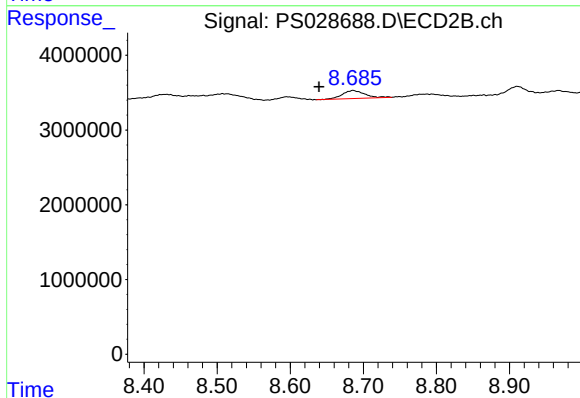


#8 DICHLORPROP

R.T.: 8.686 min
Delta R.T.: 0.046 min
Response: 2284768
Conc: 1.43 ng/ml

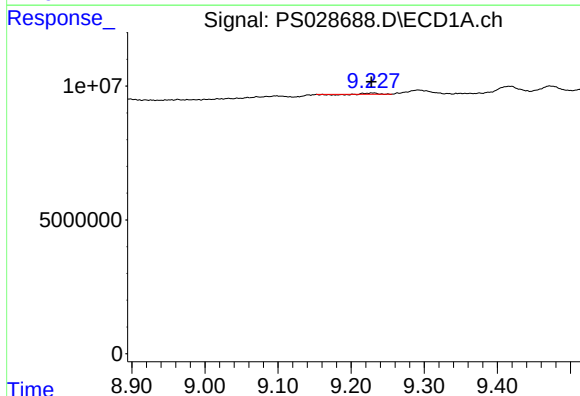


#11 2,4,5-TP (SILVEX)

R.T.: 9.227 min
Delta R.T.: 0.000 min
Response: 167810
Conc: N.D.

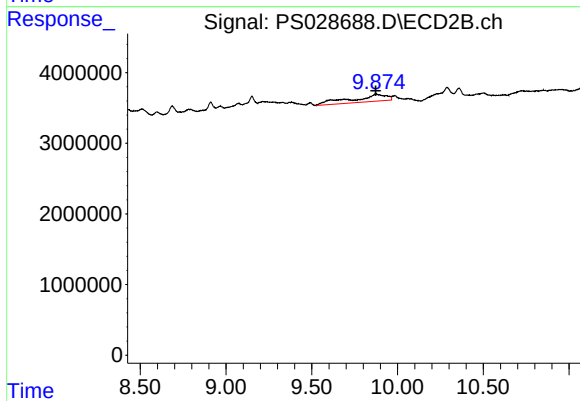

#11 2,4,5-TP (SILVEX)


R.T.: 9.873 min
Delta R.T.: 0.000 min
Response: 14357605
Conc: 1.50 ng/ml

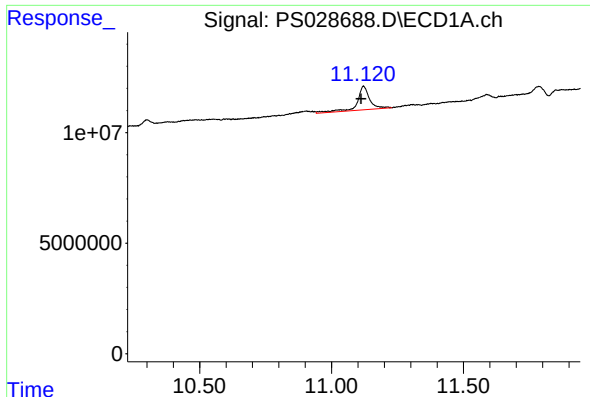

#15 Picloram


R.T.: 11.121 min
Delta R.T.: 0.010 min
Response: 35173178
Conc: 1.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

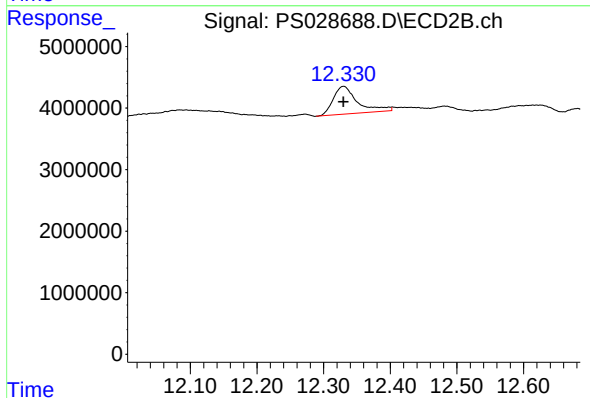


#15 Picloram

R.T.: 12.330 min
Delta R.T.: 0.000 min
Response: 11592134
Conc: N.D.

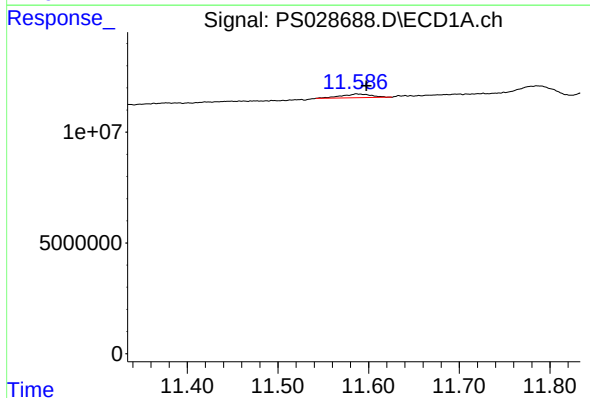

#16 DCPA

R.T.: 11.589 min
Delta R.T.: -0.008 min
Response: 3859786
Conc: N.D.

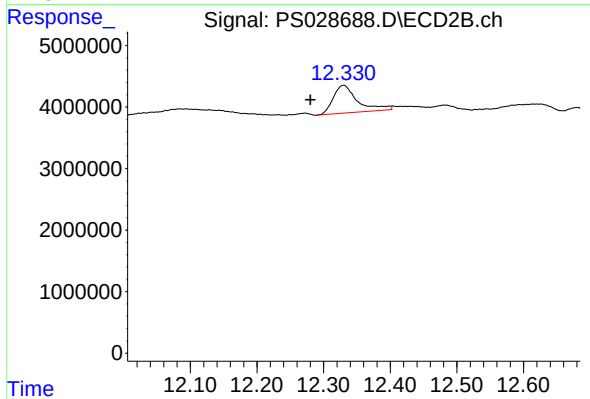

#16 DCPA

R.T.: 12.330 min
Delta R.T.: 0.049 min
Response: 11592134
Conc: 1.04 ng/ml