

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120424\
 Data File : PS028692.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2024 11:19
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 23:29:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	7.721	1356.0E6	615.2E6	505.545	456.686
Target Compounds							
1) T	Dalapon	2.674f	2.723f	12012863	3948273	4.140	1.808 #
2) T	3,5-DICHL...	6.385	0.000	1006059	0	<MDL	N.D. #
3) T	4-Nitroph...	7.019	0.000	7194990	0	4.186	N.D. #
5) T	DICAMBA	7.413	7.918	1000009	5280110	<MDL	<MDL #
7) T	MCPA	7.782f	8.237f	953703	10452377	<MDL	1.684 #
8) T	DICHLORPROP	8.090f	8.686f	1370280	4266735	<MDL	2.669 #
10) T	Pentachlo...	8.650	0.000	2844416	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.228	9.870	1790276	8403668	<MDL	<MDL #
12) T	2,4,5-T	9.525	10.290	6740468	9508025	<MDL	1.021 #
13) T	2,4-DB	10.088	0.000	1106009	0	<MDL	N.D. #
14) T	DINOSEB	11.289	0.000	8166017	0	<MDL	N.D. #
15) T	Picloram	11.121	12.330	48699093	21892933	1.638	1.698
16) T	DCPA	11.582	12.330f	8858169	21892933	<MDL	1.973 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120424\
Data File : PS028692.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2024 11:19
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 23:29:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

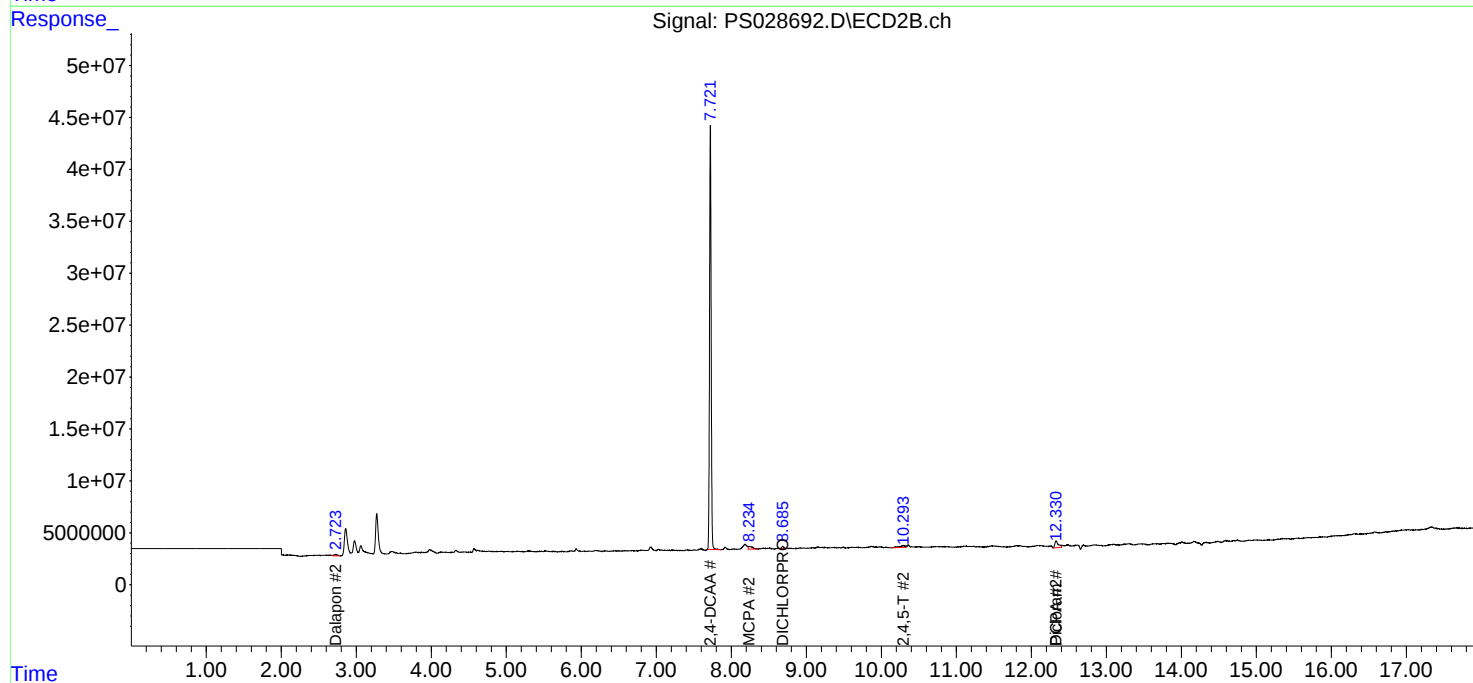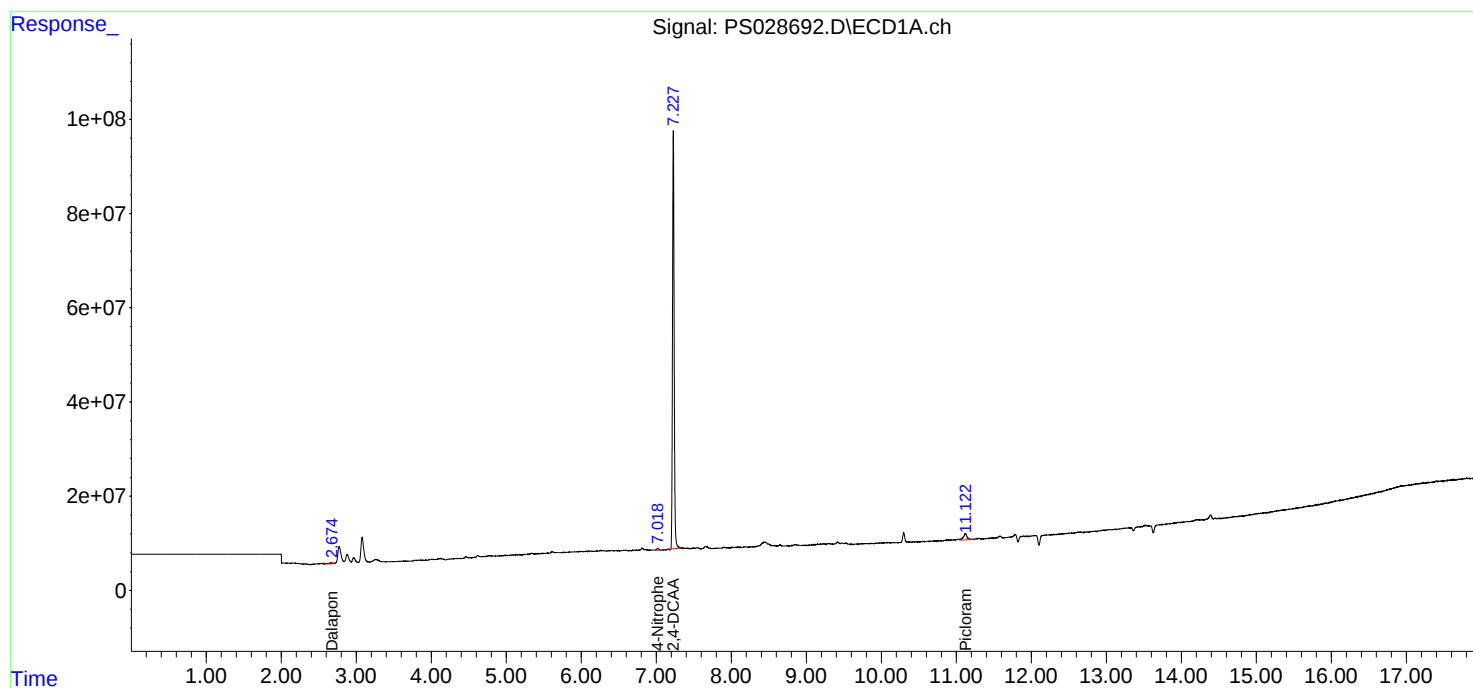


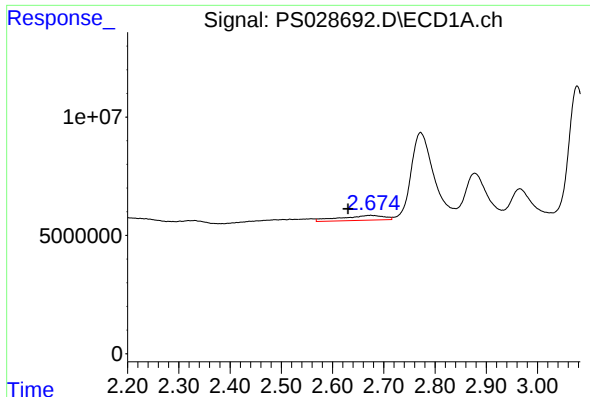

#1 Dalapon


R.T.: 2.674 min
Delta R.T.: 0.044 min
Response: 12012863
Conc: 4.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

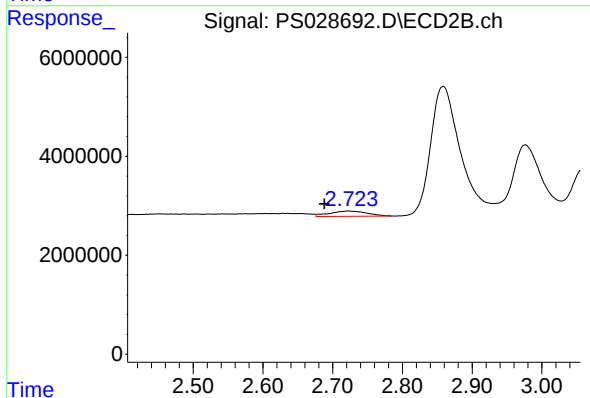


#1 Dalapon

R.T.: 2.723 min
Delta R.T.: 0.034 min
Response: 3948273
Conc: 1.81 ng/ml

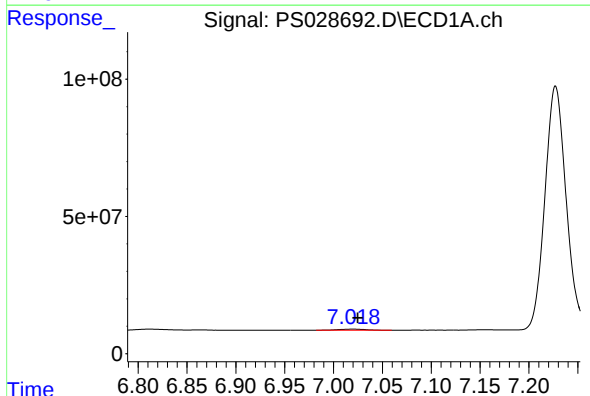


#3 4-Nitrophenol

R.T.: 7.019 min
Delta R.T.: -0.005 min
Response: 7194990
Conc: 4.19 ng/ml

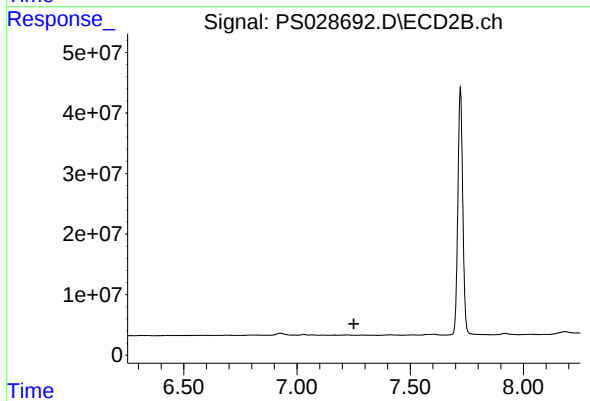

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.251 min
Response: 0
Conc: N.D.

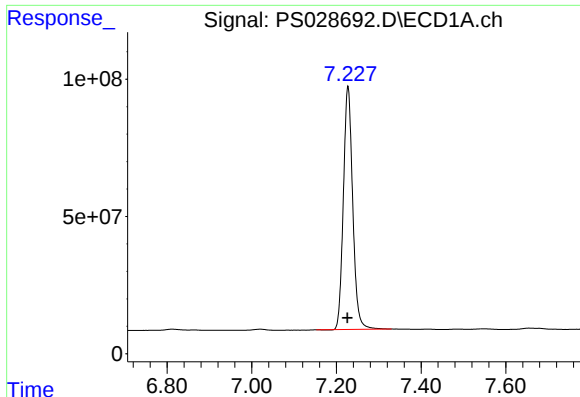

#4 2,4-DCAA


R.T.: 7.227 min
Delta R.T.: 0.001 min
Response: 1356043857
Conc: 505.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

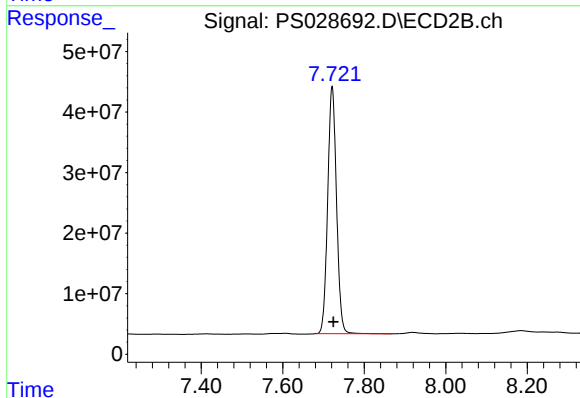


#4 2,4-DCAA

R.T.: 7.721 min
Delta R.T.: -0.003 min
Response: 615169601
Conc: 456.69 ng/ml

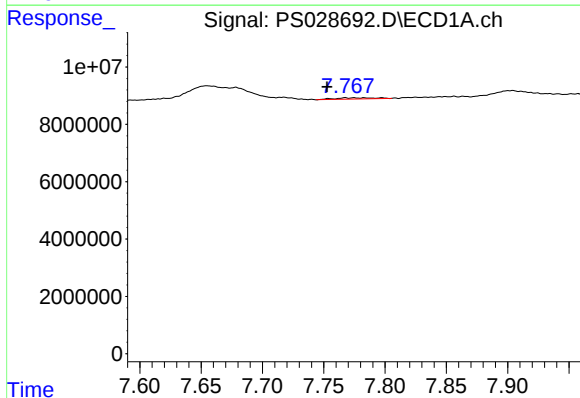


#7 MCPA

R.T.: 7.782 min
Delta R.T.: 0.029 min
Response: 953703
Conc: N.D.

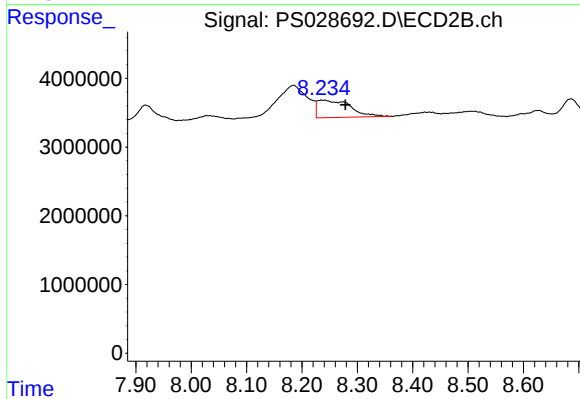

#7 MCPA


R.T.: 8.237 min
Delta R.T.: -0.042 min
Response: 10452377
Conc: 1.68 ug/ml

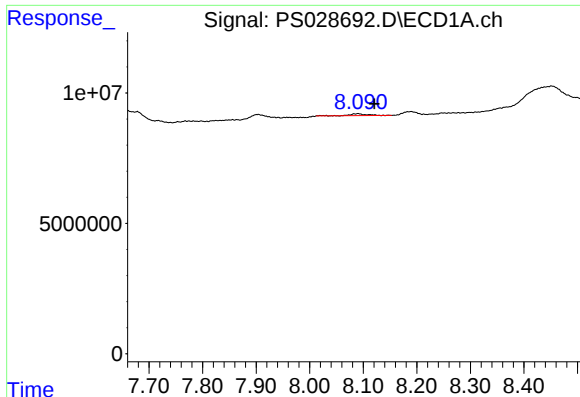

#8 DICHLORPROP


R.T.: 8.090 min
Delta R.T.: -0.031 min
Response: 1370280
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

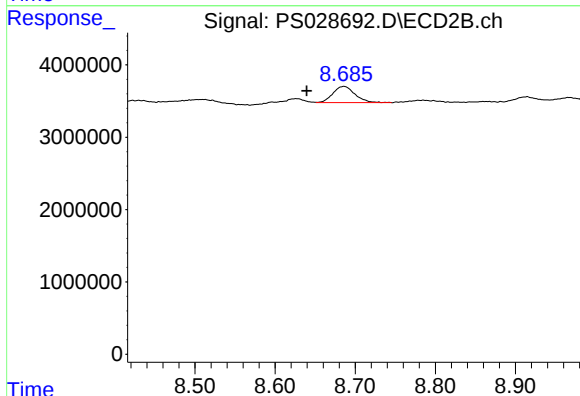


#8 DICHLORPROP

R.T.: 8.686 min
Delta R.T.: 0.046 min
Response: 4266735
Conc: 2.67 ng/ml

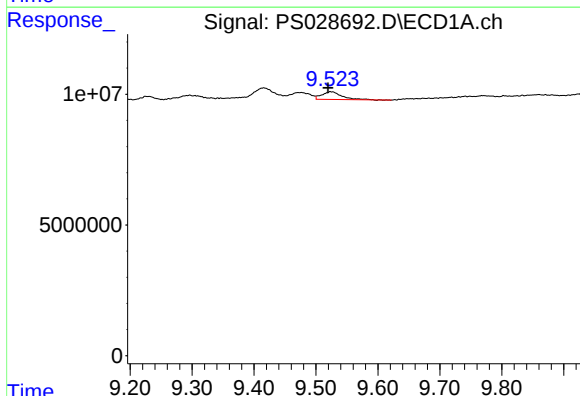


#12 2,4,5-T

R.T.: 9.525 min
Delta R.T.: 0.005 min
Response: 6740468
Conc: N.D.

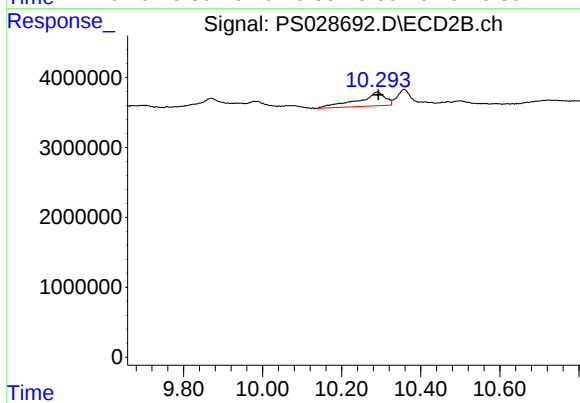

#12 2,4,5-T


R.T.: 10.290 min
Delta R.T.: -0.002 min
Response: 9508025
Conc: 1.02 ng/ml

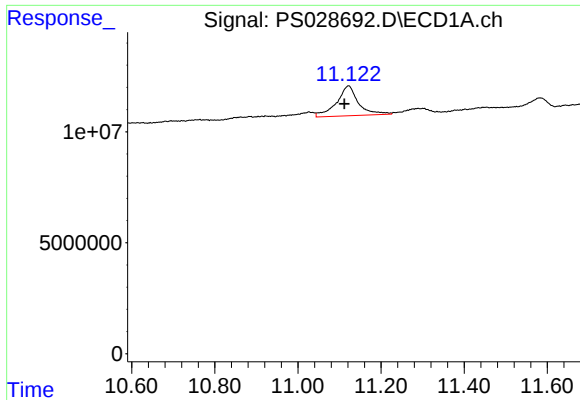

#15 Picloram


R.T.: 11.121 min
Delta R.T.: 0.010 min
Response: 48699093
Conc: 1.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

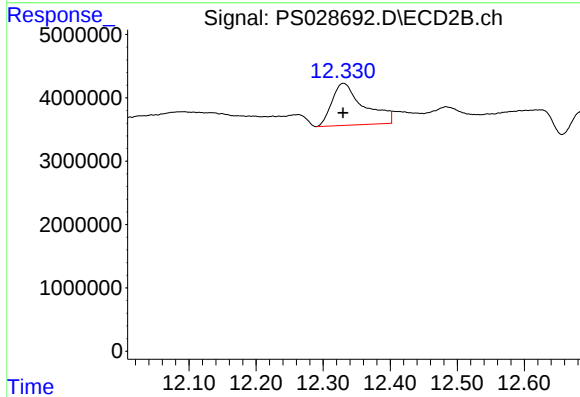


#15 Picloram

R.T.: 12.330 min
Delta R.T.: 0.000 min
Response: 21892933
Conc: 1.70 ng/ml

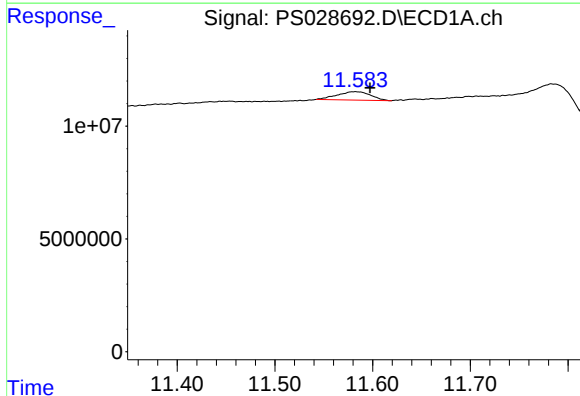

#16 DCPA

R.T.: 11.582 min
Delta R.T.: -0.015 min
Response: 8858169
Conc: N.D.

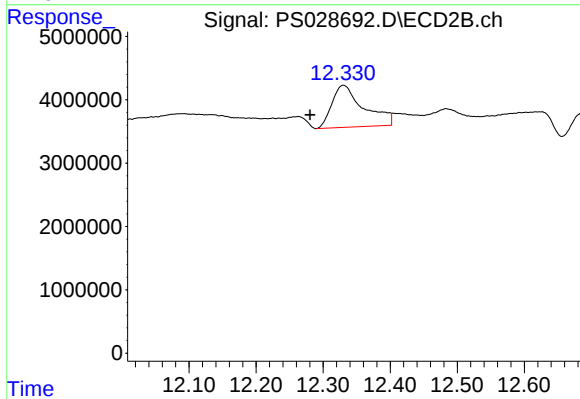

#16 DCPA

R.T.: 12.330 min
Delta R.T.: 0.050 min
Response: 21892933
Conc: 1.97 ng/ml