

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120425\
 Data File : PS032607.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2025 11:33
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 00:39:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120325.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 03 13:46:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.016	7.381	2075.9E6	1613.3E6	375.814	300.916
Target Compounds							
2) T	3,5-DICHL...	0.000	6.407f	0	5545845	N.D.	<MDL
5) T	DICAMBA	0.000	7.587	0	3209368	N.D.	<MDL
7) T	MCPA	0.000	7.952f	0	103.0E6	N.D.	6.205
8) T	DICHLORPROP	0.000	8.322f	0	28106574	N.D.	5.658
9) T	2,4-D	0.000	8.656f	0	1381488	N.D.	<MDL
10) T	Pentachlo...	0.000	9.092	0	2399200	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	9.500	0	22906821	N.D.	<MDL
12) T	2,4,5-T	0.000	9.926	0	41199194	N.D.	1.475
13) T	2,4-DB	0.000	10.480	0	37866677	N.D.	9.296
14) T	DINOSEB	0.000	10.866	0	259.5E6	N.D.	14.347
16) T	DCPA	0.000	11.820f	0	39354403	N.D.	1.157



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120425\
Data File : PS032607.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2025 11:33
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 00:39:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120325.M
Quant Title : 8080.M
QLast Update : Wed Dec 03 13:46:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

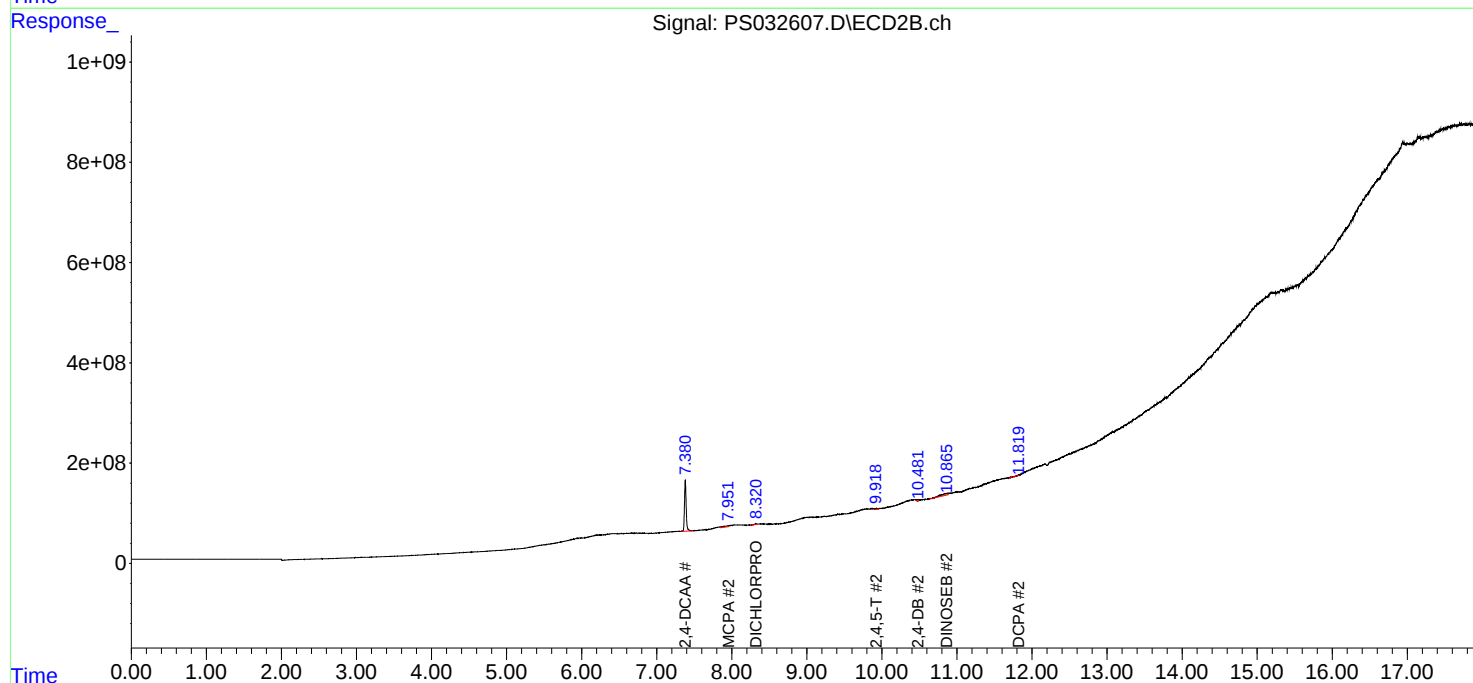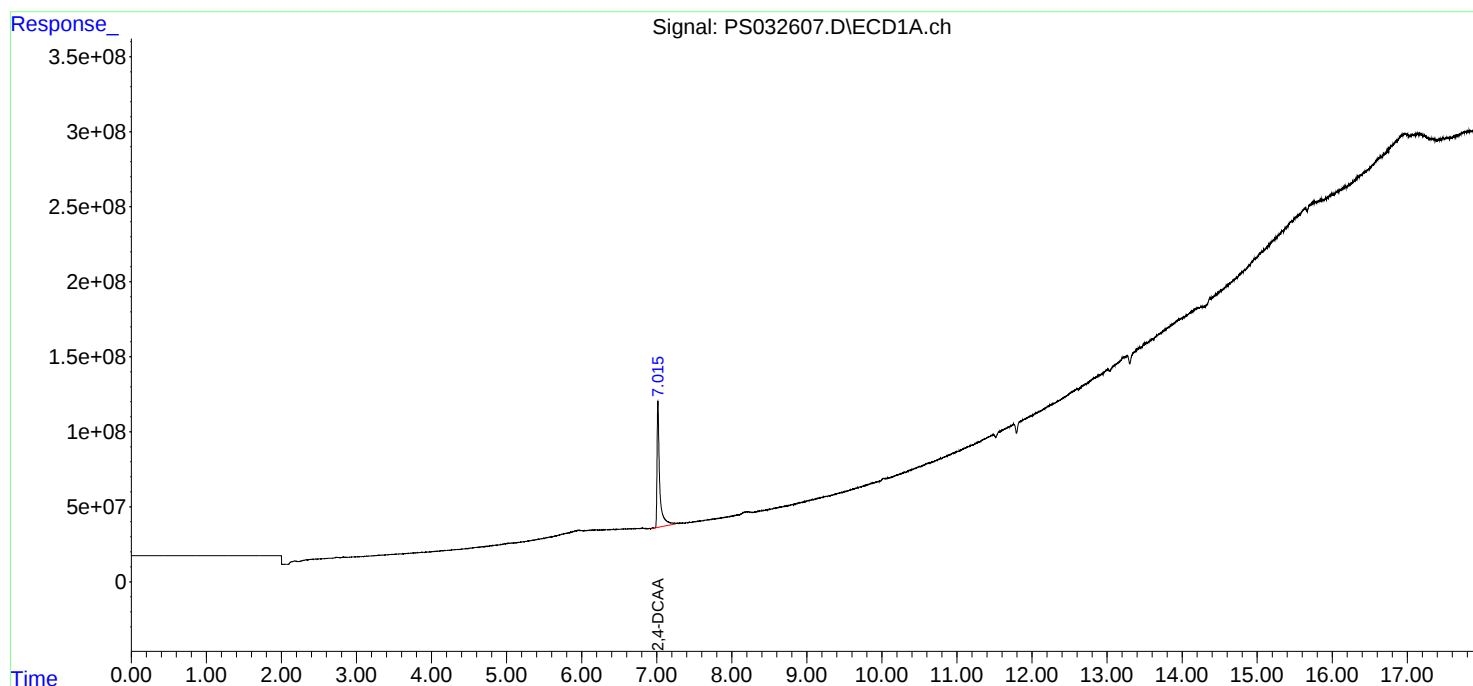


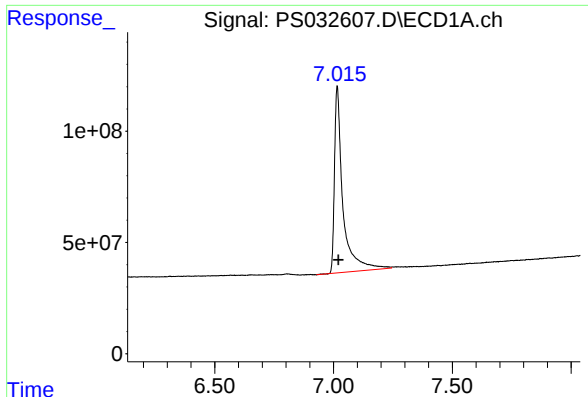

#4 2,4-DCAA


R.T.: 7.016 min
Delta R.T.: -0.006 min
Response: 2075868651
Conc: 375.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

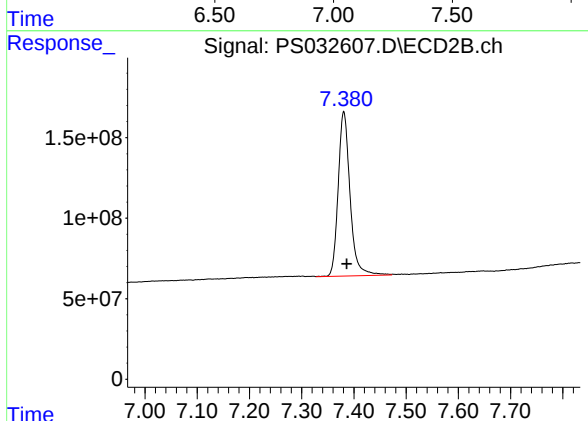


#4 2,4-DCAA

R.T.: 7.381 min
Delta R.T.: -0.006 min
Response: 1613273835
Conc: 300.92 ng/ml

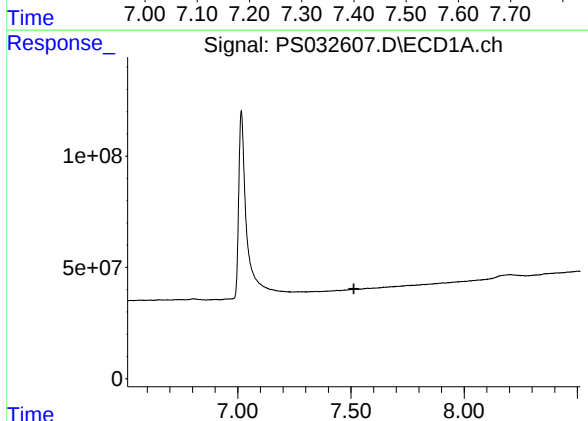


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.513 min
Response: 0
Conc: N.D.

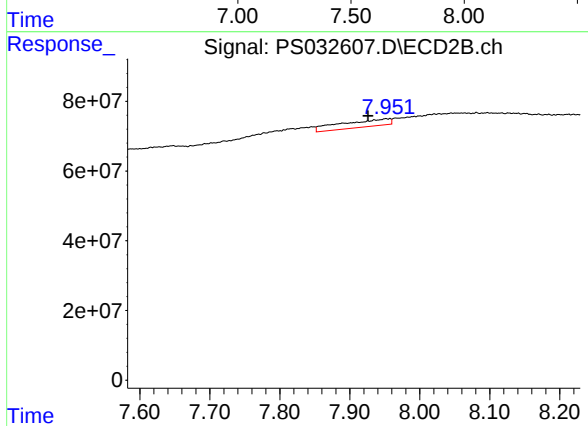

#7 MCPA


R.T.: 7.952 min
Delta R.T.: 0.026 min
Response: 103042680
Conc: 6.21 ug/ml

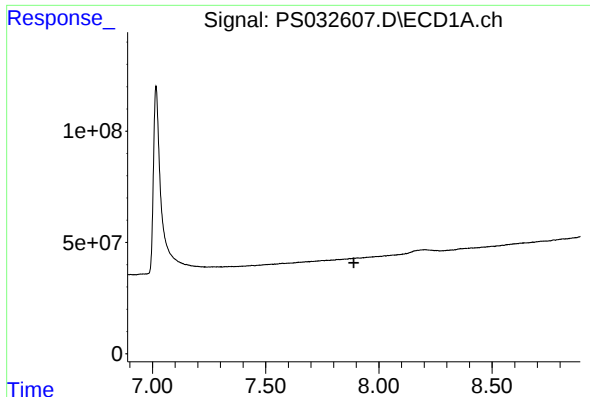

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.890 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

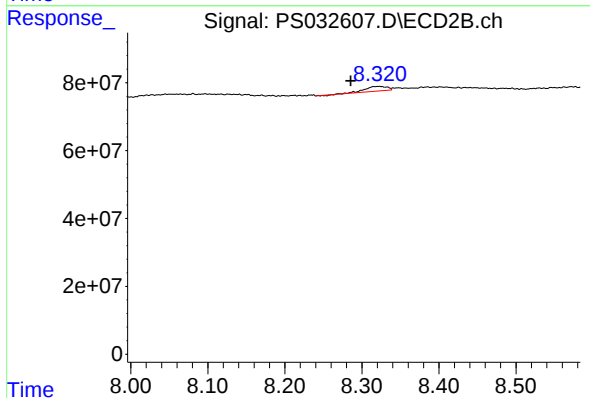


#8 DICHLORPROP

R.T.: 8.322 min
Delta R.T.: 0.037 min
Response: 28106574
Conc: 5.66 ng/ml

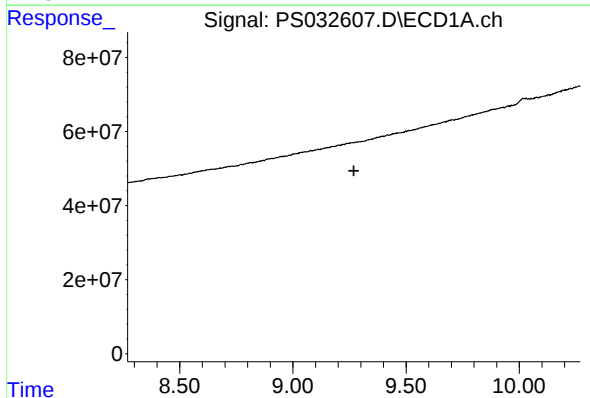


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.269 min
Response: 0
Conc: N.D.

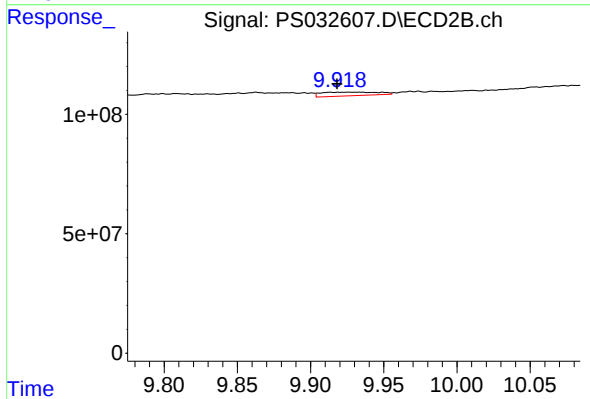

#12 2,4,5-T


R.T.: 9.926 min
Delta R.T.: 0.008 min
Response: 41199194
Conc: 1.48 ng/ml

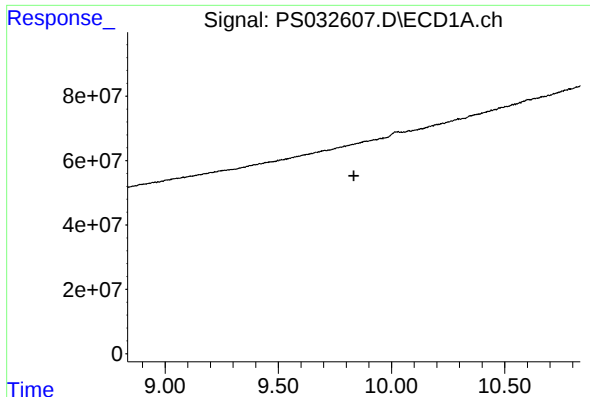

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.834 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

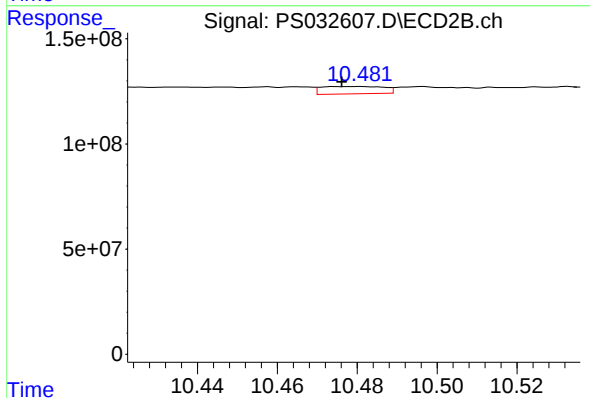


#13 2,4-DB

R.T.: 10.480 min
Delta R.T.: 0.004 min
Response: 37866677
Conc: 9.30 ng/ml

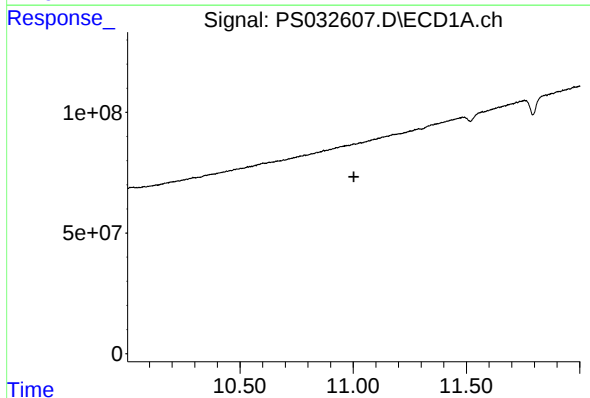


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.003 min
Response: 0
Conc: N.D.

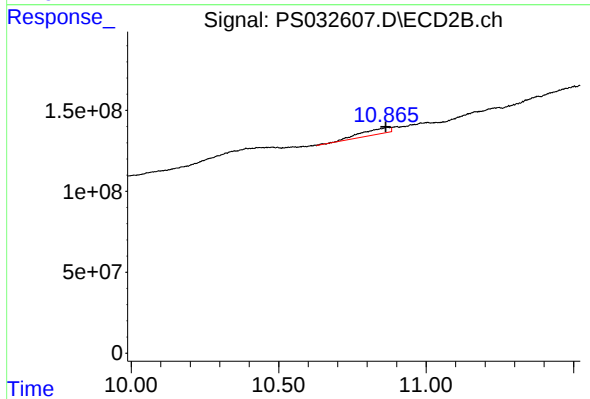

#14 DINOSEB


R.T.: 10.866 min
Delta R.T.: 0.003 min
Response: 259461618
Conc: 14.35 ng/ml

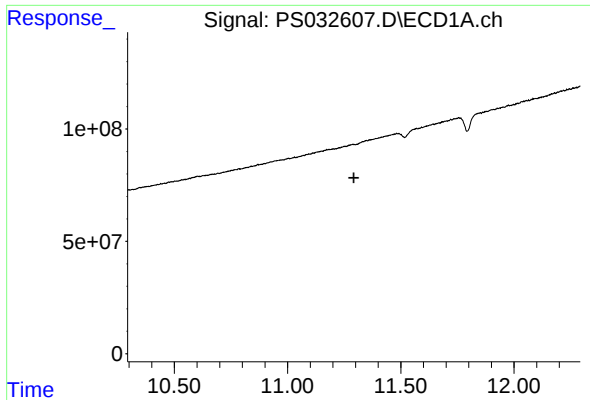

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

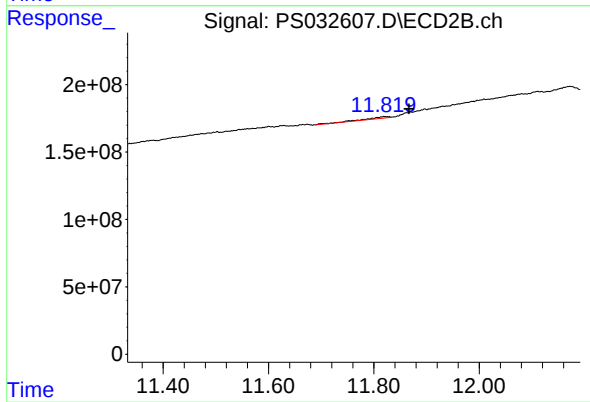

#16 DCPA

R.T.: 11.820 min
Delta R.T.: -0.047 min
Response: 39354403
Conc: 1.16 ng/ml