

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120425\
 Data File : PS032615.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2025 18:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 00:43:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120325.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 03 13:46:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.014	7.378	1885.0E6	1511.1E6	341.258	281.867
Target Compounds							
2) T	3,5-DICHL...	0.000	6.352f	0	3441102	N.D.	<MDL
6) T	MCP	7.373	7.729f	1953054	2224239	<MDL	<MDL #
7) T	MCPA	0.000	7.929	0	84666119	N.D.	5.099
9) T	2,4-D	0.000	8.613	0	5470492	N.D.	<MDL
10) T	Pentachlo...	0.000	9.081	0	6944018	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	9.503	0	123.3E6	N.D.	4.299
13) T	2,4-DB	9.835	10.474	2229922	22247992	<MDL	5.462 #
14) T	DINOSEB	0.000	10.873	0	467.3E6	N.D.	25.841
15) T	Picloram	0.000	12.029f	0	335.9E6	N.D.	9.330
16) T	DCPA	0.000	11.879	0	53749254	N.D.	1.580



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120425\
Data File : PS032615.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2025 18:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 00:43:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120325.M
Quant Title : 8080.M
QLast Update : Wed Dec 03 13:46:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

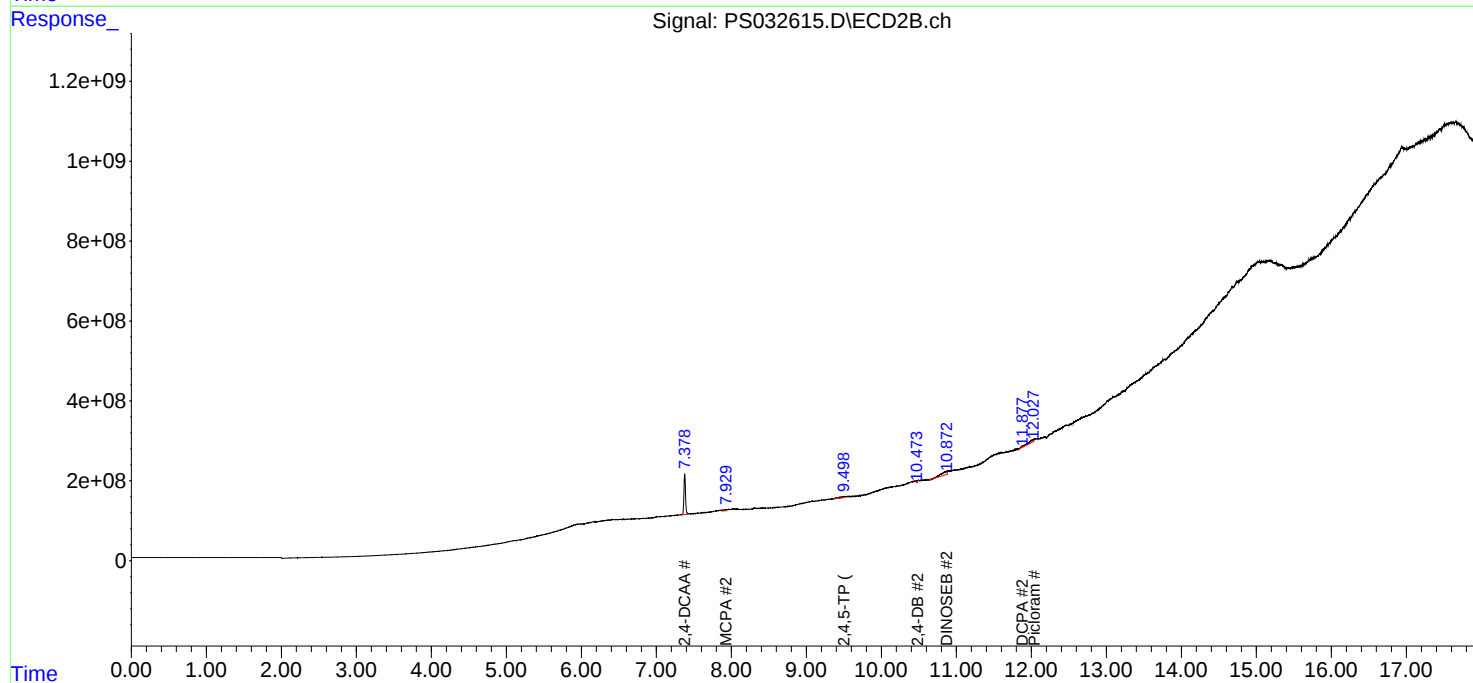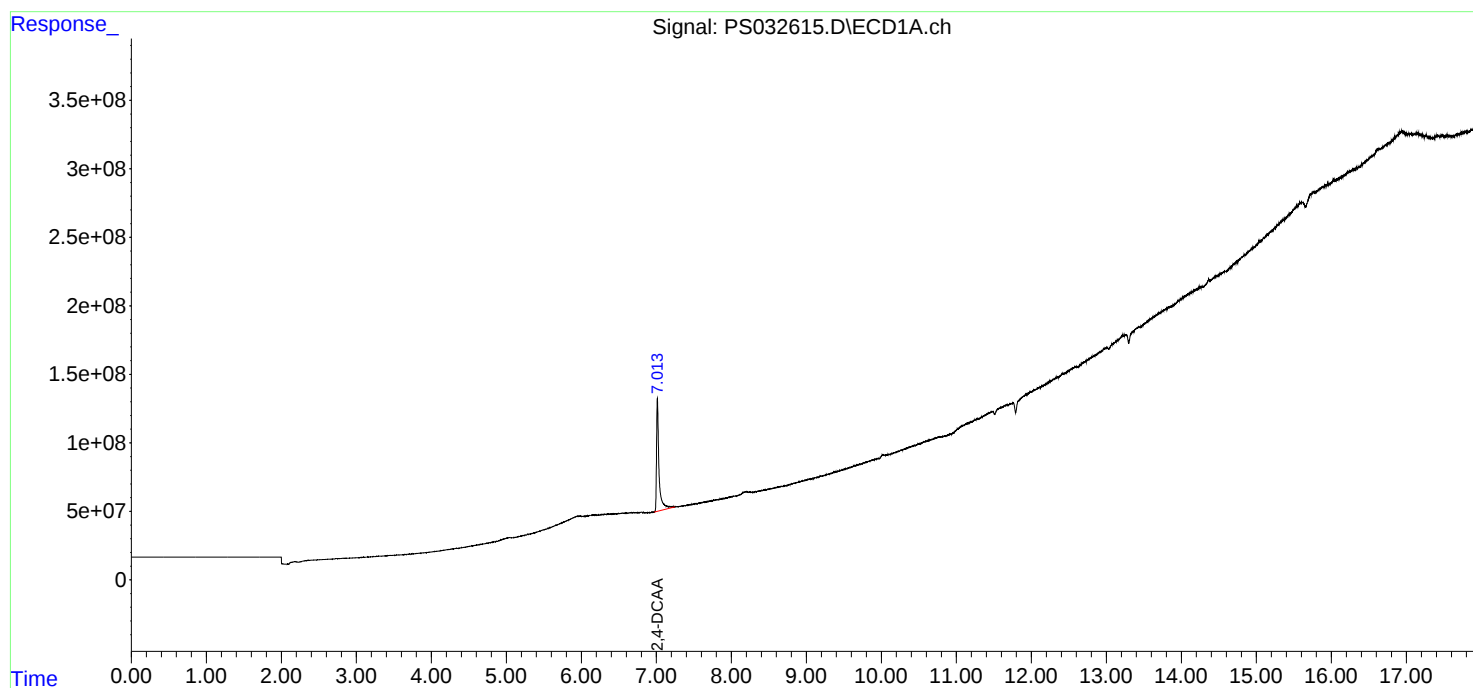


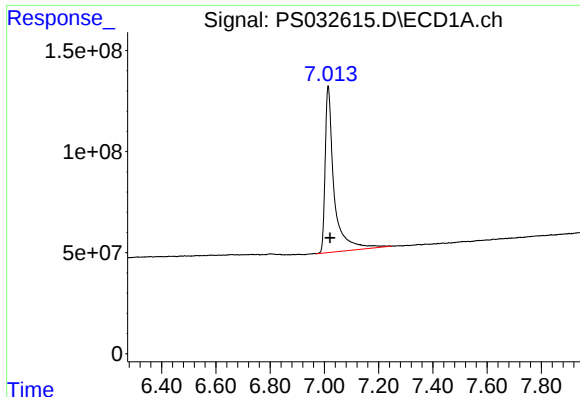

#4 2,4-DCAA


R.T.: 7.014 min
Delta R.T.: -0.007 min
Response: 1884993474
Conc: 341.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

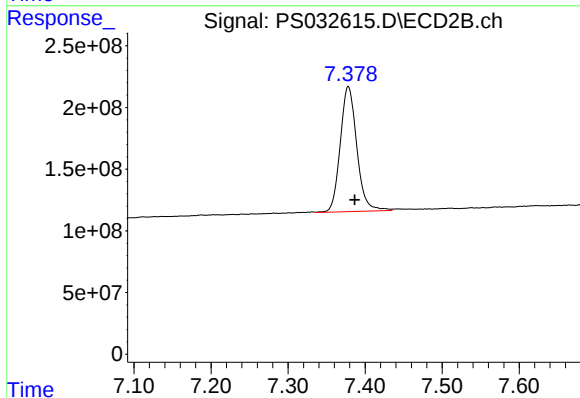


#4 2,4-DCAA

R.T.: 7.378 min
Delta R.T.: -0.008 min
Response: 1511147311
Conc: 281.87 ng/ml

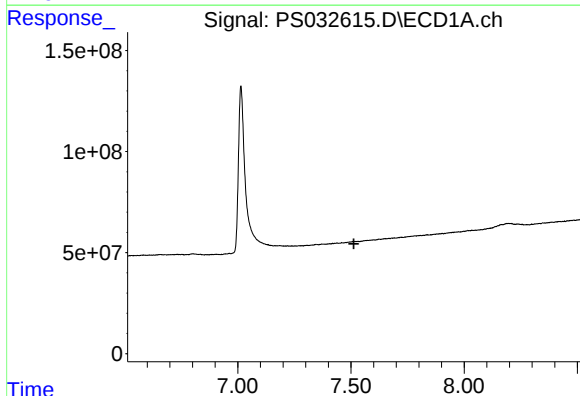


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.513 min
Response: 0
Conc: N.D.

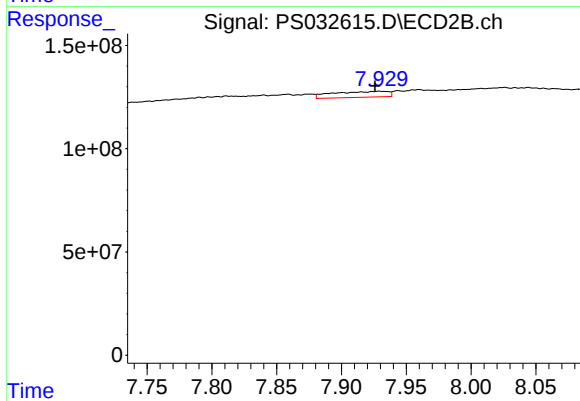

#7 MCPA


R.T.: 7.929 min
Delta R.T.: 0.003 min
Response: 84666119
Conc: 5.10 ug/ml

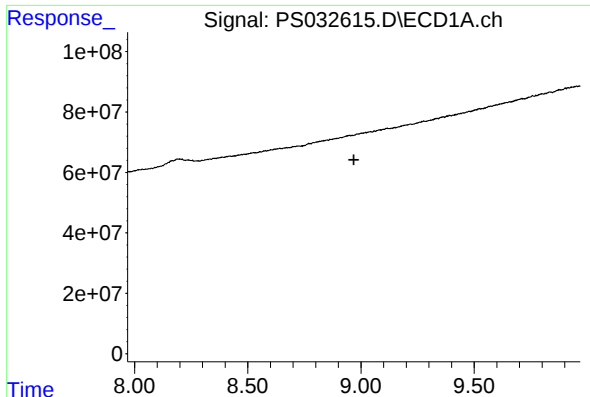

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 8.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

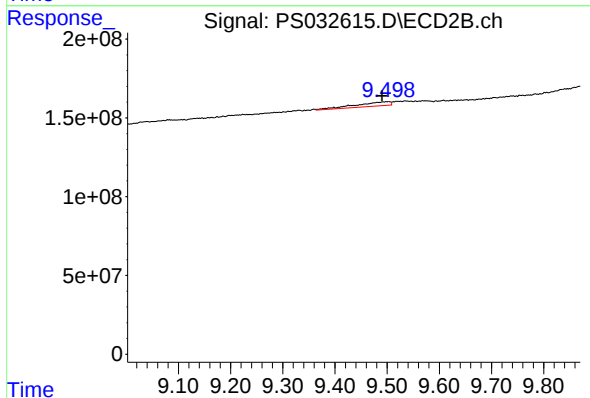


#11 2,4,5-TP (SILVEX)

R.T.: 9.503 min
Delta R.T.: 0.013 min
Response: 123339268
Conc: 4.30 ng/ml

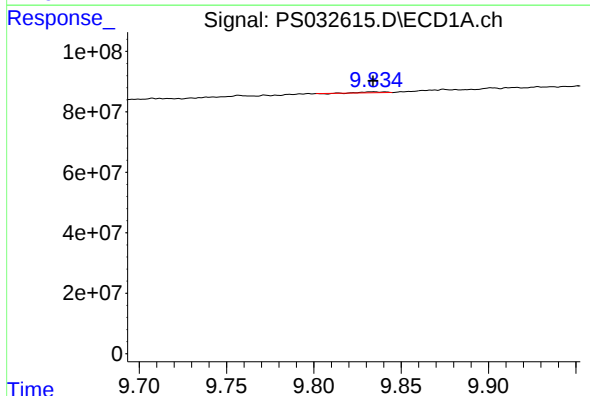


#13 2,4-DB

R.T.: 9.835 min
Delta R.T.: 0.000 min
Response: 2229922
Conc: N.D.

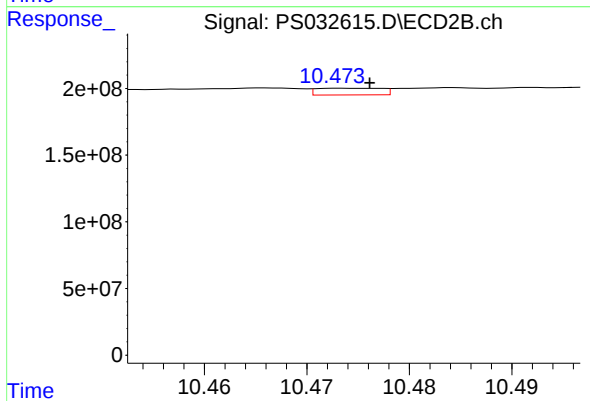

#13 2,4-DB


R.T.: 10.474 min
Delta R.T.: -0.002 min
Response: 22247992
Conc: 5.46 ng/ml

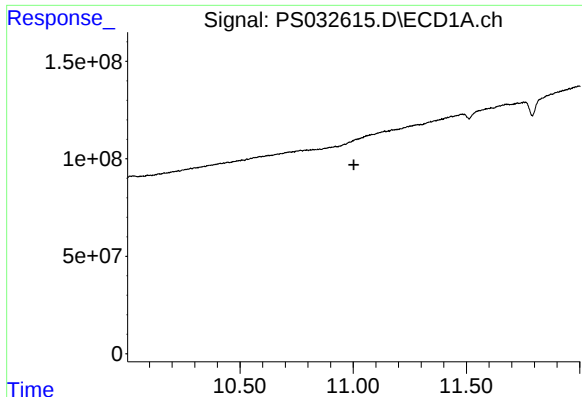

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

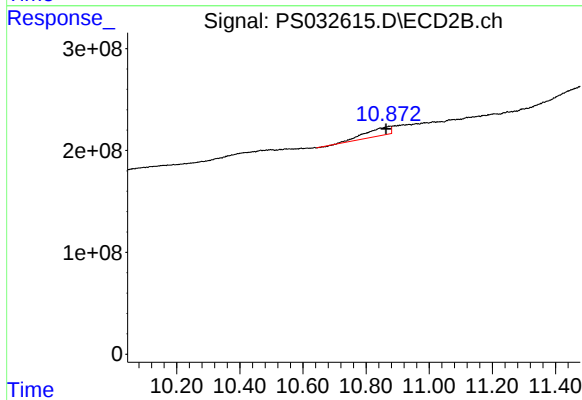


#14 DINOSEB

R.T.: 10.873 min
Delta R.T.: 0.009 min
Response: 467325760
Conc: 25.84 ng/ml

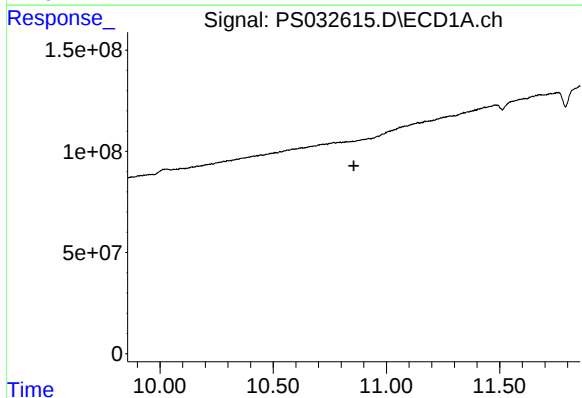


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 10.856 min
Response: 0
Conc: N.D.

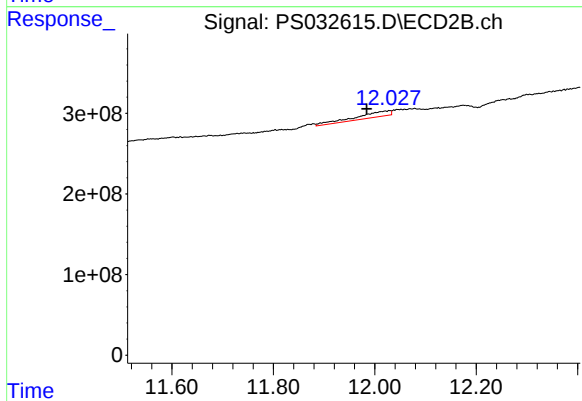

#15 Picloram


R.T.: 12.029 min
Delta R.T.: 0.045 min
Response: 335853433
Conc: 9.33 ng/ml

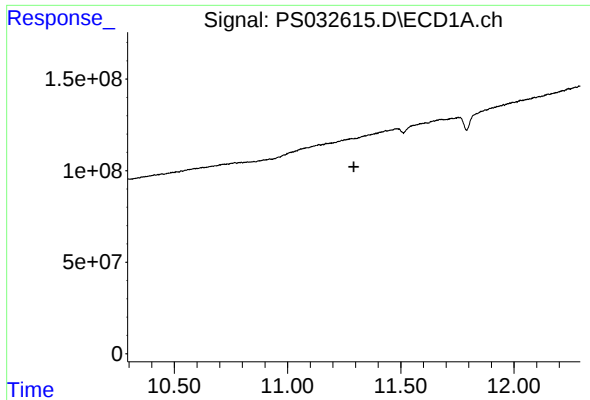

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

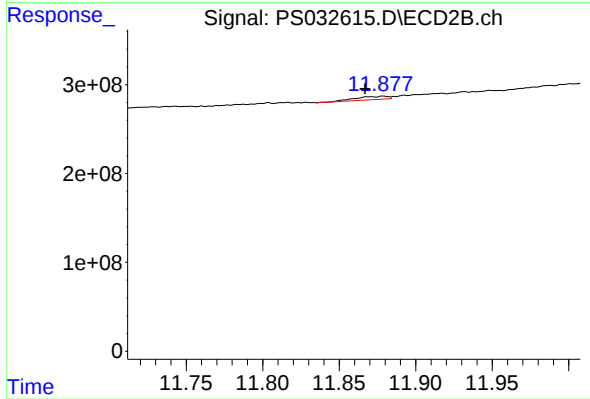

#16 DCPA

R.T.: 11.879 min
Delta R.T.: 0.012 min
Response: 53749254
Conc: 1.58 ng/ml