

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120425\
 Data File : PS032619.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2025 20:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 00:45:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120325.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 03 13:46:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.011	7.377	1675.9E6	1558.2E6	303.398	290.641
Target Compounds							
2) T	3,5-DICHL...	6.232	6.360	5176876	1977449	<MDL	<MDL #
5) T	DICAMBA	7.195	7.583	7538878	6749552	<MDL	<MDL #
8) T	DICHLORPROP	0.000	8.312f	0	46455220	N.D.	9.351
10) T	Pentachlo...	0.000	9.079	0	12793196	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	9.517f	0	242.0E6	N.D.	8.435



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120425\
Data File : PS032619.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2025 20:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 00:45:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120325.M
Quant Title : 8080.M
QLast Update : Wed Dec 03 13:46:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

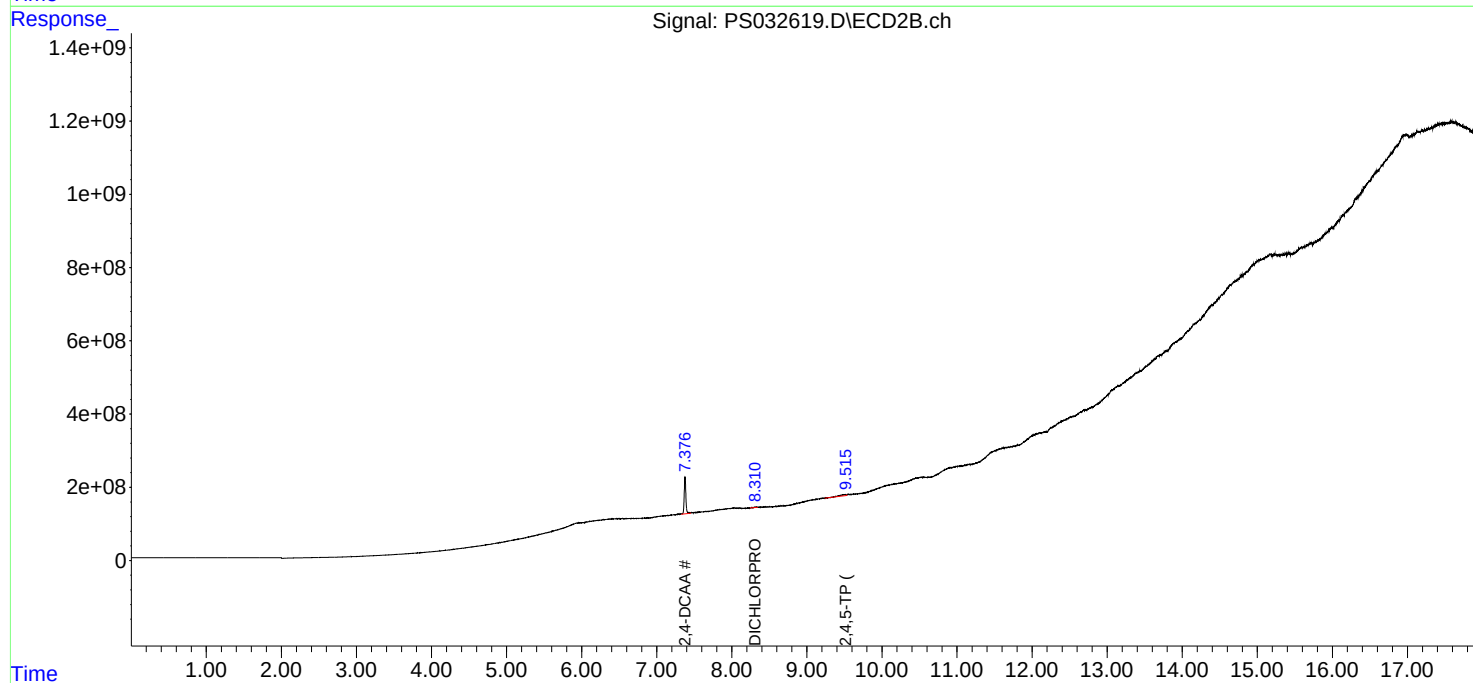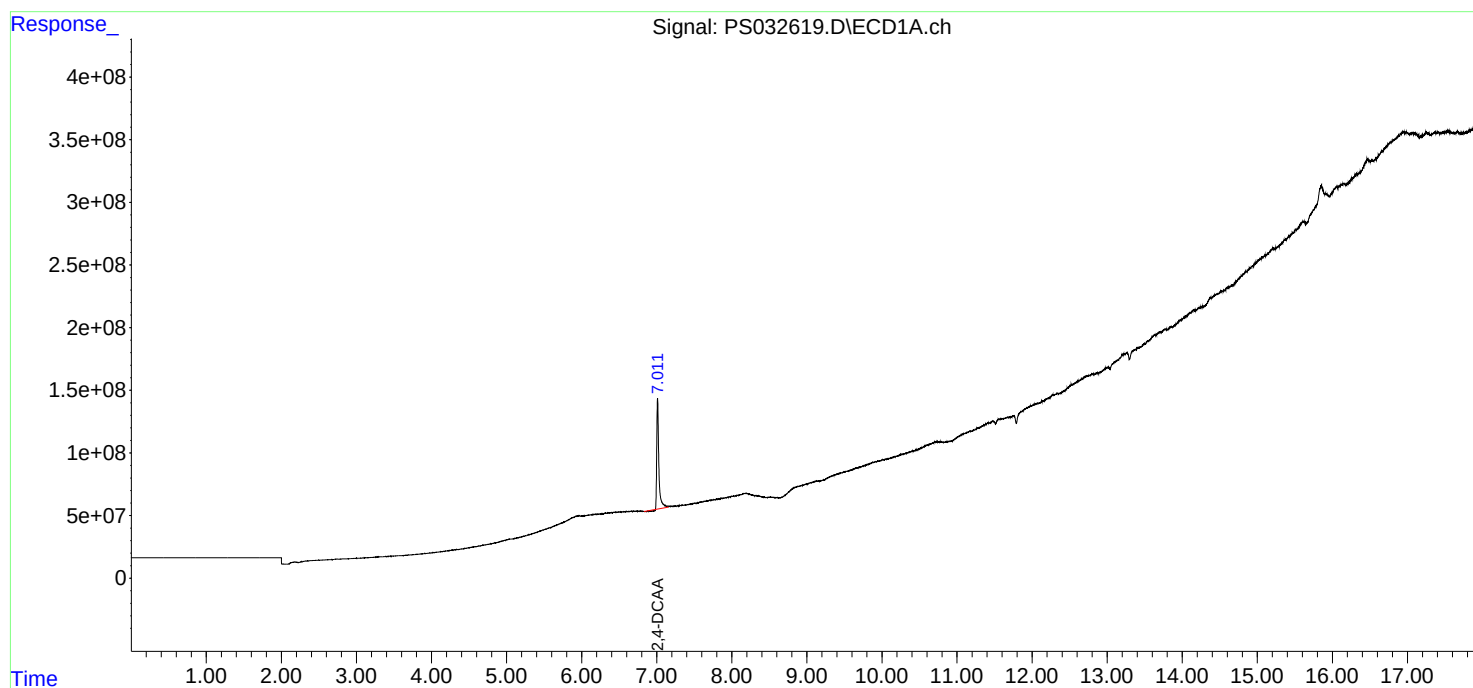


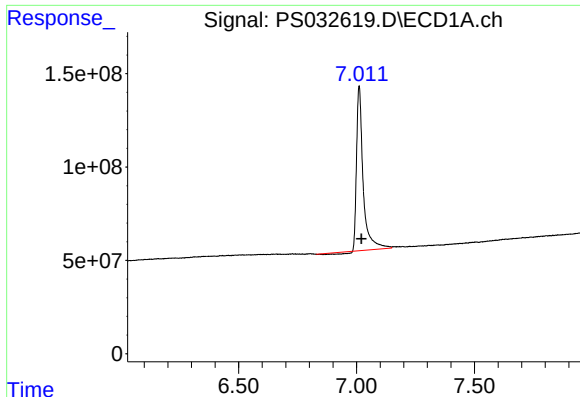

#4 2,4-DCAA


R.T.: 7.011 min
Delta R.T.: -0.010 min
Response: 1675866348
Conc: 303.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

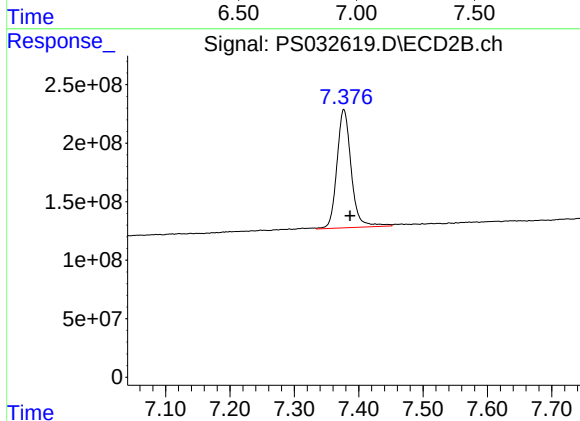


#4 2,4-DCAA

R.T.: 7.377 min
Delta R.T.: -0.010 min
Response: 1558189869
Conc: 290.64 ng/ml

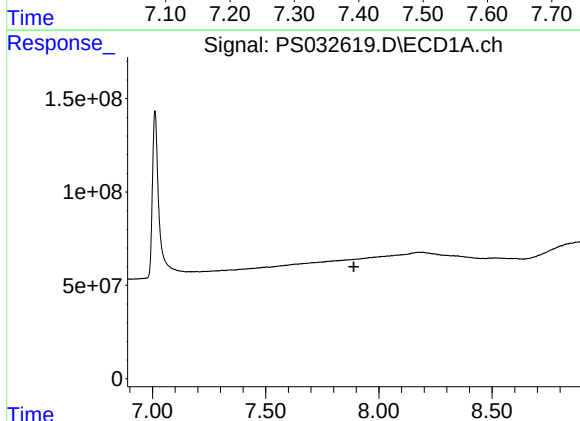


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.890 min
Response: 0
Conc: N.D.

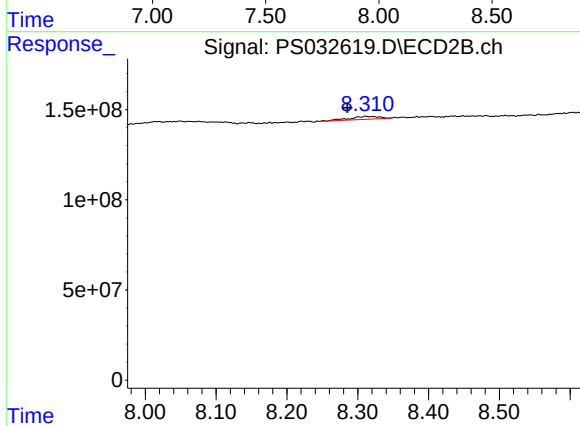

#8 DICHLORPROP


R.T.: 8.312 min
Delta R.T.: 0.026 min
Response: 46455220
Conc: 9.35 ng/ml

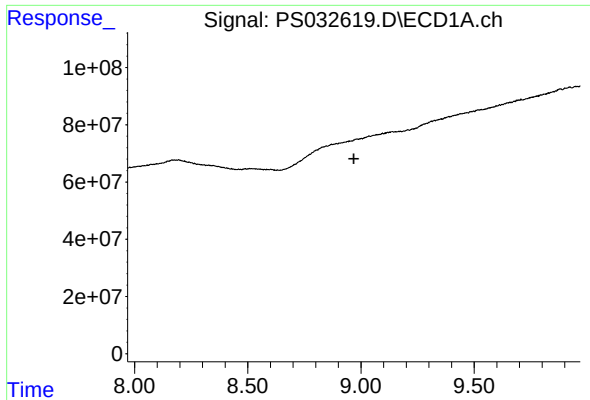

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 8.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

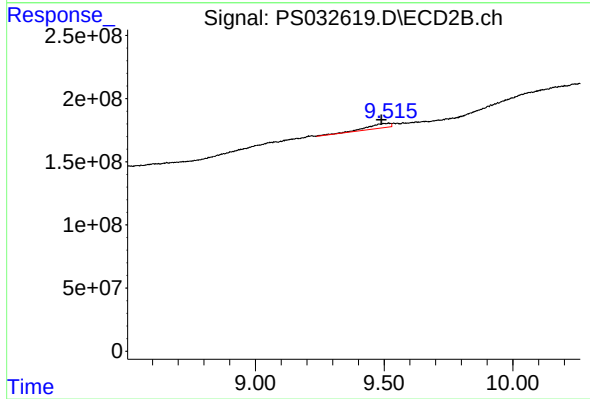

#11 2,4,5-TP (SILVEX)

R.T.: 9.517 min
Delta R.T.: 0.027 min
Response: 241976570
Conc: 8.43 ng/ml