

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120425\
Data File : PS032611.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2025 16:38
Operator : AR\AJ
Sample : PB170818BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB170818BL

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/05/2025
Supervised By :mohammad ahmed 12/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 00:40:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120325.M
Quant Title : 8080.M
QLast Update : Wed Dec 03 13:46:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.009	7.373	1862.2E6	1602.9E6	337.132m	298.985m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120425\
Data File : PS032611.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2025 16:38
Operator : AR\AJ
Sample : PB170818BL
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
PB170818BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/05/2025
Supervised By : mohammad ahmed 12/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 00:40:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120325.M
Quant Title : 8080.M
QLast Update : Wed Dec 03 13:46:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

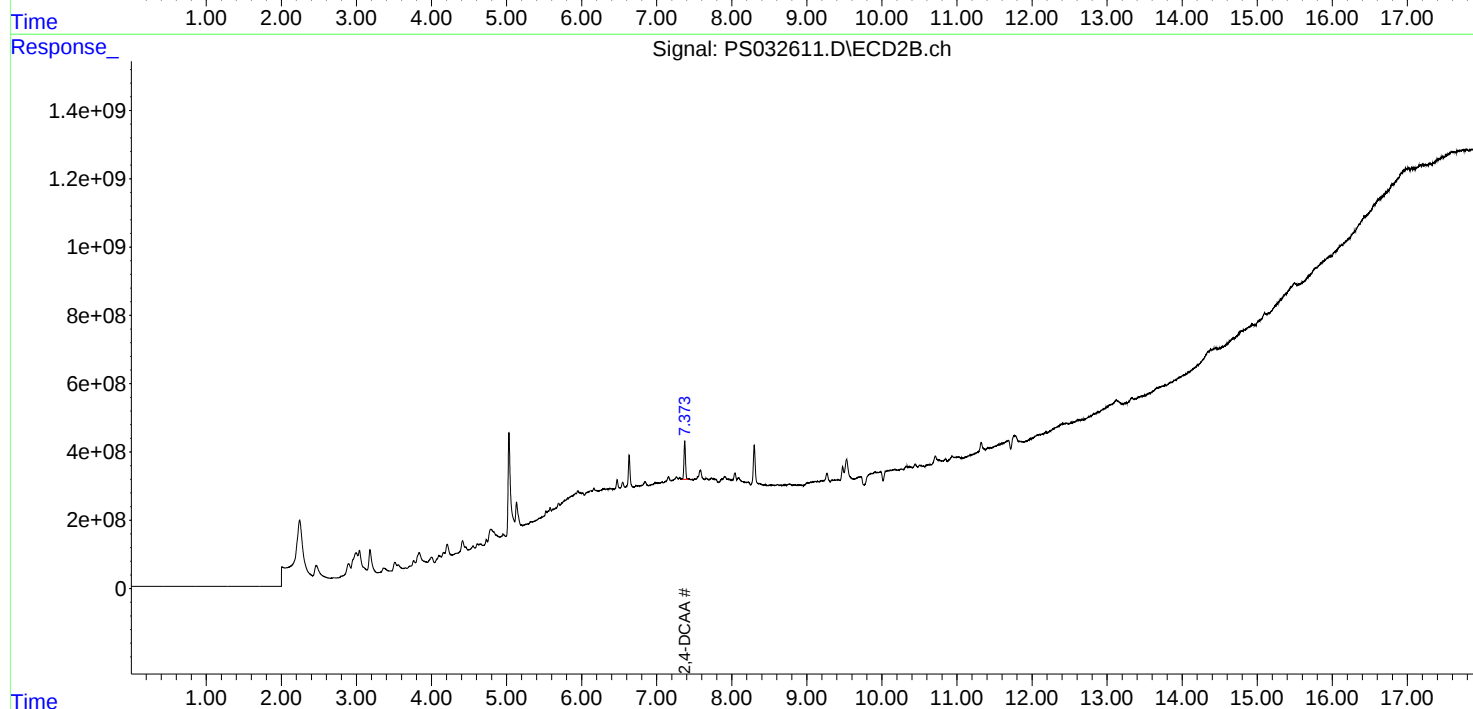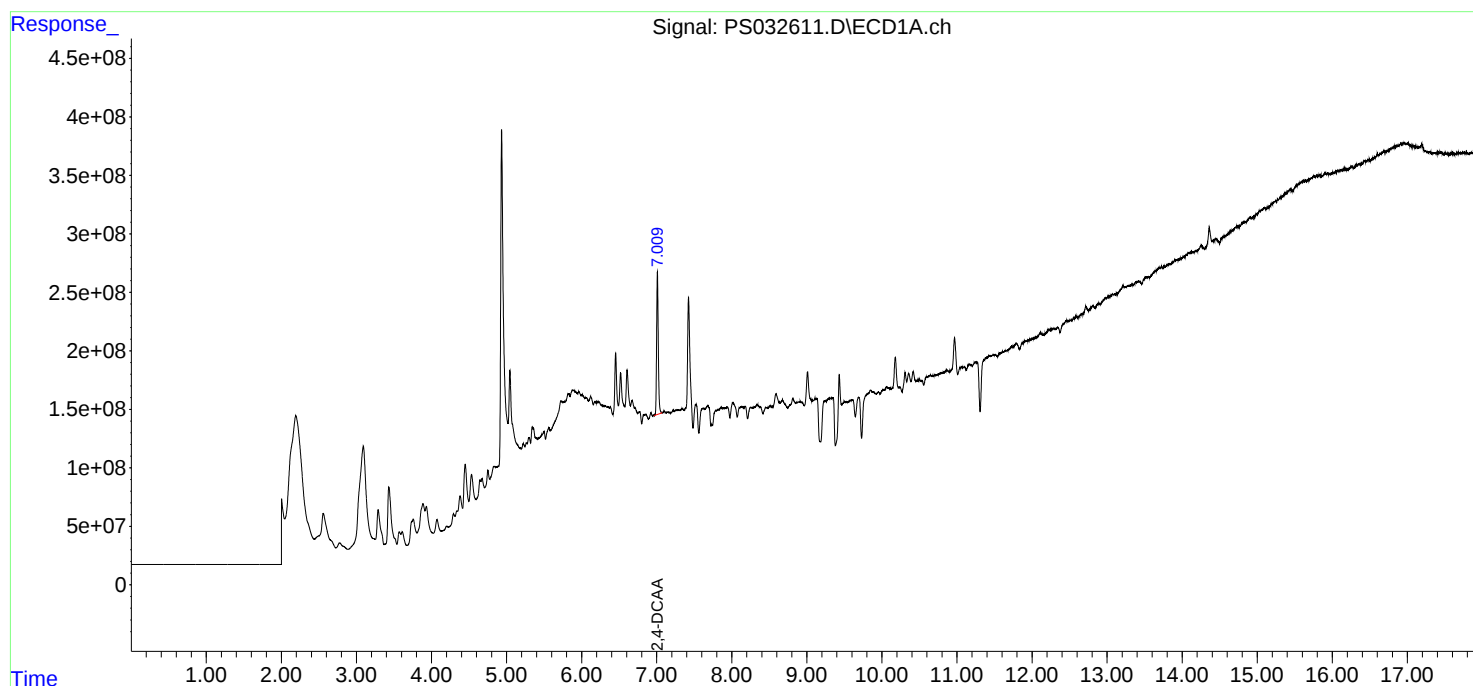

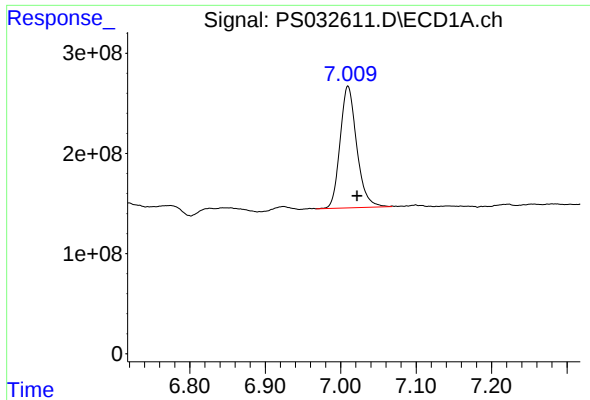


#4 2,4-DCAA

R.T.: 7.009 min
Delta R.T.: -0.012 min
Response: 1862201193
Conc: 337.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB170818BL

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/05/2025
Supervised By :mohammad ahmed 12/08/2025

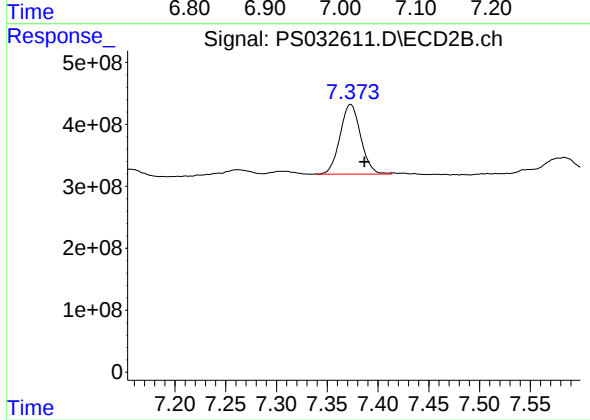

#4 2,4-DCAA

R.T.: 7.373 min
Delta R.T.: -0.014 min
Response: 1602924895
Conc: 298.99 ng/ml m