

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120522\
 Data File : PS021325.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2022 18:20
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 01:16:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
 Quant Title : 8080.M
 QLast Update : Thu Nov 17 00:46:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.412	6.845	1288.1E6	779.6E6	592.404	515.568
Target Compounds							
3) T	4-Nitroph...	6.258	0.000	8475953	0	6.274	N.D. #
7) T	MCPA	6.801f	0.000	25927892	0	2.698	N.D. #
8) T	DICHLORPROP	0.000	7.668	0	4148680	N.D.	2.430
11) T	2,4,5-TP ...	0.000	8.699	0	9389594	N.D.	<MDL
12) T	2,4,5-T	8.373	9.137f	9651605	767025	<MDL	<MDL #
13) T	2,4-DB	8.882	9.639	12360468	562674	5.408	<MDL #
14) T	DINOSEB	9.912	9.937	83316342	1004310	7.264	<MDL #
15) T	Picloram	9.799	0.000	72932949	0	3.627	N.D. #
16) T	DCPA	10.207	0.000	48074818	0	2.543	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120522\
Data File : PS021325.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2022 18:20
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 01:16:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
Quant Title : 8080.M
QLast Update : Thu Nov 17 00:46:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

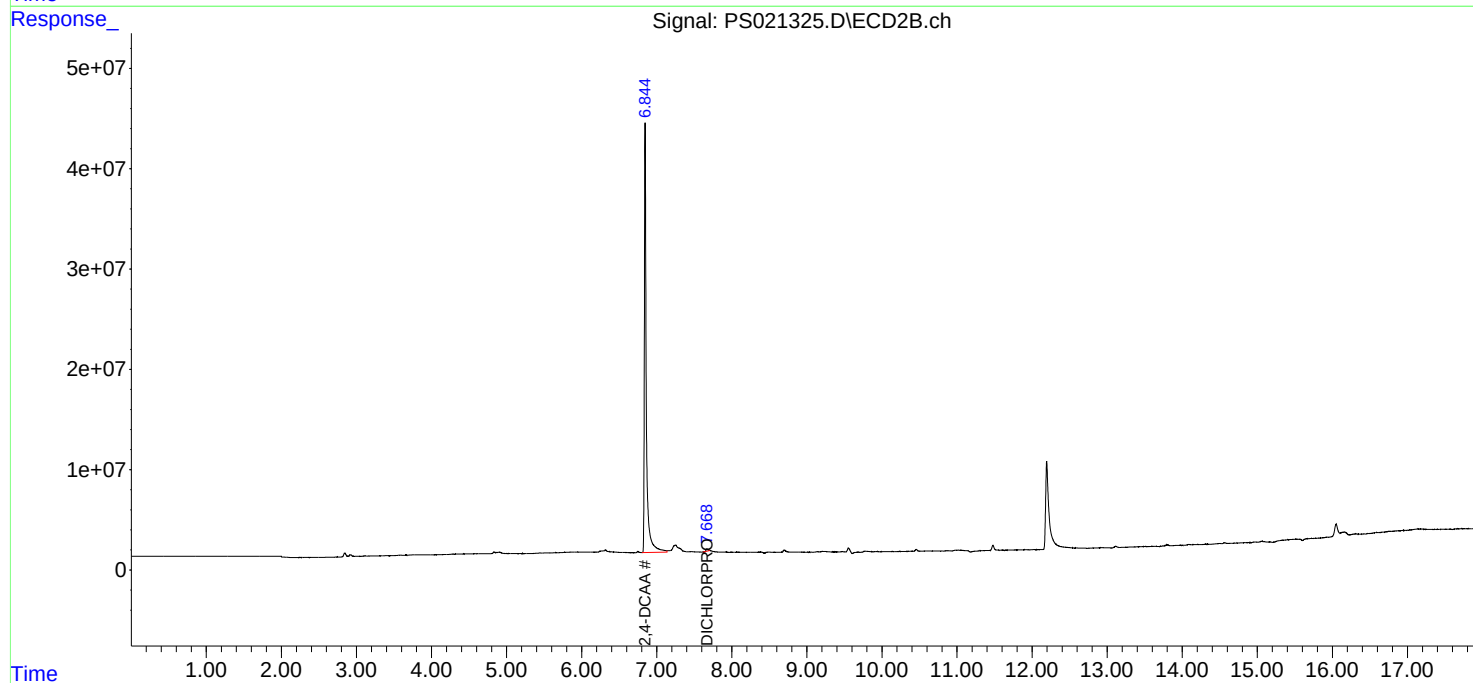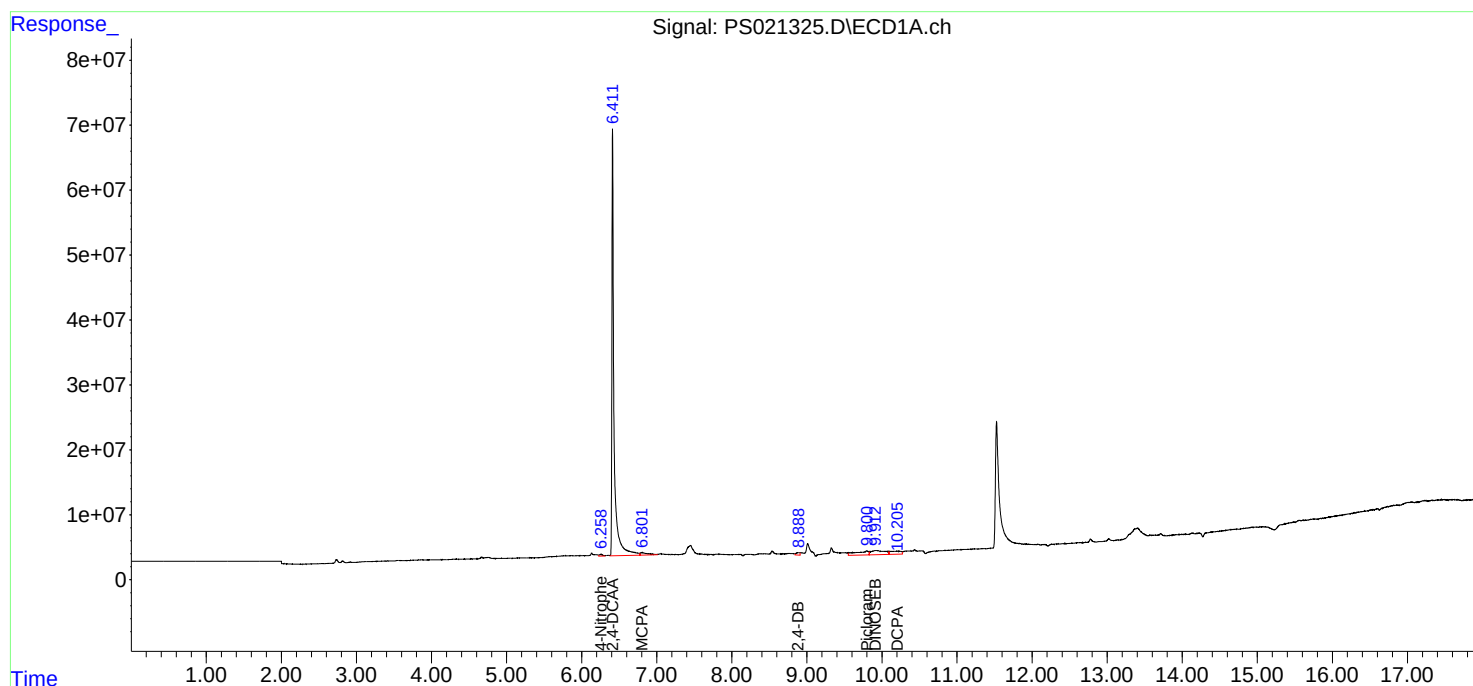


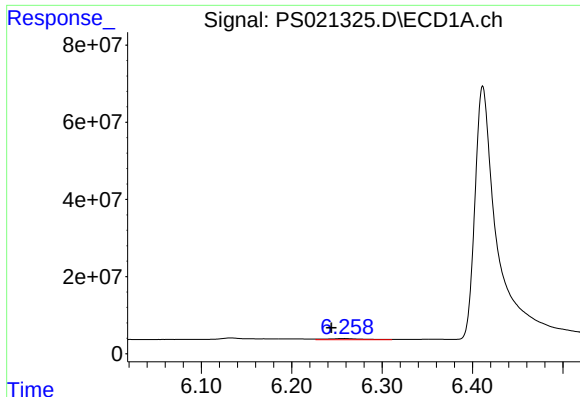

#3 4-Nitrophenol


R.T.: 6.258 min
Delta R.T.: 0.014 min
Response: 8475953
Conc: 6.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

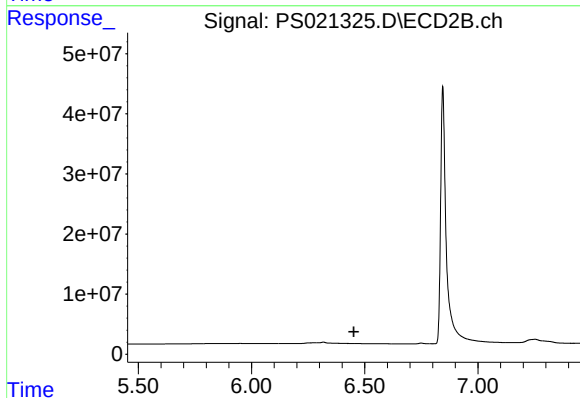


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.452 min
Response: 0
Conc: N.D.

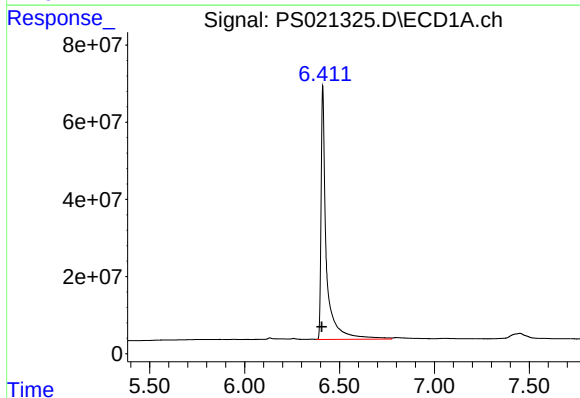


#4 2,4-DCAA

R.T.: 6.412 min
Delta R.T.: 0.005 min
Response: 1288060013
Conc: 592.40 ng/ml

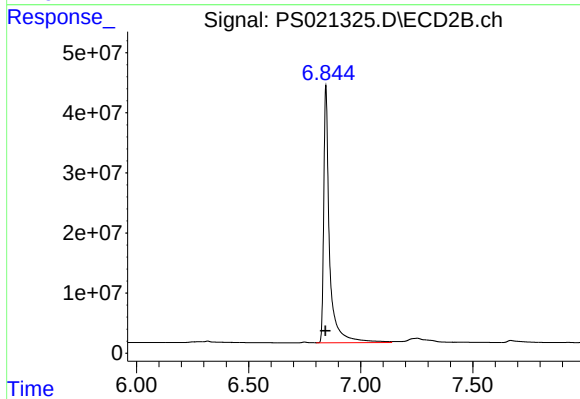

#4 2,4-DCAA


R.T.: 6.845 min
Delta R.T.: 0.003 min
Response: 779599911
Conc: 515.57 ng/ml

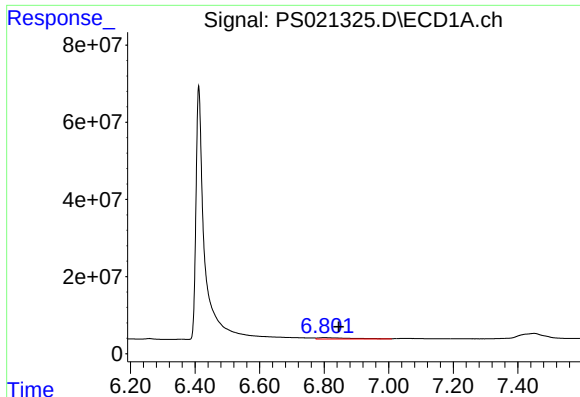

#7 MCPA


R.T.: 6.801 min
Delta R.T.: -0.043 min
Response: 25927892
Conc: 2.70 ug/ml

Instrument :
ECD_S
ClientSampleId :

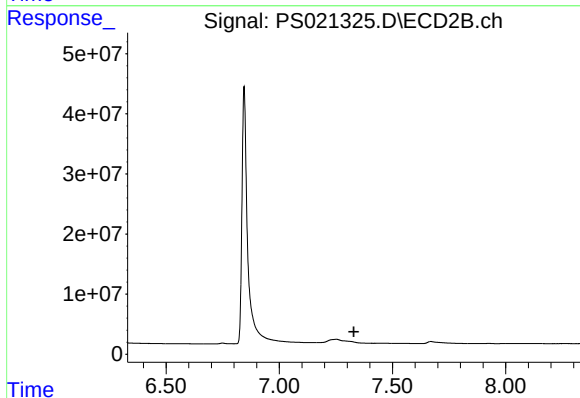


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.330 min
Response: 0
Conc: N.D.

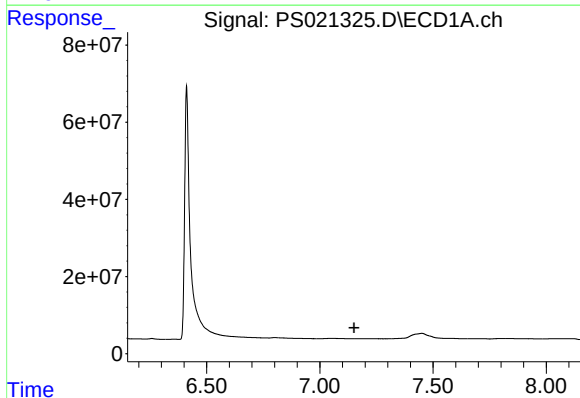


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.151 min
Response: 0
Conc: N.D.

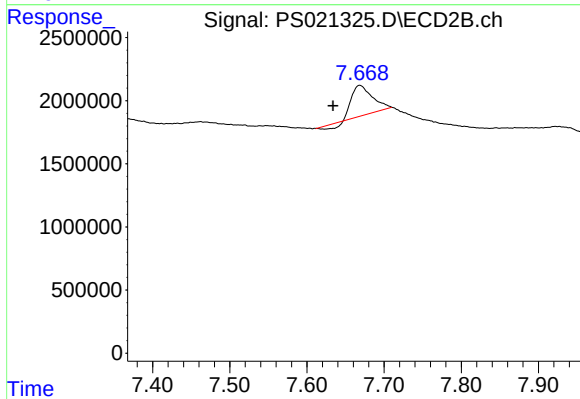

#8 DICHLORPROP


R.T.: 7.668 min
Delta R.T.: 0.035 min
Response: 4148680
Conc: 2.43 ng/ml

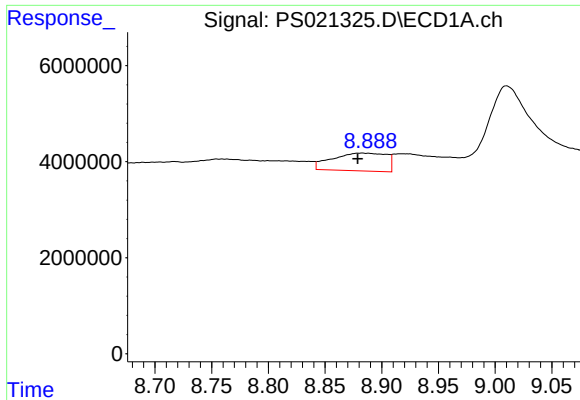

#13 2,4-DB


R.T.: 8.882 min
Delta R.T.: 0.004 min
Response: 12360468
Conc: 5.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

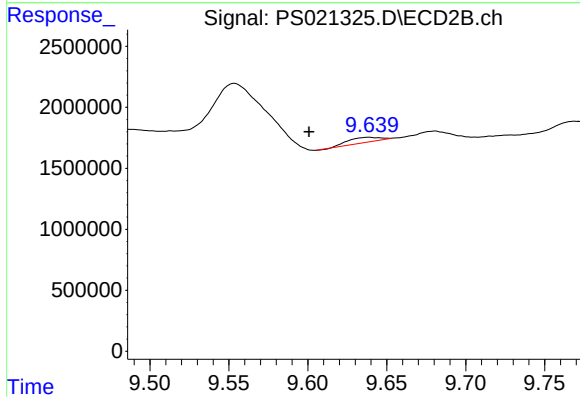


#13 2,4-DB

R.T.: 9.639 min
Delta R.T.: 0.038 min
Response: 562674
Conc: N.D.

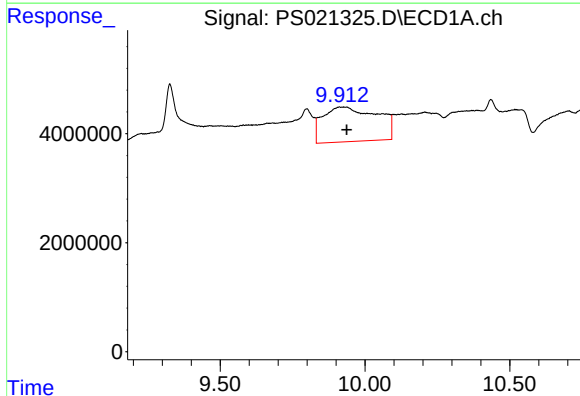


#14 DINOSEB

R.T.: 9.912 min
Delta R.T.: -0.025 min
Response: 83316342
Conc: 7.26 ng/ml

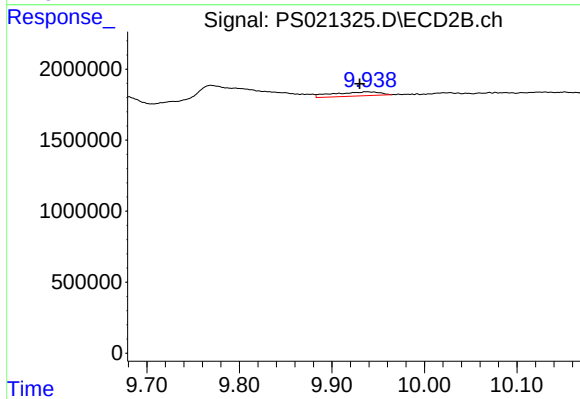

#14 DINOSEB


R.T.: 9.937 min
Delta R.T.: 0.007 min
Response: 1004310
Conc: N.D.

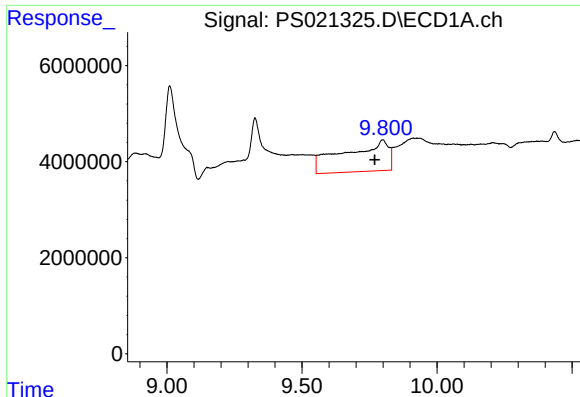

#15 Picloram


R.T.: 9.799 min
Delta R.T.: 0.029 min
Response: 72932949
Conc: 3.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

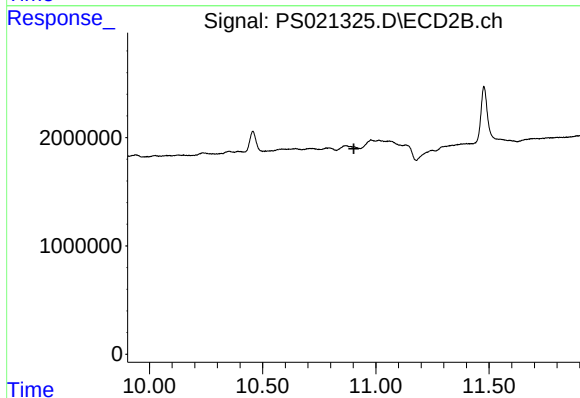


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.903 min
Response: 0
Conc: N.D.

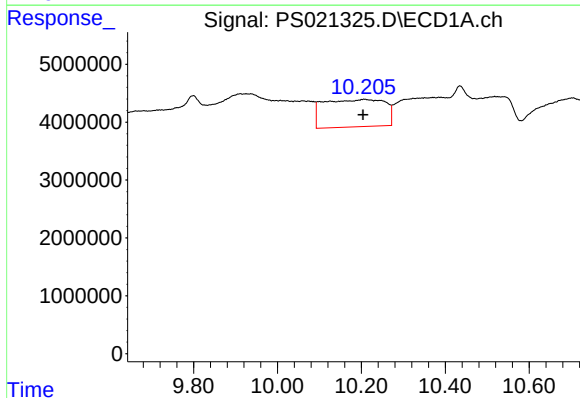

#16 DCPA

R.T.: 10.207 min
Delta R.T.: 0.003 min
Response: 48074818
Conc: 2.54 ng/ml

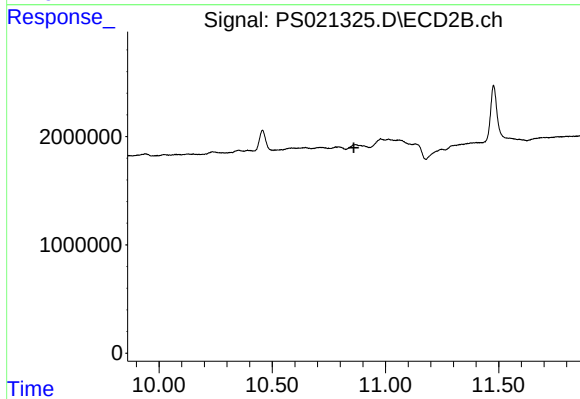

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.860 min
Response: 0
Conc: N.D.