

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120522\
 Data File : PS021331.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2022 21:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 01:19:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
 Quant Title : 8080.M
 QLast Update : Thu Nov 17 00:46:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.412	6.845	1282.7E6	782.0E6	589.960	517.138
Target Compounds							
2) T	3,5-DICHL...	5.757	0.000	16113932	0	5.096	N.D. #
3) T	4-Nitroph...	6.258	0.000	7723589	0	5.717	N.D. #
6) T	MCP	0.000	7.153	0	3550601	N.D.	<MDL
7) T	MCPA	6.831	0.000	37714518	0	3.924	N.D. #
8) T	DICHLORPROP	0.000	7.695f	0	1597244	N.D.	<MDL
10) T	Pentachlo...	7.591	0.000	6711138	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.703	0	4675732	N.D.	<MDL
12) T	2,4,5-T	8.379	9.143f	9043789	1899311	<MDL	<MDL #
13) T	2,4-DB	8.921f	9.640	10161844	589800	4.446	<MDL #
14) T	DINOSEB	9.937	9.938	69007352	1793032	6.017	<MDL #
15) T	Picloram	9.798	10.862f	22316045	4921195	1.110	<MDL #
16) T	DCPA	10.206	10.862	21898256	4921195	1.159	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120522\
Data File : PS021331.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2022 21:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 01:19:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
Quant Title : 8080.M
QLast Update : Thu Nov 17 00:46:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

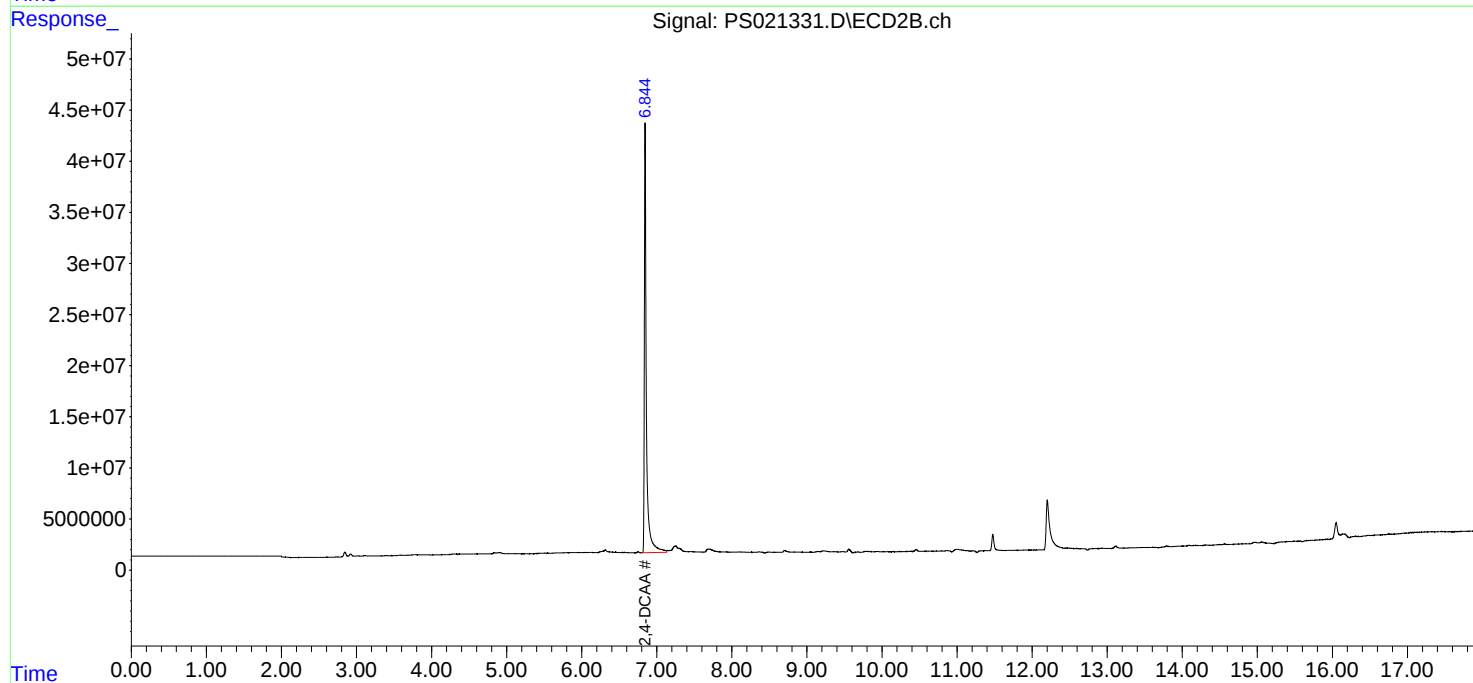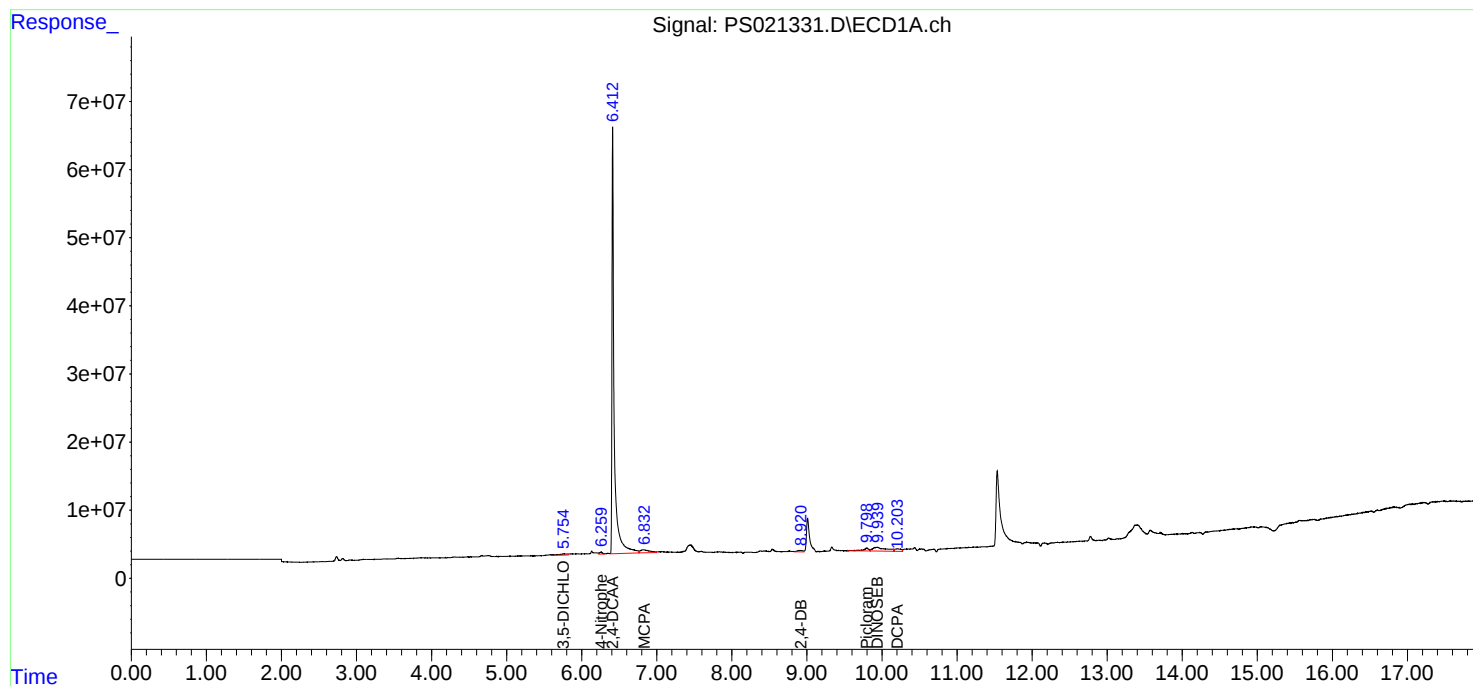


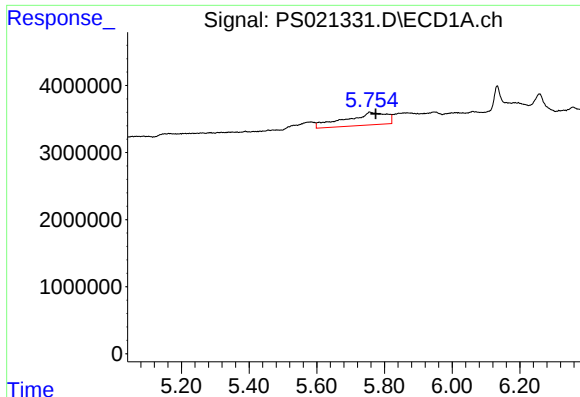

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.757 min
Delta R.T.: -0.017 min
Response: 16113932
Conc: 5.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

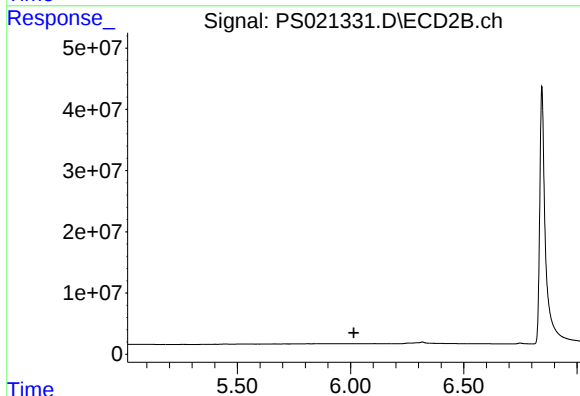


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.014 min
Response: 0
Conc: N.D.

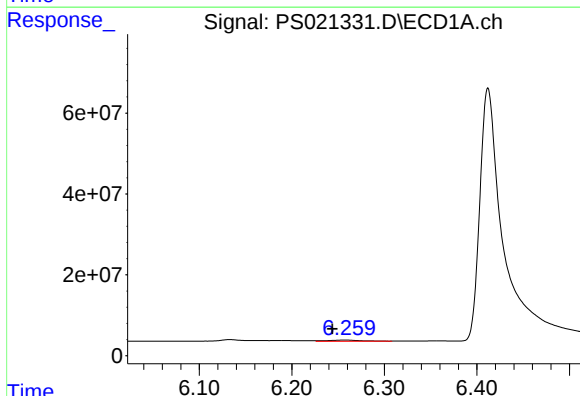


#3 4-Nitrophenol

R.T.: 6.258 min
Delta R.T.: 0.014 min
Response: 7723589
Conc: 5.72 ng/ml

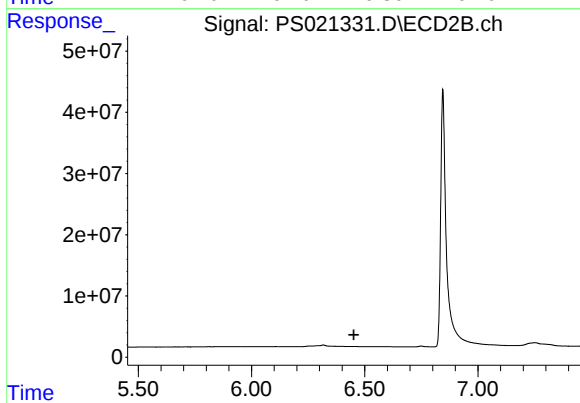

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.452 min
Response: 0
Conc: N.D.

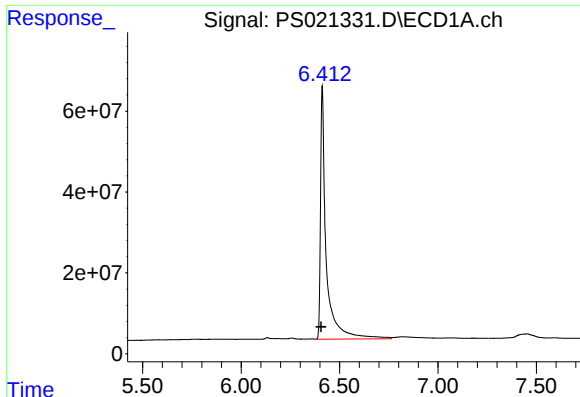

#4 2,4-DCAA


R.T.: 6.412 min
Delta R.T.: 0.006 min
Response: 1282747076
Conc: 589.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

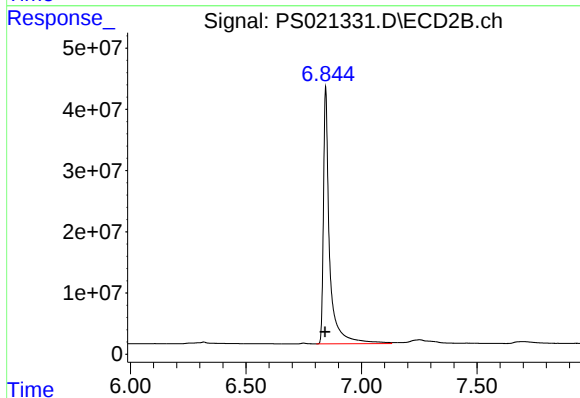


#4 2,4-DCAA

R.T.: 6.845 min
Delta R.T.: 0.003 min
Response: 781972770
Conc: 517.14 ng/ml

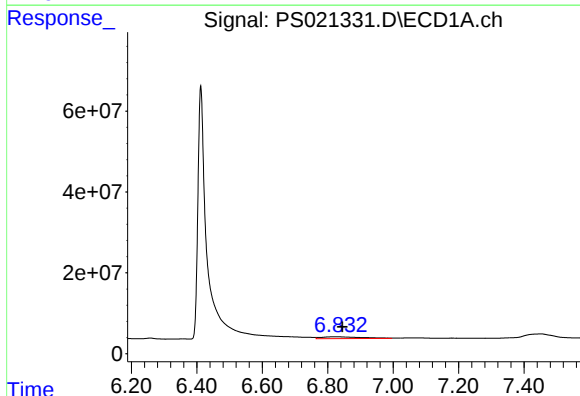


#7 MCPA

R.T.: 6.831 min
Delta R.T.: -0.014 min
Response: 37714518
Conc: 3.92 ug/ml

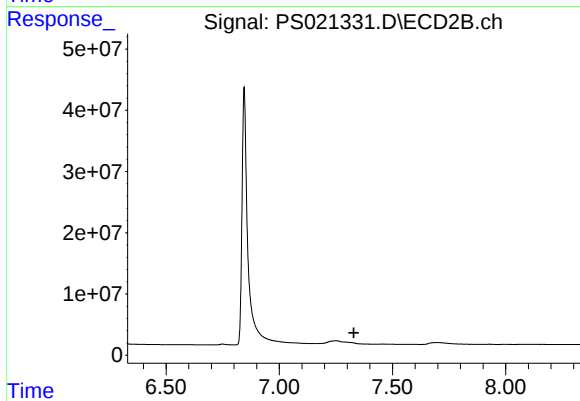

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.330 min
Response: 0
Conc: N.D.

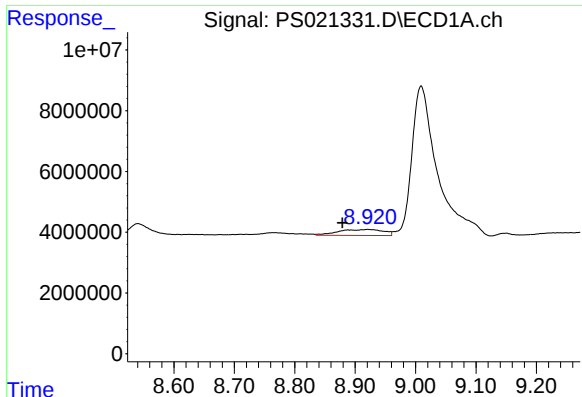

#13 2,4-DB


R.T.: 8.921 min
Delta R.T.: 0.042 min
Response: 10161844
Conc: 4.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

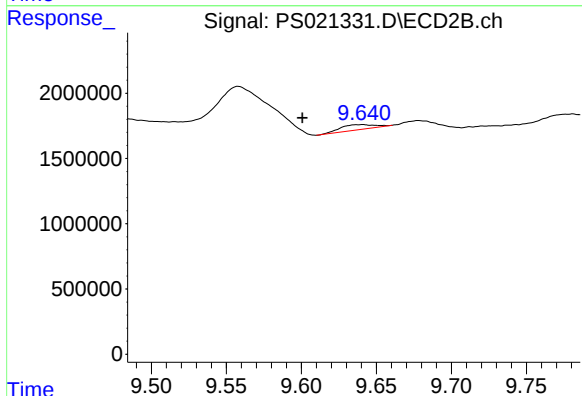


#13 2,4-DB

R.T.: 9.640 min
Delta R.T.: 0.039 min
Response: 589800
Conc: N.D.

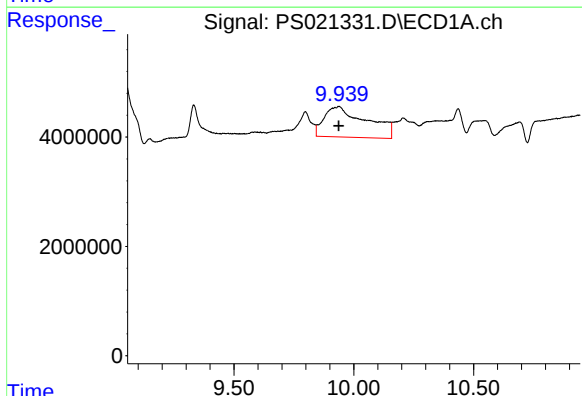


#14 DINOSEB

R.T.: 9.937 min
Delta R.T.: 0.000 min
Response: 69007352
Conc: 6.02 ng/ml

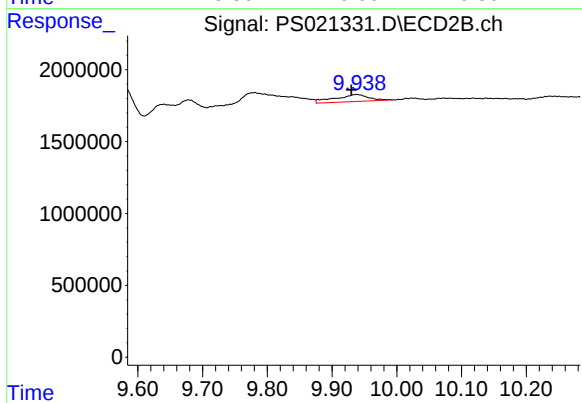

#14 DINOSEB


R.T.: 9.938 min
Delta R.T.: 0.008 min
Response: 1793032
Conc: N.D.

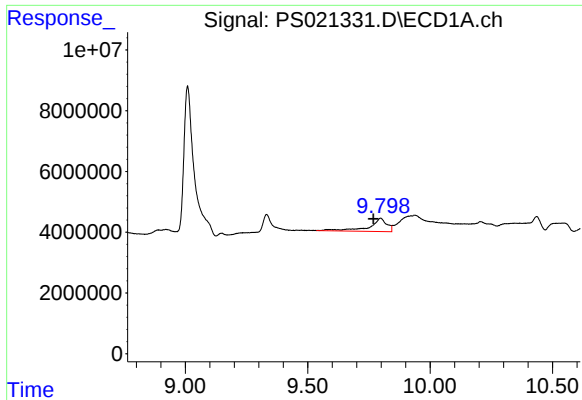

#15 Picloram


R.T.: 9.798 min
Delta R.T.: 0.028 min
Response: 22316045
Conc: 1.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

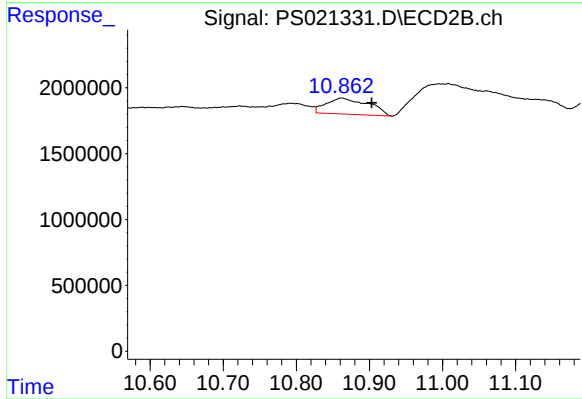


#15 Picloram

R.T.: 10.862 min
Delta R.T.: -0.041 min
Response: 4921195
Conc: N.D.

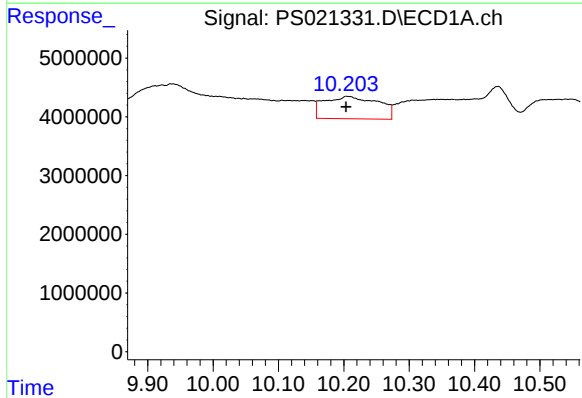

#16 DCPA

R.T.: 10.206 min
Delta R.T.: 0.002 min
Response: 21898256
Conc: 1.16 ng/ml

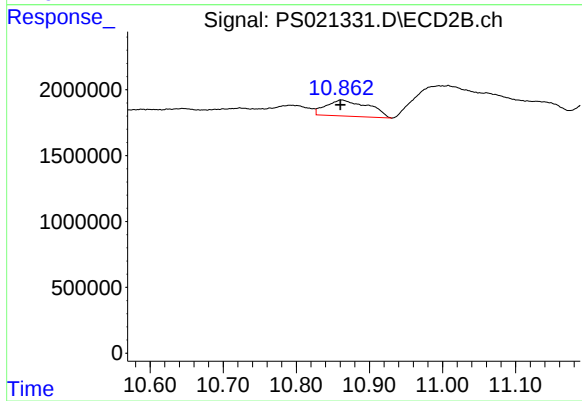

#16 DCPA

R.T.: 10.862 min
Delta R.T.: 0.002 min
Response: 4921195
Conc: N.D.