

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120523\
 Data File : PS024992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2023 10:00
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 23:27:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	2.512	2.567	9772535	5290088	3.389 4.612 #
2) T	3,5-DICHL...	5.698	0.000	847307	0	<MDL N.D. #
5) T	DICAMBA	0.000	6.973f	0	2515256	N.D. <MDL
6) T	MCPP	0.000	6.973f	0	2515256	N.D. 1.213
7) T	MCPA	0.000	7.171f	0	17008957	N.D. 5.171
8) T	DICHLORPROP	0.000	7.559	0	993383	N.D. 1.263
9) T	2,4-D	7.249	0.000	10519499	0	3.463 N.D. #
11) T	2,4,5-TP ...	0.000	8.559f	0	855215	N.D. <MDL
12) T	2,4,5-T	0.000	8.981	0	317243	N.D. <MDL
15) T	Picloram	9.680	10.763	64083897	17943726	3.289 2.741
16) T	DCPA	0.000	10.763	0	17943726	N.D. 3.311



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120523\
Data File : PS024992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2023 10:00
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 23:27:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

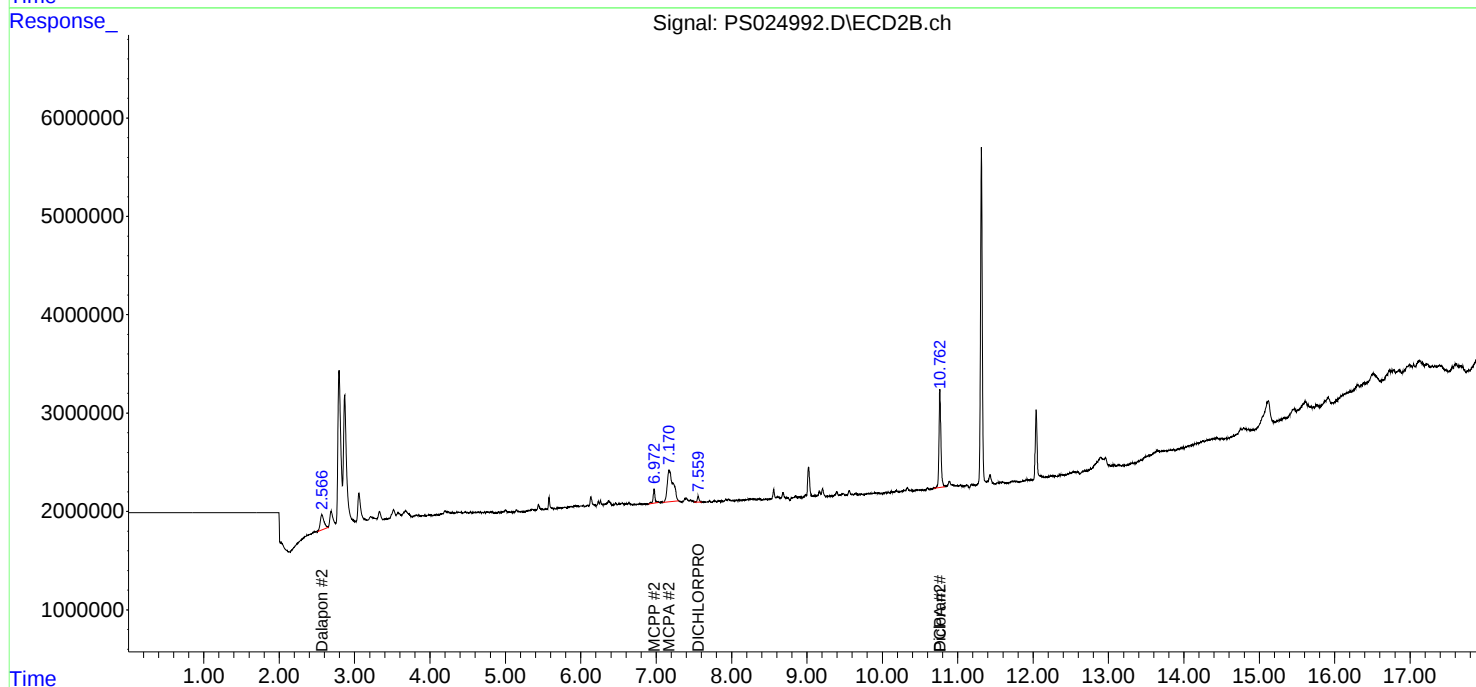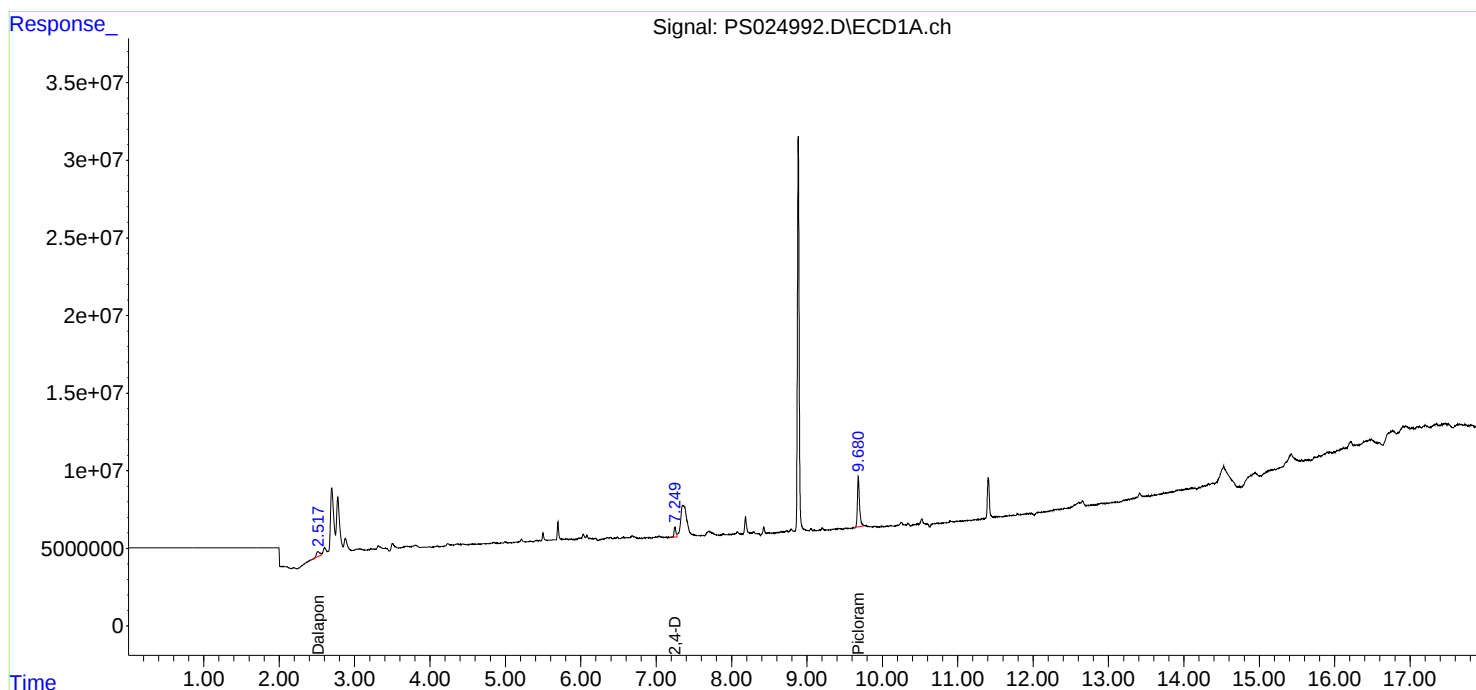


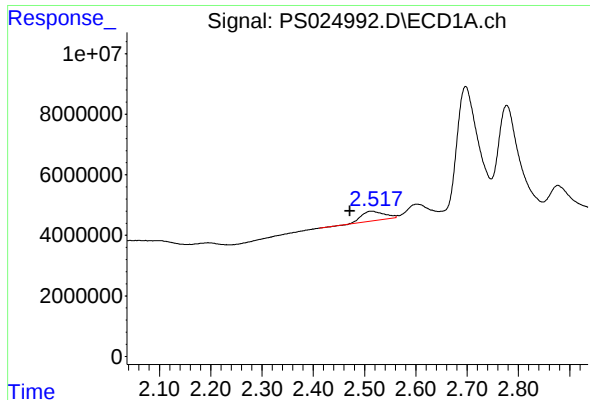

#1 Dalapon


R.T.: 2.512 min
Delta R.T.: 0.040 min
Response: 9772535
Conc: 3.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

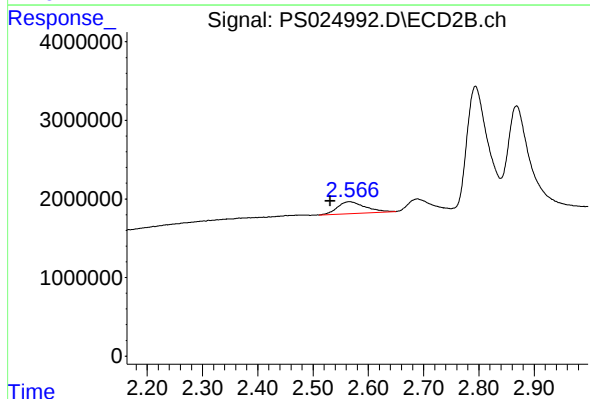


#1 Dalapon

R.T.: 2.567 min
Delta R.T.: 0.035 min
Response: 5290088
Conc: 4.61 ng/ml

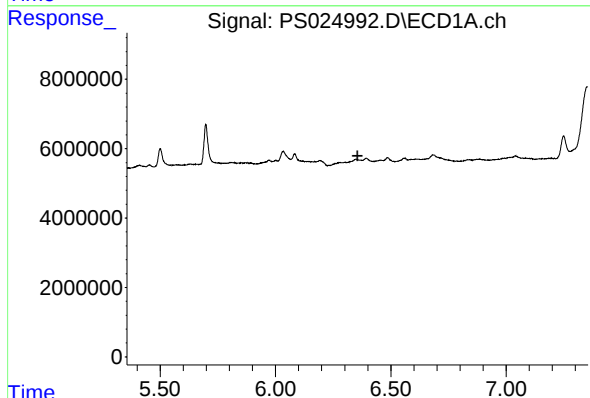


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

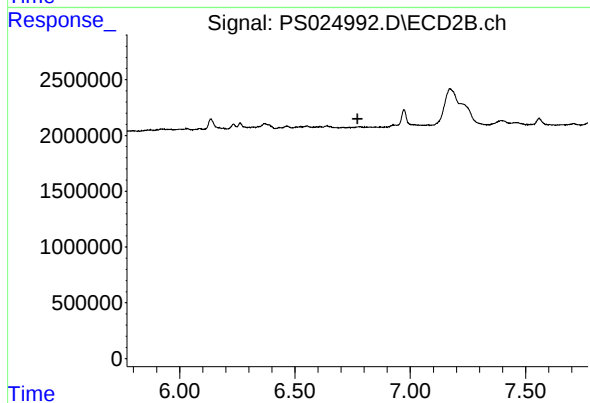

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.771 min
Response: 0
Conc: N.D.

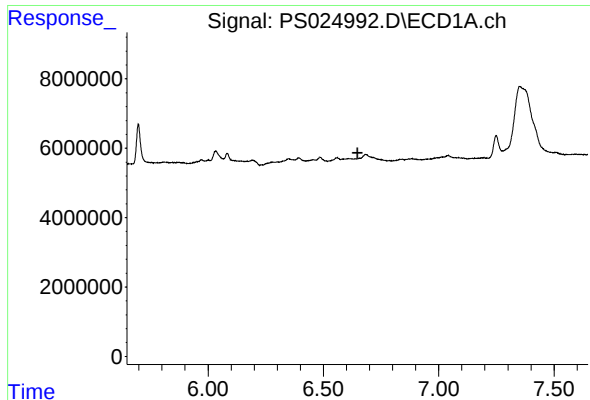

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 6.648 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

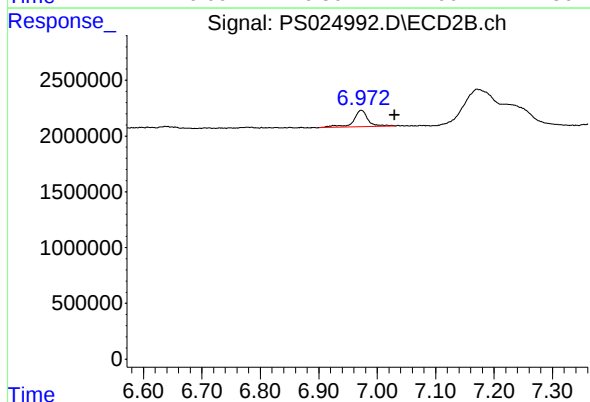


#6 MCPP

R.T.: 6.973 min
Delta R.T.: -0.057 min
Response: 2515256
Conc: 1.21 ug/ml

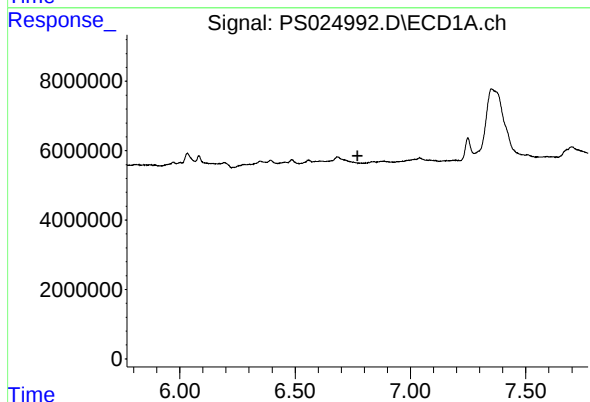


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

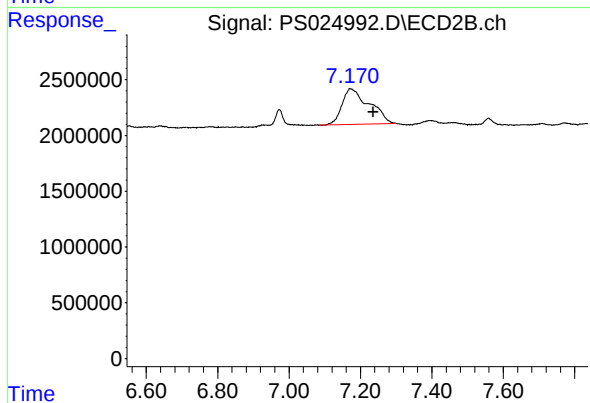

#7 MCPA


R.T.: 7.171 min
Delta R.T.: -0.065 min
Response: 17008957
Conc: 5.17 ug/ml

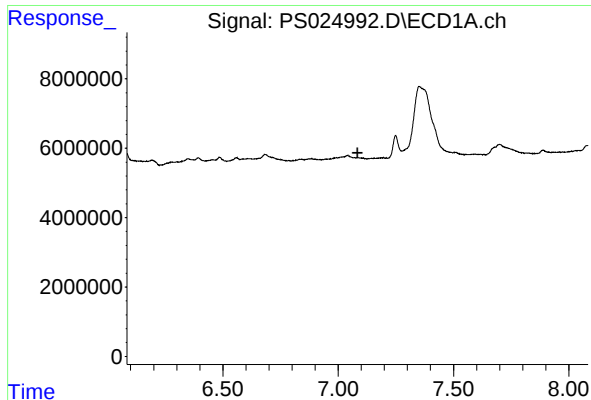

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

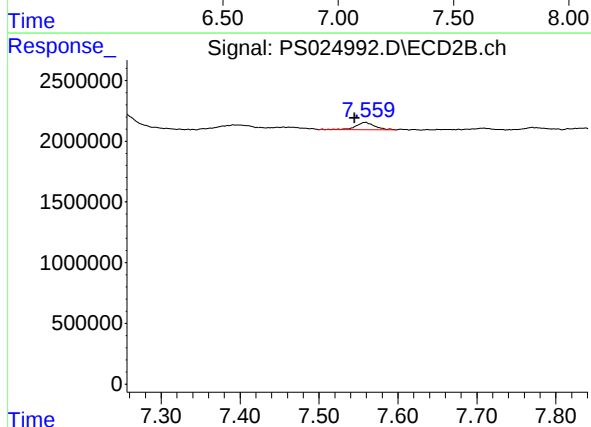


#8 DICHLORPROP

R.T.: 7.559 min
Delta R.T.: 0.014 min
Response: 993383
Conc: 1.26 ng/ml

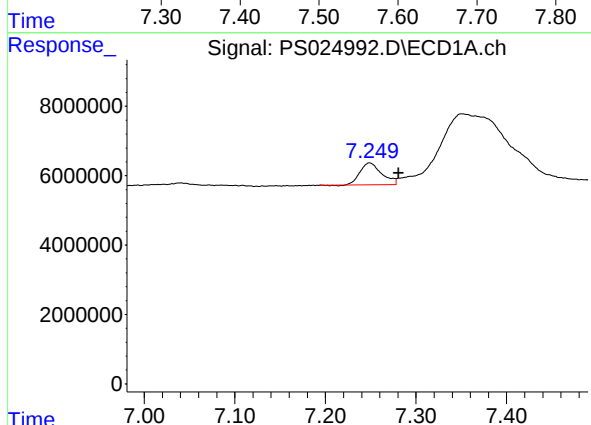


#9 2,4-D

R.T.: 7.249 min
Delta R.T.: -0.032 min
Response: 10519499
Conc: 3.46 ng/ml

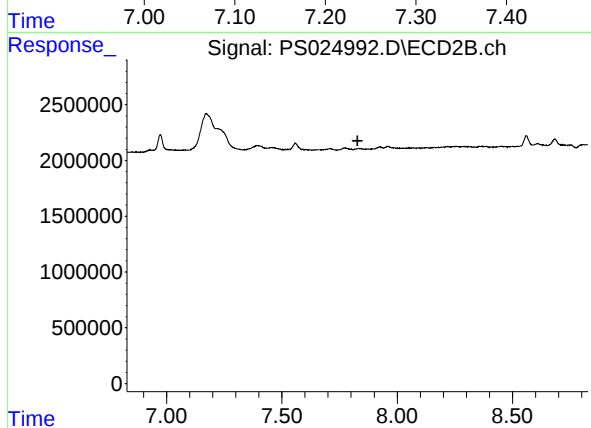

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.828 min
Response: 0
Conc: N.D.

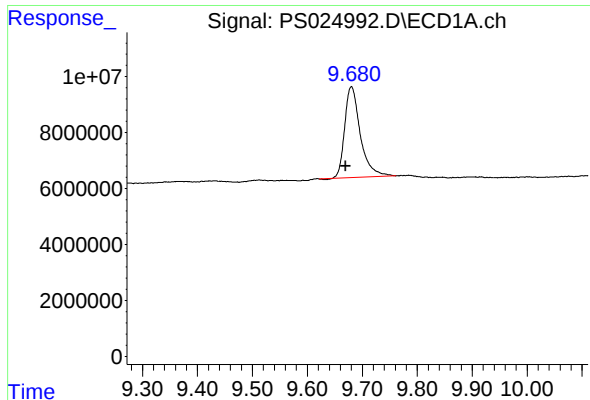

#15 Picloram


R.T.: 9.680 min
Delta R.T.: 0.010 min
Response: 64083897
Conc: 3.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

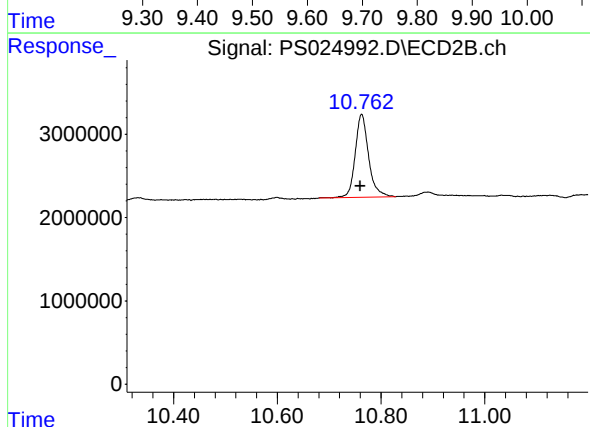


#15 Picloram

R.T.: 10.763 min
Delta R.T.: 0.003 min
Response: 17943726
Conc: 2.74 ng/ml

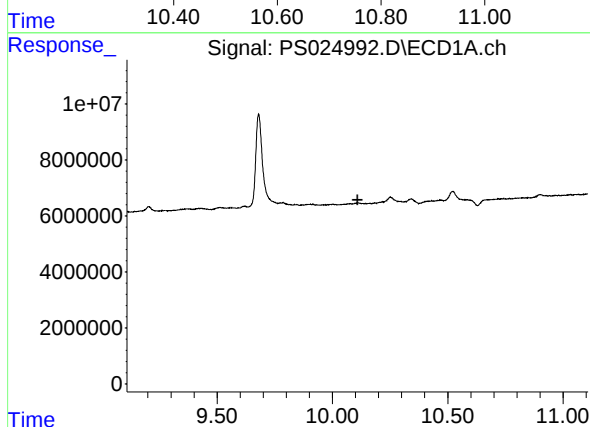

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

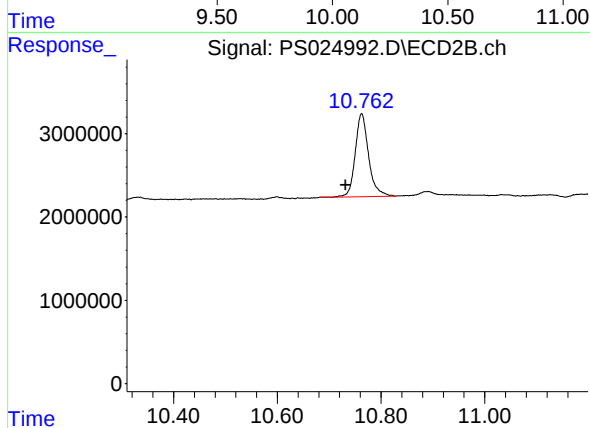

#16 DCPA

R.T.: 10.763 min
Delta R.T.: 0.031 min
Response: 17943726
Conc: 3.31 ng/ml