

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120523\
 Data File : PS024993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2023 10:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 23:27:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.356	6.771	1167.6E6	371.0E6	521.750	511.975
Target Compounds						
1) T Dalapon	2.512	2.567	9466788	4748602	3.283	4.140 #
5) T DICAMBA	0.000	6.971	0	529262	N.D.	<MDL
6) T MCPP	0.000	6.971f	0	529262	N.D.	<MDL
7) T MCPA	0.000	7.225	0	5465386	N.D.	1.662
8) T DICHLORPROP	0.000	7.560	0	1175729	N.D.	1.495
11) T 2,4,5-TP ...	0.000	8.561f	0	940247	N.D.	<MDL
12) T 2,4,5-T	0.000	8.981	0	297629	N.D.	<MDL
15) T Picloram	9.682	10.764	59535836	15227349	3.055	2.326
16) T DCPA	0.000	10.764	0	15227349	N.D.	2.810



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120523\
Data File : PS024993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2023 10:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 23:27:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

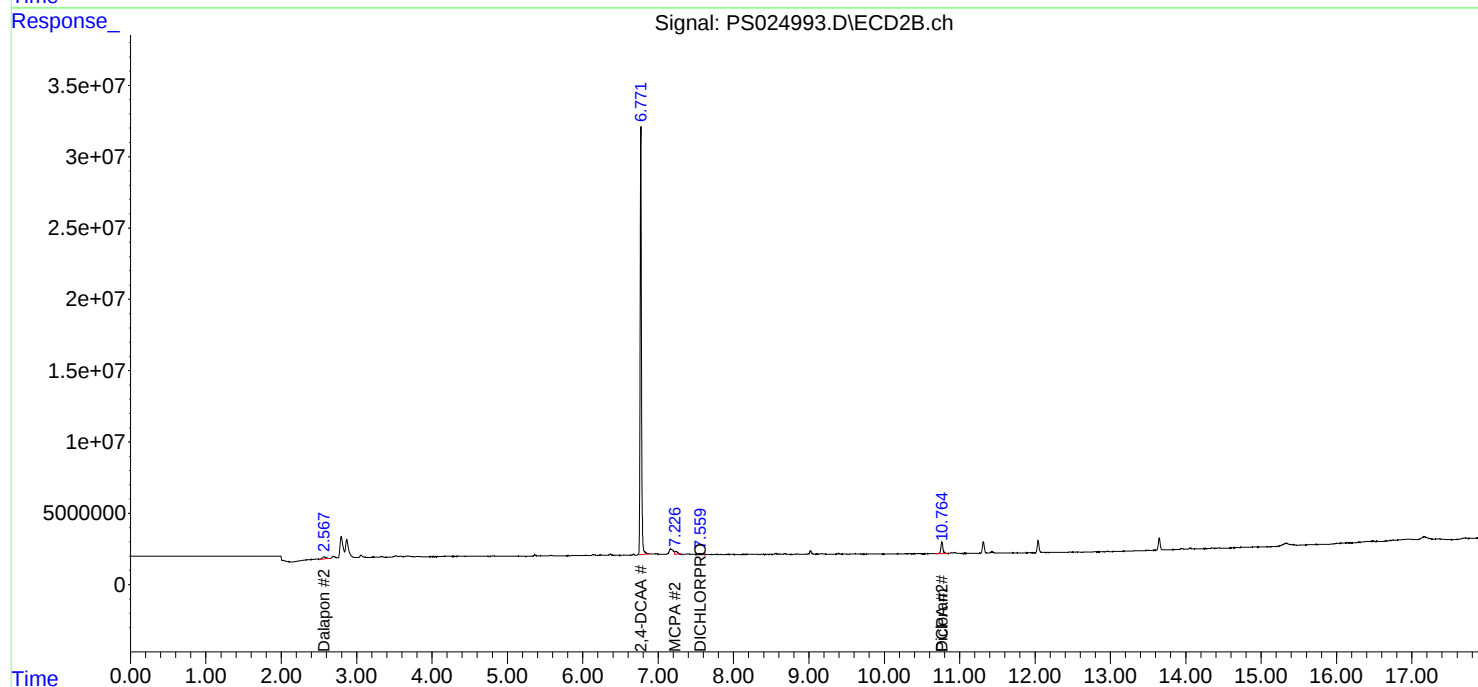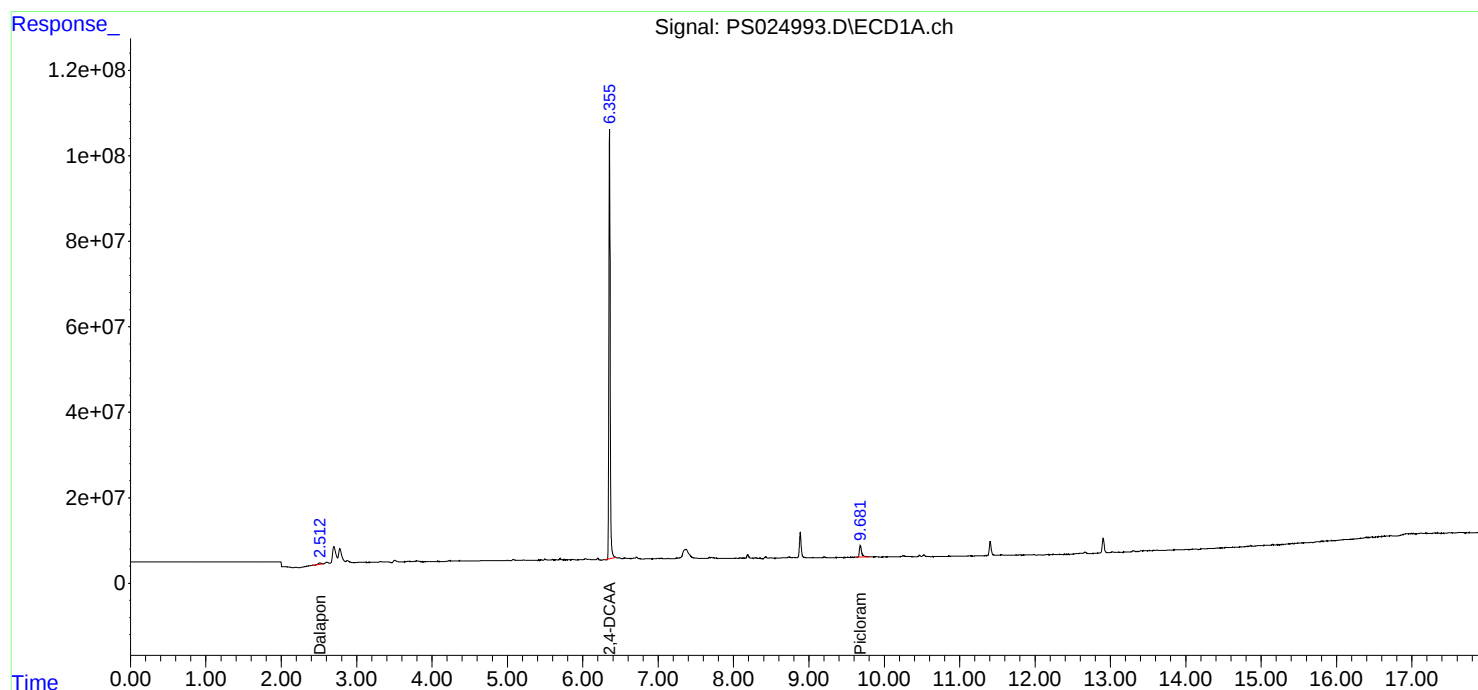


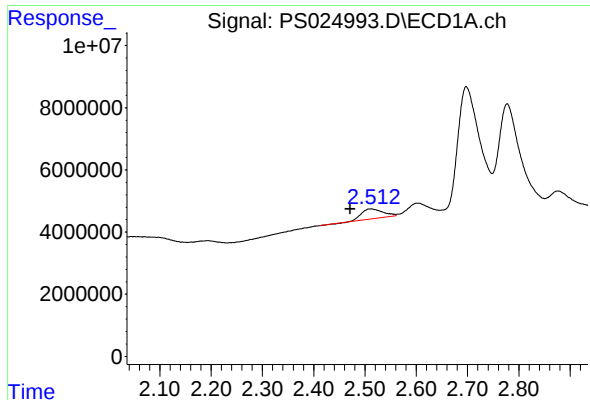

#1 Dalapon


R.T.: 2.512 min
Delta R.T.: 0.040 min
Response: 9466788
Conc: 3.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

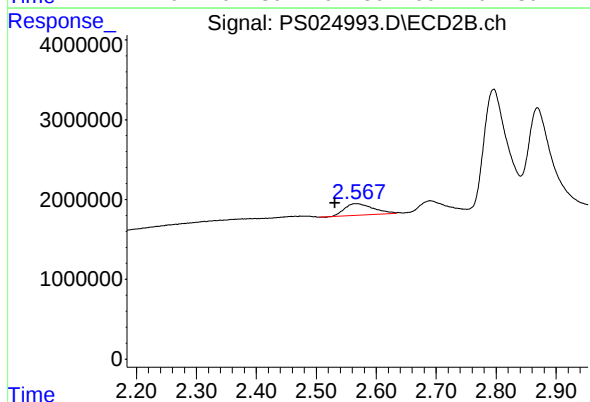


#1 Dalapon

R.T.: 2.567 min
Delta R.T.: 0.036 min
Response: 4748602
Conc: 4.14 ng/ml

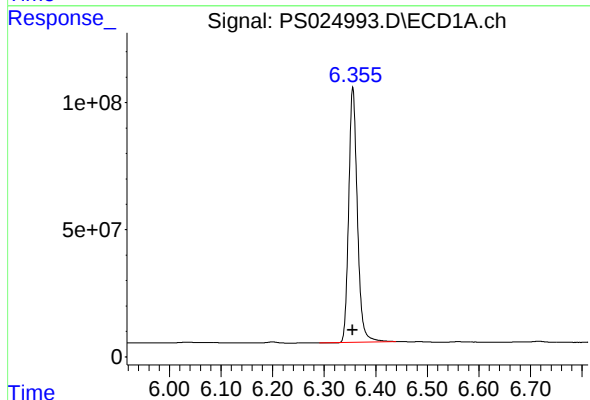


#4 2,4-DCAA

R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 1167594626
Conc: 521.75 ng/ml

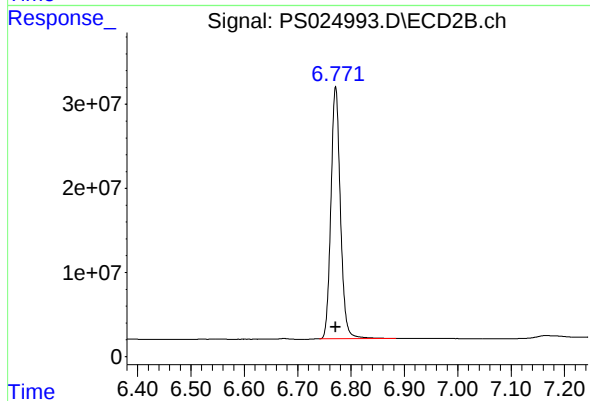

#4 2,4-DCAA


R.T.: 6.771 min
Delta R.T.: 0.000 min
Response: 370954194
Conc: 511.98 ng/ml

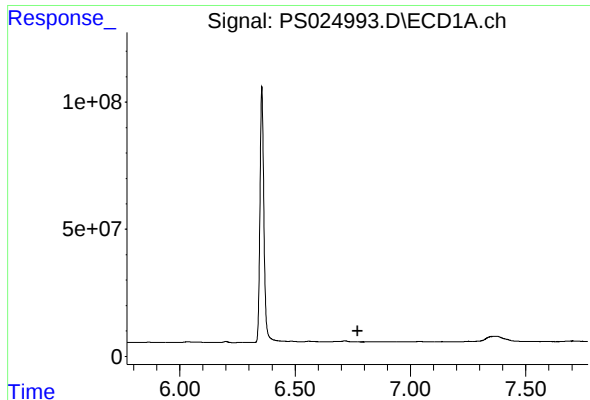

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

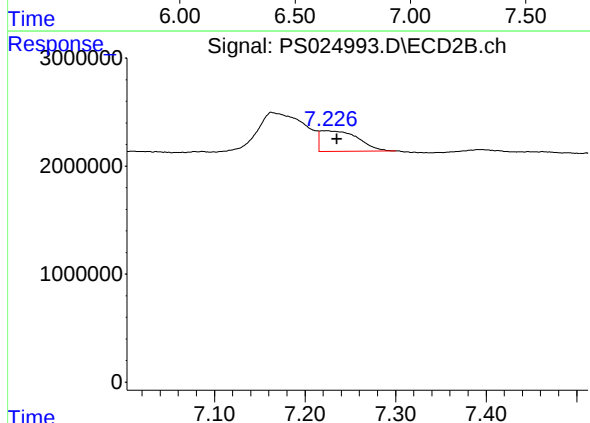


#7 MCPA

R.T.: 7.225 min
Delta R.T.: -0.010 min
Response: 5465386
Conc: 1.66 ug/ml

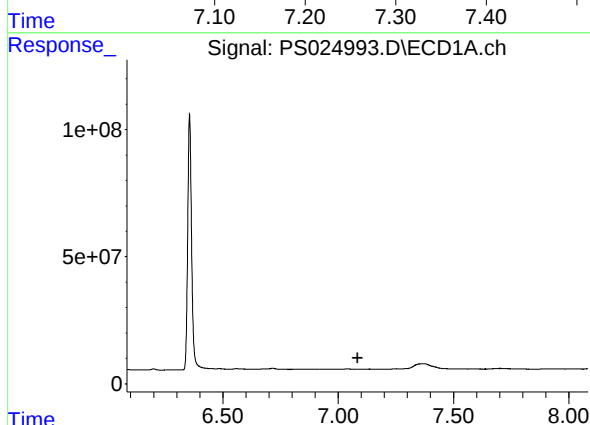


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

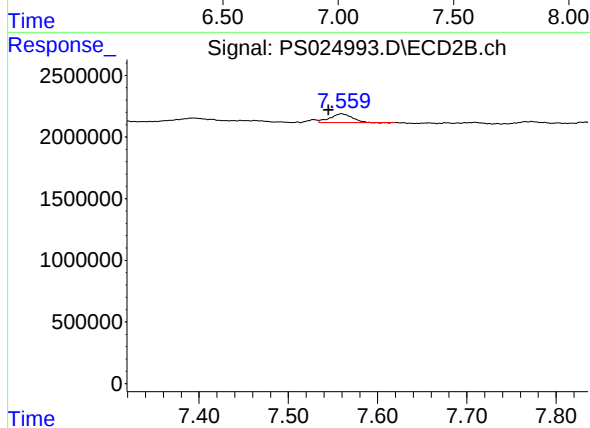

#8 DICHLORPROP


R.T.: 7.560 min
Delta R.T.: 0.015 min
Response: 1175729
Conc: 1.49 ng/ml

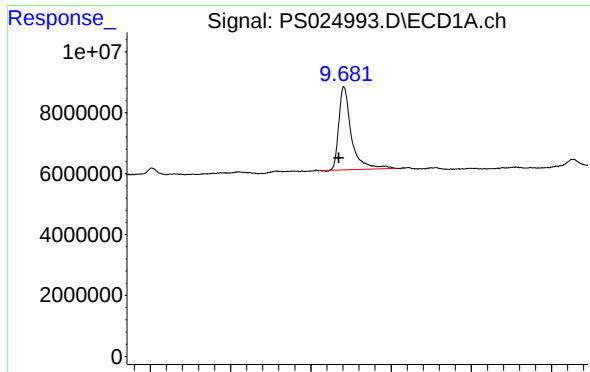

#15 Picloram


R.T.: 9.682 min
Delta R.T.: 0.013 min
Response: 59535836
Conc: 3.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

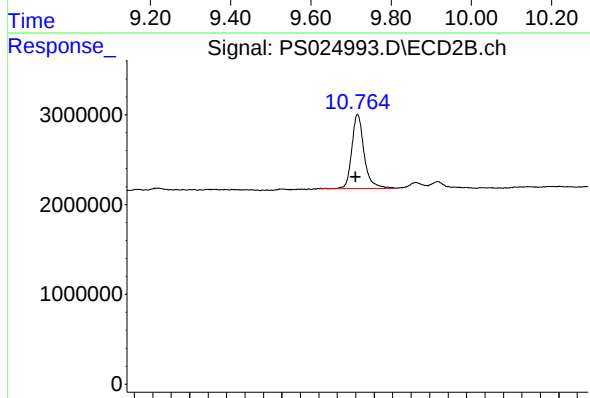


#15 Picloram

R.T.: 10.764 min
Delta R.T.: 0.004 min
Response: 15227349
Conc: 2.33 ng/ml

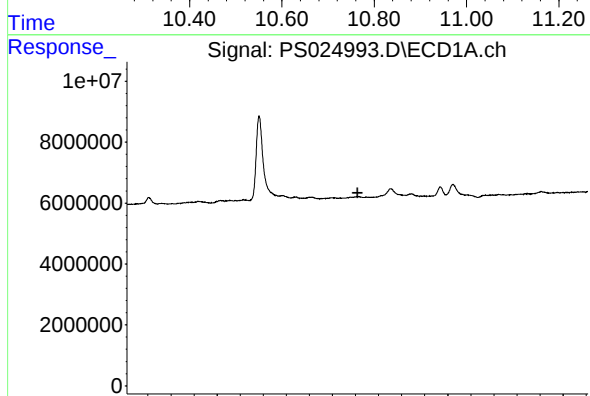

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

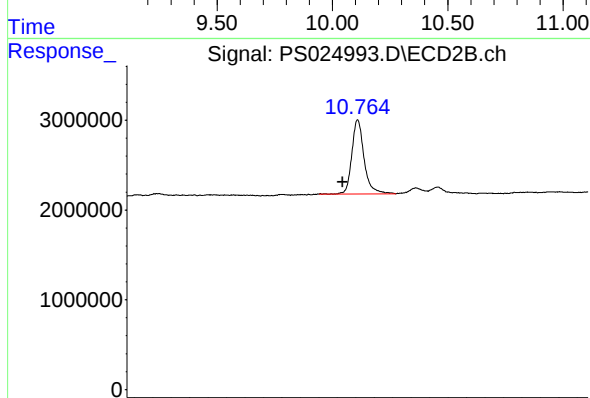

#16 DCPA

R.T.: 10.764 min
Delta R.T.: 0.032 min
Response: 15227349
Conc: 2.81 ng/ml