

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120523\
 Data File : PS025017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2023 21:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 23:31:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.355	6.770	1157.0E6	371.2E6	517.004	512.356
Target Compounds							
1) T	Dalapon	2.509	2.564	9303197	3984297	3.226	3.474
2) T	3,5-DICHL...	5.697	0.000	2130069	0	<MDL	N.D. #
5) T	DICAMBA	0.000	6.972f	0	3799975	N.D.	1.226
6) T	MCP	6.678	6.972f	3411797	3799975	<MDL	1.832 #
8) T	DICHLORPROP	0.000	7.557	0	3176529	N.D.	4.038
9) T	2,4-D	7.246	0.000	21592810	0	7.109	N.D. #
12) T	2,4,5-T	0.000	8.979	0	717480	N.D.	<MDL
13) T	2,4-DB	0.000	9.480	0	784692	N.D.	1.418
15) T	Picloram	9.678	10.763	19229568	6913423	<MDL	1.056 #
16) T	DCPA	0.000	10.763	0	6913423	N.D.	1.276



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120523\
Data File : PS025017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2023 21:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 05 23:31:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

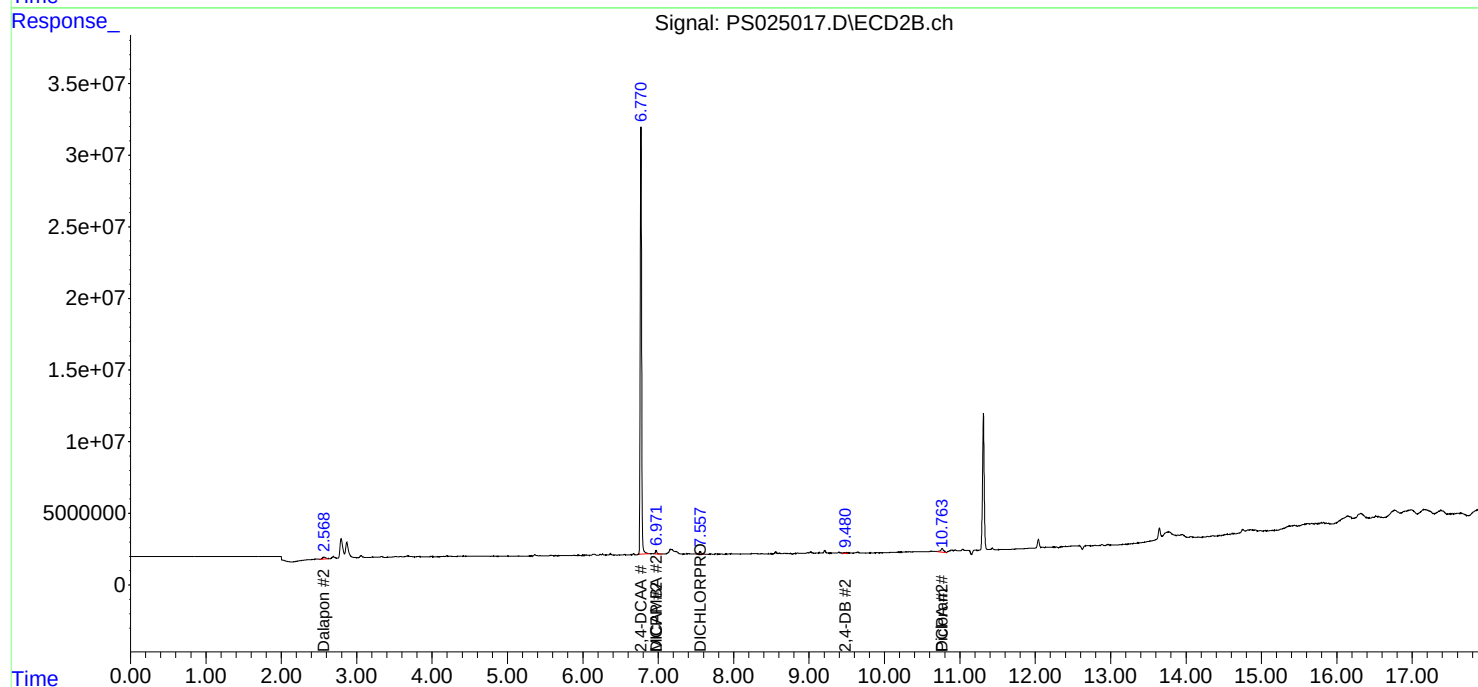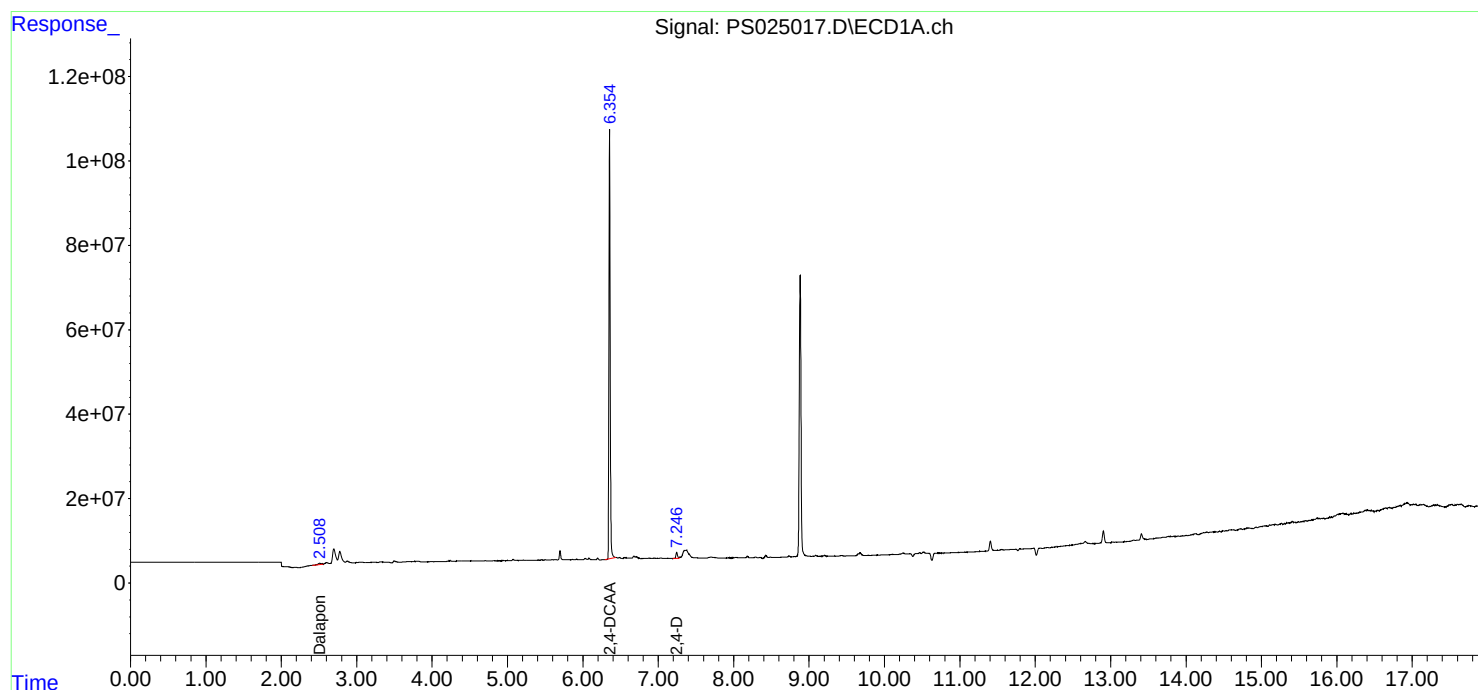


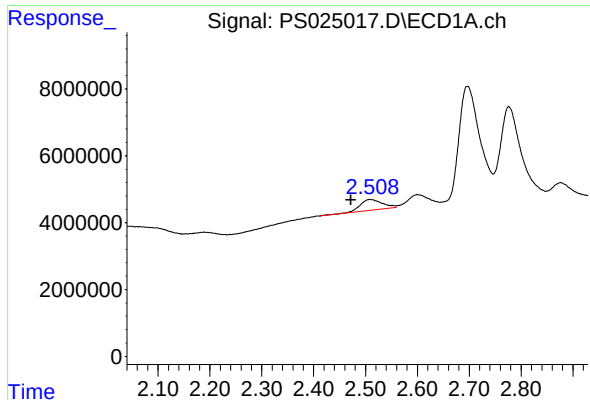

#1 Dalapon


R.T.: 2.509 min
Delta R.T.: 0.037 min
Response: 9303197
Conc: 3.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

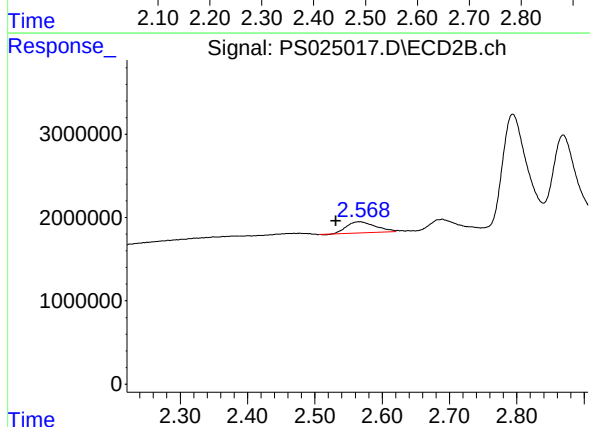


#1 Dalapon

R.T.: 2.564 min
Delta R.T.: 0.033 min
Response: 3984297
Conc: 3.47 ng/ml

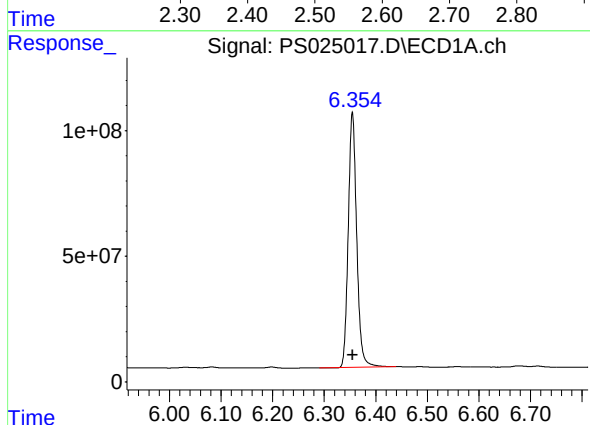


#4 2,4-DCAA

R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 1156973448
Conc: 517.00 ng/ml

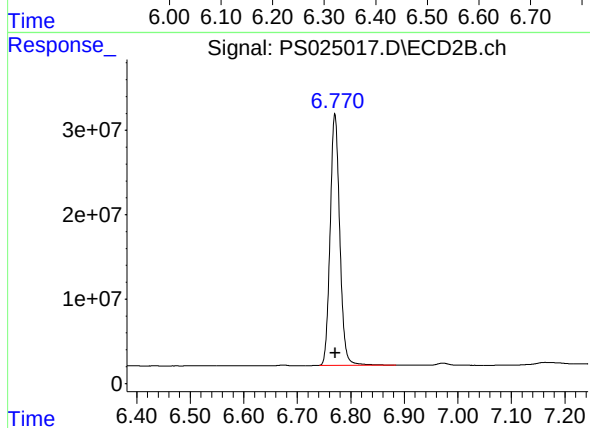

#4 2,4-DCAA


R.T.: 6.770 min
Delta R.T.: 0.000 min
Response: 371229739
Conc: 512.36 ng/ml

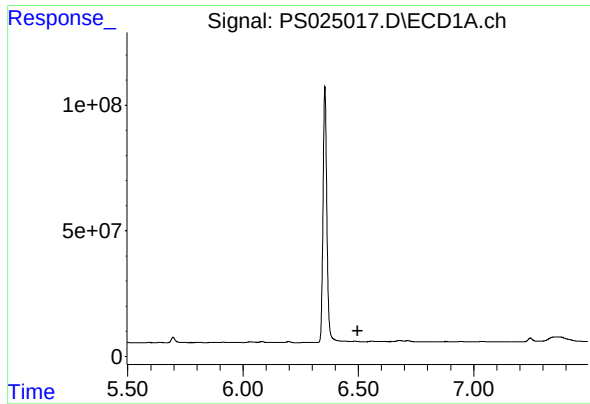

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

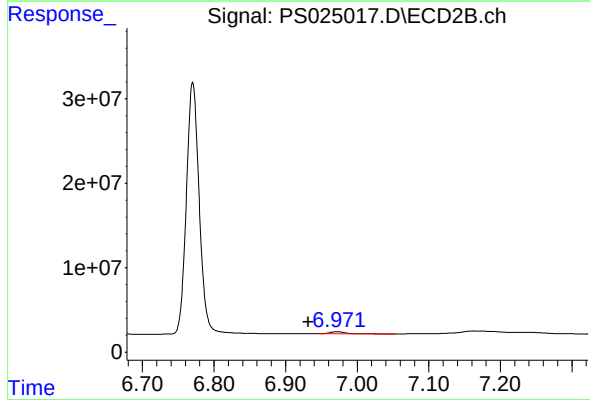


#5 DICAMBA

R.T.: 6.972 min
Delta R.T.: 0.040 min
Response: 3799975
Conc: 1.23 ng/ml

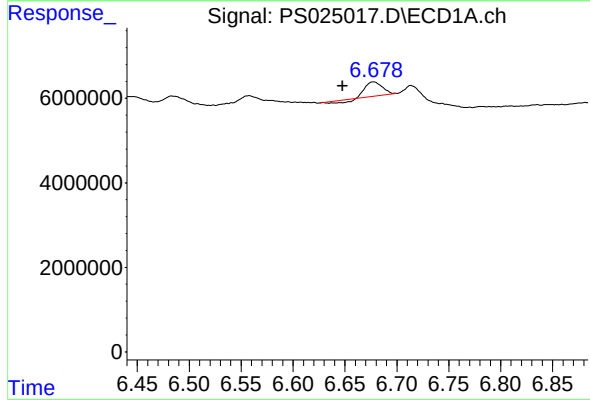


#6 MCPP

R.T.: 6.678 min
Delta R.T.: 0.030 min
Response: 3411797
Conc: N.D.

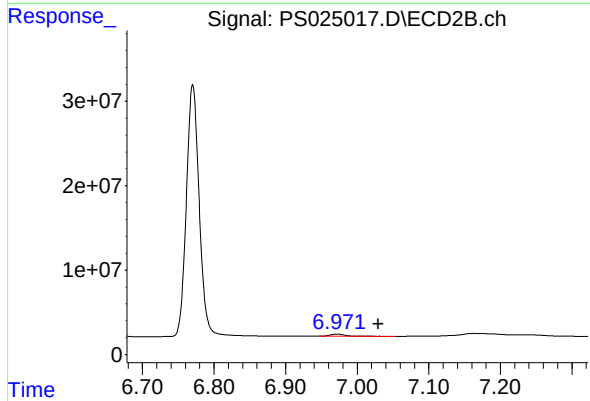

#6 MCPP


R.T.: 6.972 min
Delta R.T.: -0.058 min
Response: 3799975
Conc: 1.83 ug/ml

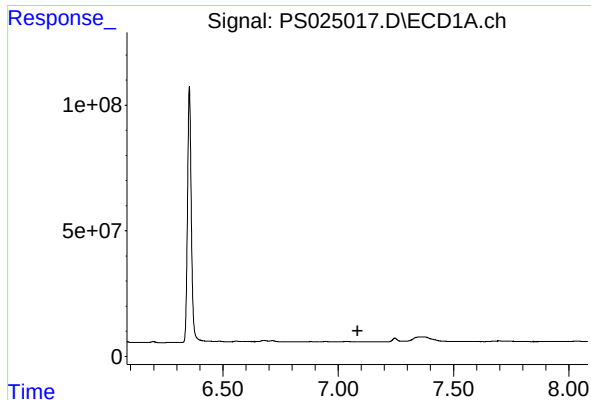

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

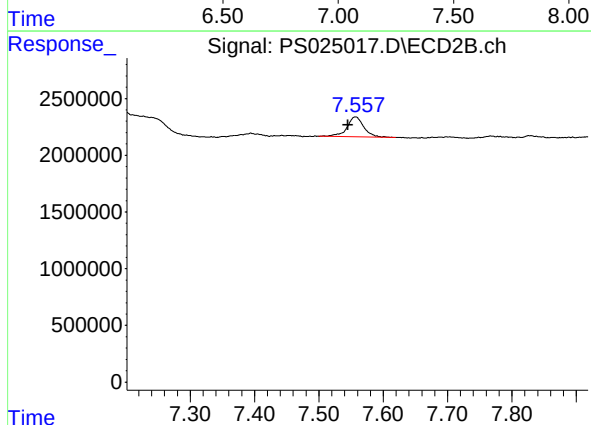


#8 DICHLORPROP

R.T.: 7.557 min
Delta R.T.: 0.012 min
Response: 3176529
Conc: 4.04 ng/ml

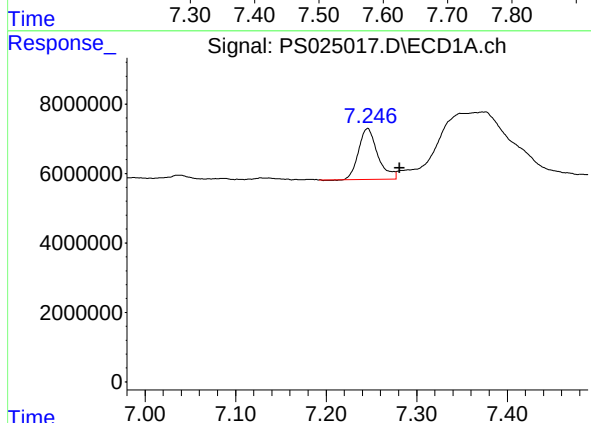


#9 2,4-D

R.T.: 7.246 min
Delta R.T.: -0.035 min
Response: 21592810
Conc: 7.11 ng/ml

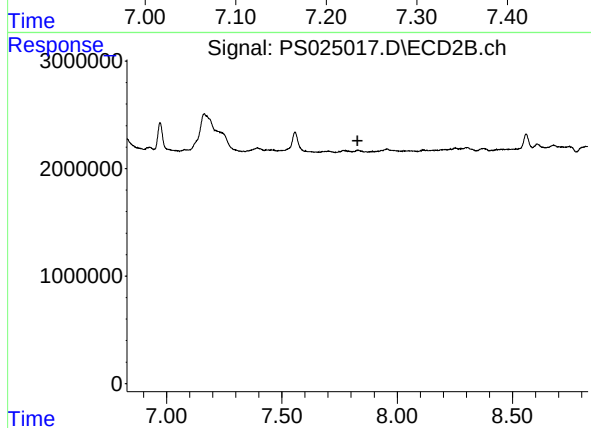

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.828 min
Response: 0
Conc: N.D.

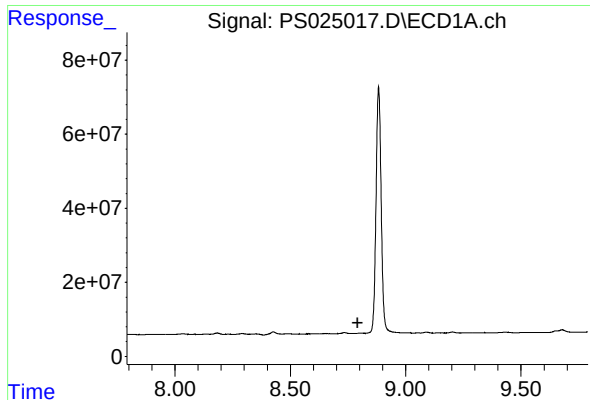

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

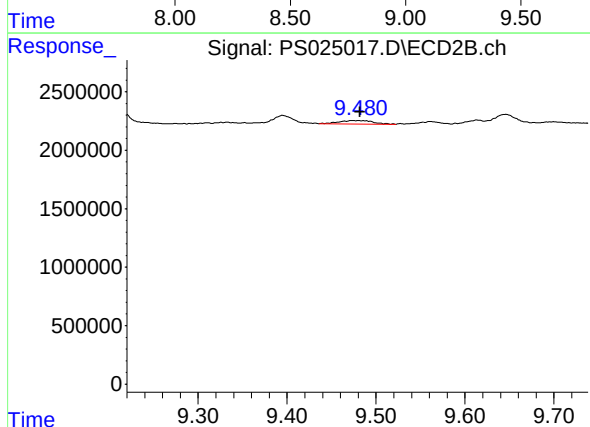


#13 2,4-DB

R.T.: 9.480 min
Delta R.T.: -0.002 min
Response: 784692
Conc: 1.42 ng/ml

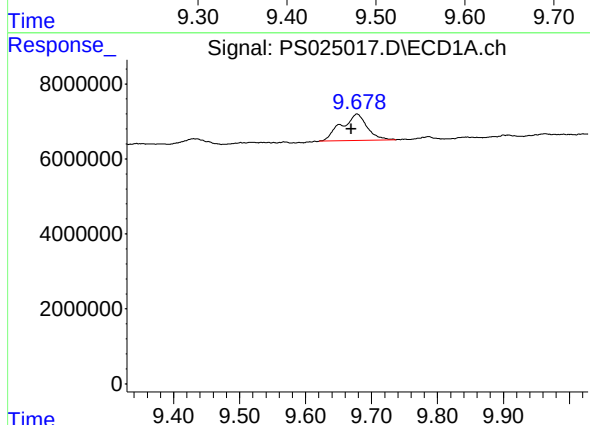


#15 Picloram

R.T.: 9.678 min
Delta R.T.: 0.008 min
Response: 19229568
Conc: N.D.

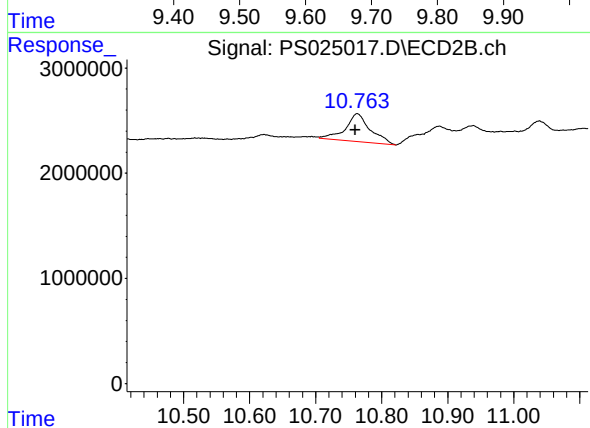

#15 Picloram


R.T.: 10.763 min
Delta R.T.: 0.003 min
Response: 6913423
Conc: 1.06 ng/ml

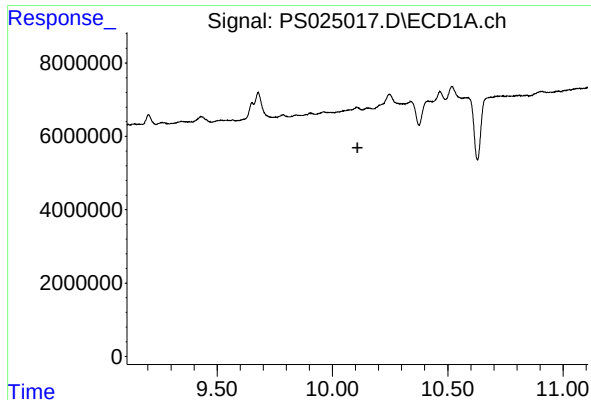

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

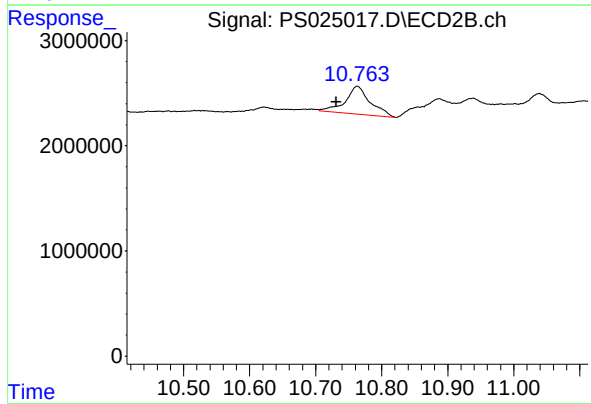

#16 DCPA

R.T.: 10.763 min
Delta R.T.: 0.031 min
Response: 6913423
Conc: 1.28 ng/ml