

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120523\
 Data File : PS024999.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2023 13:08
 Operator : AR\AJ
 Sample : 05599-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
ClientSampleId :
 LKWD-BACKFILL-03

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/06/2023
 Supervised By :Ankita Jodhani 12/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 23:28:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.354	6.771	741.1E6	197.3E6	331.187m	272.321

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120523\
 Data File : PS024999.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2023 13:08
 Operator : AR\AJ
 Sample : 05599-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1



Instrument :
 ECD_S
ClientSampleId :
 LKWD-BACKFILL-03


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/06/2023
 Supervised By :Ankita Jodhani 12/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 05 23:28:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

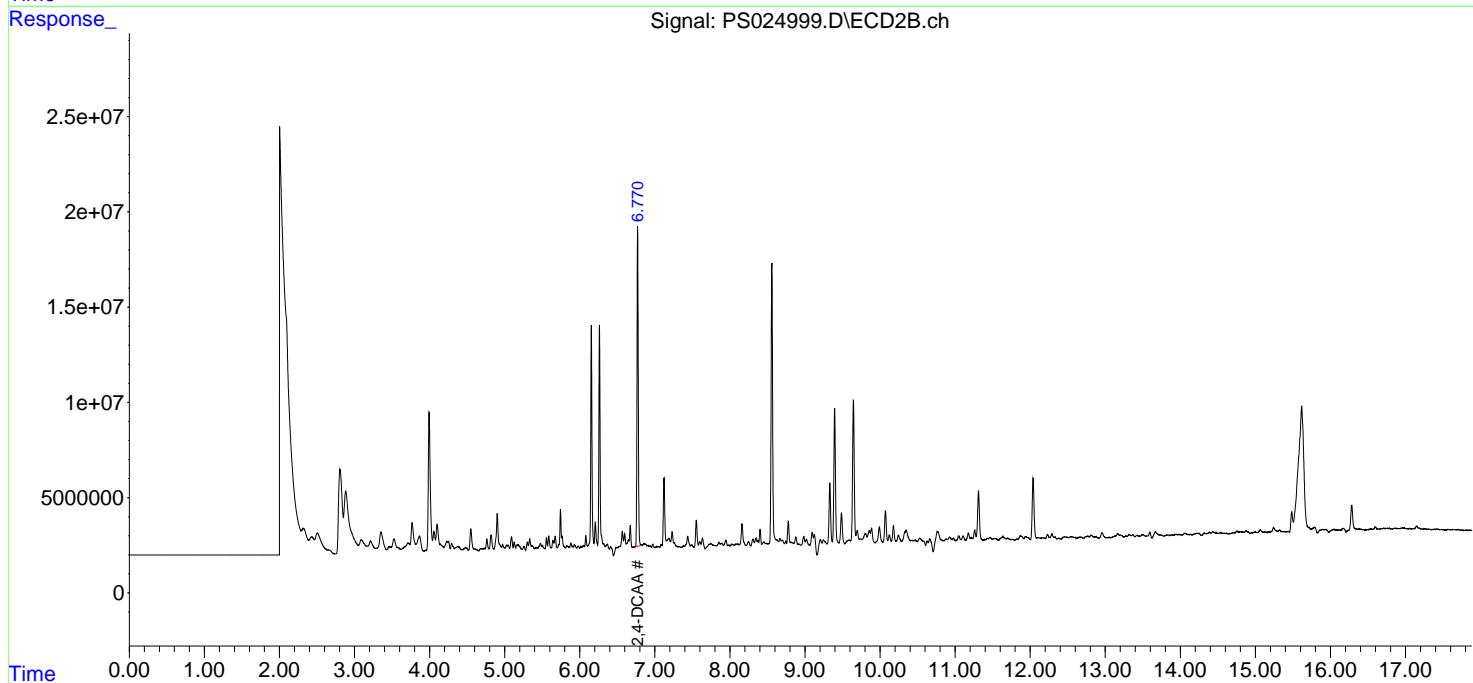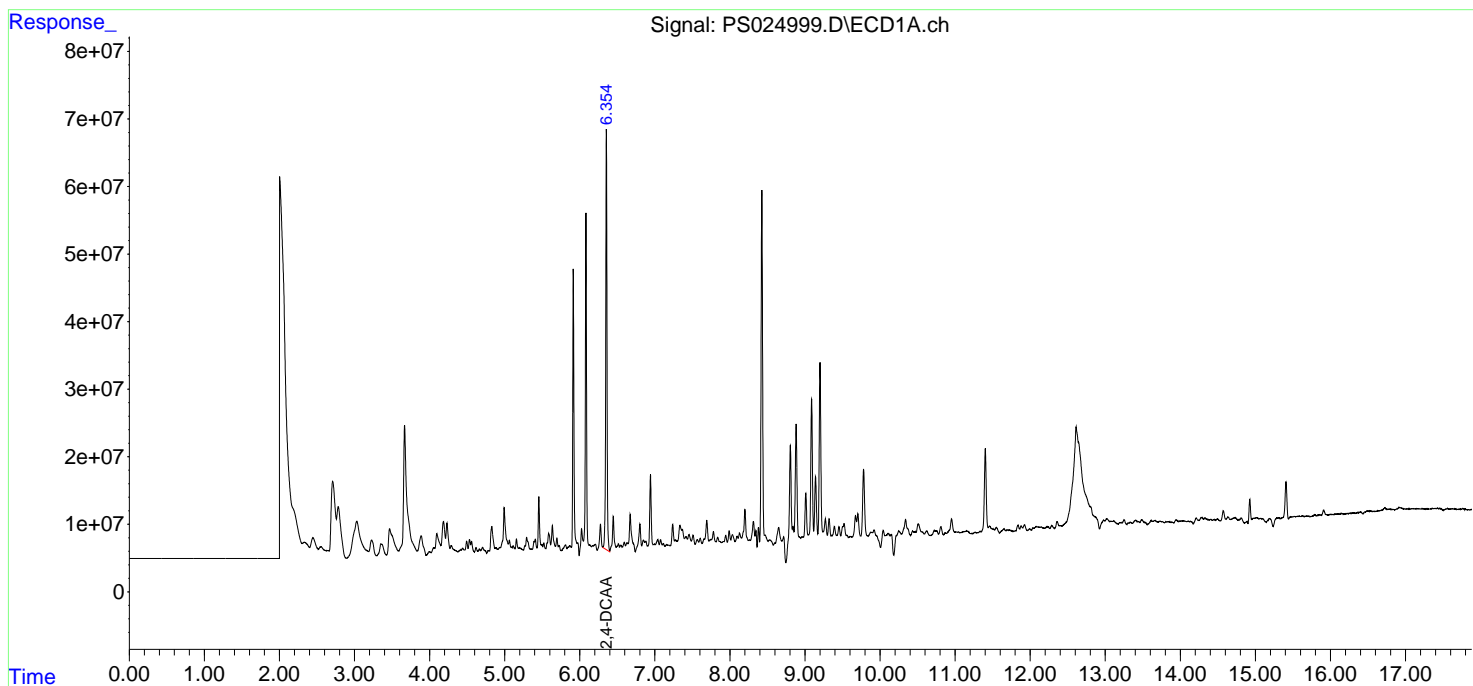

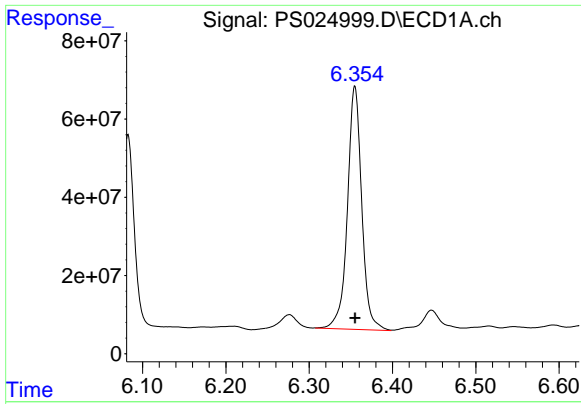


#4 2,4-DCAA

R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 741144135
Conc: 331.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
LKWD-BACKFILL-03

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/06/2023
Supervised By :Ankita Jodhani 12/06/2023

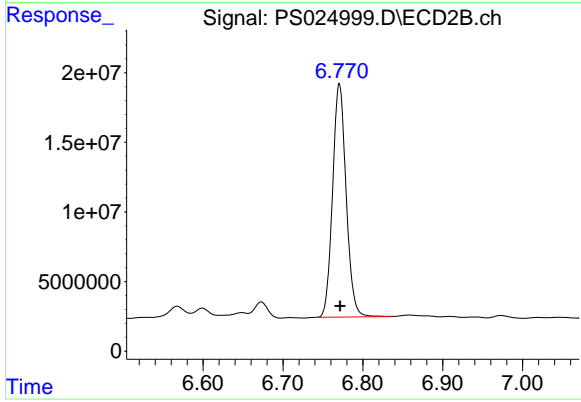

#4 2,4-DCAA

R.T.: 6.771 min
Delta R.T.: 0.000 min
Response: 197311143
Conc: 272.32 ng/ml