

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120524\
 Data File : PS028694.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2024 10:46
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 00:14:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
1) T	Dalapon	2.674f	0.000	10980672	0	3.784	N.D. #
2) T	3,5-DICHL...	6.418	0.000	447639	0	<MDL	N.D. #
3) T	4-Nitroph...	7.017	0.000	1782465	0	1.037	N.D. #
5) T	DICAMBA	0.000	7.927	0	2923221	N.D.	<MDL
7) T	MCPA	7.792f	8.243f	305026	10035981	<MDL	1.617 #
8) T	DICHLORPROP	8.089f	0.000	767282	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.190f	0.000	580661	0	<MDL	N.D. #
12) T	2,4,5-T	9.531	10.295	917527	7024296	<MDL	<MDL #
13) T	2,4-DB	10.105	0.000	521553	0	<MDL	N.D. #
15) T	Picloram	11.133	12.336	29348781	5748737	<MDL	<MDL #
16) T	DCPA	11.589	0.000	2728613	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120524\
Data File : PS028694.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2024 10:46
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 00:14:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

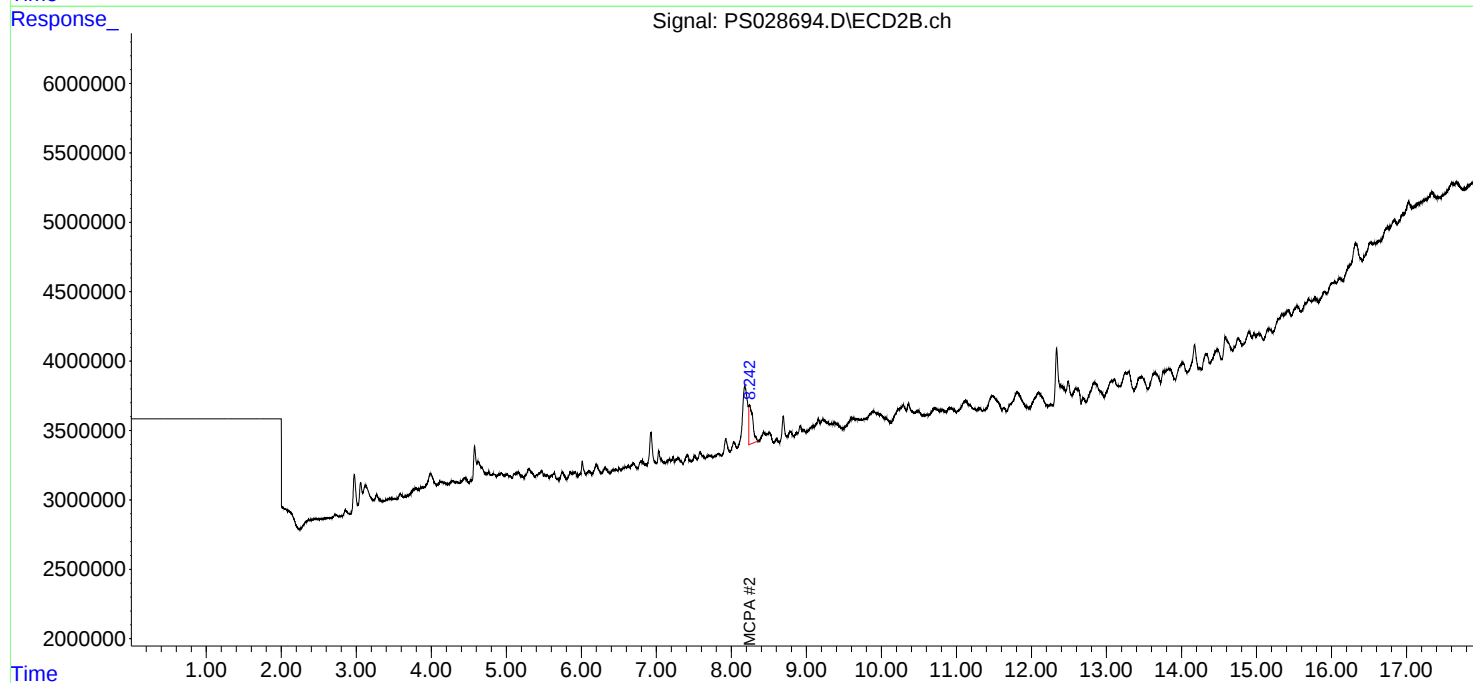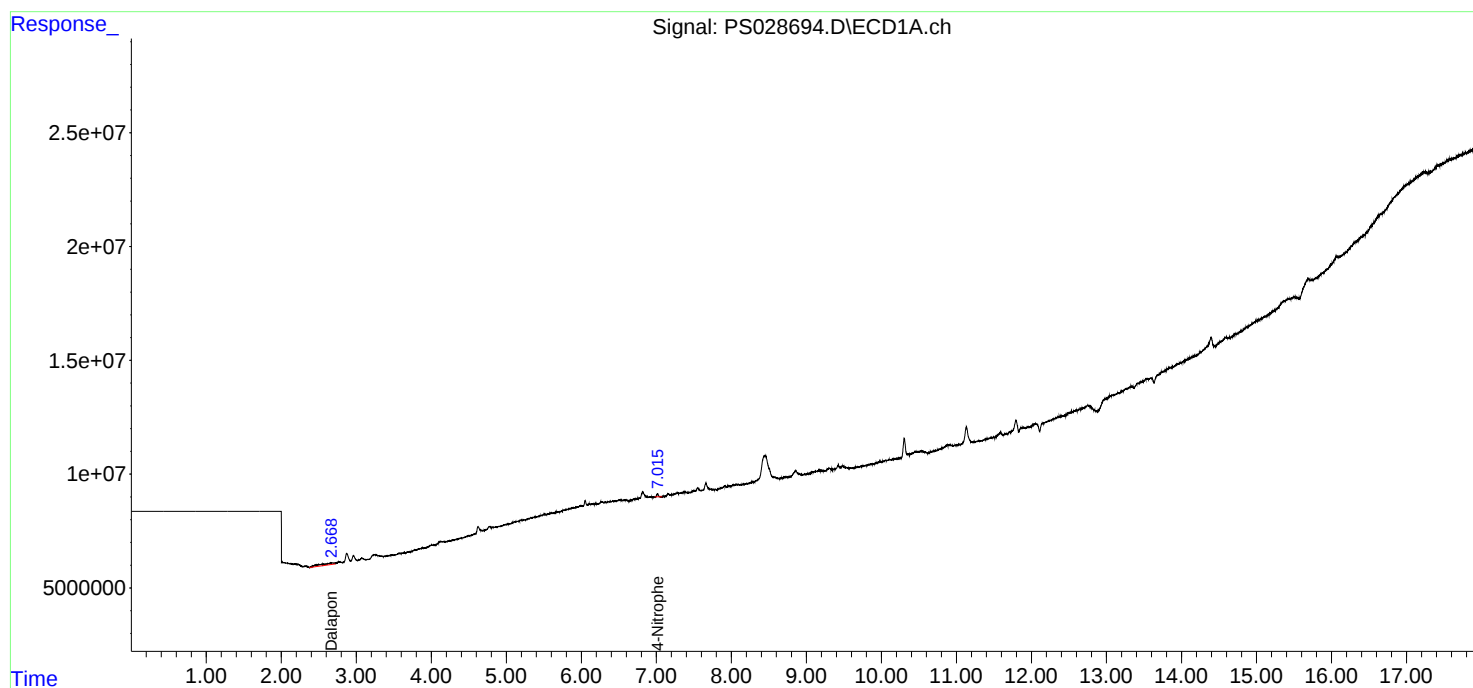


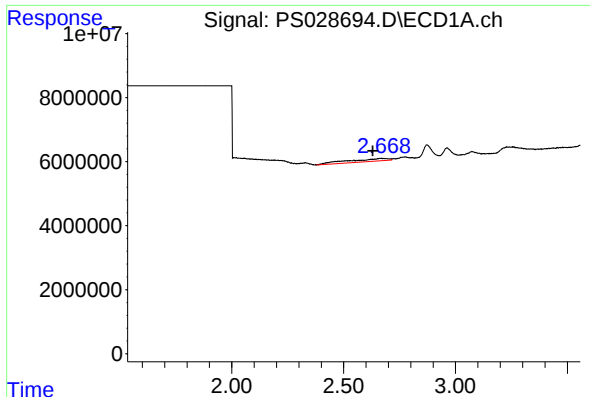

#1 Dalapon


R.T.: 2.674 min
Delta R.T.: 0.044 min
Response: 10980672
Conc: 3.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

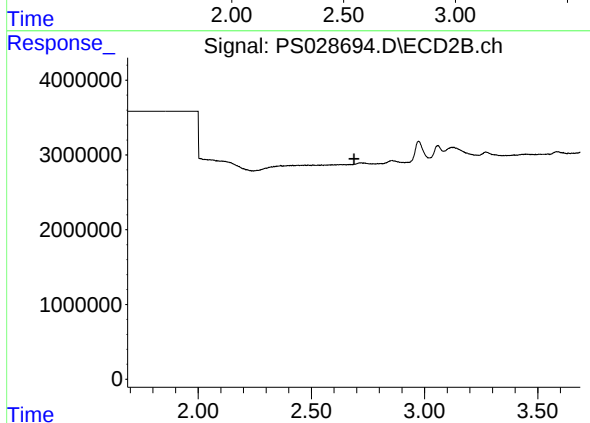


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.688 min
Response: 0
Conc: N.D.

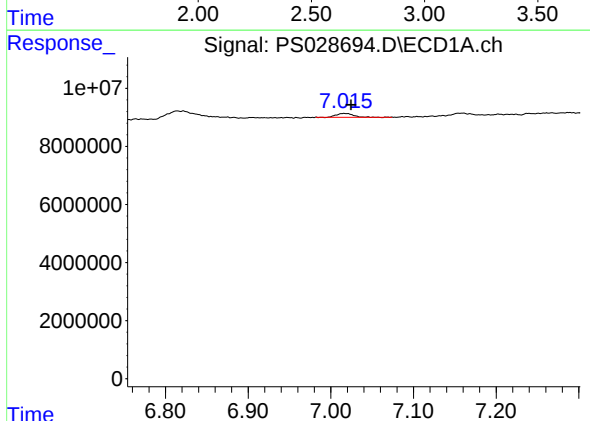


#3 4-Nitrophenol

R.T.: 7.017 min
Delta R.T.: -0.008 min
Response: 1782465
Conc: 1.04 ng/ml

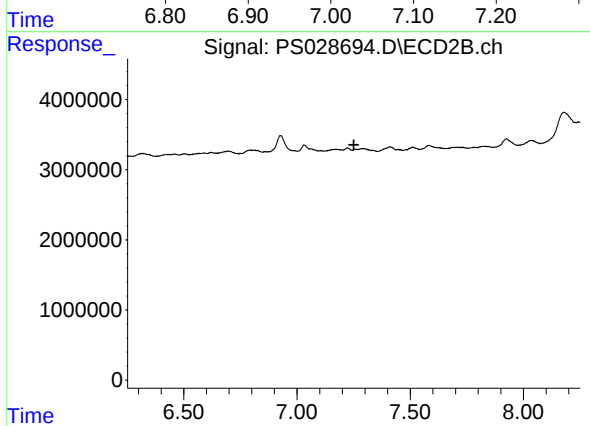

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.251 min
Response: 0
Conc: N.D.

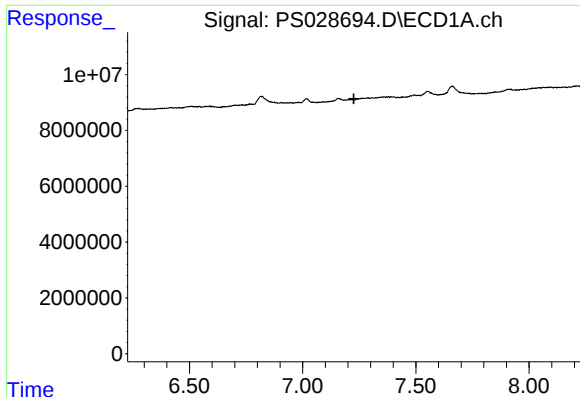

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.226 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

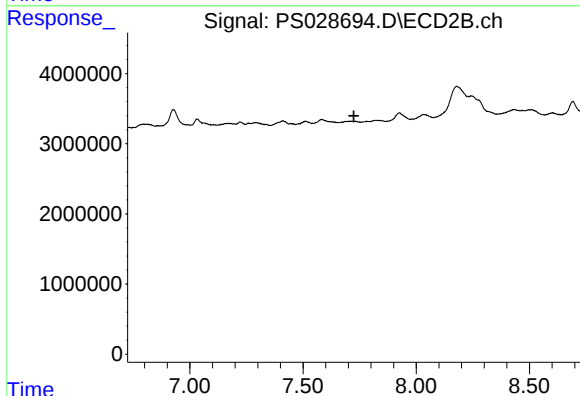


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 7.725 min
Response: 0
Conc: N.D.

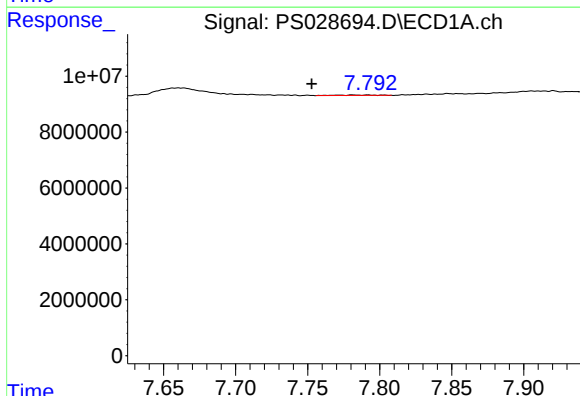

#7 MCPA

R.T.: 7.792 min
Delta R.T.: 0.039 min
Response: 305026
Conc: N.D.

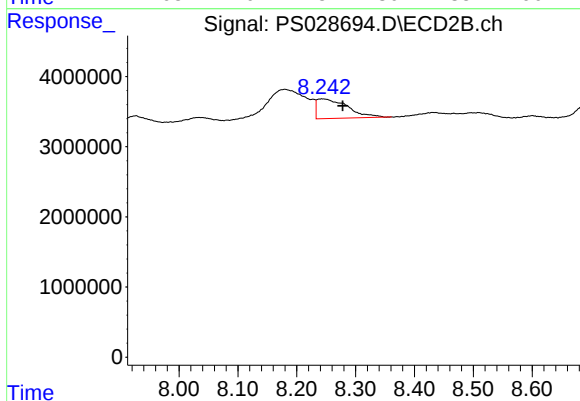

#7 MCPA

R.T.: 8.243 min
Delta R.T.: -0.035 min
Response: 10035981
Conc: 1.62 ug/ml