

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120524\
 Data File : PS028695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2024 11:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 00:14:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.231	7.724	1384.1E6	594.4E6	516.023	441.231
Target Compounds							
1) T	Dalapon	2.675f	0.000	22310545	0	7.688	N.D. #
2) T	3,5-DICHL...	6.445f	0.000	648736	0	<MDL	N.D. #
3) T	4-Nitroph...	7.025	0.000	5777675	0	3.361	N.D. #
5) T	DICAMBA	0.000	7.922	0	3597436	N.D.	<MDL
7) T	MCPA	7.779f	0.000	486580	0	<MDL	N.D. #
8) T	DICHLORPROP	8.097	0.000	1872230	0	<MDL	N.D. #
10) T	Pentachlo...	8.654	0.000	1255567	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.237	0.000	1177429	0	<MDL	N.D. #
12) T	2,4,5-T	9.533	10.293	2256580	5113220	<MDL	<MDL #
14) T	DINOSEB	11.306	0.000	2276300	0	<MDL	N.D. #
15) T	Picloram	11.135	12.337	22479469	8441909	<MDL	<MDL #
16) T	DCPA	11.597	0.000	2168701	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120524\
Data File : PS028695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2024 11:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 00:14:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

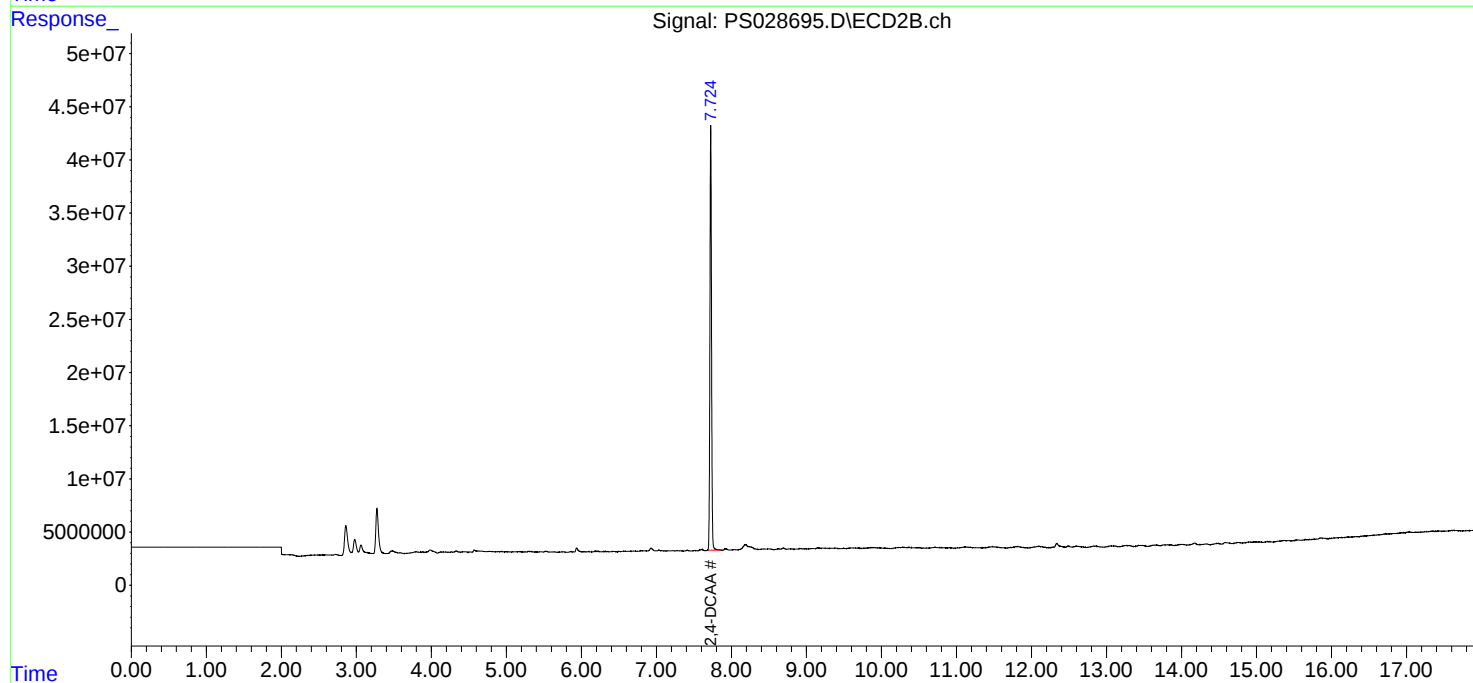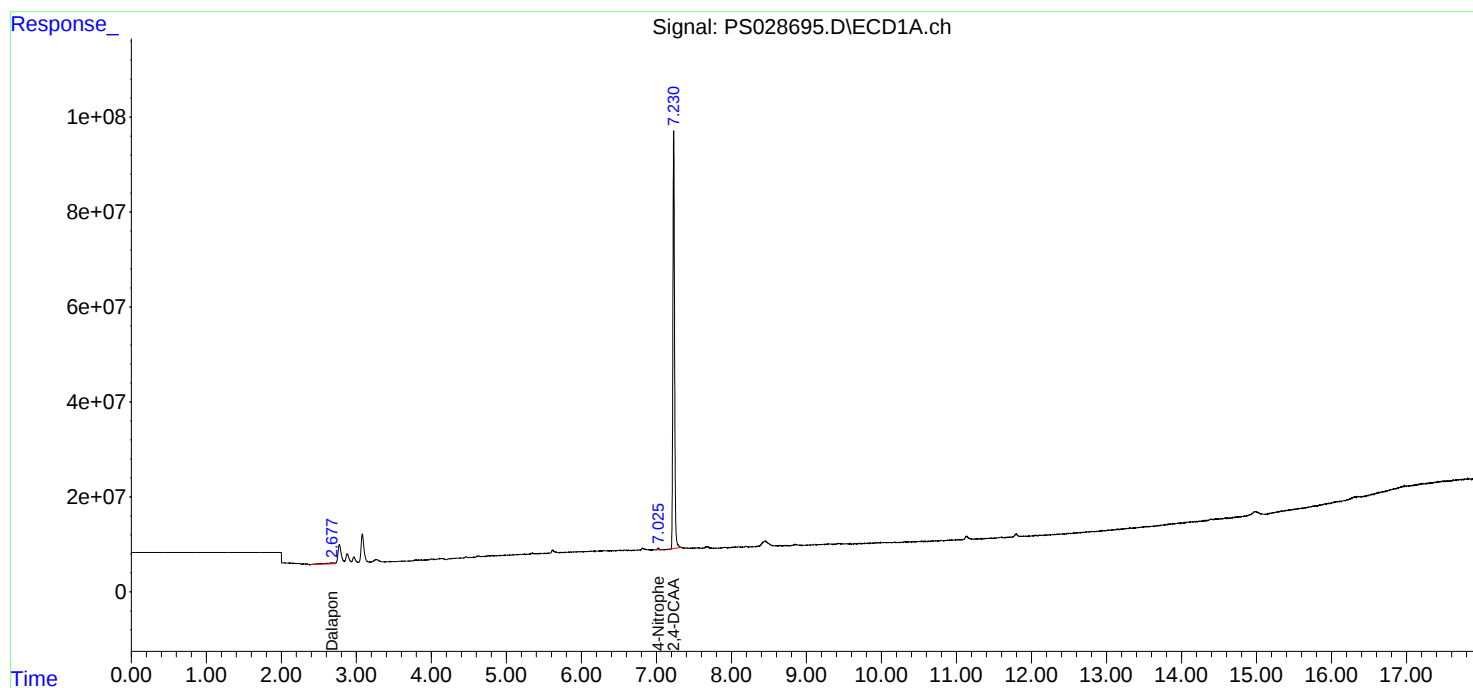


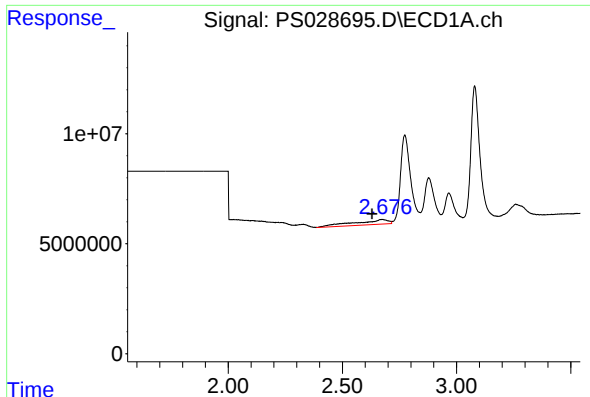

#1 Dalapon


R.T.: 2.675 min
Delta R.T.: 0.045 min
Response: 22310545
Conc: 7.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

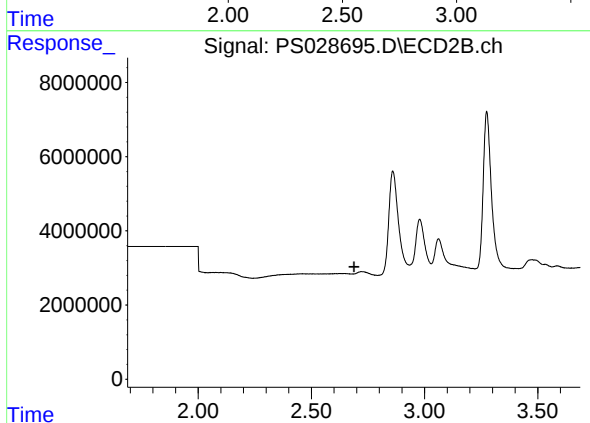


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.688 min
Response: 0
Conc: N.D.

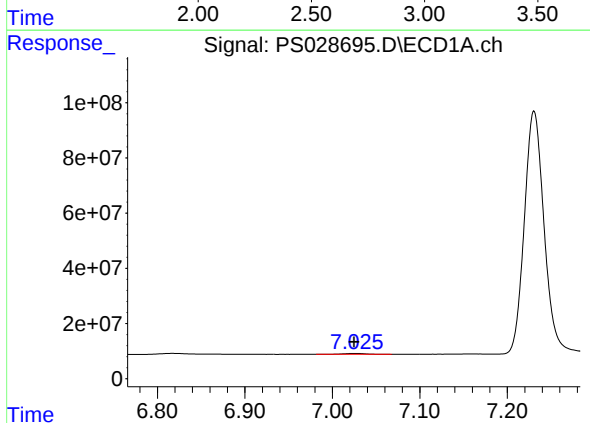


#3 4-Nitrophenol

R.T.: 7.025 min
Delta R.T.: 0.000 min
Response: 5777675
Conc: 3.36 ng/ml

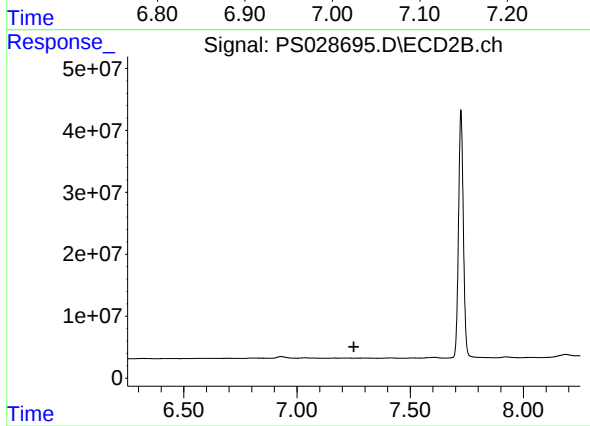

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.251 min
Response: 0
Conc: N.D.

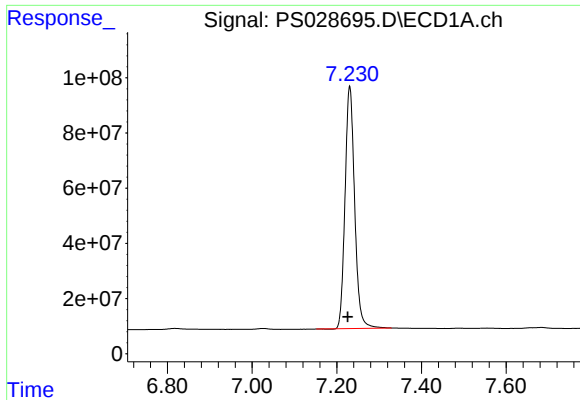

#4 2,4-DCAA

R.T.: 7.231 min
Delta R.T.: 0.004 min
Response: 1384149922
Conc: 516.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

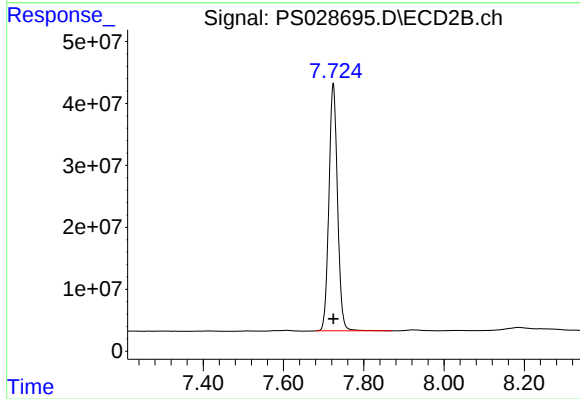

#4 2,4-DCAA

R.T.: 7.724 min
Delta R.T.: 0.000 min
Response: 594351873
Conc: 441.23 ng/ml