

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120524\
 Data File : PS028698.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2024 13:03
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 00:15:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.230	7.724	1379.1E6	600.9E6	514.141	446.104
Target Compounds							
1) T	Dalapon	2.671f	0.000	20508012	0	7.067	N.D. #
3) T	4-Nitroph...	7.023	0.000	6533817	0	3.801	N.D. #
5) T	DICAMBA	7.416	7.922	419650	4108720	<MDL	<MDL #
7) T	MCPA	7.783f	0.000	527000	0	<MDL	N.D. #
8) T	DICHLORPROP	8.092f	0.000	2302588	0	<MDL	N.D. #
10) T	Pentachlo...	8.652	0.000	3241599	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.233	9.872	1858404	3592989	<MDL	<MDL #
12) T	2,4,5-T	9.529	10.293	8048081	9650168	<MDL	1.037 #
13) T	2,4-DB	10.099	0.000	2001551	0	<MDL	N.D. #
14) T	DINOSEB	11.297	0.000	7949992	0	<MDL	N.D. #
15) T	Picloram	11.132	12.335	95977744	25994339	3.228	2.017 #
16) T	DCPA	11.587	0.000	11240077	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120524\
Data File : PS028698.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2024 13:03
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 00:15:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

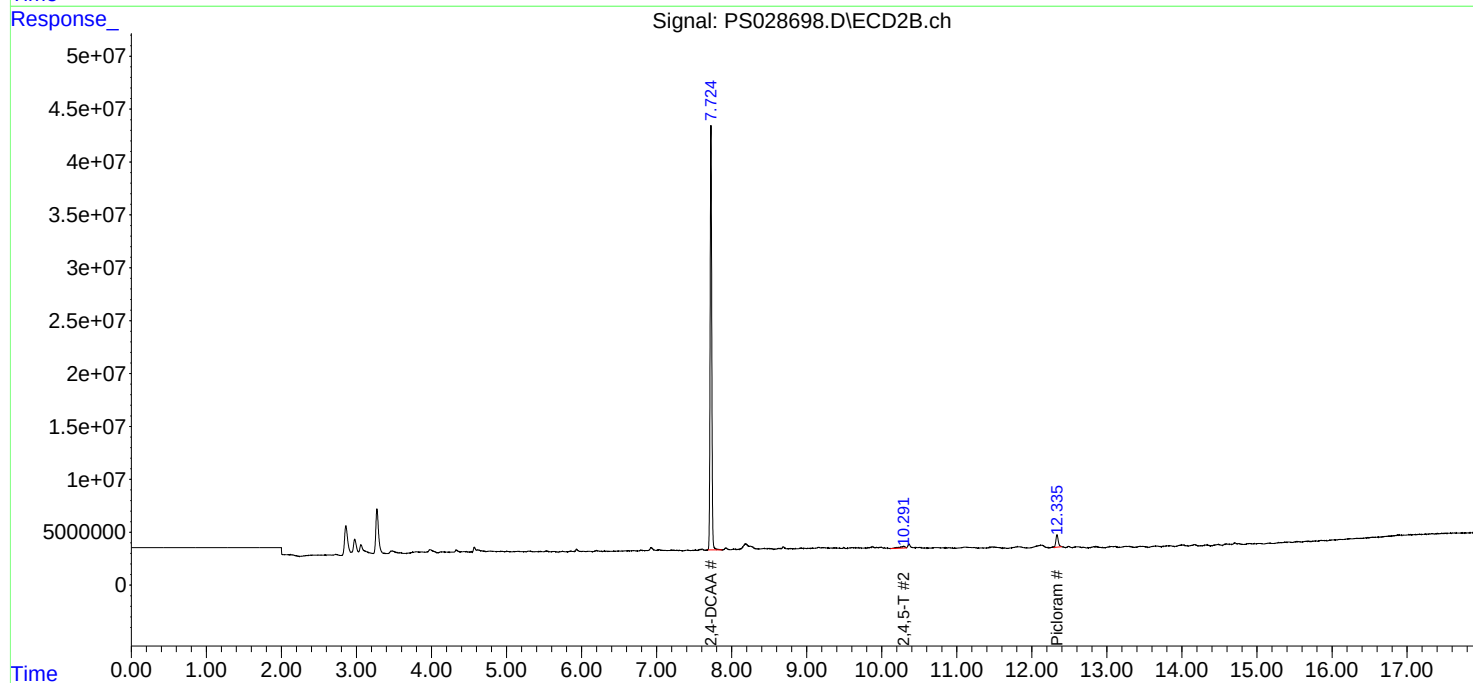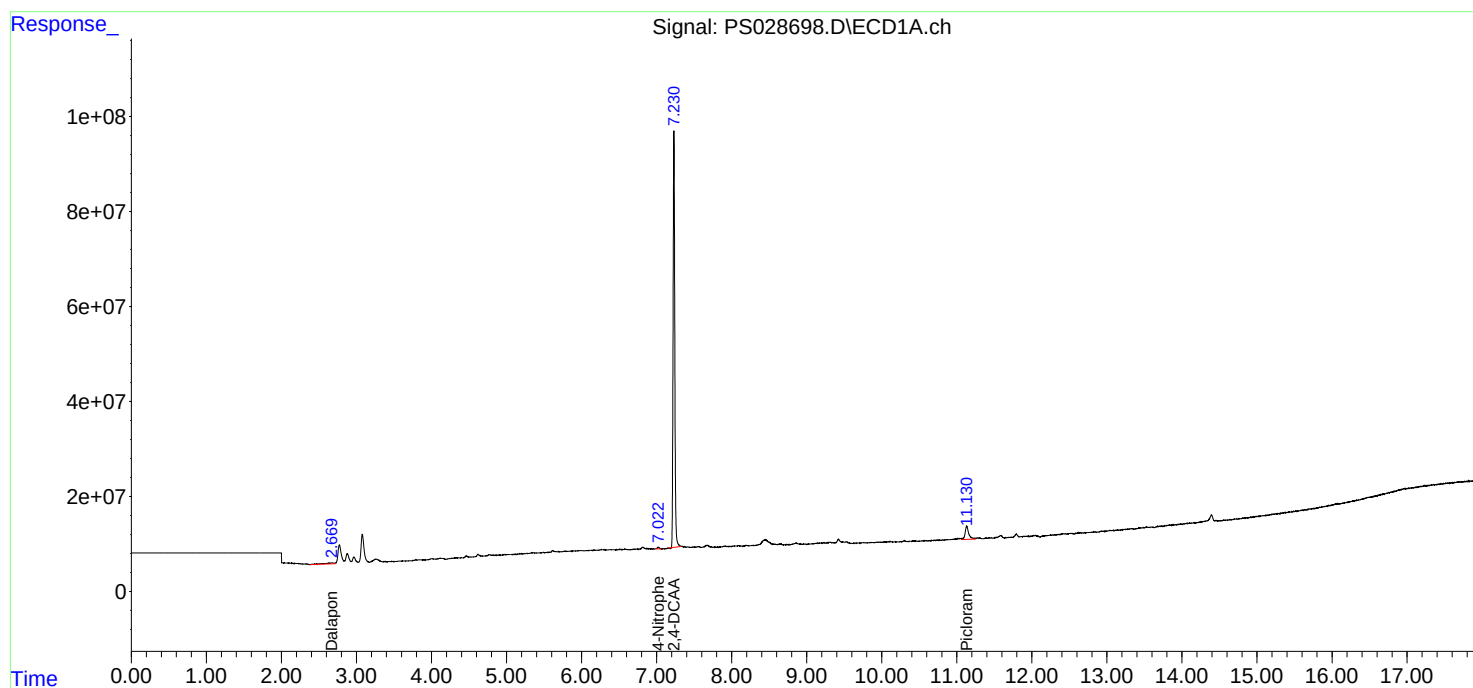


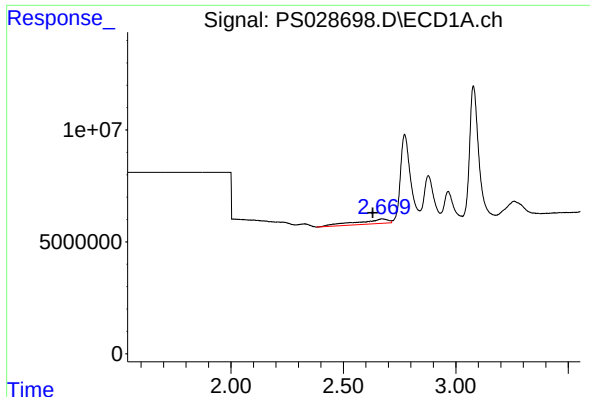

#1 Dalapon


R.T.: 2.671 min
Delta R.T.: 0.041 min
Response: 20508012
Conc: 7.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

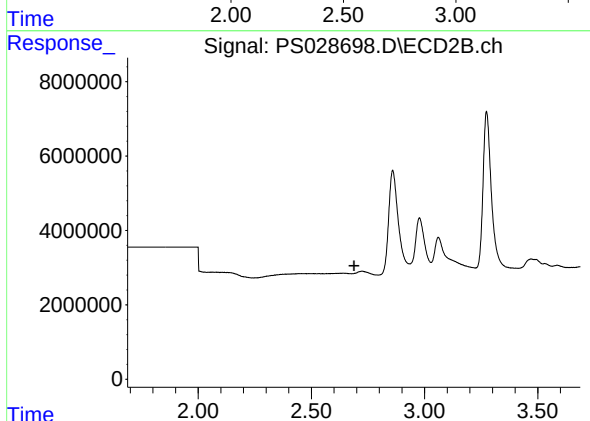


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.688 min
Response: 0
Conc: N.D.

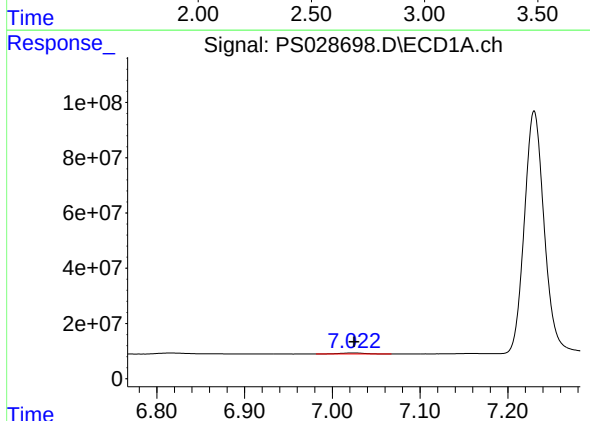


#3 4-Nitrophenol

R.T.: 7.023 min
Delta R.T.: -0.002 min
Response: 6533817
Conc: 3.80 ng/ml

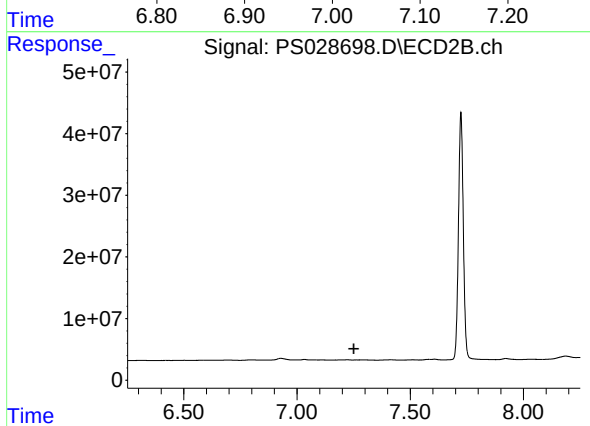

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.251 min
Response: 0
Conc: N.D.

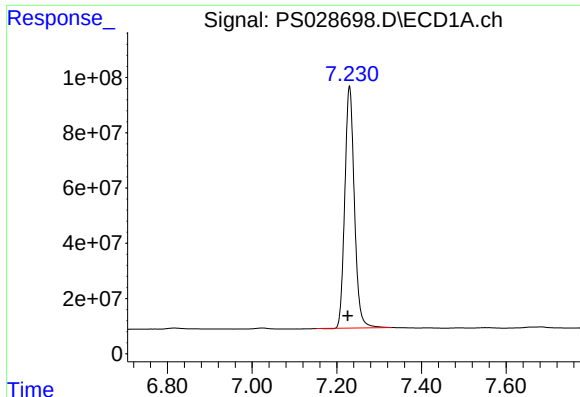

#4 2,4-DCAA


R.T.: 7.230 min
Delta R.T.: 0.004 min
Response: 1379102046
Conc: 514.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

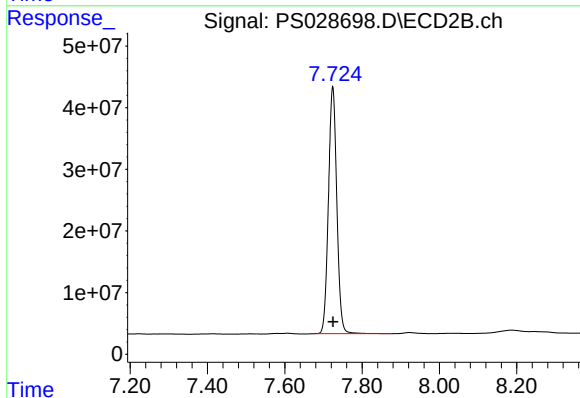


#4 2,4-DCAA

R.T.: 7.724 min
Delta R.T.: 0.000 min
Response: 600915284
Conc: 446.10 ng/ml

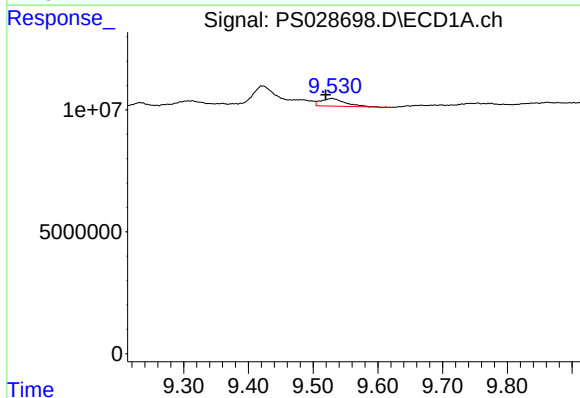


#12 2,4,5-T

R.T.: 9.529 min
Delta R.T.: 0.009 min
Response: 8048081
Conc: N.D.

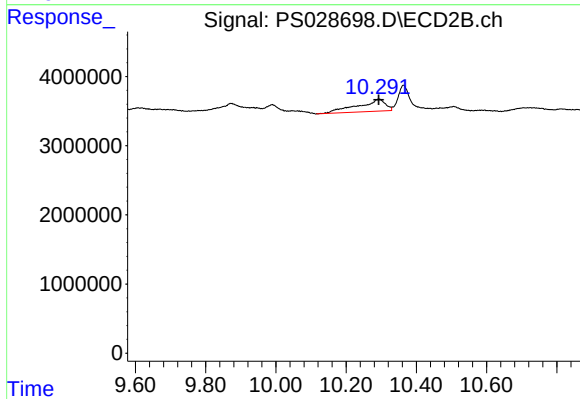

#12 2,4,5-T


R.T.: 10.293 min
Delta R.T.: 0.000 min
Response: 9650168
Conc: 1.04 ng/ml

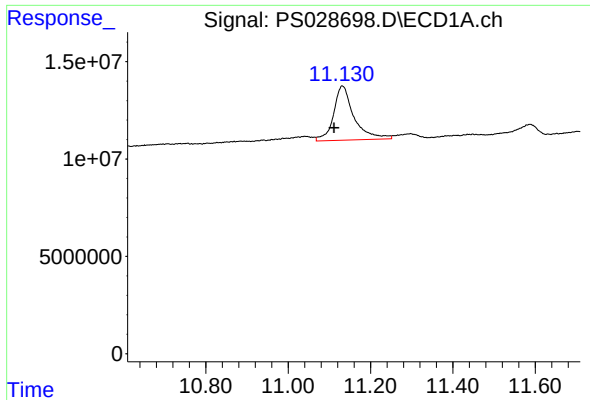

#15 Picloram

R.T.: 11.132 min
Delta R.T.: 0.020 min
Response: 95977744
Conc: 3.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

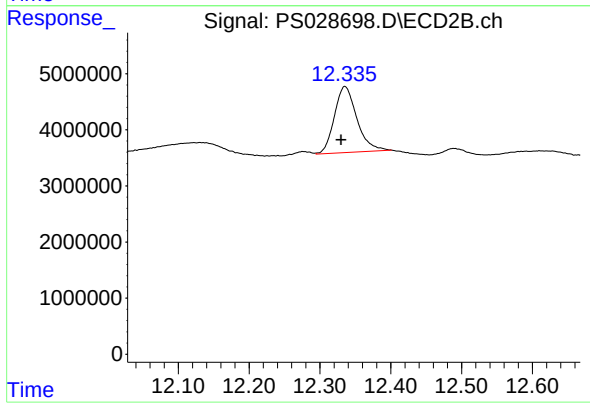

#15 Picloram

R.T.: 12.335 min
Delta R.T.: 0.006 min
Response: 25994339
Conc: 2.02 ng/ml