

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120524\
 Data File : PS028710.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2024 20:42
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 04:32:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	7.722	1360.5E6	612.0E6	507.218	454.302
Target Compounds							
1) T	Dalapon	2.675f	0.000	21495579	0	7.408	N.D. #
3) T	4-Nitroph...	7.022	0.000	5426738	0	3.157	N.D. #
5) T	DICAMBA	0.000	7.919	0	4518829	N.D.	<MDL
7) T	MCPA	0.000	8.239f	0	9834029	N.D.	1.585
8) T	DICHLORPROP	8.089f	8.686f	48959	3988725	<MDL	2.495 #
10) T	Pentachlo...	8.651	0.000	1560800	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.229	0.000	1291755	0	<MDL	N.D. #
12) T	2,4,5-T	9.527	10.291	3473970	8403995	<MDL	<MDL #
15) T	Picloram	11.125	12.335	11412094	4215779	<MDL	<MDL #
16) T	DCPA	11.597	0.000	2617421	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120524\
Data File : PS028710.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2024 20:42
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 04:32:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

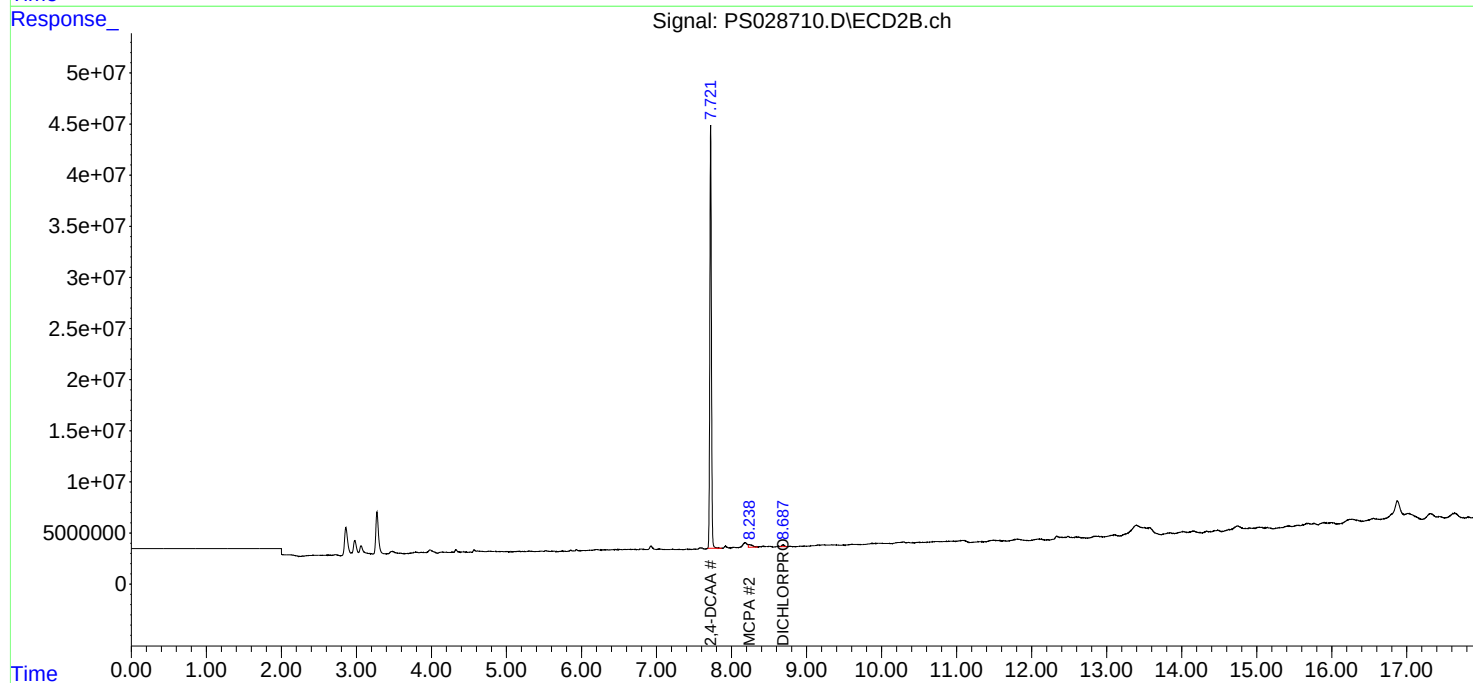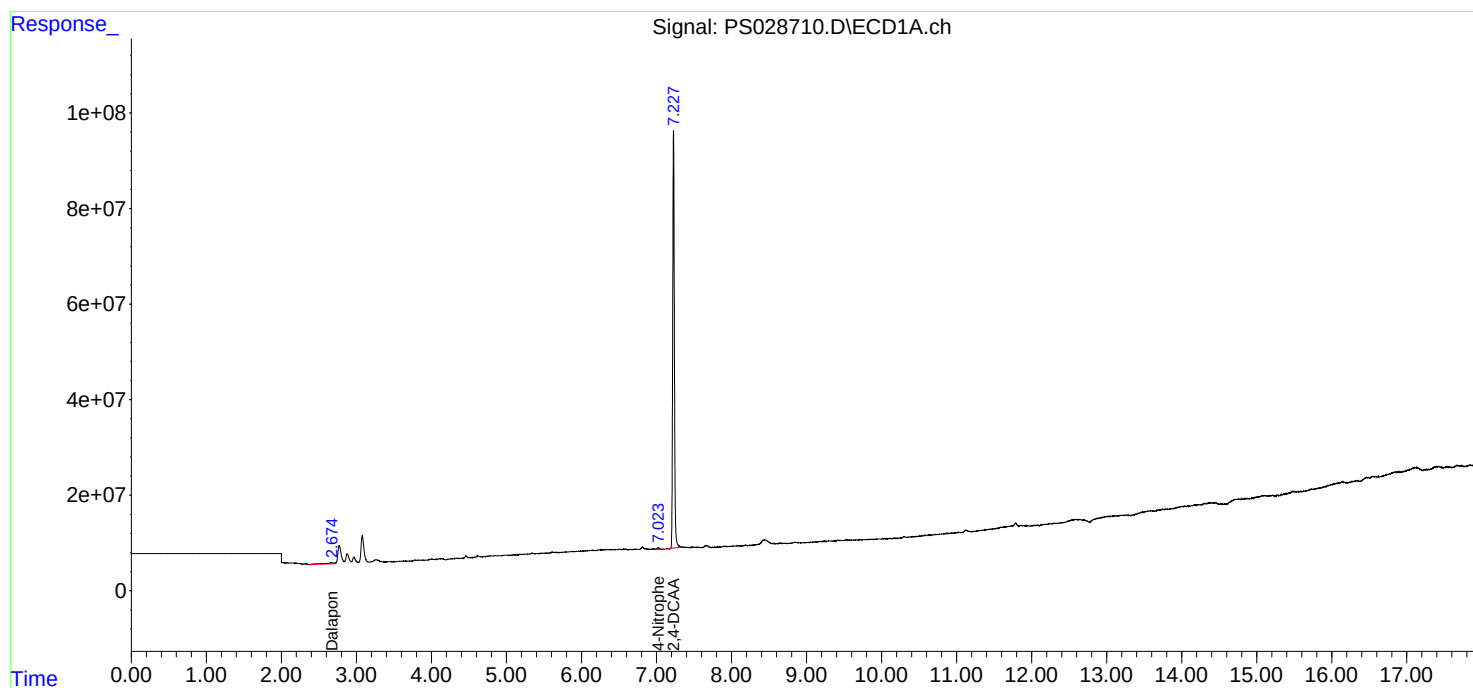


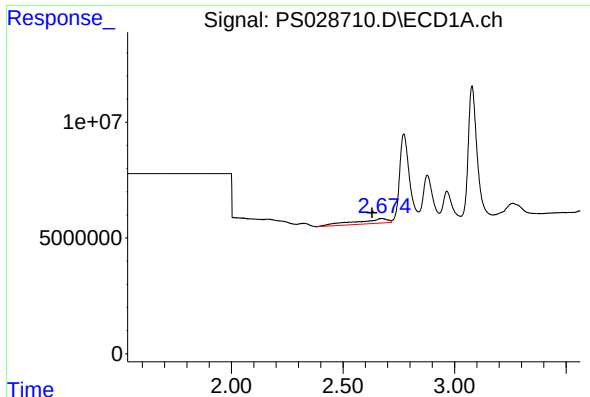

#1 Dalapon


R.T.: 2.675 min
Delta R.T.: 0.045 min
Response: 21495579
Conc: 7.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

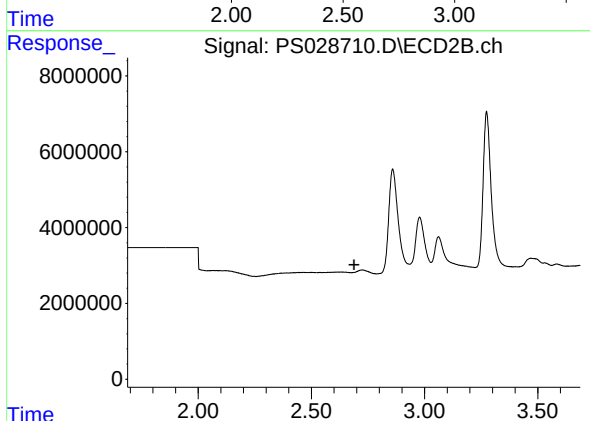


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.688 min
Response: 0
Conc: N.D.

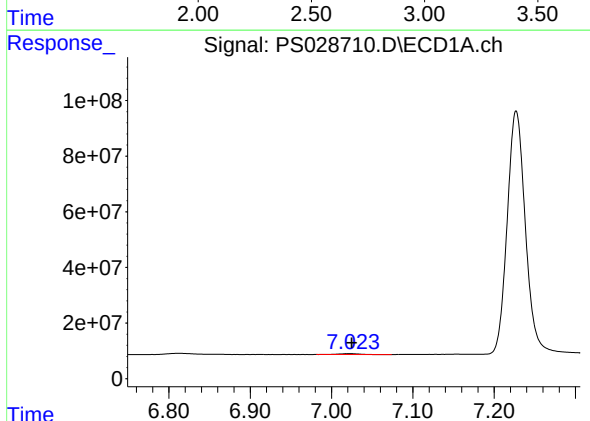


#3 4-Nitrophenol

R.T.: 7.022 min
Delta R.T.: -0.002 min
Response: 5426738
Conc: 3.16 ng/ml

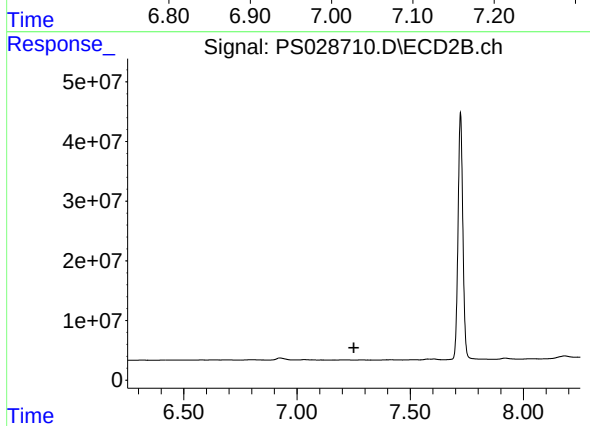

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.251 min
Response: 0
Conc: N.D.

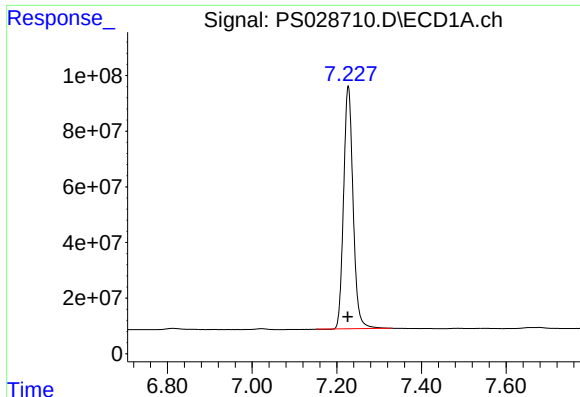

#4 2,4-DCAA


R.T.: 7.227 min
Delta R.T.: 0.001 min
Response: 1360533049
Conc: 507.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

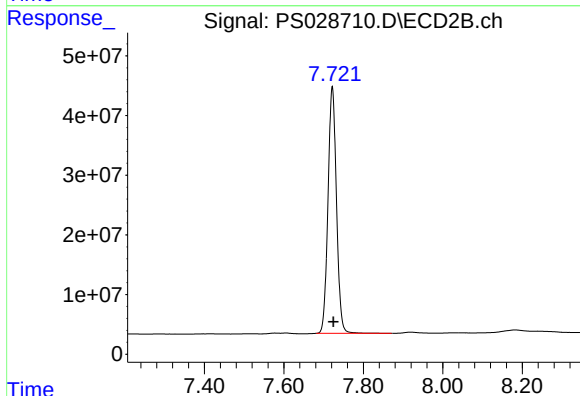


#4 2,4-DCAA

R.T.: 7.722 min
Delta R.T.: -0.003 min
Response: 611958581
Conc: 454.30 ng/ml

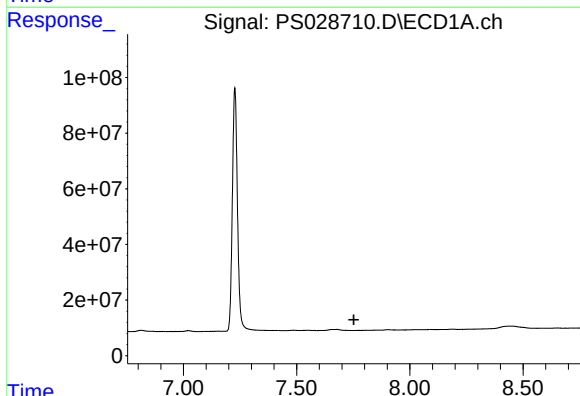


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.753 min
Response: 0
Conc: N.D.

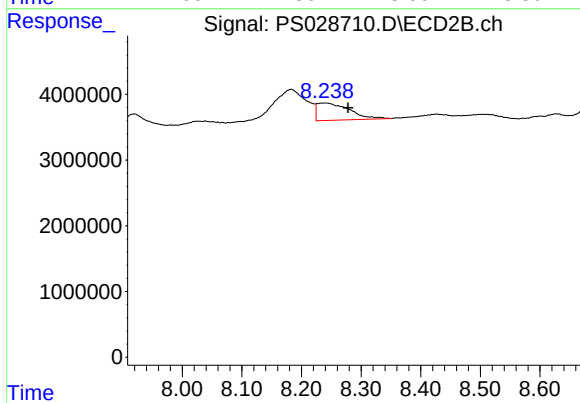

#7 MCPA


R.T.: 8.239 min
Delta R.T.: -0.040 min
Response: 9834029
Conc: 1.58 ug/ml

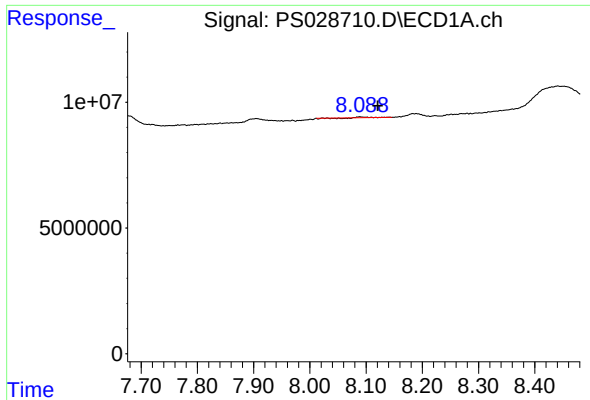

#8 DICHLORPROP

R.T.: 8.089 min
Delta R.T.: -0.032 min
Response: 48959
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

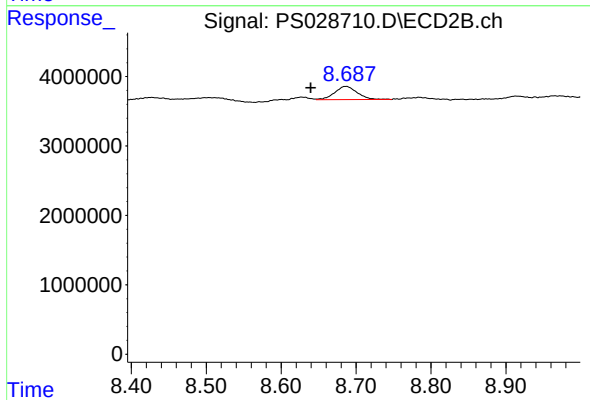

#8 DICHLORPROP

R.T.: 8.686 min
Delta R.T.: 0.047 min
Response: 3988725
Conc: 2.50 ng/ml