

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120525\
 Data File : PS032627.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Dec 2025 13:31
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 00:25:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120325.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 03 13:46:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.007	7.374	1644.0E6	1586.1E6	297.628	295.840
Target Compounds							
2) T	3,5-DICHL...	6.232	6.349f	3712305	1247736	<MDL	<MDL #
3) T	4-Nitroph...	6.834f	0.000	17881272	0	14.253	N.D. #
5) T	DICAMBA	0.000	7.591	0	3684254	N.D.	<MDL
6) T	MCP	0.000	7.679	0	1075939	N.D.	<MDL
7) T	MCPA	0.000	7.931	0	14020370	N.D.	<MDL
8) T	DICHLORPROP	7.883	8.274	110.7E6	1802993	20.546	<MDL #
9) T	2,4-D	0.000	8.652f	0	19601560	N.D.	3.490
10) T	Pentachlo...	8.378	9.111	5001677	33764722	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	9.532f	0	533.7E6	N.D.	18.602
12) T	2,4,5-T	9.224f	0.000	7531360	0	<MDL	N.D. #
13) T	2,4-DB	0.000	10.525f	0	708.4E6	N.D.	173.894
14) T	DINOSEB	0.000	10.909f	0	4677.0E6	N.D.	258.620



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120525\
Data File : PS032627.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Dec 2025 13:31
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 00:25:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120325.M
Quant Title : 8080.M
QLast Update : Wed Dec 03 13:46:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

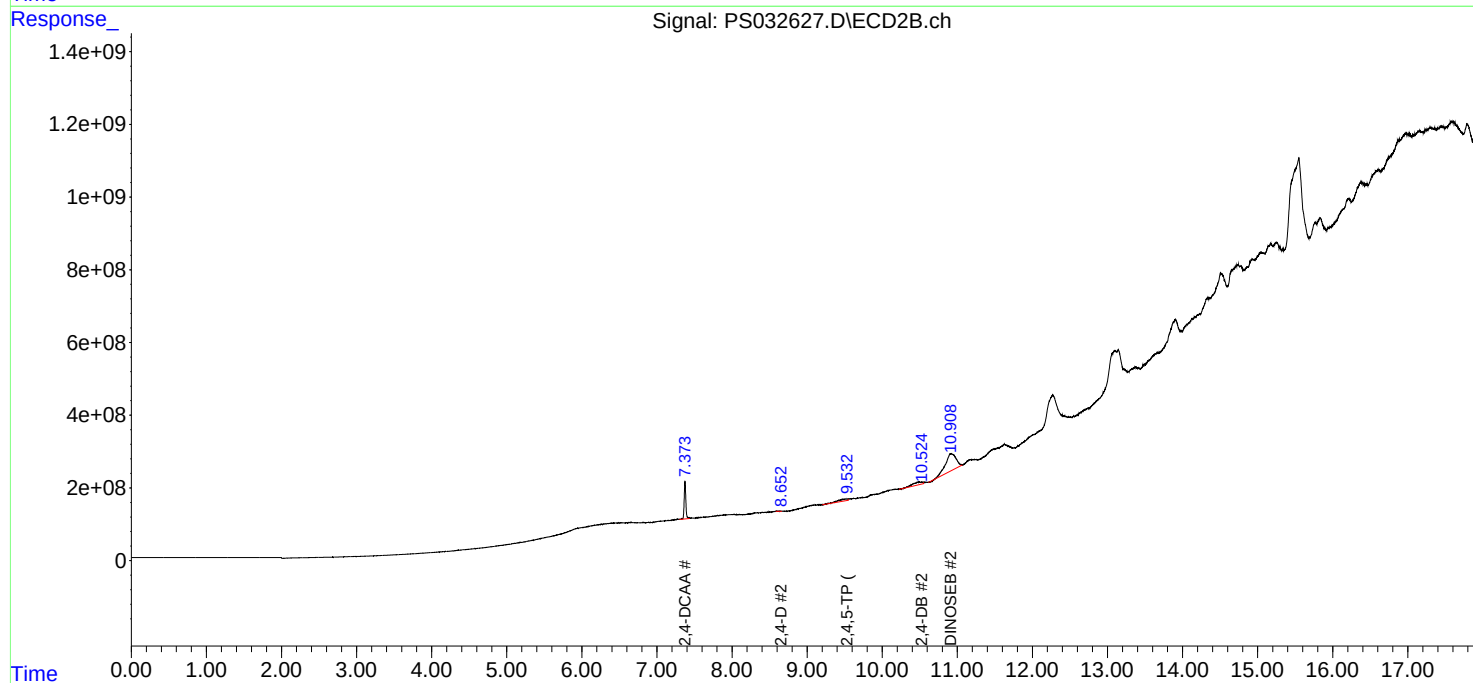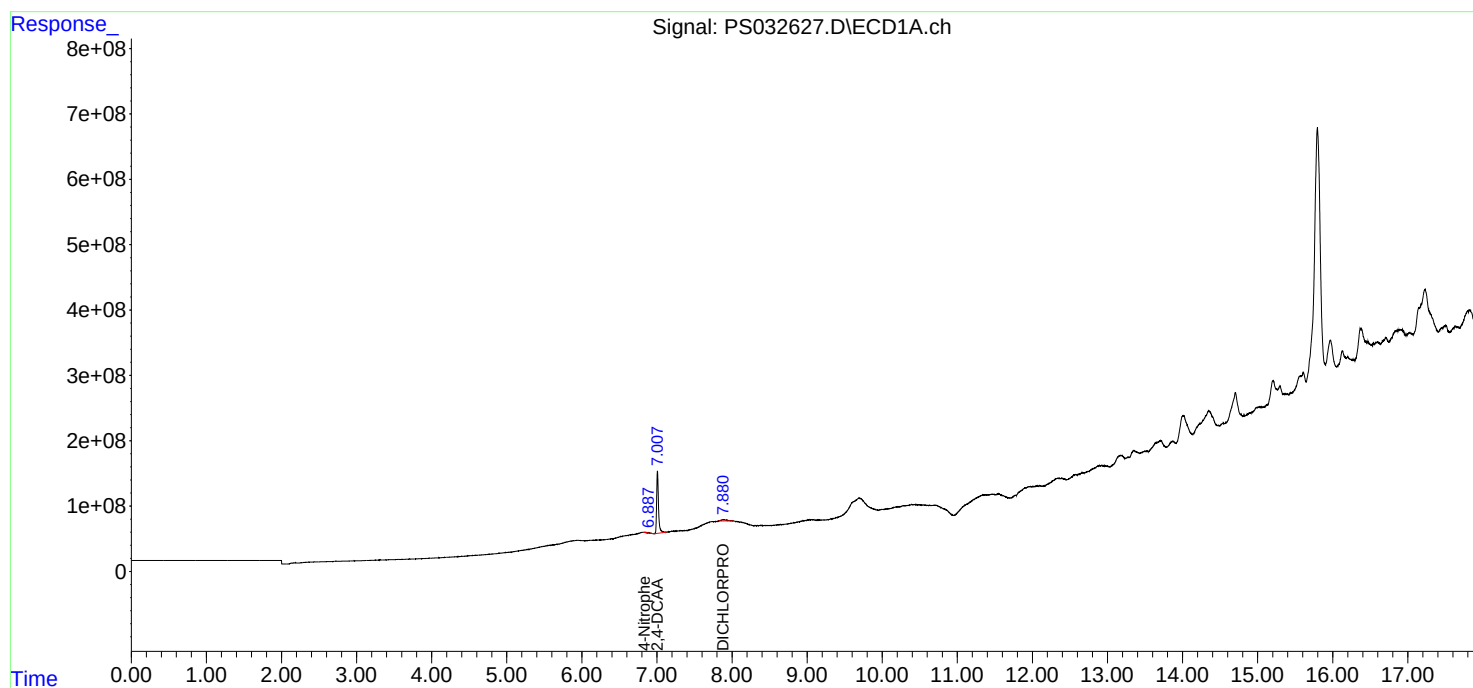


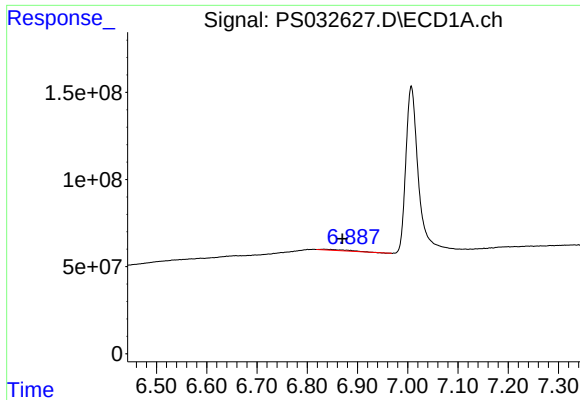

#3 4-Nitrophenol


R.T.: 6.834 min
Delta R.T.: -0.036 min
Response: 17881272
Conc: 14.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

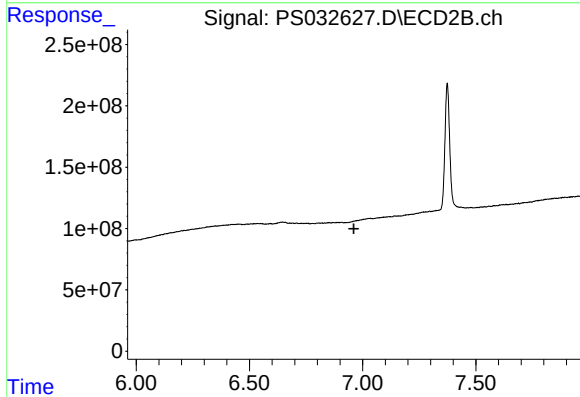


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.961 min
Response: 0
Conc: N.D.

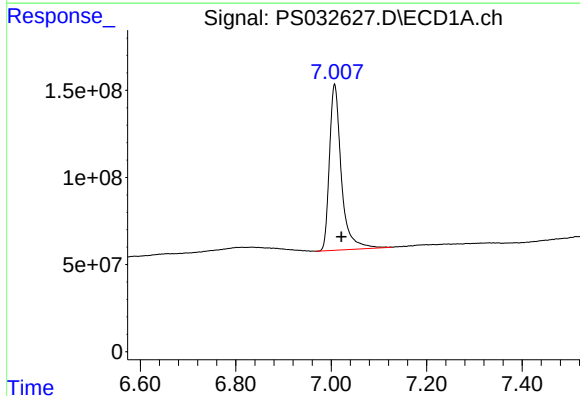


#4 2,4-DCAA

R.T.: 7.007 min
Delta R.T.: -0.014 min
Response: 1643991320
Conc: 297.63 ng/ml

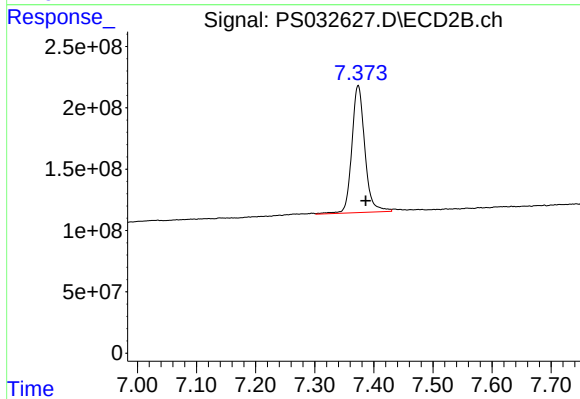

#4 2,4-DCAA


R.T.: 7.374 min
Delta R.T.: -0.013 min
Response: 1586062370
Conc: 295.84 ng/ml

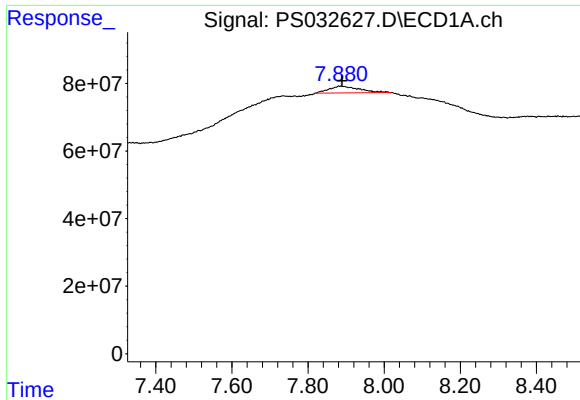

#8 DICHLORPROP


R.T.: 7.883 min
Delta R.T.: -0.006 min
Response: 110737112
Conc: 20.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

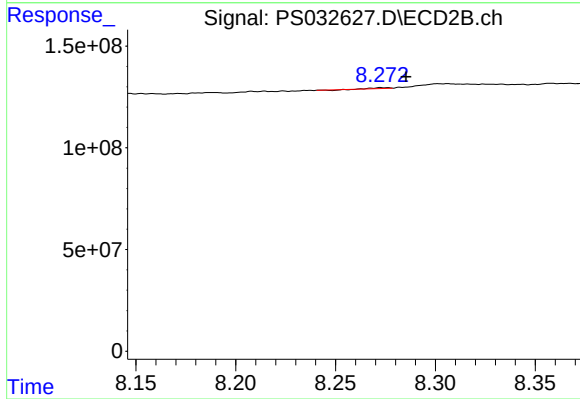


#8 DICHLORPROP

R.T.: 8.274 min
Delta R.T.: -0.012 min
Response: 1802993
Conc: N.D.

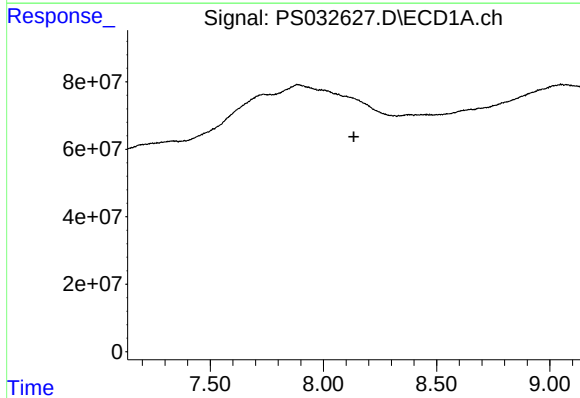


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

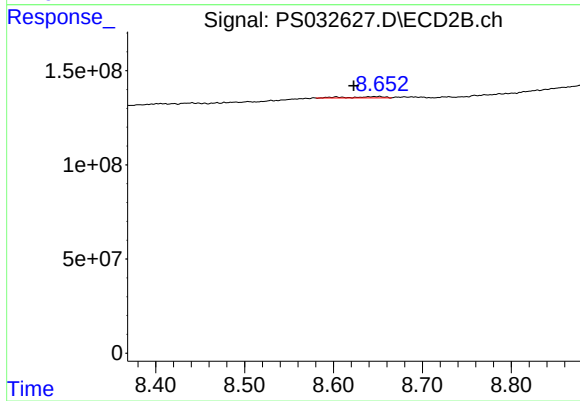

#9 2,4-D


R.T.: 8.652 min
Delta R.T.: 0.029 min
Response: 19601560
Conc: 3.49 ng/ml

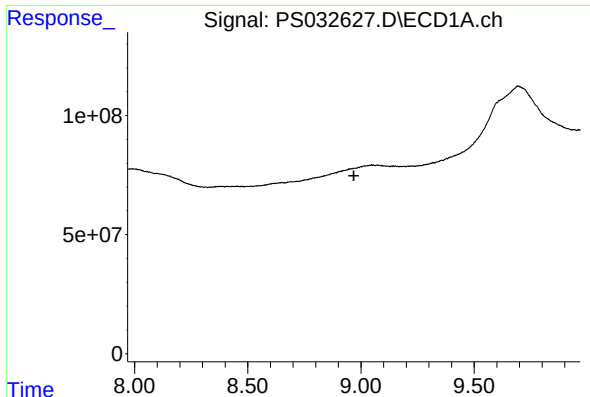

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 8.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

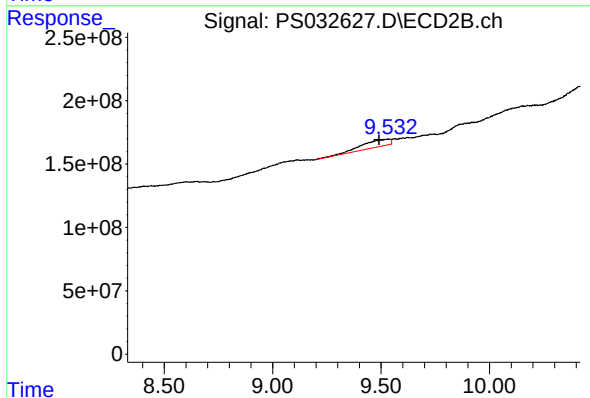


#11 2,4,5-TP (SILVEX)

R.T.: 9.532 min
Delta R.T.: 0.042 min
Response: 533650544
Conc: 18.60 ng/ml

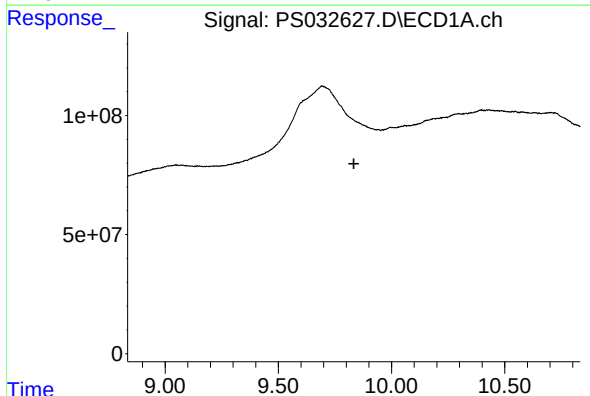


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 9.834 min
Response: 0
Conc: N.D.

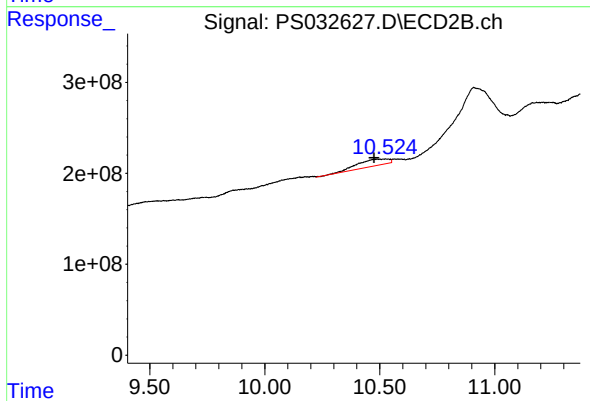

#13 2,4-DB


R.T.: 10.525 min
Delta R.T.: 0.049 min
Response: 708368319
Conc: 173.89 ng/ml

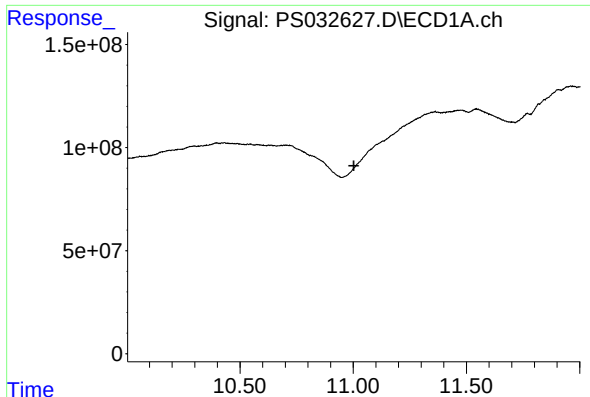

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.003 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

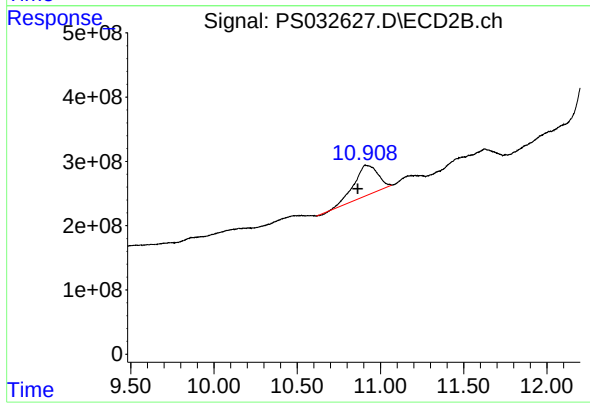

#14 DINOSEB

R.T.: 10.909 min
Delta R.T.: 0.045 min
Response: 4677023789
Conc: 258.62 ng/ml