

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120618\
 Data File : PS002514.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2018 20:21
 Operator : EI\SJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 05:57:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 10 05:54:48 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.420	10.915	240.4E6	295.2E6	750.000	750.000
Target Compounds							
1) T	Dalapon	2.944	2.385	321.1E6	316.5E6	682.500	682.500
2) T	3,5-DICHL...	9.851	9.071	335.8E6	338.2E6	697.500	697.500
3) T	4-Nitroph...	11.013	10.061	110.9E6	124.1E6	682.500	682.500
5) T	DICAMBA	11.729	11.198	1023.2E6	1035.9E6	705.000	705.000
6) T	MCPD	12.069	11.429	71543567	69063283	70.500	70.500
7) T	MCPA	12.319	11.804	108.9E6	106.3E6	69.750	69.750
8) T	DICHLORPROP	12.915	12.322	253.1E6	261.0E6	705.000	705.000
9) T	2,4-D	13.274	12.792	255.9E6	308.4E6	705.000	705.000
10) T	Pentachlo...	13.651	13.337	3650.9E6	3844.0E6	712.500	712.500
11) T	2,4,5-TP ...	14.519	13.956	1422.4E6	1540.3E6	712.500	712.500
12) T	2,4,5-T	14.917	14.518	1378.5E6	1248.2E6	712.500	712.500
13) T	2,4-DB	15.663	15.169	164.6E6	181.4E6	712.500	712.500
14) T	DINOSEB	17.138	15.596	1037.6E6	1094.7E6	705.000	705.000
15) T	Picloram	16.906	16.773	1883.7E6	2005.9E6	712.500	712.500
16) T	DCPA	17.481	16.825	1794.1E6	2191.2E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120618\
Data File : PS002514.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2018 20:21
Operator : EI\SJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 05:57:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
Quant Title : 8080.M
QLast Update : Mon Dec 10 05:54:48 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

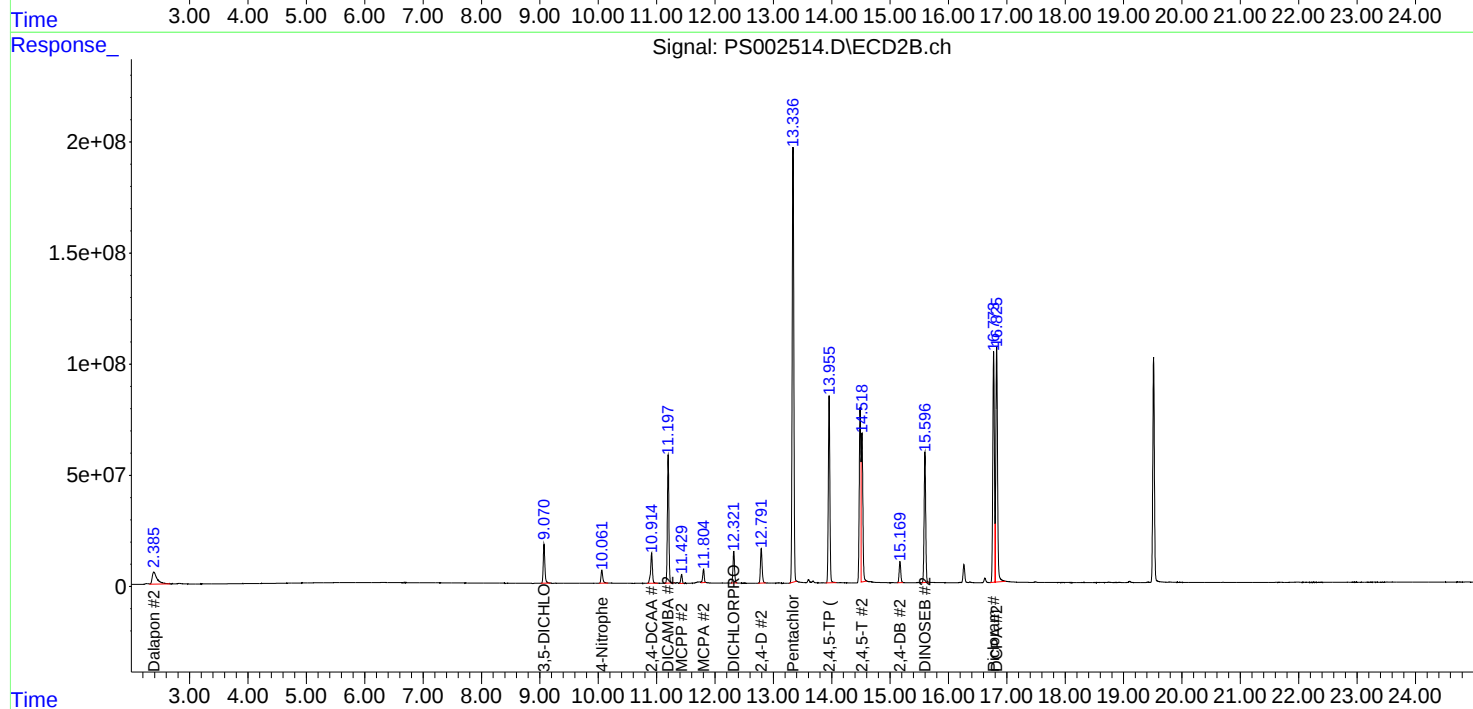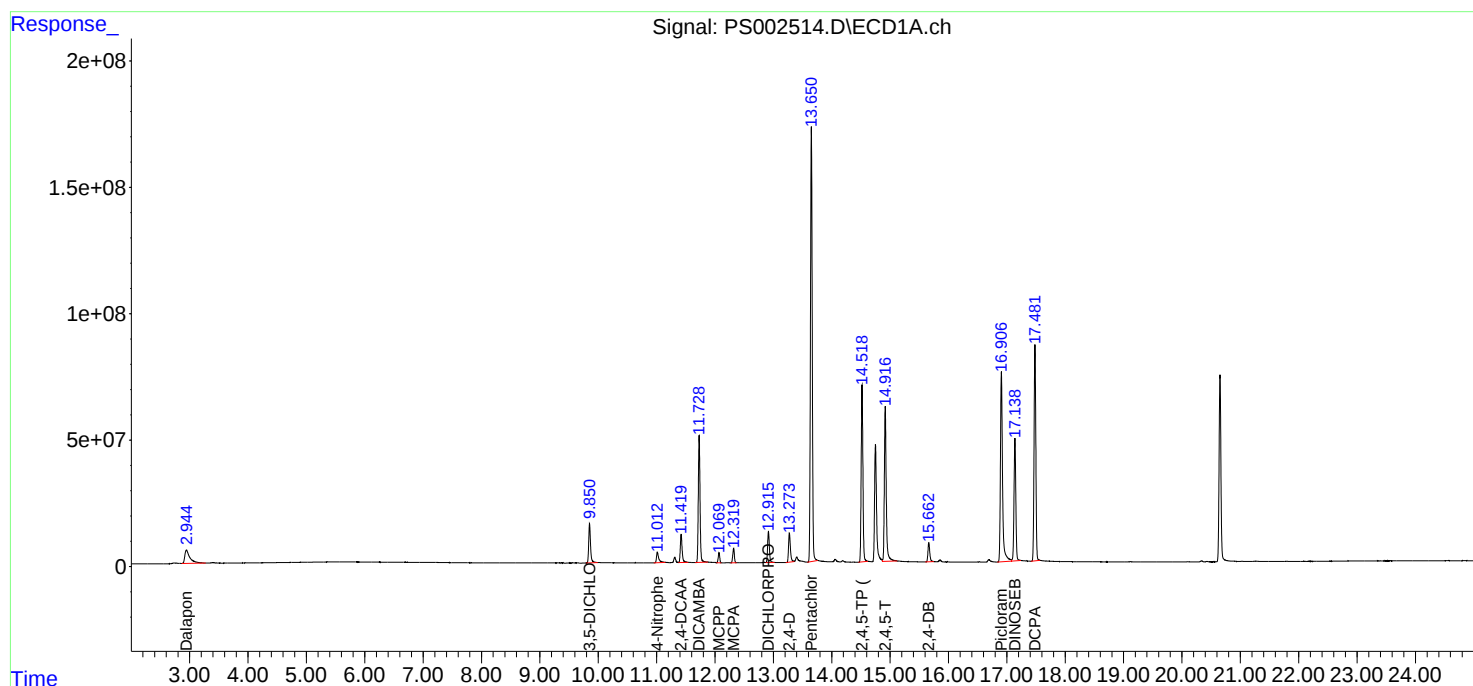


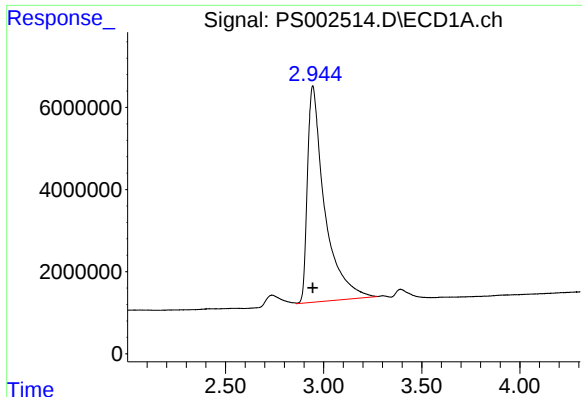

#1 Dalapon


R.T.: 2.944 min
Delta R.T.: 0.000 min
Response: 321071502
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

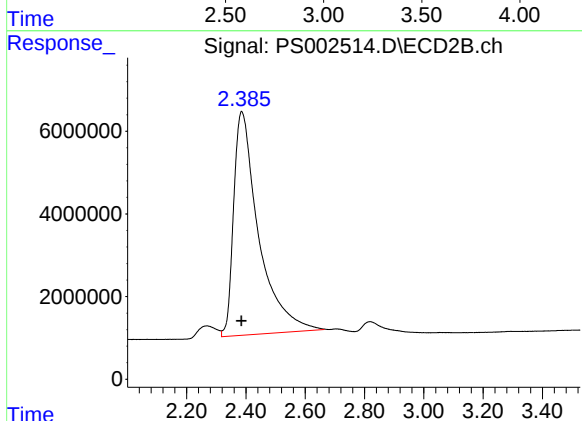


#1 Dalapon

R.T.: 2.385 min
Delta R.T.: 0.000 min
Response: 316515501
Conc: 682.50 ng/ml

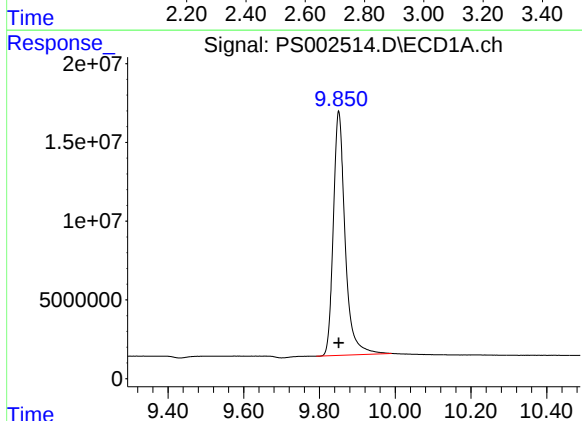


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.851 min
Delta R.T.: 0.000 min
Response: 335780235
Conc: 697.50 ng/ml

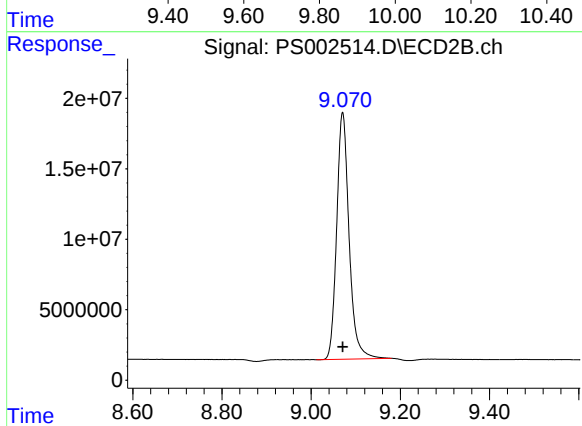

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.071 min
Delta R.T.: 0.000 min
Response: 338176091
Conc: 697.50 ng/ml

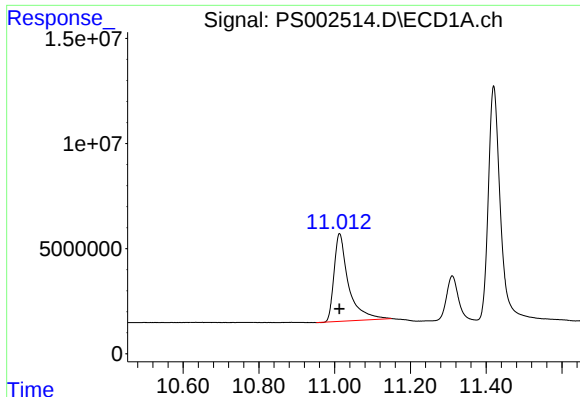

#3 4-Nitrophenol


R.T.: 11.013 min
Delta R.T.: 0.000 min
Response: 110942579
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

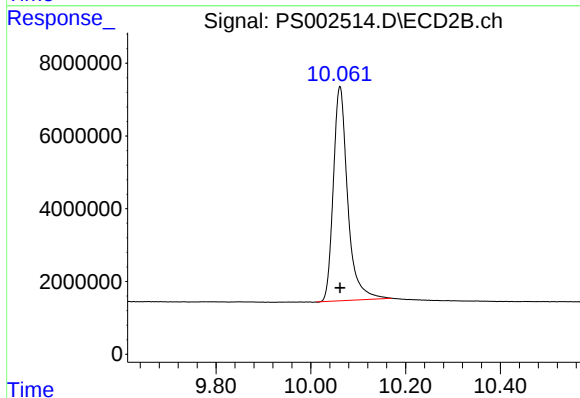


#3 4-Nitrophenol

R.T.: 10.061 min
Delta R.T.: 0.000 min
Response: 124098855
Conc: 682.50 ng/ml

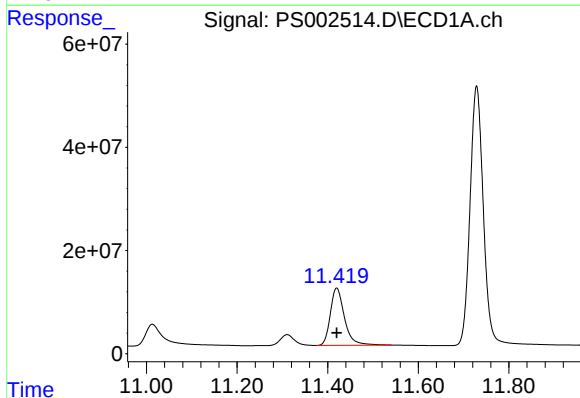


#4 2,4-DCAA

R.T.: 11.420 min
Delta R.T.: 0.000 min
Response: 240439120
Conc: 750.00 ng/ml

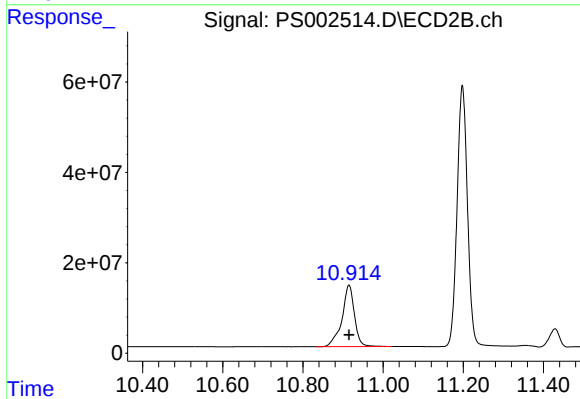

#4 2,4-DCAA


R.T.: 10.915 min
Delta R.T.: 0.000 min
Response: 295219158
Conc: 750.00 ng/ml

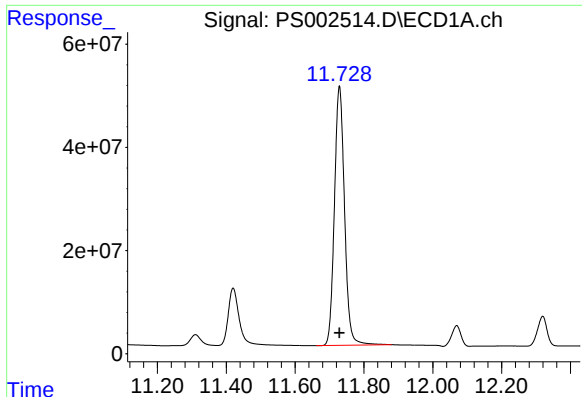

#5 DICAMBA


R.T.: 11.729 min
Delta R.T.: 0.000 min
Response: 1023213928
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

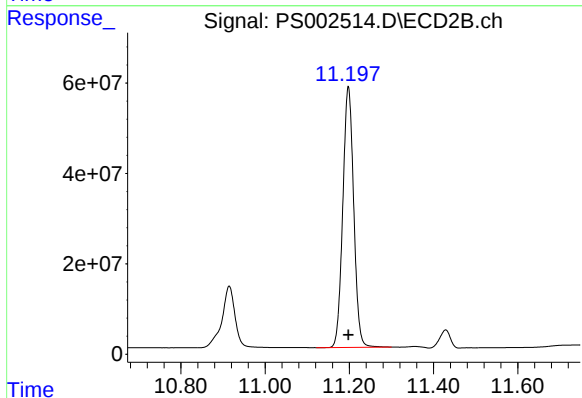


#5 DICAMBA

R.T.: 11.198 min
Delta R.T.: 0.000 min
Response: 1035933799
Conc: 705.00 ng/ml

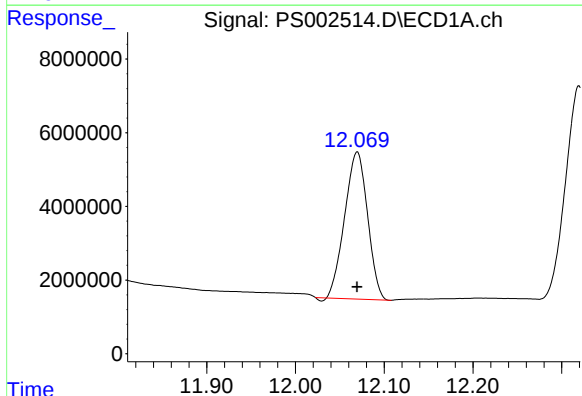


#6 MCP

R.T.: 12.069 min
Delta R.T.: 0.000 min
Response: 71543567
Conc: 70.50 ug/ml

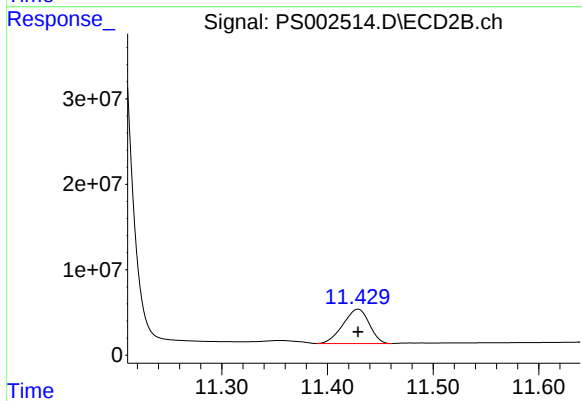

#6 MCP


R.T.: 11.429 min
Delta R.T.: 0.000 min
Response: 69063283
Conc: 70.50 ug/ml

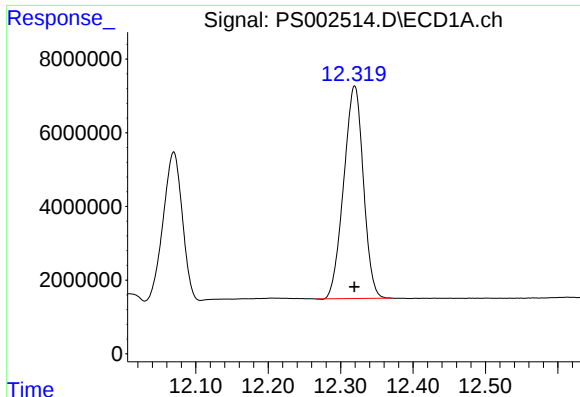

#7 MCPA


R.T.: 12.319 min
Delta R.T.: 0.000 min
Response: 108863224
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

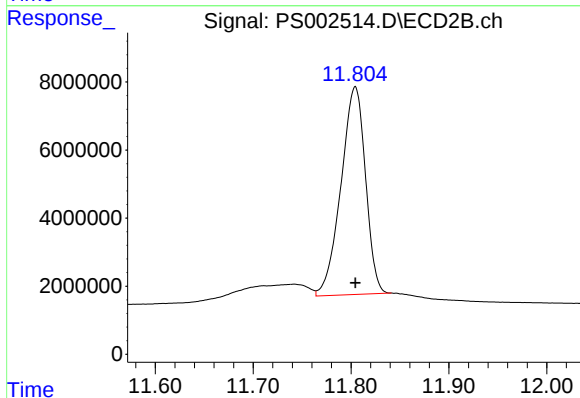


#7 MCPA

R.T.: 11.804 min
Delta R.T.: 0.000 min
Response: 106254225
Conc: 69.75 ug/ml

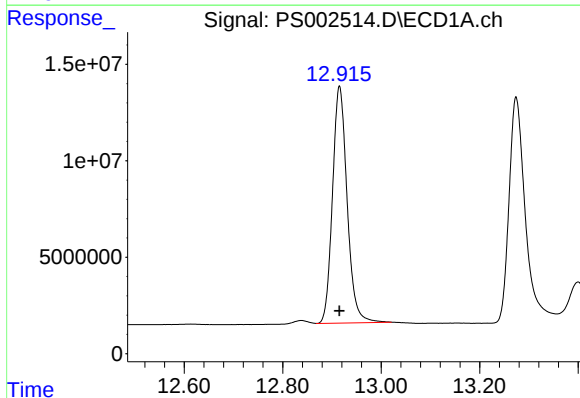


#8 DICHLORPROP

R.T.: 12.915 min
Delta R.T.: 0.000 min
Response: 253147346
Conc: 705.00 ng/ml

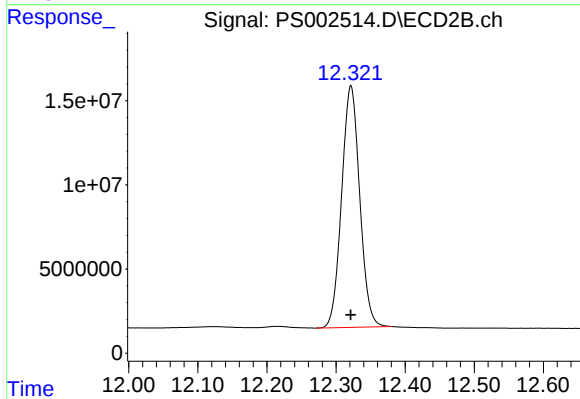

#8 DICHLORPROP


R.T.: 12.322 min
Delta R.T.: 0.000 min
Response: 261008048
Conc: 705.00 ng/ml

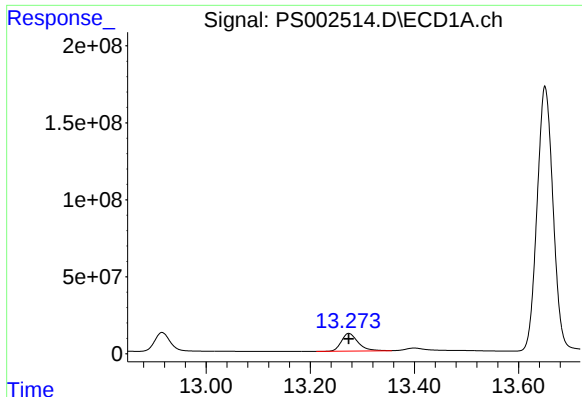

#9 2,4-D


R.T.: 13.274 min
Delta R.T.: 0.000 min
Response: 255850076
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

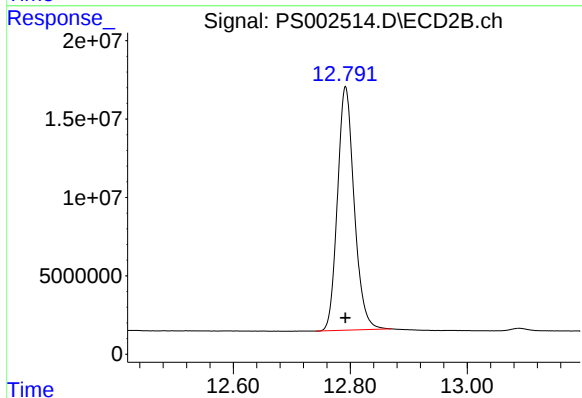


#9 2,4-D

R.T.: 12.792 min
Delta R.T.: 0.000 min
Response: 308381511
Conc: 705.00 ng/ml

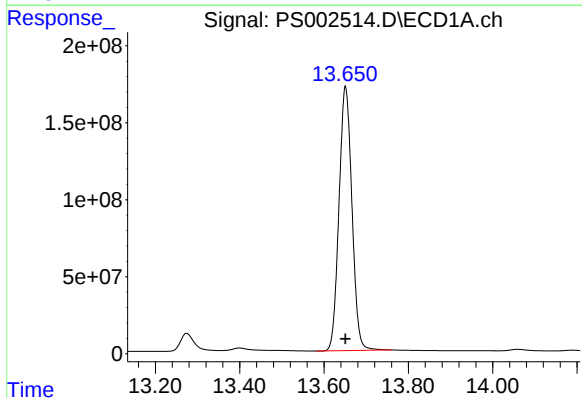


#10 Pentachlorophenol

R.T.: 13.651 min
Delta R.T.: 0.000 min
Response: 3650881238
Conc: 712.50 ng/ml

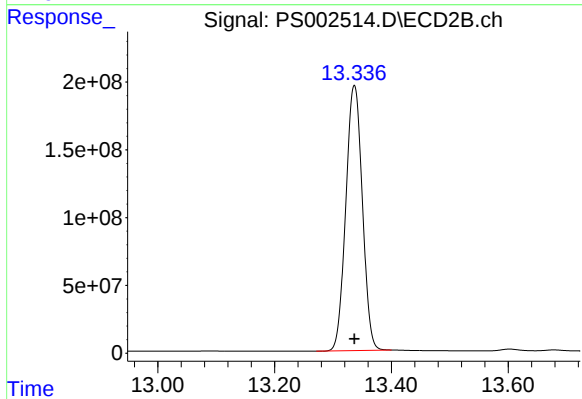

#10 Pentachlorophenol


R.T.: 13.337 min
Delta R.T.: 0.000 min
Response: 3844012139
Conc: 712.50 ng/ml

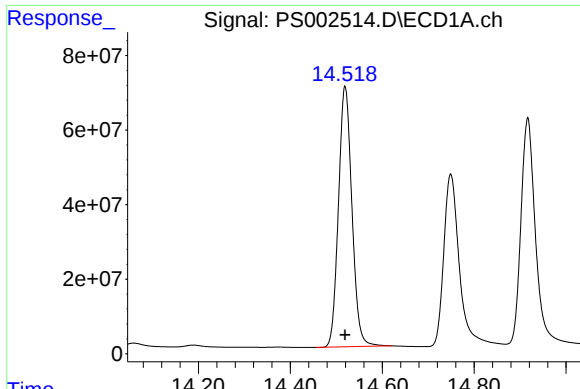

#11 2,4,5-TP (SILVEX)


R.T.: 14.519 min
Delta R.T.: 0.000 min
Response: 1422449337
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

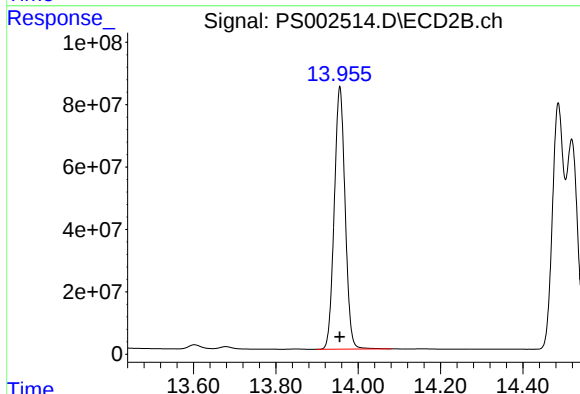


#11 2,4,5-TP (SILVEX)

R.T.: 13.956 min
Delta R.T.: 0.000 min
Response: 1540297174
Conc: 712.50 ng/ml

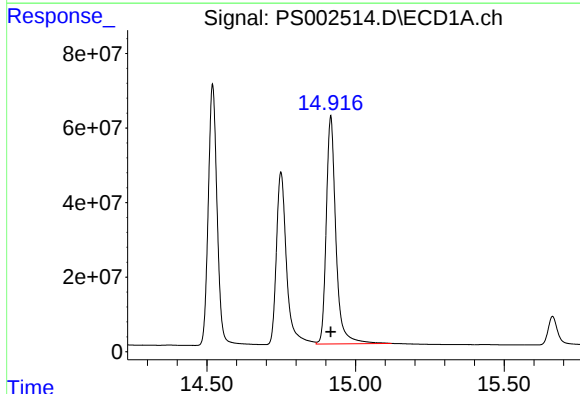


#12 2,4,5-T

R.T.: 14.917 min
Delta R.T.: 0.000 min
Response: 1378477008
Conc: 712.50 ng/ml

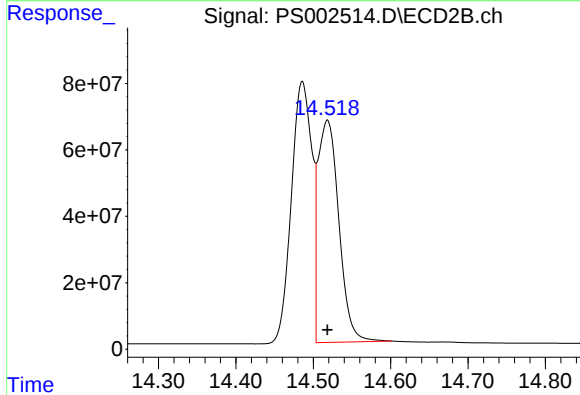

#12 2,4,5-T


R.T.: 14.518 min
Delta R.T.: 0.000 min
Response: 1248151017
Conc: 712.50 ng/ml

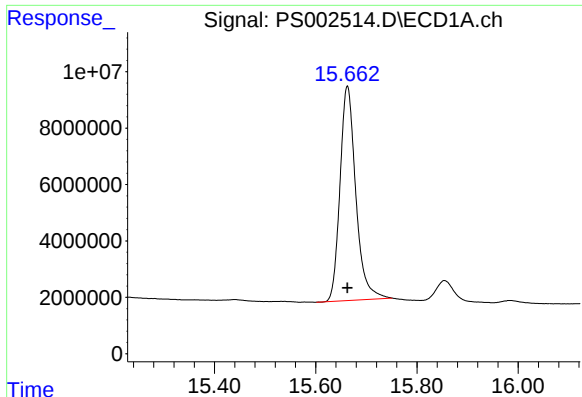

#13 2,4-DB


R.T.: 15.663 min
Delta R.T.: 0.000 min
Response: 164587189
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

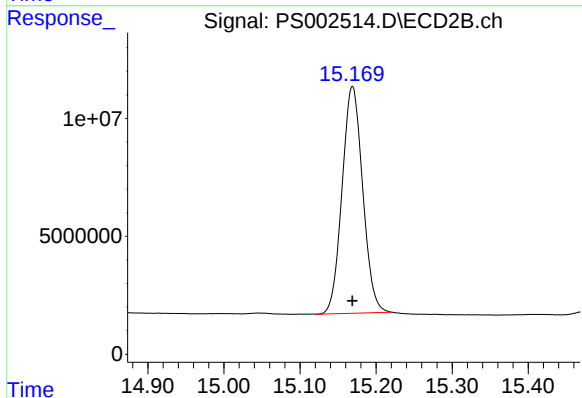


#13 2,4-DB

R.T.: 15.169 min
Delta R.T.: 0.000 min
Response: 181356641
Conc: 712.50 ng/ml

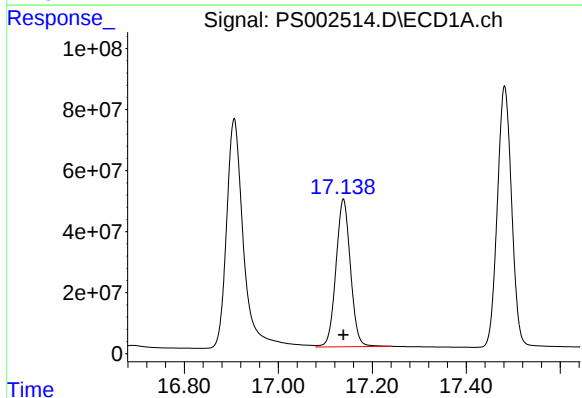


#14 DINOSEB

R.T.: 17.138 min
Delta R.T.: 0.000 min
Response: 1037556117
Conc: 705.00 ng/ml

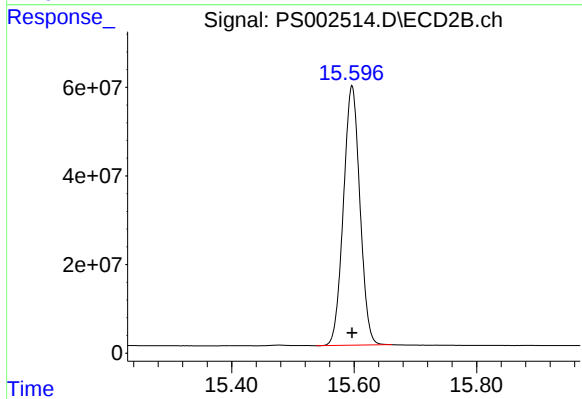

#14 DINOSEB


R.T.: 15.596 min
Delta R.T.: 0.000 min
Response: 1094673508
Conc: 705.00 ng/ml

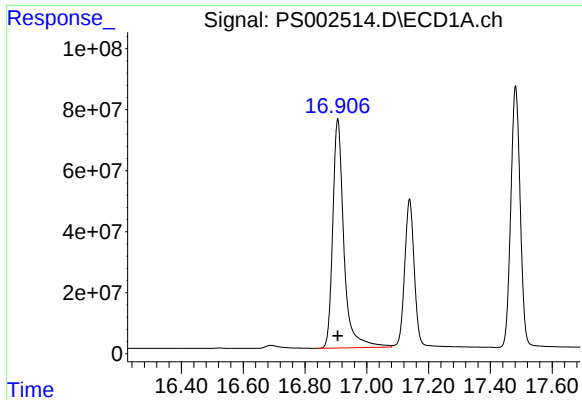

#15 Picloram


R.T.: 16.906 min
Delta R.T.: 0.000 min
Response: 1883718218
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

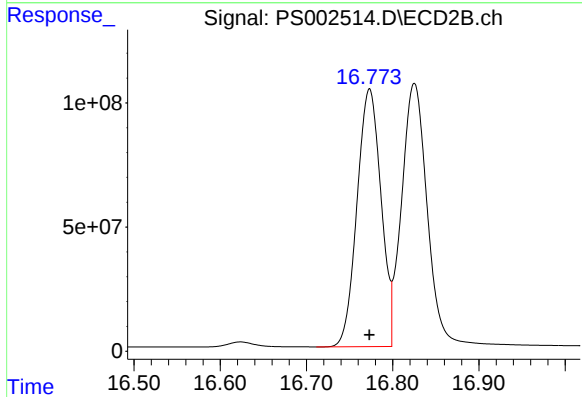


#15 Picloram

R.T.: 16.773 min
Delta R.T.: 0.000 min
Response: 2005918301
Conc: 712.50 ng/ml

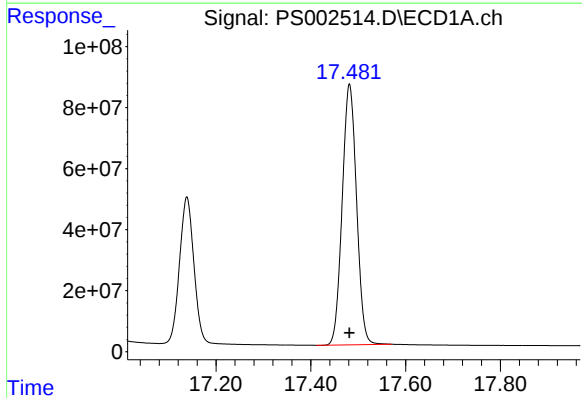

#16 DCPA

R.T.: 17.481 min
Delta R.T.: 0.000 min
Response: 1794110676
Conc: 720.00 ng/ml

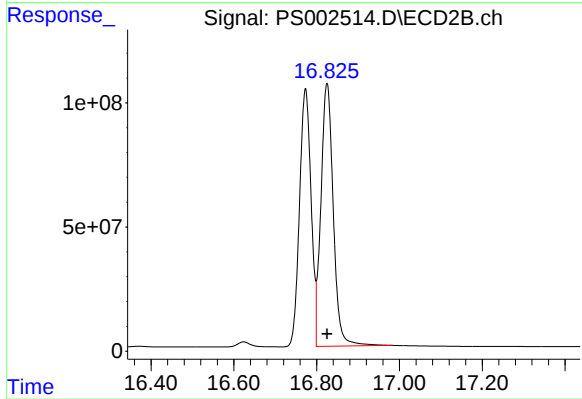

#16 DCPA

R.T.: 16.825 min
Delta R.T.: 0.000 min
Response: 2191169440
Conc: 720.00 ng/ml