

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007911.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 10:58
 Operator : SM\AJ
 Sample : PB125239BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB125239BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 11:15:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.430	5.154	469.7E6	276.4E6	300.228	356.163
Target Compounds							
1) T	Dalapon	1.992	1.711	114.0E6	218.1E6	55.909	183.581 #
2) T	3,5-DICHL...	0.000	4.488	0	38729819	N.D.	37.425
5) T	DICAMBA	5.516	0.000	77365681	0	13.598	N.D. #
7) T	MCPA	5.893	5.521	25545774	23970786	4.283	7.522 #
9) T	2,4-D	0.000	6.056	0	13361826	N.D.	15.122
10) T	Pentachlo...	0.000	6.445	0	7527623	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.757	0	23246422	N.D.	5.420
15) T	Picloram	0.000	8.925	0	42439724	N.D.	6.871



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007911.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 10:58
Operator : SM\AJ
Sample : PB125239BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB125239BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 11:15:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

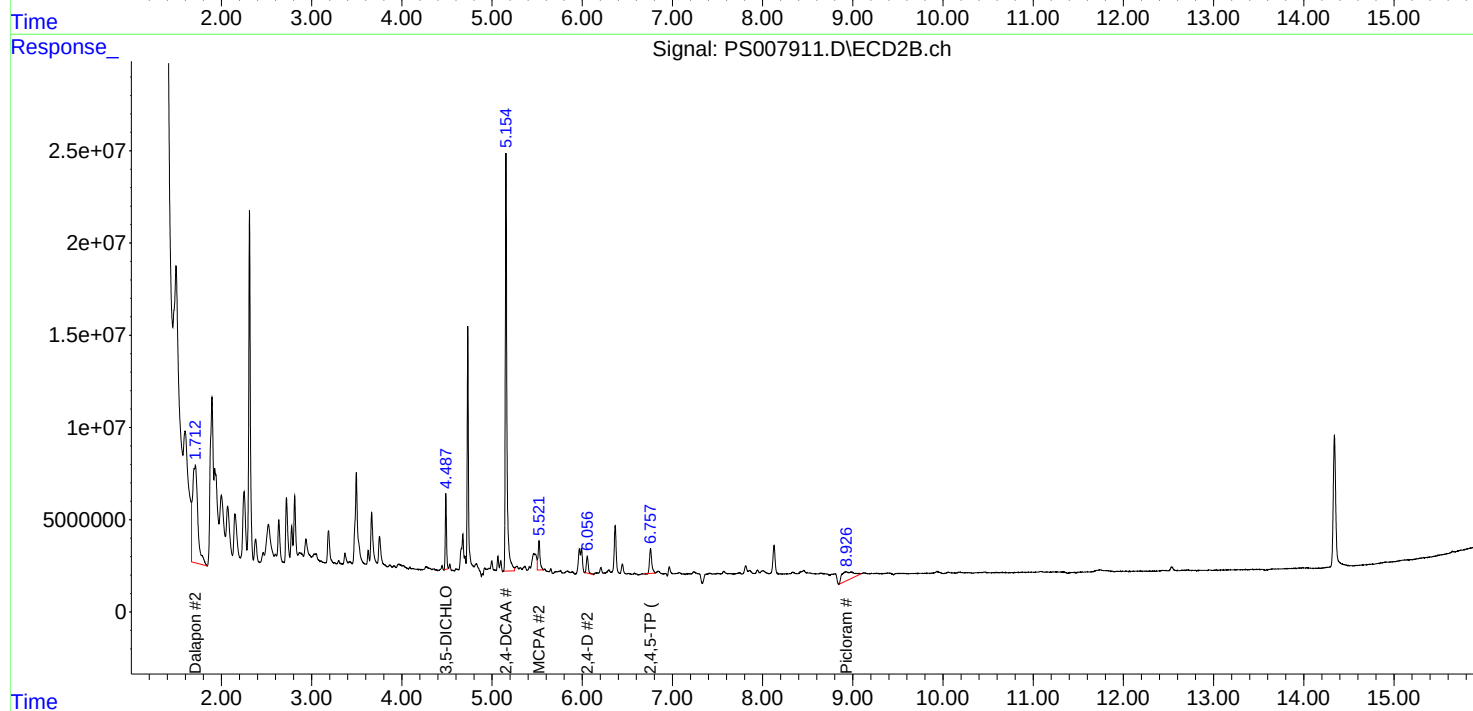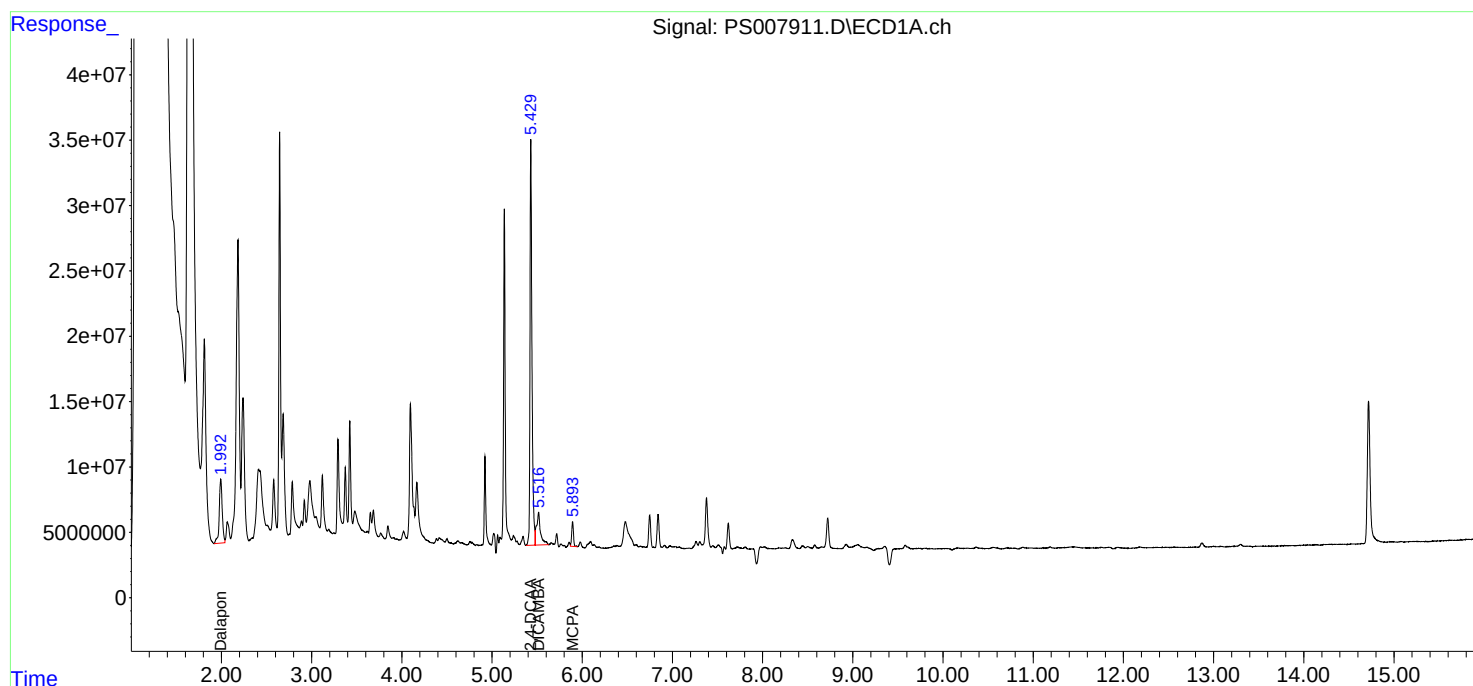


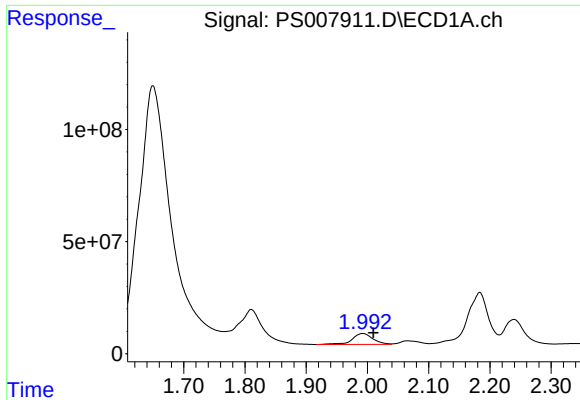

#1 Dalapon


R.T.: 1.992 min
Delta R.T.: -0.018 min
Response: 114017312
Conc: 55.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125239BL

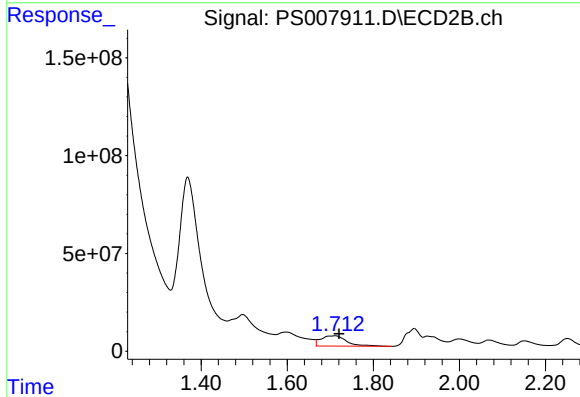


#1 Dalapon

R.T.: 1.711 min
Delta R.T.: -0.010 min
Response: 218056093
Conc: 183.58 ng/ml

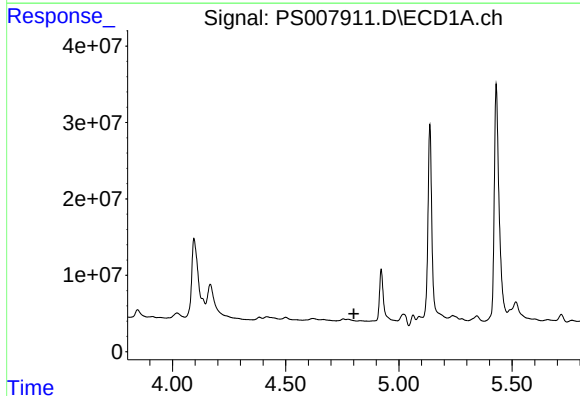


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

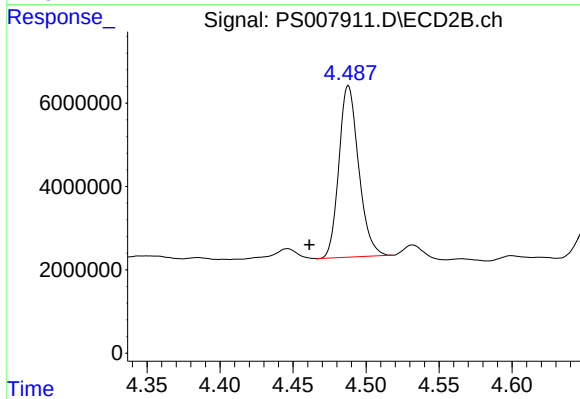

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.488 min
Delta R.T.: 0.027 min
Response: 38729819
Conc: 37.42 ng/ml

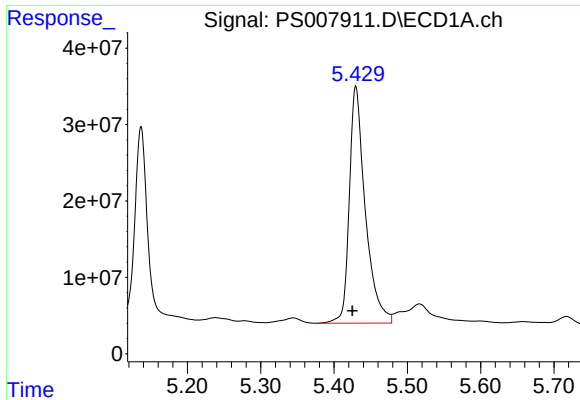

#4 2,4-DCAA


R.T.: 5.430 min
Delta R.T.: 0.005 min
Response: 469656280
Conc: 300.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125239BL

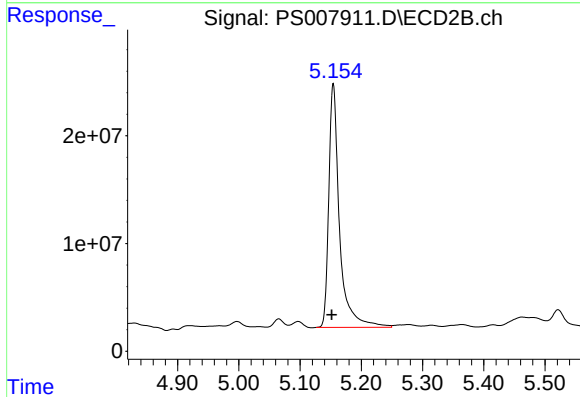


#4 2,4-DCAA

R.T.: 5.154 min
Delta R.T.: 0.003 min
Response: 276353539
Conc: 356.16 ng/ml

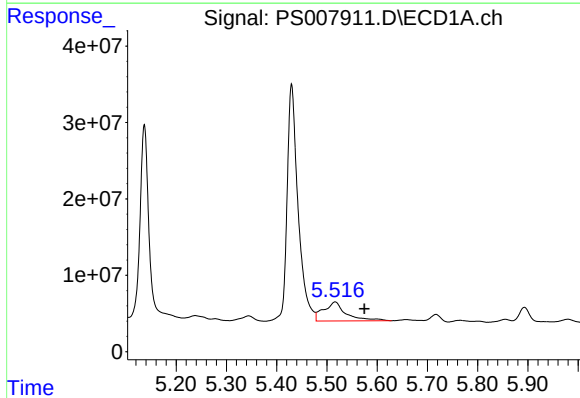


#5 DICAMBA

R.T.: 5.516 min
Delta R.T.: -0.058 min
Response: 77365681
Conc: 13.60 ng/ml

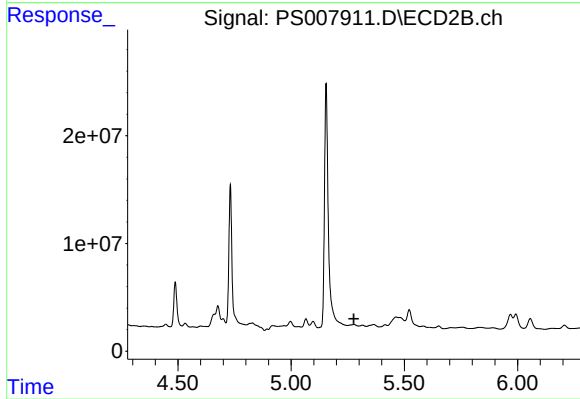

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

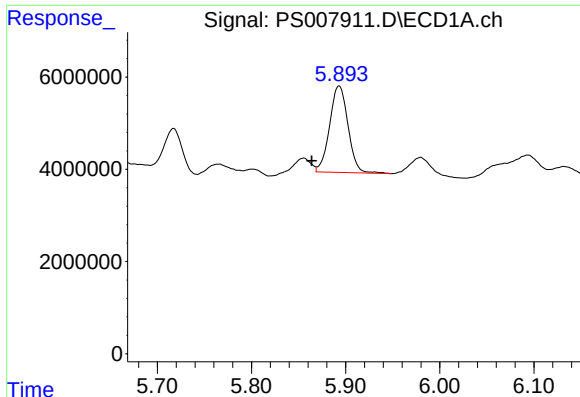

#7 MCPA


R.T.: 5.893 min
Delta R.T.: 0.029 min
Response: 25545774
Conc: 4.28 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB125239BL

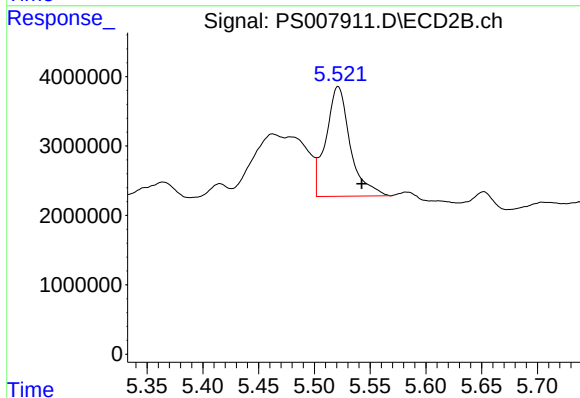


#7 MCPA

R.T.: 5.521 min
Delta R.T.: -0.021 min
Response: 23970786
Conc: 7.52 ug/ml

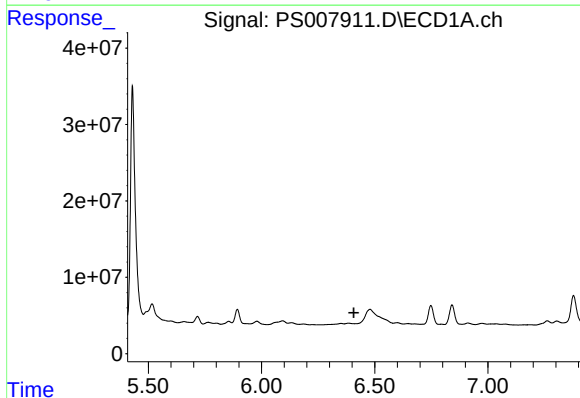


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.408 min
Response: 0
Conc: N.D.

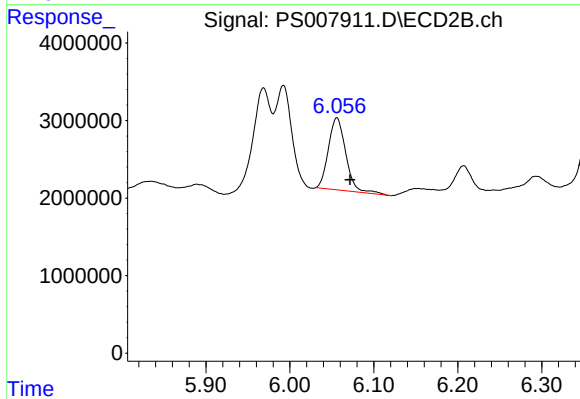

#9 2,4-D


R.T.: 6.056 min
Delta R.T.: -0.016 min
Response: 13361826
Conc: 15.12 ng/ml

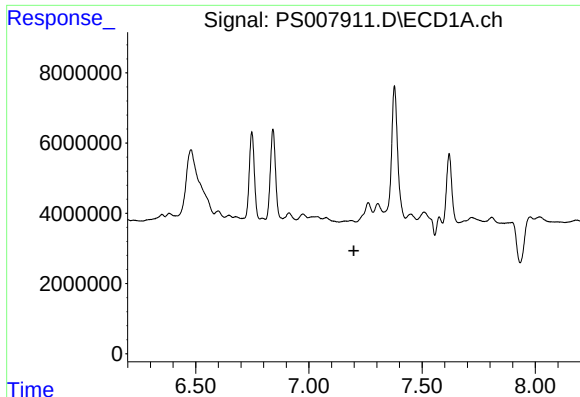

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB125239BL

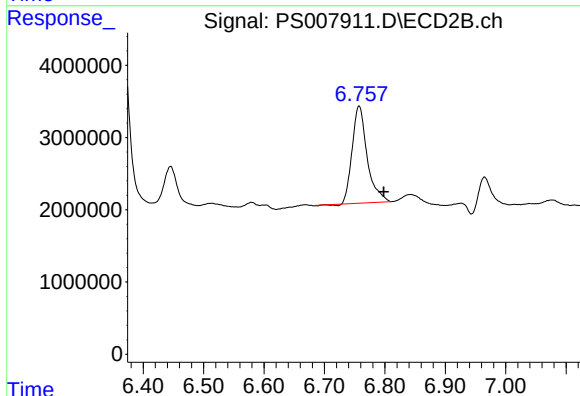


#11 2,4,5-TP (SILVEX)

R.T.: 6.757 min
Delta R.T.: -0.040 min
Response: 23246422
Conc: 5.42 ng/ml

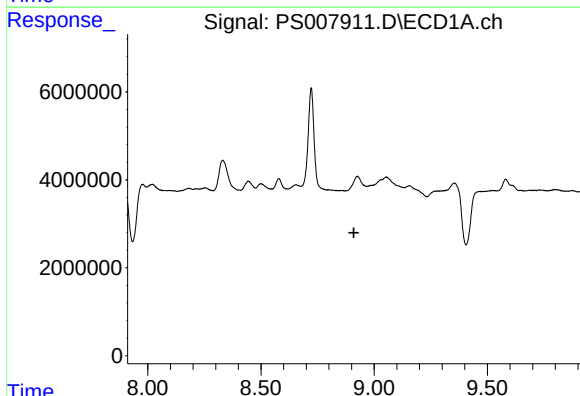

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.911 min
Response: 0
Conc: N.D.

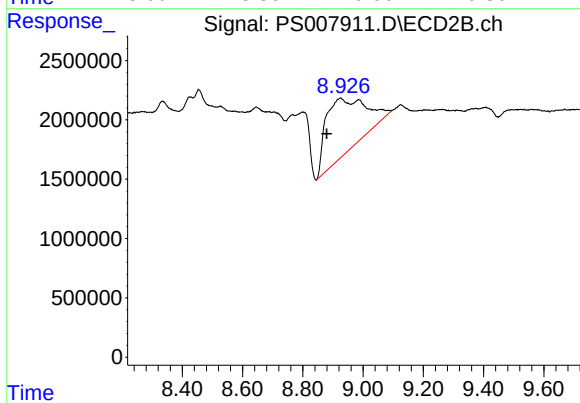

#15 Picloram

R.T.: 8.925 min
Delta R.T.: 0.046 min
Response: 42439724
Conc: 6.87 ng/ml