

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007913.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 12:47
 Operator : SM\AJ
 Sample : K6141-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CMJ-01-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 15:45:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.426	5.153	329.7E6	167.8E6	210.757	216.298
Target Compounds							
1) T	Dalapon	1.992	1.695	92594279	332.0E6	45.404	279.538 #
2) T	3,5-DICHL...	0.000	4.488	0	37821841	N.D.	36.547
5) T	DICAMBA	5.517	0.000	28893731	0	5.078	N.D. #
7) T	MCPA	5.893	5.521	32851559	30912133	5.508	9.701 #
9) T	2,4-D	0.000	6.056	0	7498133	N.D.	8.486
10) T	Pentachlo...	0.000	6.444	0	7723290	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.750	0	29173685	N.D.	6.802
13) T	2,4-DB	8.012	0.000	79983192	0	65.148	N.D. #
16) T	DCPA	0.000	8.798	0	26722962	N.D.	4.657



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007913.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 12:47
Operator : SM\AJ
Sample : K6141-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CMJ-01-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 15:45:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

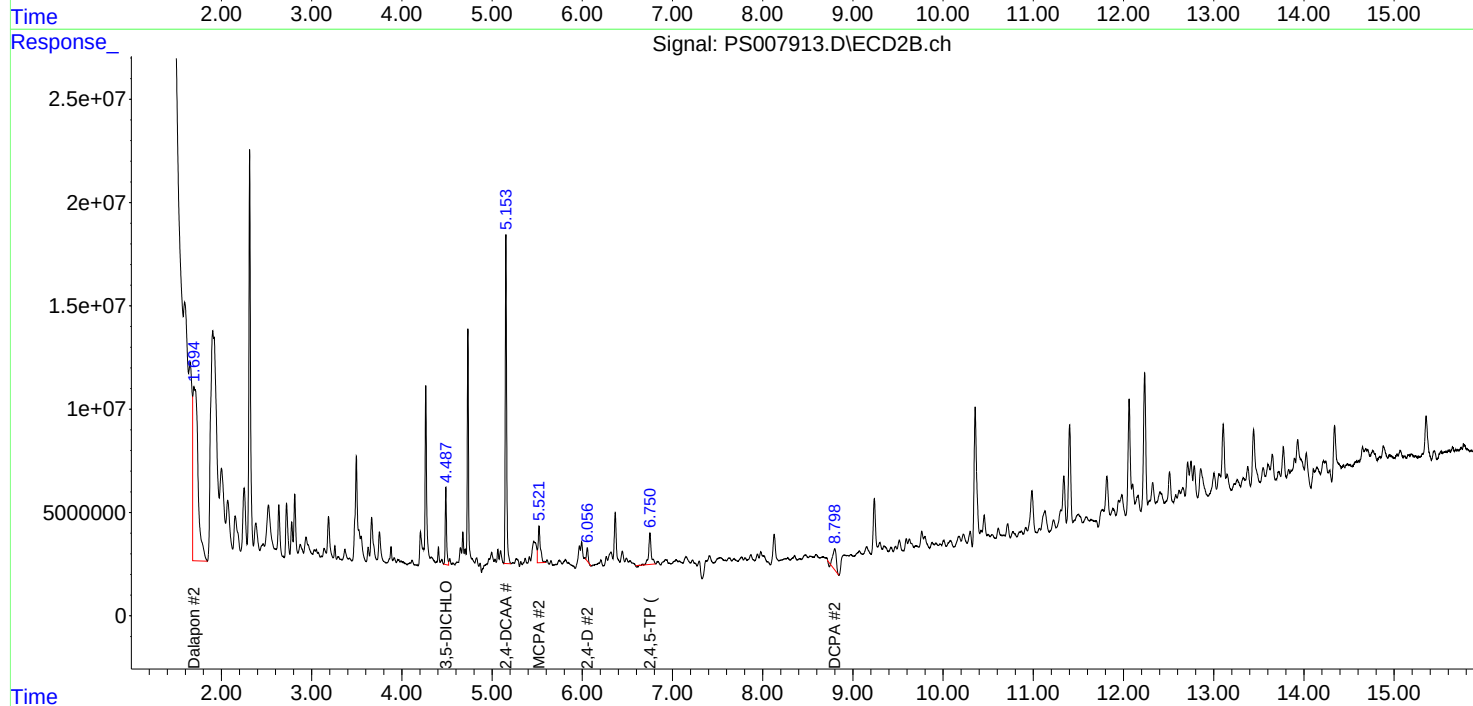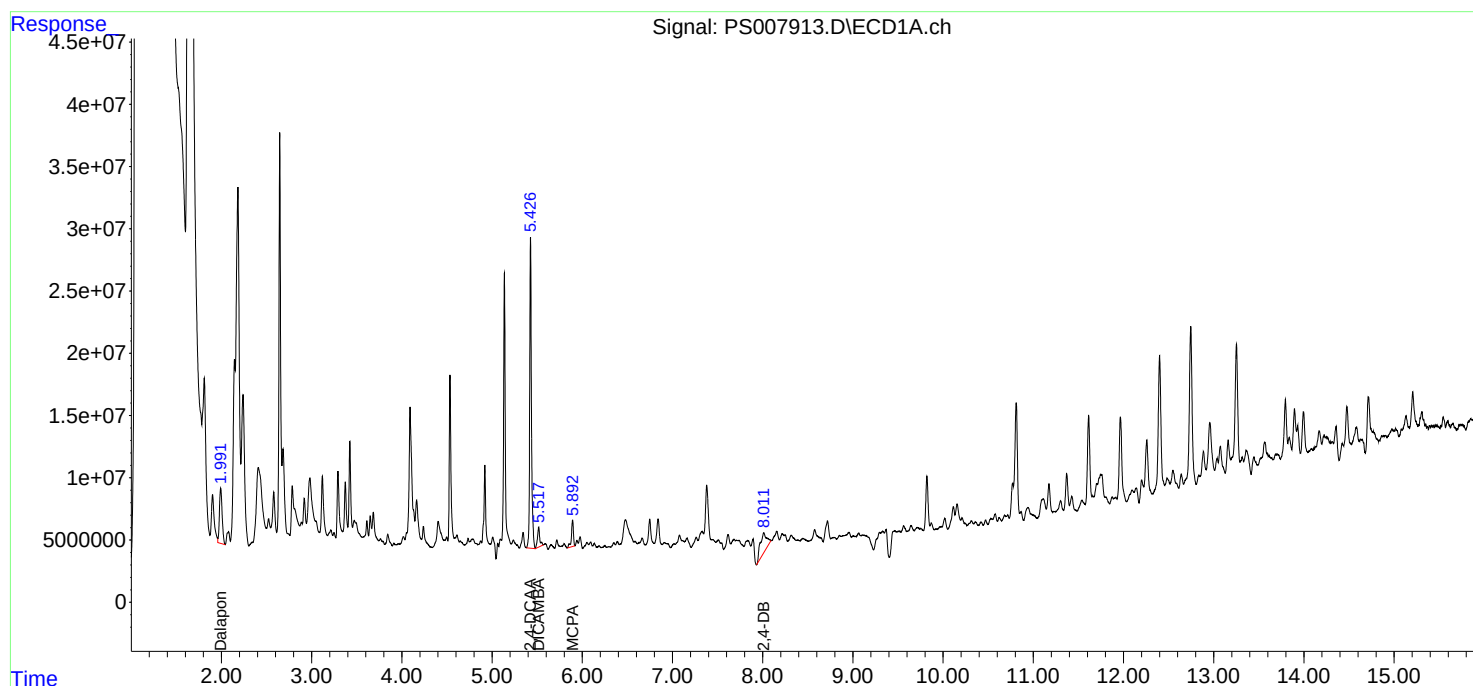


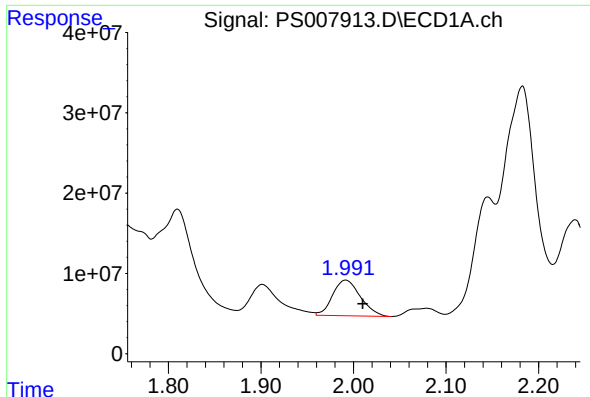

#1 Dalapon


R.T.: 1.992 min
Delta R.T.: -0.018 min
Response: 92594279
Conc: 45.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
CMJ-01-COMP

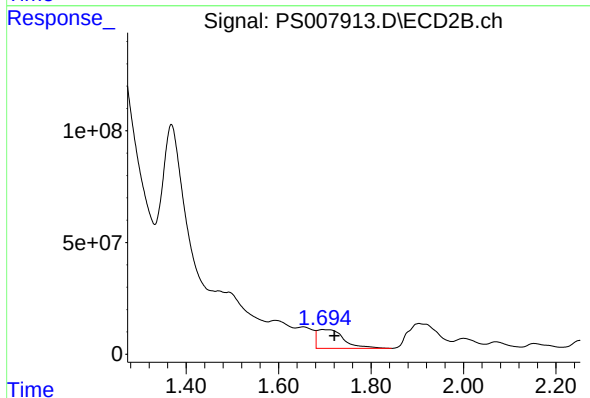


#1 Dalapon

R.T.: 1.695 min
Delta R.T.: -0.025 min
Response: 332032608
Conc: 279.54 ng/ml

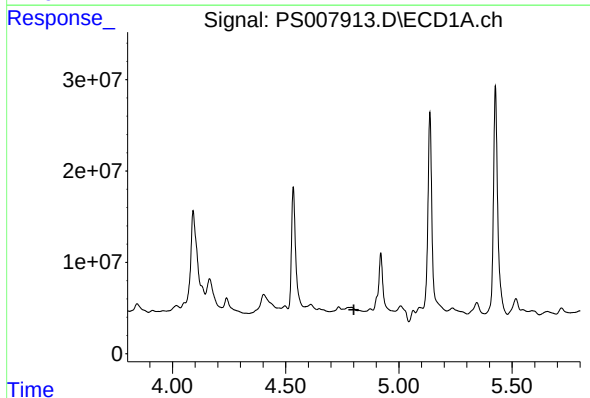


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

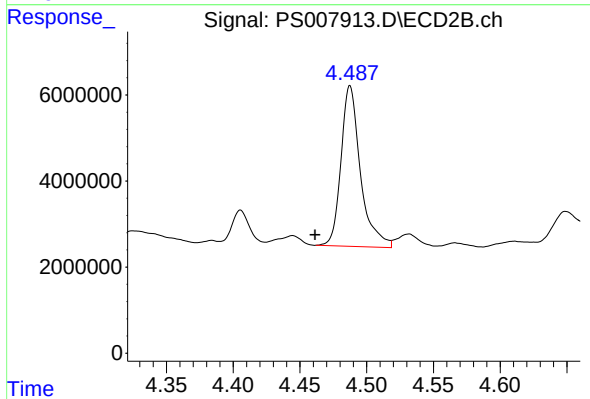

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.488 min
Delta R.T.: 0.026 min
Response: 37821841
Conc: 36.55 ng/ml

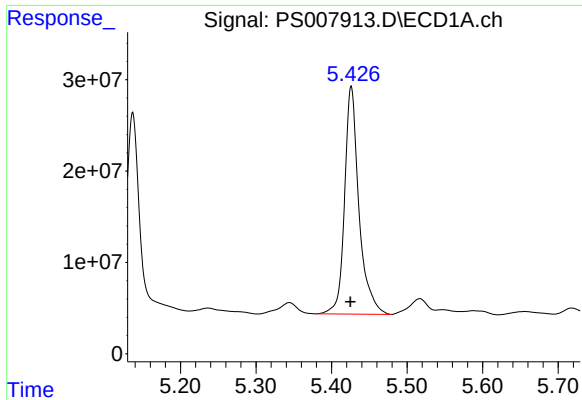

#4 2,4-DCAA


R.T.: 5.426 min
Delta R.T.: 0.001 min
Response: 329694922
Conc: 210.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
CMJ-01-COMP

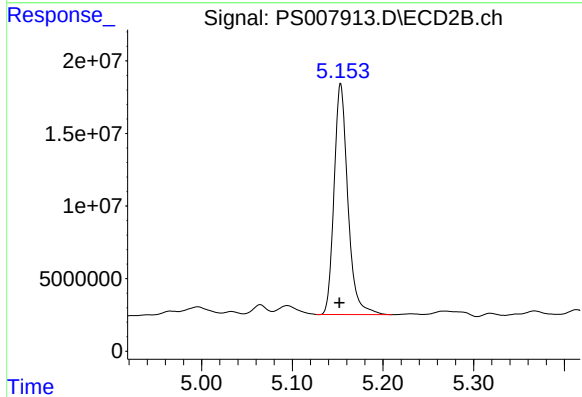


#4 2,4-DCAA

R.T.: 5.153 min
Delta R.T.: 0.002 min
Response: 167829491
Conc: 216.30 ng/ml

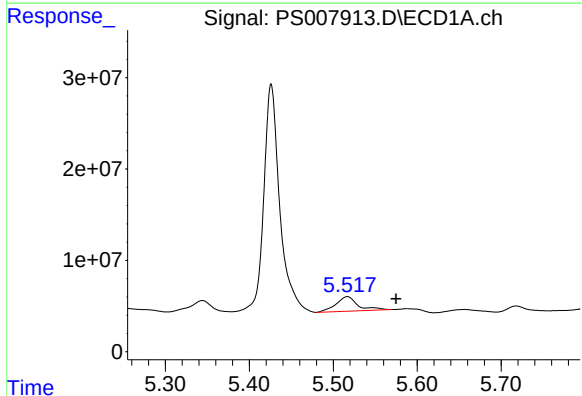


#5 DICAMBA

R.T.: 5.517 min
Delta R.T.: -0.058 min
Response: 28893731
Conc: 5.08 ng/ml

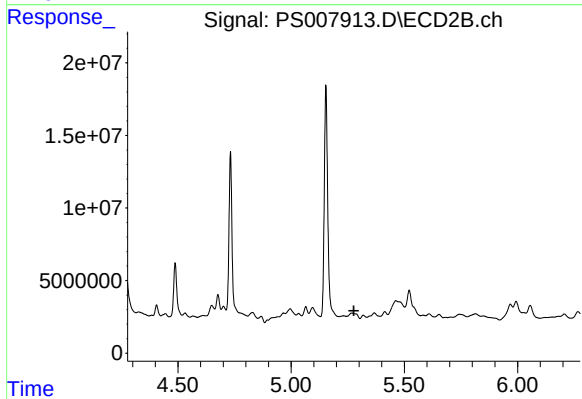

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

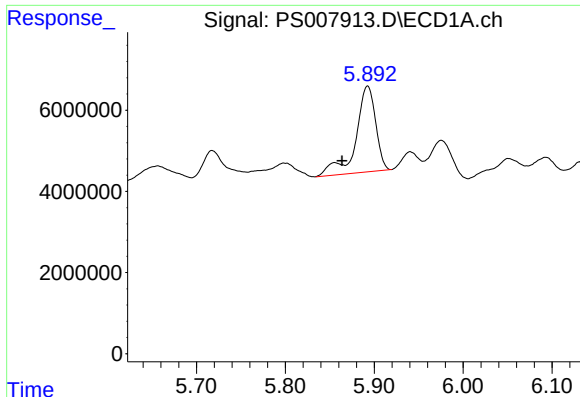

#7 MCPA


R.T.: 5.893 min
Delta R.T.: 0.029 min
Response: 32851559
Conc: 5.51 ug/ml

Instrument :
ECD_S
ClientSampleId :
CMJ-01-COMP

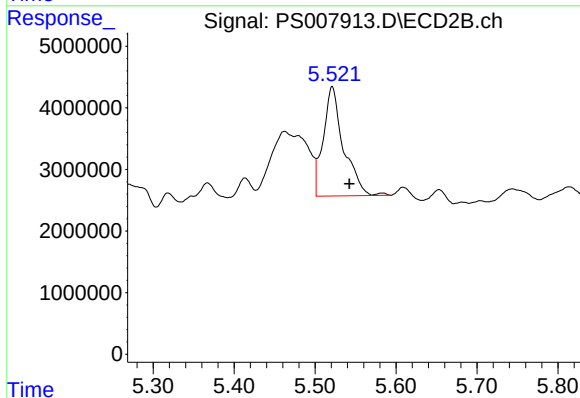


#7 MCPA

R.T.: 5.521 min
Delta R.T.: -0.021 min
Response: 30912133
Conc: 9.70 ug/ml

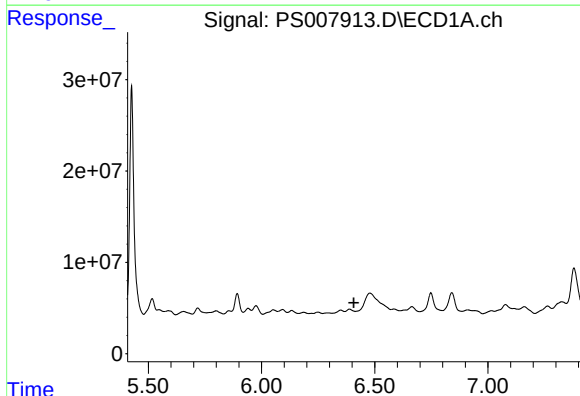


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.408 min
Response: 0
Conc: N.D.

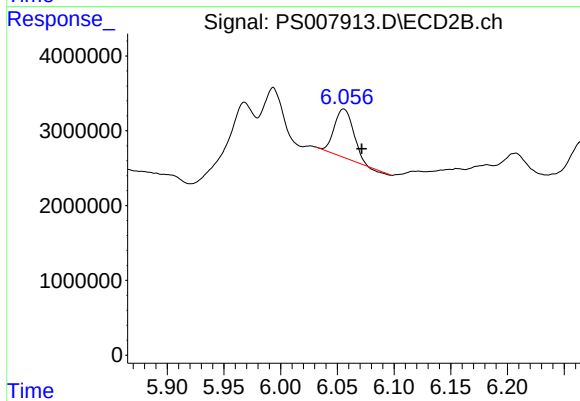

#9 2,4-D


R.T.: 6.056 min
Delta R.T.: -0.016 min
Response: 7498133
Conc: 8.49 ng/ml

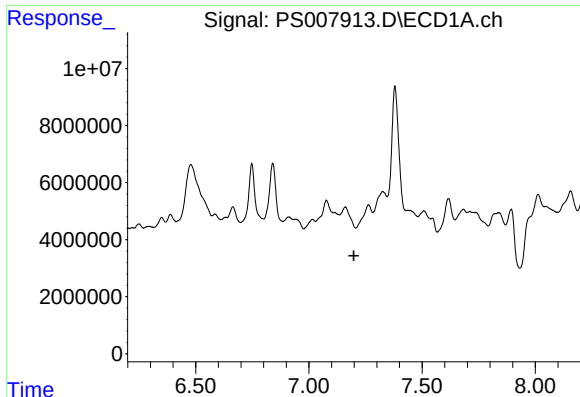

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CMJ-01-COMP

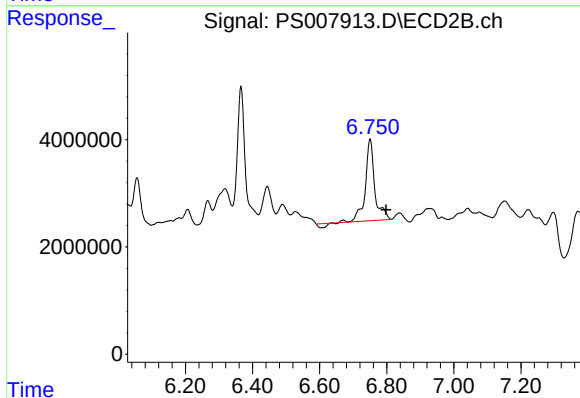


#11 2,4,5-TP (SILVEX)

R.T.: 6.750 min
Delta R.T.: -0.048 min
Response: 29173685
Conc: 6.80 ng/ml

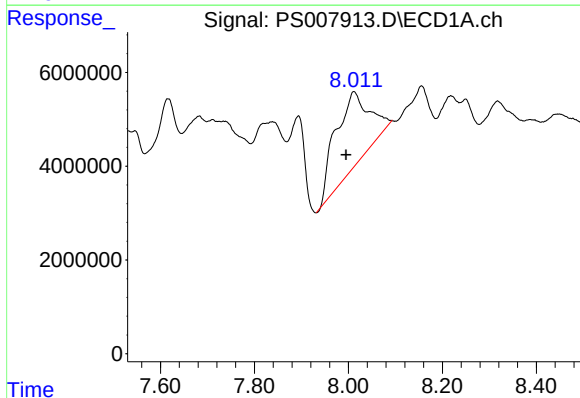


#13 2,4-DB

R.T.: 8.012 min
Delta R.T.: 0.017 min
Response: 79983192
Conc: 65.15 ng/ml

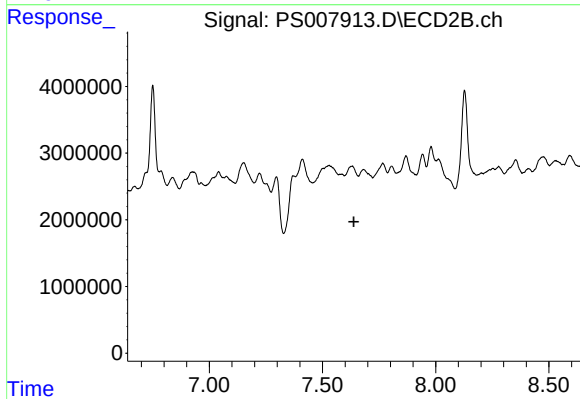

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 7.638 min
Response: 0
Conc: N.D.

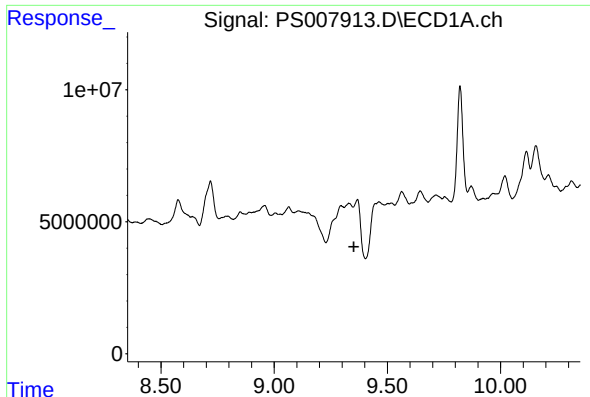

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CMJ-01-COMP

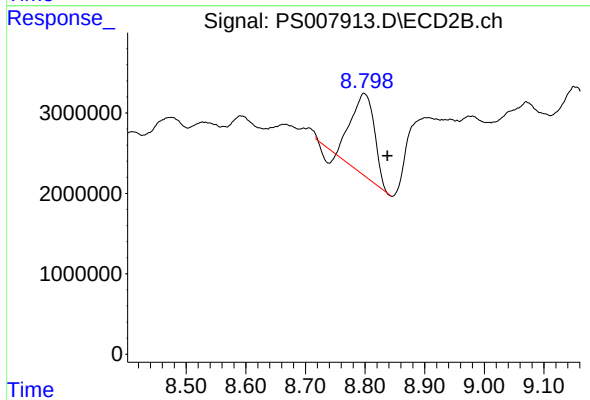

#16 DCPA

R.T.: 8.798 min
Delta R.T.: -0.039 min
Response: 26722962
Conc: 4.66 ng/ml