

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007916.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 13:53
 Operator : SM\AJ
 Sample : K6135-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-34

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 15:46:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.429	5.156	59256768	16386827	37.880	21.119 #
Target Compounds							
1) T	Dalapon	1.991	1.696	105.2E6	418.9E6	51.570	352.647 #
2) T	3,5-DICHL...	0.000	4.487	0	79691506	N.D.	77.006
3) T	4-Nitroph...	0.000	4.830	0	17497919	N.D.	38.639
5) T	DICAMBA	5.516	0.000	43483153	0	7.643	N.D. #
7) T	MCPA	5.892	5.521	33176837	31892493	5.563	10.008 #
9) T	2,4-D	6.475	6.056	83966576	7104651	52.192	8.040 #
10) T	Pentachlo...	0.000	6.439	0	16972155	N.D.	1.555
11) T	2,4,5-TP ...	0.000	6.749	0	36508624	N.D.	8.513
14) T	DINOSEB	0.000	7.942	0	5171180	N.D.	1.581
15) T	Picloram	0.000	8.928	0	28114976	N.D.	4.552
16) T	DCPA	0.000	8.799	0	15964939	N.D.	2.782



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007916.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 13:53
Operator : SM\AJ
Sample : K6135-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-34

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 15:46:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

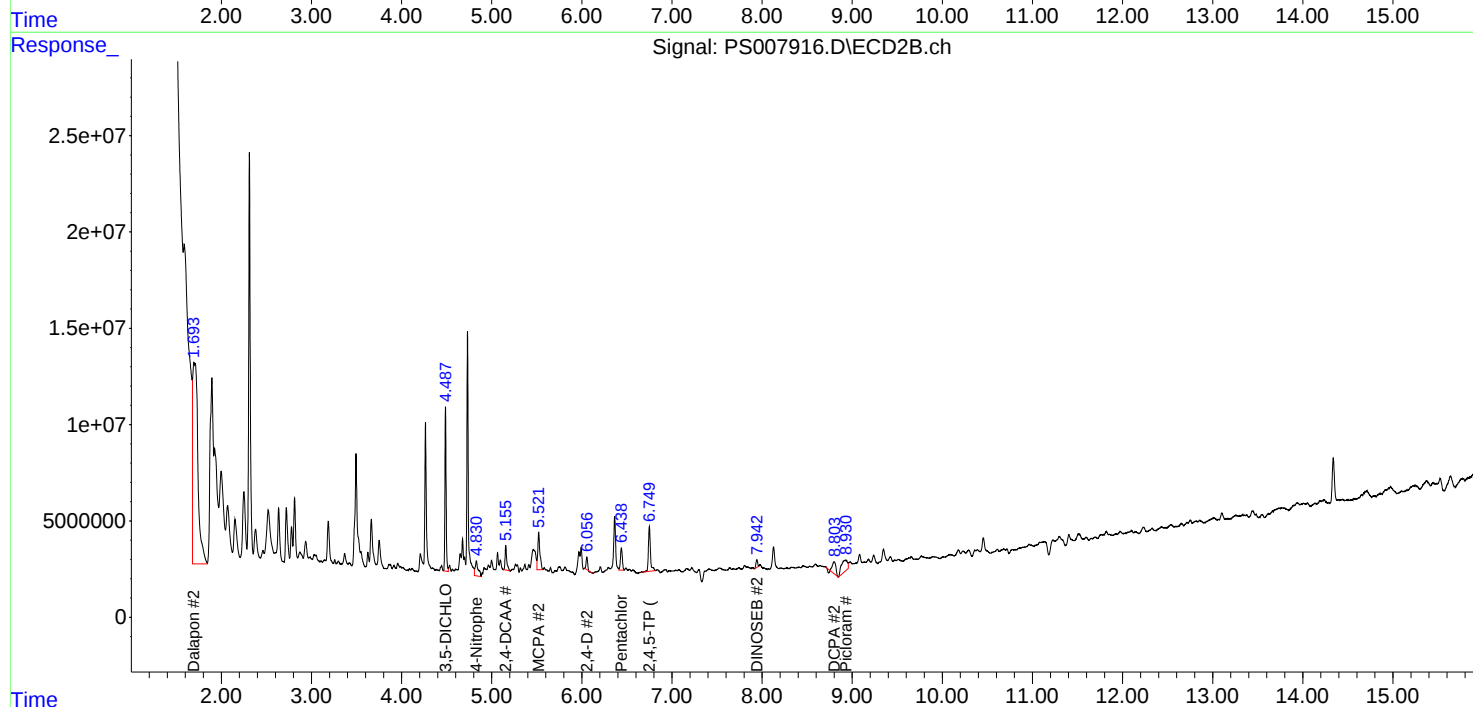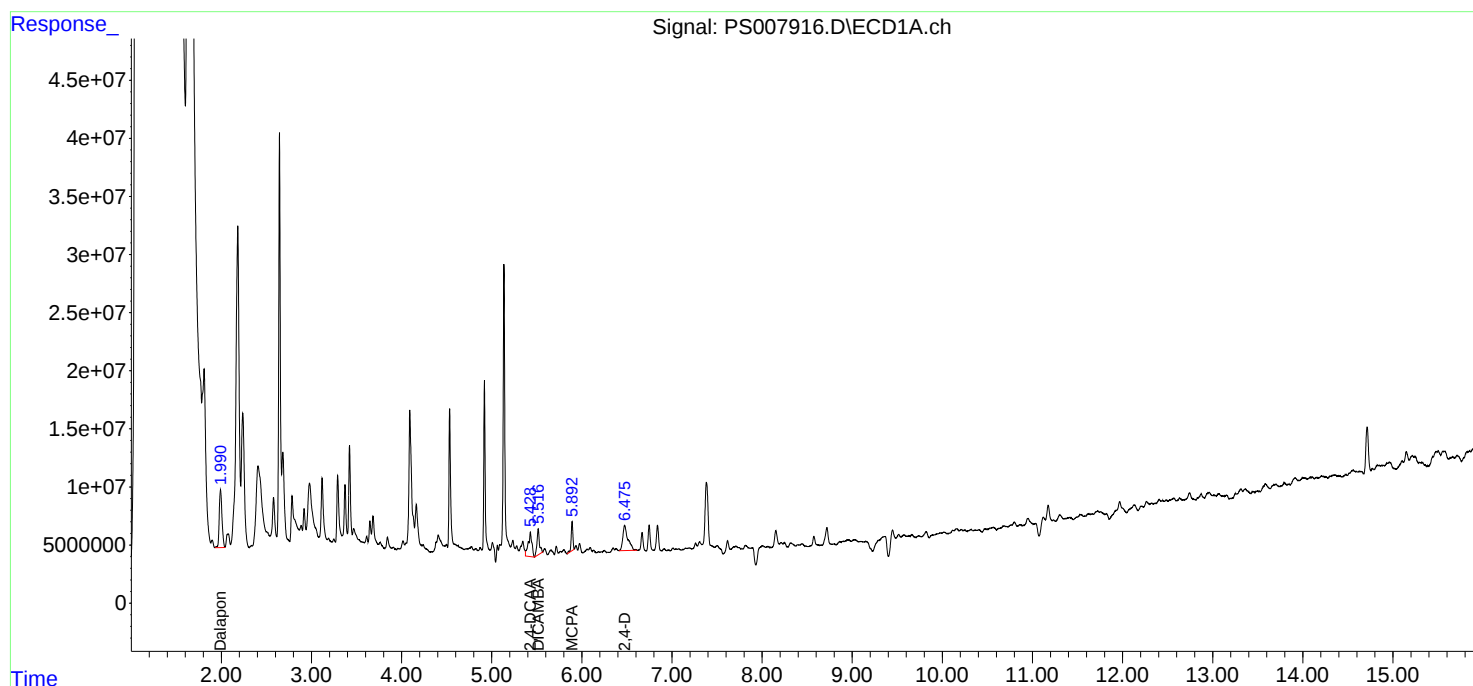


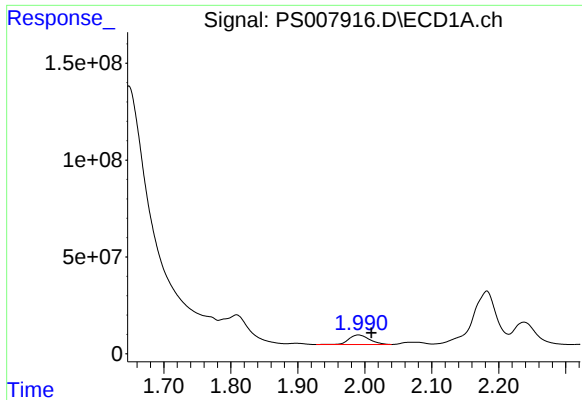

#1 Dalapon


R.T.: 1.991 min
Delta R.T.: -0.019 min
Response: 105168260
Conc: 51.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-34

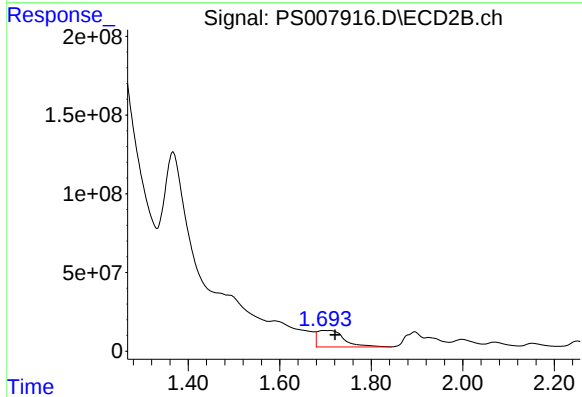


#1 Dalapon

R.T.: 1.696 min
Delta R.T.: -0.025 min
Response: 418871705
Conc: 352.65 ng/ml

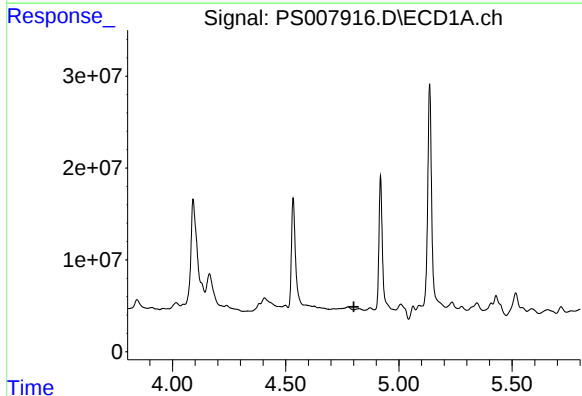


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

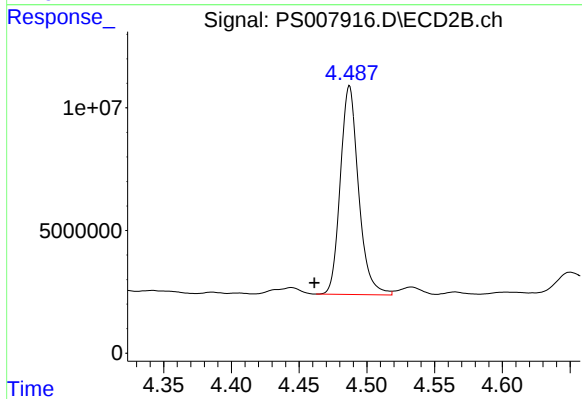

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.487 min
Delta R.T.: 0.026 min
Response: 79691506
Conc: 77.01 ng/ml

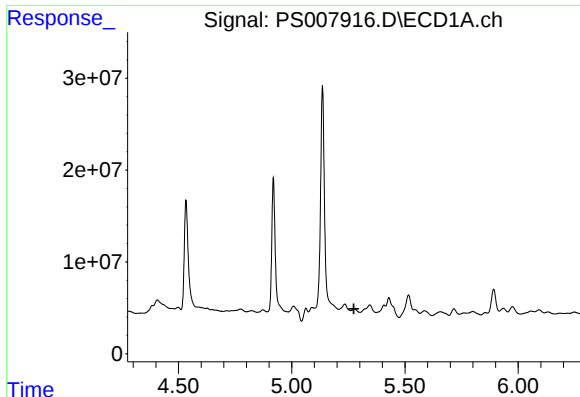

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-34

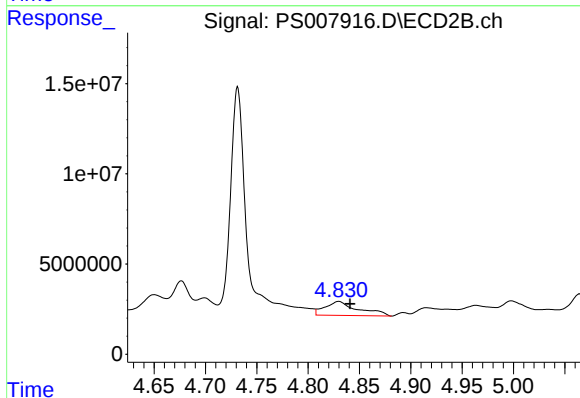


#3 4-Nitrophenol

R.T.: 4.830 min
Delta R.T.: -0.011 min
Response: 17497919
Conc: 38.64 ng/ml

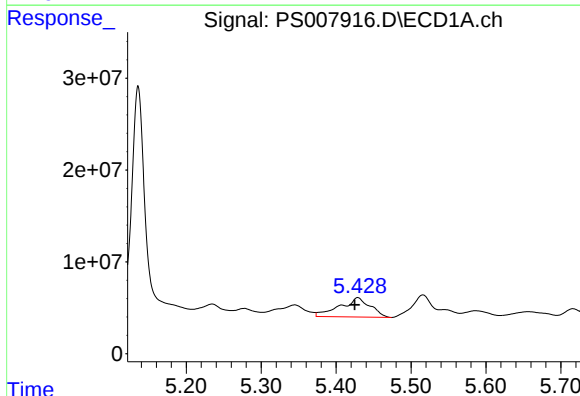


#4 2,4-DCAA

R.T.: 5.429 min
Delta R.T.: 0.004 min
Response: 59256768
Conc: 37.88 ng/ml

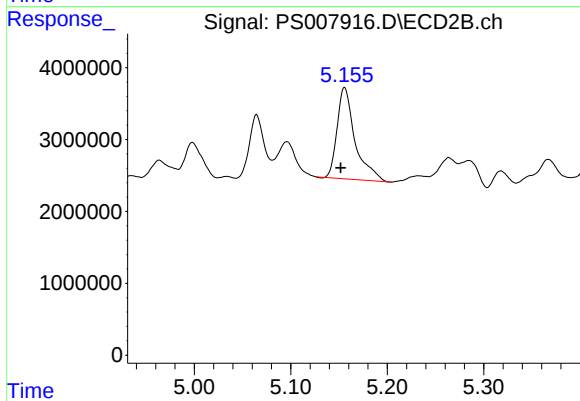

#4 2,4-DCAA


R.T.: 5.156 min
Delta R.T.: 0.004 min
Response: 16386827
Conc: 21.12 ng/ml

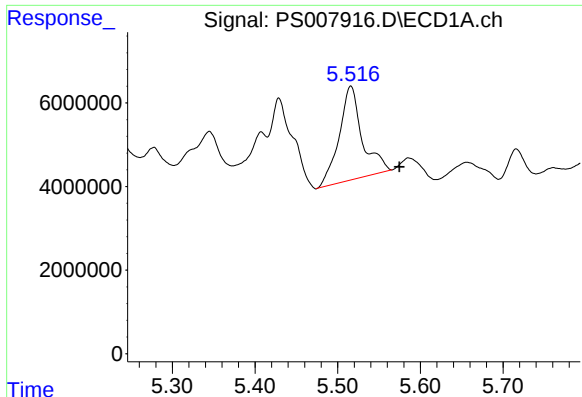

#5 DICAMBA


R.T.: 5.516 min
Delta R.T.: -0.059 min
Response: 43483153
Conc: 7.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-34

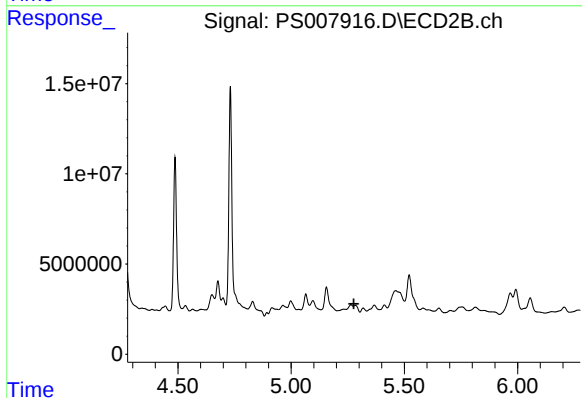


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

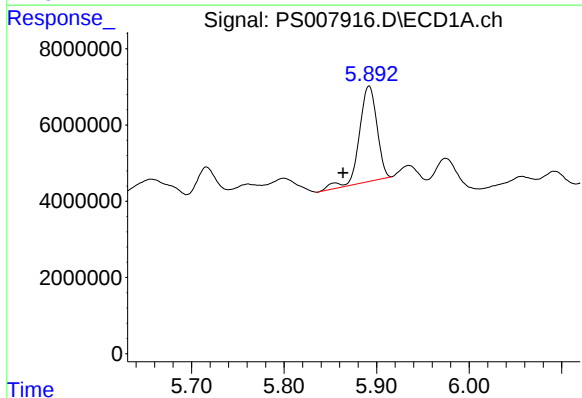


#7 MCPA

R.T.: 5.892 min
Delta R.T.: 0.028 min
Response: 33176837
Conc: 5.56 ug/ml

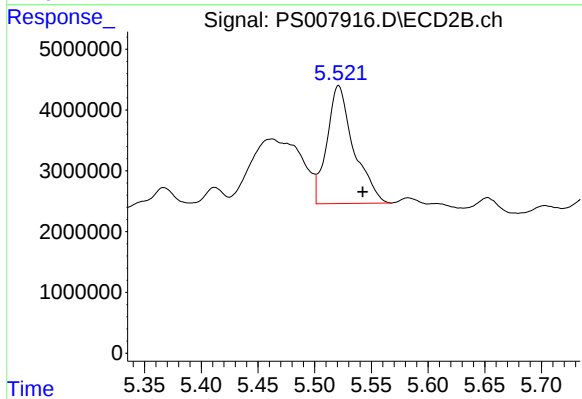

#7 MCPA


R.T.: 5.521 min
Delta R.T.: -0.021 min
Response: 31892493
Conc: 10.01 ug/ml

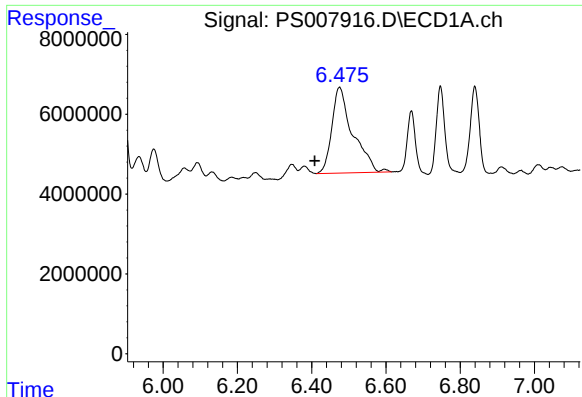

#9 2,4-D


R.T.: 6.475 min
Delta R.T.: 0.067 min
Response: 83966576
Conc: 52.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-34

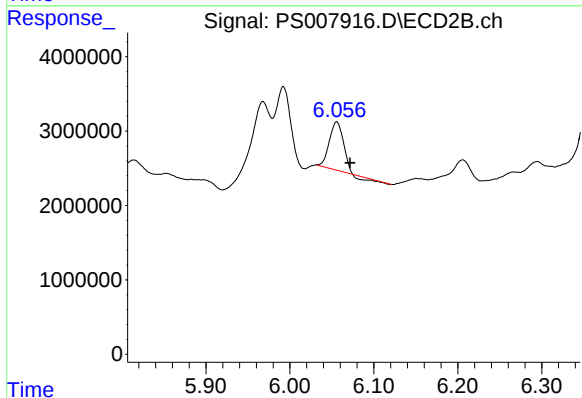


#9 2,4-D

R.T.: 6.056 min
Delta R.T.: -0.016 min
Response: 7104651
Conc: 8.04 ng/ml

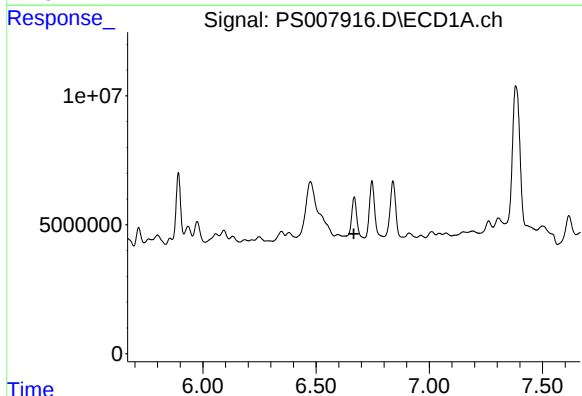


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.667 min
Response: 0
Conc: N.D.

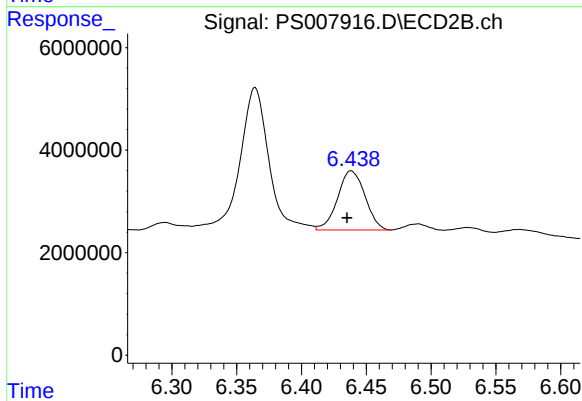

#10 Pentachlorophenol


R.T.: 6.439 min
Delta R.T.: 0.003 min
Response: 16972155
Conc: 1.55 ng/ml

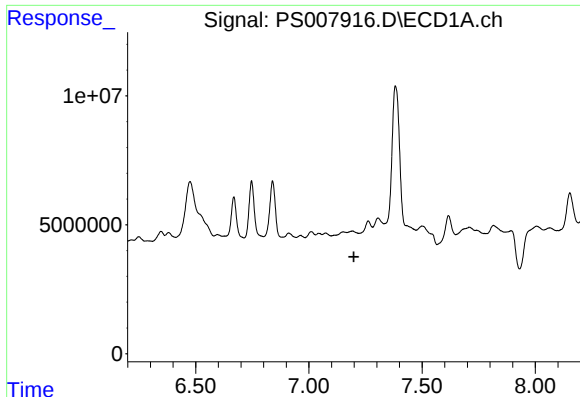

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-34

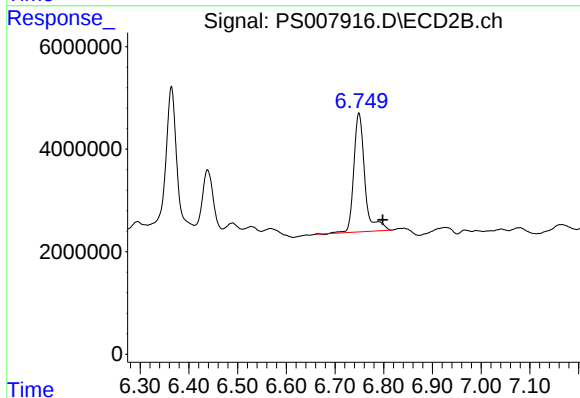


#11 2,4,5-TP (SILVEX)

R.T.: 6.749 min
Delta R.T.: -0.049 min
Response: 36508624
Conc: 8.51 ng/ml

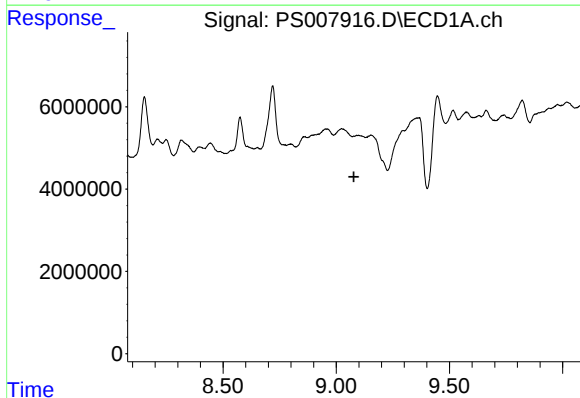


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.078 min
Response: 0
Conc: N.D.

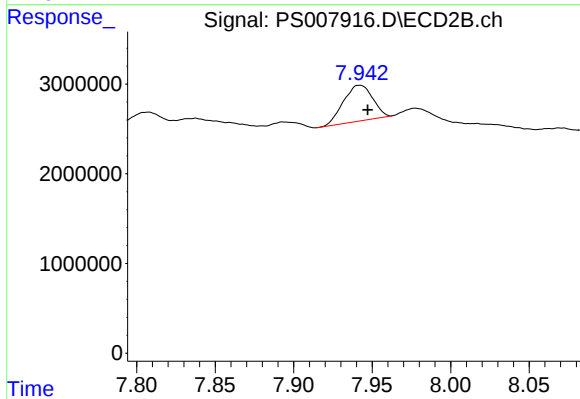

#14 DINOSEB


R.T.: 7.942 min
Delta R.T.: -0.005 min
Response: 5171180
Conc: 1.58 ng/ml

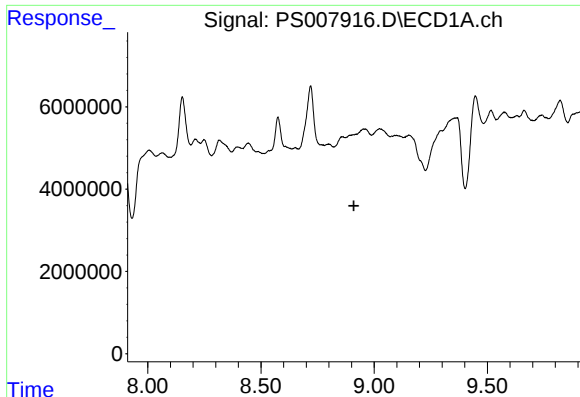

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 8.911 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-34

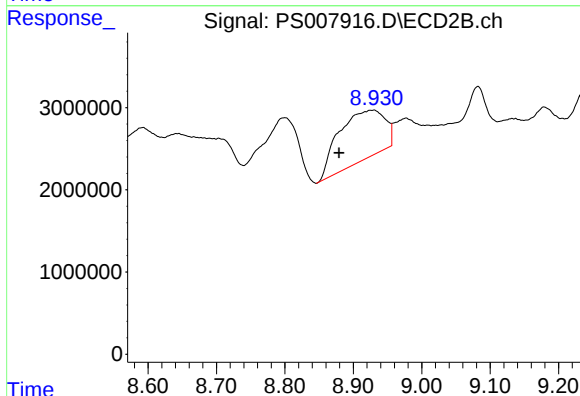


#15 Picloram

R.T.: 8.928 min
Delta R.T.: 0.049 min
Response: 28114976
Conc: 4.55 ng/ml

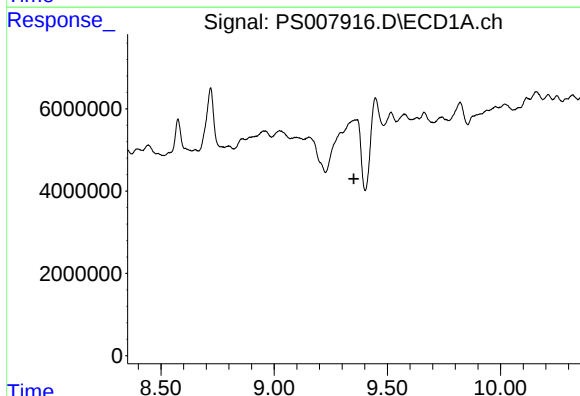

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.352 min
Response: 0
Conc: N.D.

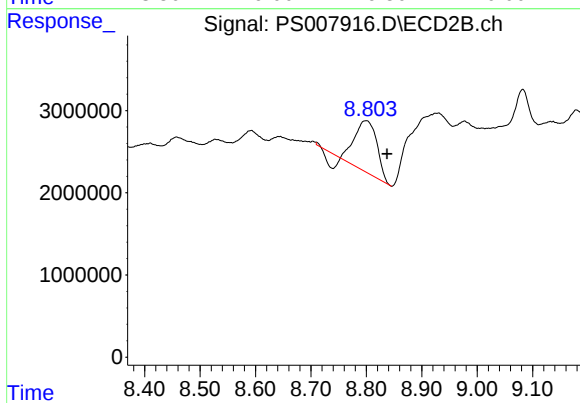

#16 DCPA

R.T.: 8.799 min
Delta R.T.: -0.038 min
Response: 15964939
Conc: 2.78 ng/ml