

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007917.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 14:15
 Operator : SM\AJ
 Sample : K6135-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-35

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 15:46:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.422	5.150	546.6E6	282.6E6	349.423	364.196
Target Compounds							
1) T	Dalapon	1.988	1.694	91198593	388.2E6	44.720	326.803 #
2) T	3,5-DICHL...	0.000	4.484	0	69759406	N.D.	67.408
3) T	4-Nitroph...	0.000	4.827	0	11649287	N.D.	25.724
5) T	DICAMBA	5.513	0.000	39566762	0	6.954	N.D. #
7) T	MCPA	5.889	5.519	27169150	28056137	4.555	8.804 #
8) T	DICHLORPROP	0.000	5.739	0	8829016	N.D.	12.317
9) T	2,4-D	6.472	6.053	24325952	5589385	15.121	6.326 #
10) T	Pentachlo...	6.665	6.436	30116839	20371525	1.385	1.866 #
11) T	2,4,5-TP ...	0.000	6.747	0	39360173	N.D.	9.177
15) T	Picloram	0.000	8.926	0	34920647	N.D.	5.654
16) T	DCPA	0.000	8.797	0	19706625	N.D.	3.434



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007917.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 14:15
Operator : SM\AJ
Sample : K6135-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-35

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 15:46:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

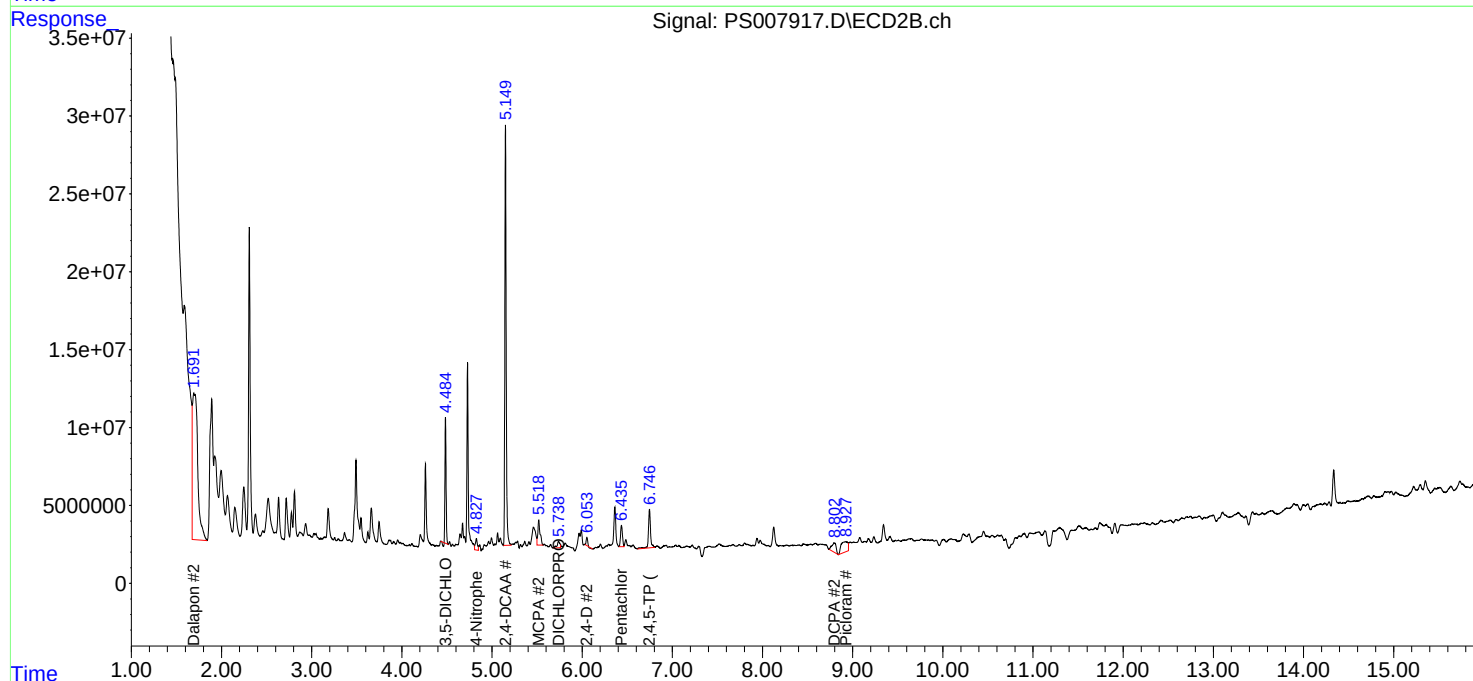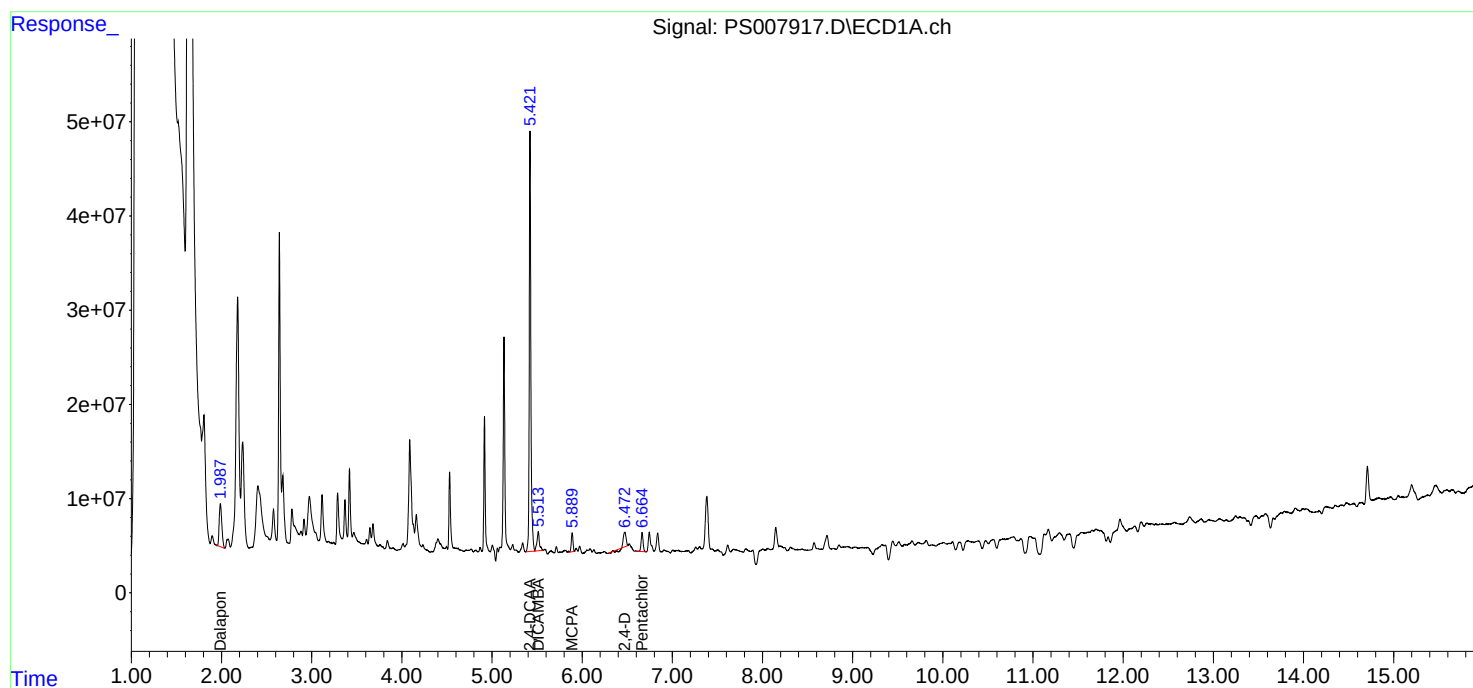


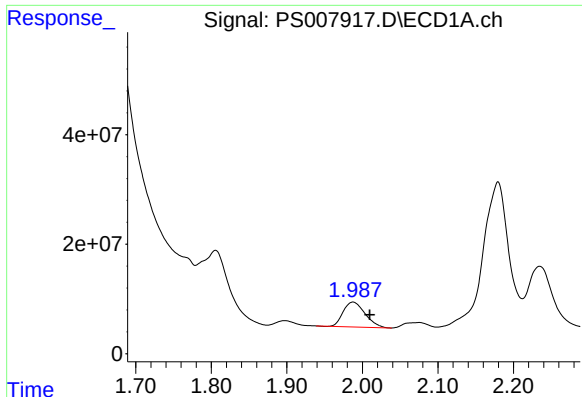

#1 Dalapon


R.T.: 1.988 min
Delta R.T.: -0.022 min
Response: 91198593
Conc: 44.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-35

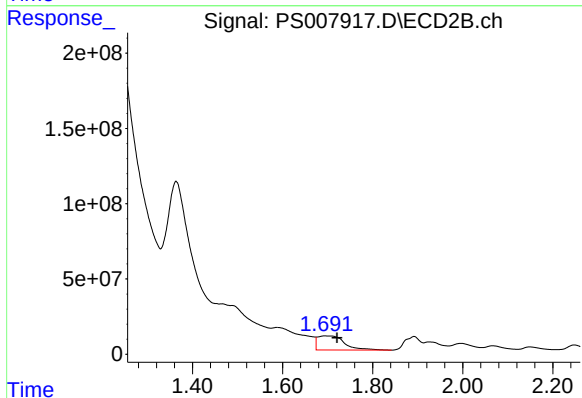


#1 Dalapon

R.T.: 1.694 min
Delta R.T.: -0.027 min
Response: 388173827
Conc: 326.80 ng/ml

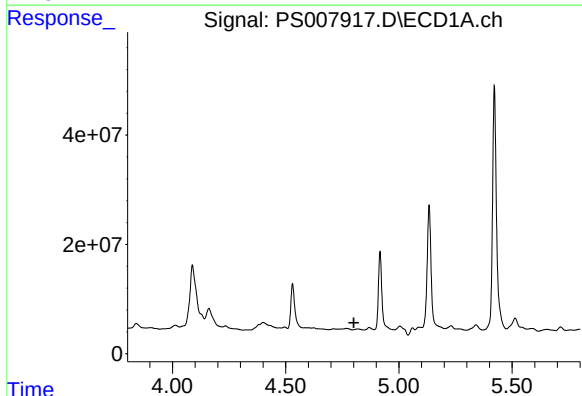


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

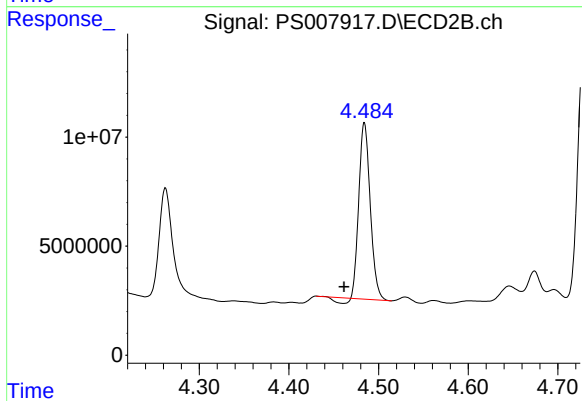

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.484 min
Delta R.T.: 0.023 min
Response: 69759406
Conc: 67.41 ng/ml

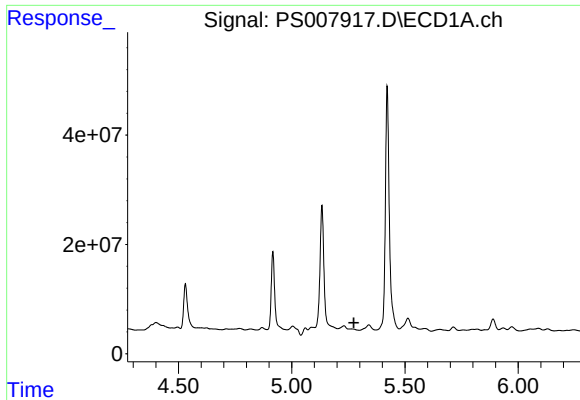

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-35

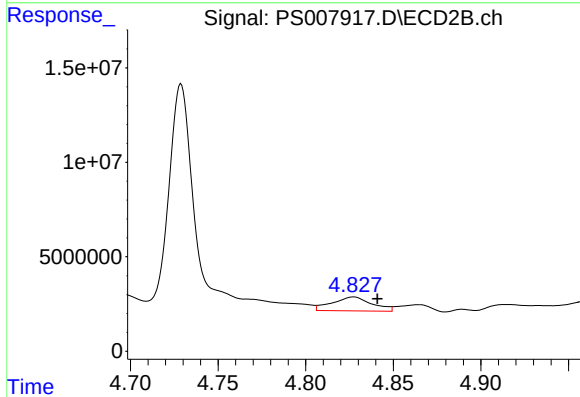


#3 4-Nitrophenol

R.T.: 4.827 min
Delta R.T.: -0.014 min
Response: 11649287
Conc: 25.72 ng/ml

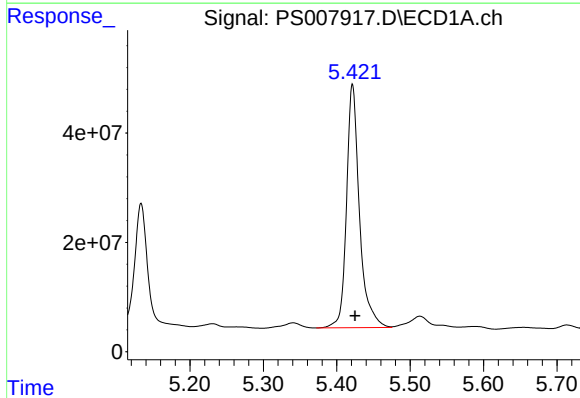


#4 2,4-DCAA

R.T.: 5.422 min
Delta R.T.: -0.003 min
Response: 546614306
Conc: 349.42 ng/ml

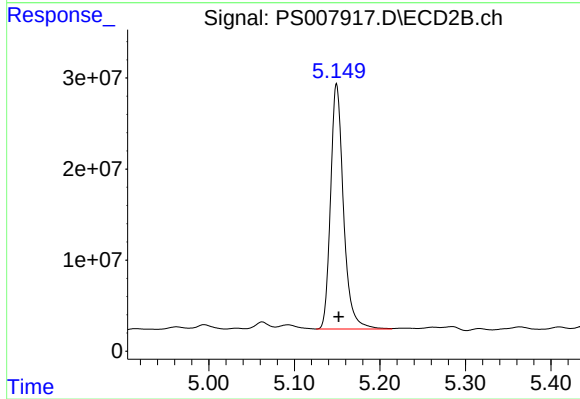

#4 2,4-DCAA


R.T.: 5.150 min
Delta R.T.: -0.002 min
Response: 282586547
Conc: 364.20 ng/ml

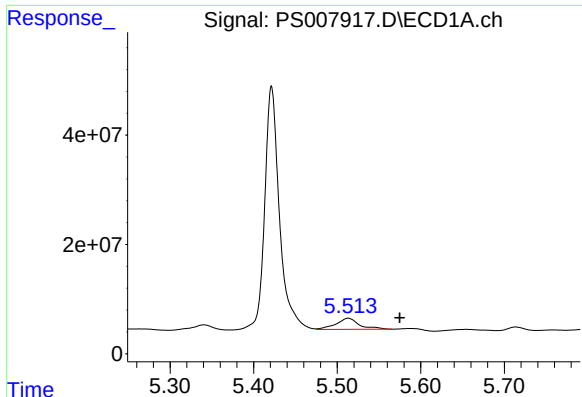

#5 DICAMBA


R.T.: 5.513 min
Delta R.T.: -0.062 min
Response: 39566762
Conc: 6.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-35

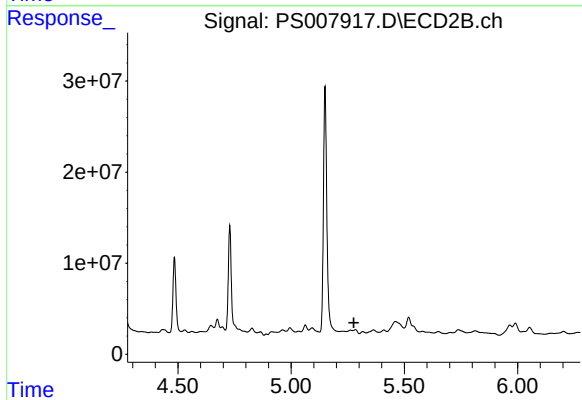


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

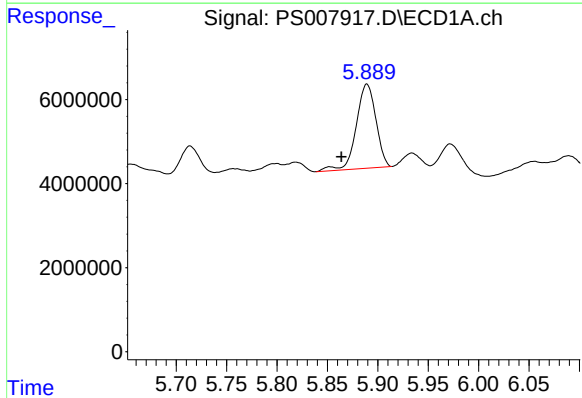


#7 MCPA

R.T.: 5.889 min
Delta R.T.: 0.025 min
Response: 27169150
Conc: 4.56 ug/ml

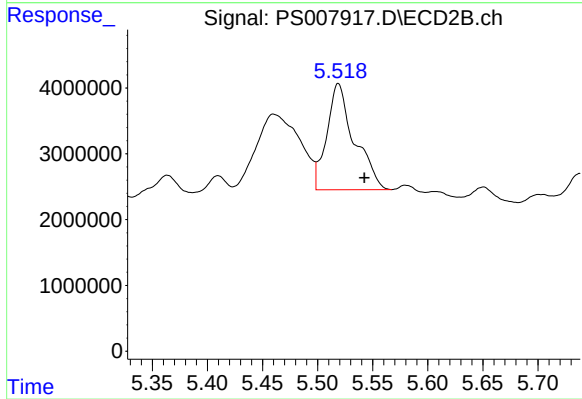

#7 MCPA


R.T.: 5.519 min
Delta R.T.: -0.024 min
Response: 28056137
Conc: 8.80 ug/ml

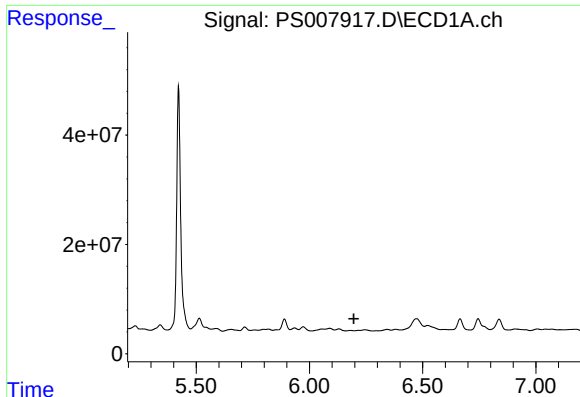

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-35

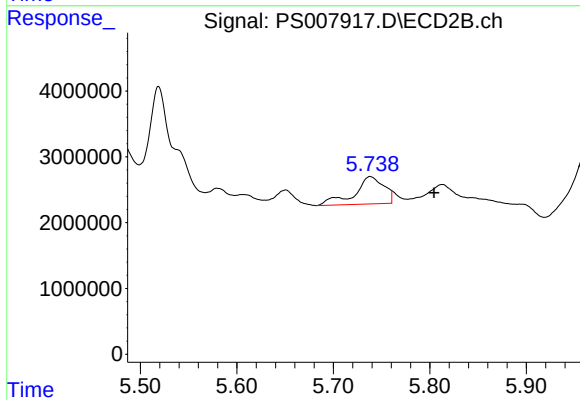


#8 DICHLORPROP

R.T.: 5.739 min
Delta R.T.: -0.066 min
Response: 8829016
Conc: 12.32 ng/ml

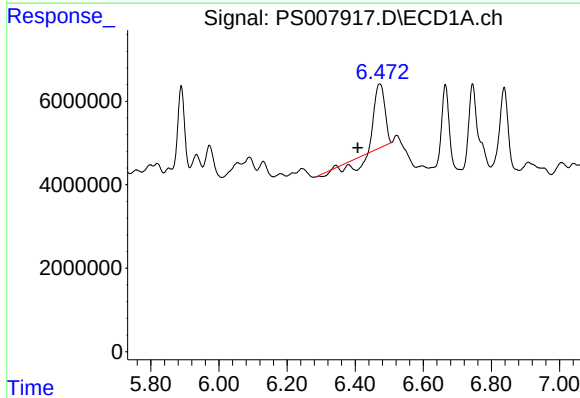


#9 2,4-D

R.T.: 6.472 min
Delta R.T.: 0.064 min
Response: 24325952
Conc: 15.12 ng/ml

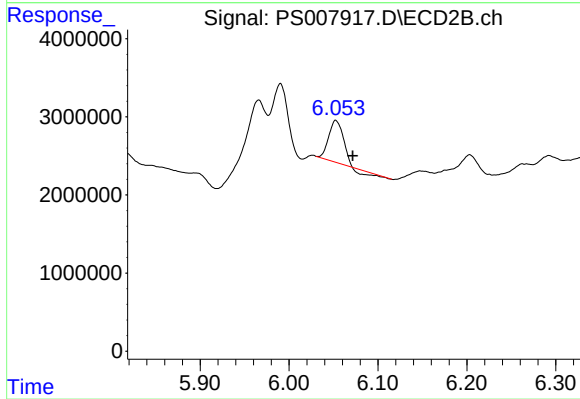

#9 2,4-D


R.T.: 6.053 min
Delta R.T.: -0.019 min
Response: 5589385
Conc: 6.33 ng/ml

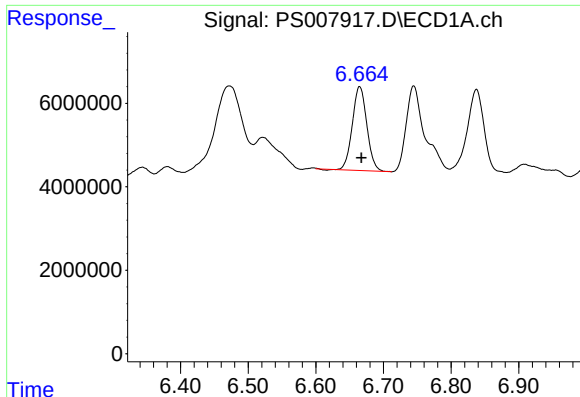

#10 Pentachlorophenol


R.T.: 6.665 min
Delta R.T.: -0.003 min
Response: 30116839
Conc: 1.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-35

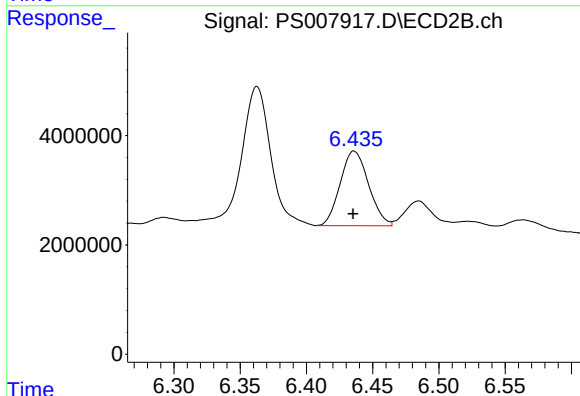


#10 Pentachlorophenol

R.T.: 6.436 min
Delta R.T.: 0.000 min
Response: 20371525
Conc: 1.87 ng/ml

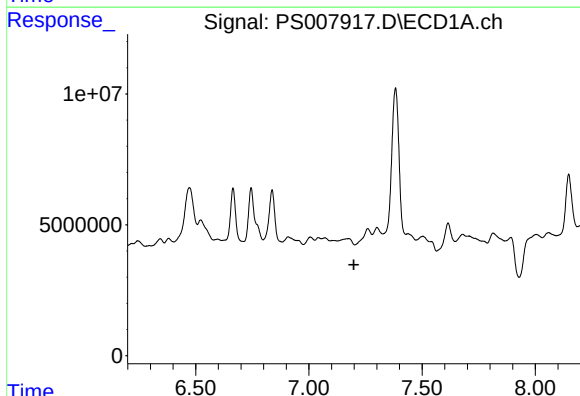


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

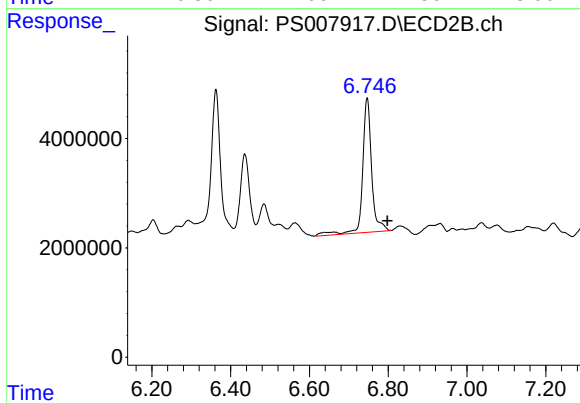

#11 2,4,5-TP (SILVEX)


R.T.: 6.747 min
Delta R.T.: -0.051 min
Response: 39360173
Conc: 9.18 ng/ml

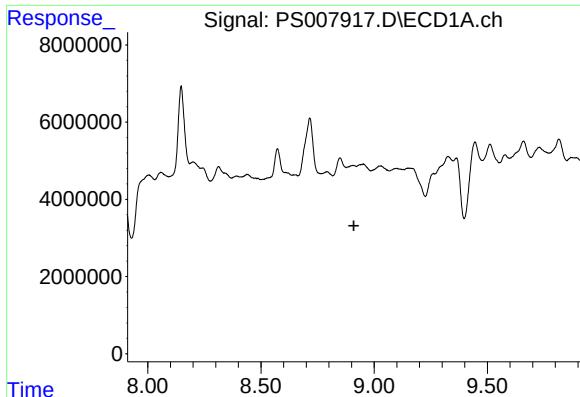

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 8.911 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-35

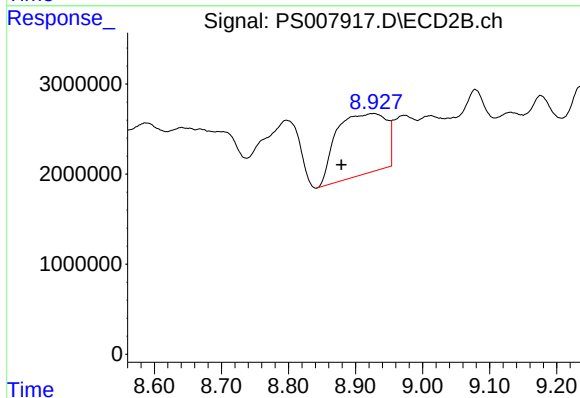


#15 Picloram

R.T.: 8.926 min
Delta R.T.: 0.047 min
Response: 34920647
Conc: 5.65 ng/ml

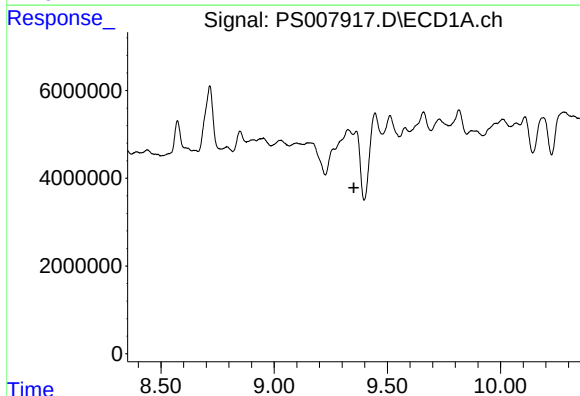

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.352 min
Response: 0
Conc: N.D.

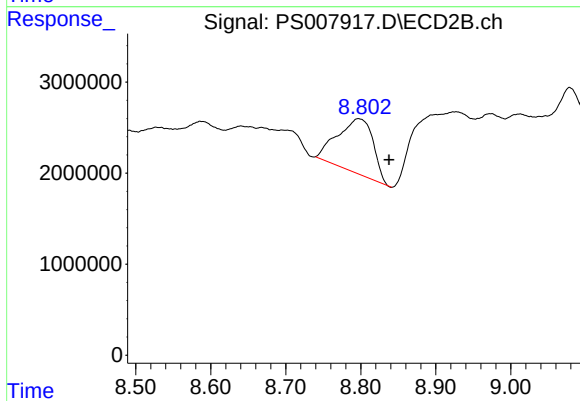

#16 DCPA

R.T.: 8.797 min
Delta R.T.: -0.040 min
Response: 19706625
Conc: 3.43 ng/ml