

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007918.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 14:37
 Operator : SM\AJ
 Sample : K6135-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-36

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 15:47:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.423	5.152	644.4E6	323.9E6	411.947	417.497
Target Compounds							
1) T	Dalapon	1.990	1.694	100.1E6	416.5E6	49.095	350.648 #
2) T	3,5-DICHL...	0.000	4.487	0	71568126	N.D.	69.156
5) T	DICAMBA	5.516	0.000	56725684	0	9.970	N.D. #
7) T	MCPA	5.891	5.542	29084036	13894979	4.876	4.360
8) T	DICHLORPROP	0.000	5.739	0	11910564	N.D.	16.616
9) T	2,4-D	6.472	6.055	83972996	4854195	52.196	5.494 #
10) T	Pentachlo...	0.000	6.440	0	11276296	N.D.	1.033
11) T	2,4,5-TP ...	0.000	6.749	0	38311729	N.D.	8.933
15) T	Picloram	0.000	8.929	0	27360625	N.D.	4.430
16) T	DCPA	0.000	8.792	0	23440628	N.D.	4.085



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007918.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 14:37
Operator : SM\AJ
Sample : K6135-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-36

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 15:47:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

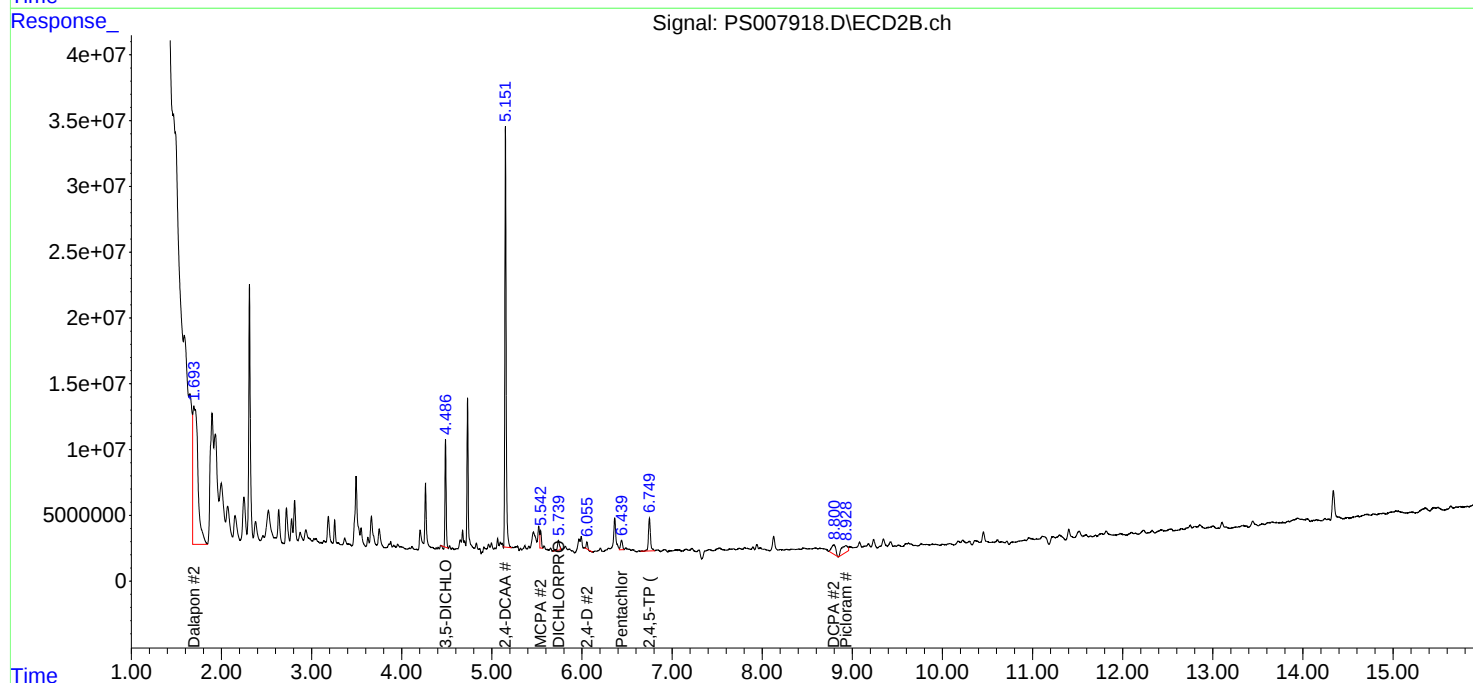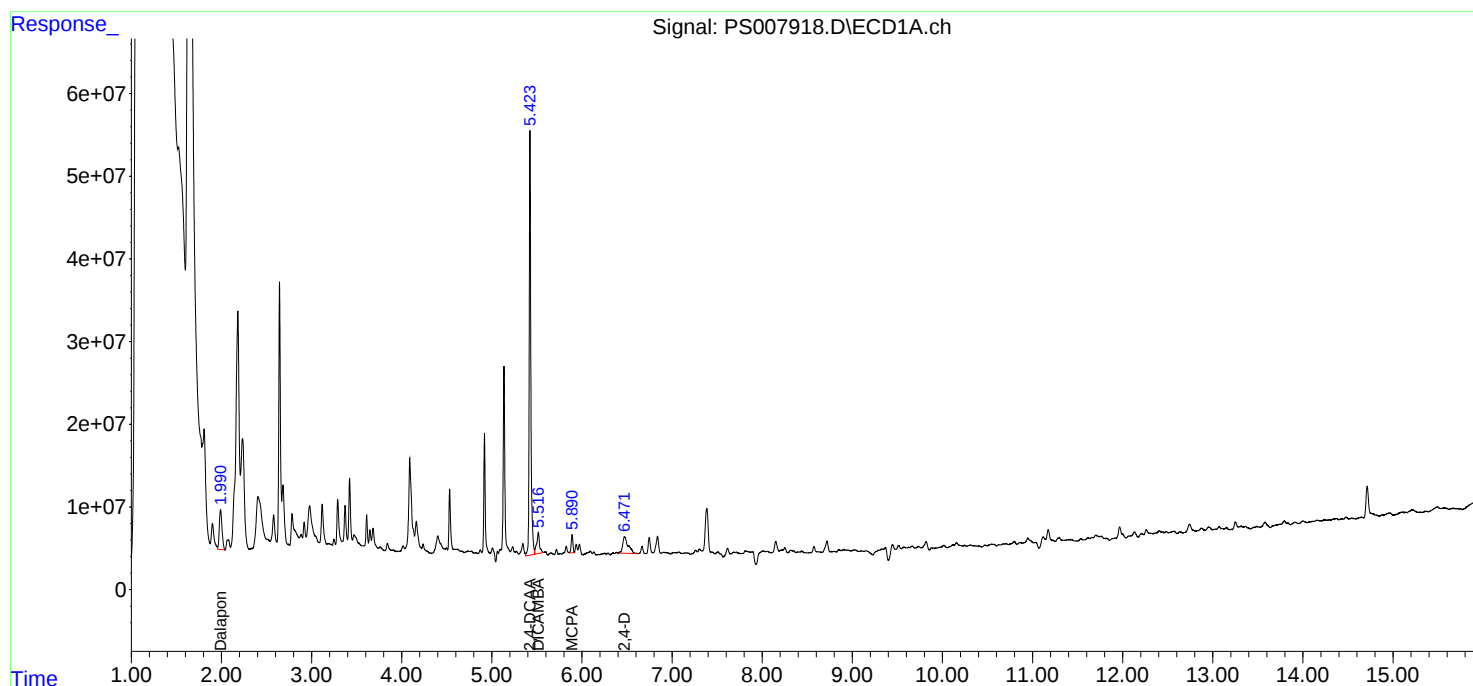


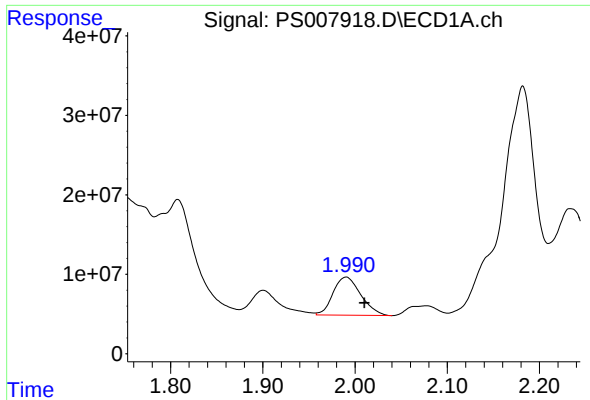

#1 Dalapon


R.T.: 1.990 min
Delta R.T.: -0.020 min
Response: 100121188
Conc: 49.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-36

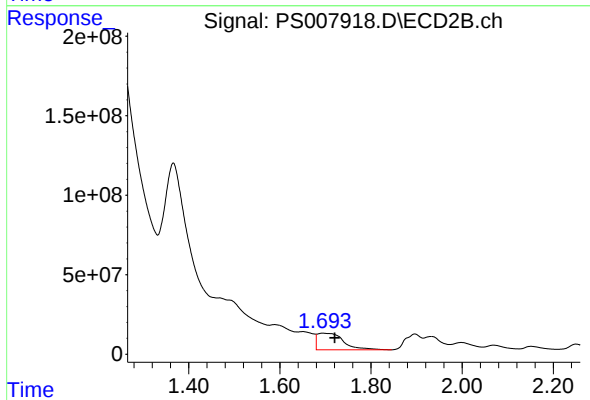


#1 Dalapon

R.T.: 1.694 min
Delta R.T.: -0.026 min
Response: 416497094
Conc: 350.65 ng/ml

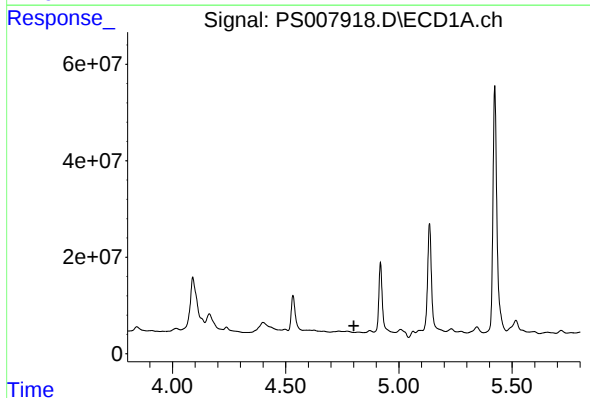


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

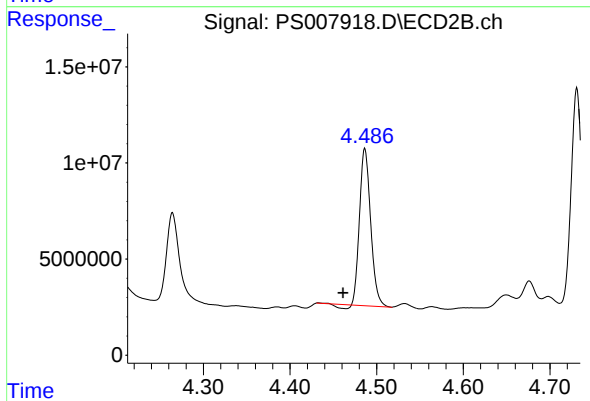

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.487 min
Delta R.T.: 0.025 min
Response: 71568126
Conc: 69.16 ng/ml

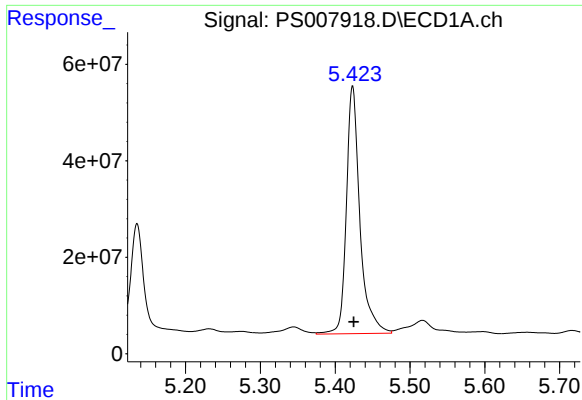

#4 2,4-DCAA


R.T.: 5.423 min
Delta R.T.: -0.002 min
Response: 644422090
Conc: 411.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-36

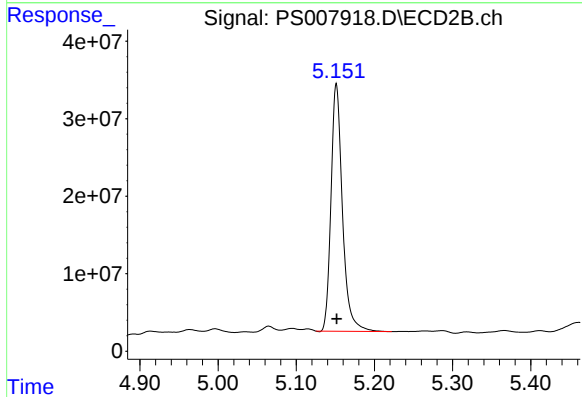


#4 2,4-DCAA

R.T.: 5.152 min
Delta R.T.: 0.000 min
Response: 323943394
Conc: 417.50 ng/ml

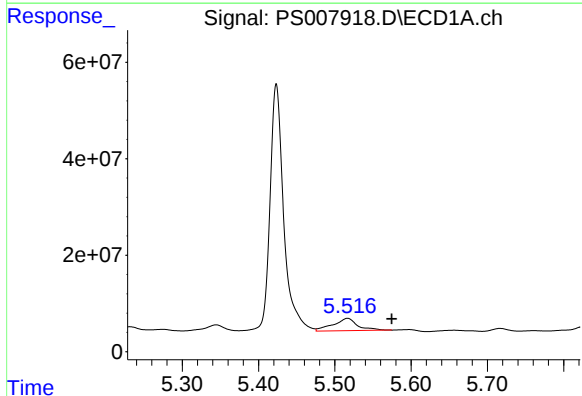


#5 DICAMBA

R.T.: 5.516 min
Delta R.T.: -0.058 min
Response: 56725684
Conc: 9.97 ng/ml

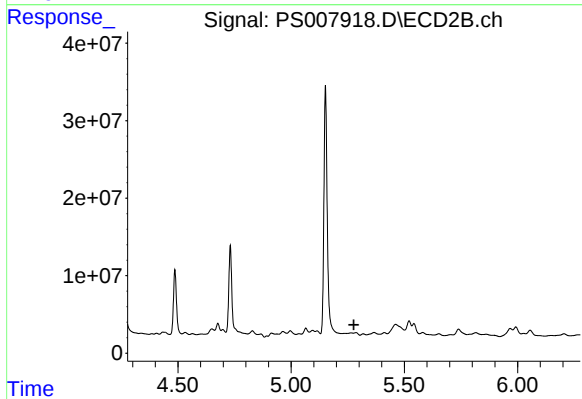

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

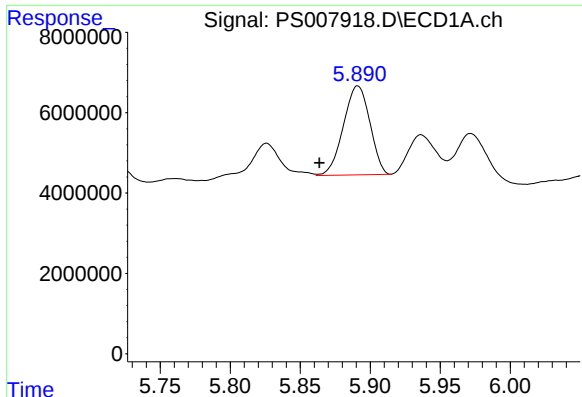

#7 MCPA


R.T.: 5.891 min
Delta R.T.: 0.027 min
Response: 29084036
Conc: 4.88 ug/ml

Instrument :
ECD_S
ClientSampleId :
COMP-36

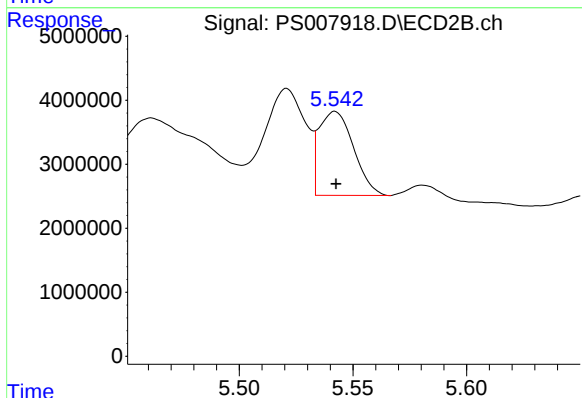


#7 MCPA

R.T.: 5.542 min
Delta R.T.: 0.000 min
Response: 13894979
Conc: 4.36 ug/ml

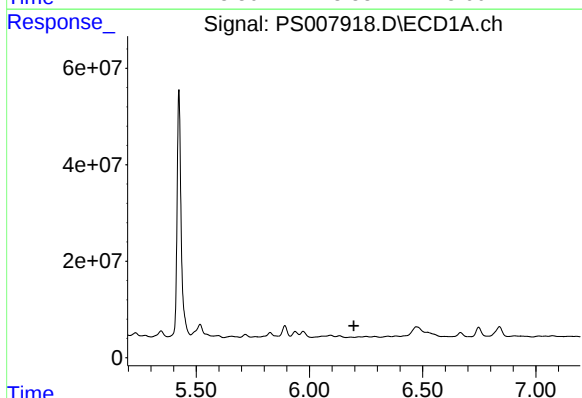


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.197 min
Response: 0
Conc: N.D.

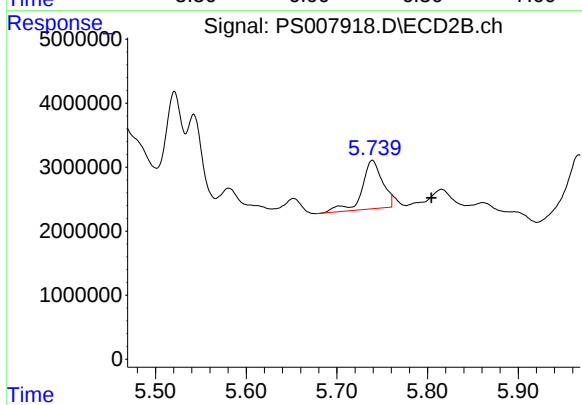

#8 DICHLORPROP


R.T.: 5.739 min
Delta R.T.: -0.065 min
Response: 11910564
Conc: 16.62 ng/ml

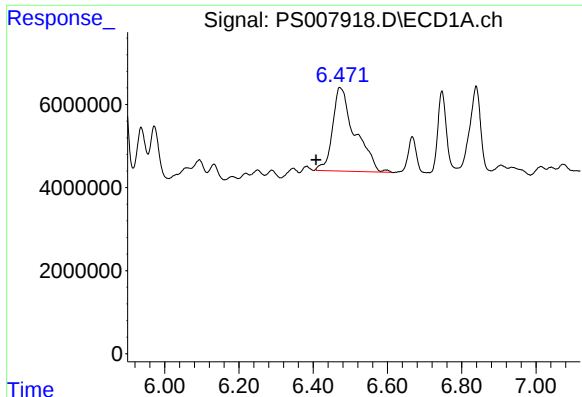

#9 2,4-D


R.T.: 6.472 min
Delta R.T.: 0.064 min
Response: 83972996
Conc: 52.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-36

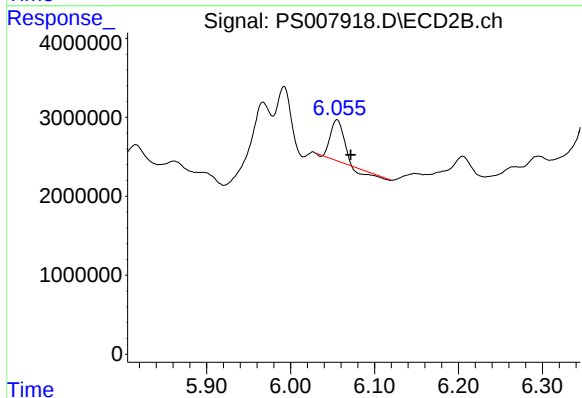


#9 2,4-D

R.T.: 6.055 min
Delta R.T.: -0.016 min
Response: 4854195
Conc: 5.49 ng/ml

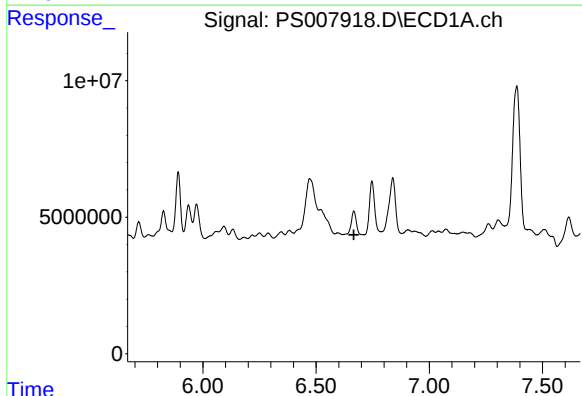


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.667 min
Response: 0
Conc: N.D.

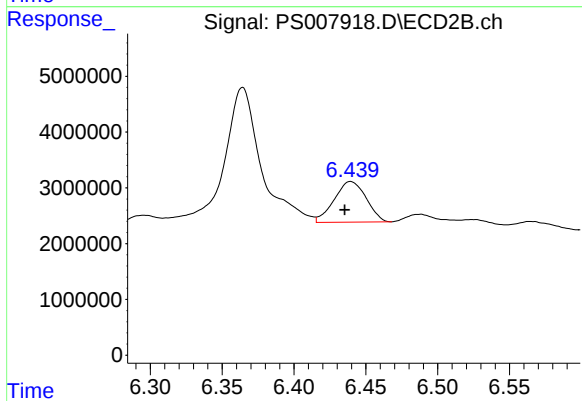

#10 Pentachlorophenol


R.T.: 6.440 min
Delta R.T.: 0.004 min
Response: 11276296
Conc: 1.03 ng/ml

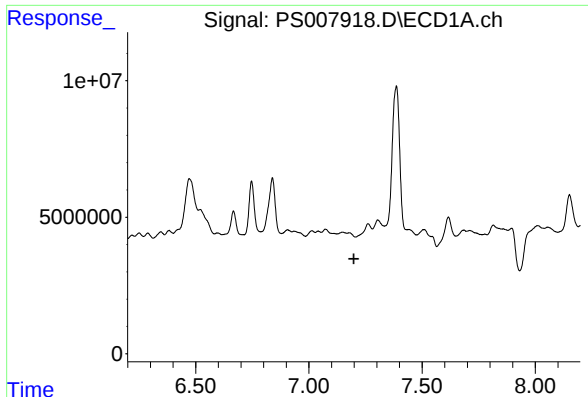

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-36

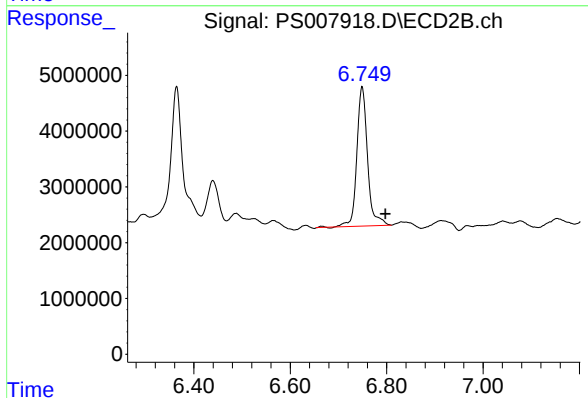


#11 2,4,5-TP (SILVEX)

R.T.: 6.749 min
Delta R.T.: -0.049 min
Response: 38311729
Conc: 8.93 ng/ml

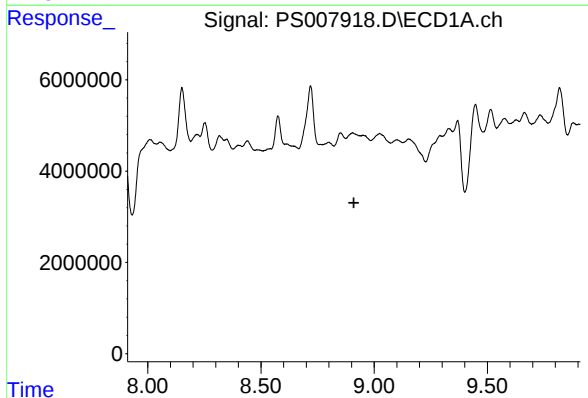


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.911 min
Response: 0
Conc: N.D.

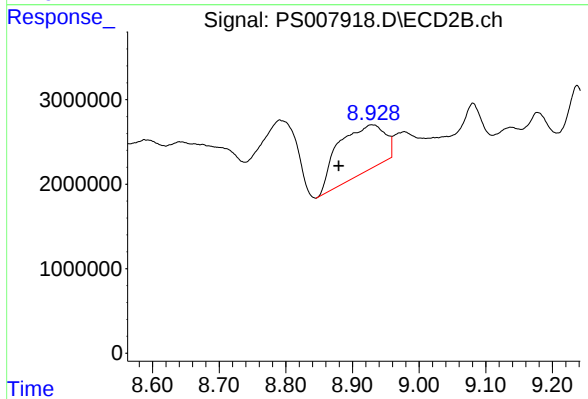

#15 Picloram


R.T.: 8.929 min
Delta R.T.: 0.050 min
Response: 27360625
Conc: 4.43 ng/ml

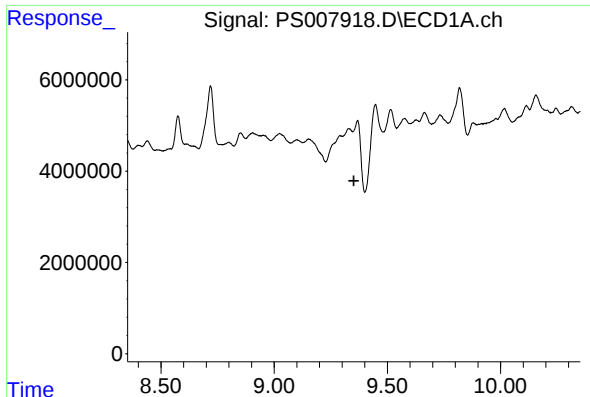

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-36

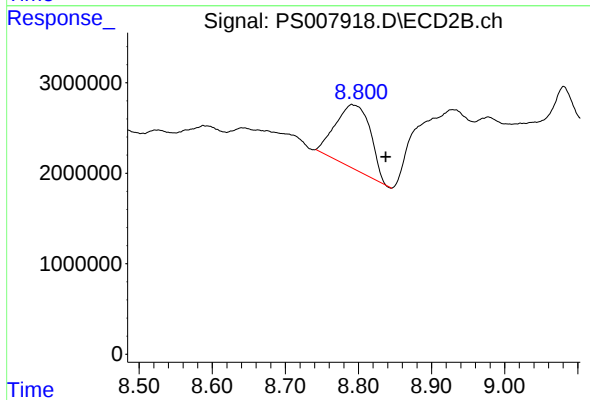

#16 DCPA

R.T.: 8.792 min
Delta R.T.: -0.046 min
Response: 23440628
Conc: 4.08 ng/ml