

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 17:30
 Operator : SM\AJ
 Sample : PB125293BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB125293BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:23:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.445	5.171	483.3E6	266.5E6	308.938	343.492
Target Compounds							
1) T	Dalapon	2.008	1.730	146.6E6	159.9E6	71.862	134.624 #
2) T	3,5-DICHL...	0.000	4.504	0	54507626	N.D.	52.671
5) T	DICAMBA	5.533	0.000	69247136	0	12.171	N.D. #
7) T	MCPA	5.909	5.538	25679487	22300065	4.306	6.998 #
9) T	2,4-D	0.000	6.073	0	9087555	N.D.	10.284
10) T	Pentachlo...	0.000	6.462	0	8054858	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.770	0	29295868	N.D.	6.831
13) T	2,4-DB	0.000	7.583	0	38111522	N.D.	70.395
14) T	DINOSEB	0.000	7.960	0	5426817	N.D.	1.659
15) T	Picloram	8.974	8.916	281.7E6	184.1E6	23.297	29.808 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 17:30
Operator : SM\AJ
Sample : PB125293BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB125293BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:23:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

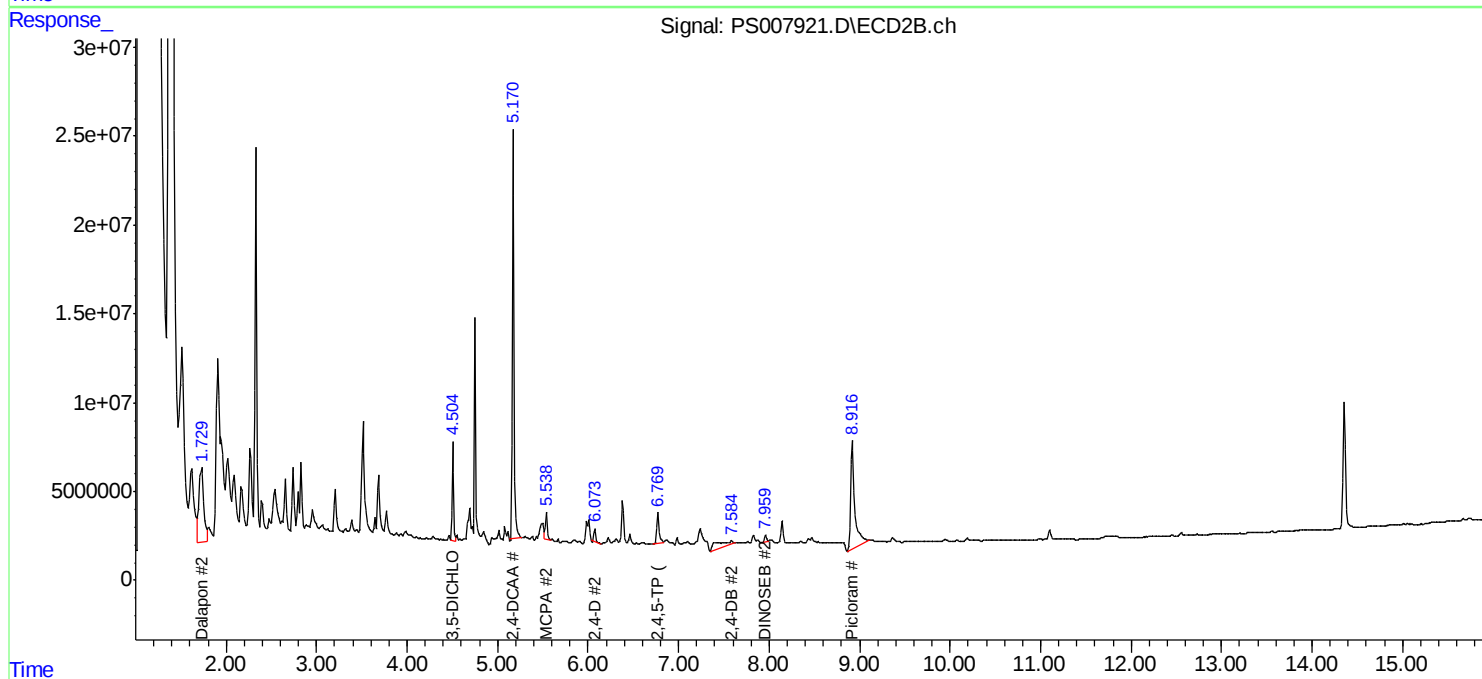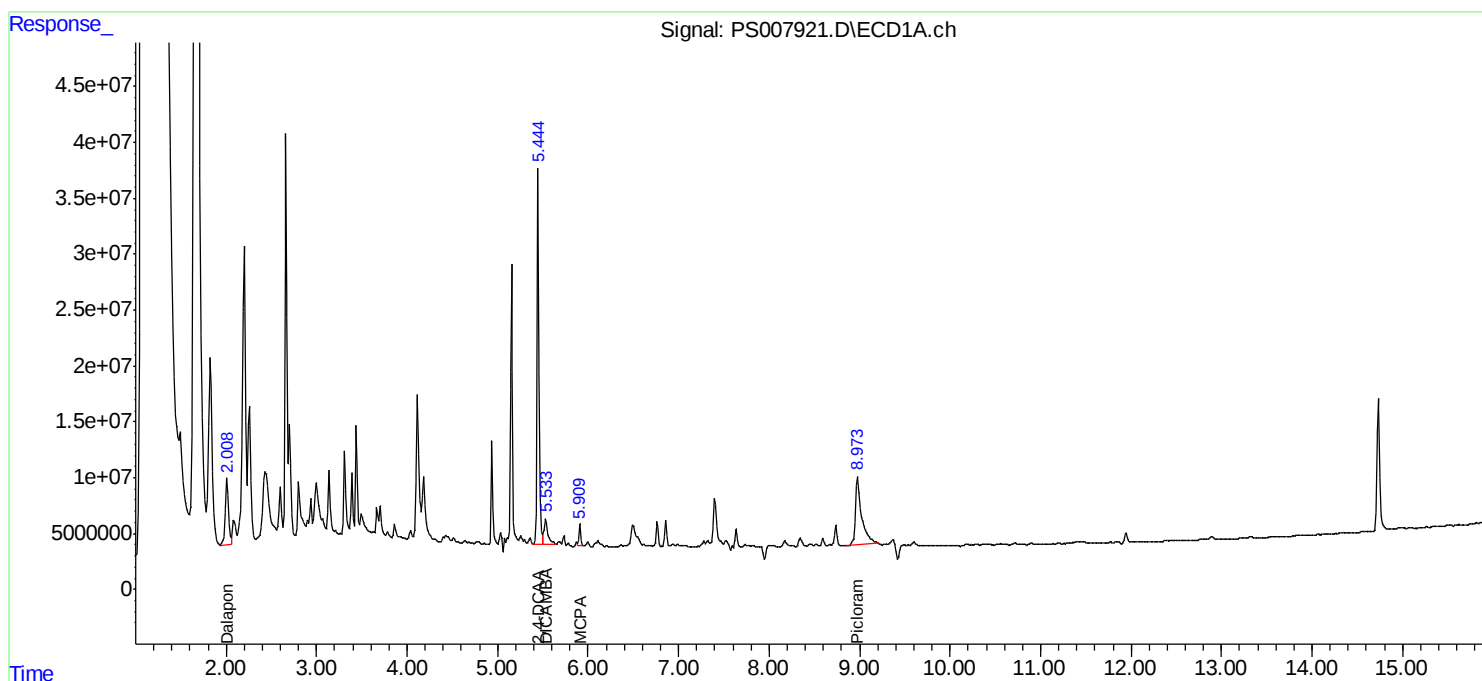


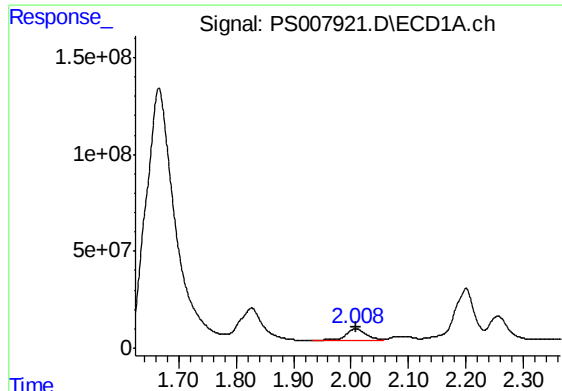

#1 Dalapon


R.T.: 2.008 min
Delta R.T.: -0.002 min
Response: 146550209
Conc: 71.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125293BL

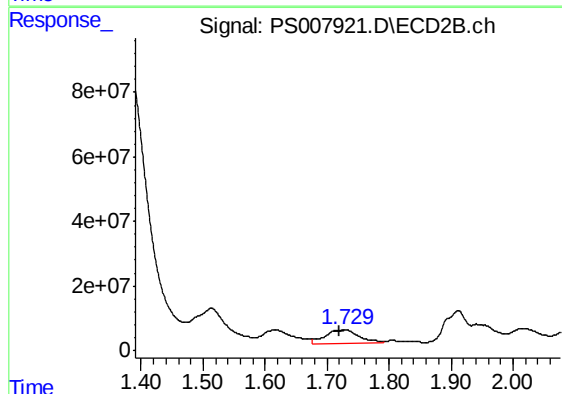


#1 Dalapon

R.T.: 1.730 min
Delta R.T.: 0.009 min
Response: 159905021
Conc: 134.62 ng/ml

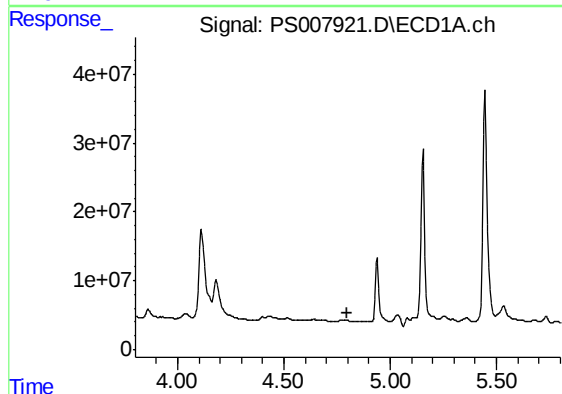


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

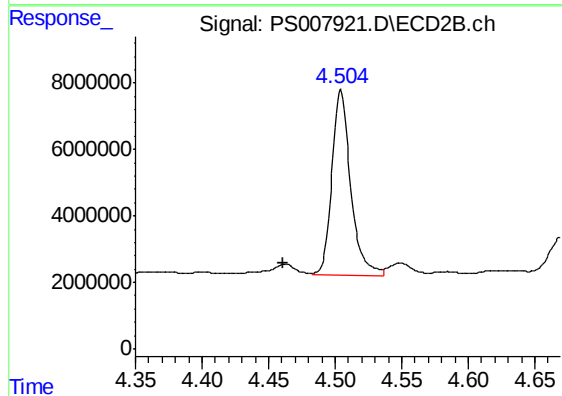

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.504 min
Delta R.T.: 0.043 min
Response: 54507626
Conc: 52.67 ng/ml

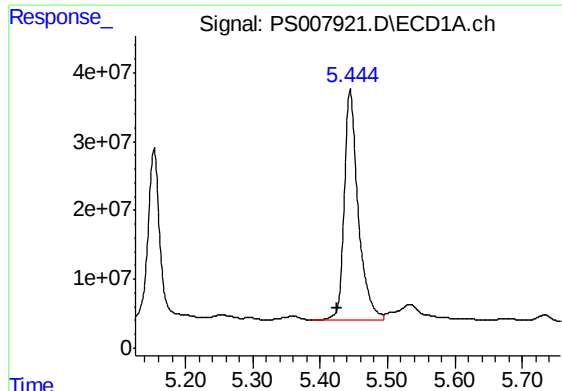

#4 2,4-DCAA


R.T.: 5.445 min
Delta R.T.: 0.020 min
Response: 483281908
Conc: 308.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125293BL

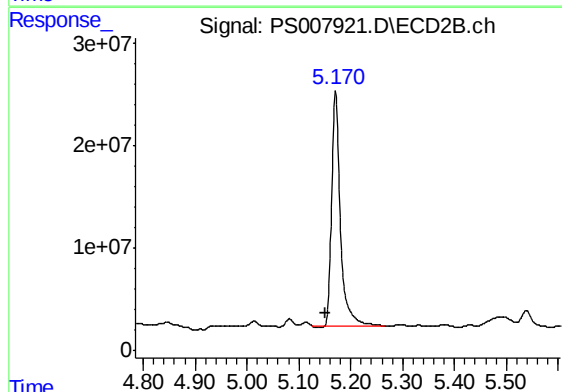


#4 2,4-DCAA

R.T.: 5.171 min
Delta R.T.: 0.019 min
Response: 266521225
Conc: 343.49 ng/ml

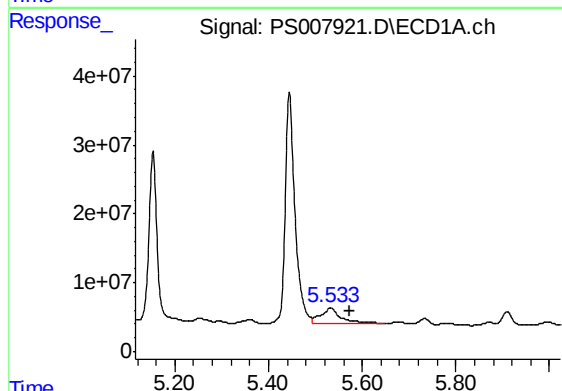


#5 DICAMBA

R.T.: 5.533 min
Delta R.T.: -0.042 min
Response: 69247136
Conc: 12.17 ng/ml

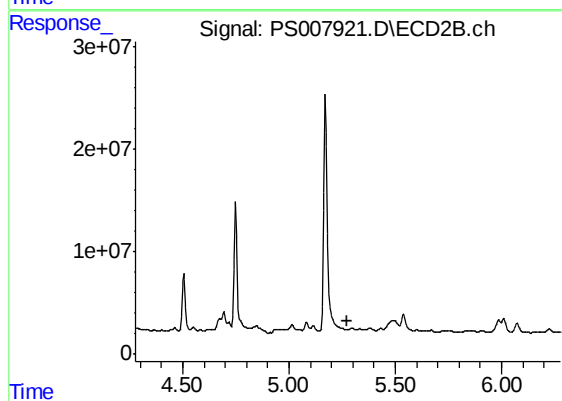

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

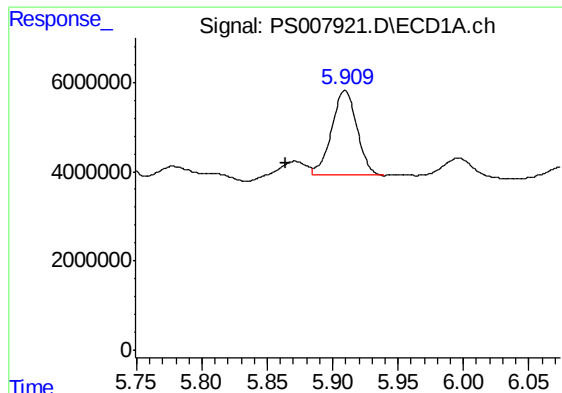

#7 MCPA


R.T.: 5.909 min
Delta R.T.: 0.046 min
Response: 25679487
Conc: 4.31 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB125293BL

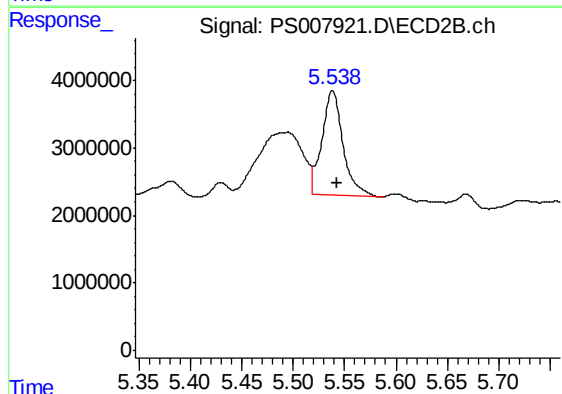


#7 MCPA

R.T.: 5.538 min
Delta R.T.: -0.004 min
Response: 22300065
Conc: 7.00 ug/ml

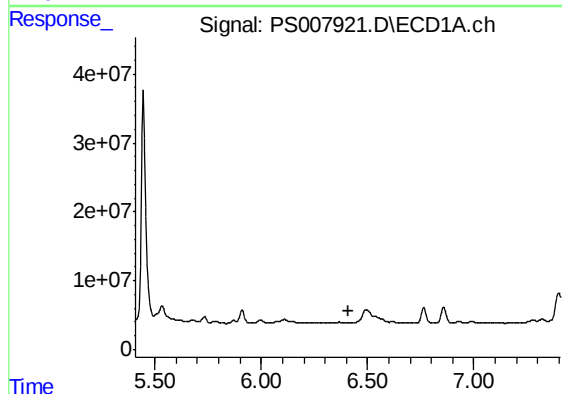


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.408 min
Response: 0
Conc: N.D.

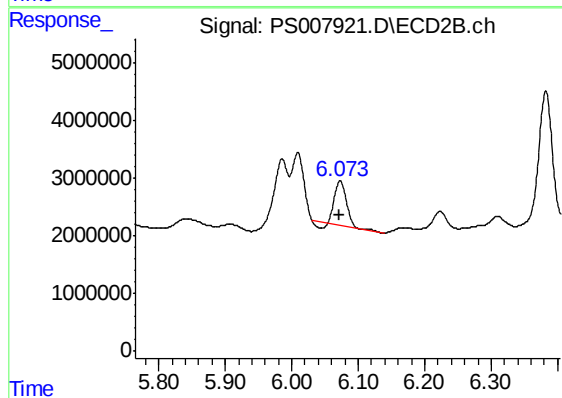

#9 2,4-D


R.T.: 6.073 min
Delta R.T.: 0.001 min
Response: 9087555
Conc: 10.28 ng/ml

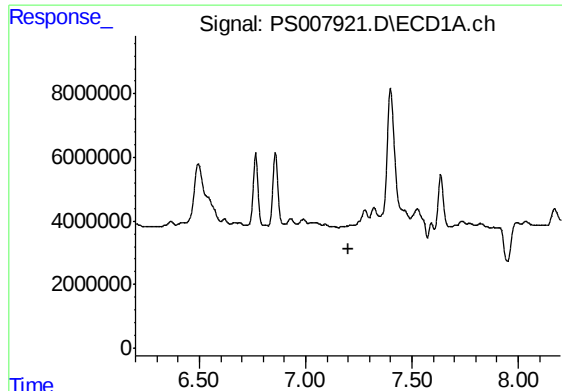

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB125293BL

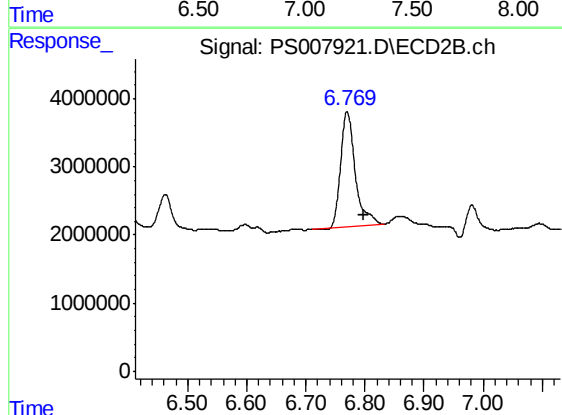


#11 2,4,5-TP (SILVEX)

R.T.: 6.770 min
Delta R.T.: -0.028 min
Response: 29295868
Conc: 6.83 ng/ml

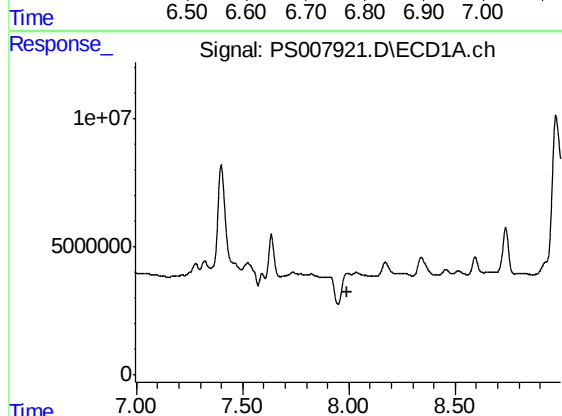


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 7.995 min
Response: 0
Conc: N.D.

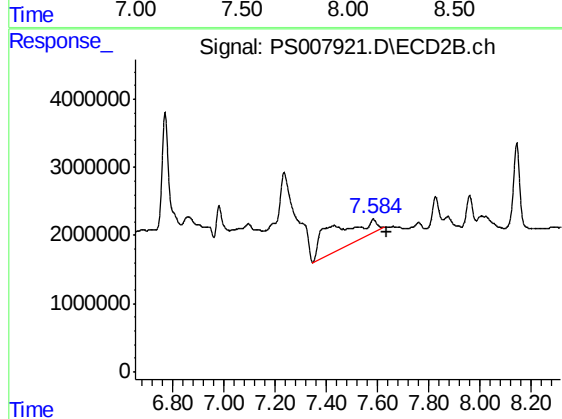

#13 2,4-DB


R.T.: 7.583 min
Delta R.T.: -0.055 min
Response: 38111522
Conc: 70.40 ng/ml

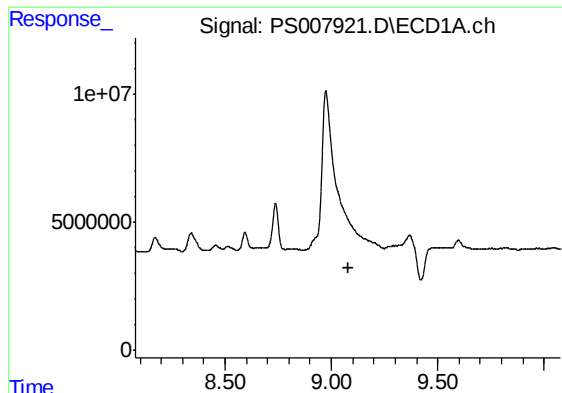

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.078 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB125293BL

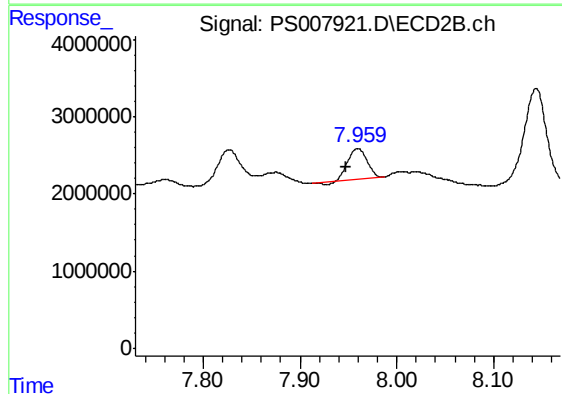


#14 DINOSEB

R.T.: 7.960 min
Delta R.T.: 0.013 min
Response: 5426817
Conc: 1.66 ng/ml

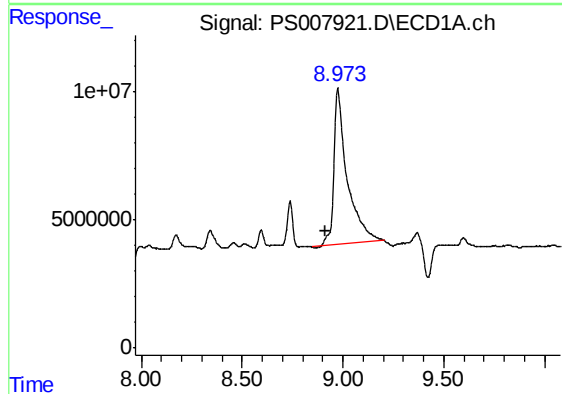

#15 Picloram

R.T.: 8.974 min
Delta R.T.: 0.063 min
Response: 281683799
Conc: 23.30 ng/ml

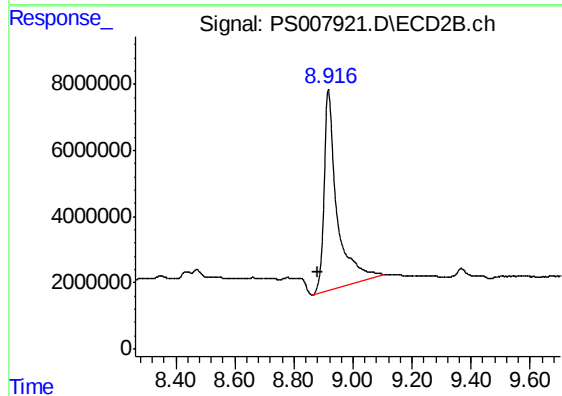

#15 Picloram

R.T.: 8.916 min
Delta R.T.: 0.037 min
Response: 184109076
Conc: 29.81 ng/ml