

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007923.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 18:14
 Operator : SM\AJ
 Sample : PB125293TB
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB125293TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:24:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.441	5.168	479.4E6	276.1E6	306.433	355.836
Target Compounds							
1) T	Dalapon	2.005	1.726	149.9E6	158.2E6	73.494	133.226 #
2) T	3,5-DICHL...	0.000	4.502	0	50200431	N.D.	48.509
5) T	DICAMBA	5.530	0.000	58453443	0	10.274	N.D. #
7) T	MCPA	5.906	5.535	45922085	25107287	7.700	7.879
9) T	2,4-D	0.000	6.070	0	10345693	N.D.	11.708
10) T	Pentachlo...	0.000	6.455	0	14962149	N.D.	1.371
11) T	2,4,5-TP ...	0.000	6.768	0	18506428	N.D.	4.315
14) T	DINOSEB	0.000	7.959	0	6021414	N.D.	1.841
15) T	Picloram	0.000	8.919	0	111.2E6	N.D.	18.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007923.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 18:14
Operator : SM\AJ
Sample : PB125293TB
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB125293TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:24:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

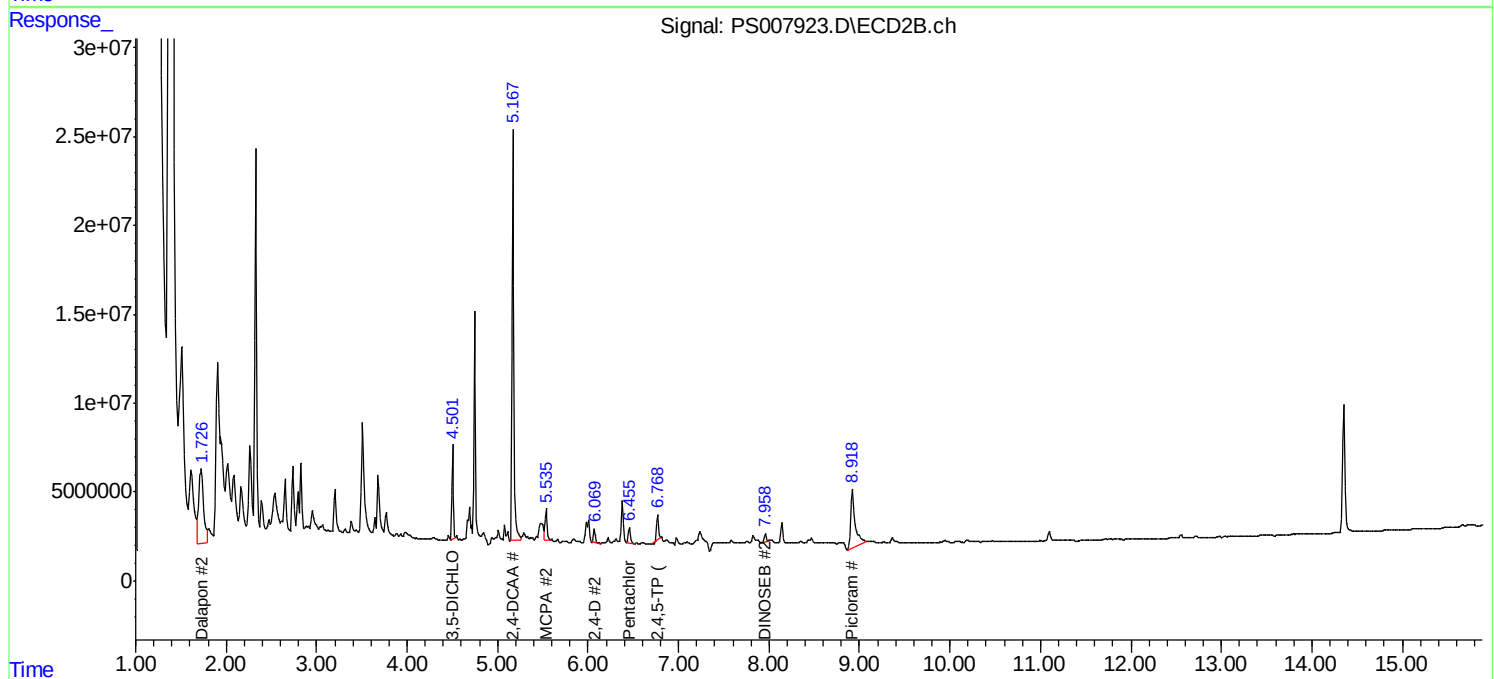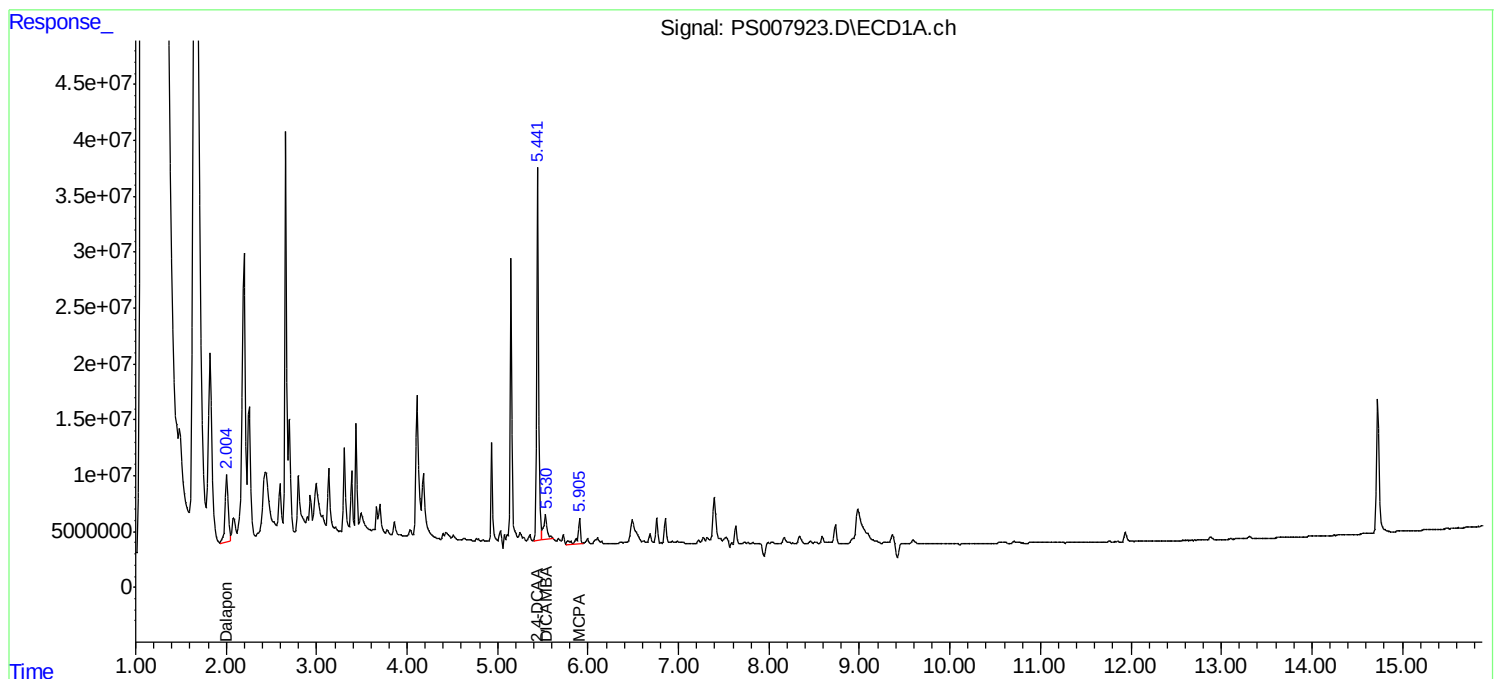


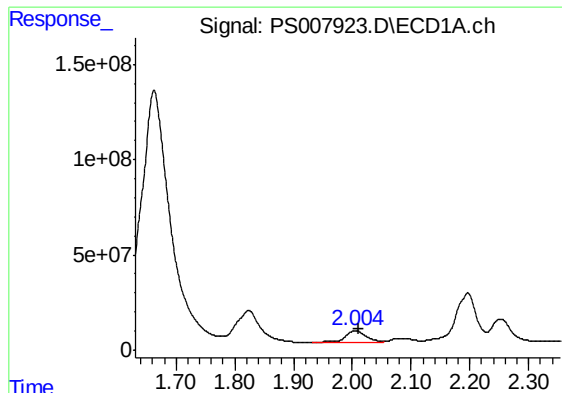

#1 Dalapon


R.T.: 2.005 min
Delta R.T.: -0.005 min
Response: 149879159
Conc: 73.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125293TB

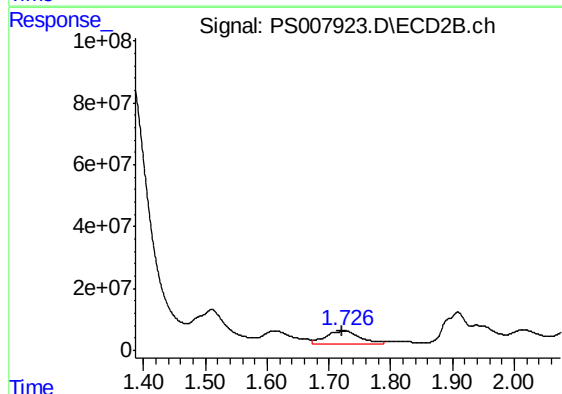


#1 Dalapon

R.T.: 1.726 min
Delta R.T.: 0.006 min
Response: 158244195
Conc: 133.23 ng/ml

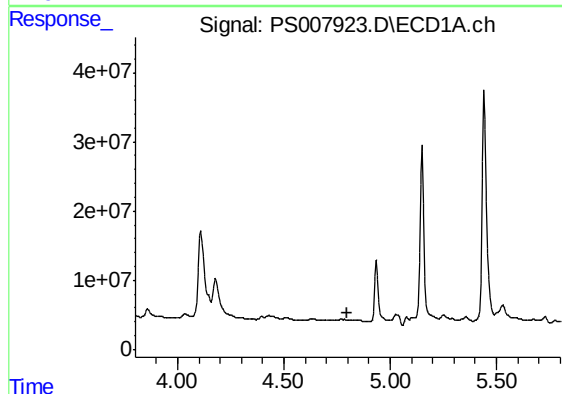


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

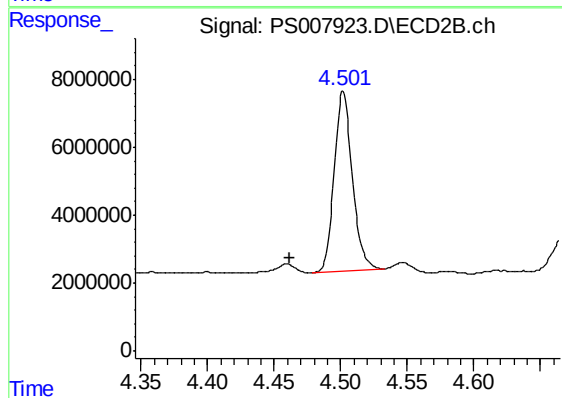

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.502 min
Delta R.T.: 0.041 min
Response: 50200431
Conc: 48.51 ng/ml

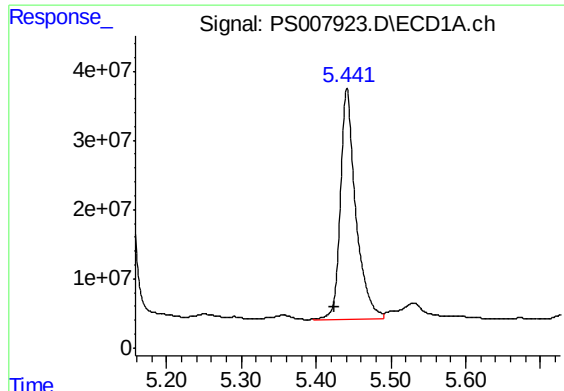

#4 2,4-DCAA


R.T.: 5.441 min
Delta R.T.: 0.016 min
Response: 479362950
Conc: 306.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125293TB

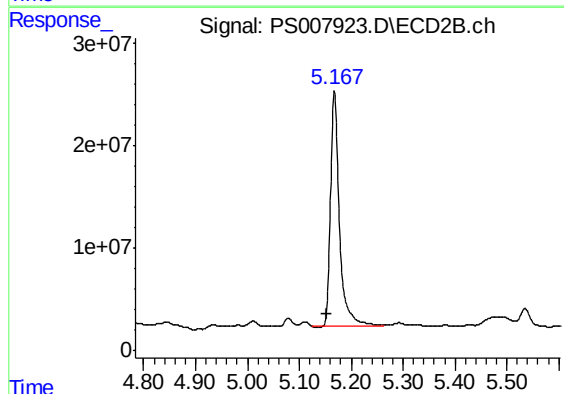


#4 2,4-DCAA

R.T.: 5.168 min
Delta R.T.: 0.016 min
Response: 276099681
Conc: 355.84 ng/ml

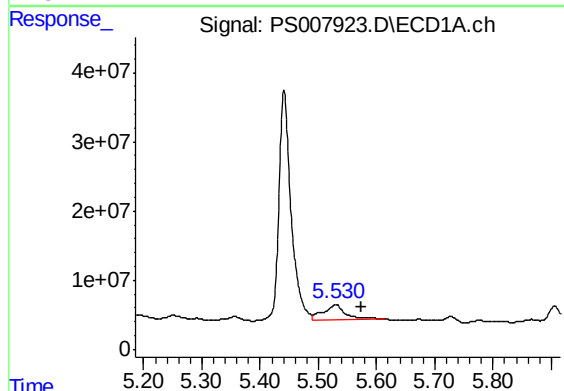


#5 DICAMBA

R.T.: 5.530 min
Delta R.T.: -0.045 min
Response: 58453443
Conc: 10.27 ng/ml

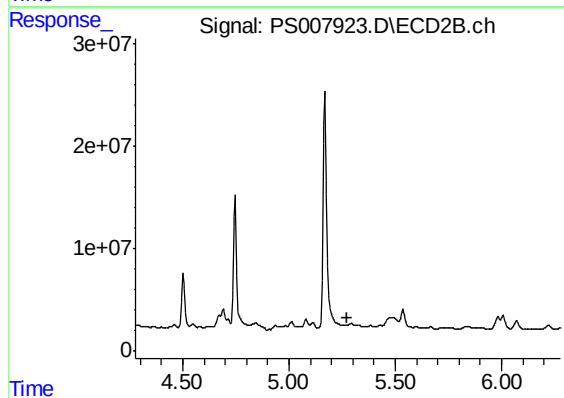

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

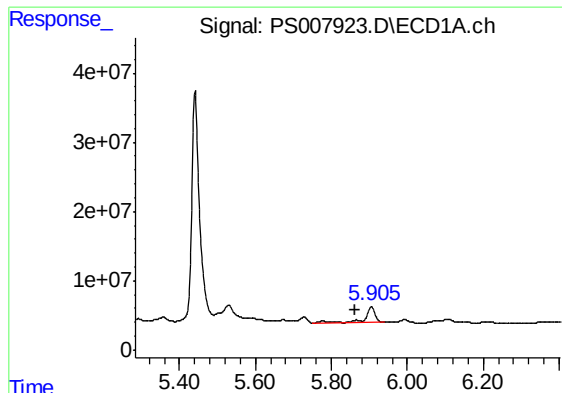

#7 MCPA


R.T.: 5.906 min
Delta R.T.: 0.042 min
Response: 45922085
Conc: 7.70 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB125293TB

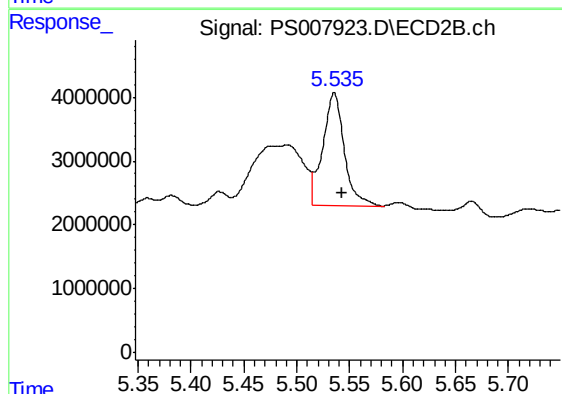


#7 MCPA

R.T.: 5.535 min
Delta R.T.: -0.007 min
Response: 25107287
Conc: 7.88 ug/ml

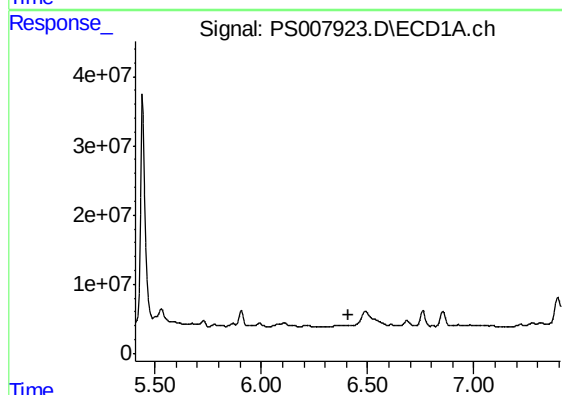


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

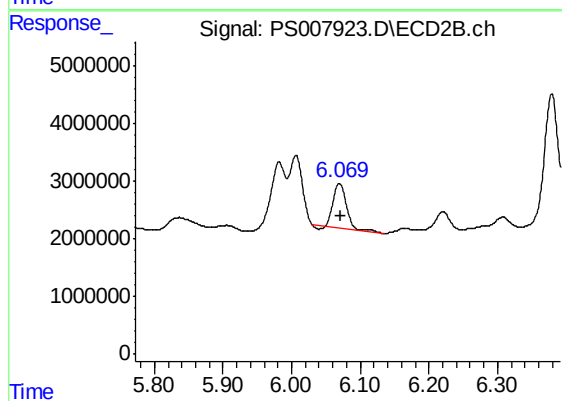

#9 2,4-D


R.T.: 6.070 min
Delta R.T.: -0.002 min
Response: 10345693
Conc: 11.71 ng/ml

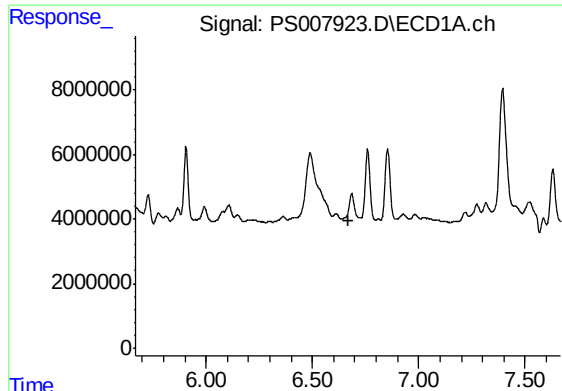

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.667 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB125293TB

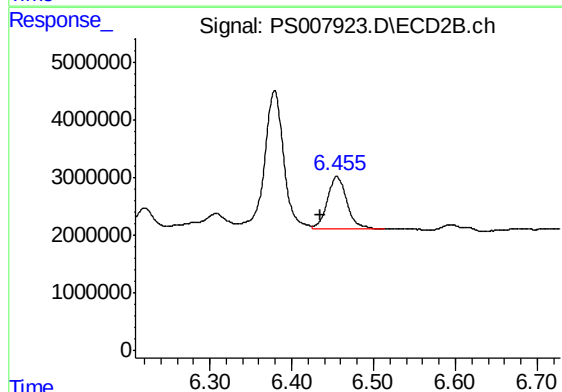


#10 Pentachlorophenol

R.T.: 6.455 min
Delta R.T.: 0.020 min
Response: 14962149
Conc: 1.37 ng/ml

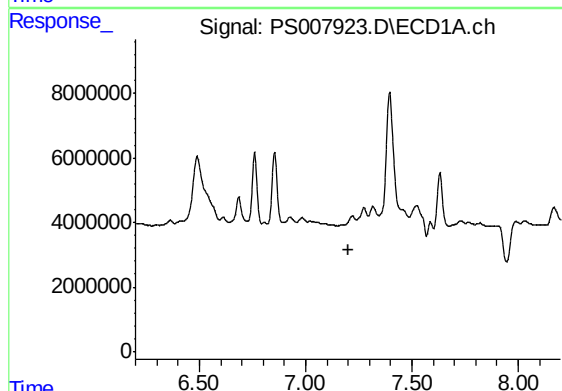


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

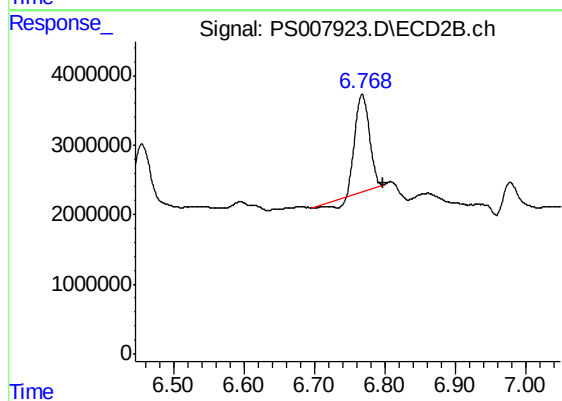

#11 2,4,5-TP (SILVEX)


R.T.: 6.768 min
Delta R.T.: -0.030 min
Response: 18506428
Conc: 4.32 ng/ml

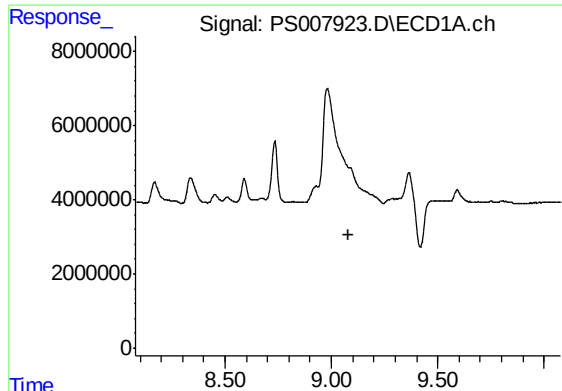

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.078 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB125293TB

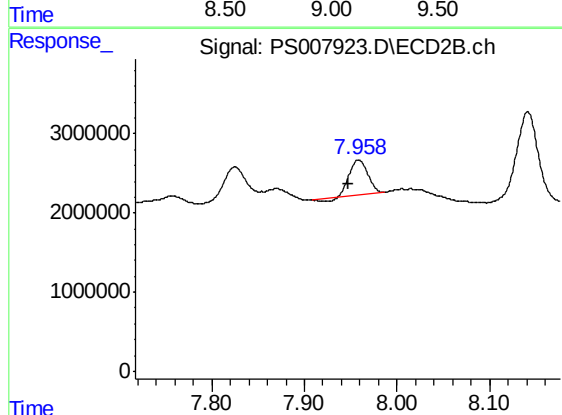


#14 DINOSEB

R.T.: 7.959 min
Delta R.T.: 0.012 min
Response: 6021414
Conc: 1.84 ng/ml

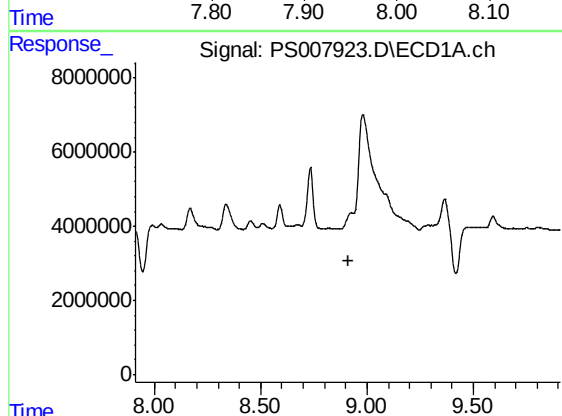

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.911 min
Response: 0
Conc: N.D.

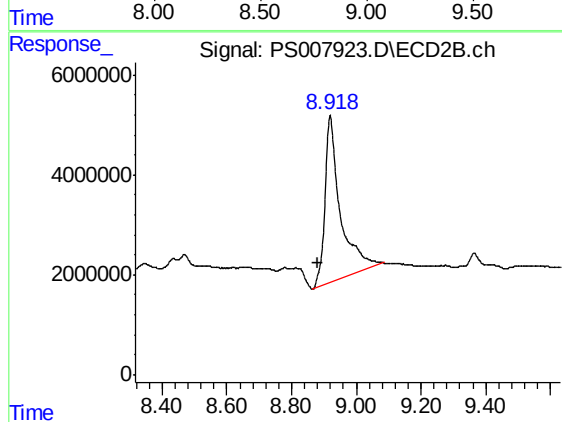

#15 Picloram

R.T.: 8.919 min
Delta R.T.: 0.040 min
Response: 111180044
Conc: 18.00 ng/ml