

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 18:35
 Operator : SM\AJ
 Sample : K6112-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OK-02-120419

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:24:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.425	5.152	752.8E6	423.6E6	481.222	545.962
Target Compounds							
2) T	3,5-DICHL...	0.000	4.486	0 91728169		N.D.	88.637
3) T	4-Nitroph...	0.000	4.830	0 22792055		N.D.	50.330
9) T	2,4-D	6.476	0.000	85070712	0	52.879	N.D. #
11) T	2,4,5-TP ...	0.000	6.749	0 75046591		N.D.	17.498
14) T	DINOSEB	0.000	7.981	0 26476801		N.D.	8.094
15) T	Picloram	8.892	8.904	82453046	1821274	6.819	<MDL #
16) T	DCPA	0.000	8.904	0 1821274		N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 18:35
Operator : SM\AJ
Sample : K6112-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
OK-02-120419

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:24:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

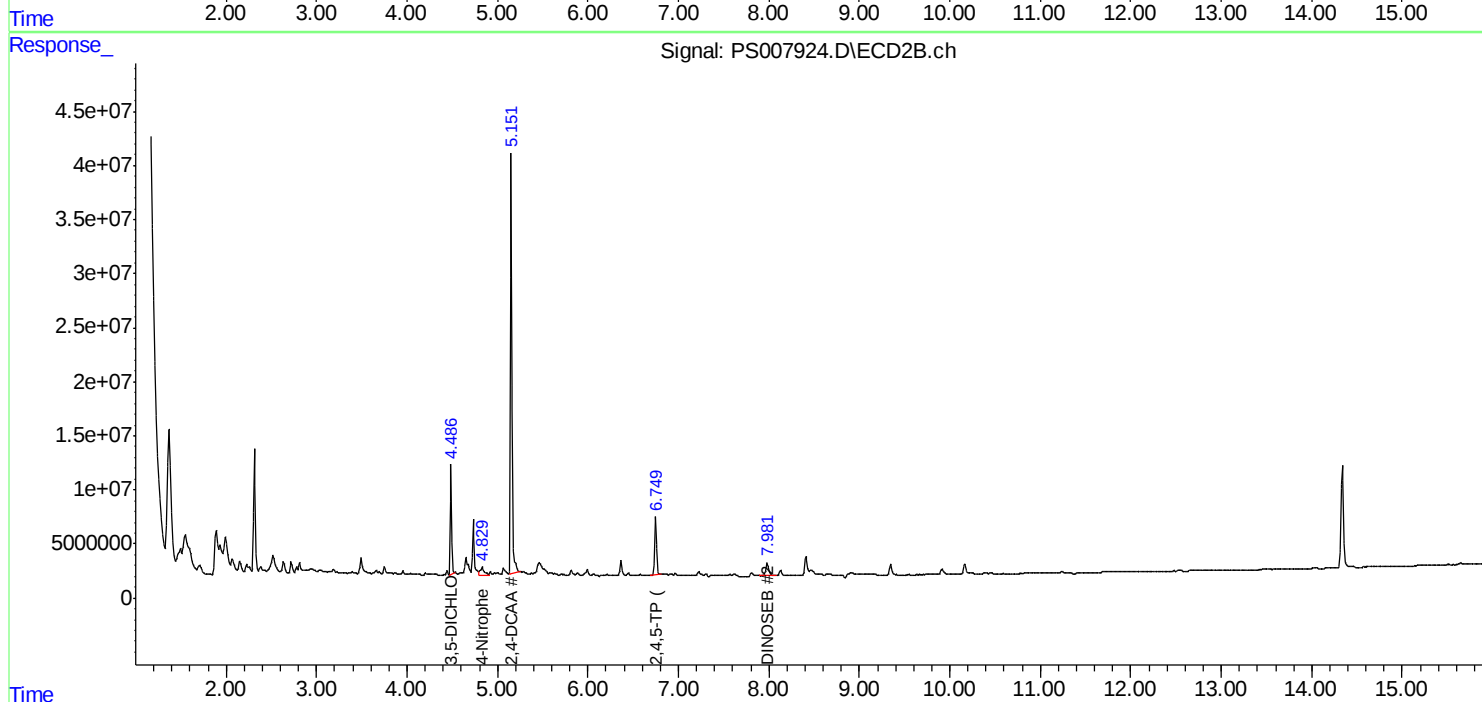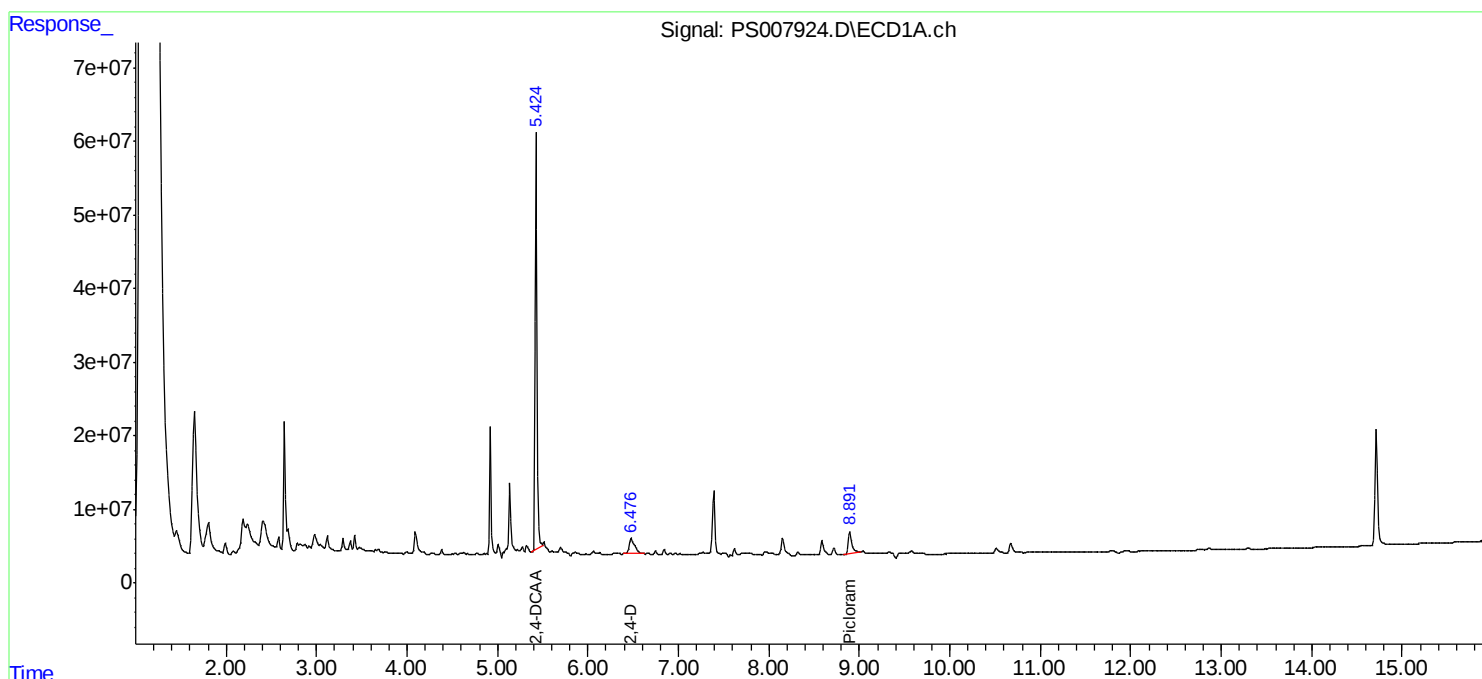


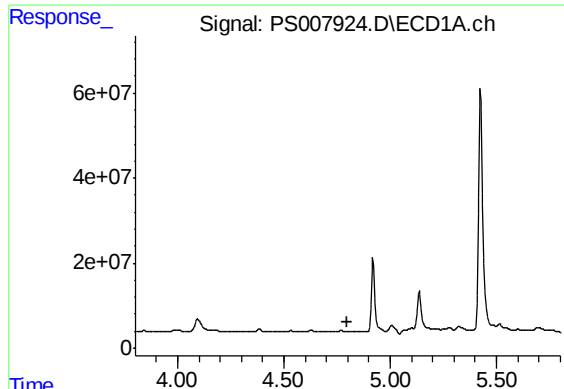

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-02-120419

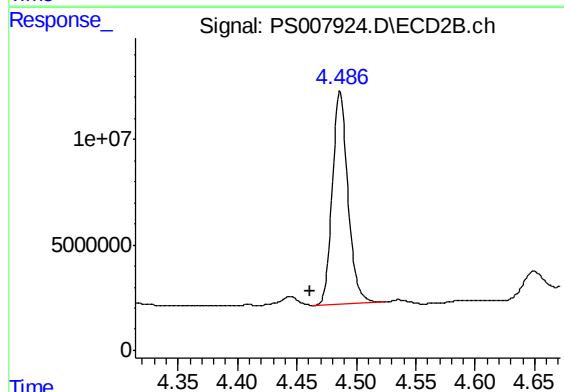


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.486 min
Delta R.T.: 0.025 min
Response: 91728169
Conc: 88.64 ng/ml

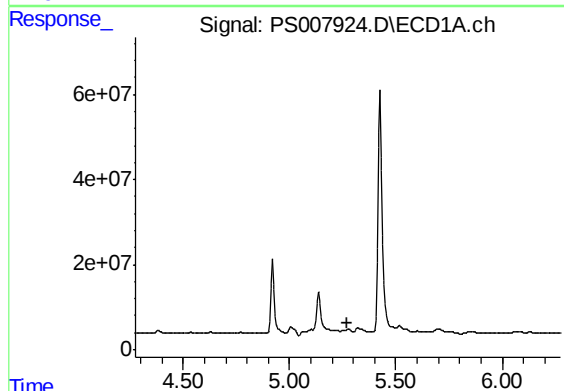


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

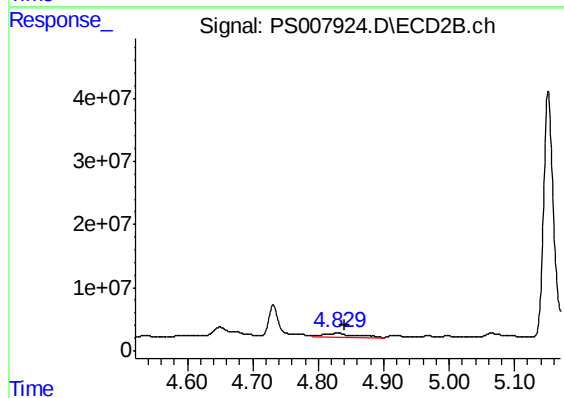

#3 4-Nitrophenol


R.T.: 4.830 min
Delta R.T.: -0.011 min
Response: 22792055
Conc: 50.33 ng/ml

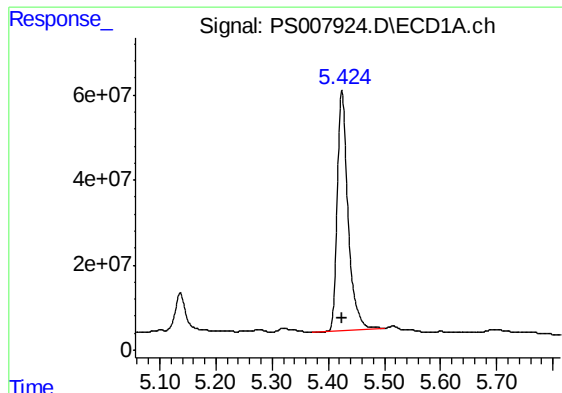

#4 2,4-DCAA


R.T.: 5.425 min
Delta R.T.: 0.000 min
Response: 752790932
Conc: 481.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-02-120419

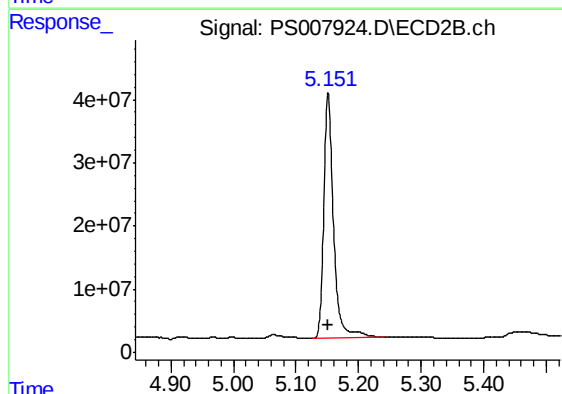


#4 2,4-DCAA

R.T.: 5.152 min
Delta R.T.: 0.000 min
Response: 423621489
Conc: 545.96 ng/ml

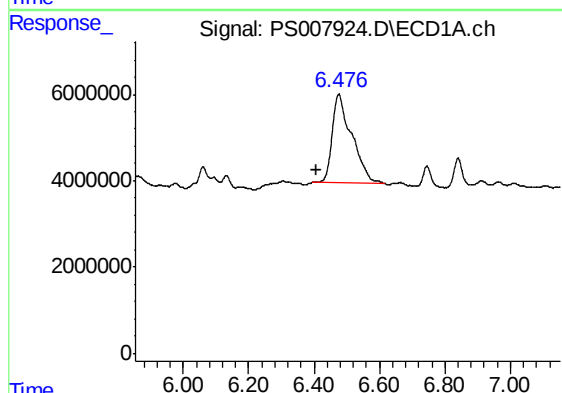


#9 2,4-D

R.T.: 6.476 min
Delta R.T.: 0.068 min
Response: 85070712
Conc: 52.88 ng/ml

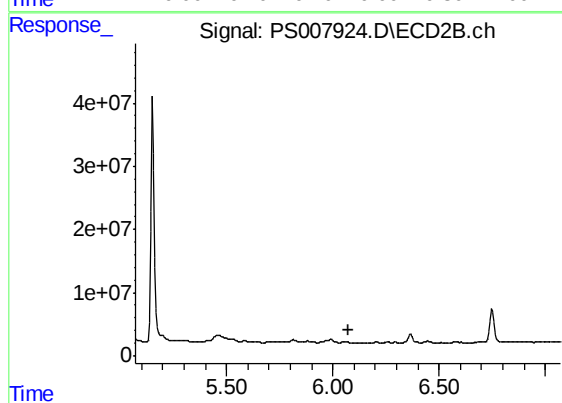

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

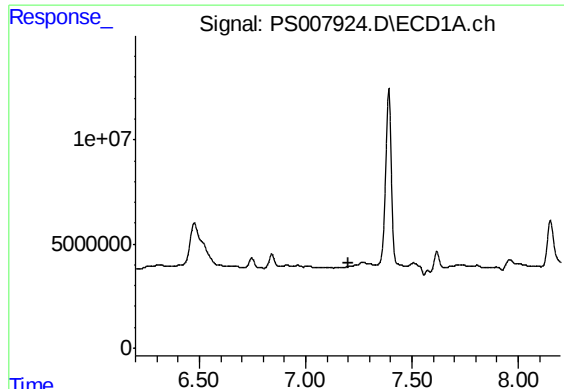

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-02-120419

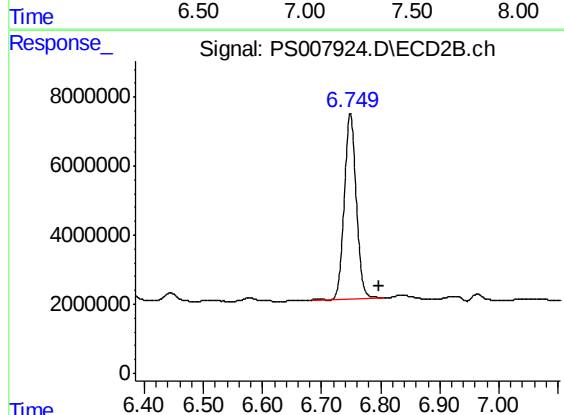


#11 2,4,5-TP (SILVEX)

R.T.: 6.749 min
Delta R.T.: -0.049 min
Response: 75046591
Conc: 17.50 ng/ml

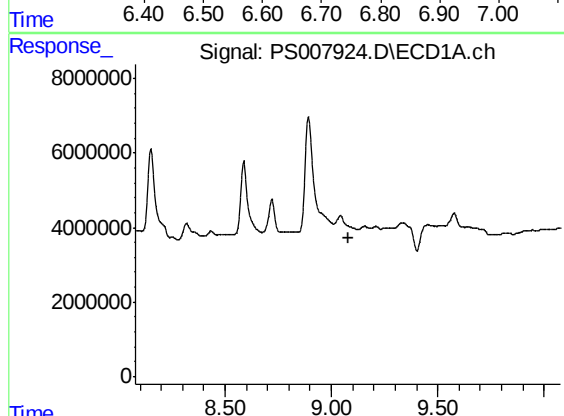


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.078 min
Response: 0
Conc: N.D.

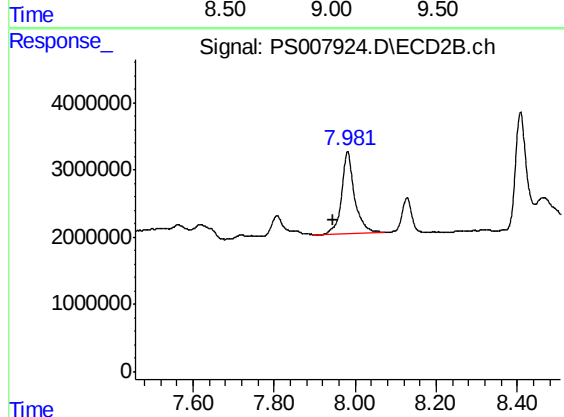

#14 DINOSEB


R.T.: 7.981 min
Delta R.T.: 0.034 min
Response: 26476801
Conc: 8.09 ng/ml

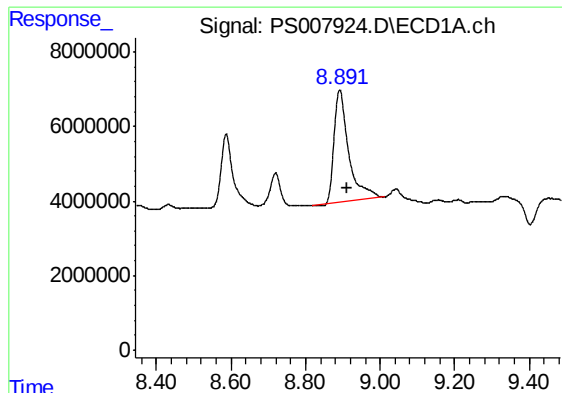

#15 Picloram

R.T.: 8.892 min
Delta R.T.: -0.019 min
Response: 82453046
Conc: 6.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-02-120419

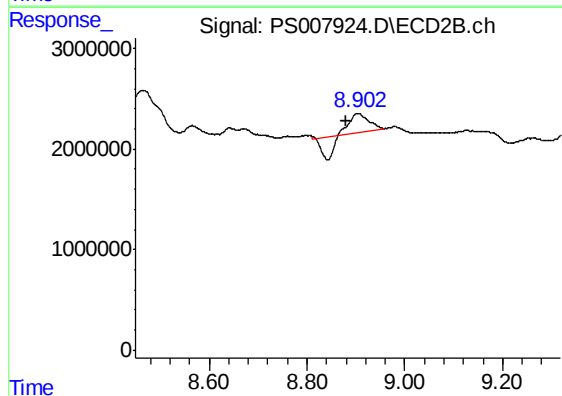

#15 Picloram

R.T.: 8.904 min
Delta R.T.: 0.024 min
Response: 1821274
Conc: N.D.