

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007926.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 19:19
 Operator : SM\AJ
 Sample : K6135-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-34

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:24:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.424	5.151	658.2E6	345.1E6	420.734	444.825
Target Compounds							
1) T	Dalapon	1.987	0.000	39369915	0	19.305	N.D. #
2) T	3,5-DICHL...	0.000	4.443	0	5151373	N.D.	4.978
3) T	4-Nitroph...	5.337	4.828	56014145	19668517	73.696	43.433 #
5) T	DICAMBA	5.514	0.000	54324412	0	9.548	N.D. #
9) T	2,4-D	6.475	0.000	85647628	0	53.237	N.D. #
11) T	2,4,5-TP ...	0.000	6.748	0	65393922	N.D.	15.248
14) T	DINOSEB	0.000	7.979	0	28887956	N.D.	8.831
15) T	Picloram	8.887	0.000	87010374	0	7.196	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007926.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 19:19
Operator : SM\AJ
Sample : K6135-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-34

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:24:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

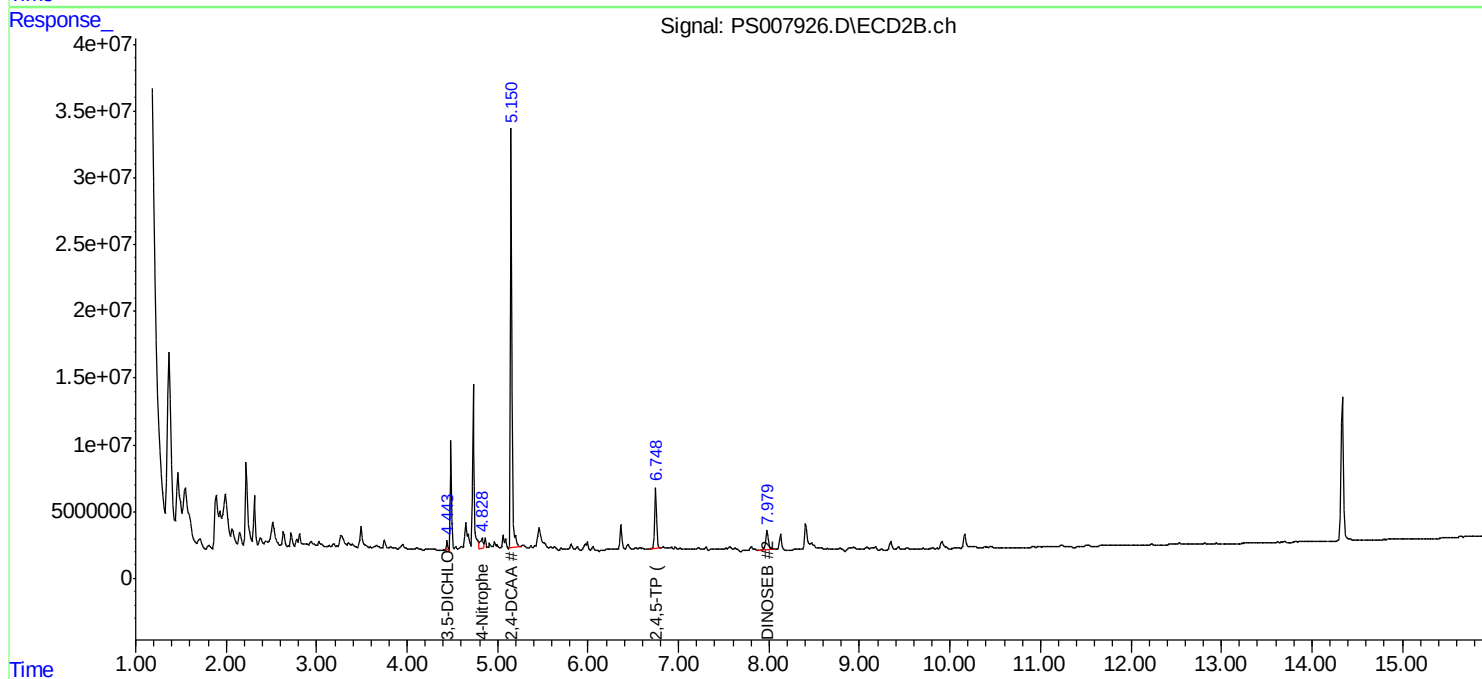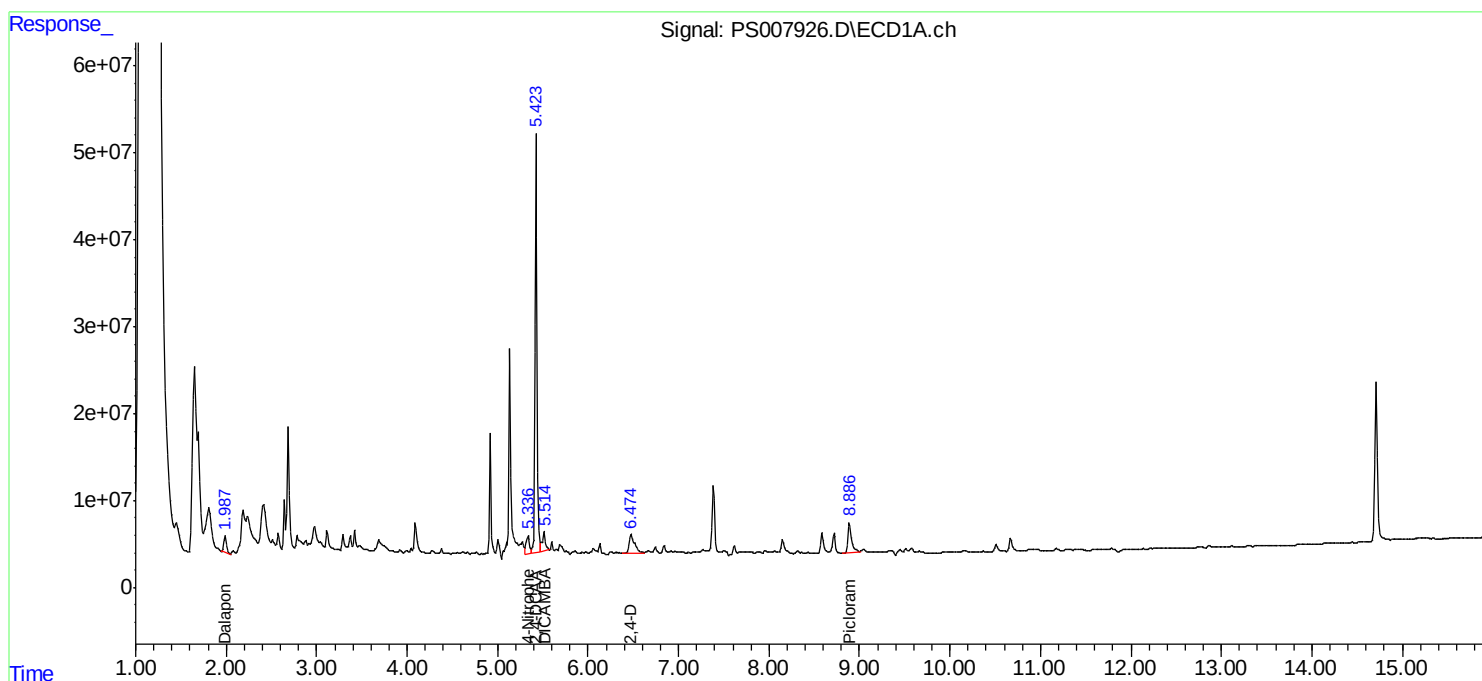


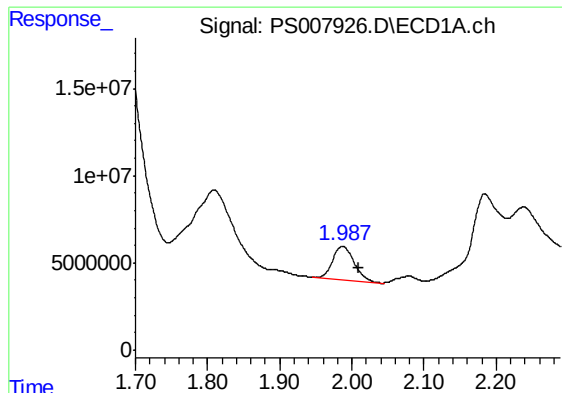

#1 Dalapon


R.T.: 1.987 min
Delta R.T.: -0.023 min
Response: 39369915
Conc: 19.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-34

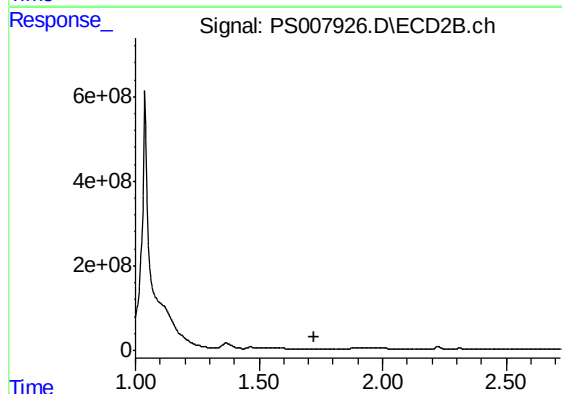


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.721 min
Response: 0
Conc: N.D.

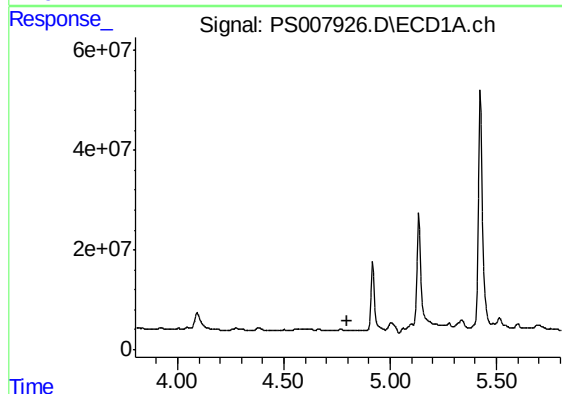


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

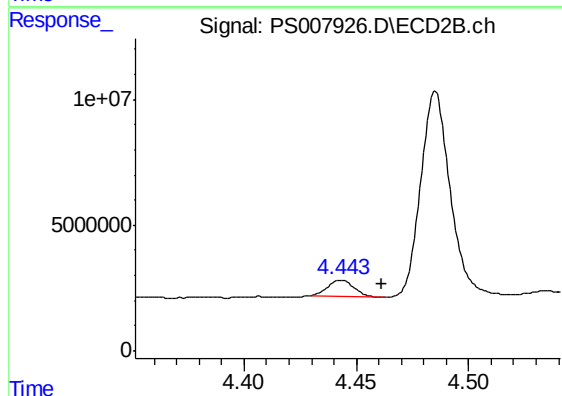

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.443 min
Delta R.T.: -0.018 min
Response: 5151373
Conc: 4.98 ng/ml

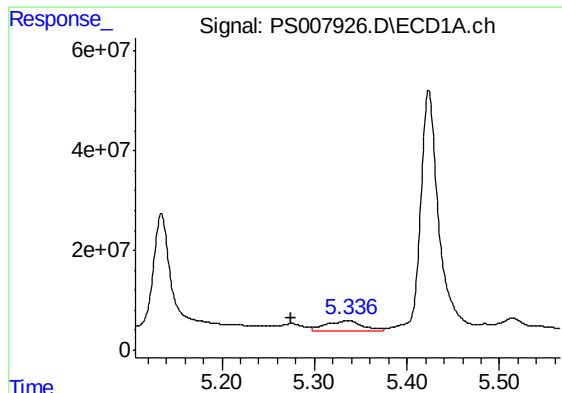

#3 4-Nitrophenol


R.T.: 5.337 min
Delta R.T.: 0.062 min
Response: 56014145
Conc: 73.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-34

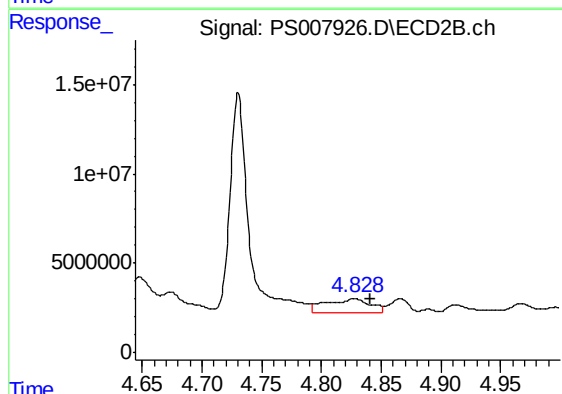


#3 4-Nitrophenol

R.T.: 4.828 min
Delta R.T.: -0.013 min
Response: 19668517
Conc: 43.43 ng/ml

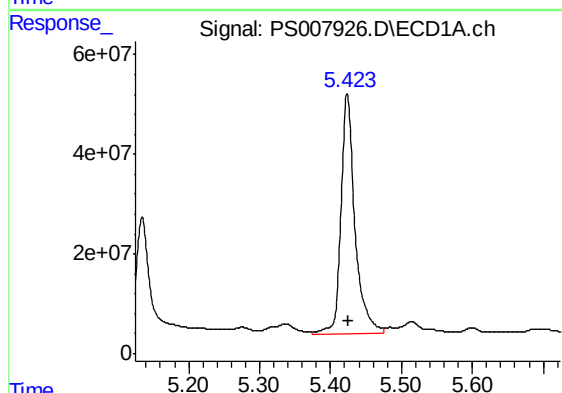


#4 2,4-DCAA

R.T.: 5.424 min
Delta R.T.: -0.001 min
Response: 658167540
Conc: 420.73 ng/ml

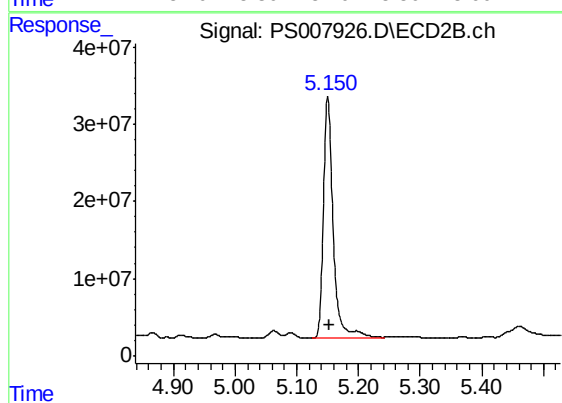

#4 2,4-DCAA


R.T.: 5.151 min
Delta R.T.: -0.001 min
Response: 345147600
Conc: 444.82 ng/ml

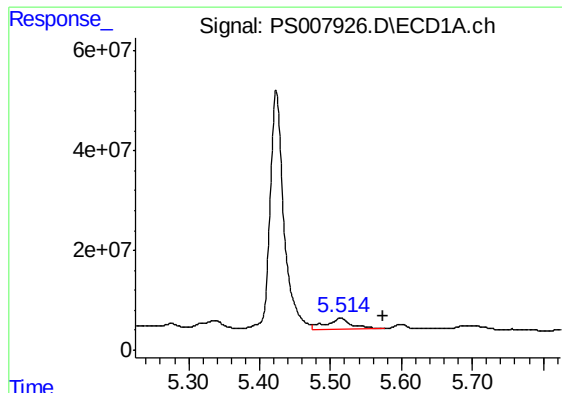

#5 DICAMBA


R.T.: 5.514 min
Delta R.T.: -0.061 min
Response: 54324412
Conc: 9.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-34

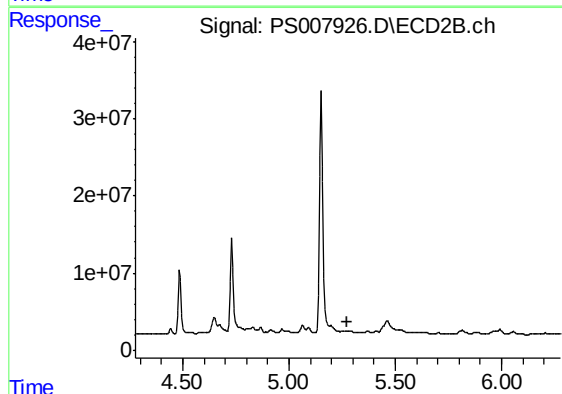


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

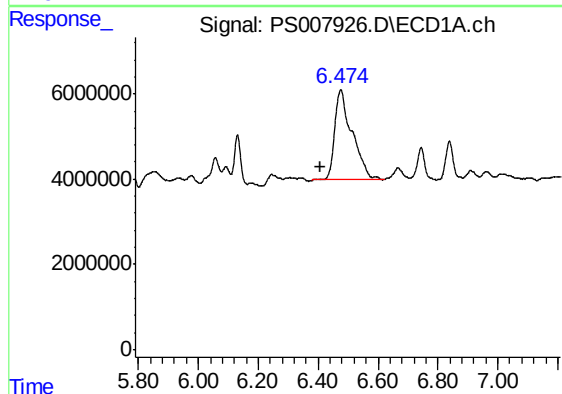


#9 2,4-D

R.T.: 6.475 min
Delta R.T.: 0.067 min
Response: 85647628
Conc: 53.24 ng/ml

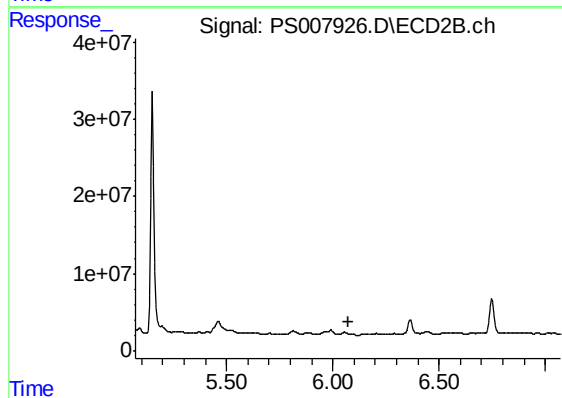

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

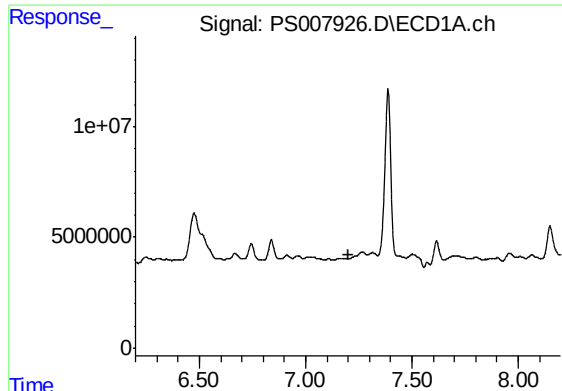

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-34

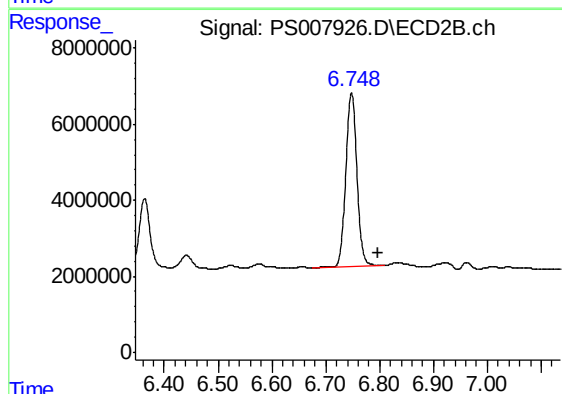


#11 2,4,5-TP (SILVEX)

R.T.: 6.748 min
Delta R.T.: -0.050 min
Response: 65393922
Conc: 15.25 ng/ml

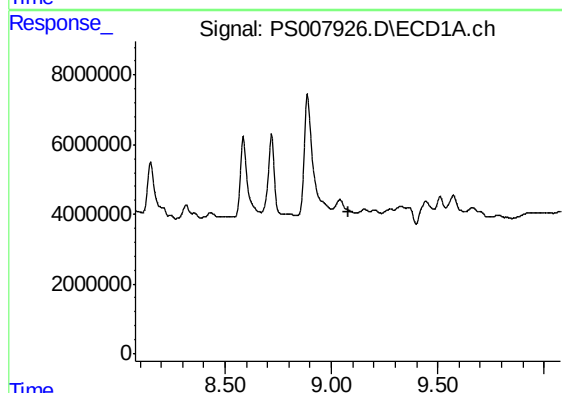


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.078 min
Response: 0
Conc: N.D.

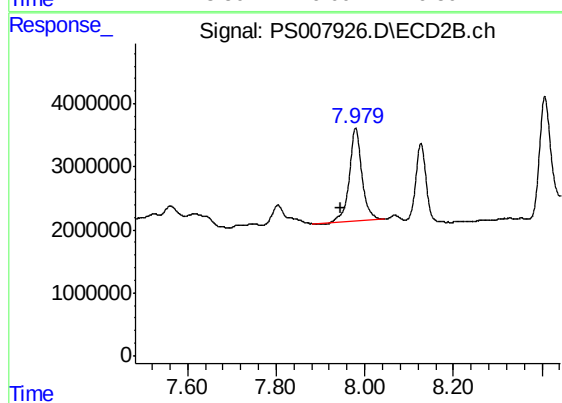

#14 DINOSEB


R.T.: 7.979 min
Delta R.T.: 0.032 min
Response: 28887956
Conc: 8.83 ng/ml

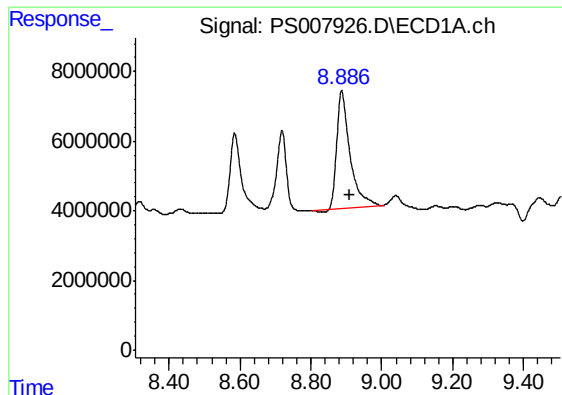

#15 Picloram

R.T.: 8.887 min
Delta R.T.: -0.024 min
Response: 87010374
Conc: 7.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-34

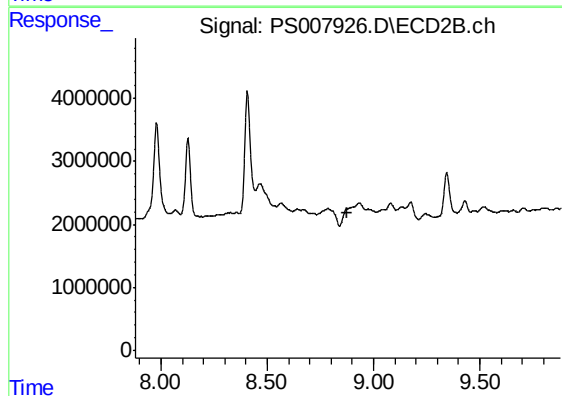

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.879 min
Response: 0
Conc: N.D.