

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 19:41
 Operator : SM\AJ
 Sample : K6135-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-35

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:25:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.426	5.153	870.1E6	439.3E6	556.197	566.134
Target Compounds							
1) T	Dalapon	1.990	1.712	34716087	35050581	17.023	29.509 #
2) T	3,5-DICHL...	0.000	4.446	0	7971147	N.D.	7.703
3) T	4-Nitroph...	5.278	4.830	37033778	21558886	48.724	47.607
5) T	DICAMBA	5.602	0.000	24845594	0	4.367	N.D. #
8) T	DICHLORPROP	6.133	5.815	40894579	6407759	28.741	8.939 #
9) T	2,4-D	0.000	6.057	0	8596014	N.D.	9.728
10) T	Pentachlo...	0.000	6.442	0	6801285	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.750	0	75568485	N.D.	17.620
14) T	DINOSEB	0.000	7.979	0	15936991	N.D.	4.872
15) T	Picloram	8.890	0.000	67311950	0	5.567	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 19:41
Operator : SM\AJ
Sample : K6135-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
COMP-35

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:25:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

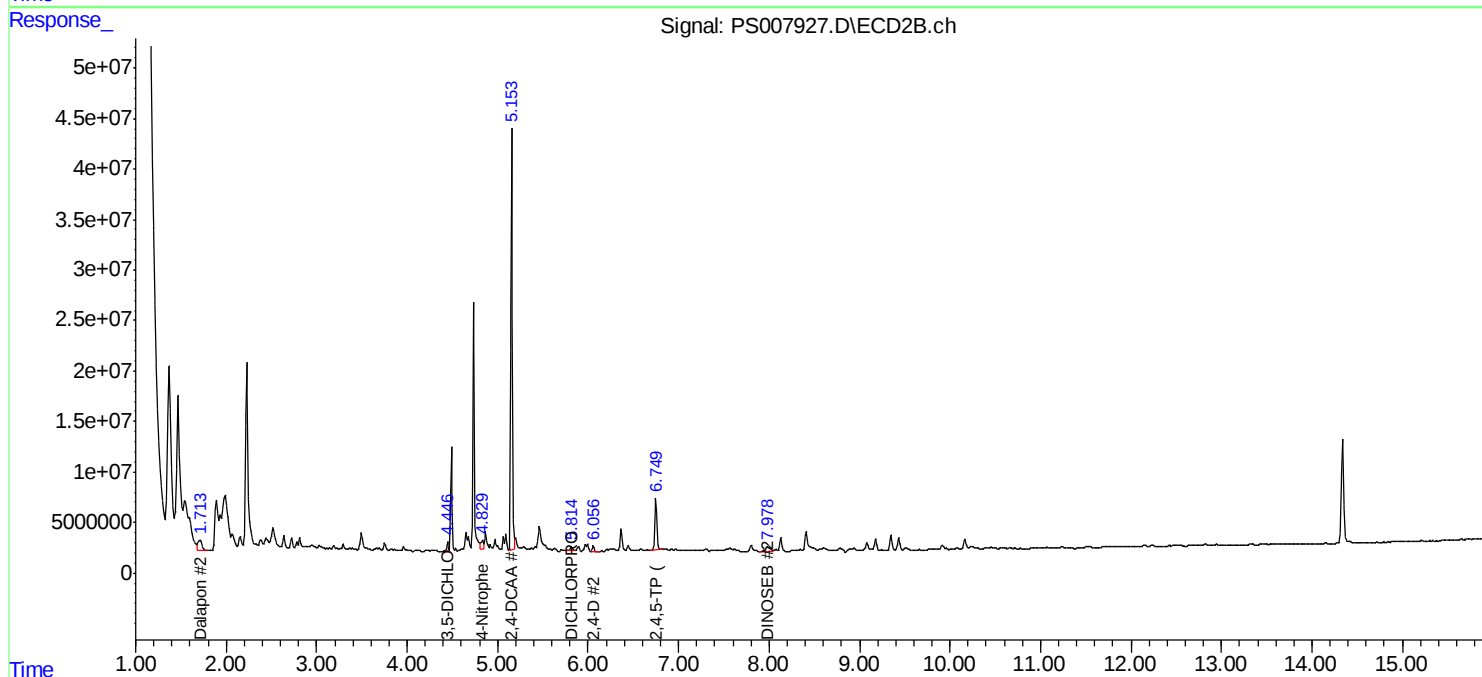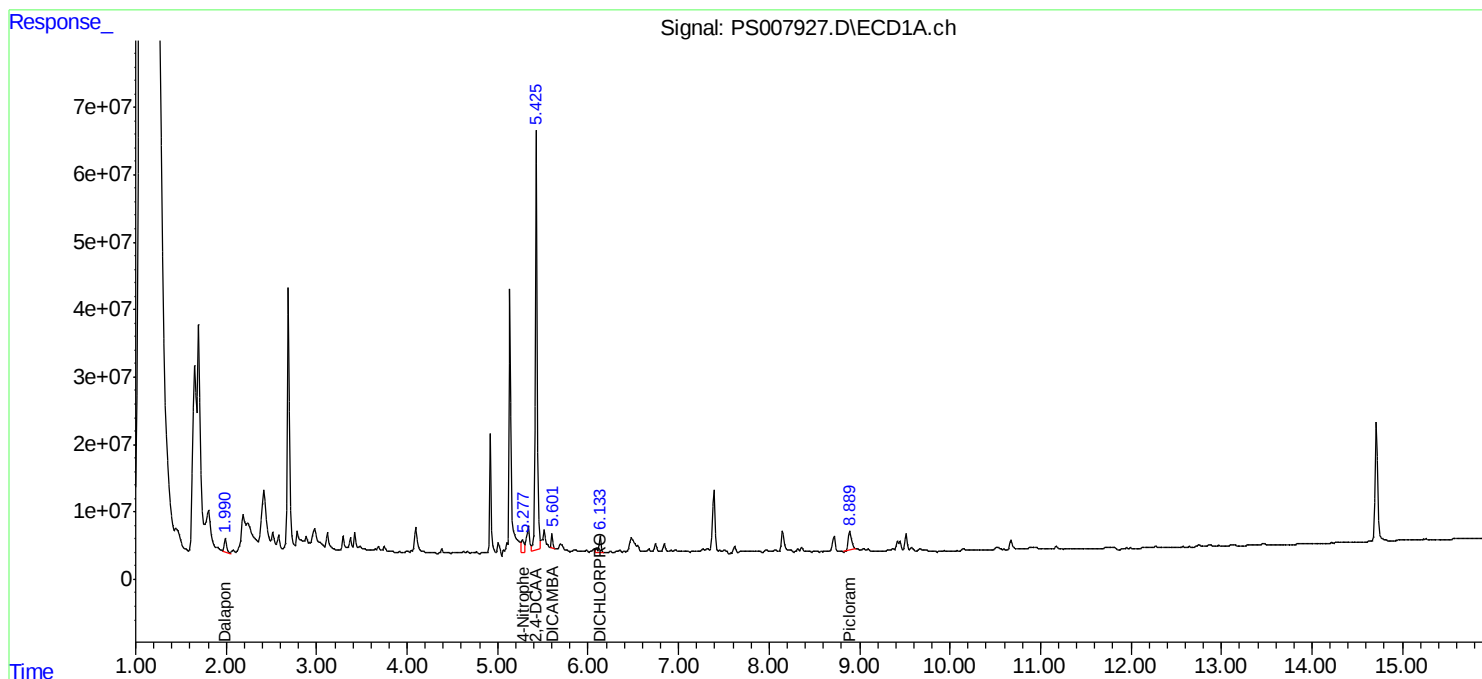


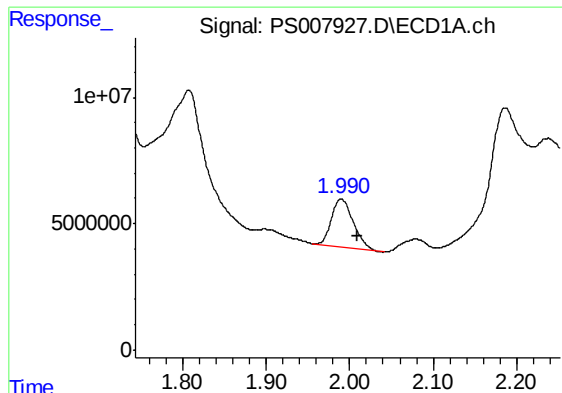

#1 Dalapon


R.T.: 1.990 min
Delta R.T.: -0.020 min
Response: 34716087
Conc: 17.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-35

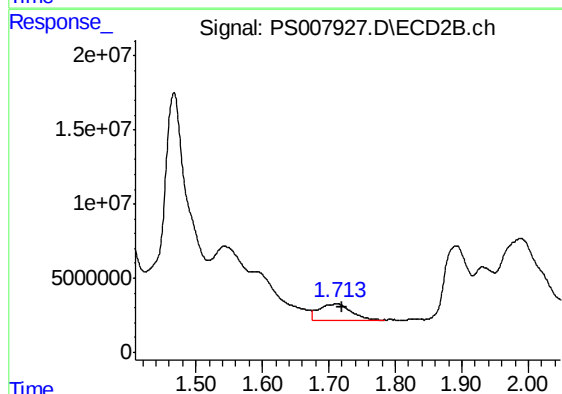


#1 Dalapon

R.T.: 1.712 min
Delta R.T.: -0.008 min
Response: 35050581
Conc: 29.51 ng/ml

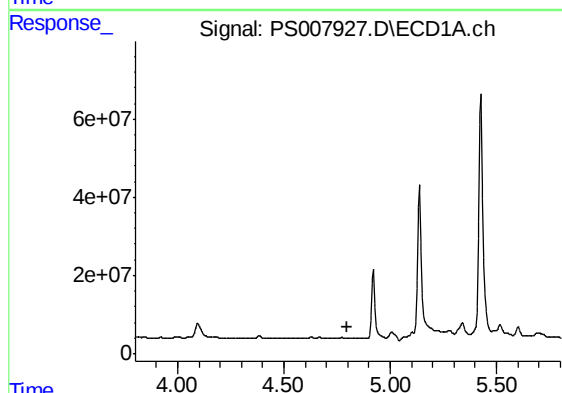


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

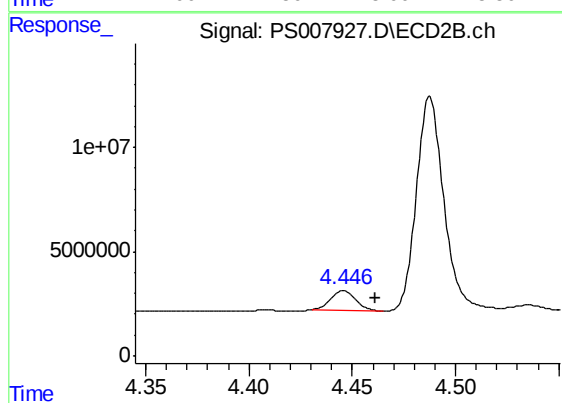

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.446 min
Delta R.T.: -0.015 min
Response: 7971147
Conc: 7.70 ng/ml

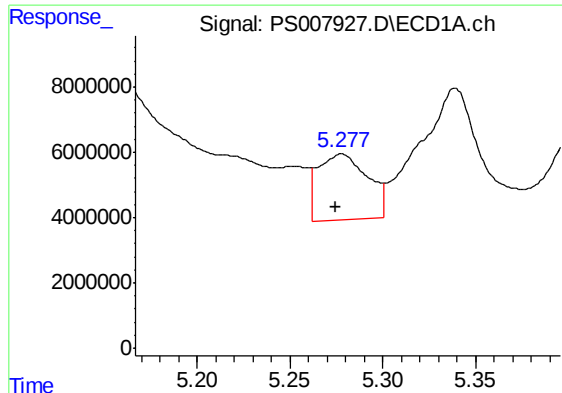

#3 4-Nitrophenol


R.T.: 5.278 min
Delta R.T.: 0.003 min
Response: 37033778
Conc: 48.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-35

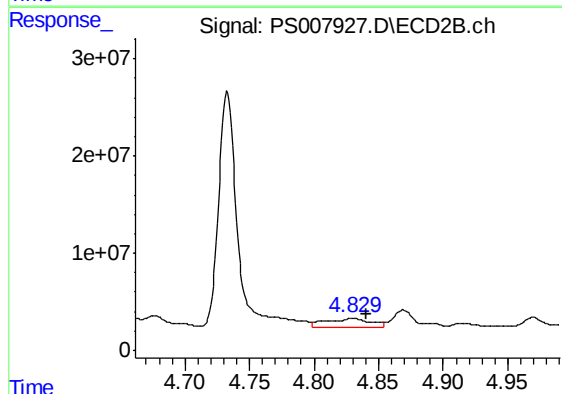


#3 4-Nitrophenol

R.T.: 4.830 min
Delta R.T.: -0.011 min
Response: 21558886
Conc: 47.61 ng/ml

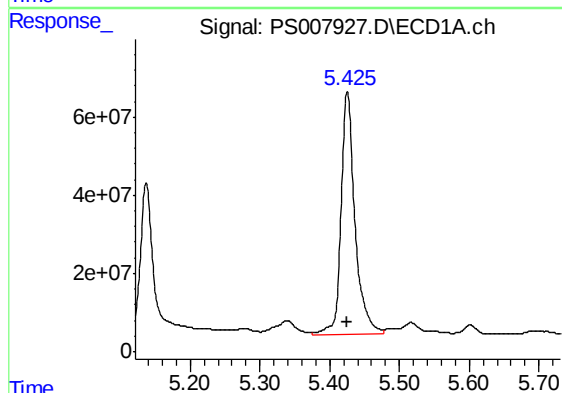


#4 2,4-DCAA

R.T.: 5.426 min
Delta R.T.: 0.000 min
Response: 870077194
Conc: 556.20 ng/ml

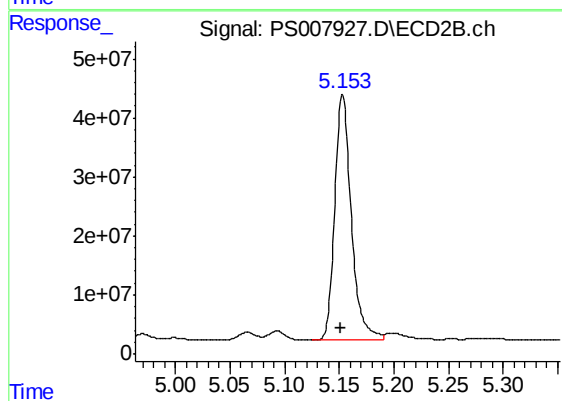

#4 2,4-DCAA


R.T.: 5.153 min
Delta R.T.: 0.001 min
Response: 439273723
Conc: 566.13 ng/ml

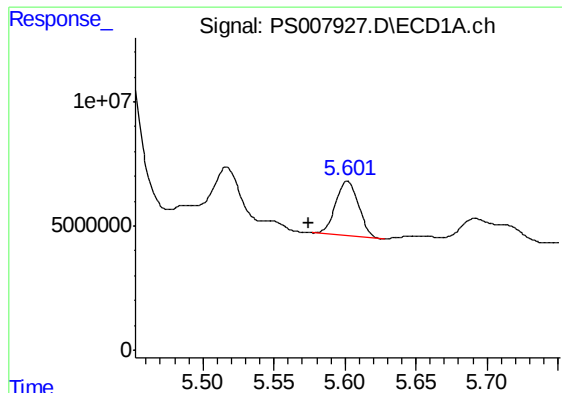

#5 DICAMBA


R.T.: 5.602 min
Delta R.T.: 0.027 min
Response: 24845594
Conc: 4.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-35

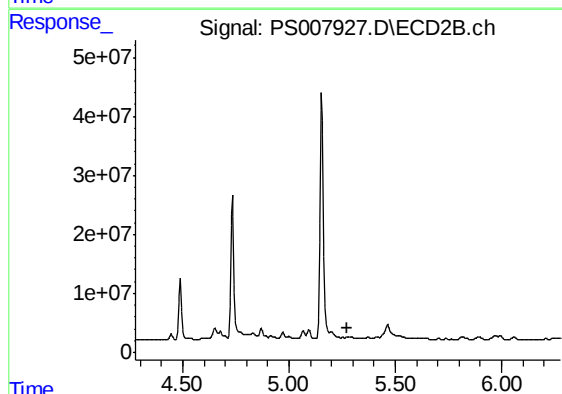


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

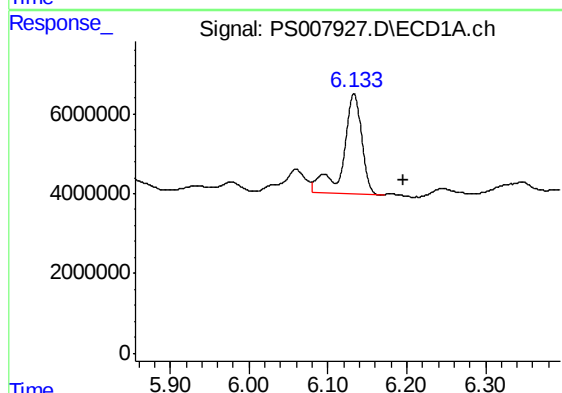


#8 DICHLORPROP

R.T.: 6.133 min
Delta R.T.: -0.063 min
Response: 40894579
Conc: 28.74 ng/ml

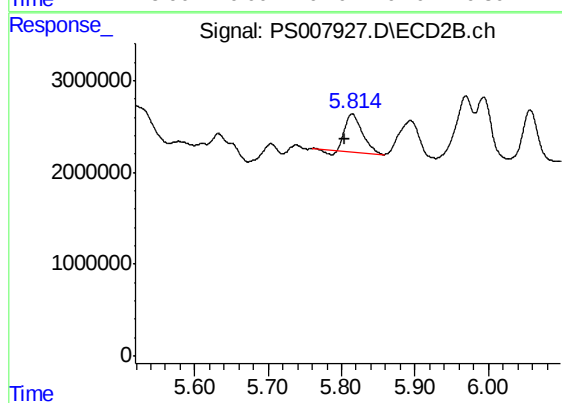

#8 DICHLORPROP


R.T.: 5.815 min
Delta R.T.: 0.010 min
Response: 6407759
Conc: 8.94 ng/ml

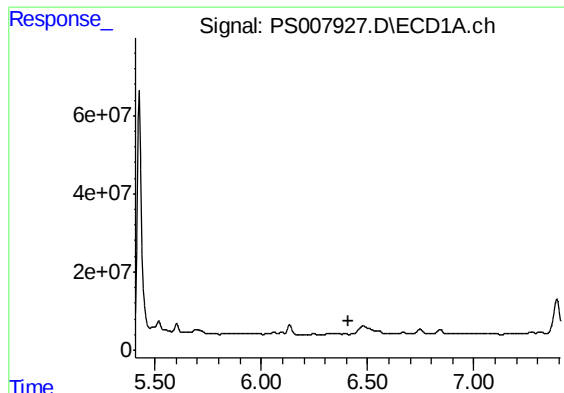

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-35

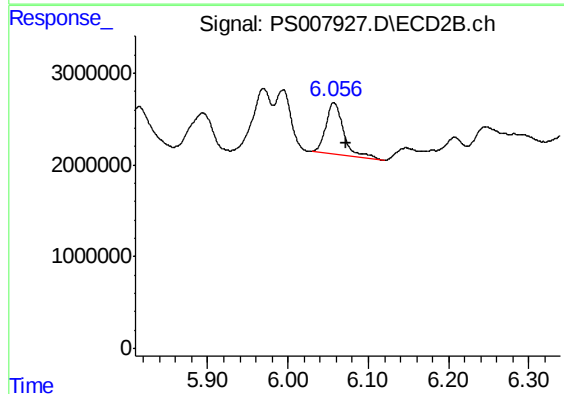


#9 2,4-D

R.T.: 6.057 min
Delta R.T.: -0.014 min
Response: 8596014
Conc: 9.73 ng/ml

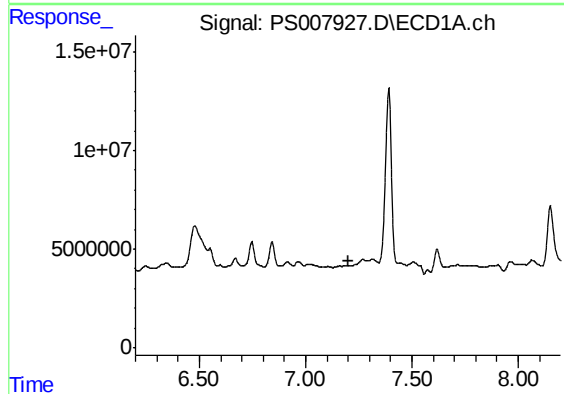


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

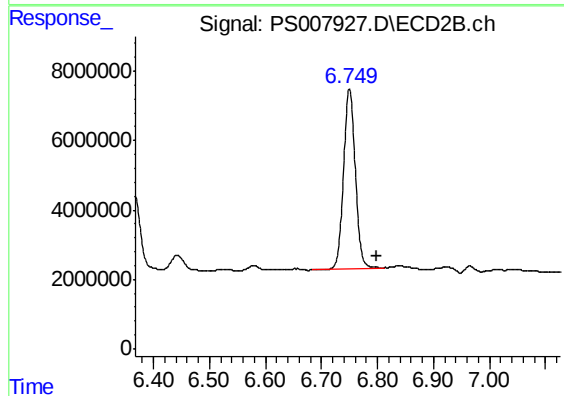

#11 2,4,5-TP (SILVEX)


R.T.: 6.750 min
Delta R.T.: -0.048 min
Response: 75568485
Conc: 17.62 ng/ml

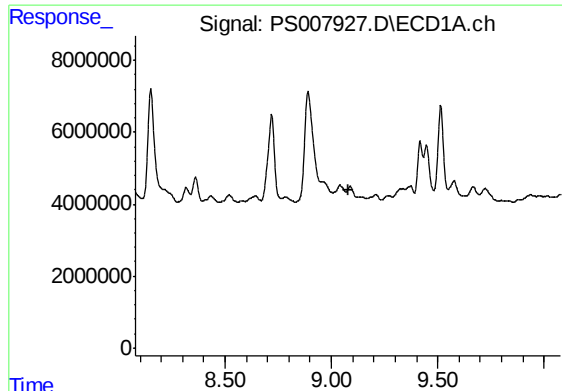

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.078 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-35

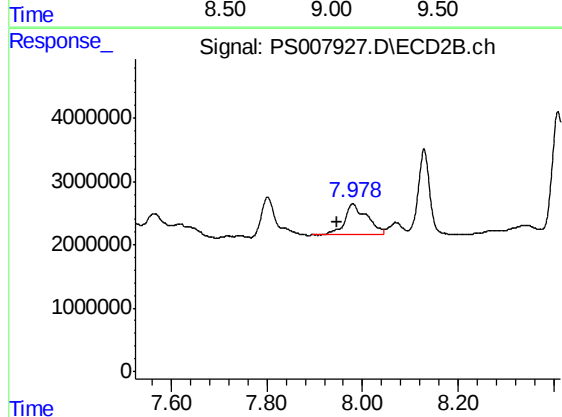


#14 DINOSEB

R.T.: 7.979 min
Delta R.T.: 0.032 min
Response: 15936991
Conc: 4.87 ng/ml

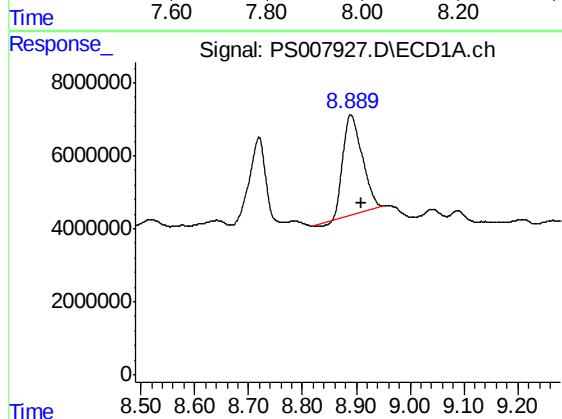

#15 Picloram

R.T.: 8.890 min
Delta R.T.: -0.021 min
Response: 67311950
Conc: 5.57 ng/ml

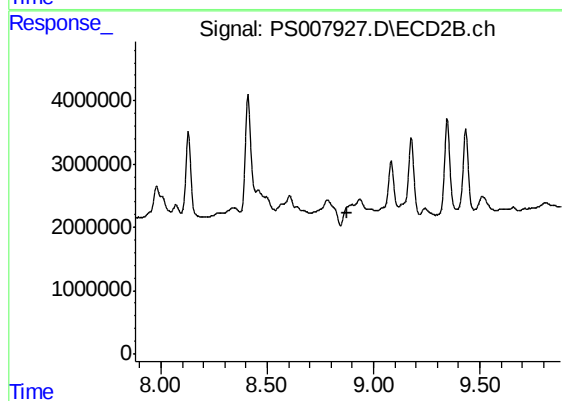

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.879 min
Response: 0
Conc: N.D.