

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007929.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 20:25
 Operator : SM\AJ
 Sample : K6141-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CMJ-01-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:25:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.425	5.152	736.5E6	417.9E6	470.811	538.555
Target Compounds							
2) T	3,5-DICHL...	0.000	4.487	0 86130044		N.D.	83.227
3) T	4-Nitroph...	0.000	4.830	0 22061881		N.D.	48.718
9) T	2,4-D	6.477	0.000	81799729	0	50.845	N.D. #
11) T	2,4,5-TP ...	0.000	6.750	0 66189491		N.D.	15.433
14) T	DINOSEB	0.000	7.982	0 18997340		N.D.	5.807
15) T	Picloram	8.893	0.000	63179629	0	5.225	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007929.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 20:25
Operator : SM\AJ
Sample : K6141-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CMJ-01-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:25:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

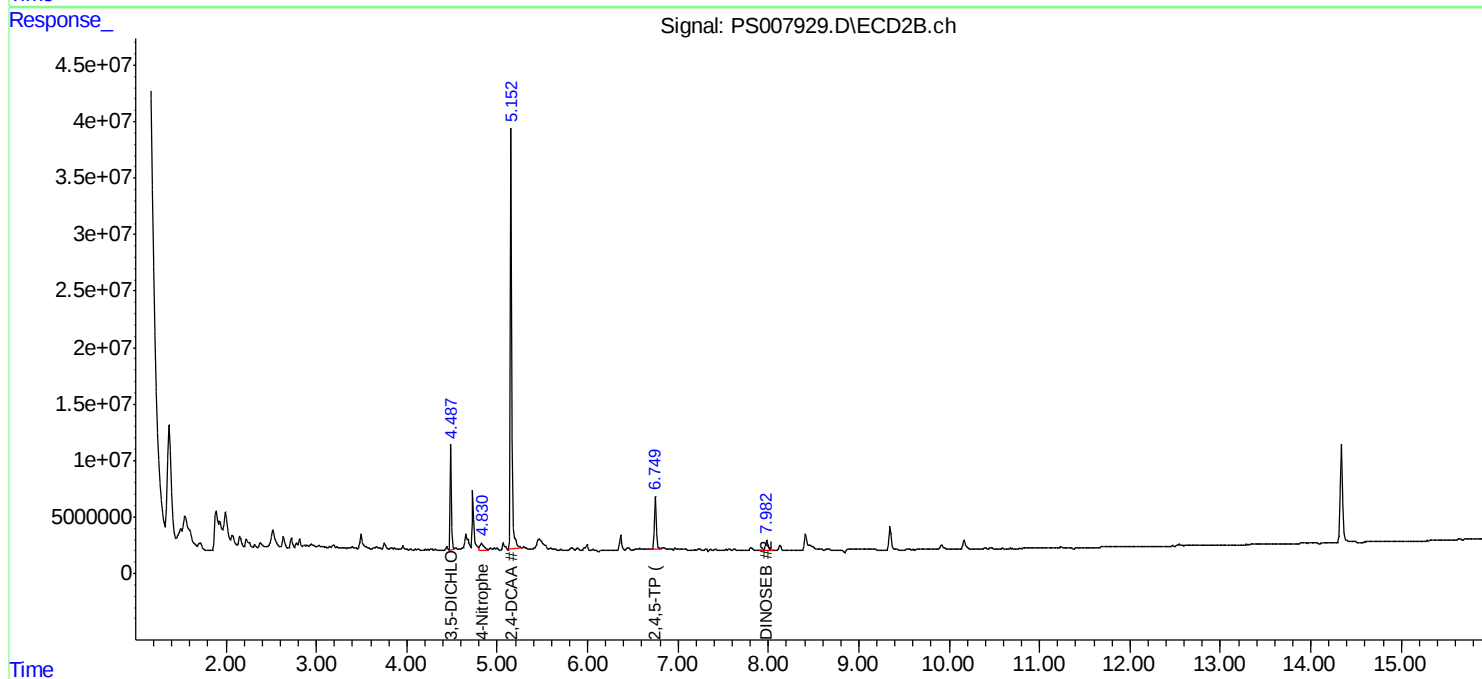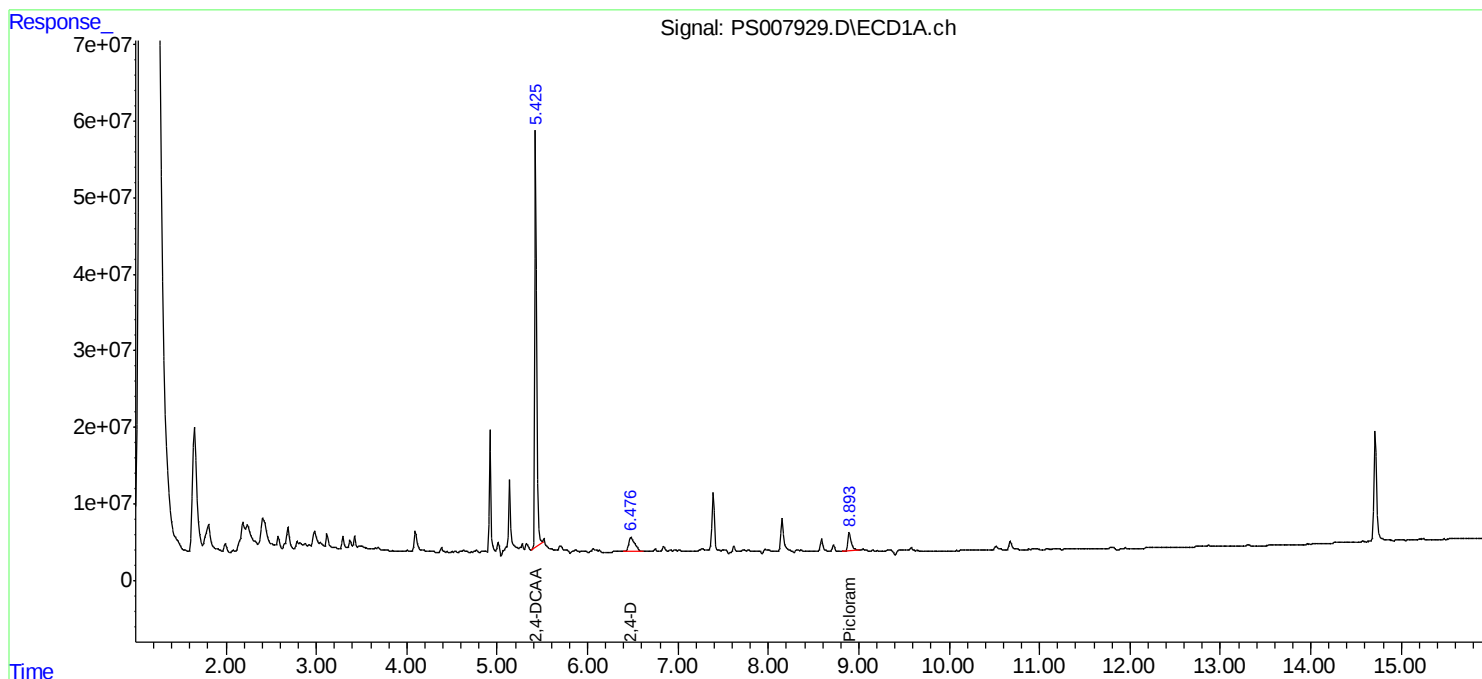


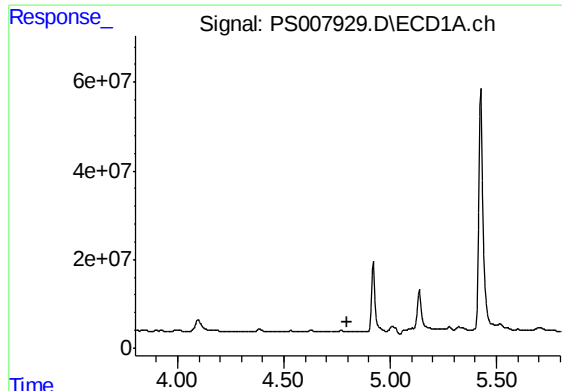

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CMJ-01-COMP

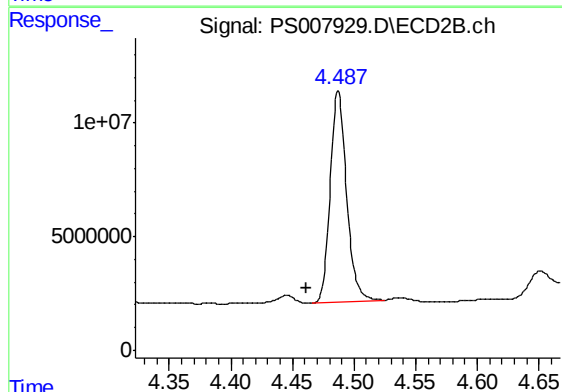


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.487 min
Delta R.T.: 0.026 min
Response: 86130044
Conc: 83.23 ng/ml

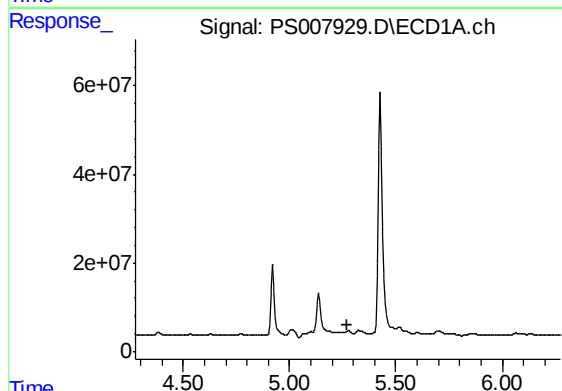


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

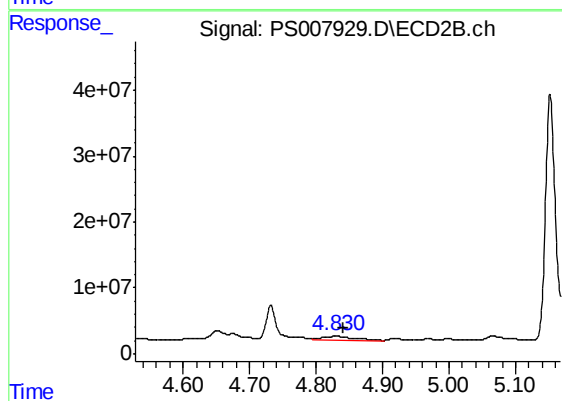

#3 4-Nitrophenol


R.T.: 4.830 min
Delta R.T.: -0.011 min
Response: 22061881
Conc: 48.72 ng/ml

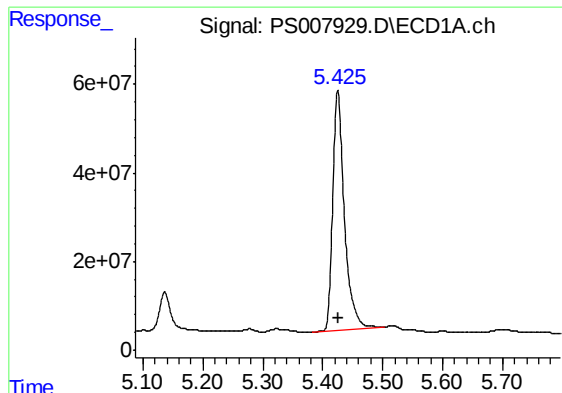

#4 2,4-DCAA


R.T.: 5.425 min
Delta R.T.: 0.000 min
Response: 736505017
Conc: 470.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
CMJ-01-COMP

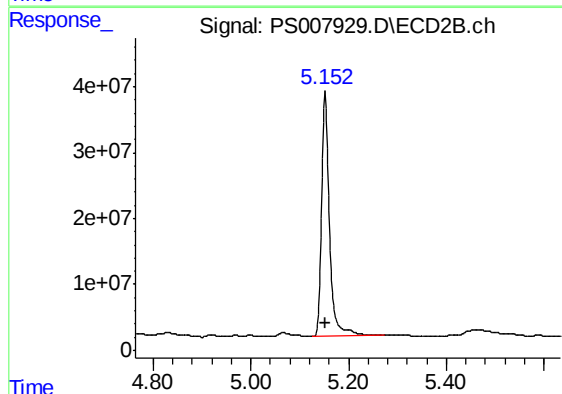


#4 2,4-DCAA

R.T.: 5.152 min
Delta R.T.: 0.000 min
Response: 417874553
Conc: 538.56 ng/ml

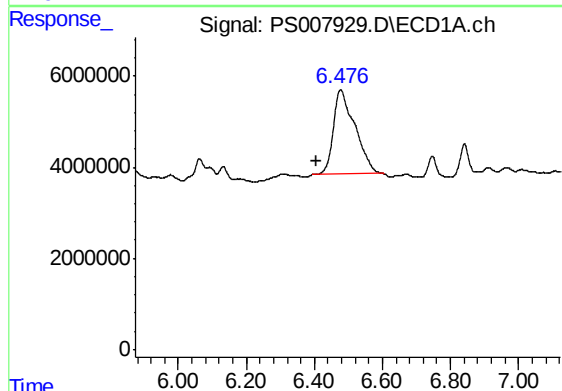


#9 2,4-D

R.T.: 6.477 min
Delta R.T.: 0.069 min
Response: 81799729
Conc: 50.85 ng/ml

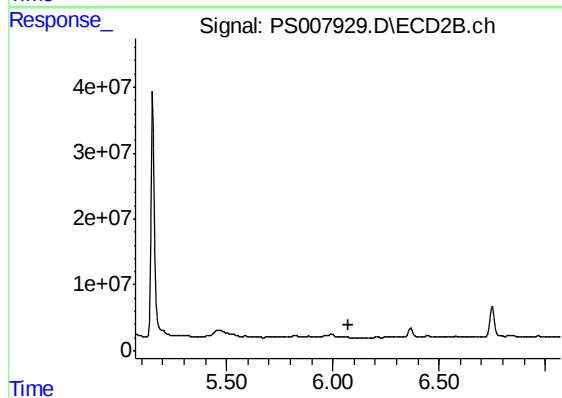

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

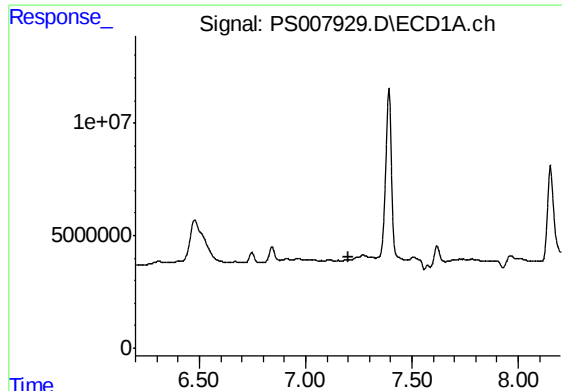

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CMJ-01-COMP

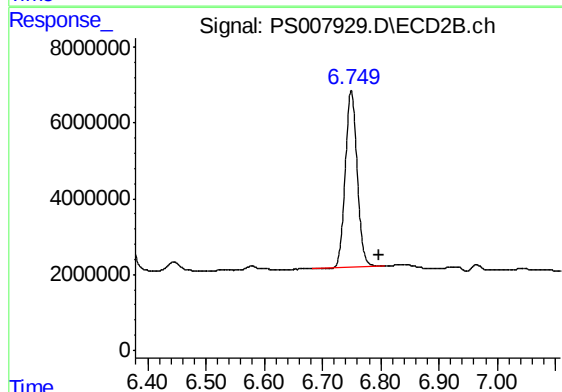


#11 2,4,5-TP (SILVEX)

R.T.: 6.750 min
Delta R.T.: -0.048 min
Response: 66189491
Conc: 15.43 ng/ml

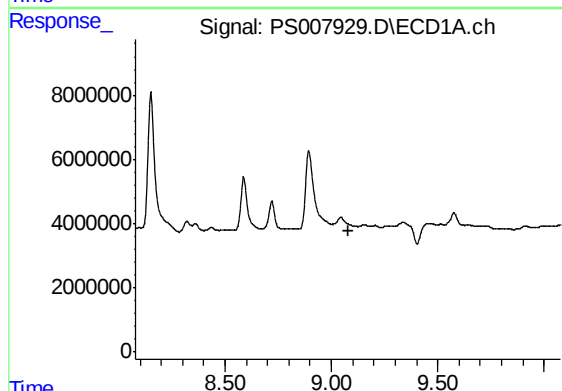


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.078 min
Response: 0
Conc: N.D.

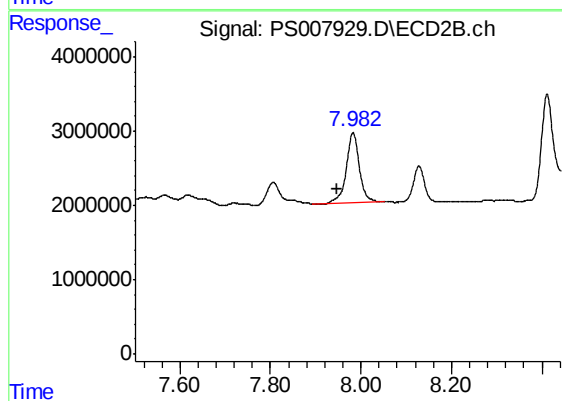

#14 DINOSEB


R.T.: 7.982 min
Delta R.T.: 0.035 min
Response: 18997340
Conc: 5.81 ng/ml

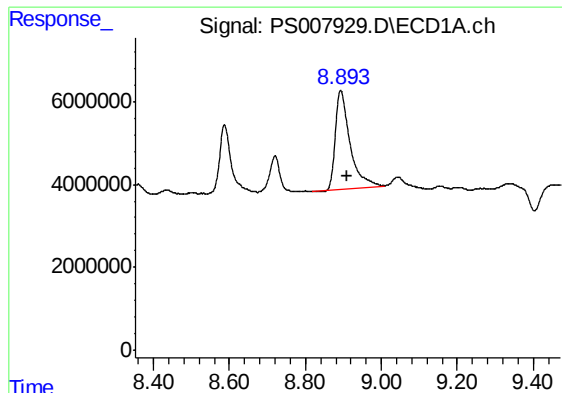

#15 Picloram

R.T.: 8.893 min
Delta R.T.: -0.017 min
Response: 63179629
Conc: 5.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
CMJ-01-COMP

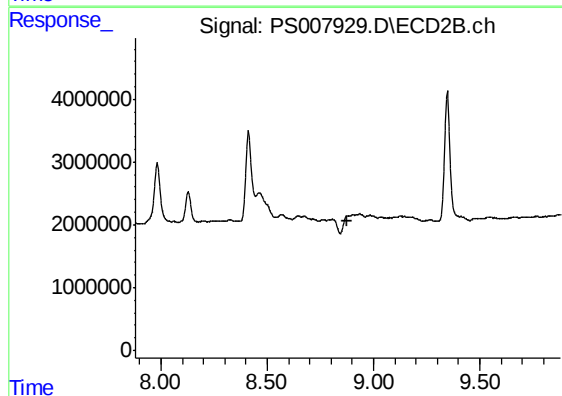

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.879 min
Response: 0
Conc: N.D.