

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007934.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 22:15
 Operator : SM\AJ
 Sample : K6147-14
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 P001-WC003

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:26:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.421	5.148	869.8E6	489.5E6	556.000	630.837
Target Compounds							
2) T	3,5-DICHL...	0.000	4.484	0	61639617	N.D.	59.562
3) T	4-Nitroph...	0.000	4.826	0	20937806	N.D.	46.236
8) T	DICHLORPROP	0.000	5.813	0	8936060	N.D.	12.466
9) T	2,4-D	6.474	0.000	81549891	0	50.690	N.D. #
10) T	Pentachlo...	0.000	6.437	0	7048051	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.745	0	47671131	N.D.	11.115
14) T	DINOSEB	0.000	7.978	0	25913138	N.D.	7.921
15) T	Picloram	8.889	0.000	59525182	0	4.923	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007934.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 22:15
Operator : SM\AJ
Sample : K6147-14
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
P001-WC003

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:26:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

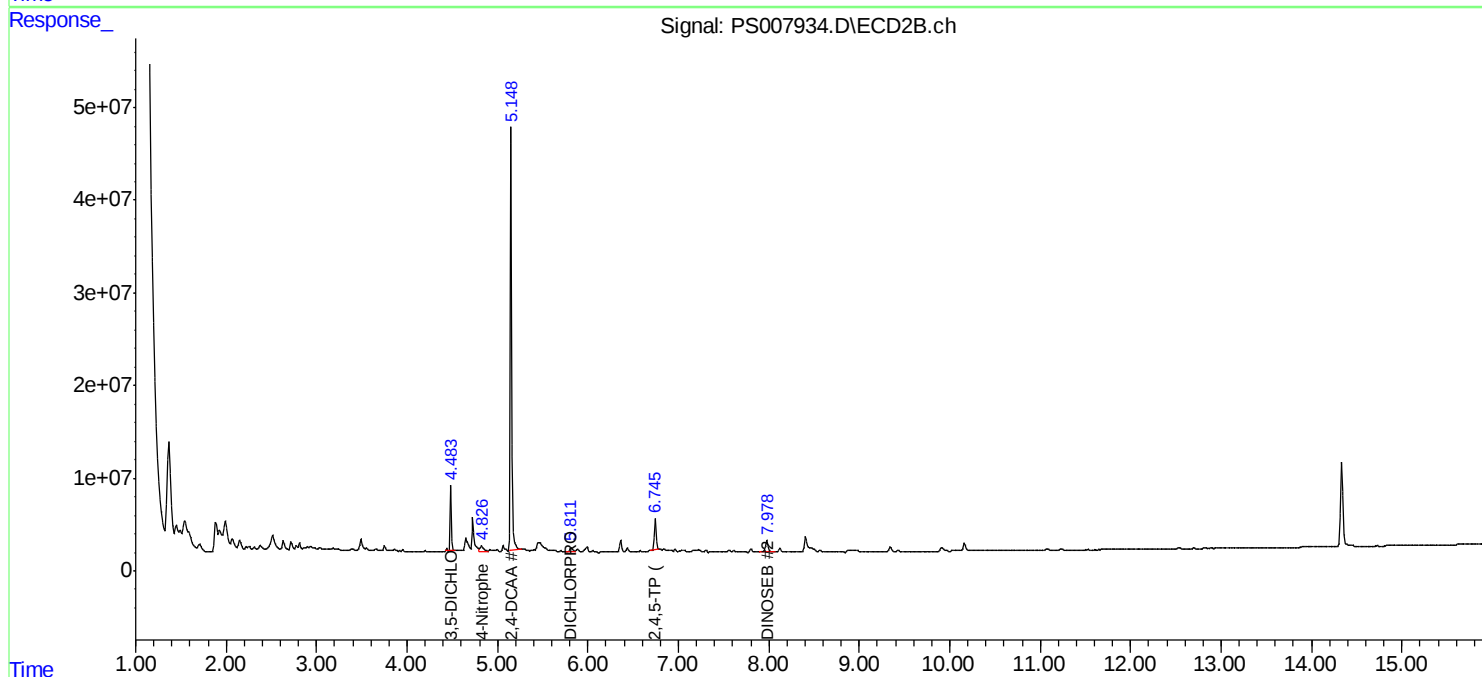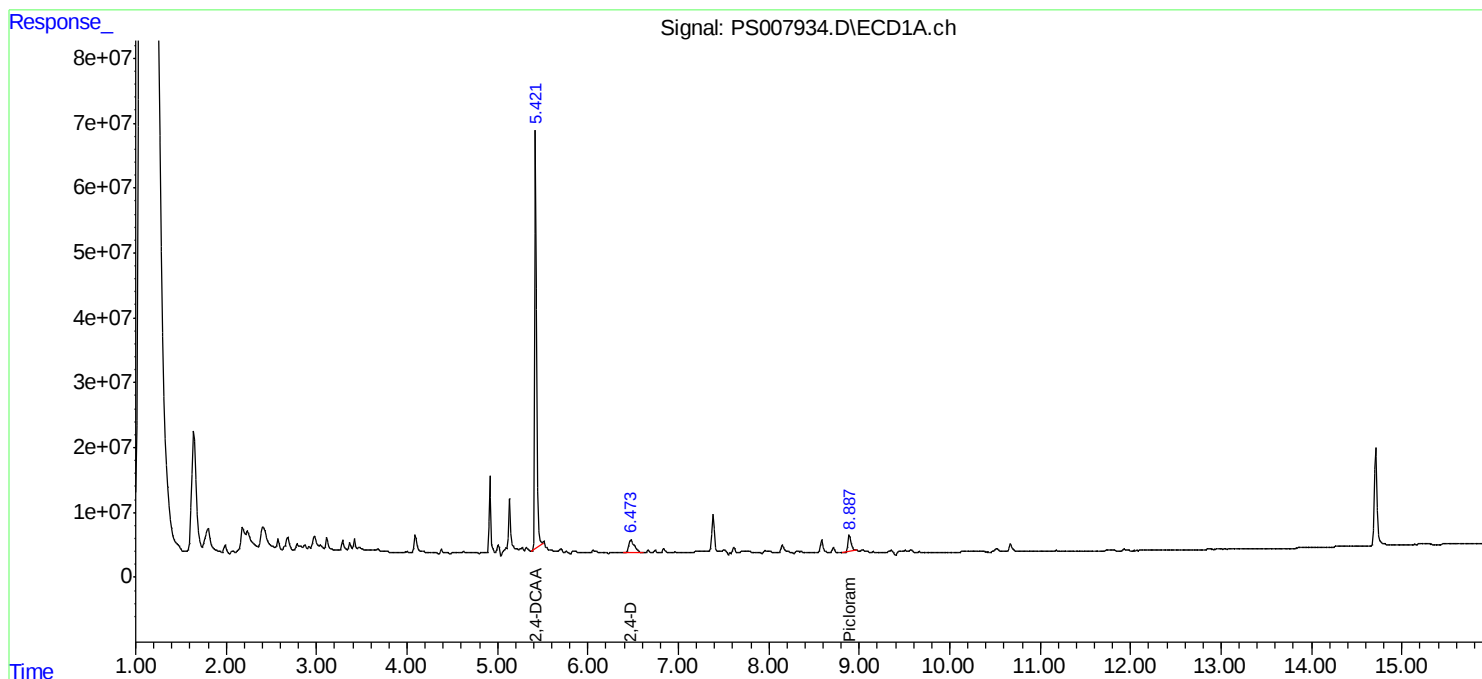


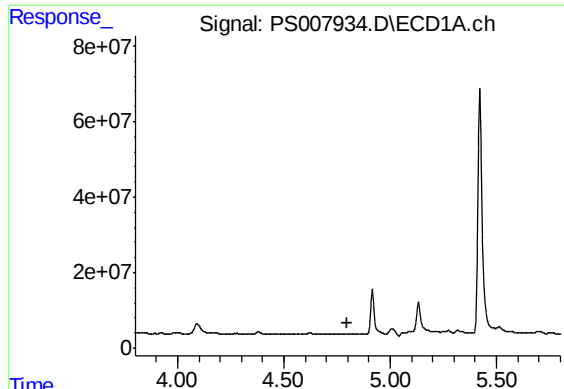

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC003

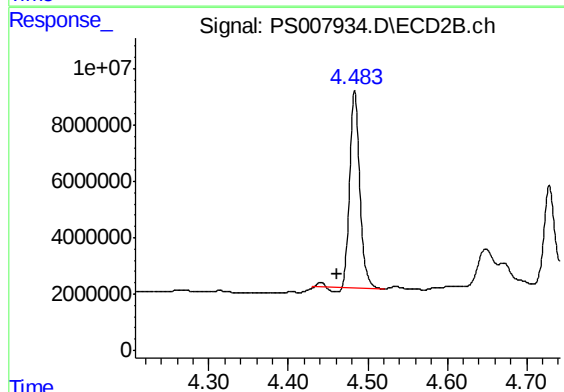


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.484 min
Delta R.T.: 0.022 min
Response: 61639617
Conc: 59.56 ng/ml

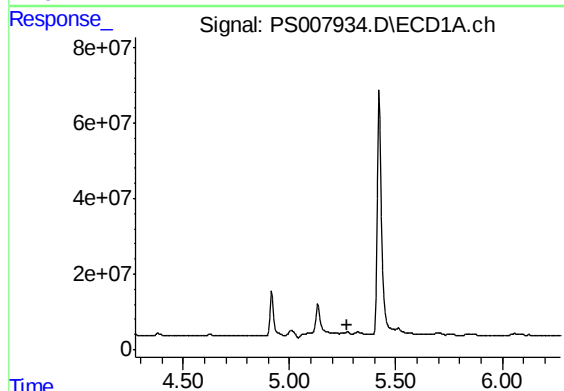


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

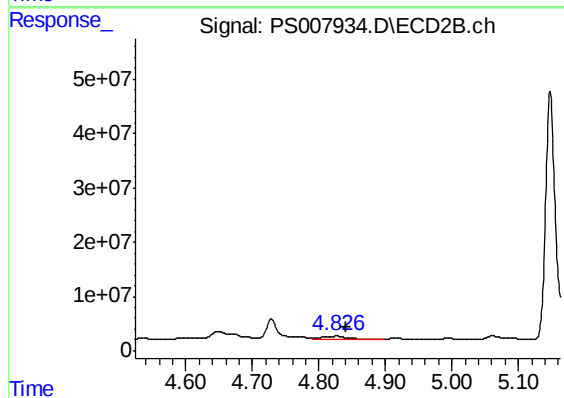

#3 4-Nitrophenol


R.T.: 4.826 min
Delta R.T.: -0.014 min
Response: 20937806
Conc: 46.24 ng/ml

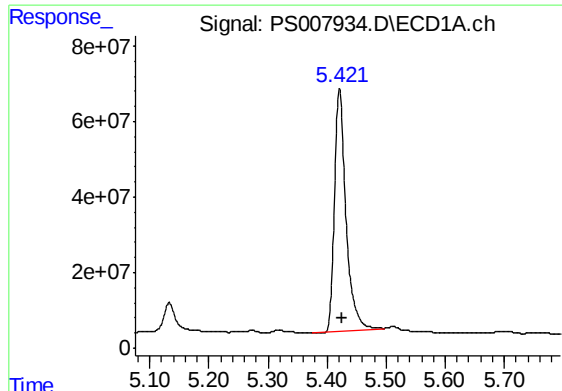

#4 2,4-DCAA


R.T.: 5.421 min
Delta R.T.: -0.004 min
Response: 869769968
Conc: 556.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
P001-WC003

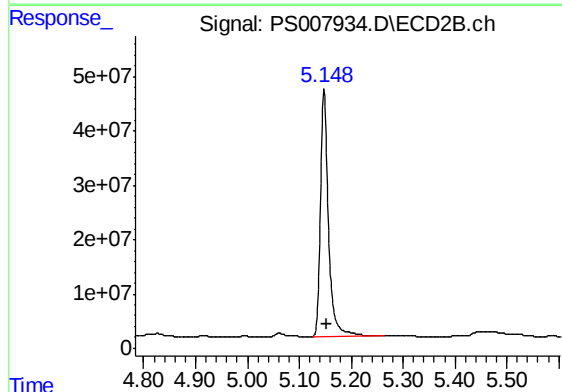


#4 2,4-DCAA

R.T.: 5.148 min
Delta R.T.: -0.004 min
Response: 489477624
Conc: 630.84 ng/ml

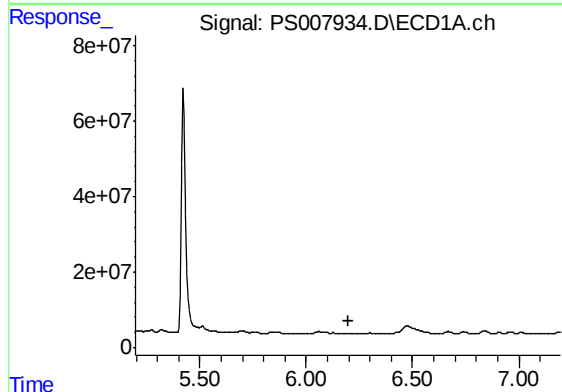


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.197 min
Response: 0
Conc: N.D.

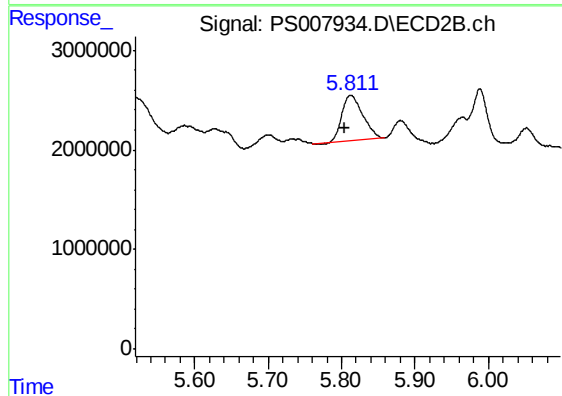

#8 DICHLORPROP


R.T.: 5.813 min
Delta R.T.: 0.008 min
Response: 8936060
Conc: 12.47 ng/ml

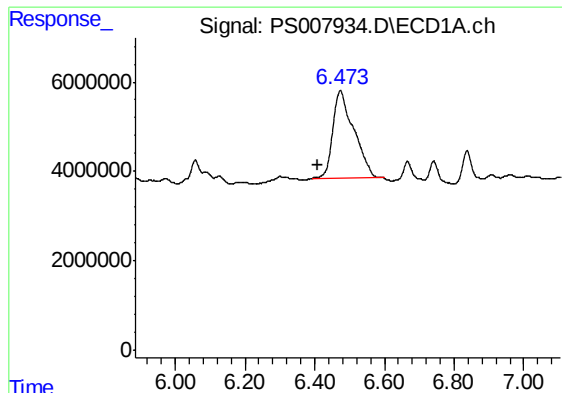

#9 2,4-D


R.T.: 6.474 min
Delta R.T.: 0.066 min
Response: 81549891
Conc: 50.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
P001-WC003

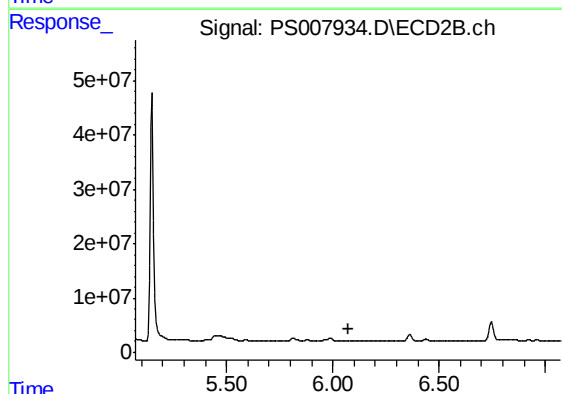


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

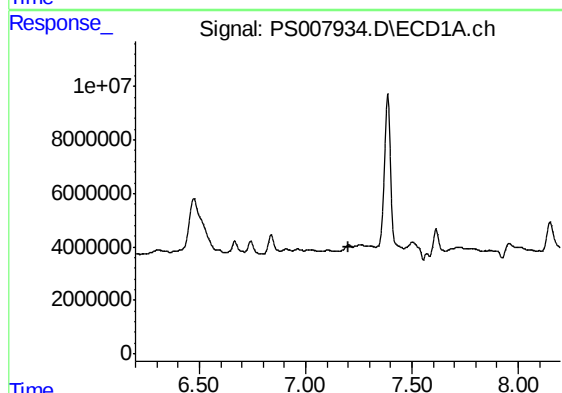


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

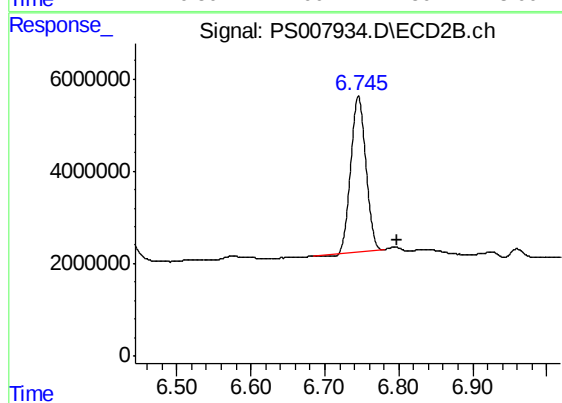

#11 2,4,5-TP (SILVEX)


R.T.: 6.745 min
Delta R.T.: -0.052 min
Response: 47671131
Conc: 11.12 ng/ml

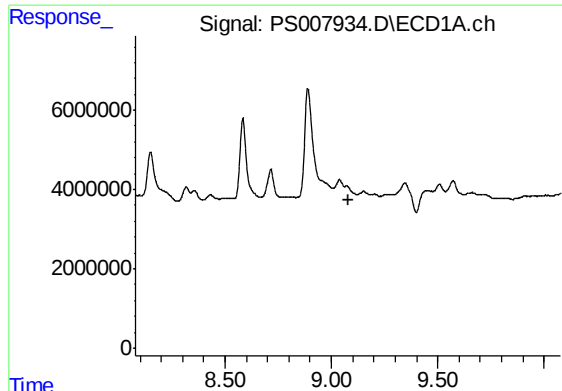

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.078 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC003

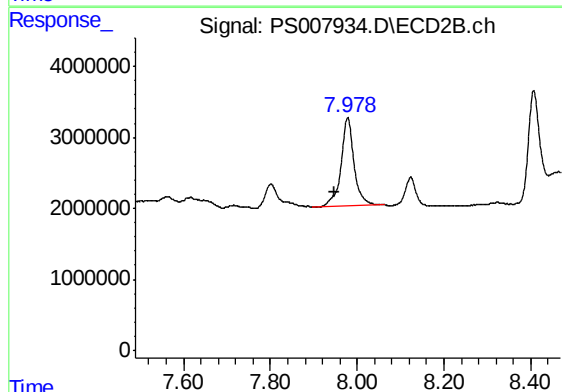


#14 DINOSEB

R.T.: 7.978 min
Delta R.T.: 0.031 min
Response: 25913138
Conc: 7.92 ng/ml

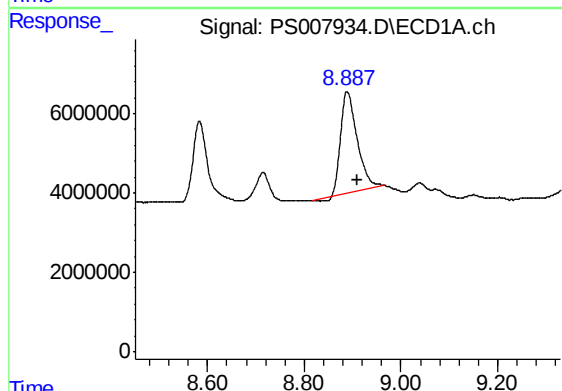

#15 Picloram

R.T.: 8.889 min
Delta R.T.: -0.022 min
Response: 59525182
Conc: 4.92 ng/ml

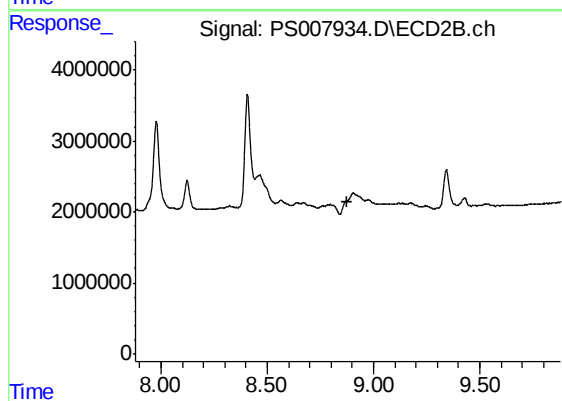

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.879 min
Response: 0
Conc: N.D.