

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 22:36
 Operator : SM\AJ
 Sample : K6147-15
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 P001-WC004

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 02:22:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.460	5.188	774.2E6	430.1E6	494.887	554.375
Target Compounds							
2) T	3,5-DICHL...	0.000	4.523	0 47026329		N.D.	45.441
7) T	MCPA	0.000	5.488	0 44294165		N.D.	13.900
8) T	DICHLORPROP	0.000	5.853	0 4615697		N.D.	6.439
10) T	Pentachlo...	0.000	6.401	0 16067739		N.D.	1.472
11) T	2,4,5-TP ...	0.000	6.785	0 34760530		N.D.	8.105
12) T	2,4,5-T	7.424	0.000	85084691	0	9.193	N.D. #
15) T	Picloram	8.931	0.000	57753850	0	4.777	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 22:36
Operator : SM\AJ
Sample : K6147-15
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
P001-WC004

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 02:22:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

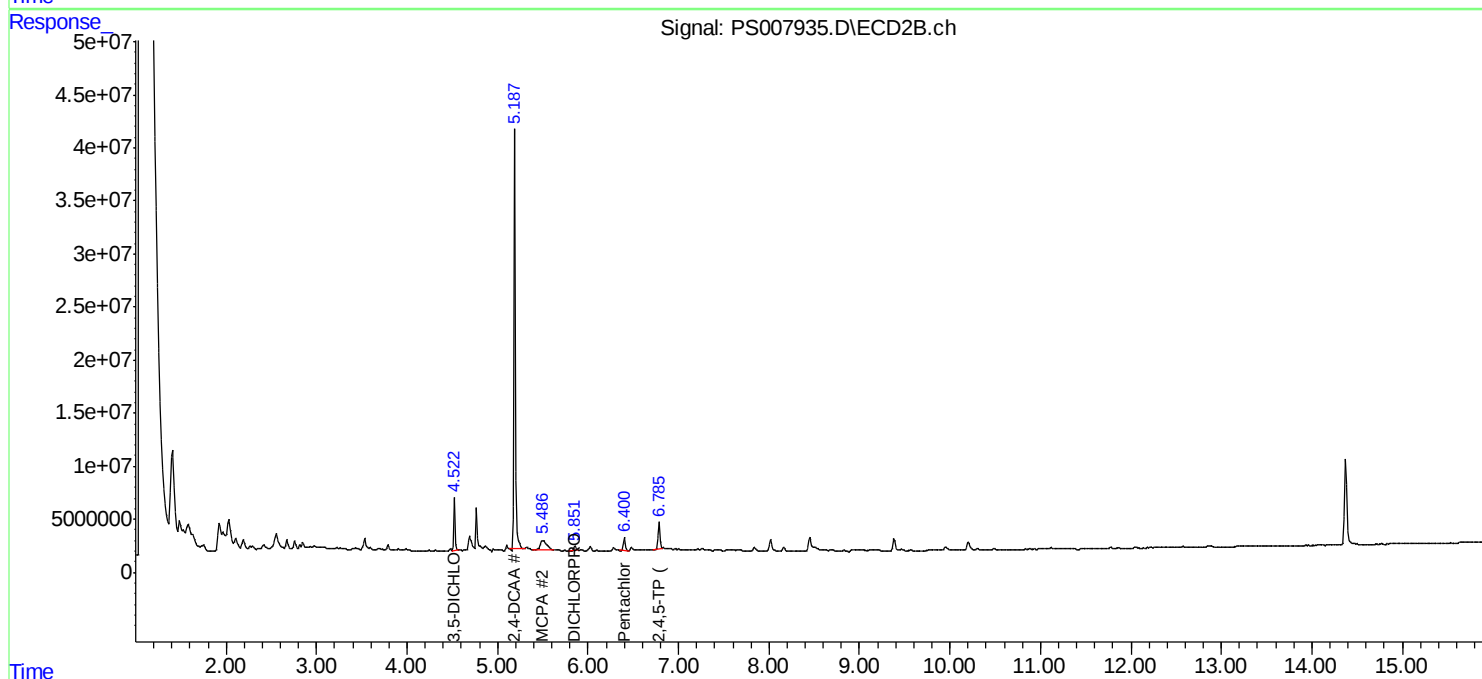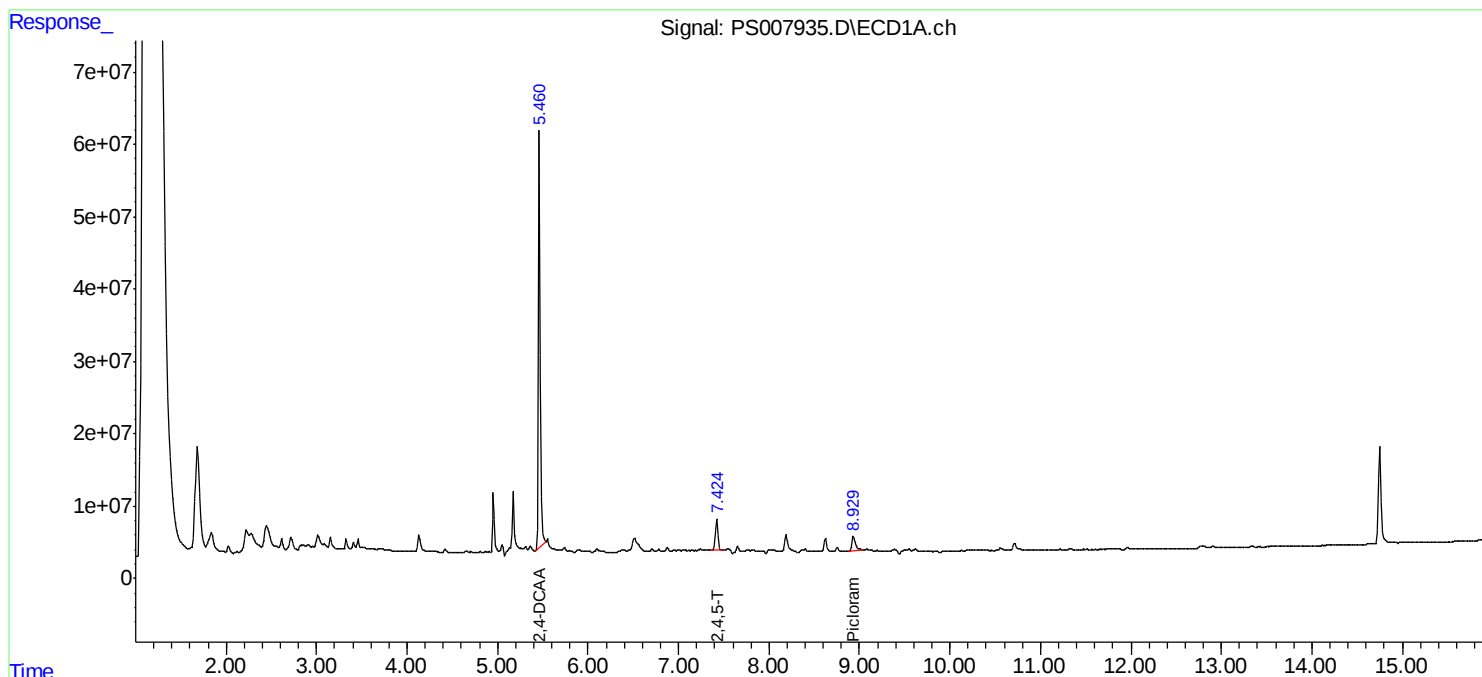


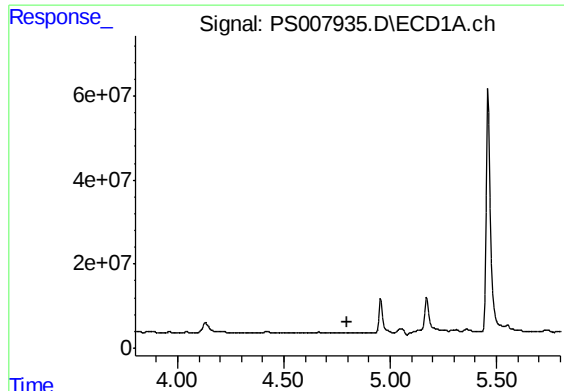

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC004

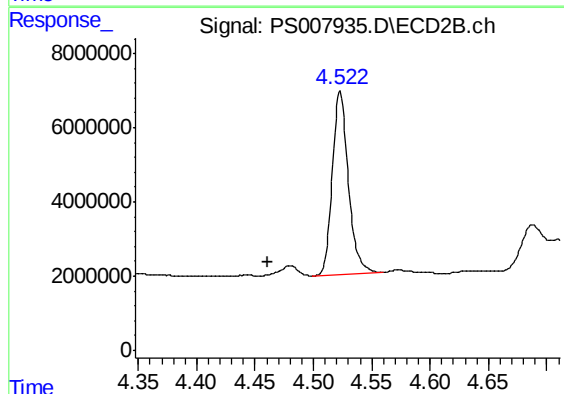


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.523 min
Delta R.T.: 0.062 min
Response: 47026329
Conc: 45.44 ng/ml

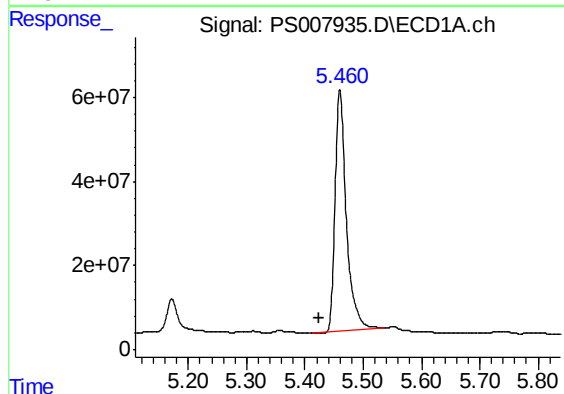


#4 2,4-DCAA

R.T.: 5.460 min
Delta R.T.: 0.035 min
Response: 774167638
Conc: 494.89 ng/ml

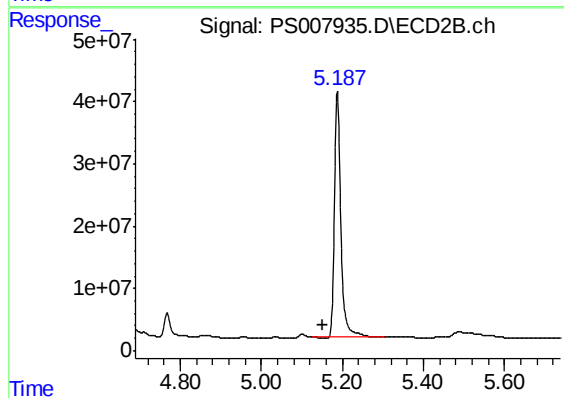

#4 2,4-DCAA


R.T.: 5.188 min
Delta R.T.: 0.036 min
Response: 430149233
Conc: 554.37 ng/ml

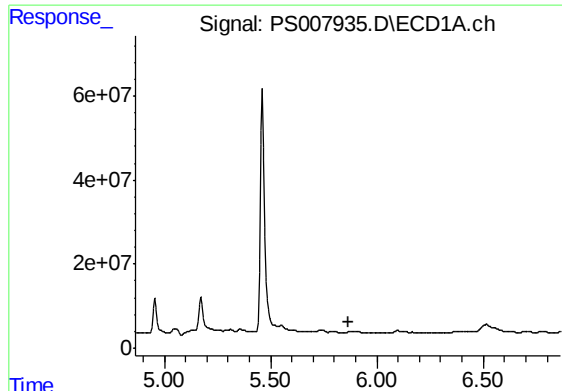

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.864 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC004

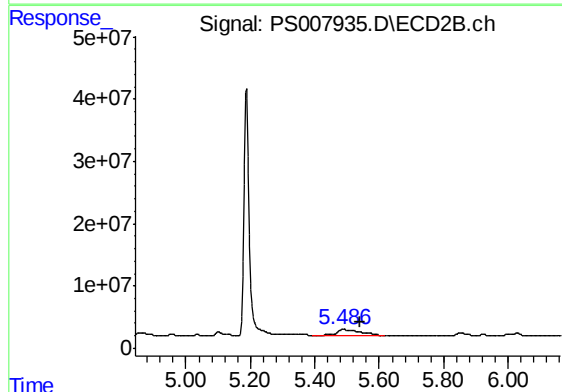


#7 MCPA

R.T.: 5.488 min
Delta R.T.: -0.054 min
Response: 44294165
Conc: 13.90 ug/ml

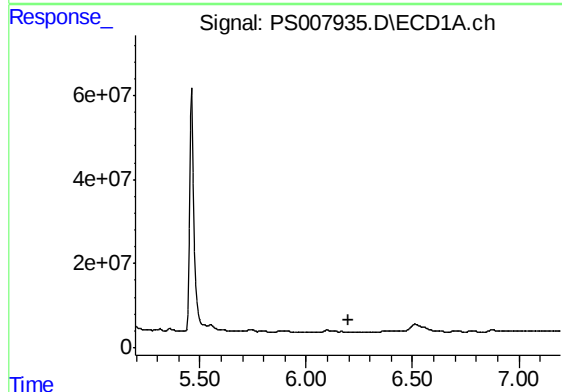


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.197 min
Response: 0
Conc: N.D.

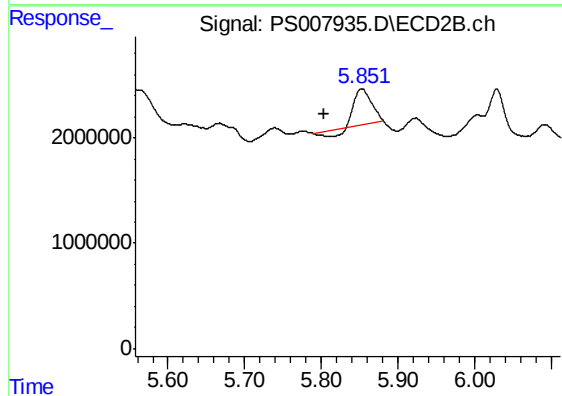

#8 DICHLORPROP


R.T.: 5.853 min
Delta R.T.: 0.048 min
Response: 4615697
Conc: 6.44 ng/ml

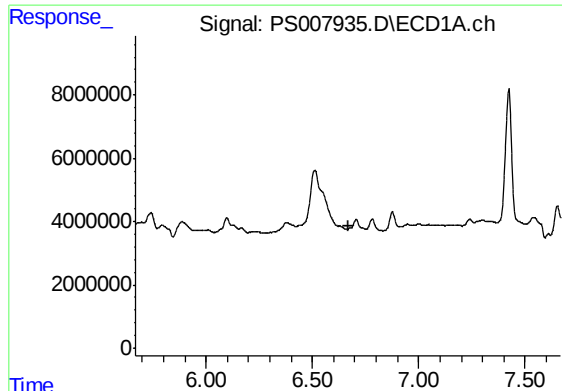

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.667 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC004

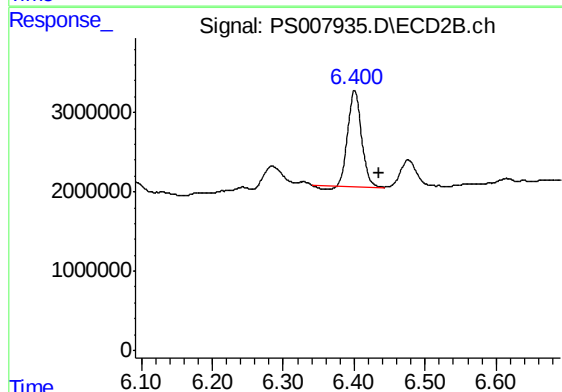


#10 Pentachlorophenol

R.T.: 6.401 min
Delta R.T.: -0.035 min
Response: 16067739
Conc: 1.47 ng/ml

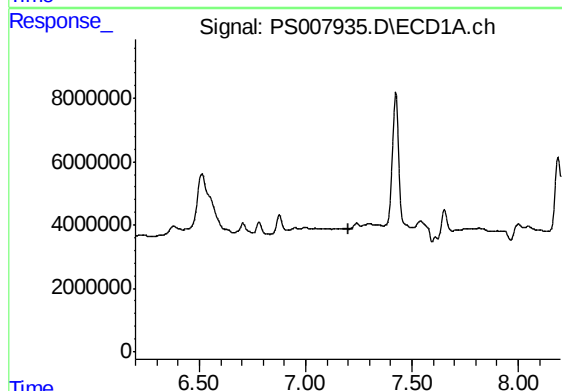


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

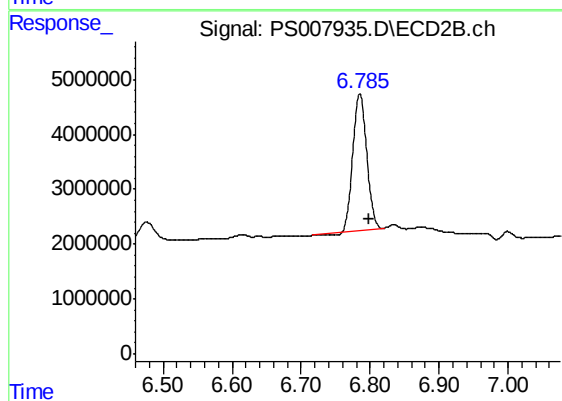

#11 2,4,5-TP (SILVEX)


R.T.: 6.785 min
Delta R.T.: -0.013 min
Response: 34760530
Conc: 8.10 ng/ml

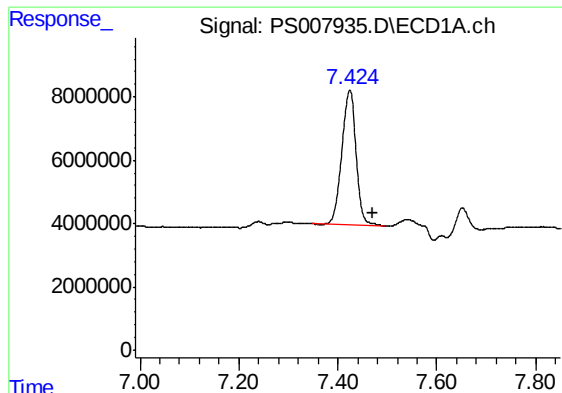

#12 2,4,5-T


R.T.: 7.424 min
Delta R.T.: -0.046 min
Response: 85084691
Conc: 9.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
P001-WC004

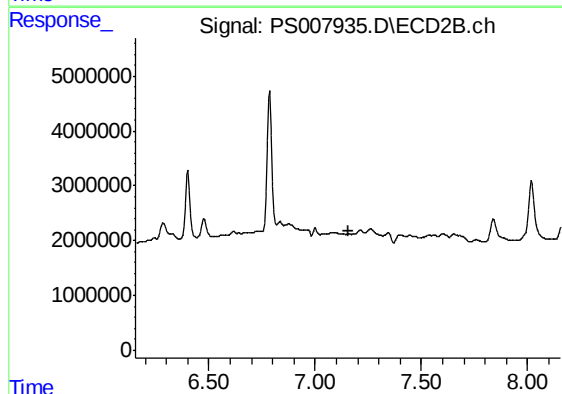


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

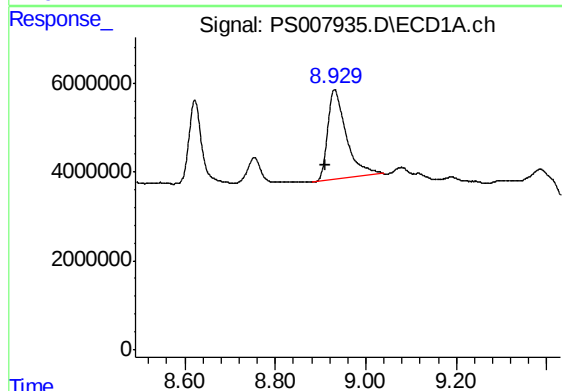

#15 Picloram

R.T.: 8.931 min
Delta R.T.: 0.020 min
Response: 57753850
Conc: 4.78 ng/ml

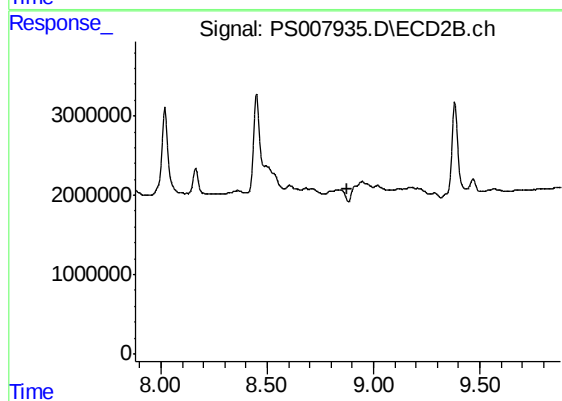

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.879 min
Response: 0
Conc: N.D.