

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007938.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2019 23:42
 Operator : SM\AJ
 Sample : K6147-16
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 P001-WC005

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 02:22:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.426	5.153	589.1E6	346.3E6	376.603	446.345
Target Compounds							
2) T	3,5-DICHL...	0.000	4.488	0	56416473	N.D.	54.515
7) T	MCPA	0.000	5.476	0	45452693	N.D.	14.263
8) T	DICHLORPROP	0.000	5.815	0	7485040	N.D.	10.442
9) T	2,4-D	6.475	0.000	187.8E6	0	116.736	N.D. #
10) T	Pentachlo...	0.000	6.438	0	7707610	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.799	0	78031178	N.D.	18.194
14) T	DINOSEB	0.000	7.982	0	23690498	N.D.	7.242
15) T	Picloram	8.895	0.000	49929837	0	4.130	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007938.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2019 23:42
Operator : SM\AJ
Sample : K6147-16
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
P001-WC005

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 02:22:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

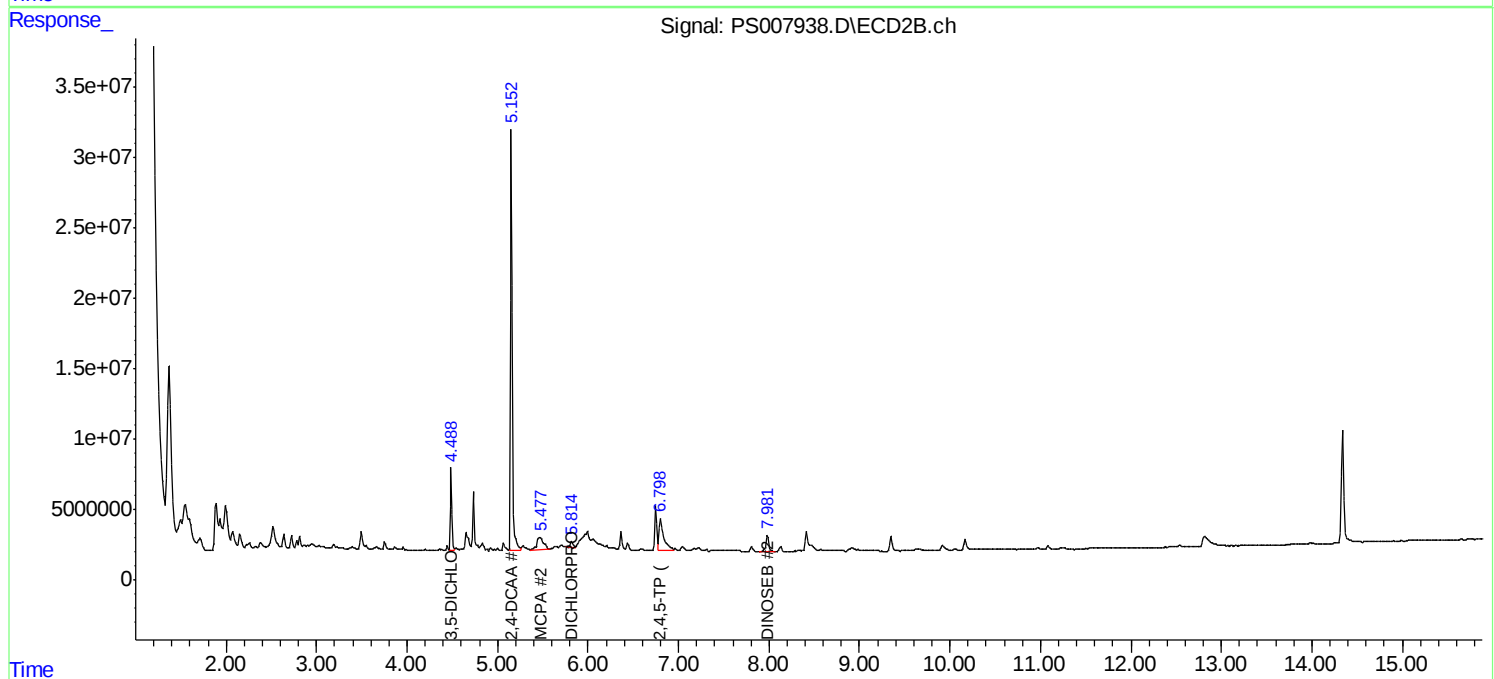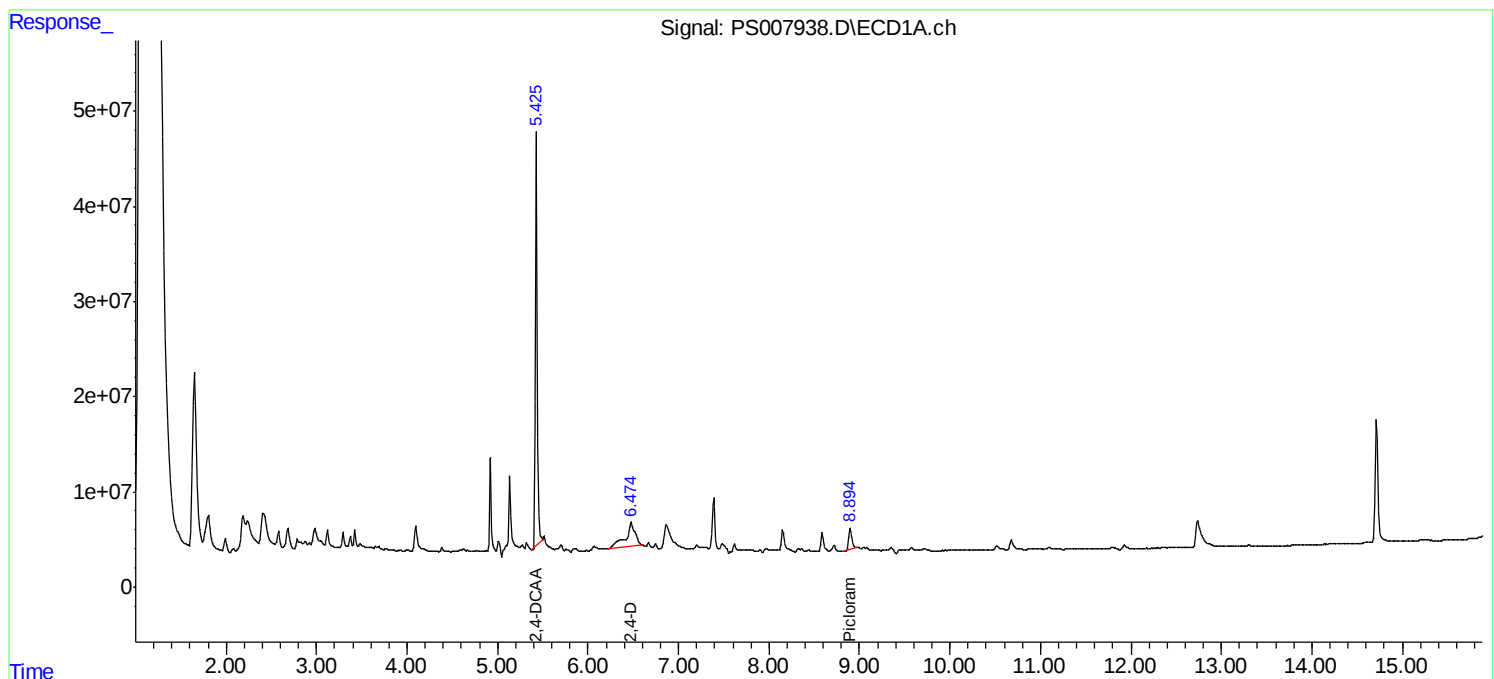


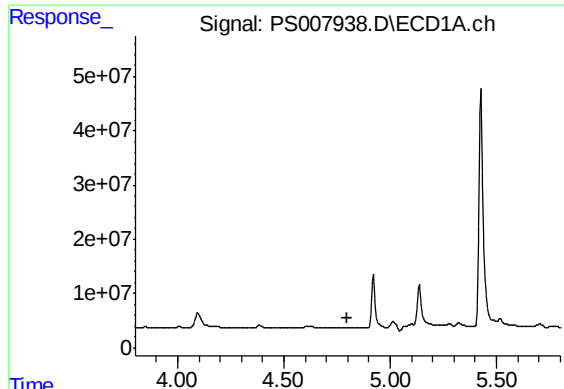

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC005

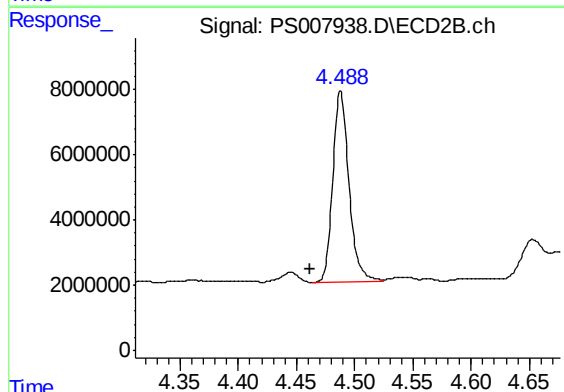


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.488 min
Delta R.T.: 0.027 min
Response: 56416473
Conc: 54.52 ng/ml

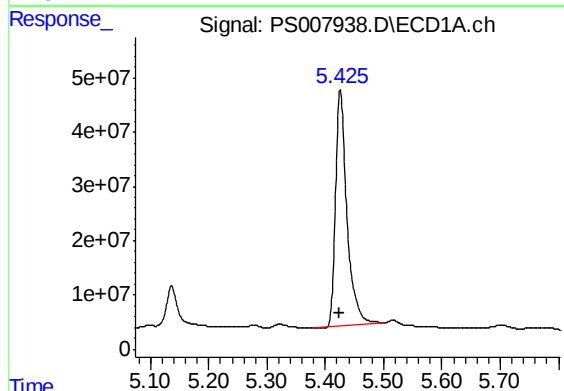


#4 2,4-DCAA

R.T.: 5.426 min
Delta R.T.: 0.000 min
Response: 589132476
Conc: 376.60 ng/ml

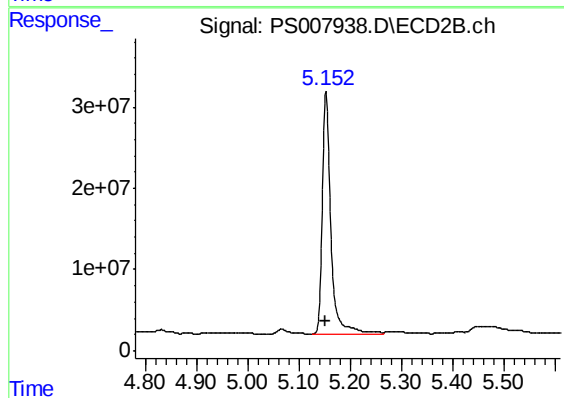

#4 2,4-DCAA


R.T.: 5.153 min
Delta R.T.: 0.000 min
Response: 346327254
Conc: 446.35 ng/ml

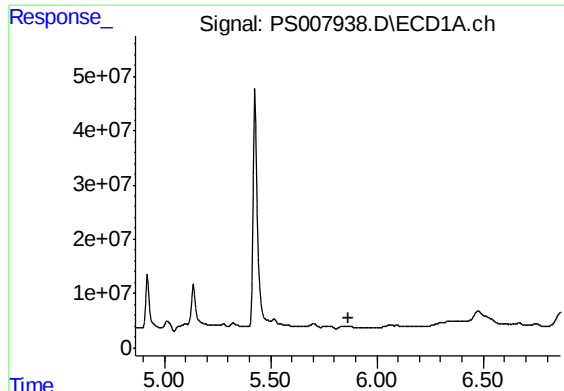

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.864 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC005

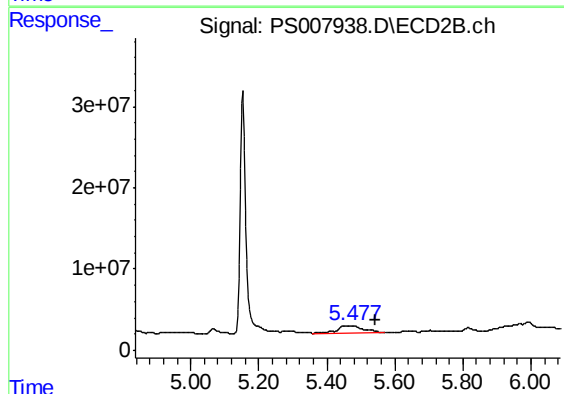


#7 MCPA

R.T.: 5.476 min
Delta R.T.: -0.067 min
Response: 45452693
Conc: 14.26 ug/ml

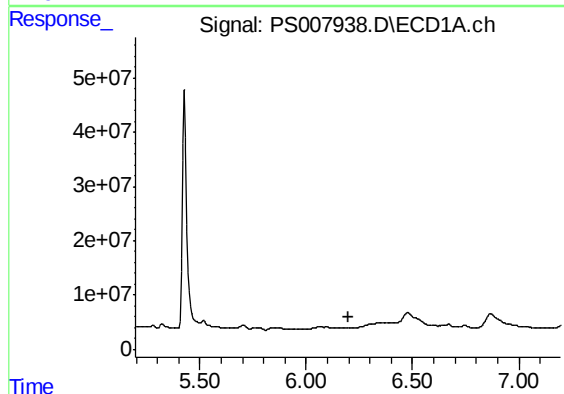


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.197 min
Response: 0
Conc: N.D.

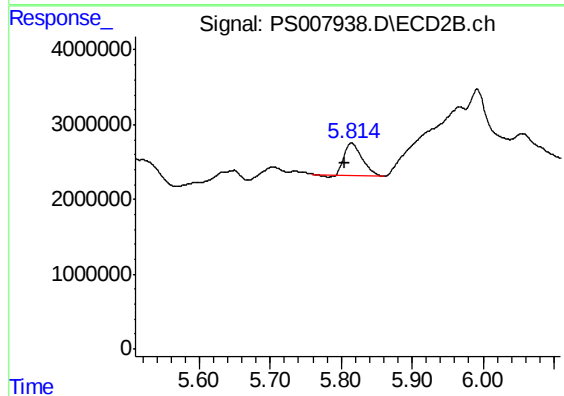

#8 DICHLORPROP


R.T.: 5.815 min
Delta R.T.: 0.011 min
Response: 7485040
Conc: 10.44 ng/ml

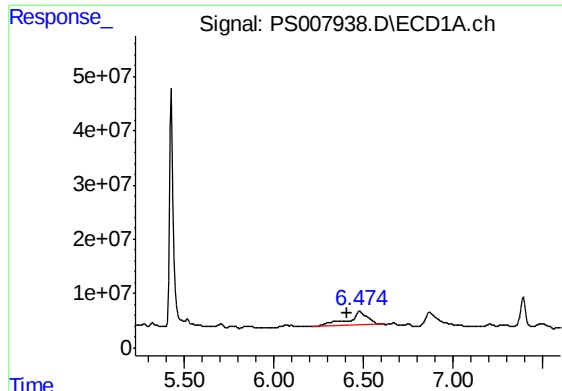

#9 2,4-D


R.T.: 6.475 min
Delta R.T.: 0.067 min
Response: 187803089
Conc: 116.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
P001-WC005

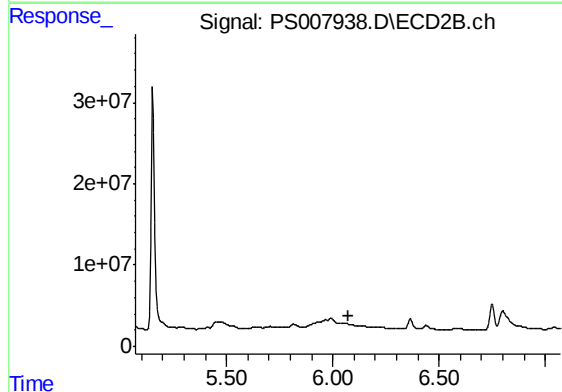


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

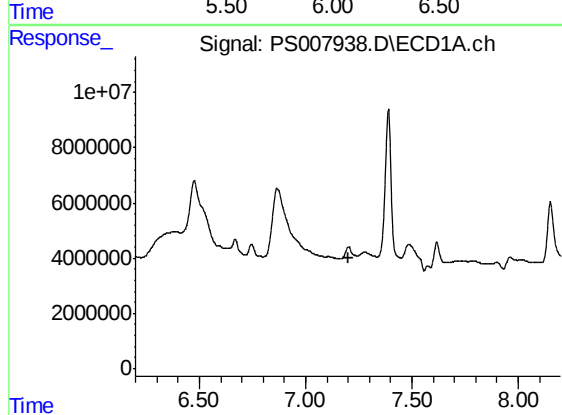


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

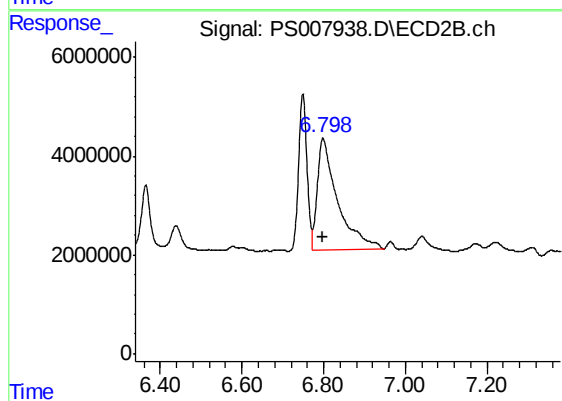

#11 2,4,5-TP (SILVEX)


R.T.: 6.799 min
Delta R.T.: 0.000 min
Response: 78031178
Conc: 18.19 ng/ml

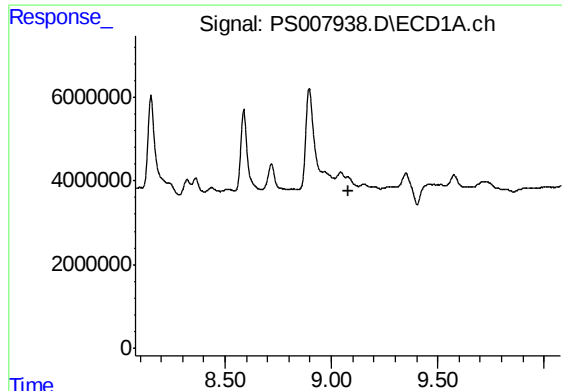

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.078 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC005

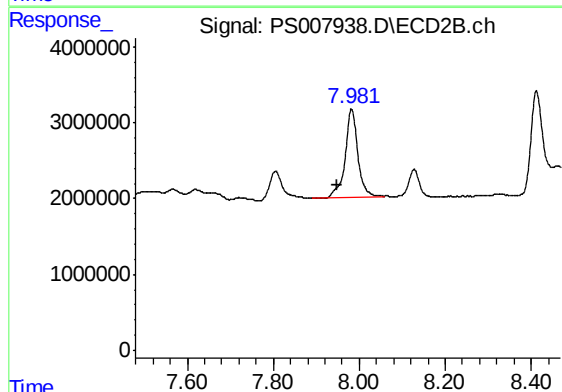


#14 DINOSEB

R.T.: 7.982 min
Delta R.T.: 0.035 min
Response: 23690498
Conc: 7.24 ng/ml

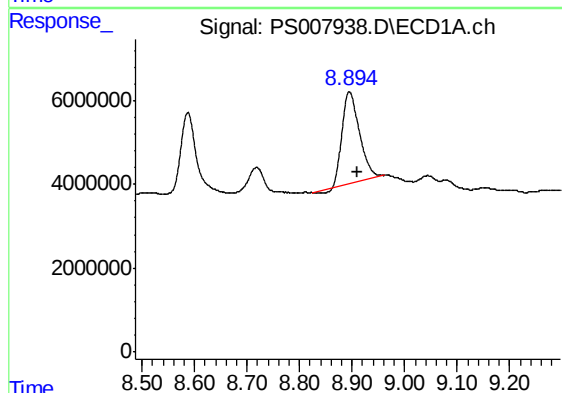

#15 Picloram

R.T.: 8.895 min
Delta R.T.: -0.016 min
Response: 49929837
Conc: 4.13 ng/ml

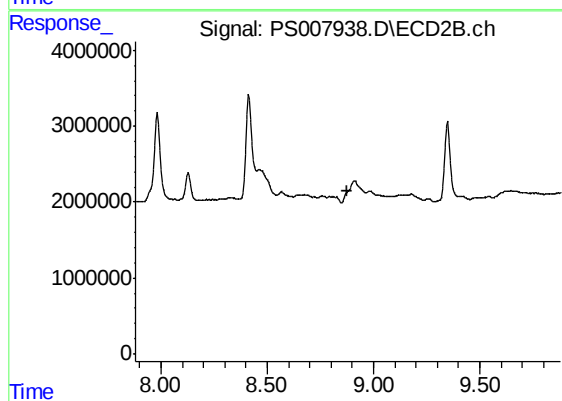

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.879 min
Response: 0
Conc: N.D.