

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007939.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2019 00:04
 Operator : SM\AJ
 Sample : K6147-17
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 P001-WC006

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 02:22:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.443	5.171	639.9E6	364.4E6	409.079	469.675
Target Compounds							
2) T	3,5-DICHL...	0.000	4.505	0 68087036		N.D.	65.792
3) T	4-Nitroph...	0.000	4.848	0 12184847		N.D.	26.907
7) T	MCPA	0.000	5.474	0 42431811		N.D.	13.316
9) T	2,4-D	0.000	6.010	0 34817541		N.D.	39.403
10) T	Pentachlo...	0.000	6.383	0 19263952		N.D.	1.765
11) T	2,4,5-TP ...	0.000	6.817	0 14041530		N.D.	3.274
12) T	2,4,5-T	7.407	0.000	120.7E6	0	13.036	N.D. #
14) T	DINOSEB	0.000	8.000	0 13563625		N.D.	4.146
15) T	Picloram	8.911	0.000	57522299	0	4.757	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007939.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2019 00:04
Operator : SM\AJ
Sample : K6147-17
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
P001-WC006

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 02:22:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

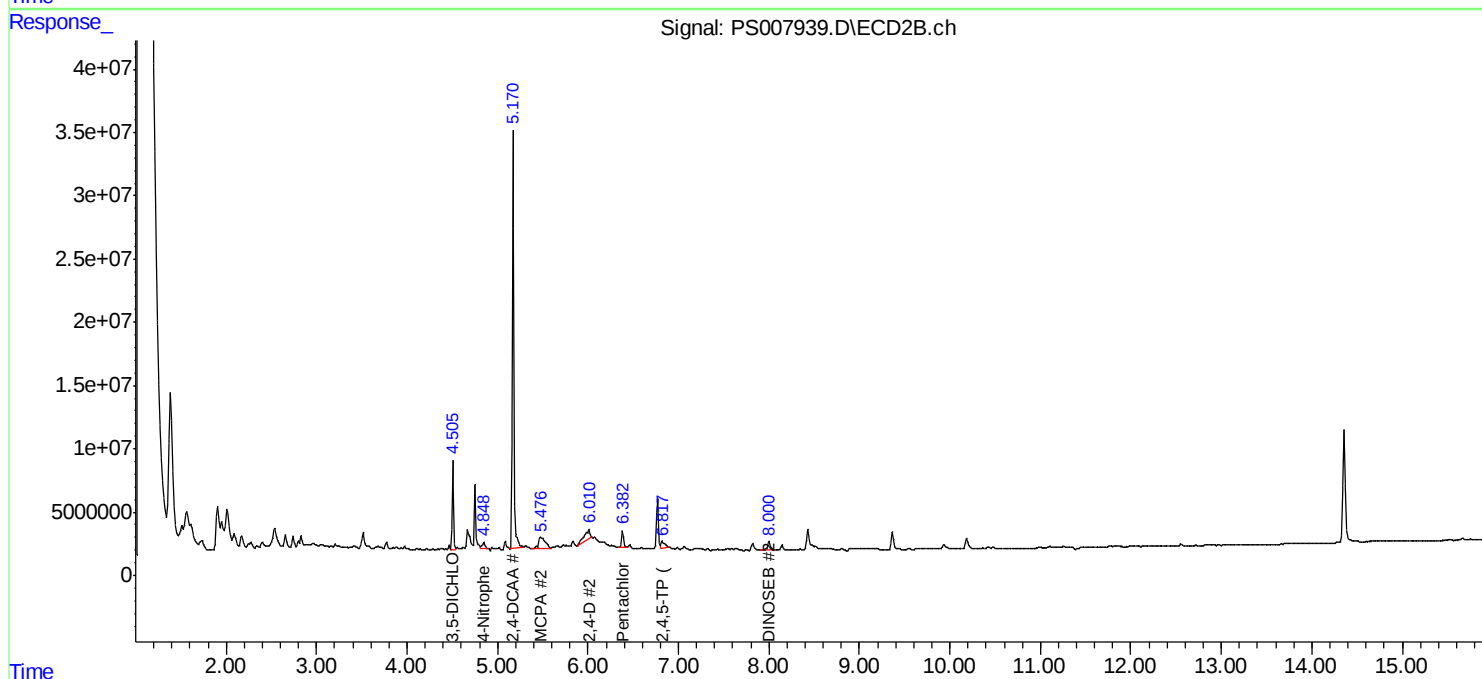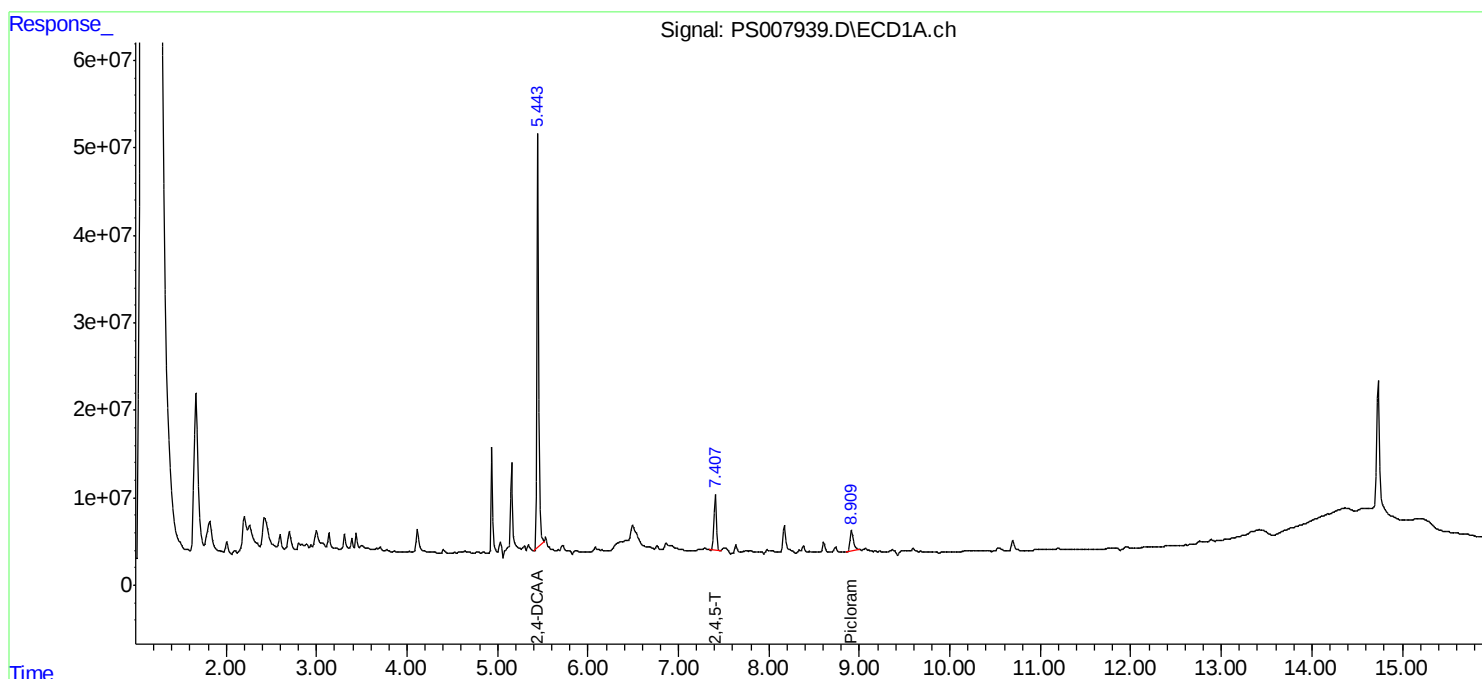


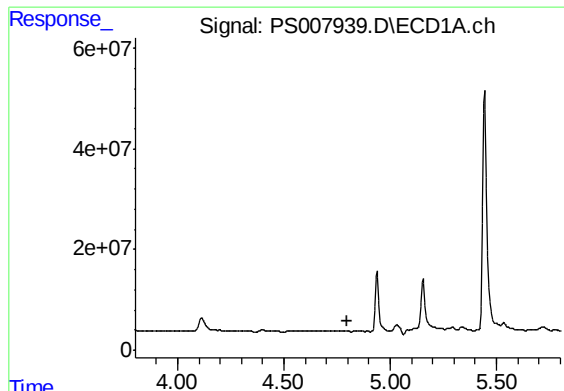

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC006

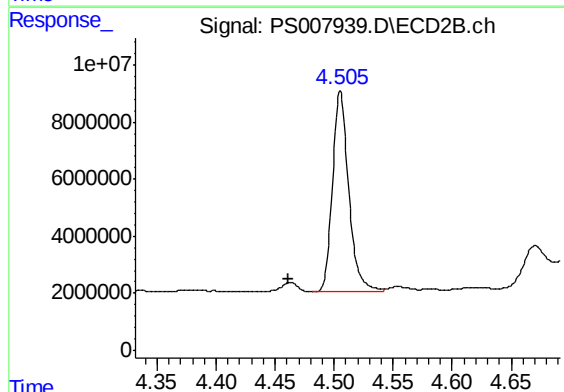


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.505 min
Delta R.T.: 0.044 min
Response: 68087036
Conc: 65.79 ng/ml

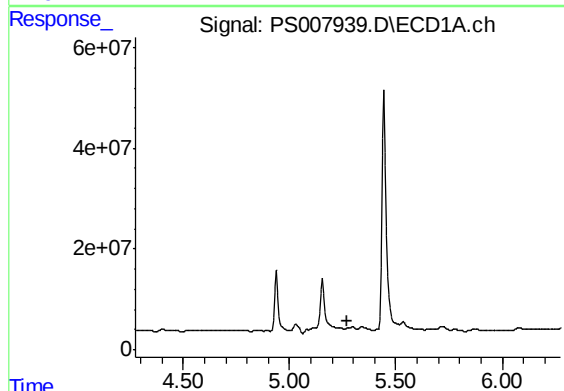


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

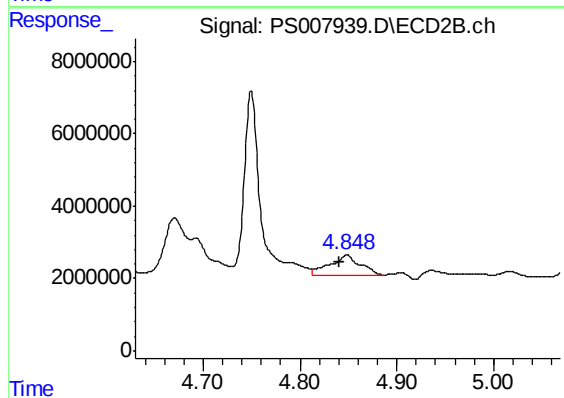

#3 4-Nitrophenol


R.T.: 4.848 min
Delta R.T.: 0.007 min
Response: 12184847
Conc: 26.91 ng/ml

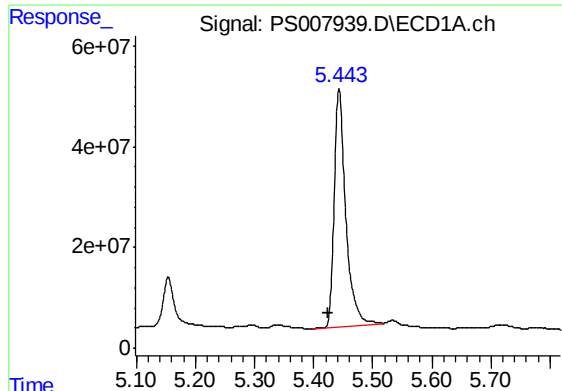

#4 2,4-DCAA


R.T.: 5.443 min
Delta R.T.: 0.018 min
Response: 639935593
Conc: 409.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
P001-WC006

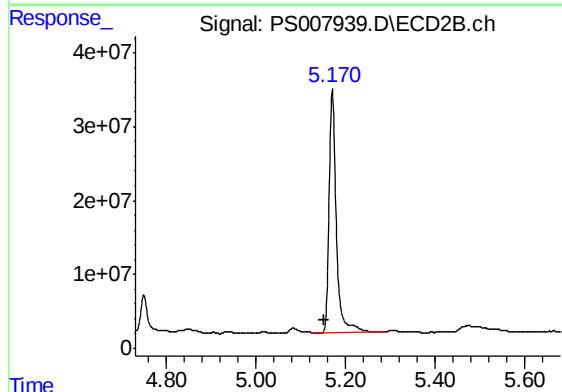


#4 2,4-DCAA

R.T.: 5.171 min
Delta R.T.: 0.019 min
Response: 364429420
Conc: 469.68 ng/ml

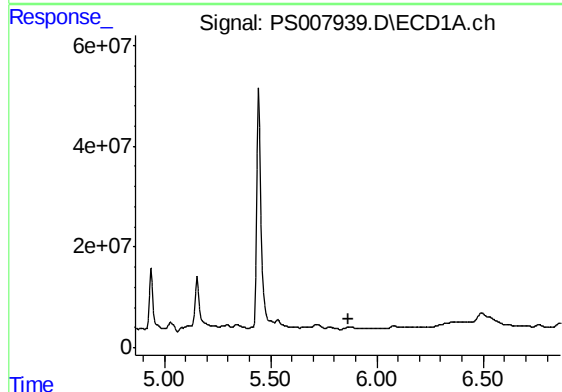


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.864 min
Response: 0
Conc: N.D.

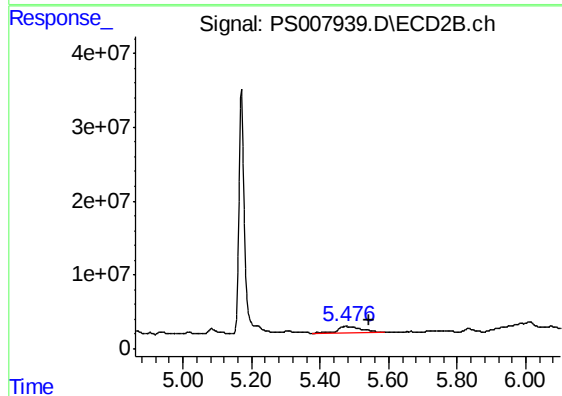

#7 MCPA


R.T.: 5.474 min
Delta R.T.: -0.069 min
Response: 42431811
Conc: 13.32 ug/ml

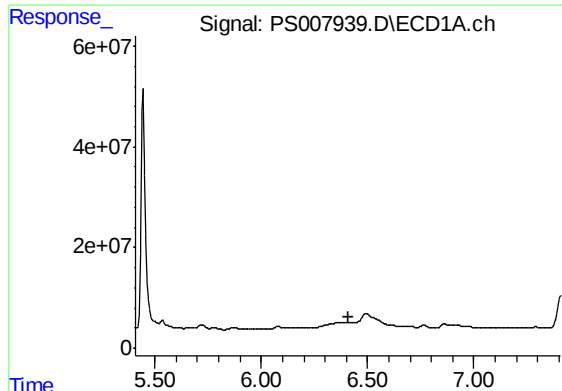

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC006

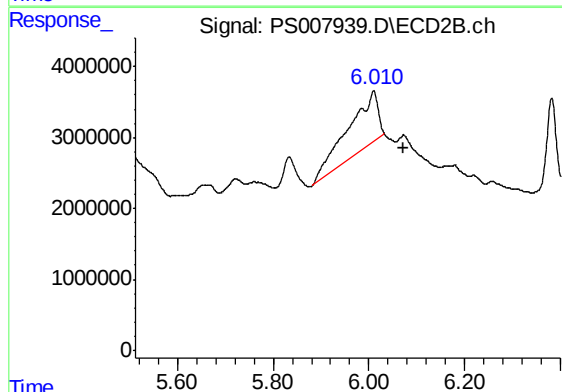


#9 2,4-D

R.T.: 6.010 min
Delta R.T.: -0.062 min
Response: 34817541
Conc: 39.40 ng/ml

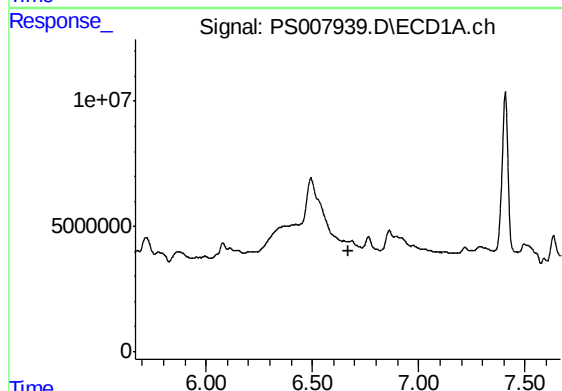


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.667 min
Response: 0
Conc: N.D.

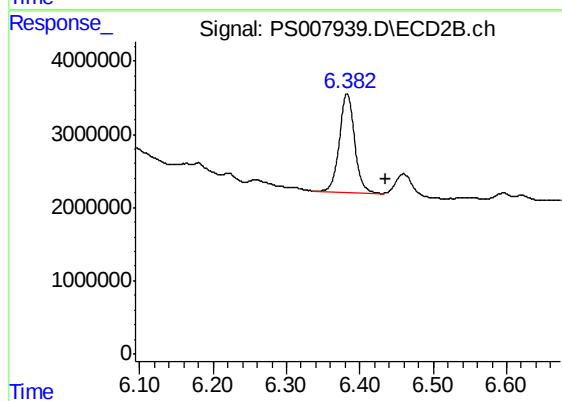

#10 Pentachlorophenol


R.T.: 6.383 min
Delta R.T.: -0.052 min
Response: 19263952
Conc: 1.76 ng/ml

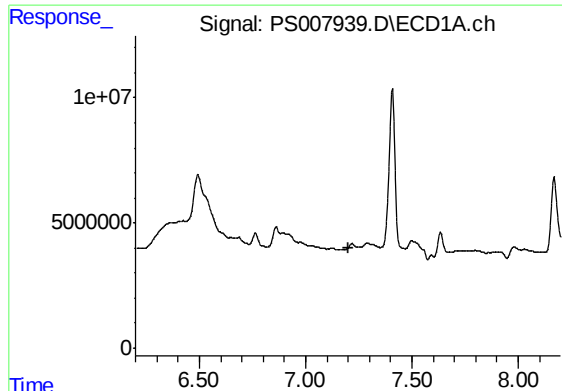

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC006

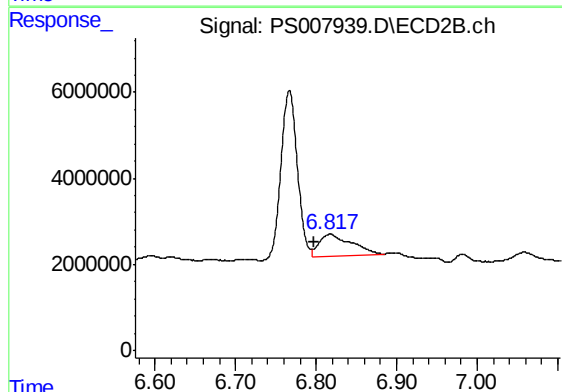


#11 2,4,5-TP (SILVEX)

R.T.: 6.817 min
Delta R.T.: 0.019 min
Response: 14041530
Conc: 3.27 ng/ml

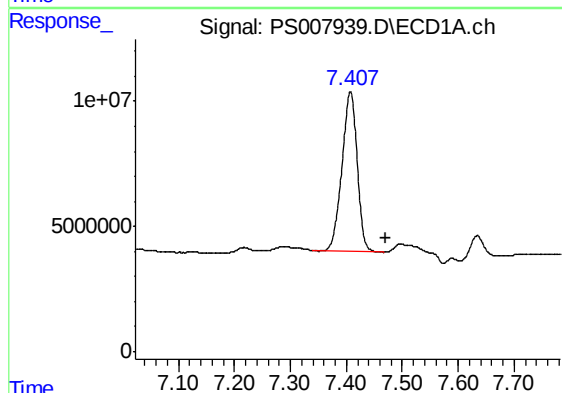


#12 2,4,5-T

R.T.: 7.407 min
Delta R.T.: -0.062 min
Response: 120651031
Conc: 13.04 ng/ml

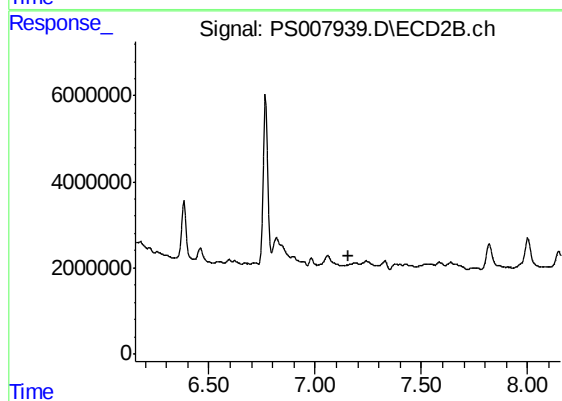

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 7.155 min
Response: 0
Conc: N.D.

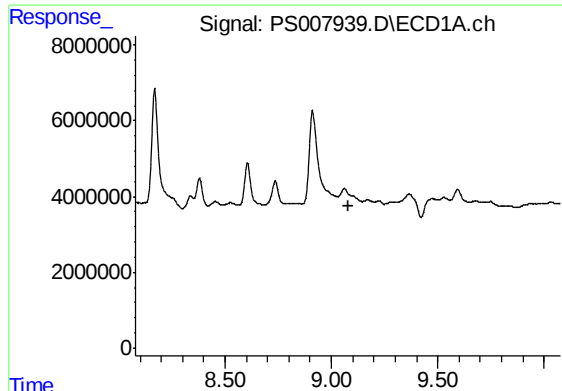

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.078 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC006

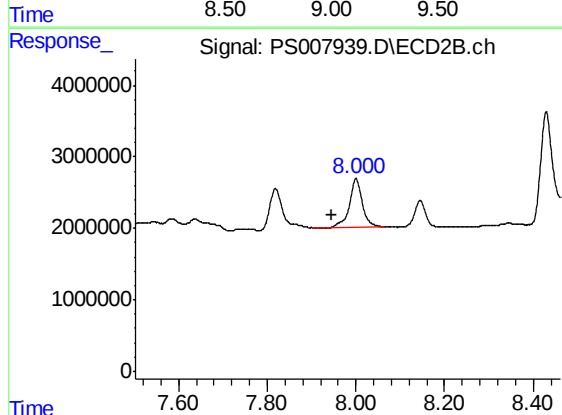


#14 DINOSEB

R.T.: 8.000 min
Delta R.T.: 0.053 min
Response: 13563625
Conc: 4.15 ng/ml

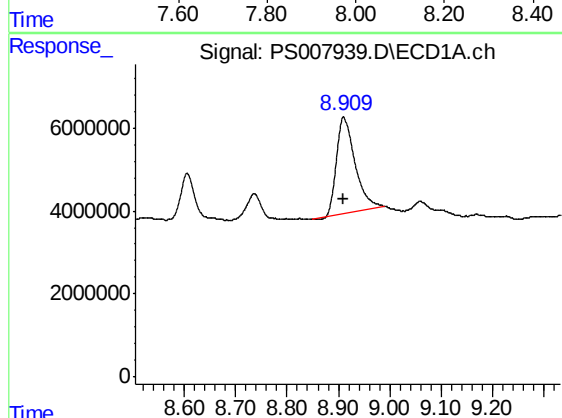

#15 Picloram

R.T.: 8.911 min
Delta R.T.: 0.000 min
Response: 57522299
Conc: 4.76 ng/ml

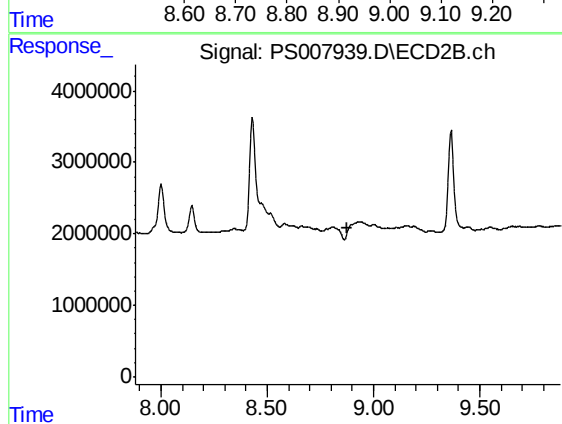

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.879 min
Response: 0
Conc: N.D.