

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007940.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2019 00:26
 Operator : SM\AJ
 Sample : K6147-18
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 P001-WC007

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 02:23:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.424	5.152	670.6E6	384.4E6	428.699	495.434
Target Compounds							
2) T	3,5-DICHL...	0.000	4.487	0	63089599	N.D.	60.963
9) T	2,4-D	6.475	0.000	84320468	0	52.412	N.D. #
11) T	2,4,5-TP ...	0.000	6.749	0	45101322	N.D.	10.516
14) T	DINOSEB	0.000	7.982	0	20815995	N.D.	6.363
15) T	Picloram	8.893	0.000	53559178	0	4.430	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007940.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2019 00:26
Operator : SM\AJ
Sample : K6147-18
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
P001-WC007

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 02:23:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

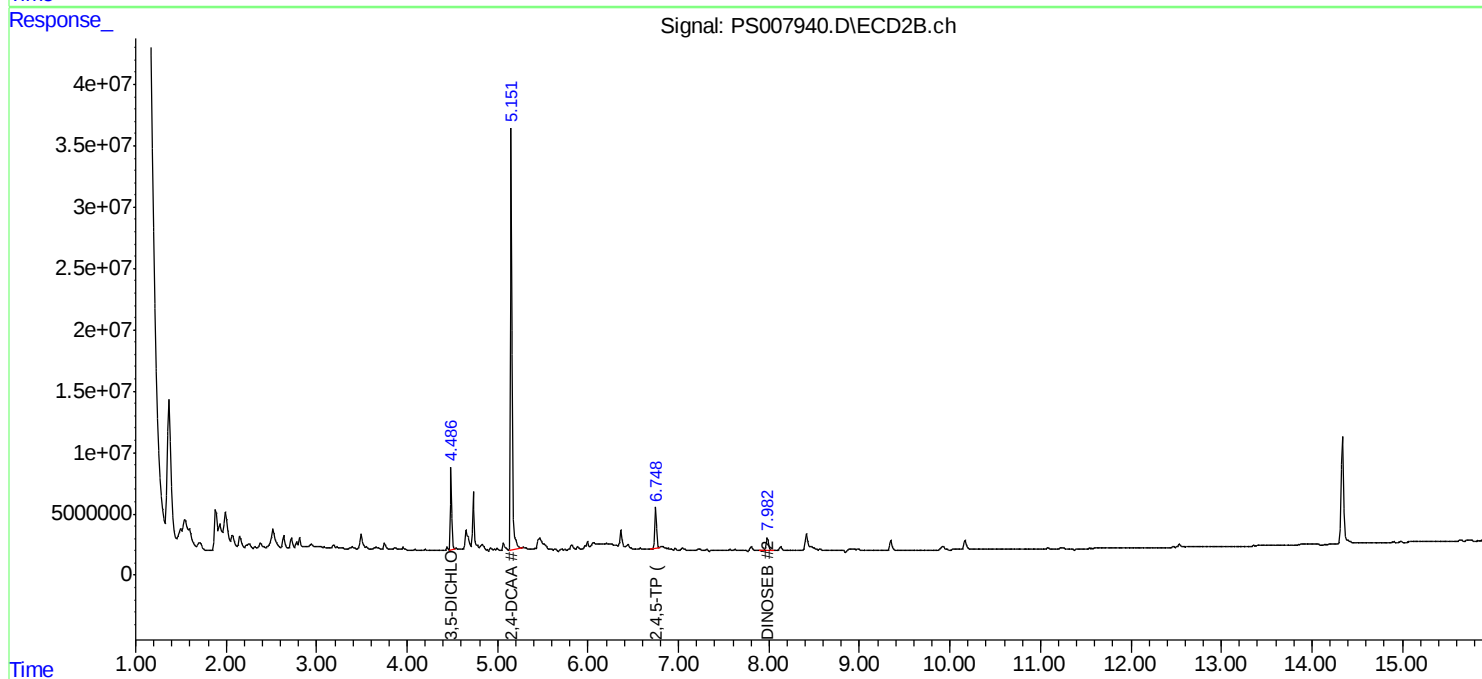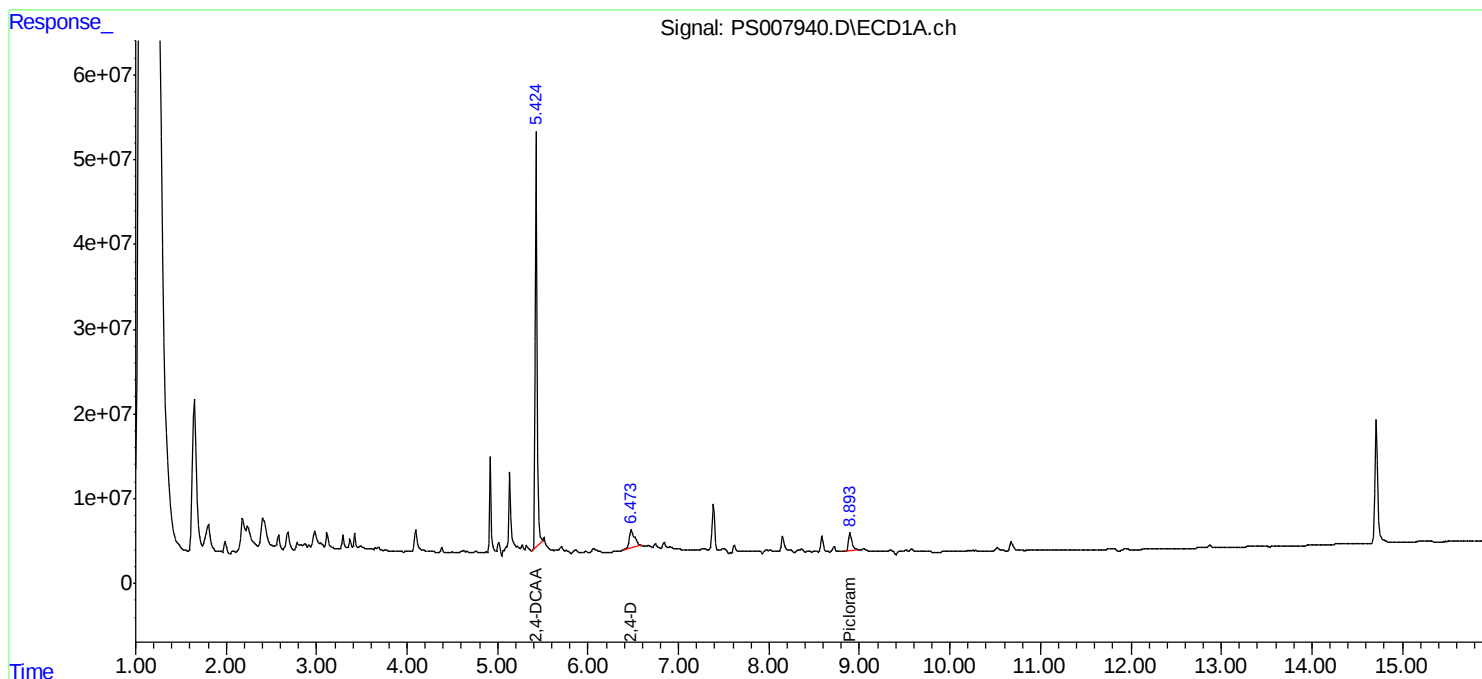


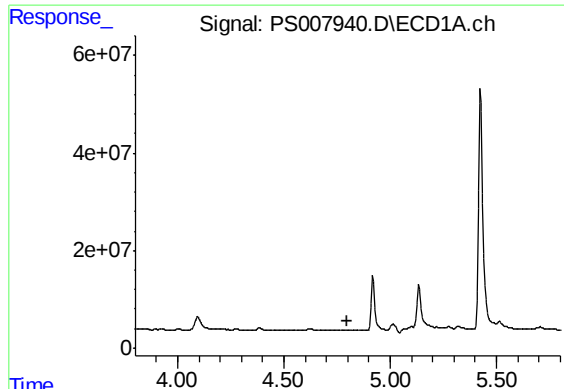

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC007

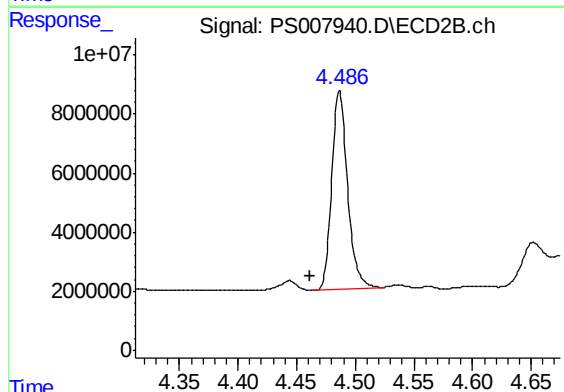


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.487 min
Delta R.T.: 0.025 min
Response: 63089599
Conc: 60.96 ng/ml

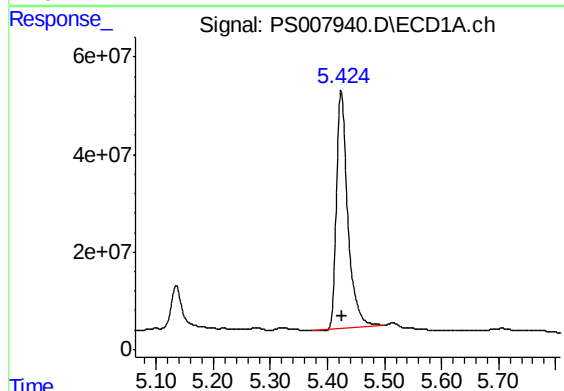


#4 2,4-DCAA

R.T.: 5.424 min
Delta R.T.: 0.000 min
Response: 670628594
Conc: 428.70 ng/ml

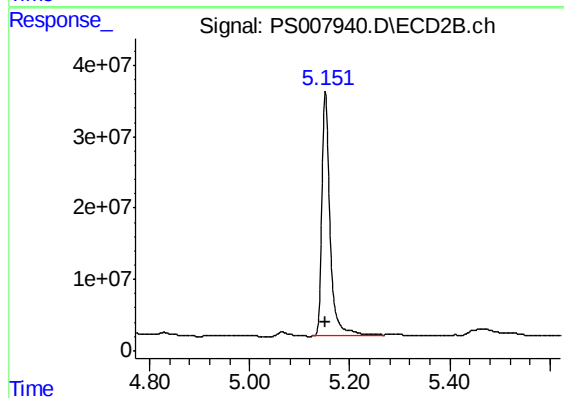

#4 2,4-DCAA


R.T.: 5.152 min
Delta R.T.: 0.000 min
Response: 384416419
Conc: 495.43 ng/ml

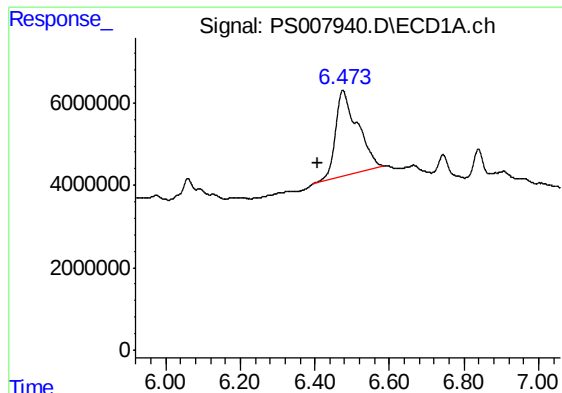

#9 2,4-D


R.T.: 6.475 min
Delta R.T.: 0.067 min
Response: 84320468
Conc: 52.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
P001-WC007

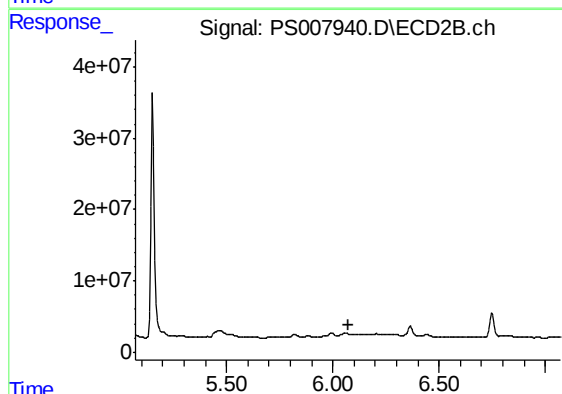


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

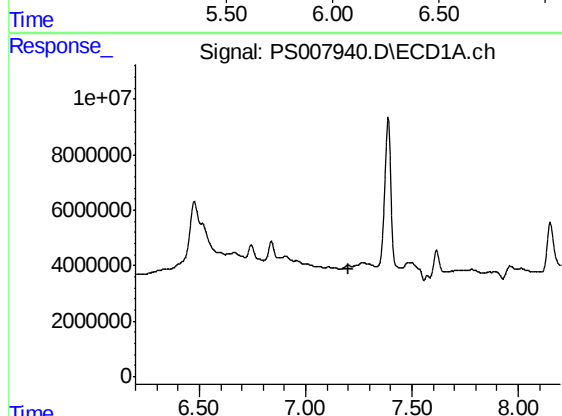


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

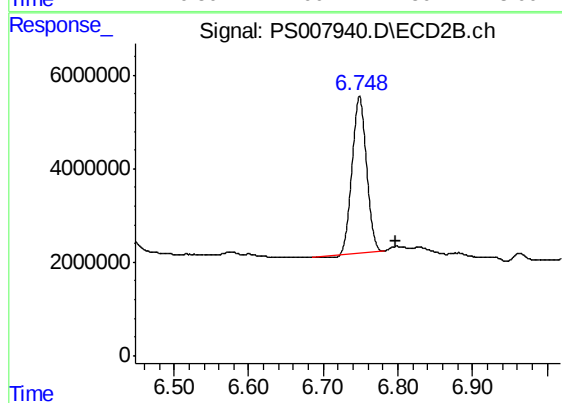

#11 2,4,5-TP (SILVEX)


R.T.: 6.749 min
Delta R.T.: -0.049 min
Response: 45101322
Conc: 10.52 ng/ml

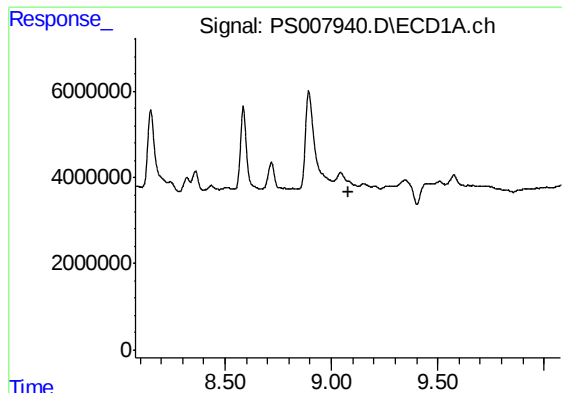

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.078 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC007

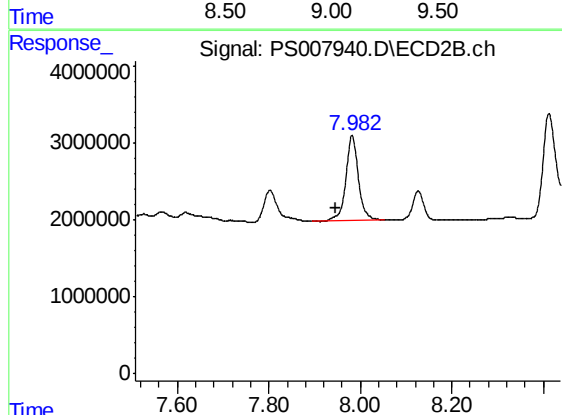


#14 DINOSEB

R.T.: 7.982 min
Delta R.T.: 0.035 min
Response: 20815995
Conc: 6.36 ng/ml

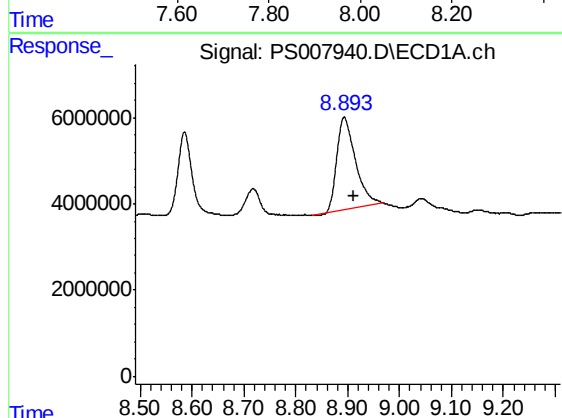

#15 Picloram

R.T.: 8.893 min
Delta R.T.: -0.017 min
Response: 53559178
Conc: 4.43 ng/ml

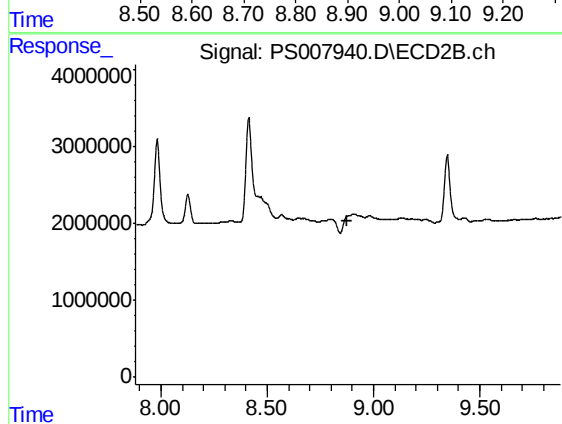

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.879 min
Response: 0
Conc: N.D.