

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007941.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2019 00:48
 Operator : SM\AJ
 Sample : K6147-19
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 P001-WC008

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 02:23:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.423	5.150	759.7E6	428.2E6	485.616	551.907
Target Compounds							
2) T	3,5-DICHL...	0.000	4.485	0 70478952	N.D.	68.104	
3) T	4-Nitroph...	0.000	4.828	0 11989609	N.D.	26.476	
8) T	DICHLORPROP	0.000	5.816	0 6777371	N.D.	9.455	
9) T	2,4-D	6.476	0.000	78351597	0	48.702	N.D. #
11) T	2,4,5-TP ...	0.000	6.748	0 48886532	N.D.	11.399	
14) T	DINOSEB	0.000	7.981	0 21634571	N.D.	6.613	
15) T	Picloram	8.893	0.000	58609757	0	4.847	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007941.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2019 00:48
Operator : SM\AJ
Sample : K6147-19
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
P001-WC008

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 02:23:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

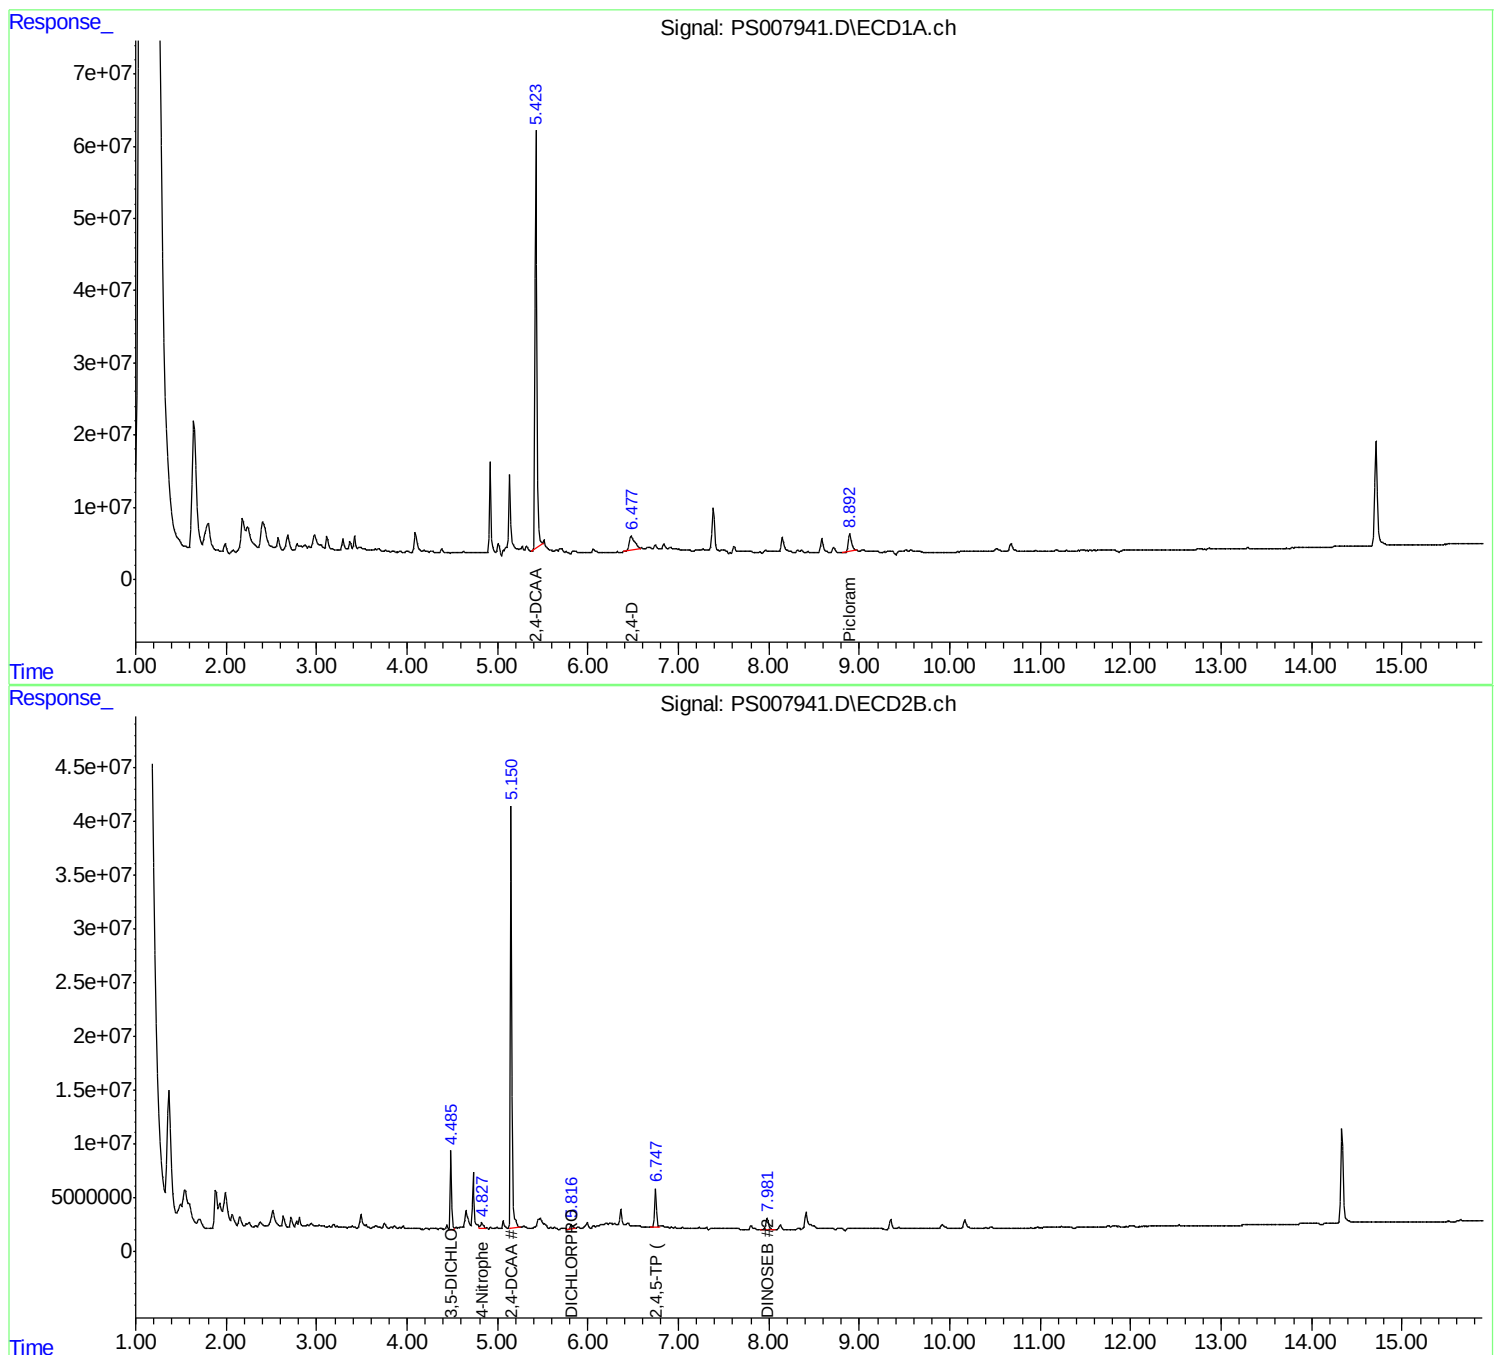


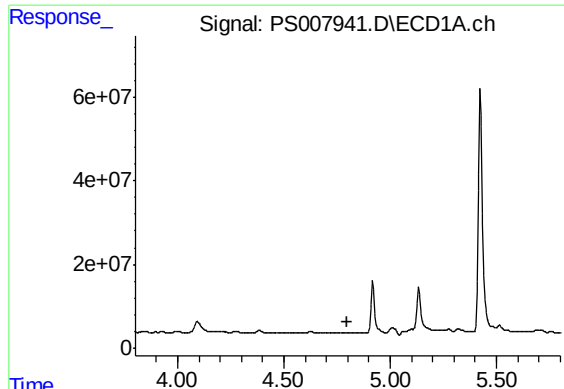

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC008

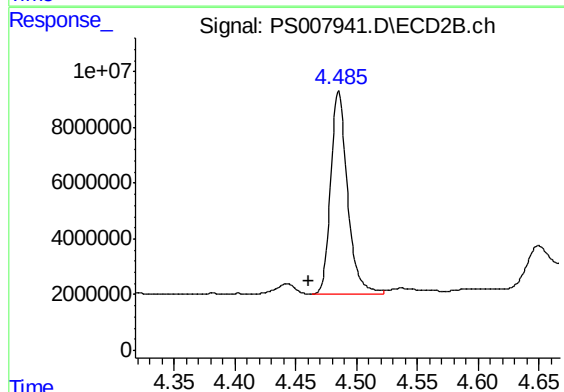


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.485 min
Delta R.T.: 0.024 min
Response: 70478952
Conc: 68.10 ng/ml

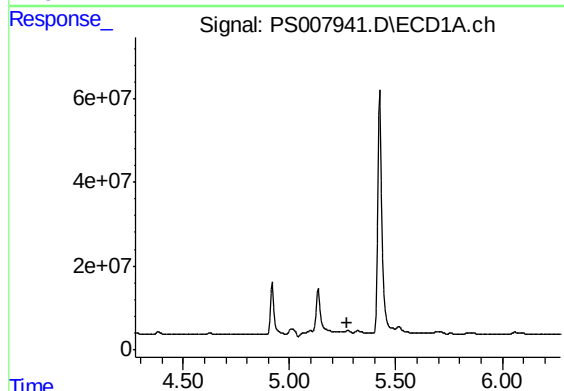


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

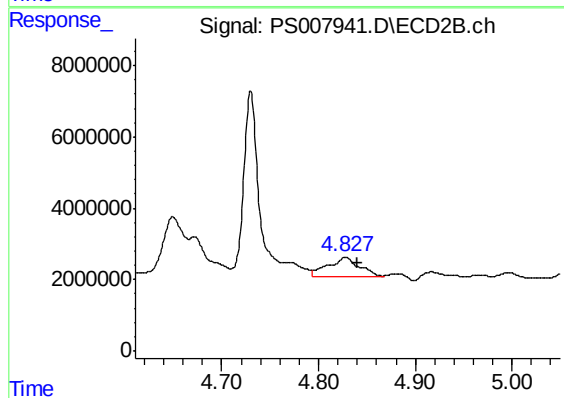

#3 4-Nitrophenol


R.T.: 4.828 min
Delta R.T.: -0.013 min
Response: 11989609
Conc: 26.48 ng/ml

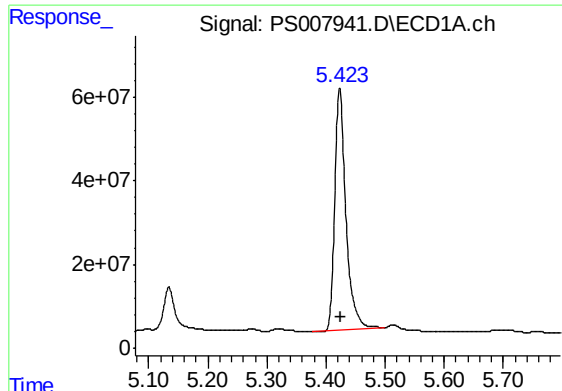

#4 2,4-DCAA


R.T.: 5.423 min
Delta R.T.: -0.002 min
Response: 759665191
Conc: 485.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
P001-WC008

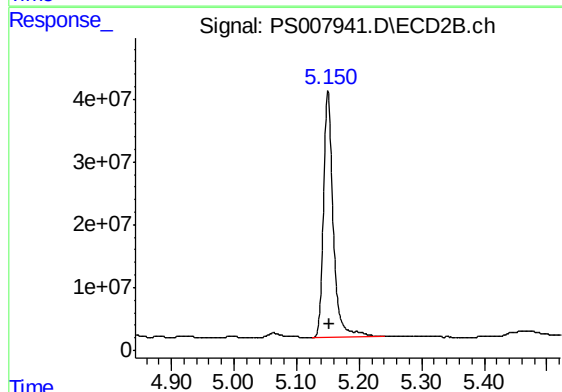


#4 2,4-DCAA

R.T.: 5.150 min
Delta R.T.: -0.002 min
Response: 428234391
Conc: 551.91 ng/ml

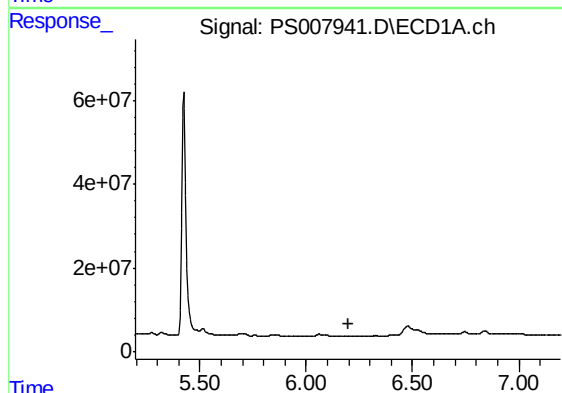


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.197 min
Response: 0
Conc: N.D.

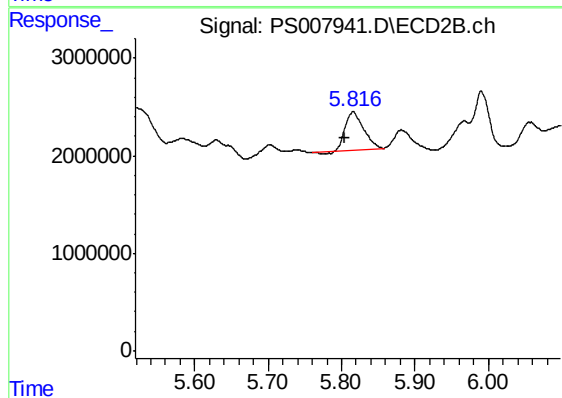

#8 DICHLORPROP


R.T.: 5.816 min
Delta R.T.: 0.012 min
Response: 6777371
Conc: 9.45 ng/ml

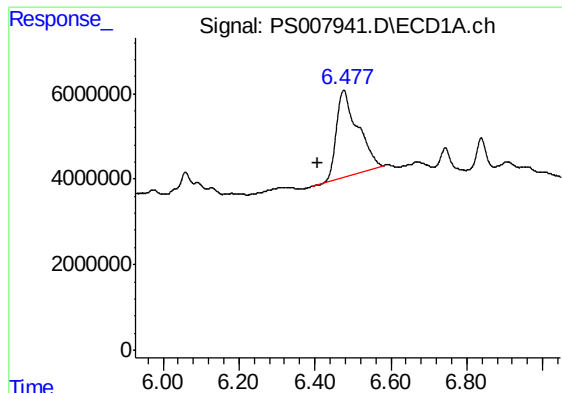

#9 2,4-D


R.T.: 6.476 min
Delta R.T.: 0.068 min
Response: 78351597
Conc: 48.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
P001-WC008

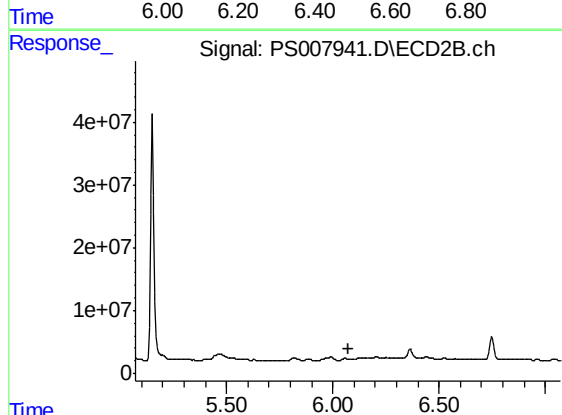


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

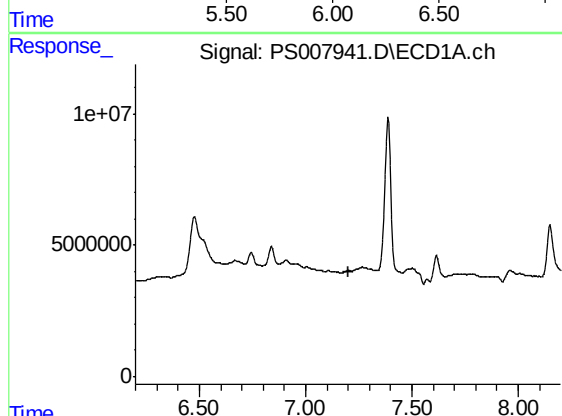


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

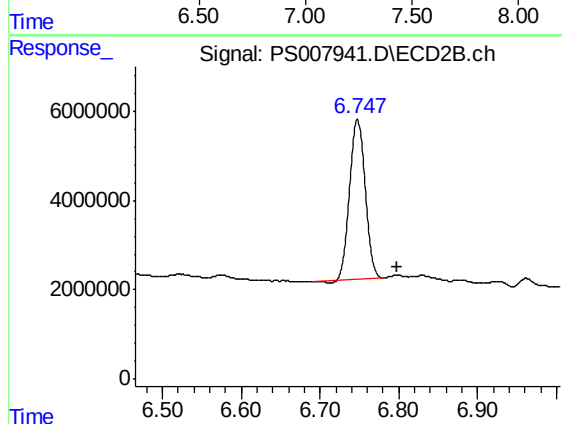

#11 2,4,5-TP (SILVEX)


R.T.: 6.748 min
Delta R.T.: -0.050 min
Response: 48886532
Conc: 11.40 ng/ml

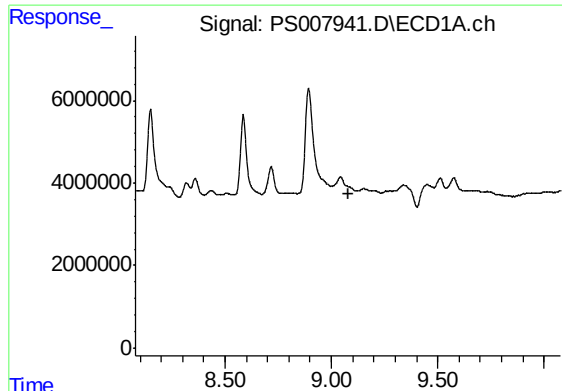

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.078 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC008

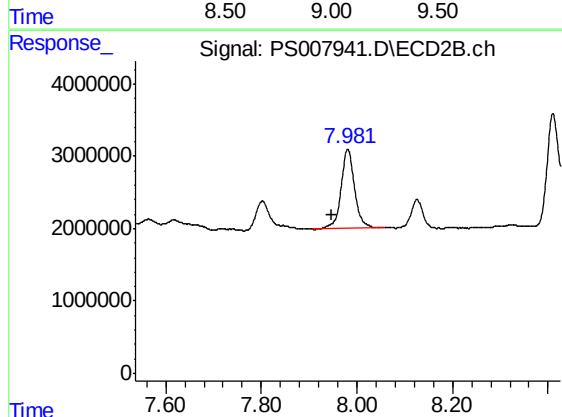


#14 DINOSEB

R.T.: 7.981 min
Delta R.T.: 0.034 min
Response: 21634571
Conc: 6.61 ng/ml

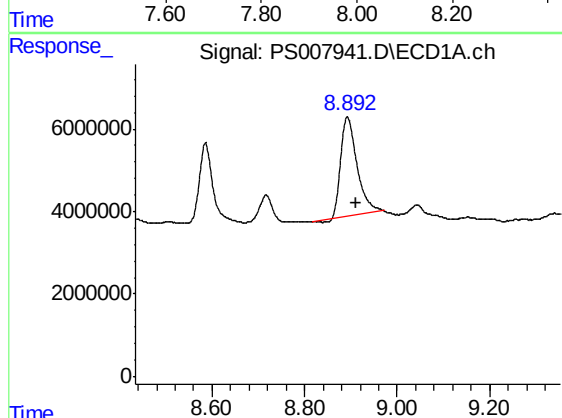

#15 Picloram

R.T.: 8.893 min
Delta R.T.: -0.018 min
Response: 58609757
Conc: 4.85 ng/ml

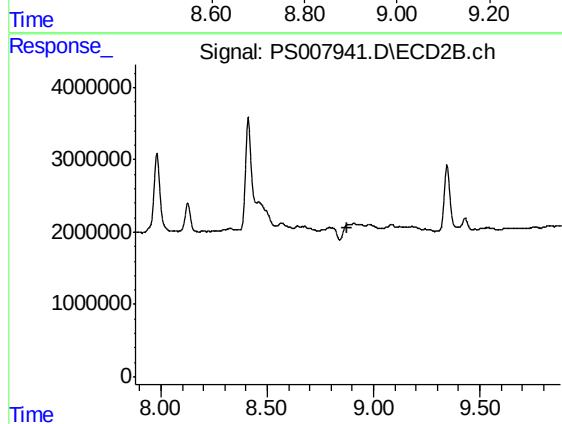

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.879 min
Response: 0
Conc: N.D.