

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
 Data File : PS007945.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2019 02:15
 Operator : SM\AJ
 Sample : K6147-21
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 P001-WC010

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 03:43:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.426	5.153	497.8E6	300.2E6	318.205	386.948
Target Compounds							
2) T	3,5-DICHL...	0.000	4.487	0 58675308		N.D.	56.698
3) T	4-Nitroph...	0.000	4.830	0 18452379		N.D.	40.747
8) T	DICHLORPROP	0.000	5.816	0 9943002		N.D.	13.871
9) T	2,4-D	6.474	0.000	84429330	0	52.480	N.D. #
10) T	Pentachlo...	0.000	6.439	0 13482084		N.D.	1.235
11) T	2,4,5-TP ...	0.000	6.749	0 39321224		N.D.	9.168
12) T	2,4,5-T	0.000	7.216	0 24128083		N.D.	5.928
14) T	DINOSEB	0.000	7.982	0 27954033		N.D.	8.545
15) T	Picloram	8.897	8.902	54717229	81638395	4.525	13.217 #
16) T	DCPA	0.000	8.902	0 81638395		N.D.	14.226



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120619\
Data File : PS007945.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2019 02:15
Operator : SM\AJ
Sample : K6147-21
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
P001-WC010

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 03:43:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

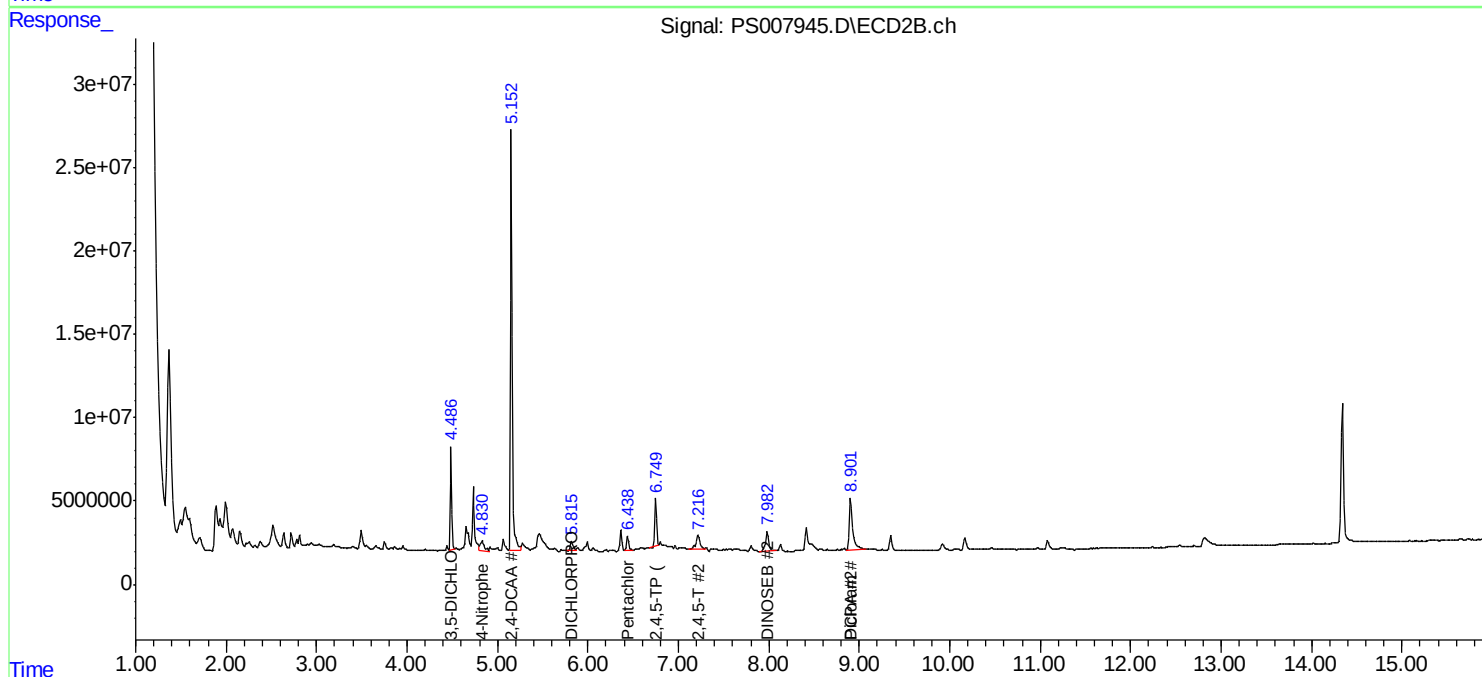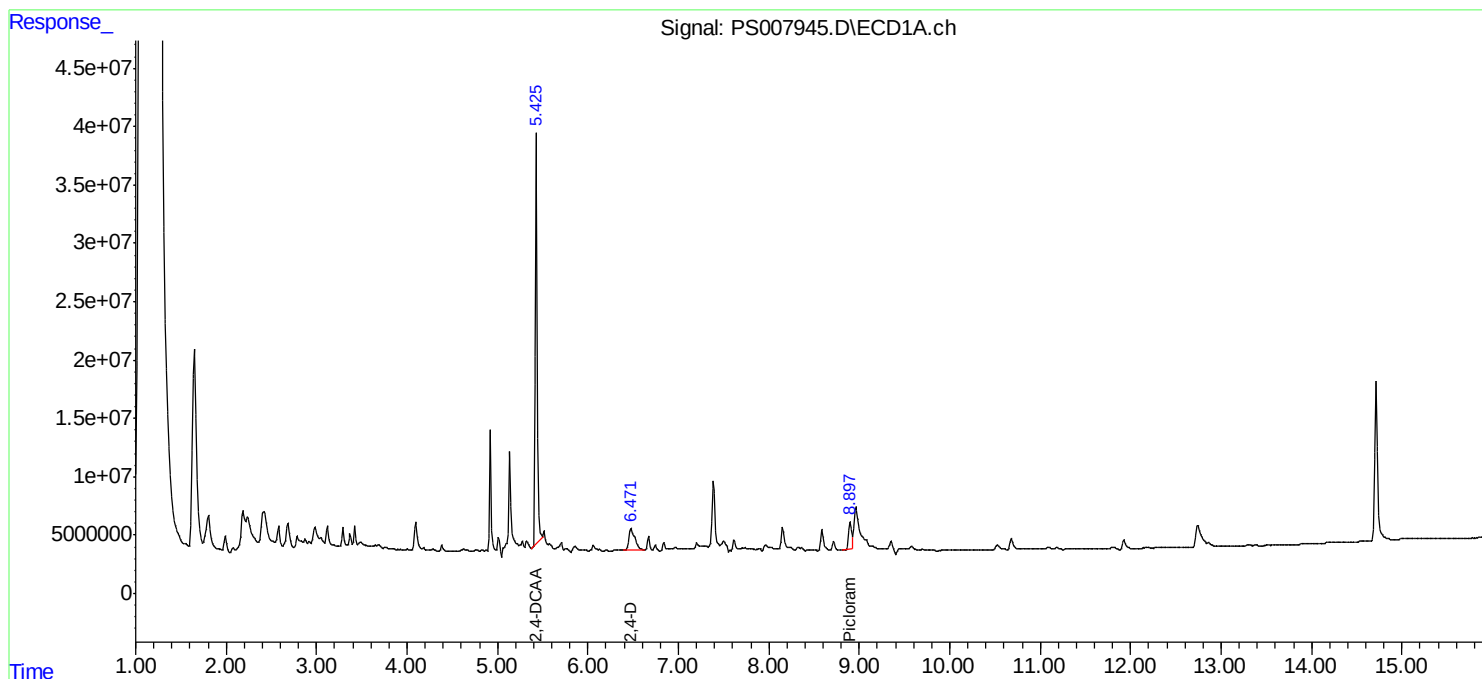


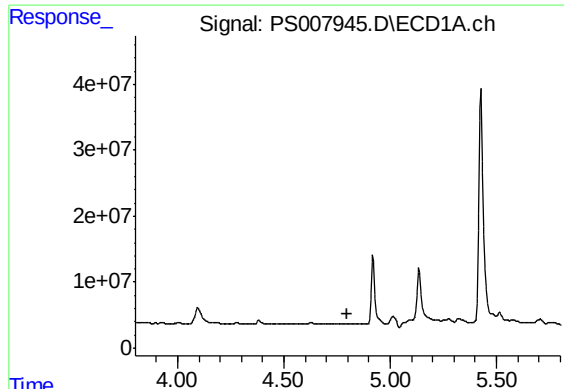

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC010

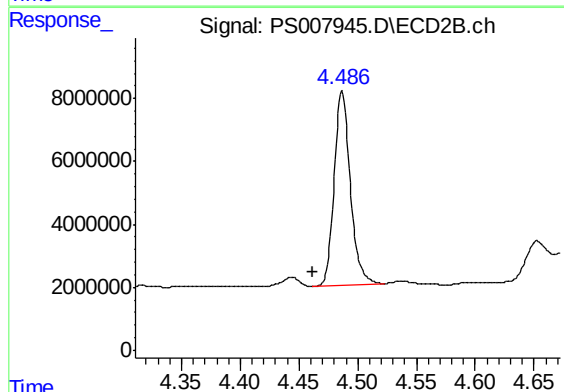


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.487 min
Delta R.T.: 0.025 min
Response: 58675308
Conc: 56.70 ng/ml

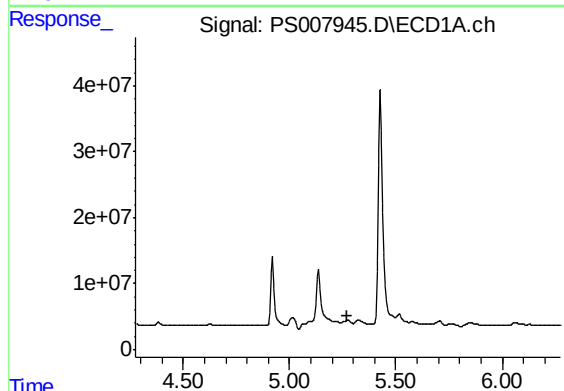


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

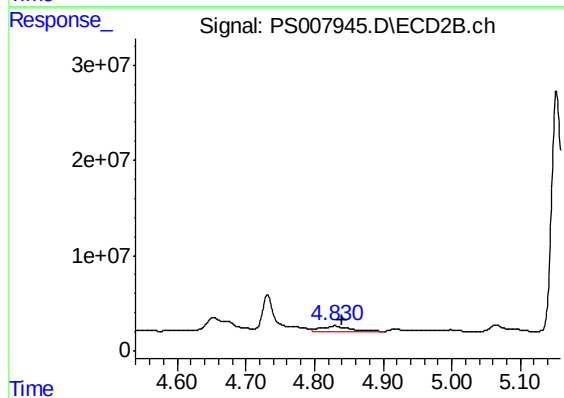

#3 4-Nitrophenol


R.T.: 4.830 min
Delta R.T.: -0.011 min
Response: 18452379
Conc: 40.75 ng/ml

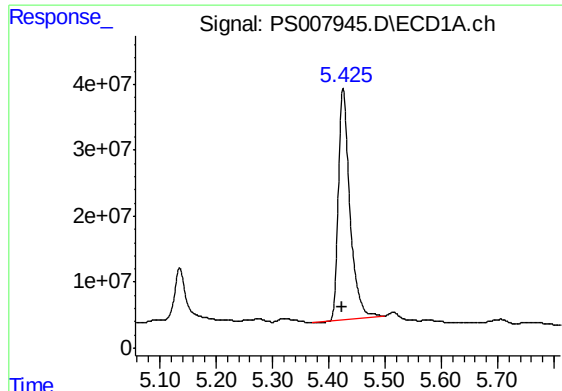

#4 2,4-DCAA


R.T.: 5.426 min
Delta R.T.: 0.000 min
Response: 497778275
Conc: 318.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
P001-WC010

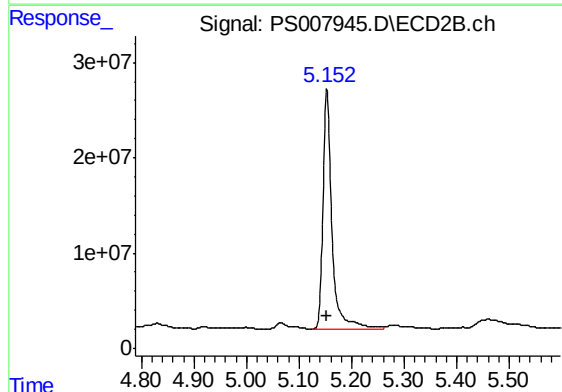


#4 2,4-DCAA

R.T.: 5.153 min
Delta R.T.: 0.000 min
Response: 300240131
Conc: 386.95 ng/ml

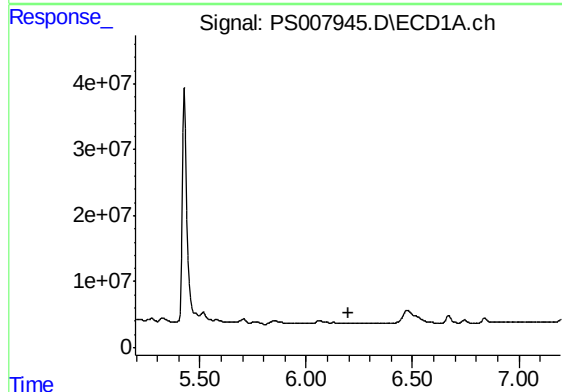


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.197 min
Response: 0
Conc: N.D.

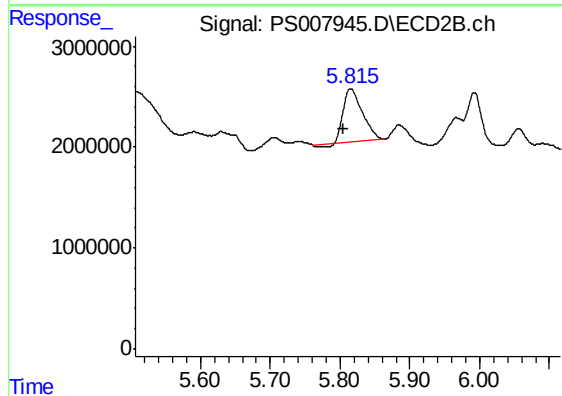

#8 DICHLORPROP


R.T.: 5.816 min
Delta R.T.: 0.011 min
Response: 9943002
Conc: 13.87 ng/ml

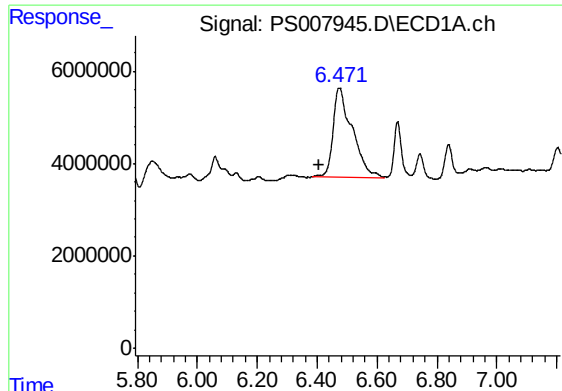

#9 2,4-D


R.T.: 6.474 min
Delta R.T.: 0.066 min
Response: 84429330
Conc: 52.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
P001-WC010

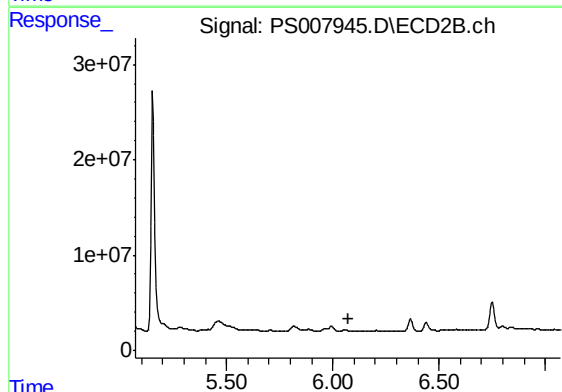


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

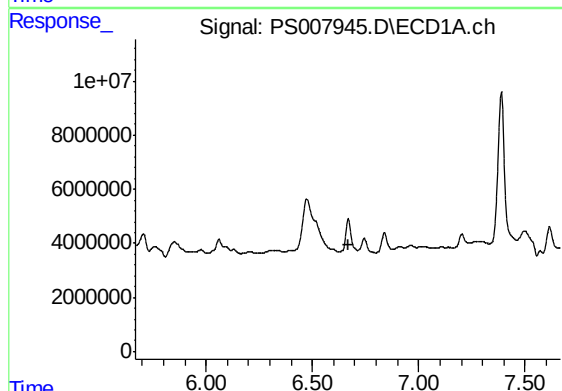


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.667 min
Response: 0
Conc: N.D.

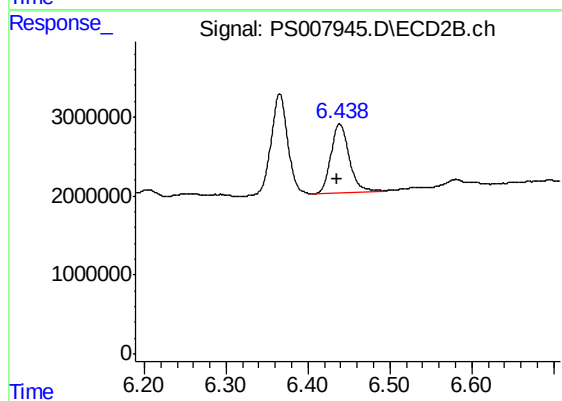

#10 Pentachlorophenol


R.T.: 6.439 min
Delta R.T.: 0.003 min
Response: 13482084
Conc: 1.24 ng/ml

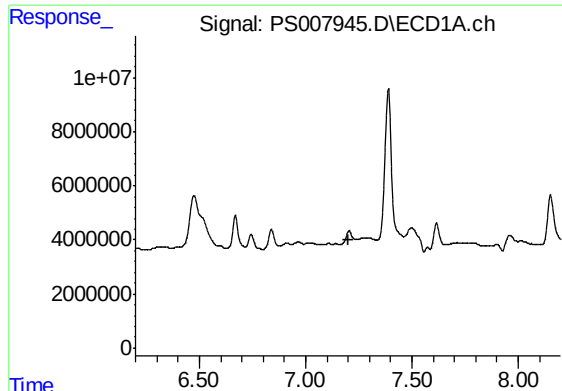

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC010

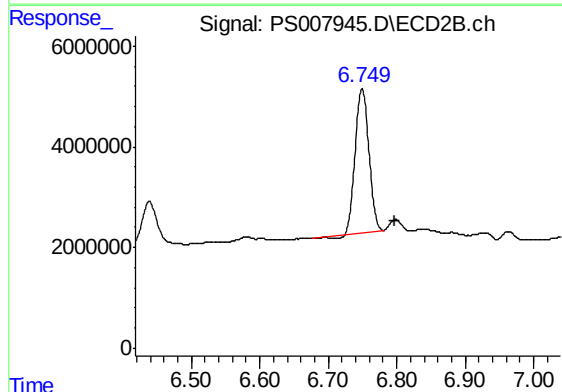


#11 2,4,5-TP (SILVEX)

R.T.: 6.749 min
Delta R.T.: -0.048 min
Response: 39321224
Conc: 9.17 ng/ml

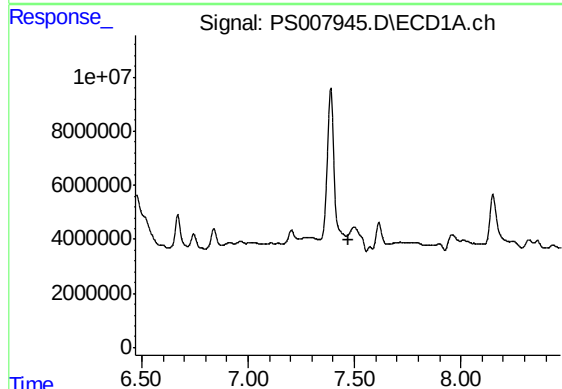


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.470 min
Response: 0
Conc: N.D.

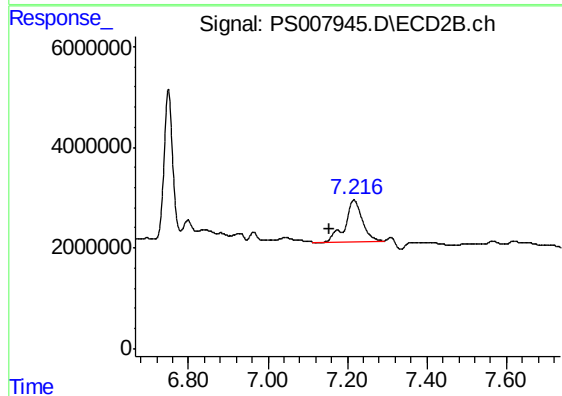

#12 2,4,5-T


R.T.: 7.216 min
Delta R.T.: 0.061 min
Response: 24128083
Conc: 5.93 ng/ml

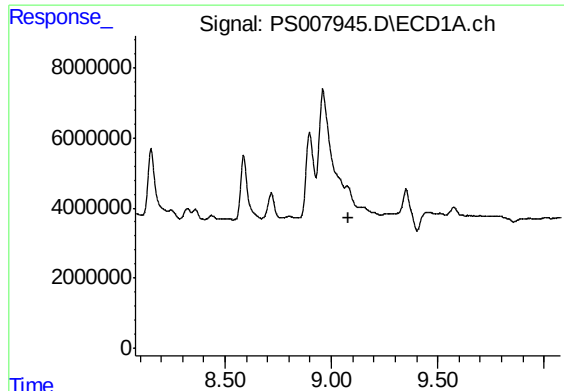

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.078 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC010

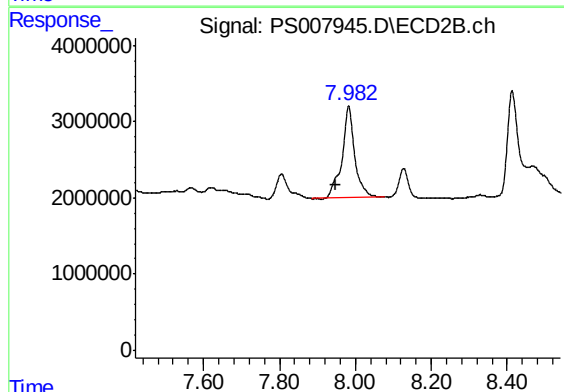


#14 DINOSEB

R.T.: 7.982 min
Delta R.T.: 0.035 min
Response: 27954033
Conc: 8.55 ng/ml

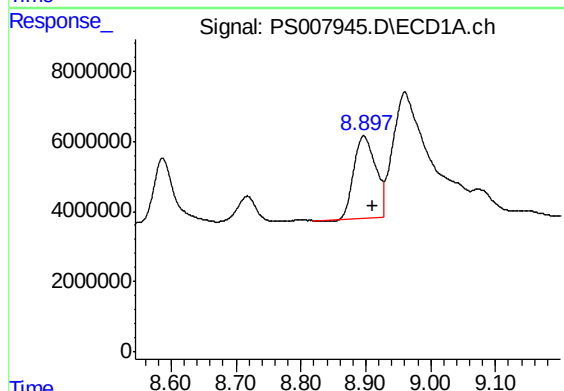


#15 Picloram

R.T.: 8.897 min
Delta R.T.: -0.013 min
Response: 54717229
Conc: 4.53 ng/ml

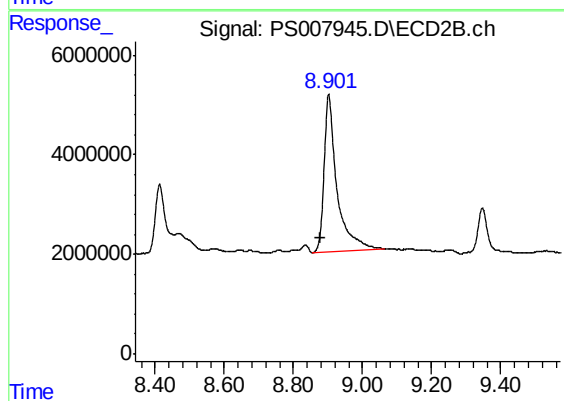

#15 Picloram


R.T.: 8.902 min
Delta R.T.: 0.023 min
Response: 81638395
Conc: 13.22 ng/ml

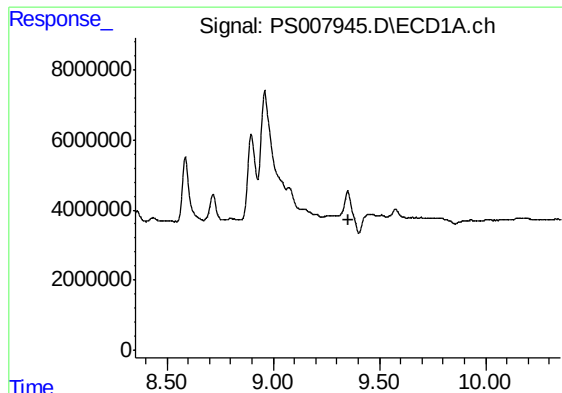

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
P001-WC010

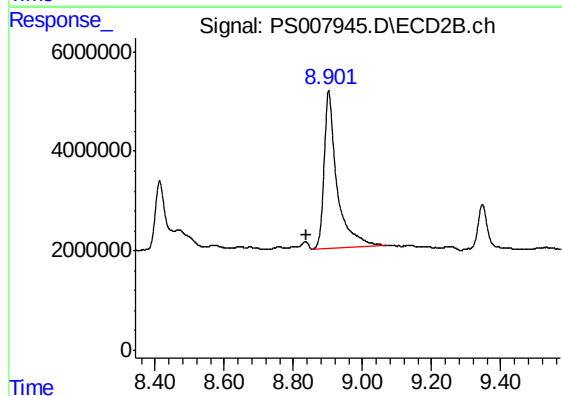

#16 DCPA

R.T.: 8.902 min
Delta R.T.: 0.065 min
Response: 81638395
Conc: 14.23 ng/ml