

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120622\
 Data File : PS021334.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2022 09:20
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 12:58:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
 Quant Title : 8080.M
 QLast Update : Thu Nov 17 00:46:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.413	6.845	1032.6E6	803.9E6	474.907	531.606
Target Compounds							
1) T	Dalapon	2.546f	0.000	858940	0	<MDL	N.D. #
3) T	4-Nitroph...	6.260	0.000	7701793	0	5.701	N.D. #
7) T	MCPA	6.804f	0.000	868379	0	<MDL	N.D. #
8) T	DICHLORPROP	7.148	0.000	591251	0	<MDL	N.D. #
10) T	Pentachlo...	7.591	0.000	469228	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.106	8.715	3290994	3117957	<MDL	<MDL #
12) T	2,4,5-T	8.336	0.000	527311	0	<MDL	N.D. #
13) T	2,4-DB	0.000	9.583	0	2739843	N.D.	2.340
14) T	DINOSEB	9.952	0.000	1479882	0	<MDL	N.D. #
15) T	Picloram	9.806	0.000	5541088	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120622\
Data File : PS021334.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2022 09:20
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 12:58:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
Quant Title : 8080.M
QLast Update : Thu Nov 17 00:46:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

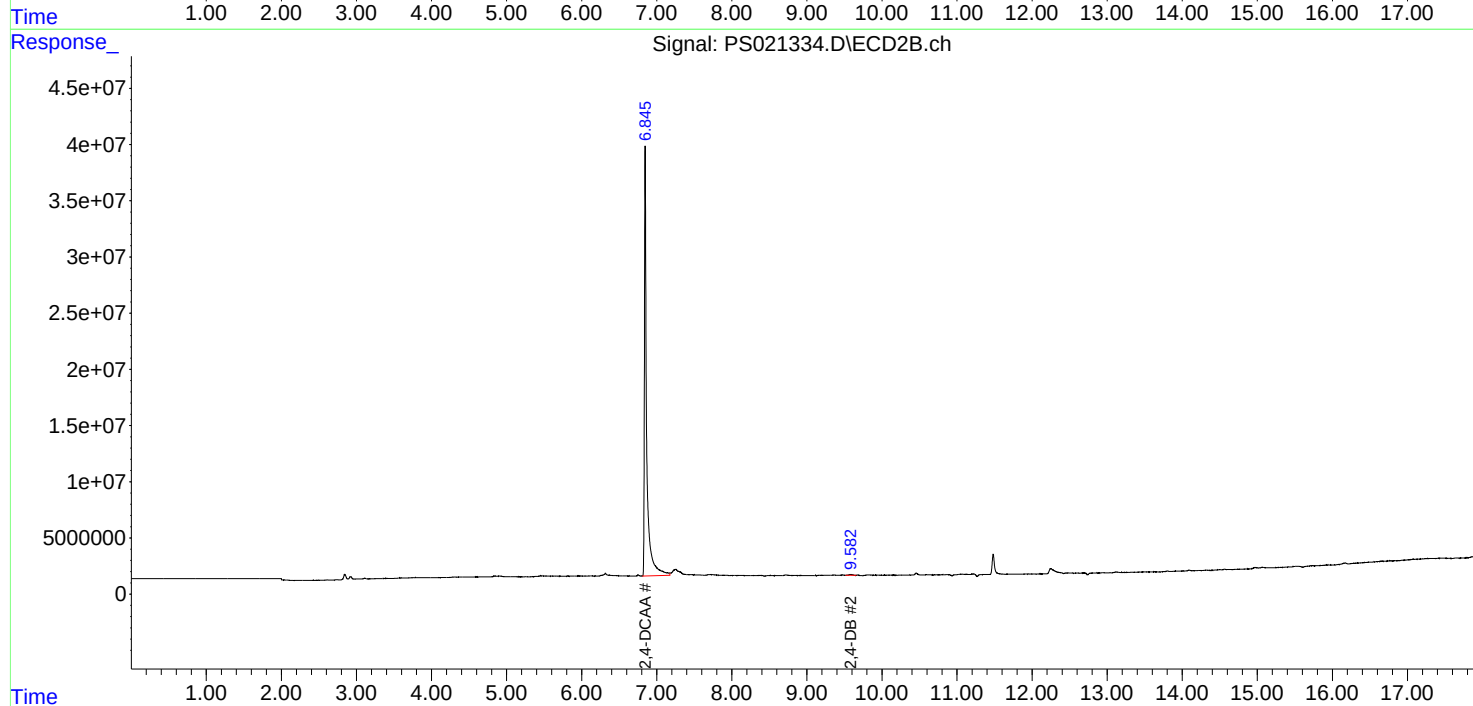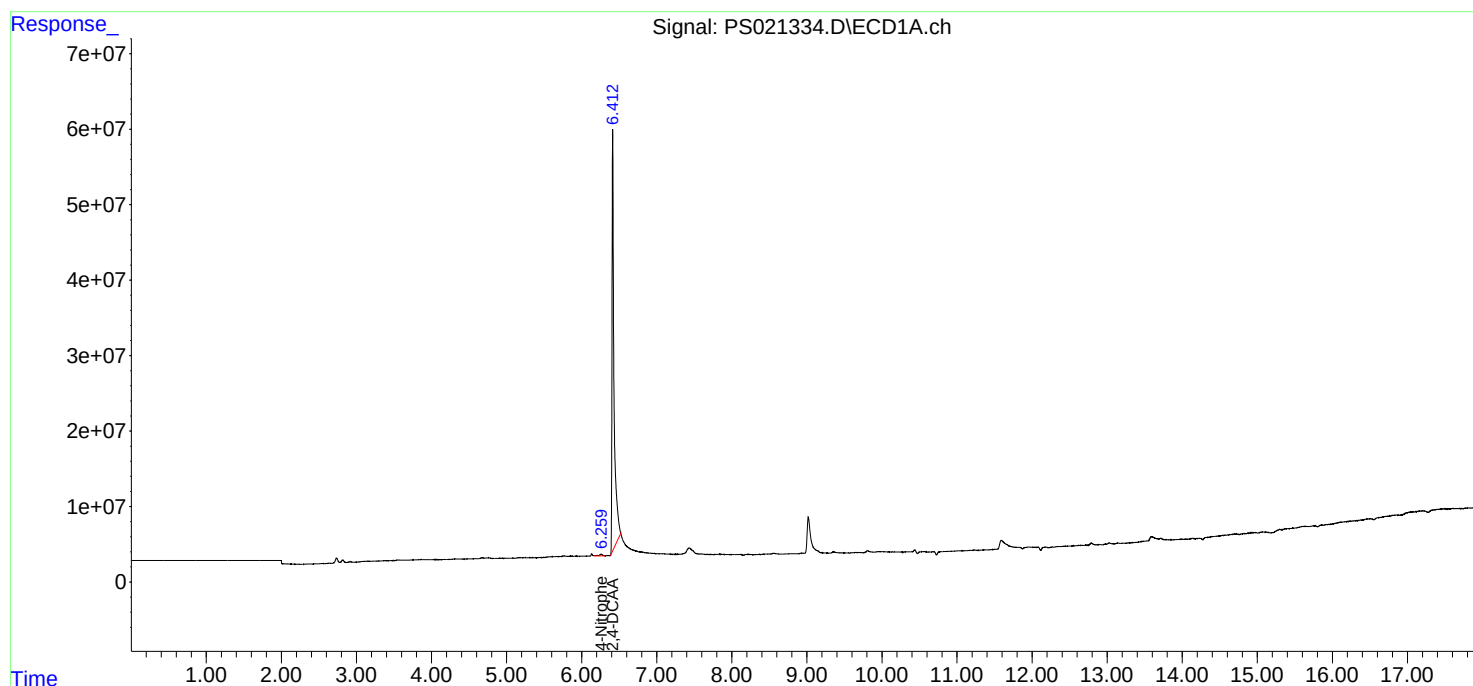


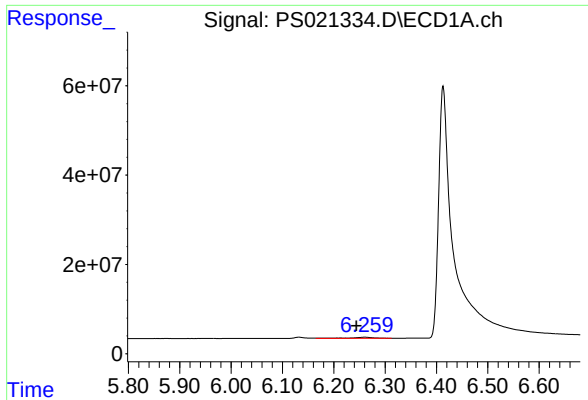

#3 4-Nitrophenol


R.T.: 6.260 min
Delta R.T.: 0.016 min
Response: 7701793
Conc: 5.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

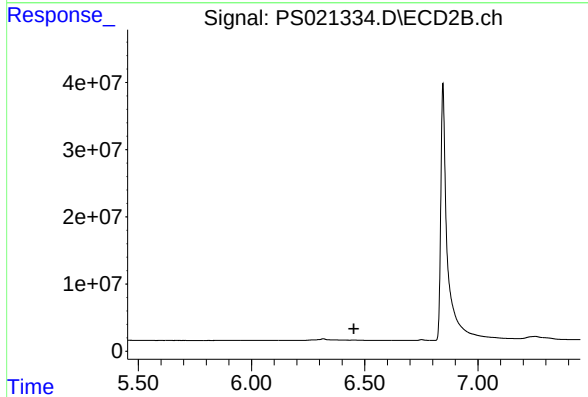


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.452 min
Response: 0
Conc: N.D.

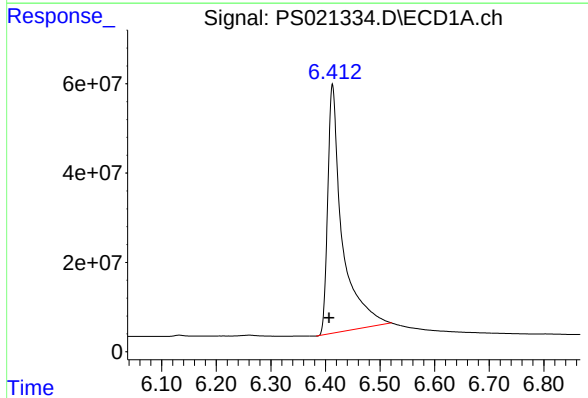


#4 2,4-DCAA

R.T.: 6.413 min
Delta R.T.: 0.006 min
Response: 1032587748
Conc: 474.91 ng/ml

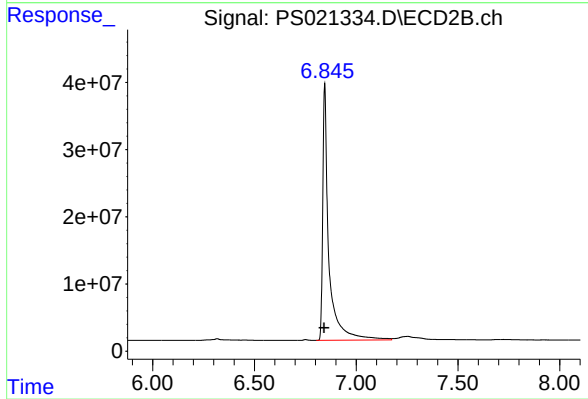

#4 2,4-DCAA


R.T.: 6.845 min
Delta R.T.: 0.003 min
Response: 803850297
Conc: 531.61 ng/ml

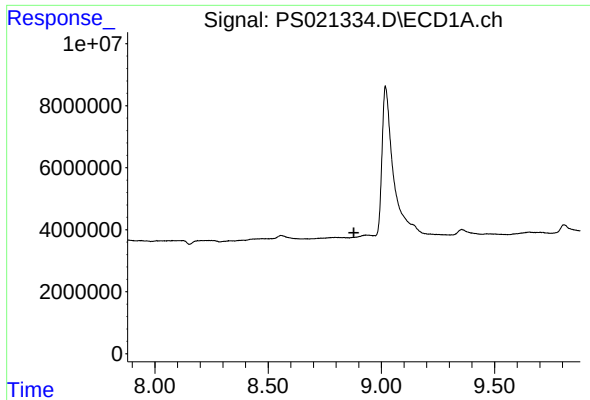

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.879 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

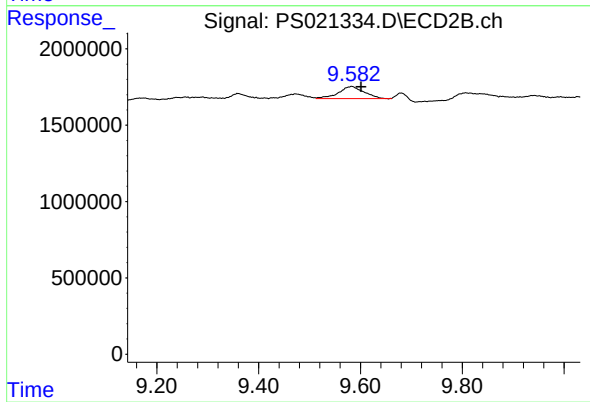

#13 2,4-DB

R.T.: 9.583 min
Delta R.T.: -0.018 min
Response: 2739843
Conc: 2.34 ng/ml