

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120622\
 Data File : PS021367.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2022 01:45
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 03:53:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
 Quant Title : 8080.M
 QLast Update : Thu Nov 17 00:46:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.409	6.842	1174.9E6	795.7E6	540.344	526.198
Target Compounds							
1) T	Dalapon	2.538	0.000	966772	0	<MDL	N.D. #
3) T	4-Nitroph...	6.250	0.000	6624201	0	4.903	N.D. #
5) T	DICAMBA	0.000	7.064f	0	3117152	N.D.	<MDL
6) T	MCP	0.000	7.064f	0	3117152	N.D.	<MDL
7) T	MCPA	6.787f	0.000	13210359	0	1.374	N.D. #
8) T	DICHLORPROP	7.162	7.671	386680	5907825	<MDL	3.460 #
9) T	2,4-D	7.352	0.000	1837582	0	<MDL	N.D. #
10) T	Pentachlo...	7.583	8.373	1205311	6900699	<MDL	<MDL #
11) T	2,4,5-TP ...	8.122	8.687	6600452	13488379	<MDL	1.356 #
12) T	2,4,5-T	8.340	9.119	8081210	1922497	<MDL	<MDL #
13) T	2,4-DB	8.871	9.625	2470872	1124773	1.081	<MDL #
14) T	DINOSEB	9.938	0.000	3584490	0	<MDL	N.D. #
15) T	Picloram	9.768	10.886	6047372	9154349	<MDL	<MDL #
16) T	DCPA	10.201	10.858	1468848	12950551	<MDL	1.082 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120622\
Data File : PS021367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2022 01:45
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 03:53:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
Quant Title : 8080.M
QLast Update : Thu Nov 17 00:46:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

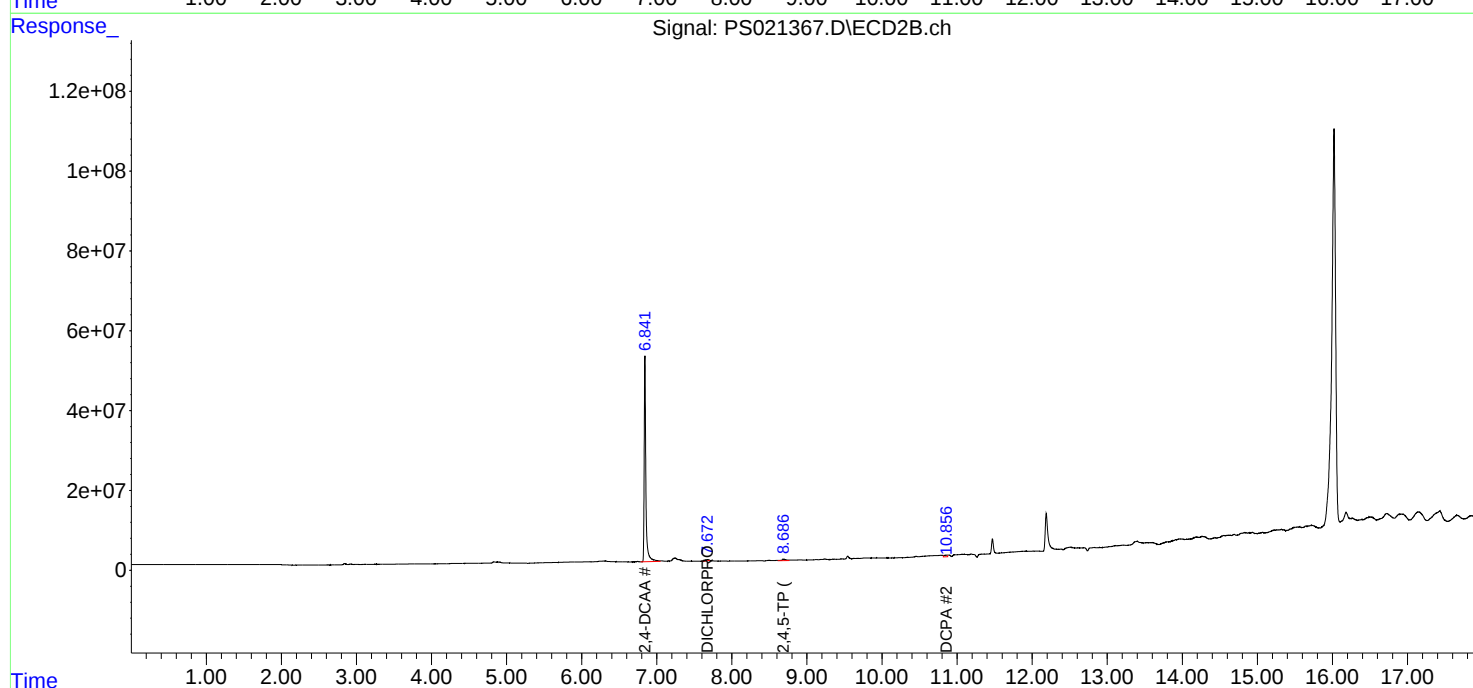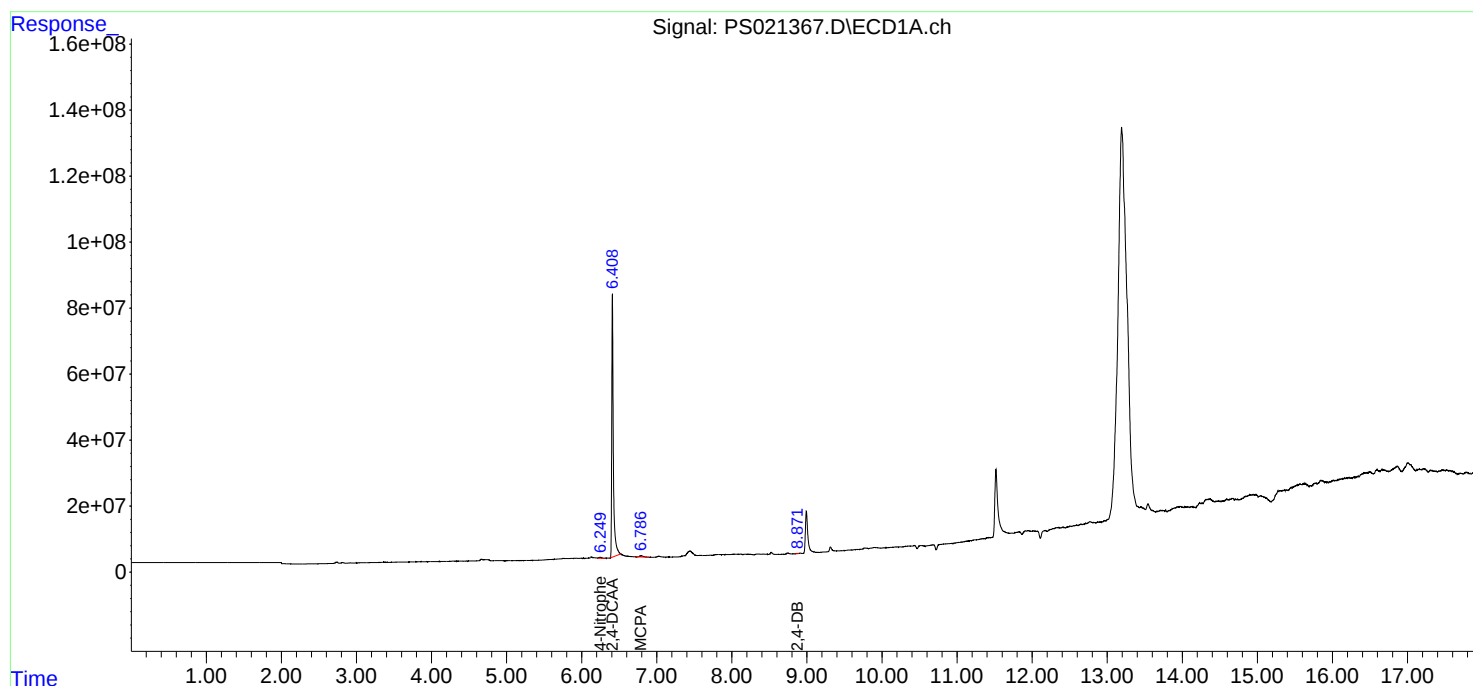


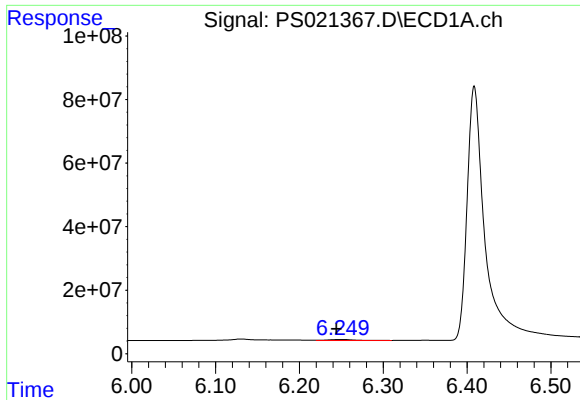

#3 4-Nitrophenol


R.T.: 6.250 min
Delta R.T.: 0.006 min
Response: 6624201
Conc: 4.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

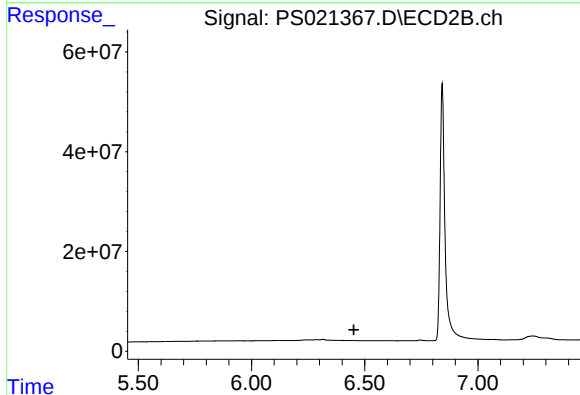


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.452 min
Response: 0
Conc: N.D.

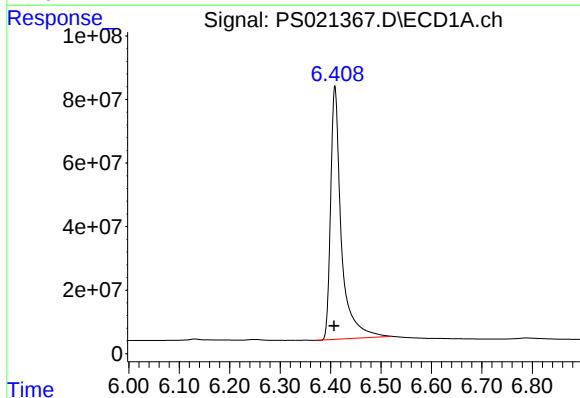


#4 2,4-DCAA

R.T.: 6.409 min
Delta R.T.: 0.002 min
Response: 1174866716
Conc: 540.34 ng/ml

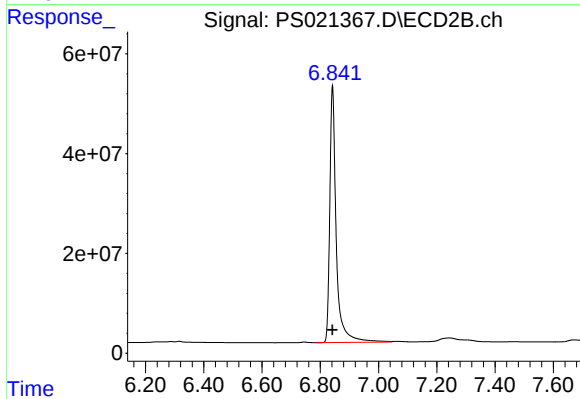

#4 2,4-DCAA


R.T.: 6.842 min
Delta R.T.: 0.000 min
Response: 795672784
Conc: 526.20 ng/ml

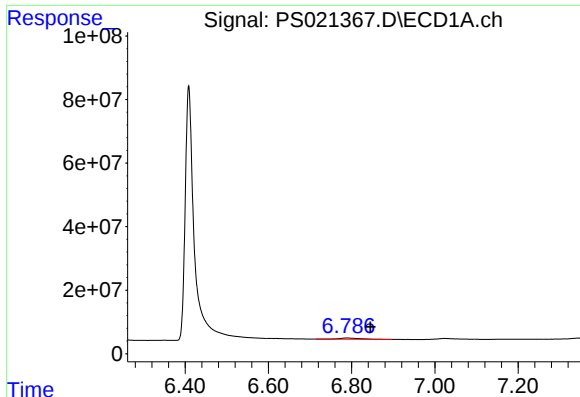

#7 MCPA


R.T.: 6.787 min
Delta R.T.: -0.058 min
Response: 13210359
Conc: 1.37 ug/ml

Instrument :
ECD_S
ClientSampleId :

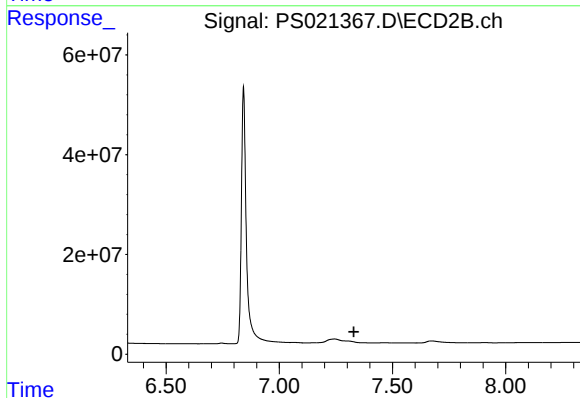


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.330 min
Response: 0
Conc: N.D.

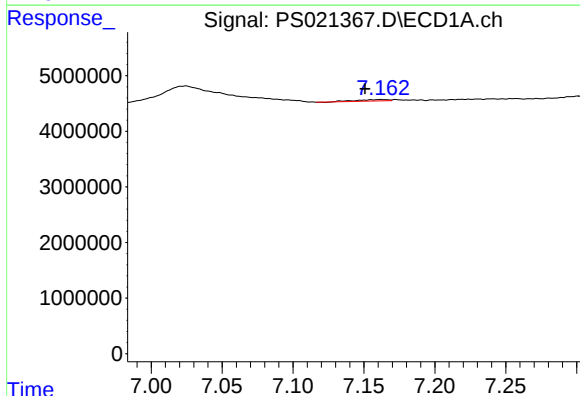


#8 DICHLORPROP

R.T.: 7.162 min
Delta R.T.: 0.011 min
Response: 386680
Conc: N.D.

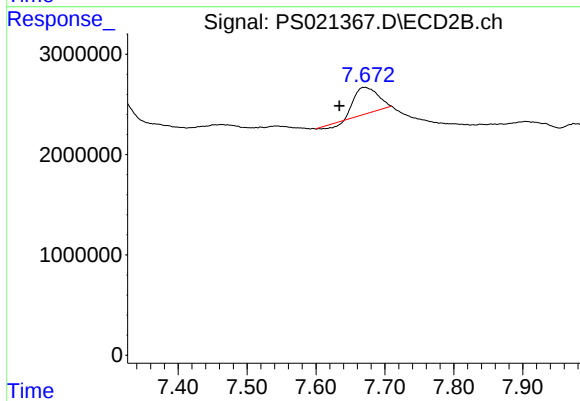

#8 DICHLORPROP


R.T.: 7.671 min
Delta R.T.: 0.037 min
Response: 5907825
Conc: 3.46 ng/ml

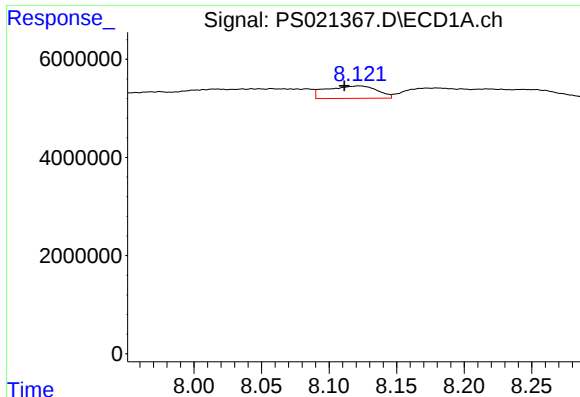

#11 2,4,5-TP (SILVEX)


R.T.: 8.122 min
Delta R.T.: 0.010 min
Response: 6600452
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

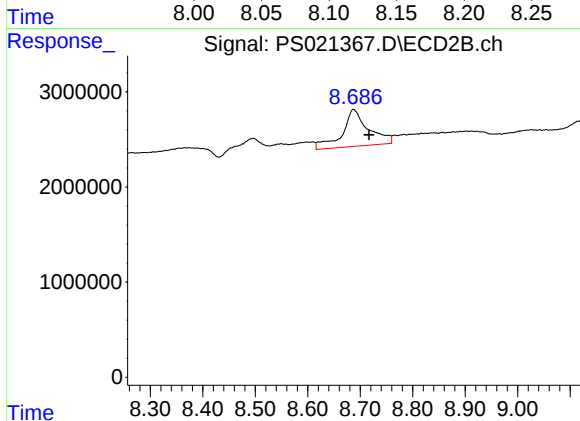


#11 2,4,5-TP (SILVEX)

R.T.: 8.687 min
Delta R.T.: -0.030 min
Response: 13488379
Conc: 1.36 ng/ml

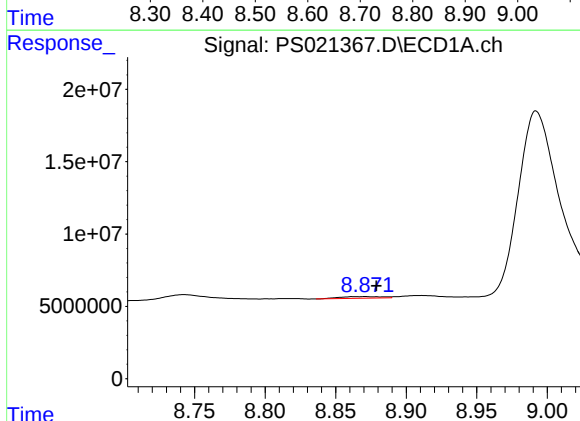


#13 2,4-DB

R.T.: 8.871 min
Delta R.T.: -0.008 min
Response: 2470872
Conc: 1.08 ng/ml

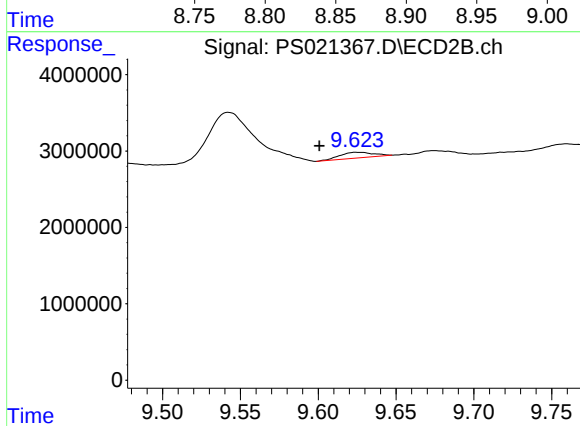

#13 2,4-DB


R.T.: 9.625 min
Delta R.T.: 0.024 min
Response: 1124773
Conc: N.D.

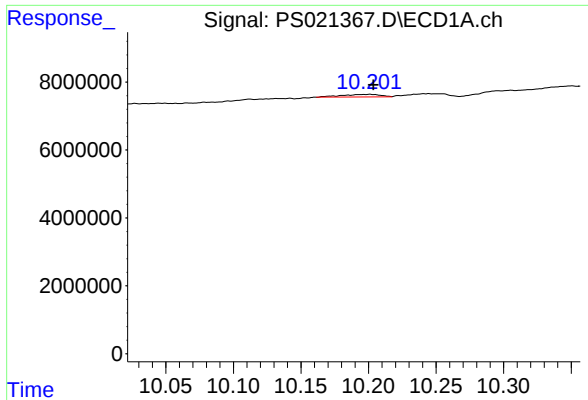

#16 DCPA

R.T.: 10.201 min
Delta R.T.: -0.003 min
Response: 1468848
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

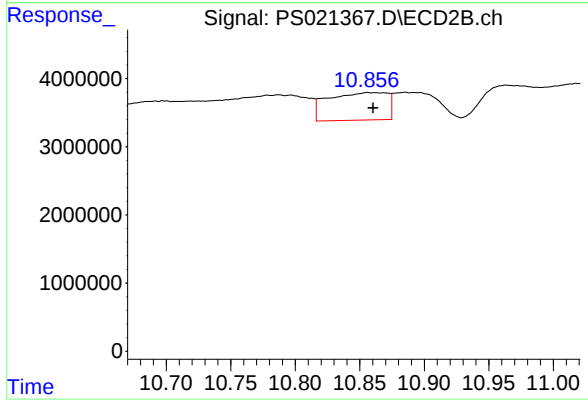

#16 DCPA

R.T.: 10.858 min
Delta R.T.: -0.002 min
Response: 12950551
Conc: 1.08 ng/ml