

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120623\
 Data File : PS025022.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2023 09:53
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:08:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	2.513f	2.564	11751108	4955508	4.075 4.320
5) T	DICAMBA	0.000	6.929	0	734697	N.D. <MDL
6) T	MCPP	6.680	6.972f	4485719	14243981	<MDL 6.867 #
7) T	MCPA	0.000	7.241	0	3482506	N.D. 1.059
8) T	DICHLORPROP	0.000	7.556	0	4043706	N.D. 5.140
9) T	2,4-D	7.246	7.830	133.0E6	321290	43.791 <MDL #
10) T	Pentachlo...	0.000	8.249	0	677933	N.D. <MDL
11) T	2,4,5-TP ...	0.000	8.608	0	373173	N.D. <MDL
12) T	2,4,5-T	8.292	8.979	8923844	1682483	<MDL <MDL #
13) T	2,4-DB	0.000	9.477	0	835942	N.D. 1.510
14) T	DINOSEB	0.000	9.809	0	988018	N.D. <MDL
15) T	Picloram	9.678	10.762	144.2E6	40195500	7.398 6.141
16) T	DCPA	0.000	10.762	0	40195500	N.D. 7.416



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120623\
Data File : PS025022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2023 09:53
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:08:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

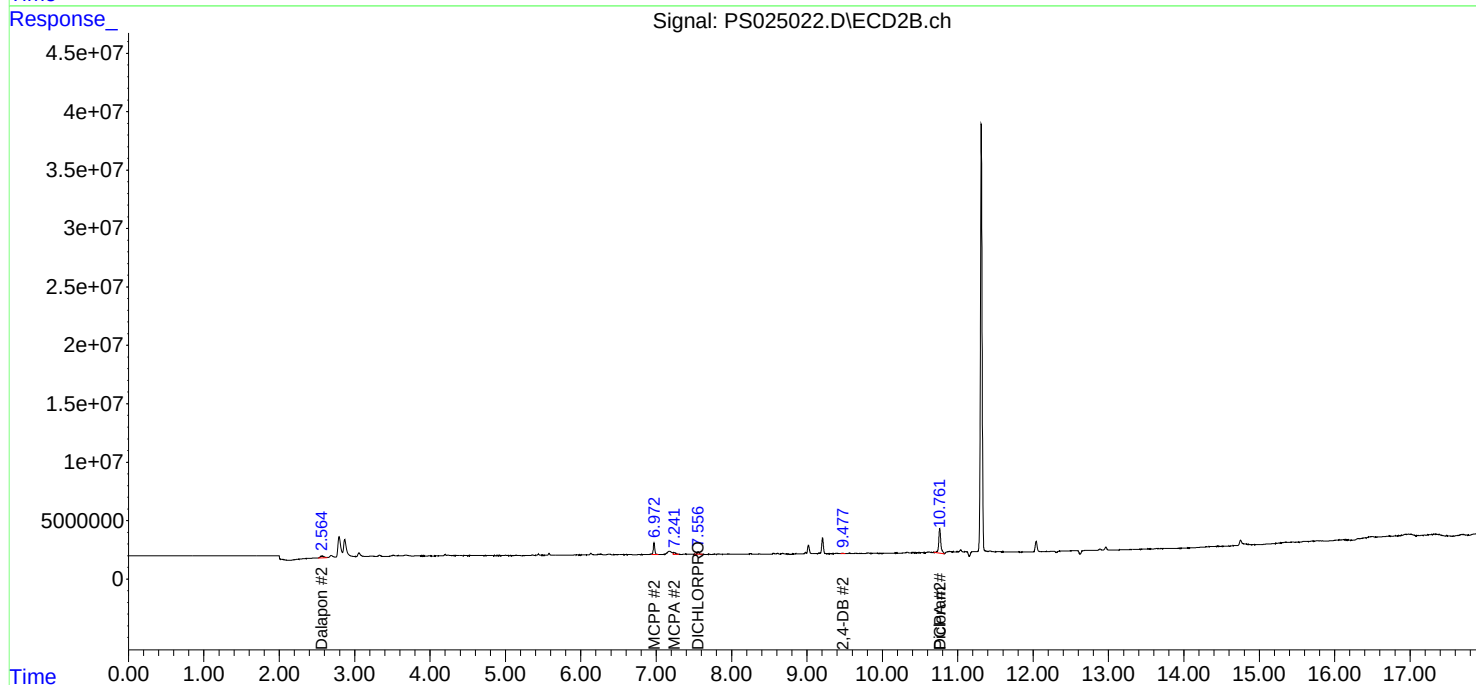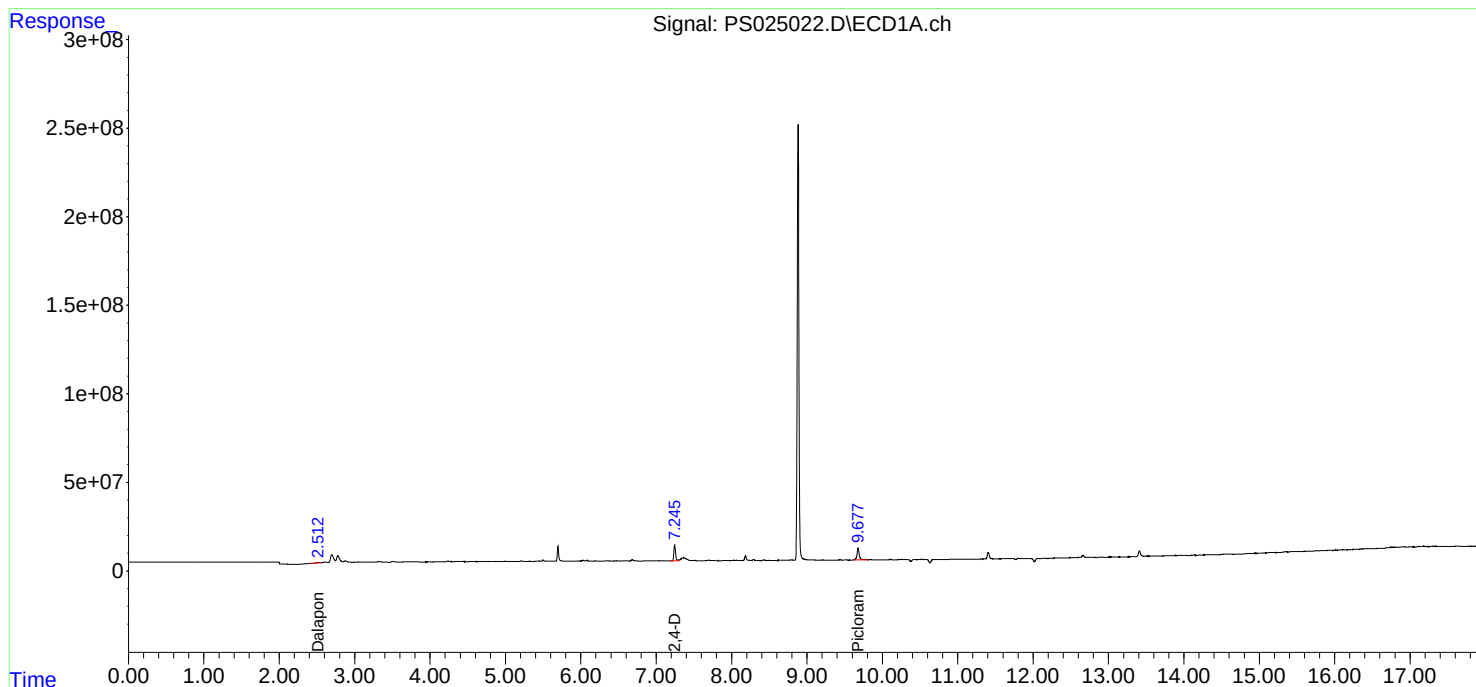


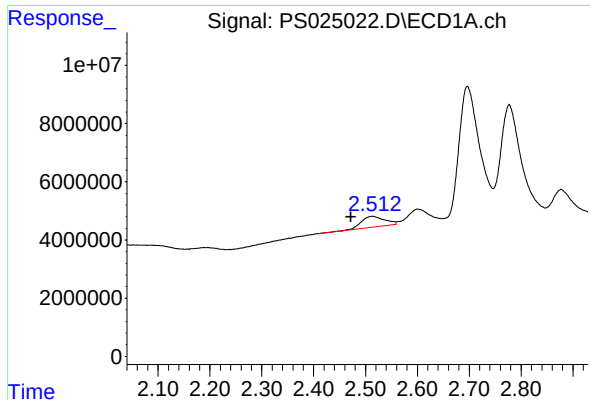

#1 Dalapon


R.T.: 2.513 min
Delta R.T.: 0.041 min
Response: 11751108
Conc: 4.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

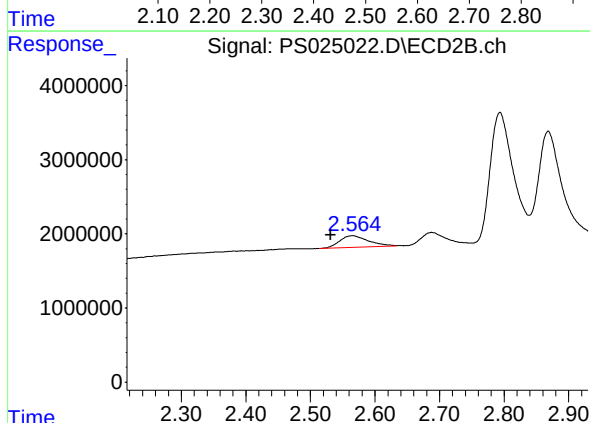


#1 Dalapon

R.T.: 2.564 min
Delta R.T.: 0.033 min
Response: 4955508
Conc: 4.32 ng/ml

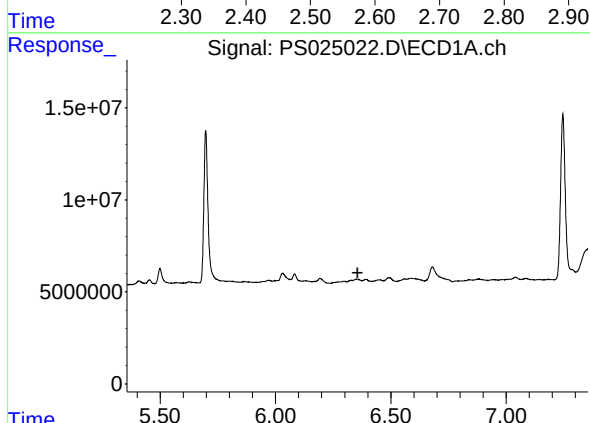


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

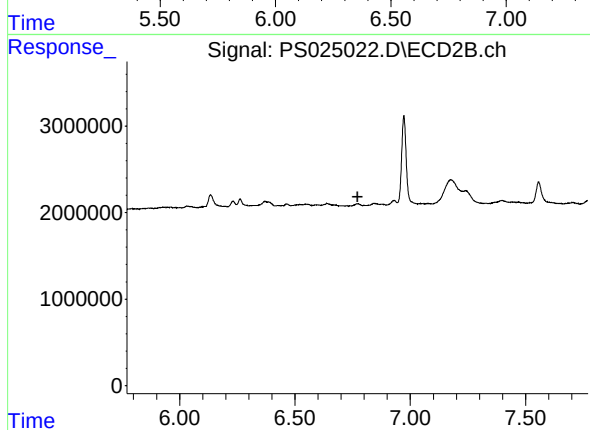

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.771 min
Response: 0
Conc: N.D.

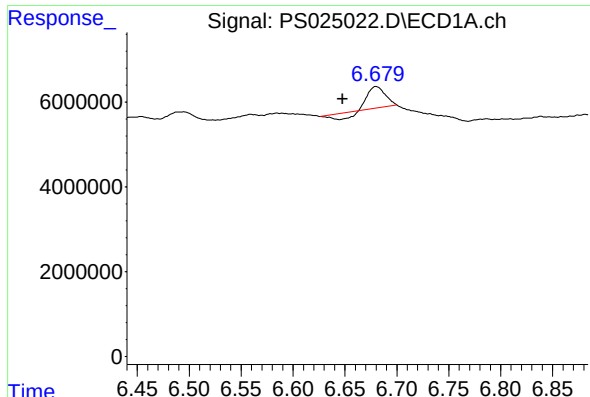

#6 MCPP


R.T.: 6.680 min
Delta R.T.: 0.032 min
Response: 4485719
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

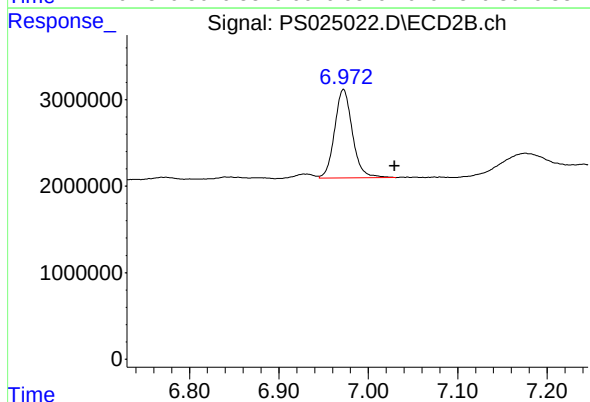


#6 MCPP

R.T.: 6.972 min
Delta R.T.: -0.057 min
Response: 14243981
Conc: 6.87 ug/ml

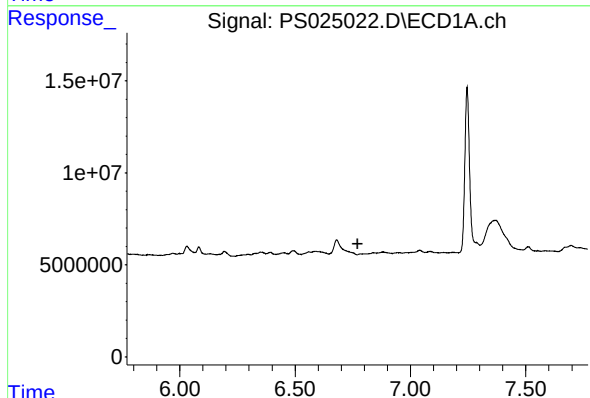


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

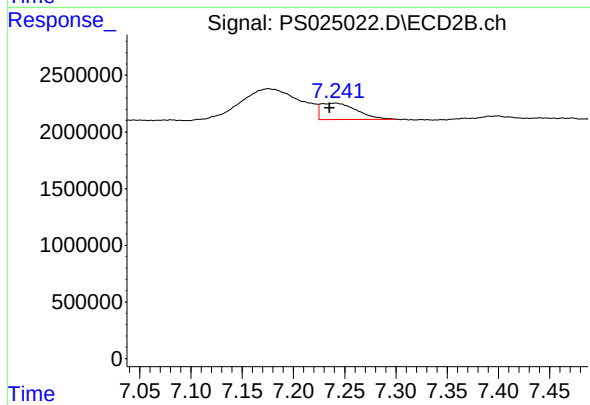

#7 MCPA


R.T.: 7.241 min
Delta R.T.: 0.006 min
Response: 3482506
Conc: 1.06 ug/ml

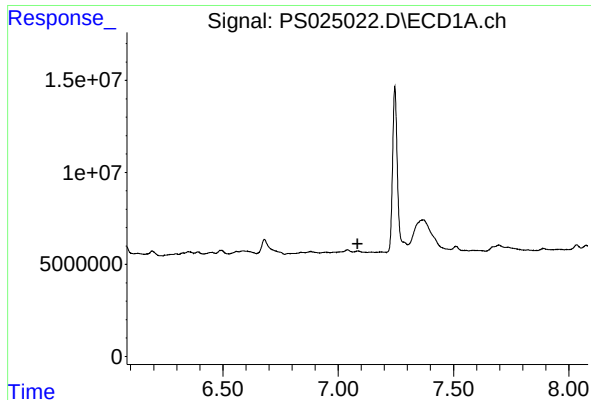

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

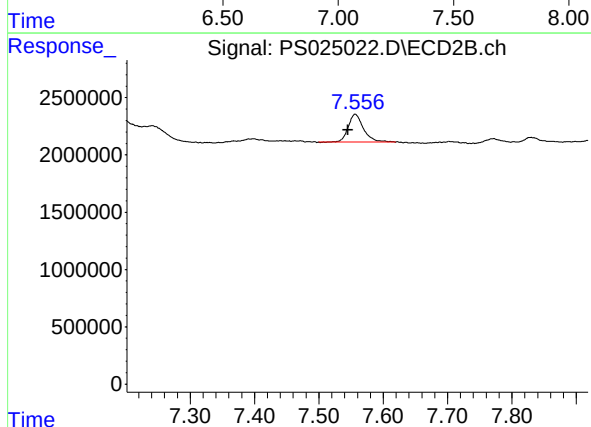


#8 DICHLORPROP

R.T.: 7.556 min
Delta R.T.: 0.011 min
Response: 4043706
Conc: 5.14 ng/ml

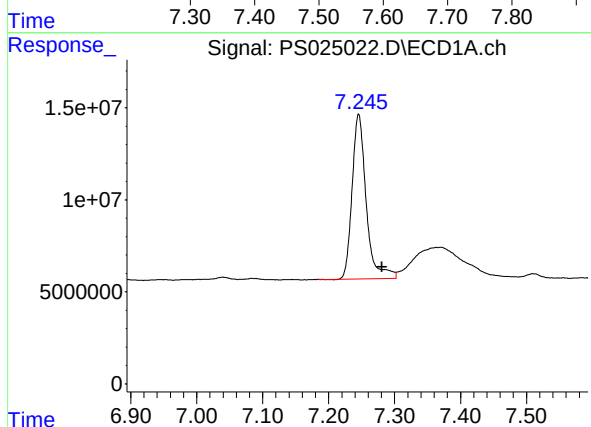


#9 2,4-D

R.T.: 7.246 min
Delta R.T.: -0.036 min
Response: 133009385
Conc: 43.79 ng/ml

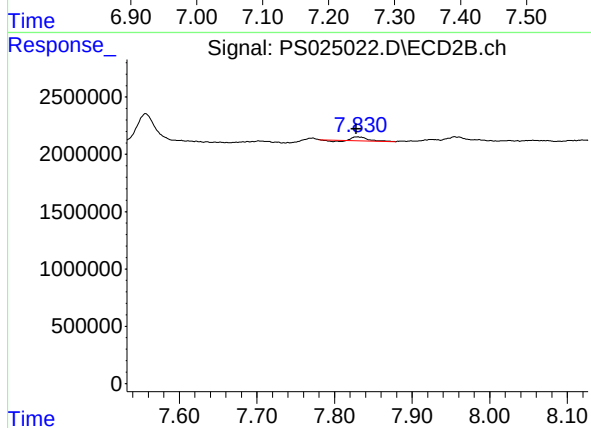

#9 2,4-D


R.T.: 7.830 min
Delta R.T.: 0.002 min
Response: 321290
Conc: N.D.

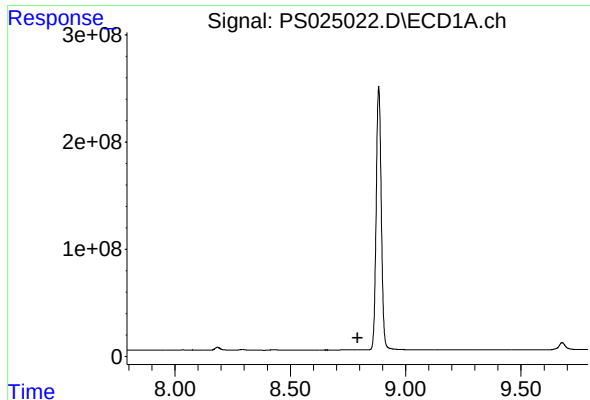

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

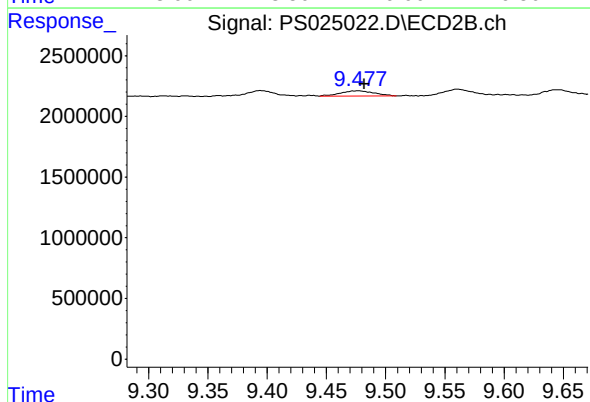


#13 2,4-DB

R.T.: 9.477 min
Delta R.T.: -0.005 min
Response: 835942
Conc: 1.51 ng/ml

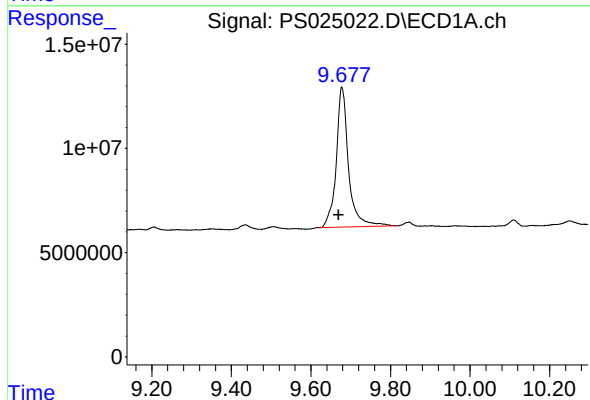


#15 Picloram

R.T.: 9.678 min
Delta R.T.: 0.008 min
Response: 144162671
Conc: 7.40 ng/ml

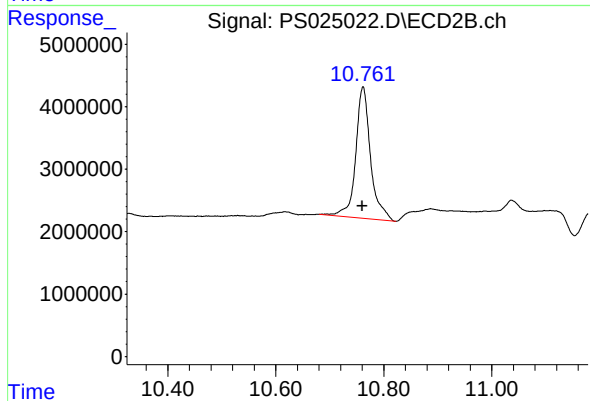

#15 Picloram


R.T.: 10.762 min
Delta R.T.: 0.002 min
Response: 40195500
Conc: 6.14 ng/ml

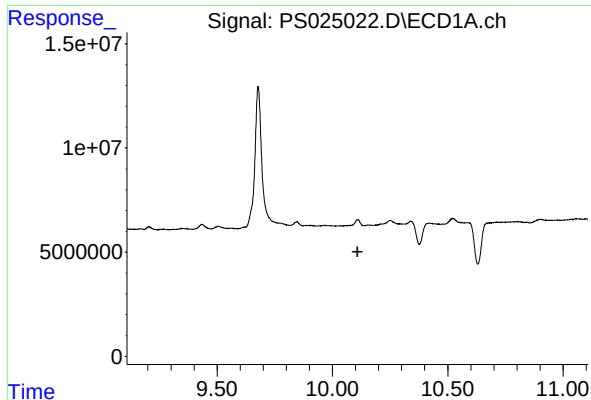

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

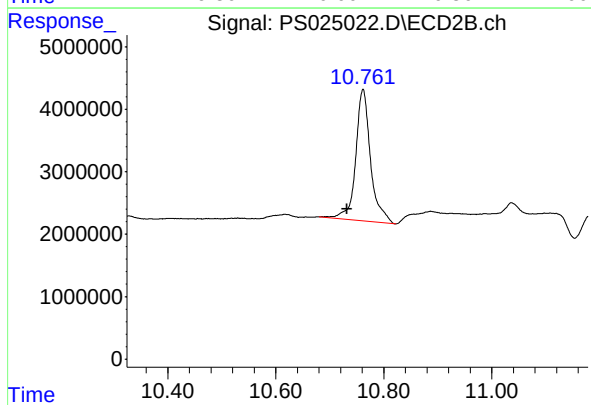

#16 DCPA

R.T.: 10.762 min
Delta R.T.: 0.030 min
Response: 40195500
Conc: 7.42 ng/ml