

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120623\
 Data File : PS025023.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2023 10:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:08:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.355	6.770	1181.1E6	376.9E6	527.785	520.234
Target Compounds							
1) T	Dalapon	2.510	2.565	10797430	4698246	3.744	4.096
2) T	3,5-DICHL...	5.697	0.000	5231042	0	1.548	N.D. #
3) T	4-Nitroph...	6.198	0.000	6908699	0	4.691	N.D. #
5) T	DICAMBA	0.000	6.972f	0	5820949	N.D.	1.879
6) T	MCP	6.679	6.972f	3331191	5820949	<MDL	2.806 #
8) T	DICHLORPROP	0.000	7.557	0	3836154	N.D.	4.877
9) T	2,4-D	7.246	7.772f	32024202	62272	10.544	<MDL #
11) T	2,4,5-TP ...	0.000	8.609	0	130573	N.D.	<MDL
12) T	2,4,5-T	0.000	8.980	0	1111999	N.D.	<MDL
13) T	2,4-DB	0.000	9.472	0	874278	N.D.	1.580
14) T	DINOSEB	0.000	9.807	0	412873	N.D.	<MDL
15) T	Picloram	9.680	10.761	96785571	25555572	4.967	3.904
16) T	DCPA	0.000	10.761	0	25555572	N.D.	4.715



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120623\
Data File : PS025023.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2023 10:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:08:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

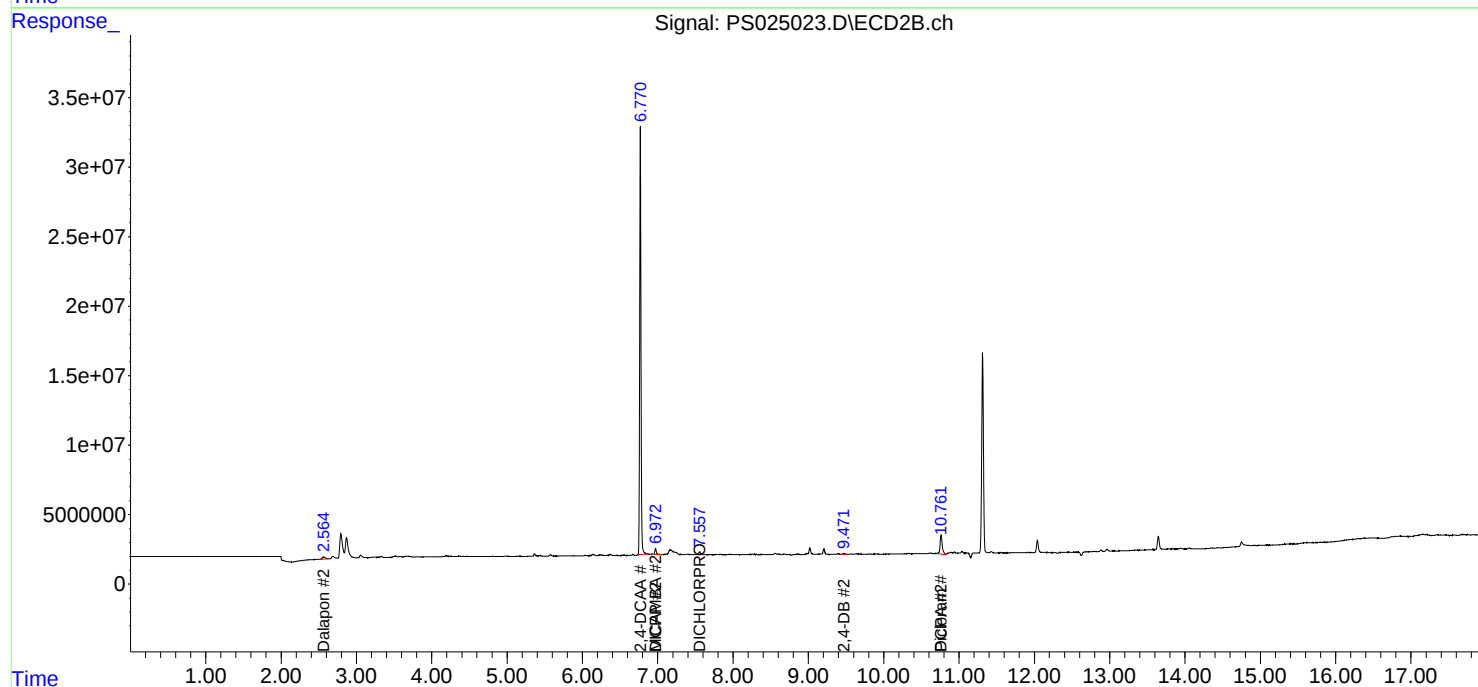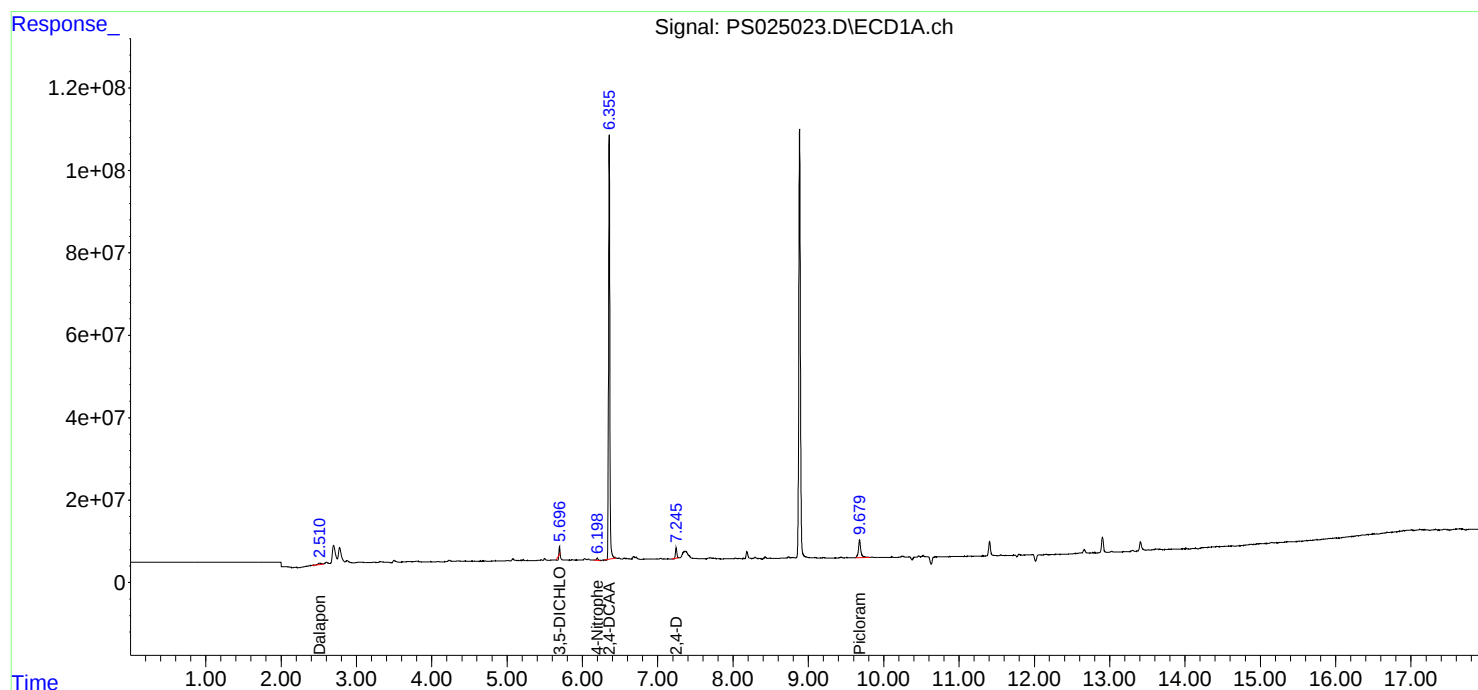


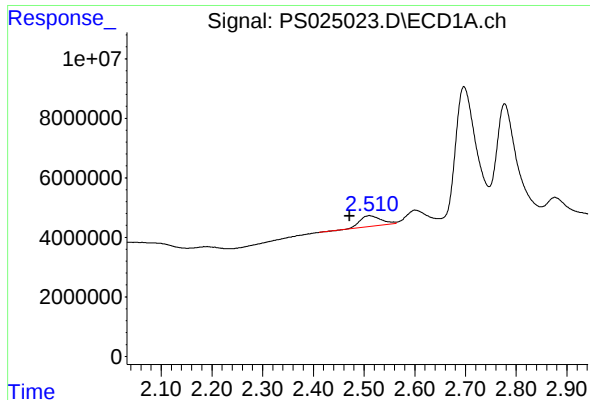

#1 Dalapon


R.T.: 2.510 min
Delta R.T.: 0.038 min
Response: 10797430
Conc: 3.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

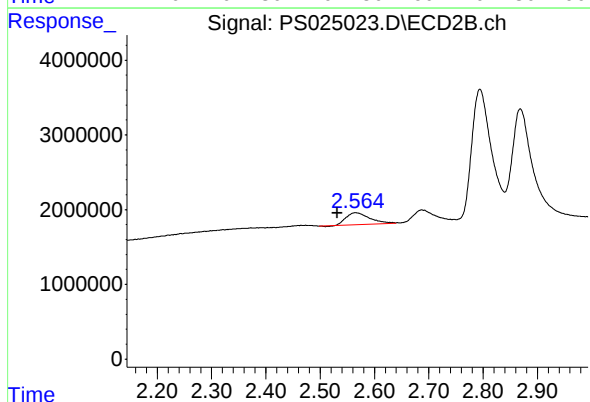


#1 Dalapon

R.T.: 2.565 min
Delta R.T.: 0.033 min
Response: 4698246
Conc: 4.10 ng/ml

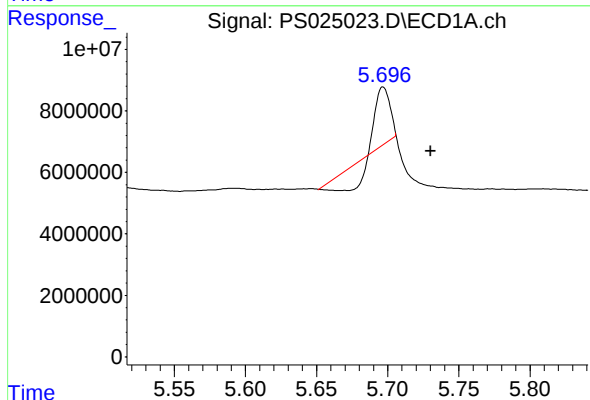


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.697 min
Delta R.T.: -0.033 min
Response: 5231042
Conc: 1.55 ng/ml

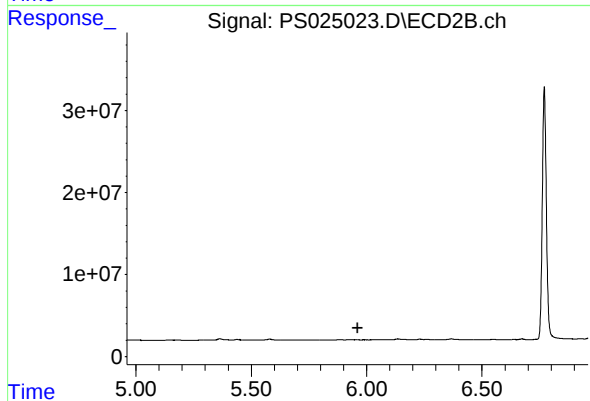

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

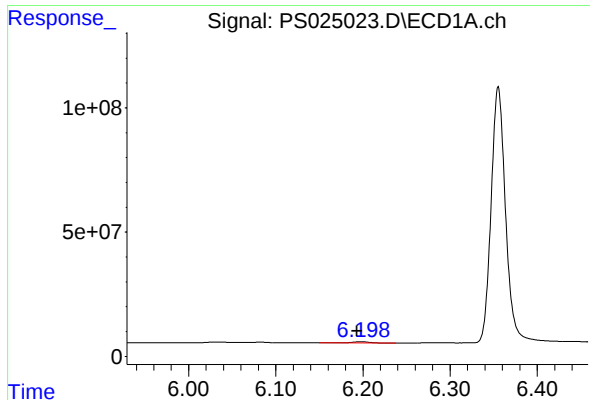

#3 4-Nitrophenol


R.T.: 6.198 min
Delta R.T.: 0.005 min
Response: 6908699
Conc: 4.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

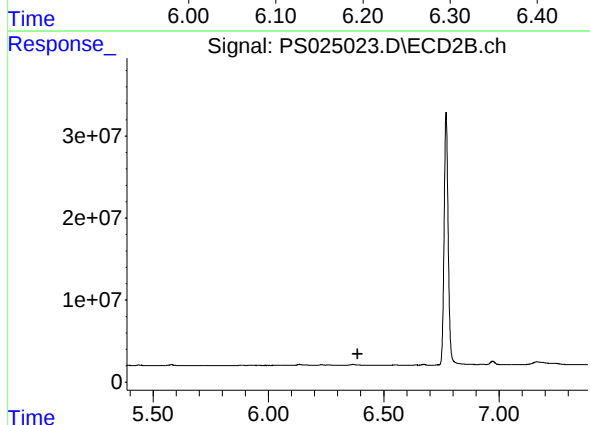


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.386 min
Response: 0
Conc: N.D.

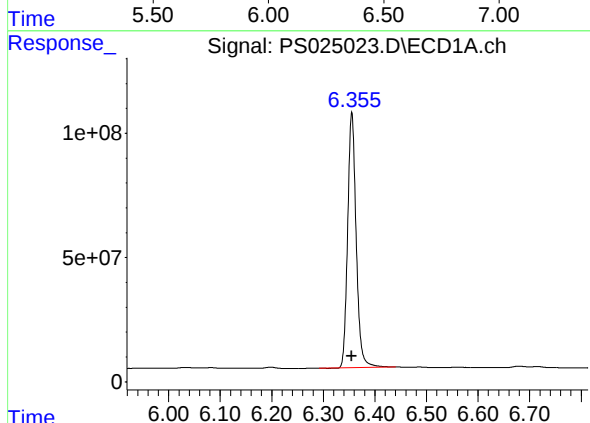


#4 2,4-DCAA

R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 1181099870
Conc: 527.78 ng/ml

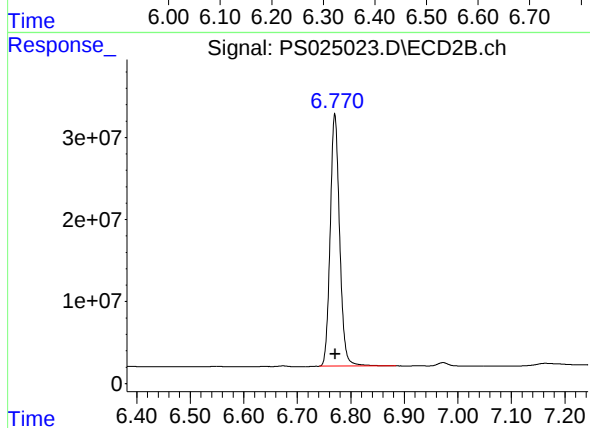

#4 2,4-DCAA


R.T.: 6.770 min
Delta R.T.: -0.001 min
Response: 376937859
Conc: 520.23 ng/ml

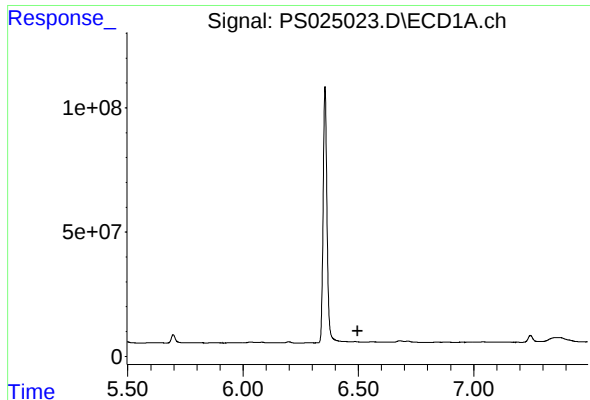

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

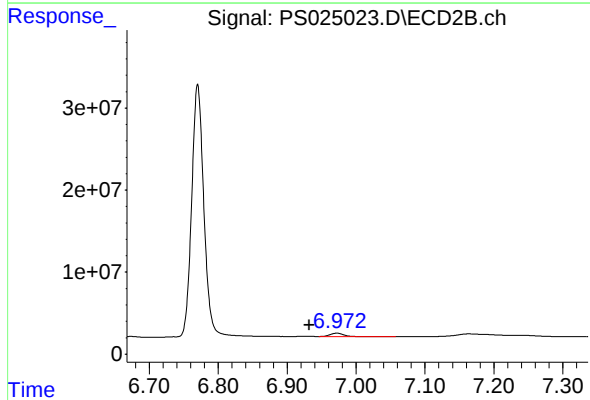


#5 DICAMBA

R.T.: 6.972 min
Delta R.T.: 0.041 min
Response: 5820949
Conc: 1.88 ng/ml

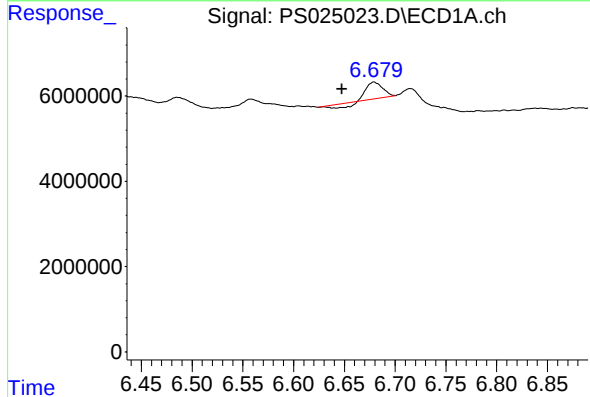


#6 MCPP

R.T.: 6.679 min
Delta R.T.: 0.032 min
Response: 3331191
Conc: N.D.

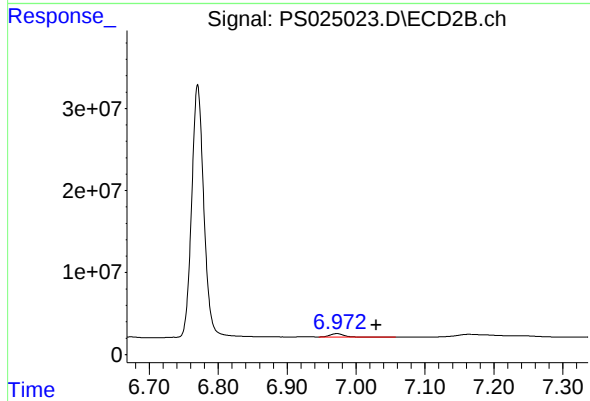

#6 MCPP


R.T.: 6.972 min
Delta R.T.: -0.057 min
Response: 5820949
Conc: 2.81 ug/ml

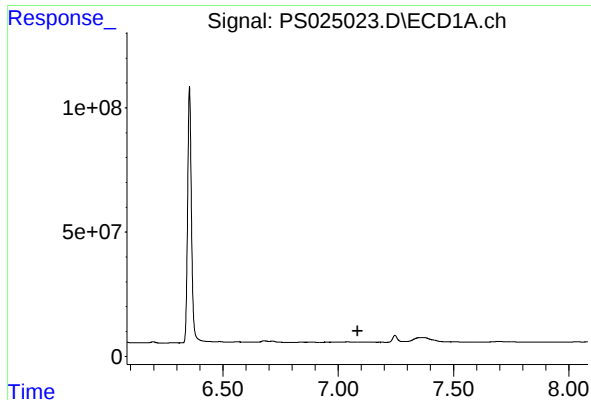

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

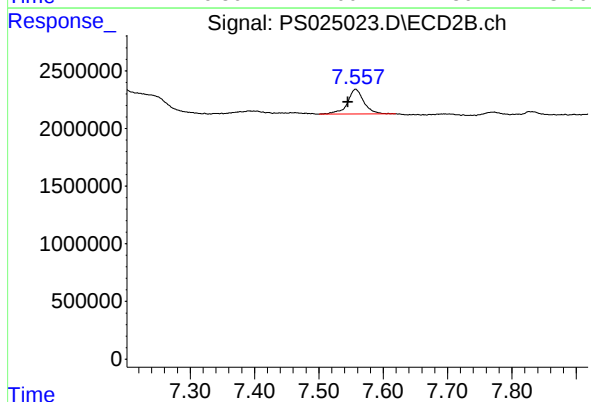


#8 DICHLORPROP

R.T.: 7.557 min
Delta R.T.: 0.012 min
Response: 3836154
Conc: 4.88 ng/ml

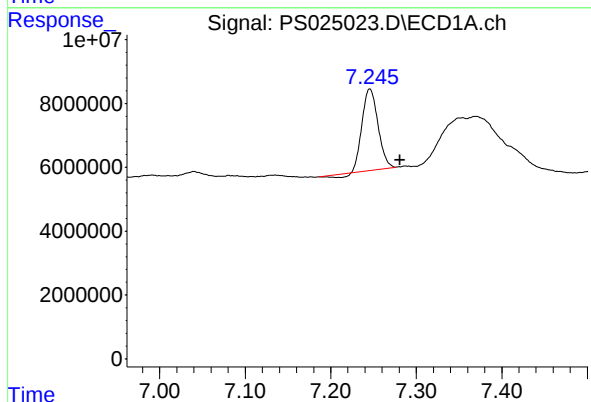


#9 2,4-D

R.T.: 7.246 min
Delta R.T.: -0.035 min
Response: 32024202
Conc: 10.54 ng/ml

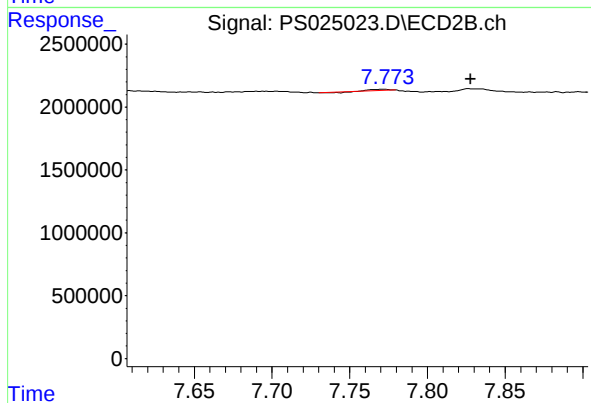

#9 2,4-D


R.T.: 7.772 min
Delta R.T.: -0.056 min
Response: 62272
Conc: N.D.

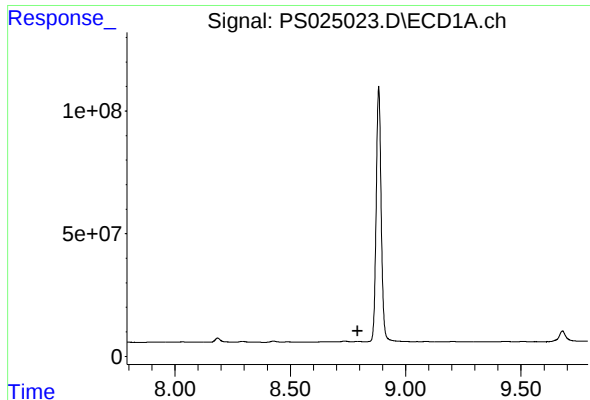

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

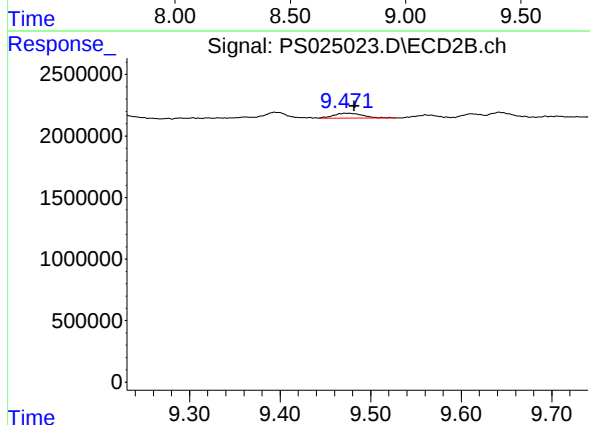


#13 2,4-DB

R.T.: 9.472 min
Delta R.T.: -0.010 min
Response: 874278
Conc: 1.58 ng/ml

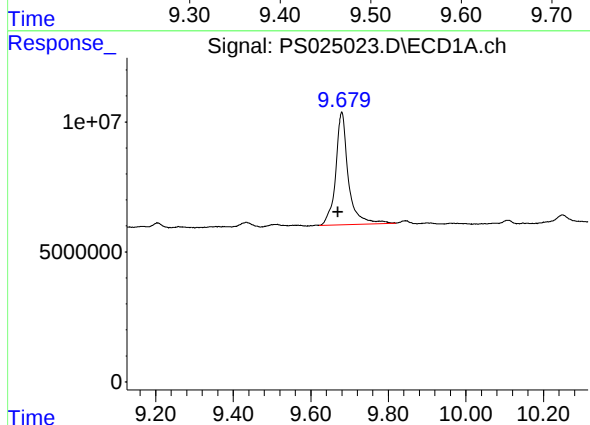


#15 Picloram

R.T.: 9.680 min
Delta R.T.: 0.010 min
Response: 96785571
Conc: 4.97 ng/ml

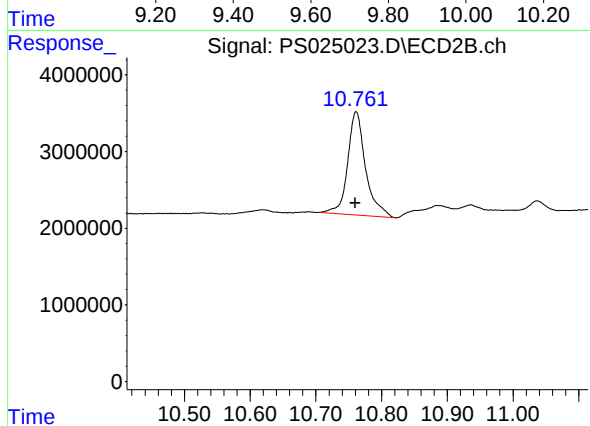

#15 Picloram


R.T.: 10.761 min
Delta R.T.: 0.001 min
Response: 25555572
Conc: 3.90 ng/ml

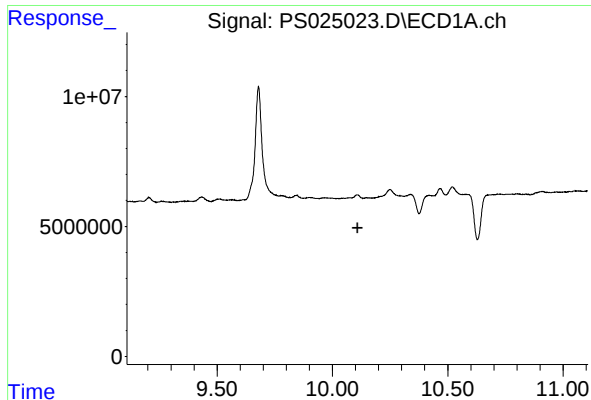

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

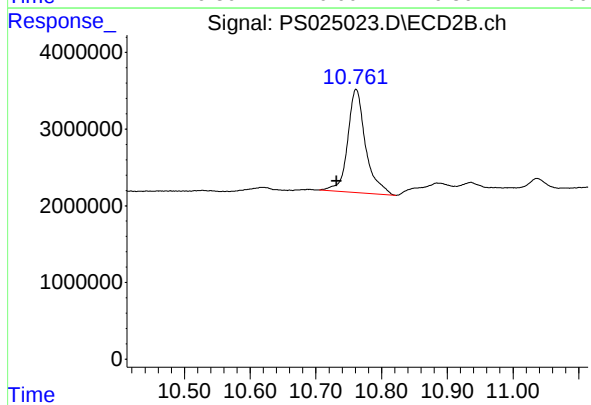

#16 DCPA

R.T.: 10.761 min
Delta R.T.: 0.030 min
Response: 25555572
Conc: 4.72 ng/ml