

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120623\
 Data File : PS025029.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2023 13:06
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:10:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.355	6.770	1195.8E6	378.0E6	534.352	521.730
Target Compounds							
1) T	Dalapon	2.509	2.560	10244592	4768530	3.553	4.157
2) T	3,5-DICHL...	5.695	0.000	8731807	0	2.583	N.D. #
3) T	4-Nitroph...	6.197	0.000	10468121	0	7.108	N.D. #
5) T	DICAMBA	0.000	6.930	0	480076	N.D.	<MDL
6) T	MCP	6.676	6.971f	5238906	4006907	<MDL	1.932 #
8) T	DICHLORPROP	0.000	7.556	0	3399771	N.D.	4.322
9) T	2,4-D	7.244	7.829	24381118	407404	8.027	<MDL #
10) T	Pentachlo...	0.000	8.253	0	612494	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.607	0	119531	N.D.	<MDL
12) T	2,4,5-T	0.000	8.978	0	1359161	N.D.	<MDL
13) T	2,4-DB	8.733f	9.468	2194860	635691	<MDL	1.149 #
14) T	DINOSEB	0.000	9.807	0	438203	N.D.	<MDL
15) T	Picloram	9.674	10.760	36551656	11122683	1.876	1.699
16) T	DCPA	0.000	10.760	0	11122683	N.D.	2.052



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120623\
Data File : PS025029.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2023 13:06
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:10:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

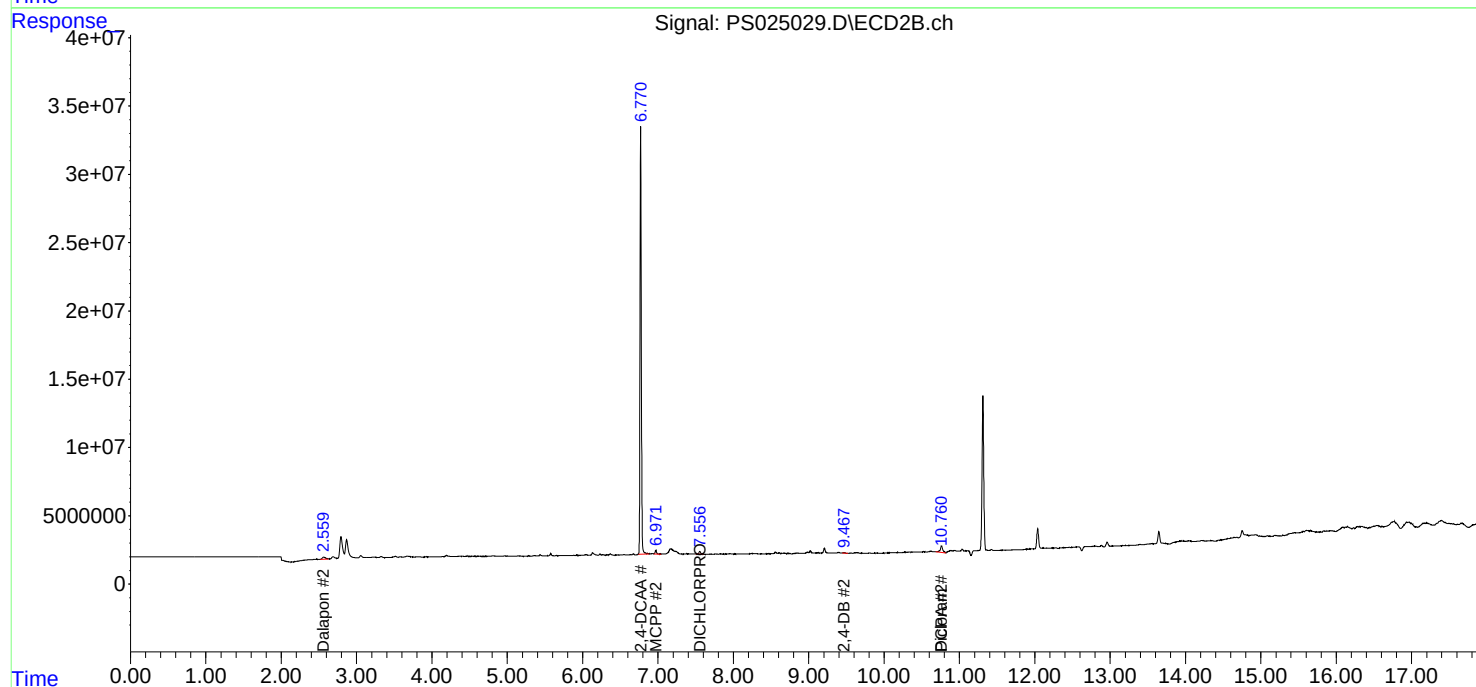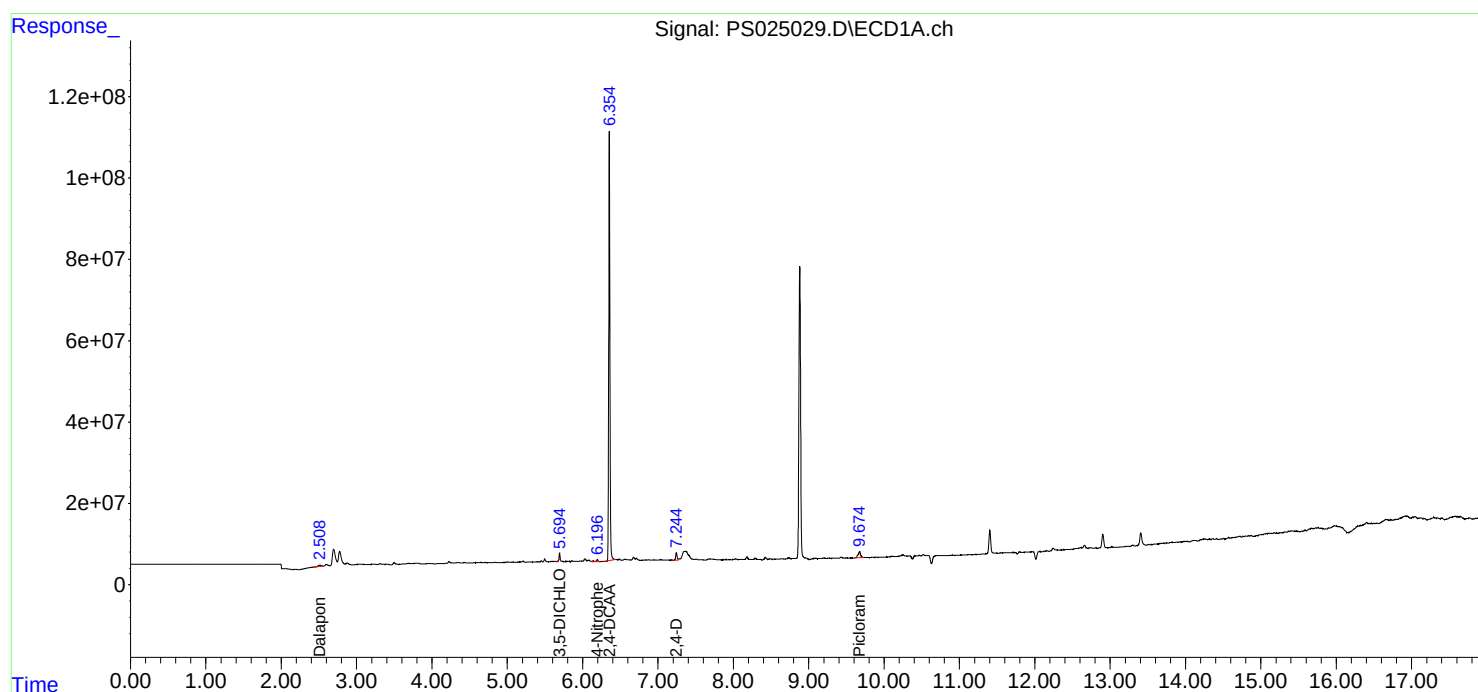


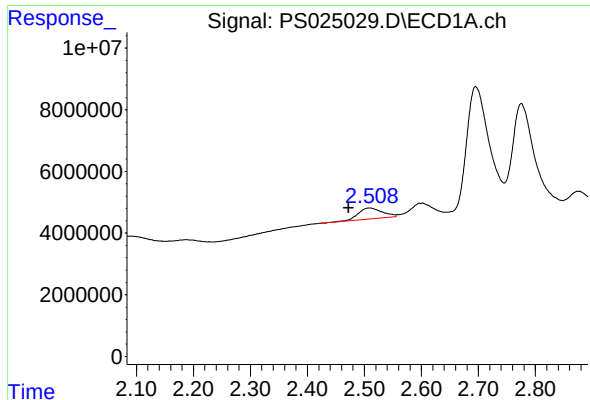

#1 Dalapon


R.T.: 2.509 min
Delta R.T.: 0.037 min
Response: 10244592
Conc: 3.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

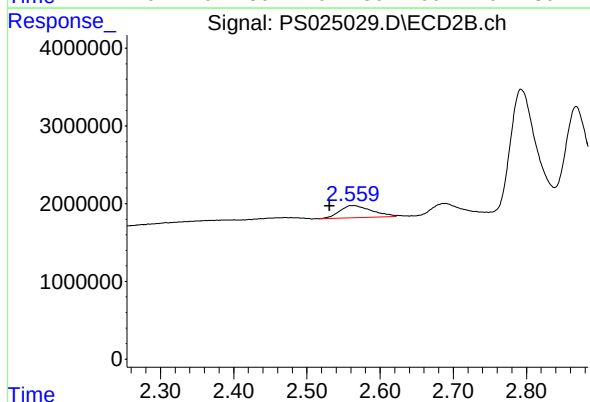


#1 Dalapon

R.T.: 2.560 min
Delta R.T.: 0.029 min
Response: 4768530
Conc: 4.16 ng/ml

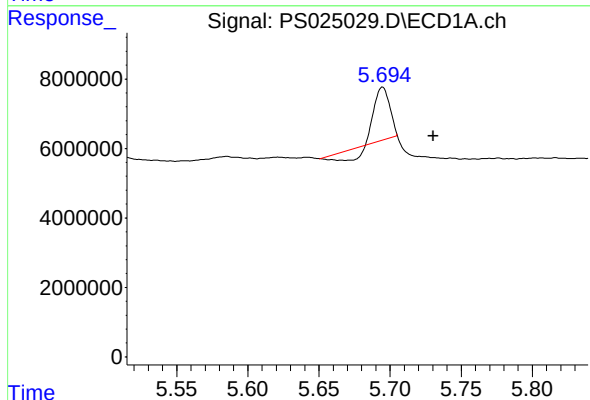


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.695 min
Delta R.T.: -0.036 min
Response: 8731807
Conc: 2.58 ng/ml

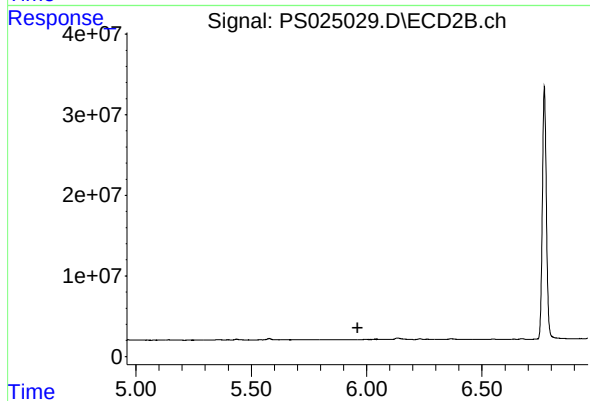

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

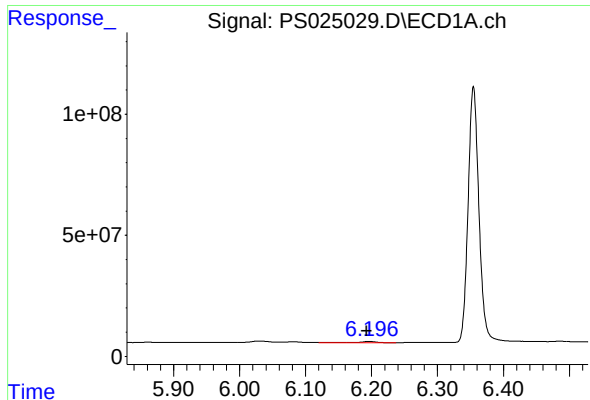

#3 4-Nitrophenol


R.T.: 6.197 min
Delta R.T.: 0.004 min
Response: 10468121
Conc: 7.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

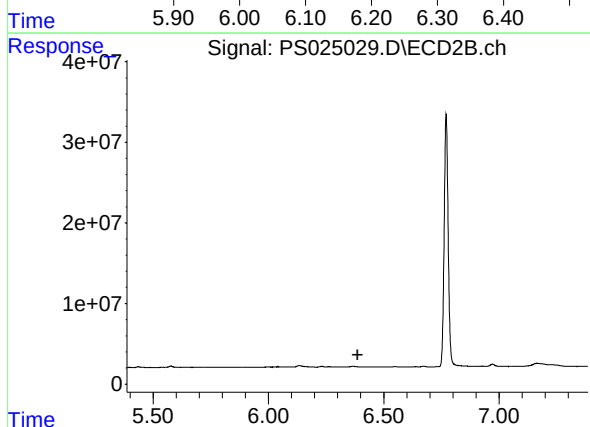


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.386 min
Response: 0
Conc: N.D.

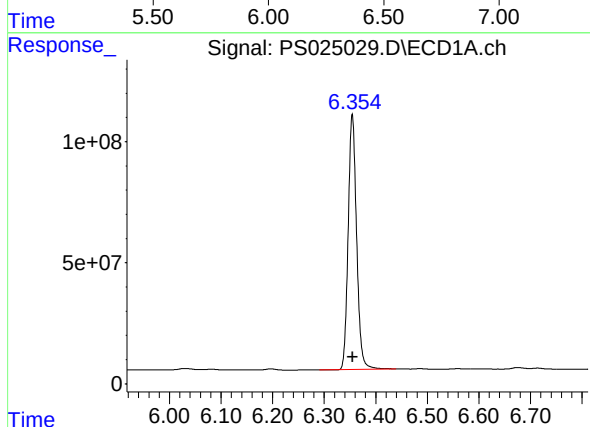


#4 2,4-DCAA

R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 1195796848
Conc: 534.35 ng/ml

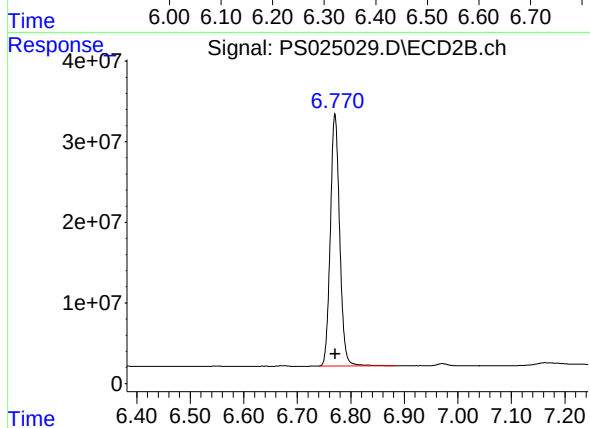

#4 2,4-DCAA


R.T.: 6.770 min
Delta R.T.: 0.000 min
Response: 378021742
Conc: 521.73 ng/ml

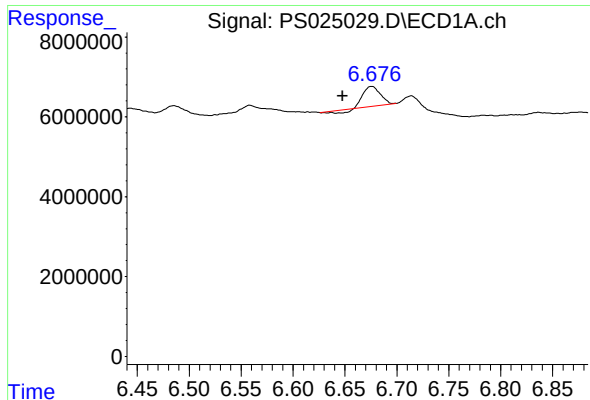

#6 MCPP


R.T.: 6.676 min
Delta R.T.: 0.028 min
Response: 5238906
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

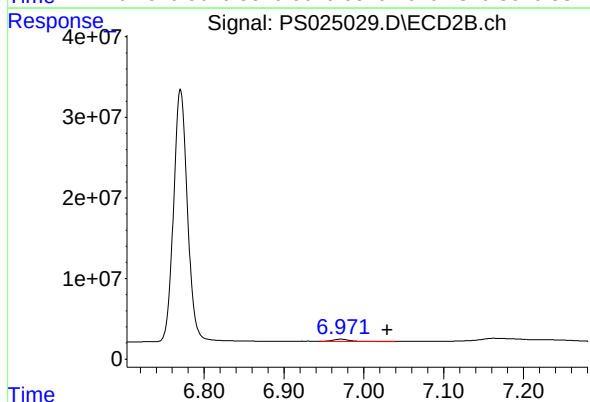


#6 MCPP

R.T.: 6.971 min
Delta R.T.: -0.058 min
Response: 4006907
Conc: 1.93 ug/ml

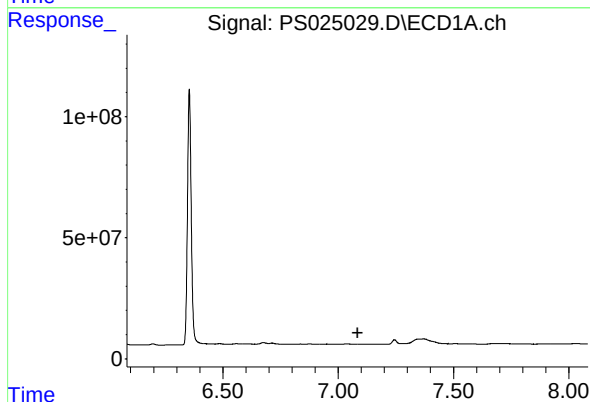


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

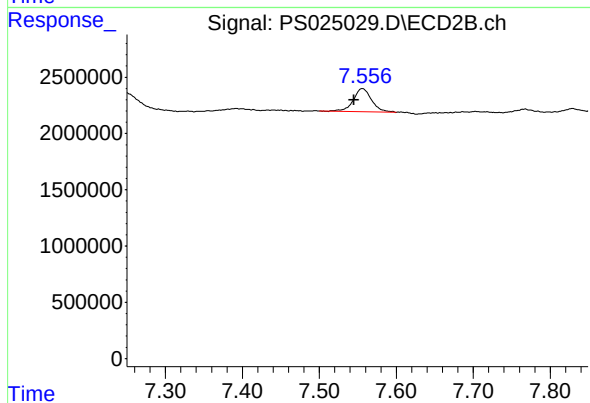

#8 DICHLORPROP


R.T.: 7.556 min
Delta R.T.: 0.011 min
Response: 3399771
Conc: 4.32 ng/ml

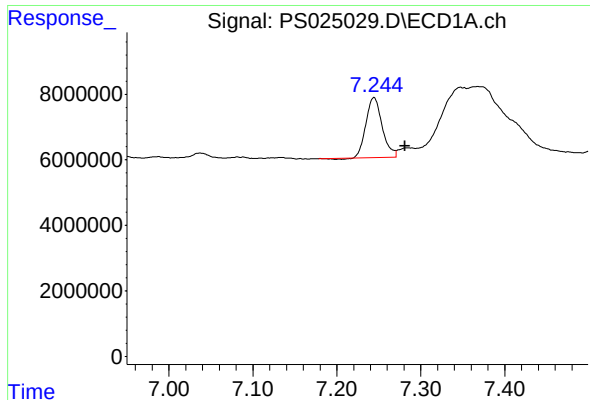

#9 2,4-D


R.T.: 7.244 min
Delta R.T.: -0.037 min
Response: 24381118
Conc: 8.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

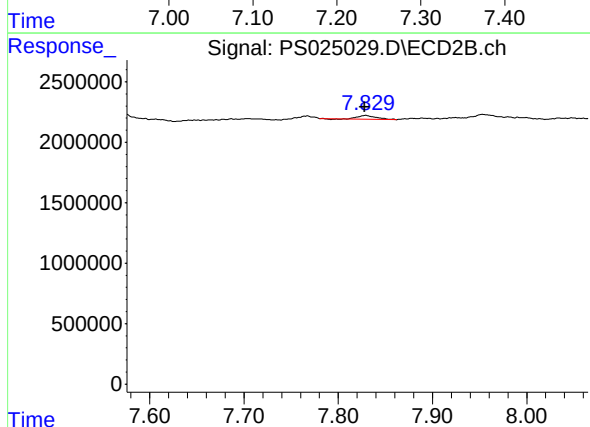


#9 2,4-D

R.T.: 7.829 min
Delta R.T.: 0.001 min
Response: 407404
Conc: N.D.

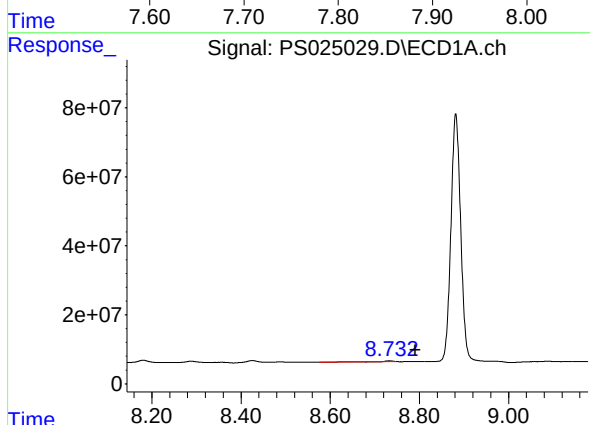


#13 2,4-DB

R.T.: 8.733 min
Delta R.T.: -0.059 min
Response: 2194860
Conc: N.D.

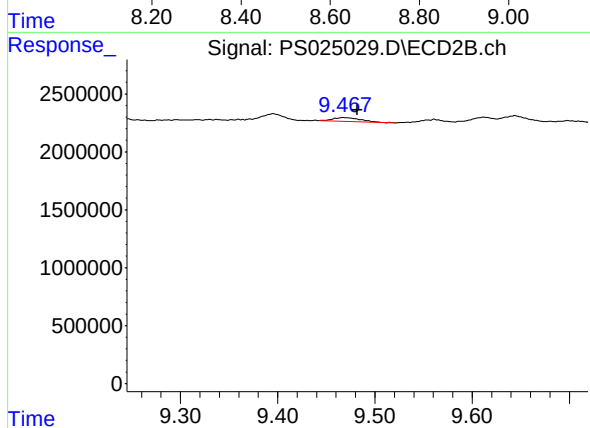

#13 2,4-DB


R.T.: 9.468 min
Delta R.T.: -0.014 min
Response: 635691
Conc: 1.15 ng/ml

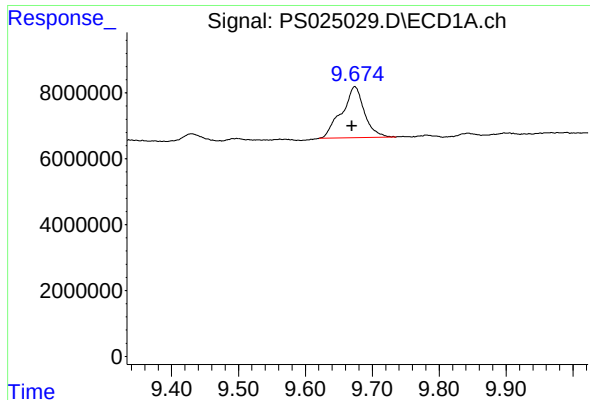

#15 Picloram


R.T.: 9.674 min
Delta R.T.: 0.004 min
Response: 36551656
Conc: 1.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

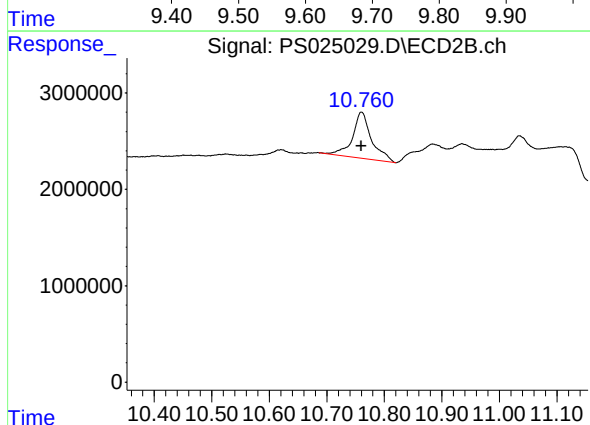


#15 Picloram

R.T.: 10.760 min
Delta R.T.: 0.000 min
Response: 11122683
Conc: 1.70 ng/ml

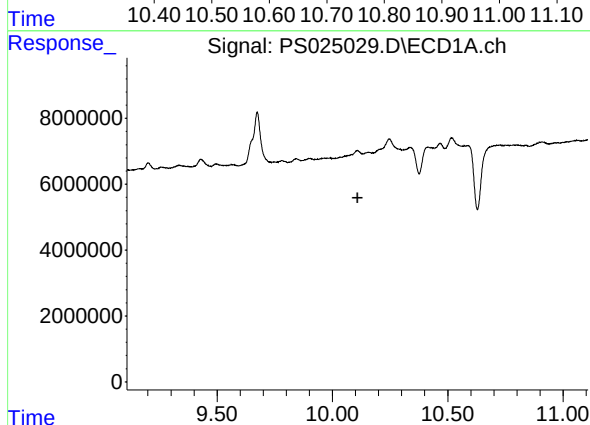

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

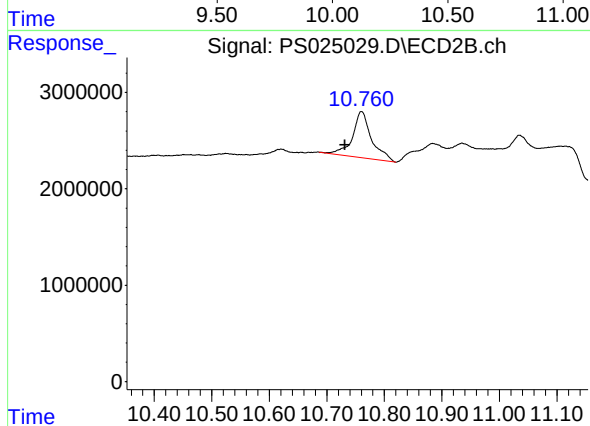

#16 DCPA

R.T.: 10.760 min
Delta R.T.: 0.029 min
Response: 11122683
Conc: 2.05 ng/ml