

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120624\
 Data File : PS028712.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 08:53
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 22:54:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
1) T	Dalapon	2.661f	0.000	3349922	0	1.154	N.D. #
2) T	3,5-DICHL...	6.386	0.000	2266188	0	<MDL	N.D. #
3) T	4-Nitroph...	7.013	0.000	7915505	0	4.605	N.D. #
5) T	DICAMBA	0.000	7.910	0	4290154	N.D.	<MDL
7) T	MCPA	7.782f	0.000	1248682	0	<MDL	N.D. #
8) T	DICHLORPROP	8.147f	8.680f	3236549	4627192	1.040	2.894 #
9) T	2,4-D	8.374	0.000	14552040	0	4.315	N.D. #
10) T	Pentachlo...	8.654	0.000	1345431	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.227	9.867	1252442	4070613	<MDL	<MDL #
12) T	2,4,5-T	9.526	10.282	2587193	7415612	<MDL	<MDL #
13) T	2,4-DB	10.081	0.000	612221	0	<MDL	N.D. #
14) T	DINOSEB	11.304	0.000	8218183	0	<MDL	N.D. #
15) T	Picloram	11.093	12.324	86151626	5200772	2.897	<MDL #
16) T	DCPA	11.599	12.324f	9245995	5200772	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120624\
Data File : PS028712.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 08:53
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 22:54:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

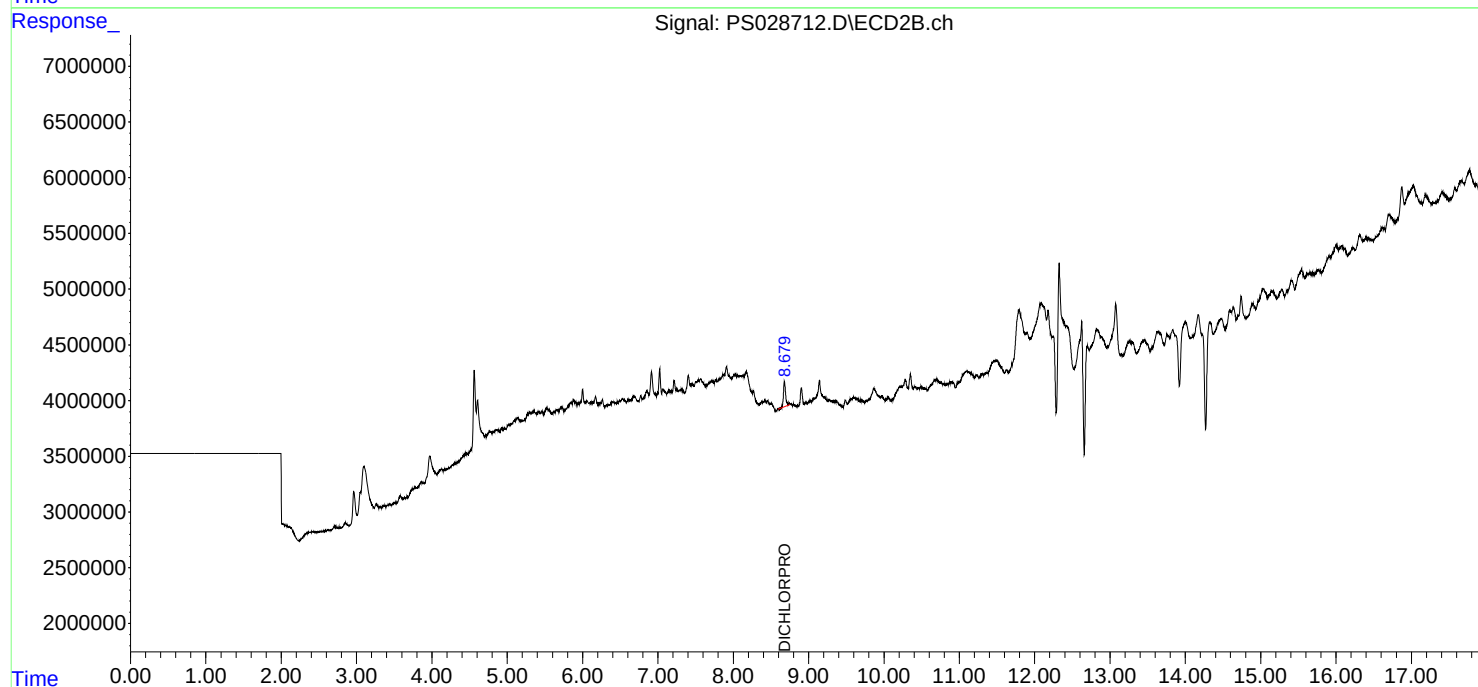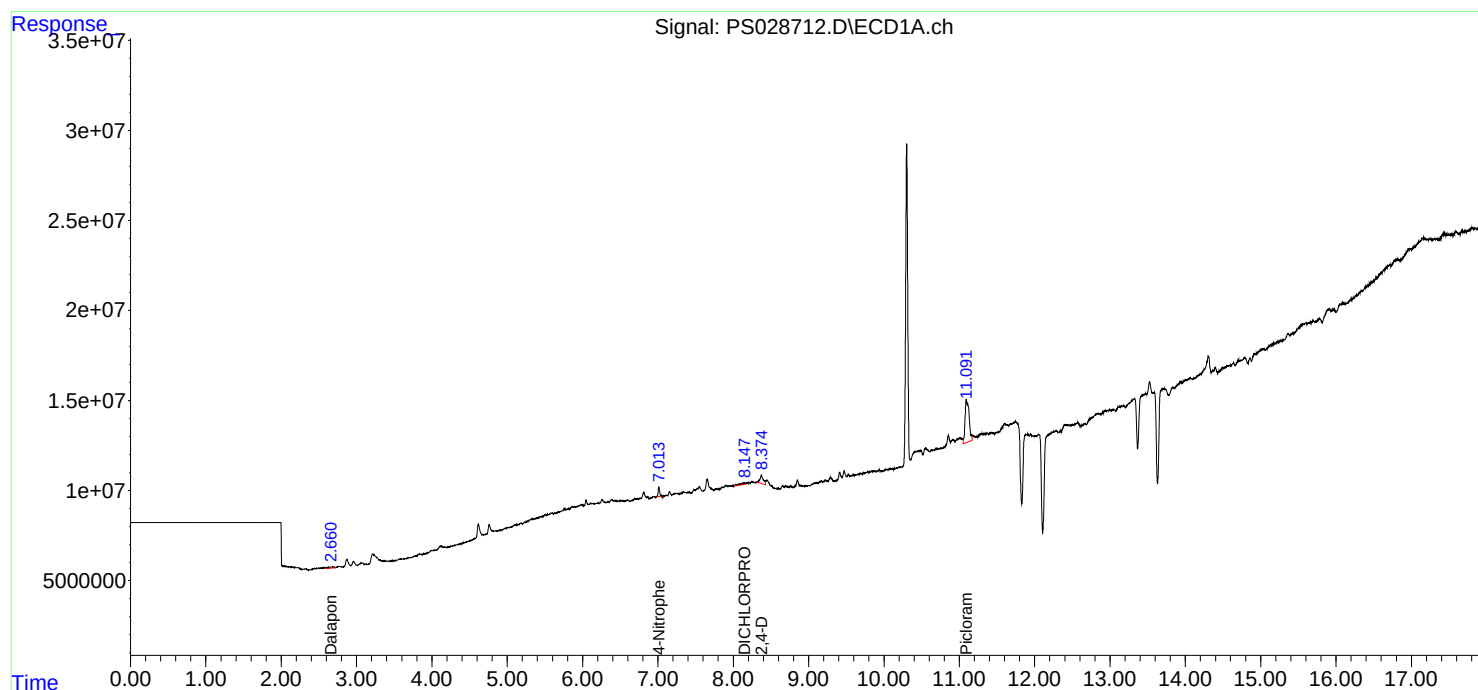


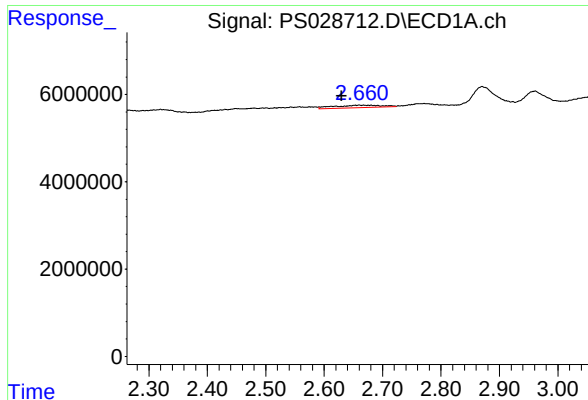

#1 Dalapon


R.T.: 2.661 min
Delta R.T.: 0.031 min
Response: 3349922
Conc: 1.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

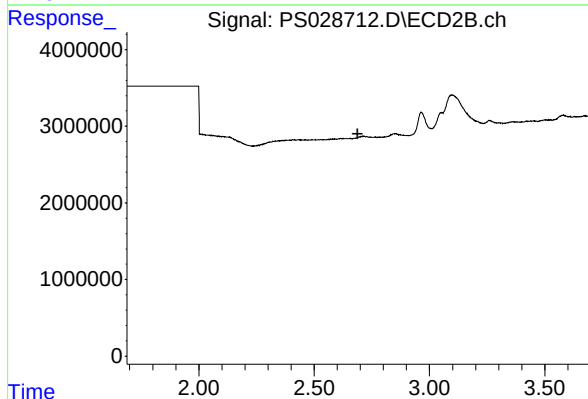


#1 Dalapon

R.T.: 0.000 min
Exp R.T.: 2.688 min
Response: 0
Conc: N.D.

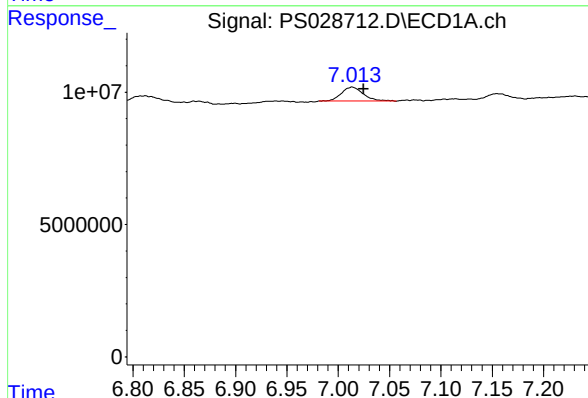


#3 4-Nitrophenol

R.T.: 7.013 min
Delta R.T.: -0.011 min
Response: 7915505
Conc: 4.60 ng/ml

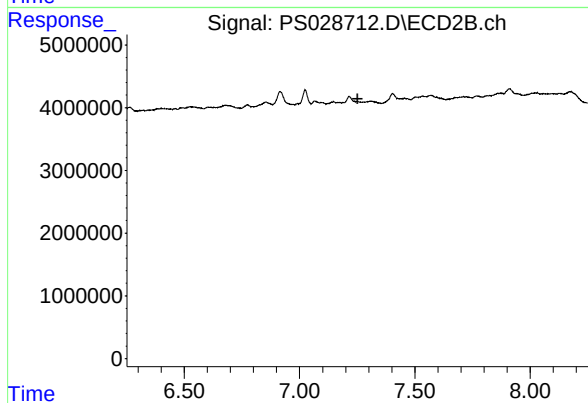

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.251 min
Response: 0
Conc: N.D.

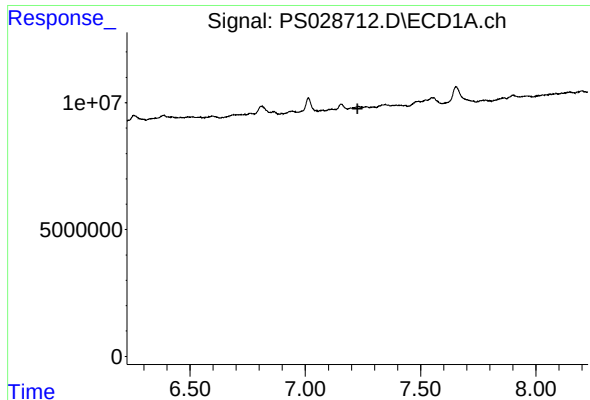

#4 2,4-DCAA


R.T.: 7.230 min
Delta R.T.: 0.004 min
Response: -2502767
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

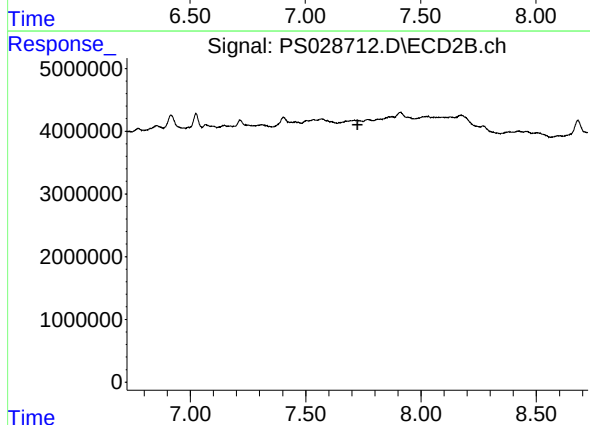


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 7.725 min
Response: 0
Conc: N.D.

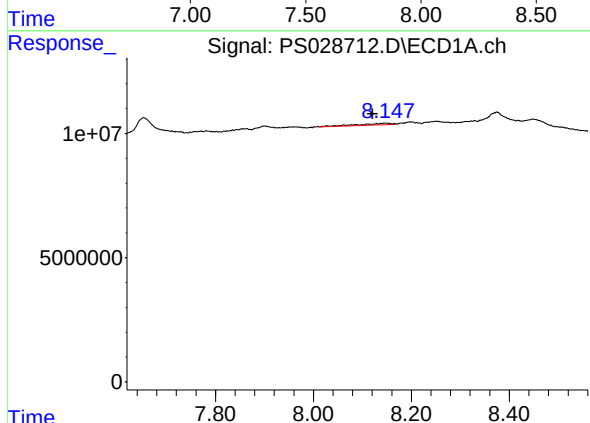


#8 DICHLORPROP

R.T.: 8.147 min
Delta R.T.: 0.026 min
Response: 3236549
Conc: 1.04 ng/ml

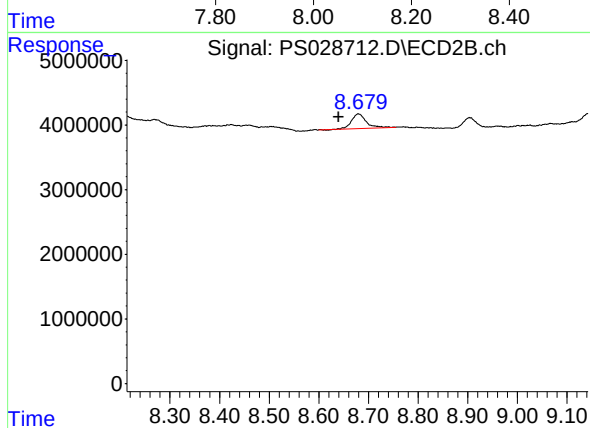

#8 DICHLORPROP


R.T.: 8.680 min
Delta R.T.: 0.040 min
Response: 4627192
Conc: 2.89 ng/ml

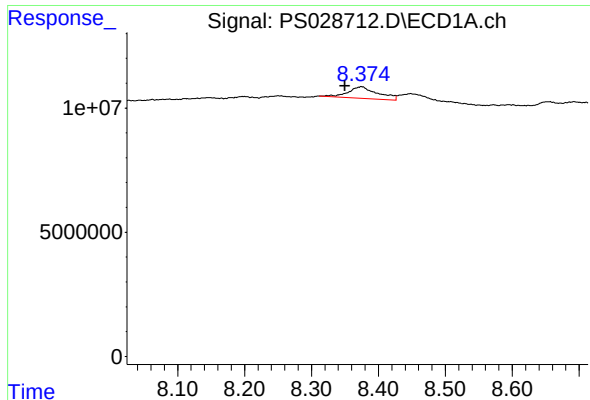

#9 2,4-D


R.T.: 8.374 min
Delta R.T.: 0.024 min
Response: 14552040
Conc: 4.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

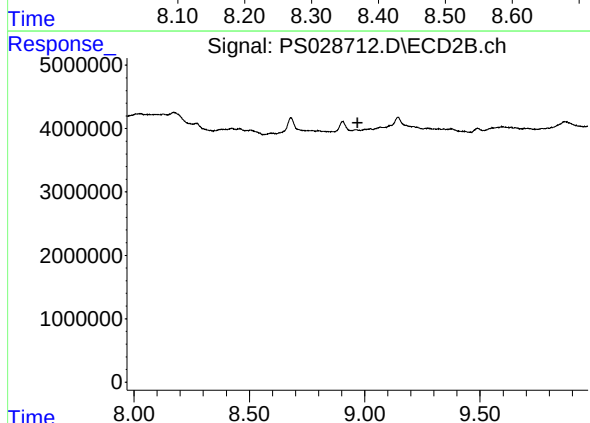


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.969 min
Response: 0
Conc: N.D.

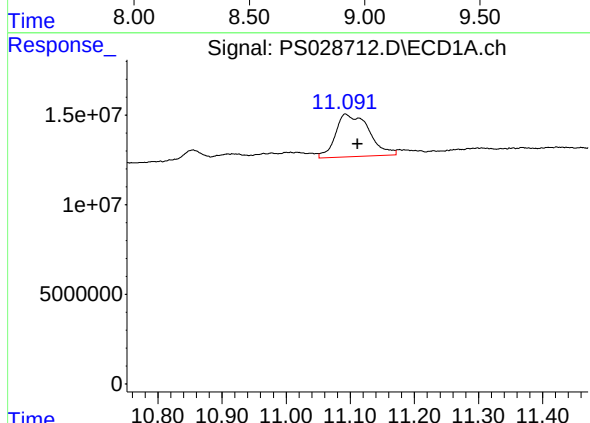

#15 Picloram

R.T.: 11.093 min
Delta R.T.: -0.019 min
Response: 86151626
Conc: 2.90 ng/ml

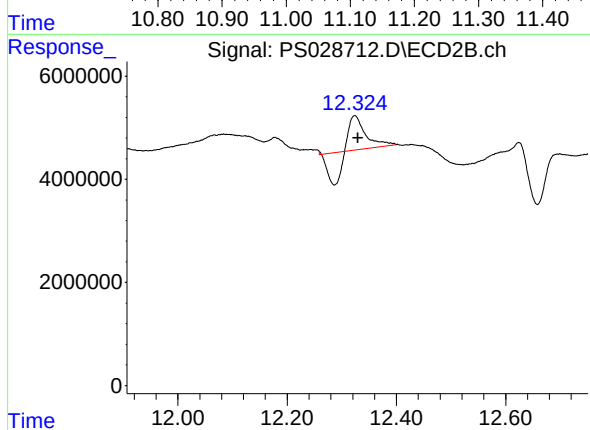

#15 Picloram

R.T.: 12.324 min
Delta R.T.: -0.006 min
Response: 5200772
Conc: N.D.