

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120624\
 Data File : PS028713.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 09:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 22:54:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.227	7.720	1343.7E6	602.8E6	500.948	447.529
Target Compounds						
1) T Dalapon	2.673f	2.722f	21236070	21273592	7.318	9.742 #
3) T 4-Nitroph...	7.018	0.000	11577838	0	6.735	N.D. #
5) T DICAMBA	0.000	7.919	0	4242453	N.D.	<MDL
7) T MCPA	7.779f	8.250f	762201	9508812	<MDL	1.532 #
8) T DICHLORPROP	8.143	8.686f	629389	4894897	<MDL	3.062 #
10) T Pentachlo...	8.649	0.000	430436	0	<MDL	N.D. #
11) T 2,4,5-TP ...	9.227	0.000	640668	0	<MDL	N.D. #
12) T 2,4,5-T	9.525	10.290	4759034	6059936	<MDL	<MDL #
13) T 2,4-DB	10.095	0.000	373247	0	<MDL	N.D. #
14) T DINOSEB	11.301	0.000	1993314	0	<MDL	N.D. #
15) T Picloram	11.124	12.331	34511894	14951881	1.161	1.160
16) T DCPA	11.590	0.000	2988730	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120624\
Data File : PS028713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 09:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 22:54:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

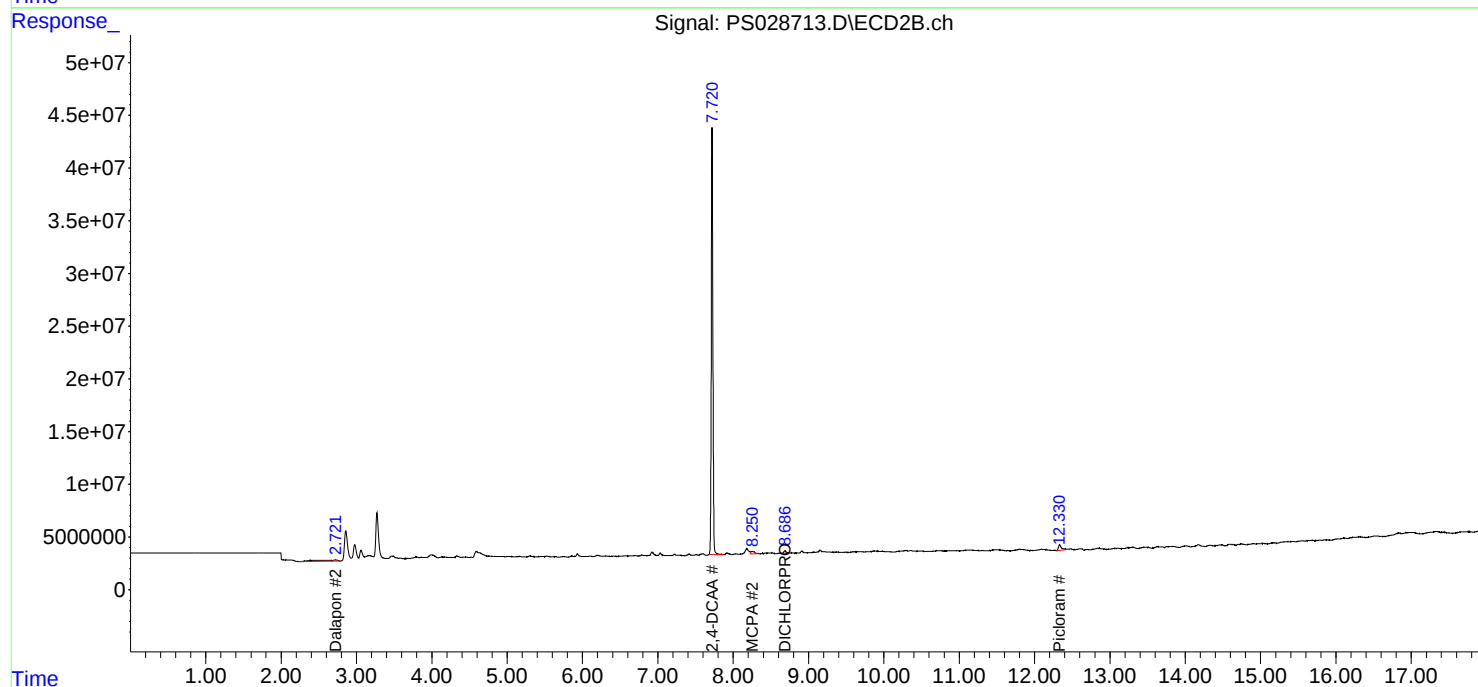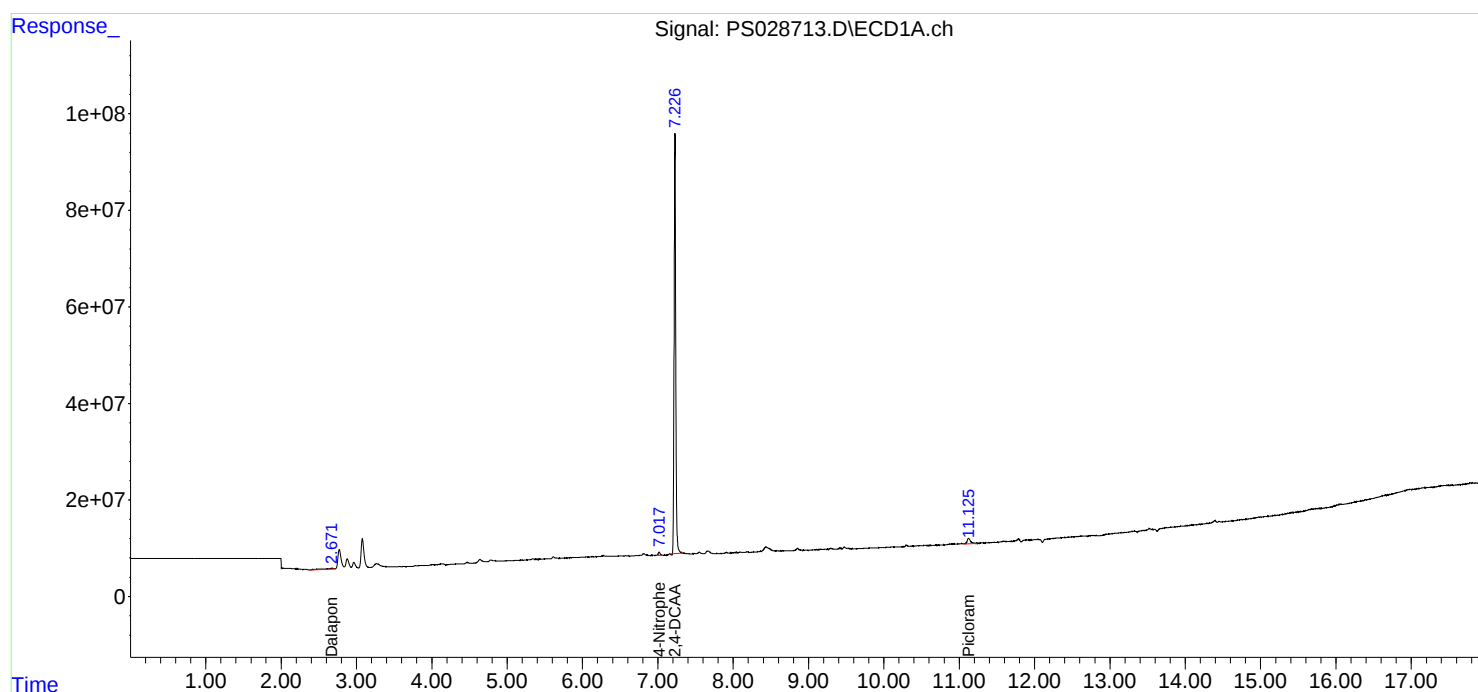


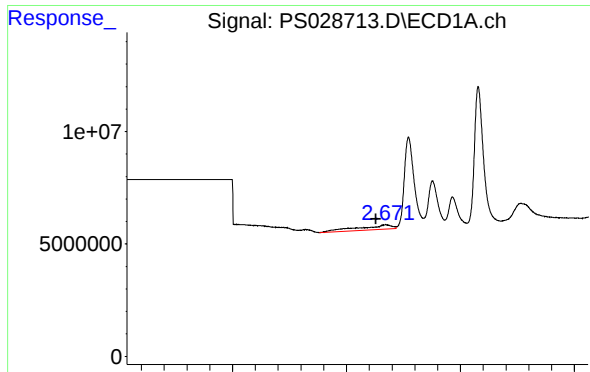

#1 Dalapon


R.T.: 2.673 min
Delta R.T.: 0.043 min
Response: 21236070
Conc: 7.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

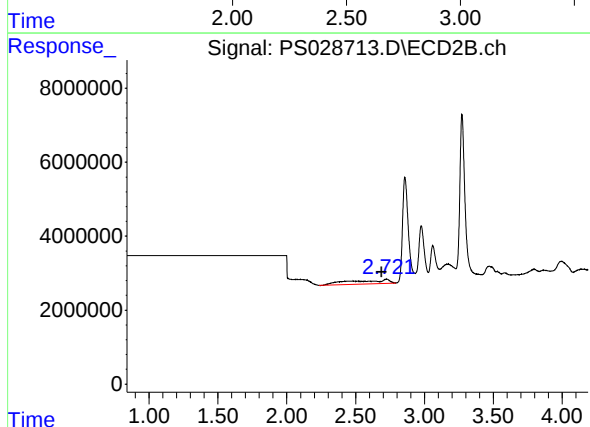


#1 Dalapon

R.T.: 2.722 min
Delta R.T.: 0.033 min
Response: 21273592
Conc: 9.74 ng/ml

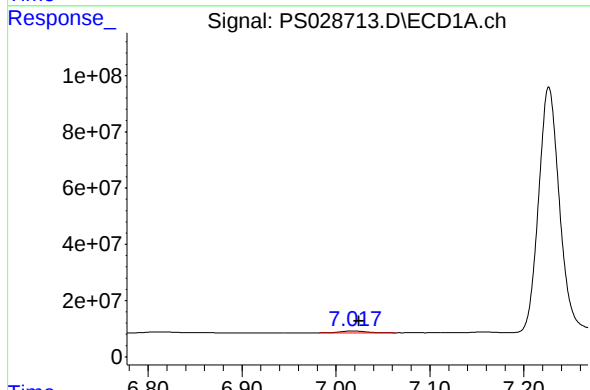


#3 4-Nitrophenol

R.T.: 7.018 min
Delta R.T.: -0.007 min
Response: 11577838
Conc: 6.74 ng/ml

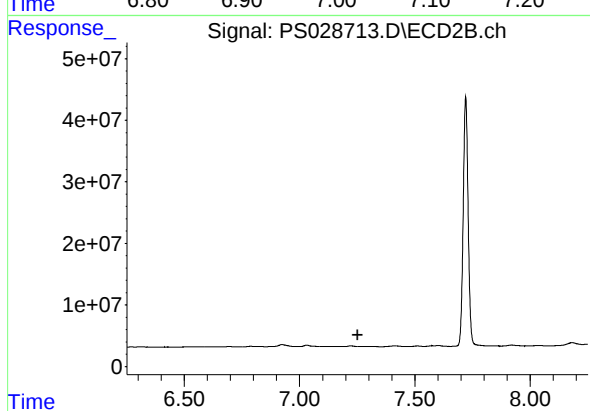

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.251 min
Response: 0
Conc: N.D.

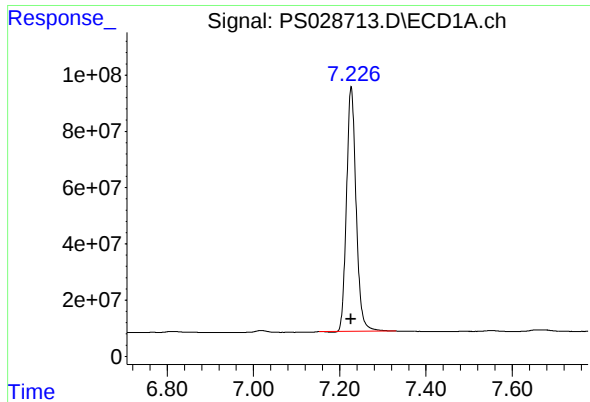

#4 2,4-DCAA


R.T.: 7.227 min
Delta R.T.: 0.000 min
Response: 1343714633
Conc: 500.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

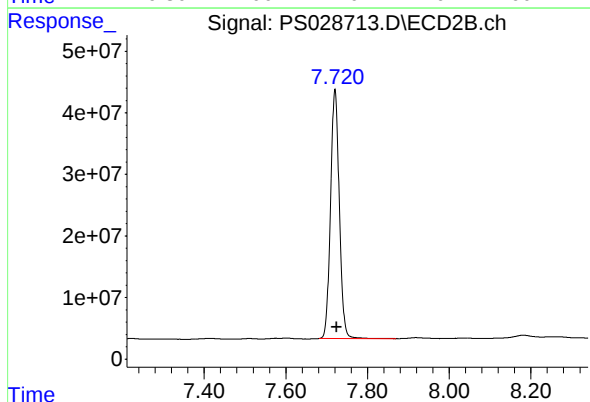


#4 2,4-DCAA

R.T.: 7.720 min
Delta R.T.: -0.004 min
Response: 602834322
Conc: 447.53 ng/ml

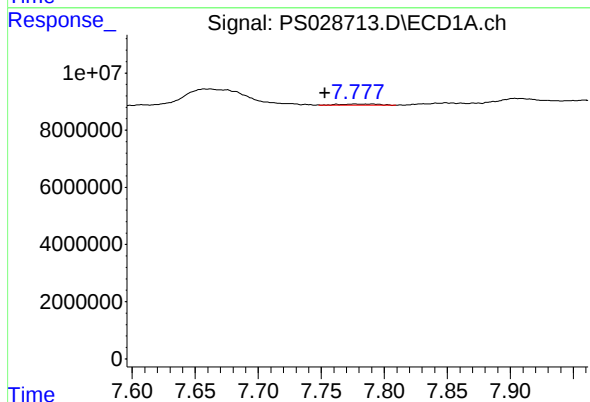


#7 MCPA

R.T.: 7.779 min
Delta R.T.: 0.026 min
Response: 762201
Conc: N.D.

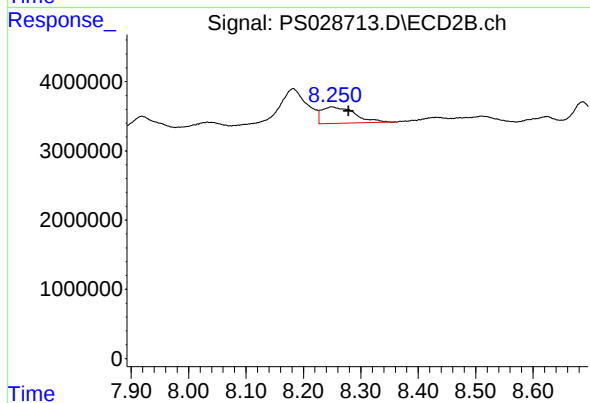

#7 MCPA


R.T.: 8.250 min
Delta R.T.: -0.029 min
Response: 9508812
Conc: 1.53 ug/ml

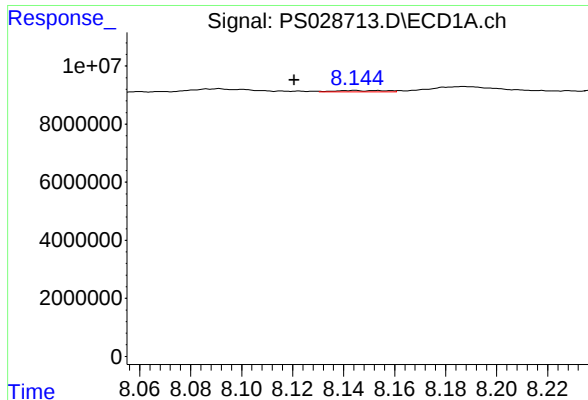

#8 DICHLORPROP


R.T.: 8.143 min
Delta R.T.: 0.023 min
Response: 629389
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

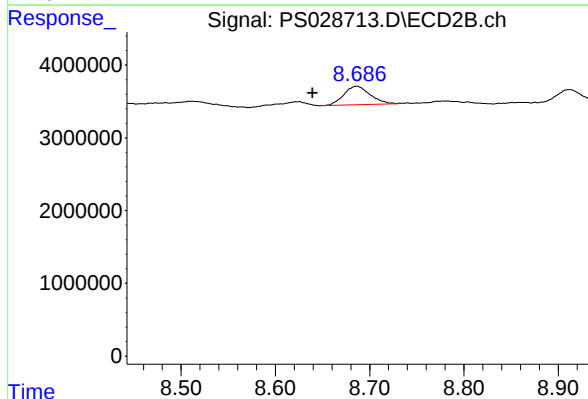


#8 DICHLORPROP

R.T.: 8.686 min
Delta R.T.: 0.047 min
Response: 4894897
Conc: 3.06 ng/ml

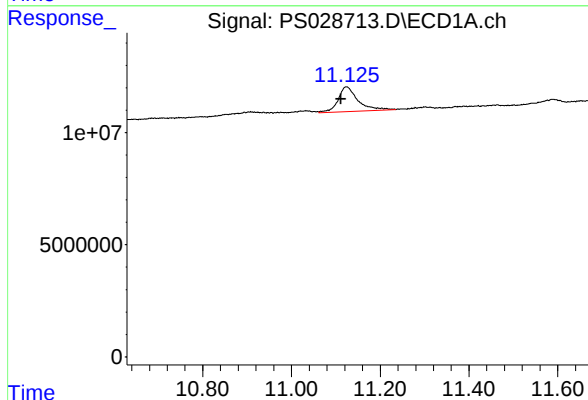

#15 Picloram

R.T.: 11.124 min
Delta R.T.: 0.012 min
Response: 34511894
Conc: 1.16 ng/ml

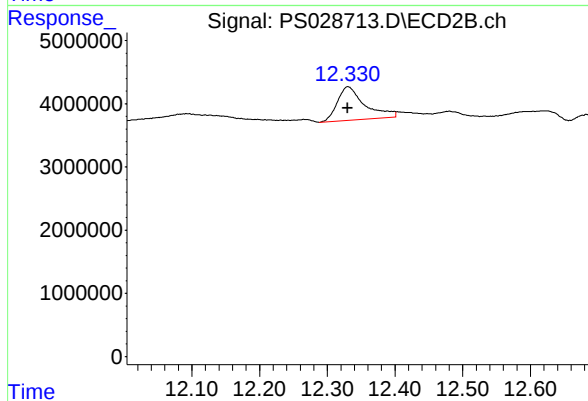

#15 Picloram

R.T.: 12.331 min
Delta R.T.: 0.000 min
Response: 14951881
Conc: 1.16 ng/ml