

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120624\
 Data File : PS028718.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 11:21
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 06 22:56:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	7.721	1344.9E6	606.7E6	501.385	450.414
Target Compounds							
1) T	Dalapon	2.671f	2.723f	20595153	4153532	7.097	1.902 #
3) T	4-Nitroph...	7.019	0.000	6538094	0	3.803	N.D. #
5) T	DICAMBA	7.416	7.917	884265	5661836	<MDL	<MDL #
7) T	MCPA	7.778f	8.241f	956084	11629890	<MDL	1.874 #
8) T	DICHLORPROP	8.123	8.684f	171991	5211988	<MDL	3.260 #
10) T	Pentachlo...	8.647	0.000	1741453	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.228	9.869	6195562	2394034	<MDL	<MDL #
12) T	2,4,5-T	9.528	10.289	20889596	8546940	1.114	<MDL #
13) T	2,4-DB	10.092	0.000	895645	0	<MDL	N.D. #
14) T	DINOSEB	11.301	0.000	2229503	0	<MDL	N.D. #
15) T	Picloram	11.117	12.328	43160807	10279210	1.451	<MDL #
16) T	DCPA	11.582	12.328f	7736902	10279210	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120624\
Data File : PS028718.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 11:21
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 06 22:56:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

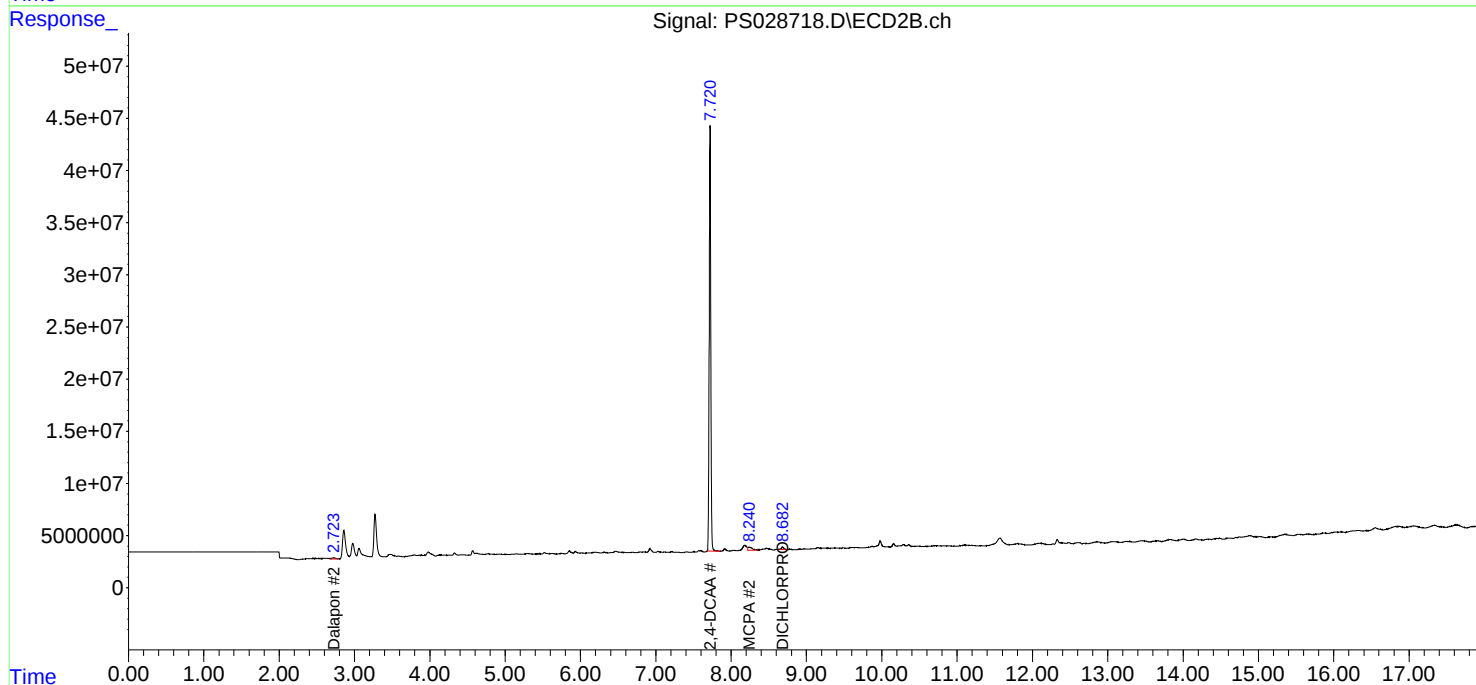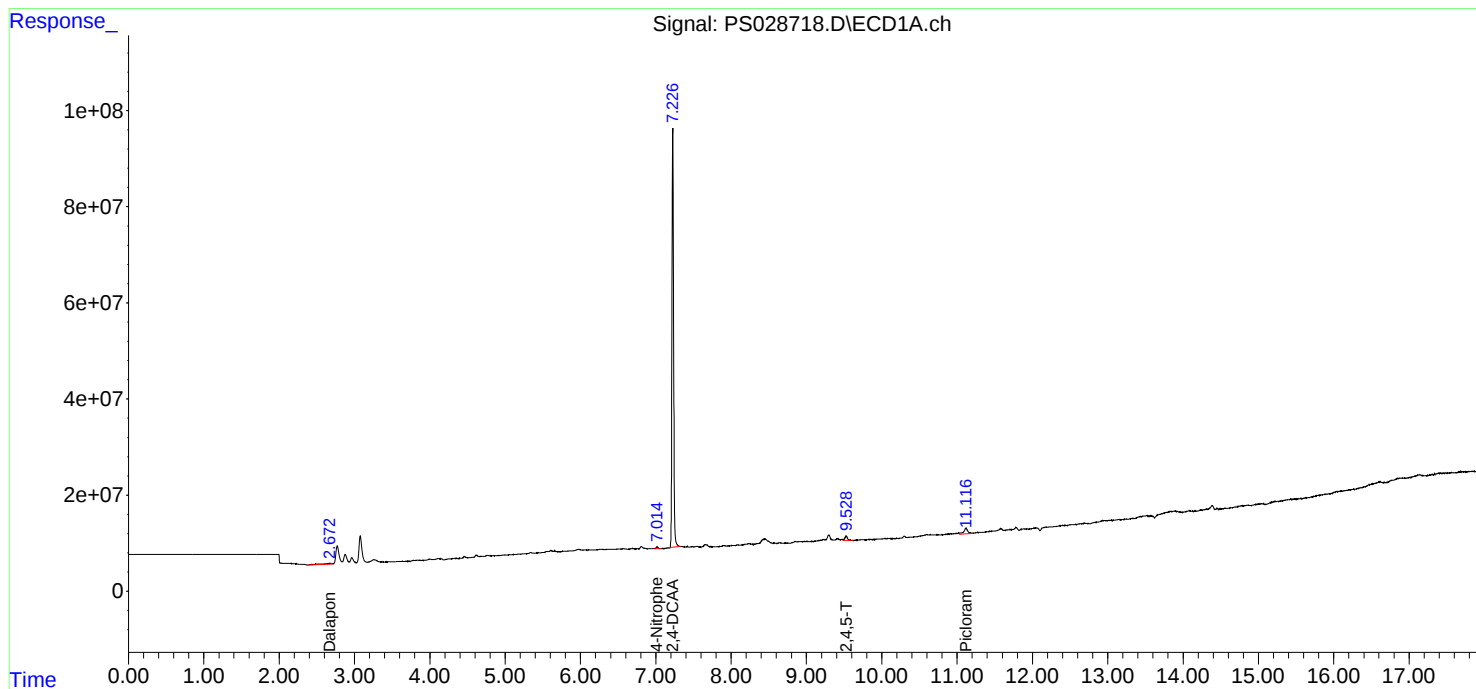


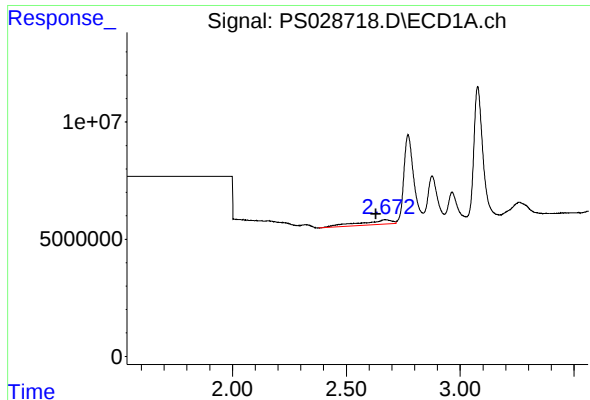

#1 Dalapon


R.T.: 2.671 min
Delta R.T.: 0.041 min
Response: 20595153
Conc: 7.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

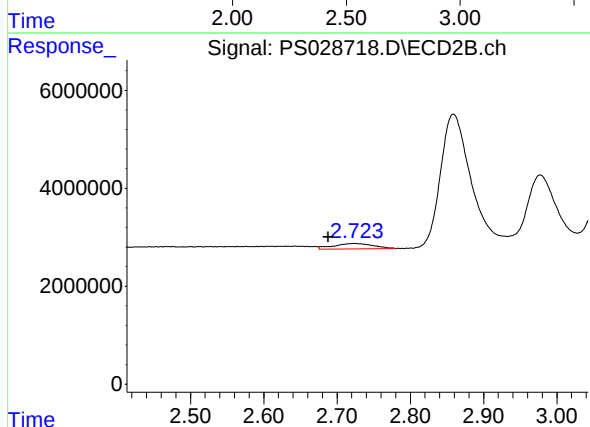


#1 Dalapon

R.T.: 2.723 min
Delta R.T.: 0.035 min
Response: 4153532
Conc: 1.90 ng/ml

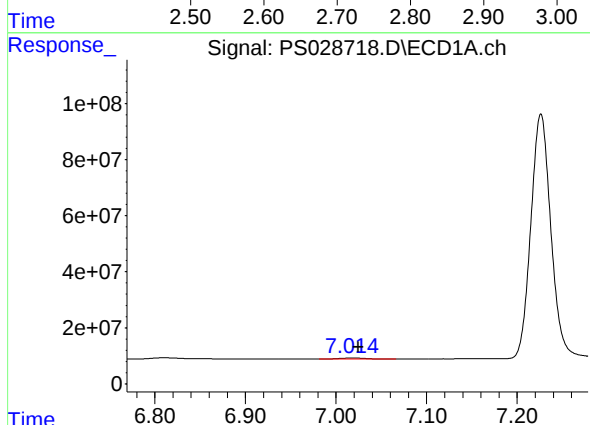


#3 4-Nitrophenol

R.T.: 7.019 min
Delta R.T.: -0.006 min
Response: 6538094
Conc: 3.80 ng/ml

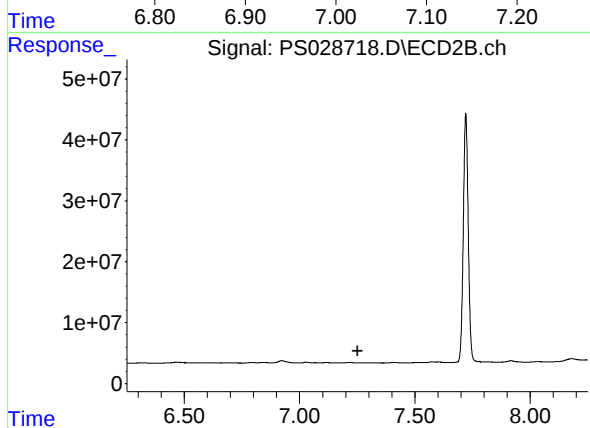

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.251 min
Response: 0
Conc: N.D.

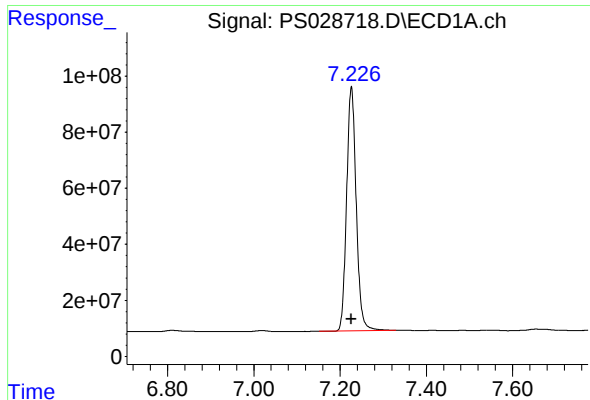

#4 2,4-DCAA


R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 1344885324
Conc: 501.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

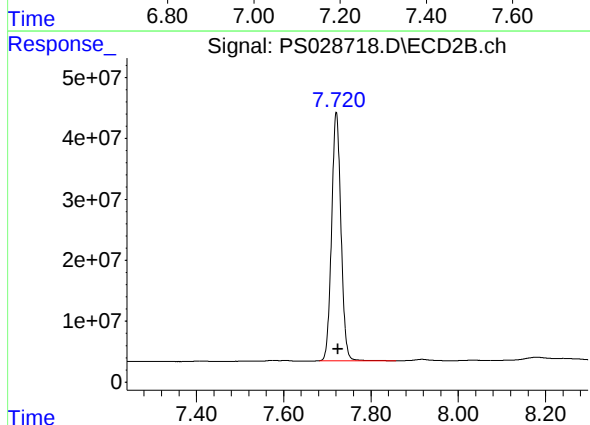


#4 2,4-DCAA

R.T.: 7.721 min
Delta R.T.: -0.004 min
Response: 606720358
Conc: 450.41 ng/ml

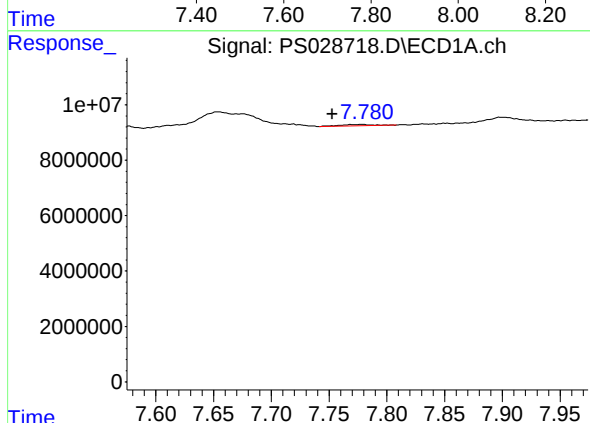


#7 MCPA

R.T.: 7.778 min
Delta R.T.: 0.025 min
Response: 956084
Conc: N.D.

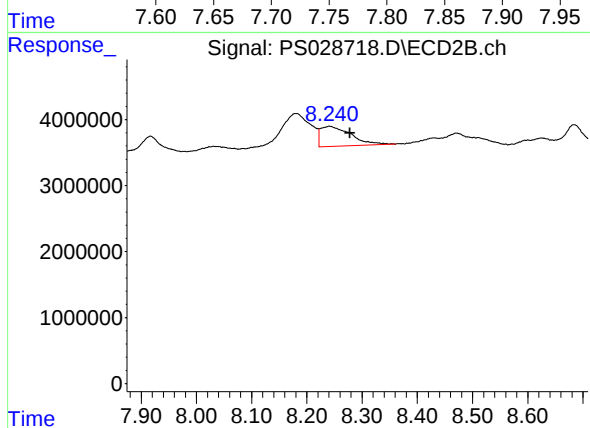

#7 MCPA


R.T.: 8.241 min
Delta R.T.: -0.037 min
Response: 11629890
Conc: 1.87 ug/ml

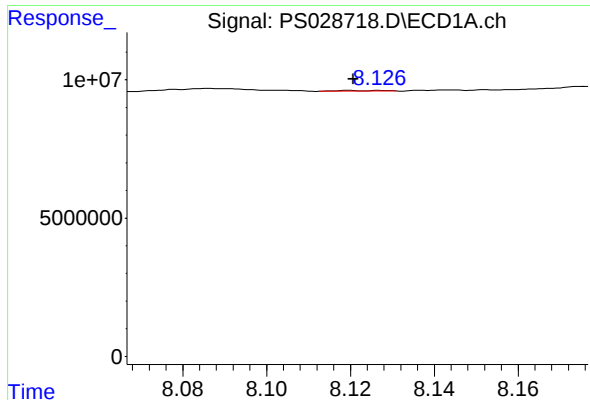

#8 DICHLORPROP


R.T.: 8.123 min
Delta R.T.: 0.002 min
Response: 171991
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

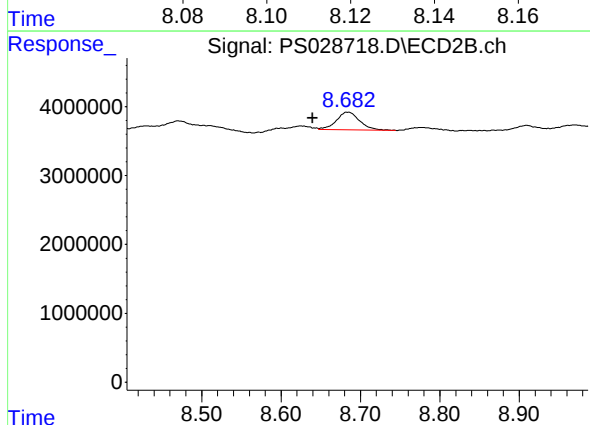


#8 DICHLORPROP

R.T.: 8.684 min
Delta R.T.: 0.044 min
Response: 5211988
Conc: 3.26 ng/ml

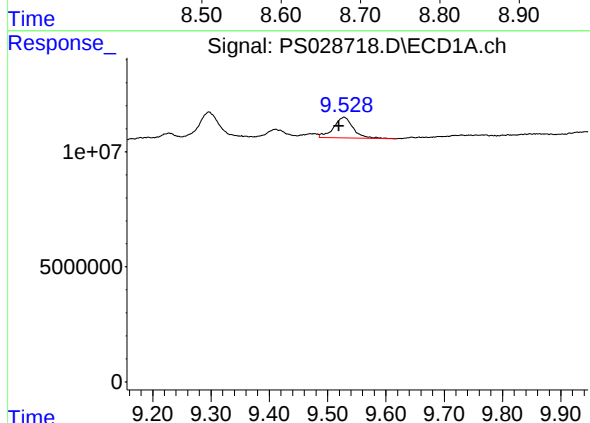


#12 2,4,5-T

R.T.: 9.528 min
Delta R.T.: 0.008 min
Response: 20889596
Conc: 1.11 ng/ml

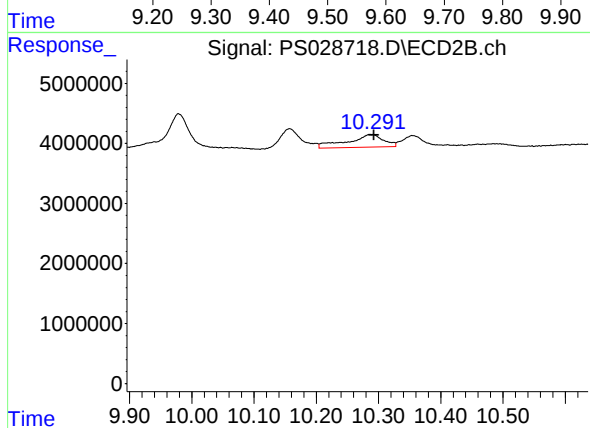

#12 2,4,5-T


R.T.: 10.289 min
Delta R.T.: -0.004 min
Response: 8546940
Conc: N.D.

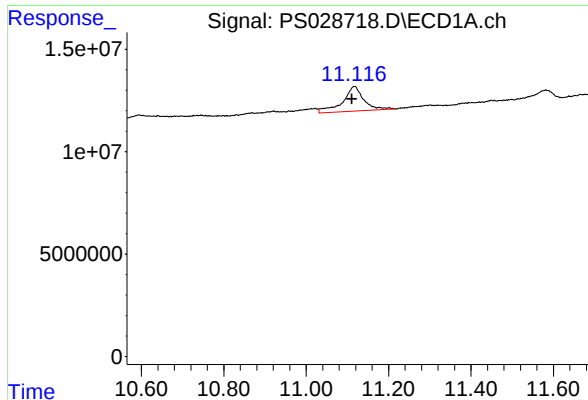

#15 Picloram

R.T.: 11.117 min
Delta R.T.: 0.005 min
Response: 43160807
Conc: 1.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

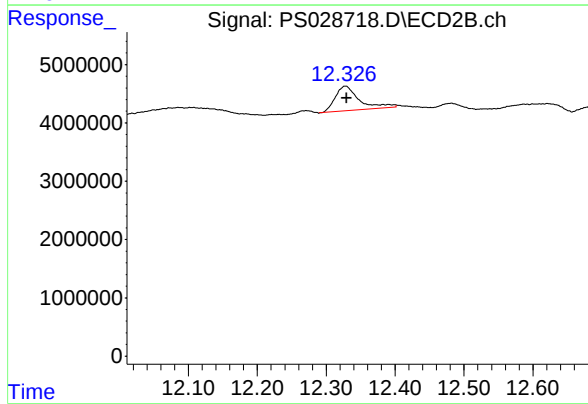

#15 Picloram

R.T.: 12.328 min
Delta R.T.: -0.002 min
Response: 10279210
Conc: N.D.