

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120718\
 Data File : PS002534.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2018 19:19
 Operator : EI\SJ
 Sample : J6214-15
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 06:31:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 10 06:14:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.394	10.890	85775496	93136460	270.227	240.806
Target Compounds							
3) T	4-Nitroph...	11.041	10.044	8265120	18913502	52.166	105.817 #
5) T	DICAMBA	11.765	11.186	9277157	8963540	6.561	6.288
6) T	MCP	12.065	11.396	22754414	4669733	22.806	4.995 #
7) T	MCPA	12.318	11.794	-3331744	38936211	N.D.	27.087
8) T	DICHLORPROP	12.950	12.302	10305190	2142736	28.981	5.991 #
10) T	Pentachlo...	13.625	13.323	12509604	3059685	2.495	0.582 #
11) T	2,4,5-TP ...	0.000	13.988	0	27346713	N.D.	13.025 #
12) T	2,4,5-T	14.935	14.545	2435405	1541697	1.296	0.901 #
13) T	2,4-DB	15.677	0.000	21787142	0	96.333	N.D. #
14) T	DINOSEB	17.108	15.612	4200970	10122712	2.887	6.633 #
15) T	Picloram	16.917	16.751	7041040	23762137	2.774	8.637 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120718\
Data File : PS002534.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2018 19:19
Operator : EI\SJ
Sample : J6214-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 06:31:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
Quant Title : 8080.M
QLast Update : Mon Dec 10 06:14:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

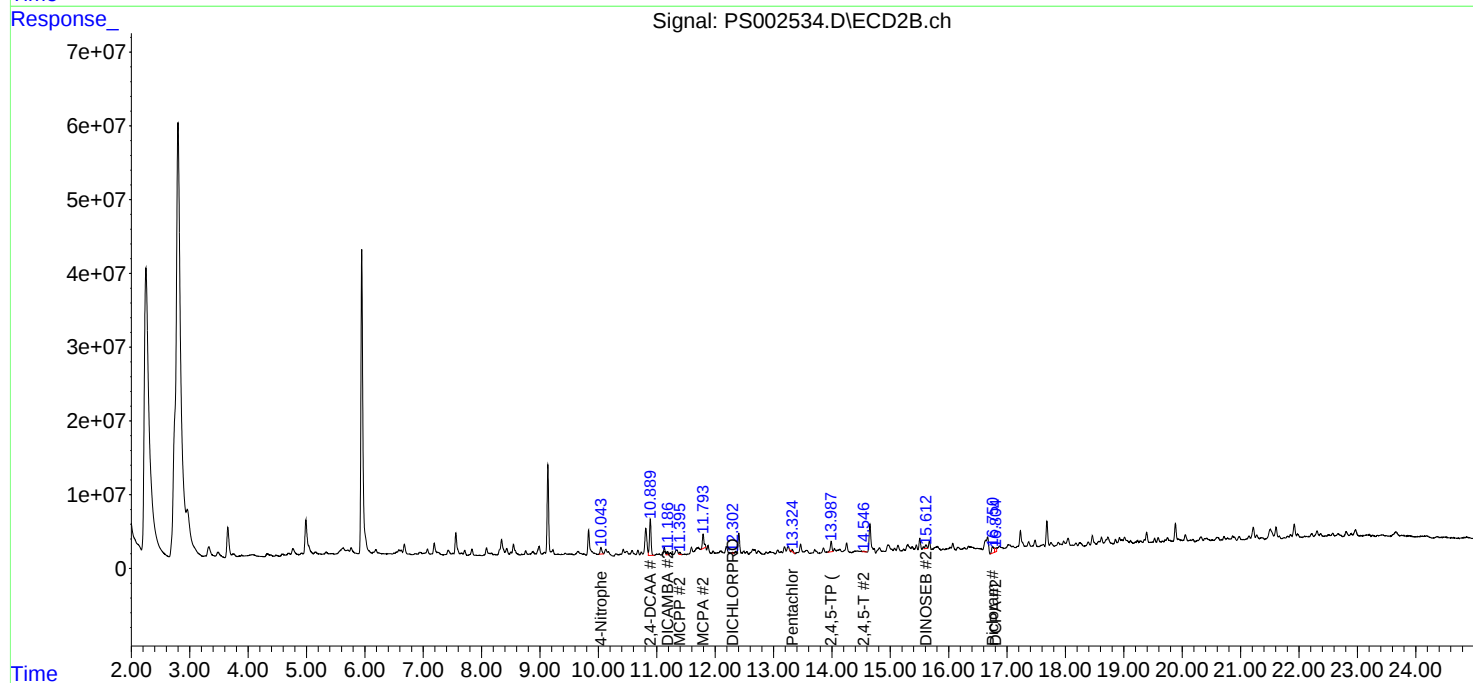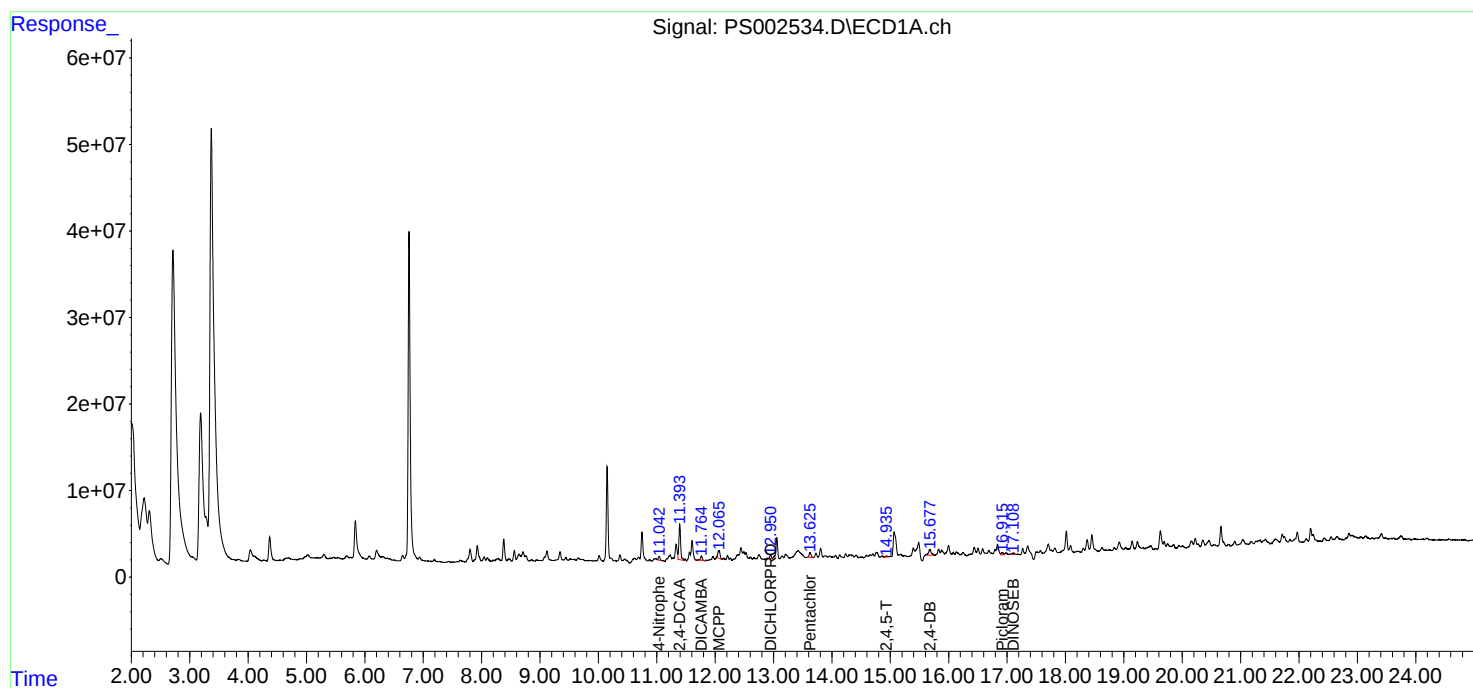


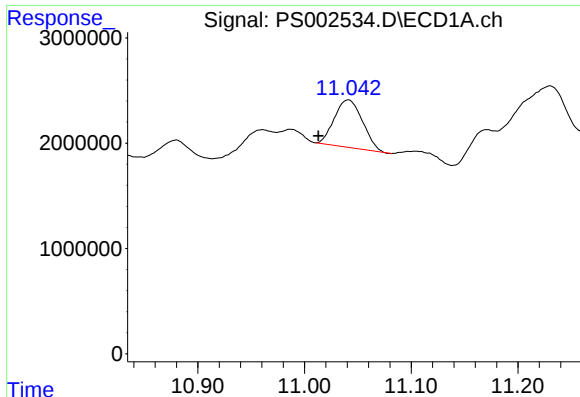

#3 4-Nitrophenol


R.T.: 11.041 min
Delta R.T.: 0.028 min
Response: 8265120
Conc: 52.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

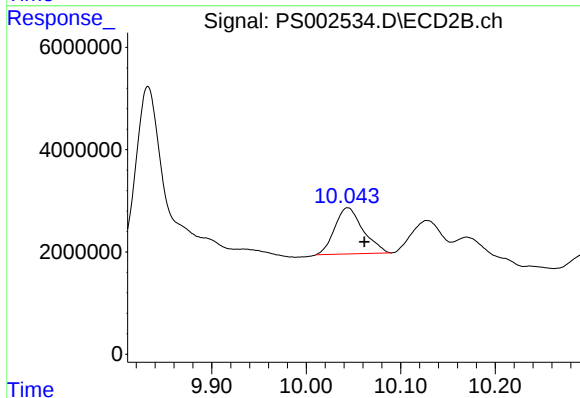


#3 4-Nitrophenol

R.T.: 10.044 min
Delta R.T.: -0.017 min
Response: 18913502
Conc: 105.82 ng/ml

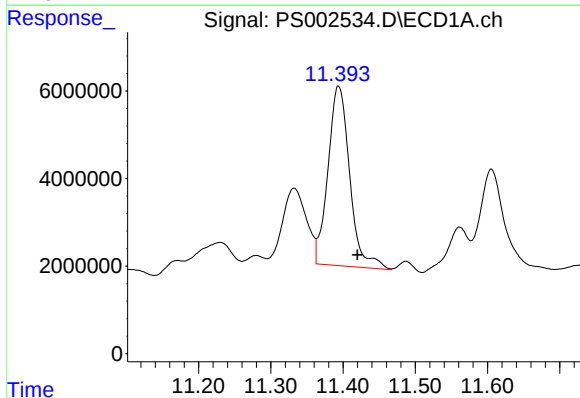


#4 2,4-DCAA

R.T.: 11.394 min
Delta R.T.: -0.026 min
Response: 85775496
Conc: 270.23 ng/ml

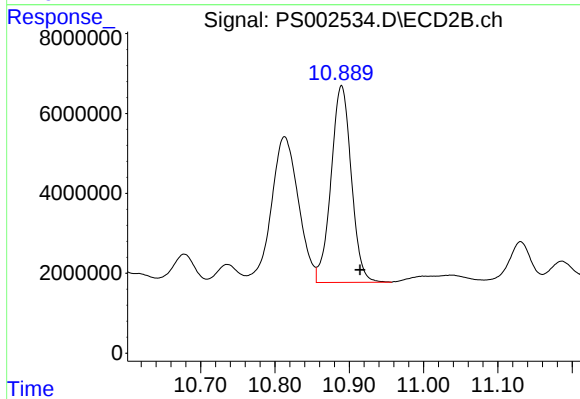

#4 2,4-DCAA


R.T.: 10.890 min
Delta R.T.: -0.025 min
Response: 93136460
Conc: 240.81 ng/ml

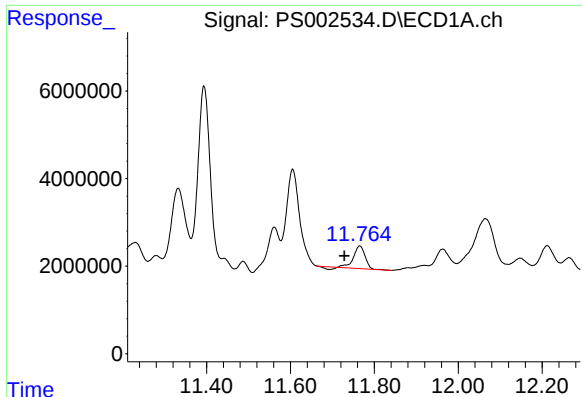

#5 DICAMBA


R.T.: 11.765 min
Delta R.T.: 0.036 min
Response: 9277157
Conc: 6.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

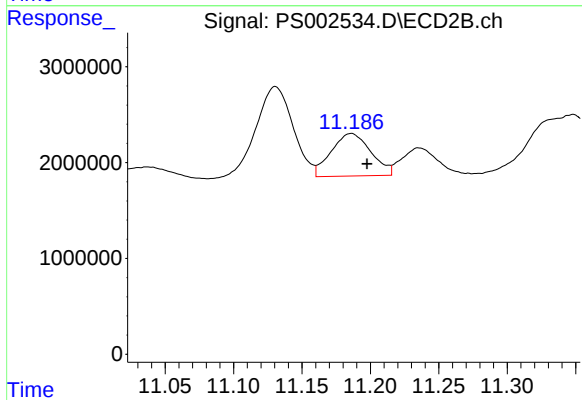


#5 DICAMBA

R.T.: 11.186 min
Delta R.T.: -0.012 min
Response: 8963540
Conc: 6.29 ng/ml

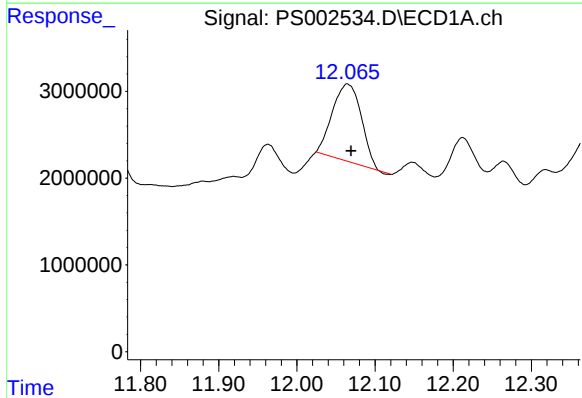


#6 MCP

R.T.: 12.065 min
Delta R.T.: -0.005 min
Response: 22754414
Conc: 22.81 ug/ml

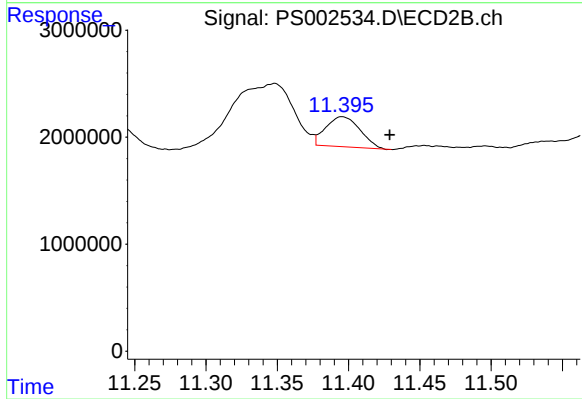

#6 MCP


R.T.: 11.396 min
Delta R.T.: -0.033 min
Response: 4669733
Conc: 4.99 ug/ml

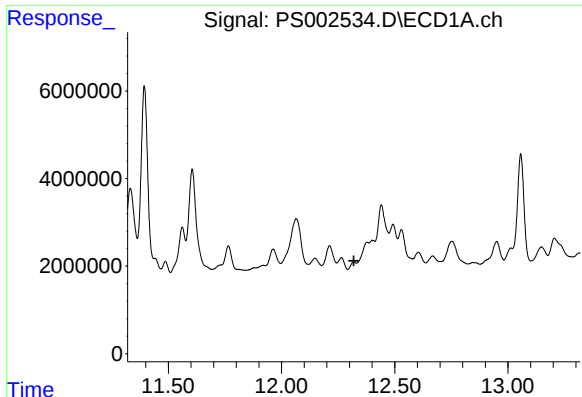

#7 MCPA


R.T.: 12.318 min
Delta R.T.: 0.000 min
Response: -3331744
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

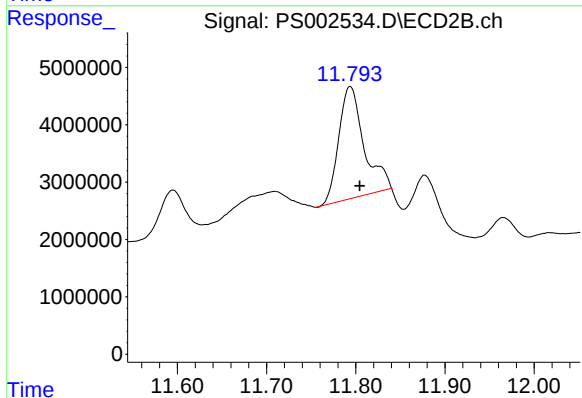


#7 MCPA

R.T.: 11.794 min
Delta R.T.: -0.011 min
Response: 38936211
Conc: 27.09 ug/ml

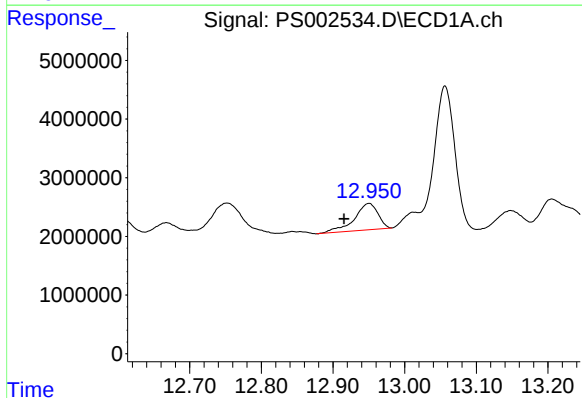


#8 DICHLORPROP

R.T.: 12.950 min
Delta R.T.: 0.034 min
Response: 10305190
Conc: 28.98 ng/ml

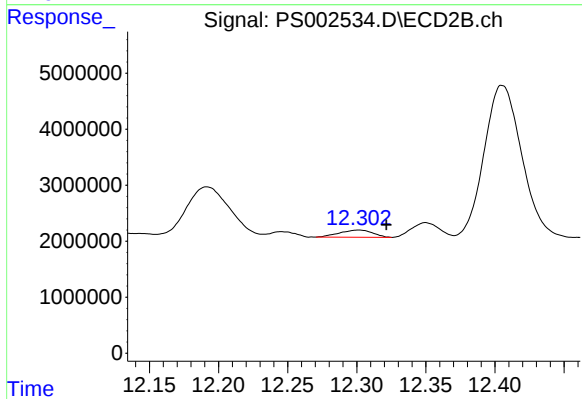

#8 DICHLORPROP


R.T.: 12.302 min
Delta R.T.: -0.020 min
Response: 2142736
Conc: 5.99 ng/ml

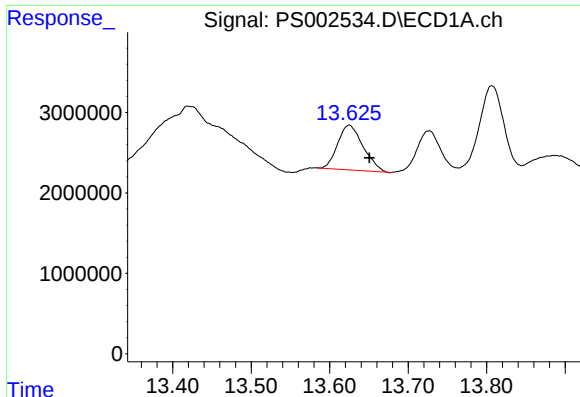

#10 Pentachlorophenol


R.T.: 13.625 min
Delta R.T.: -0.026 min
Response: 12509604
Conc: 2.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

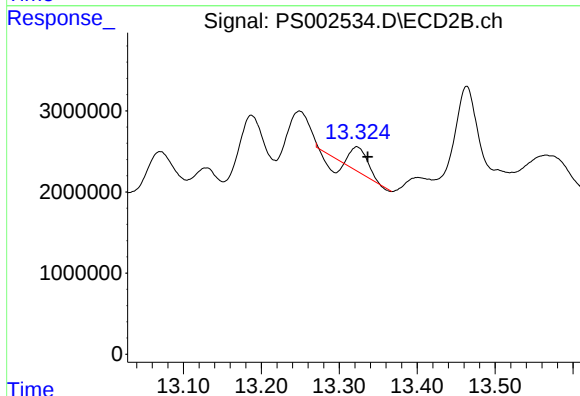


#10 Pentachlorophenol

R.T.: 13.323 min
Delta R.T.: -0.014 min
Response: 3059685
Conc: 0.58 ng/ml

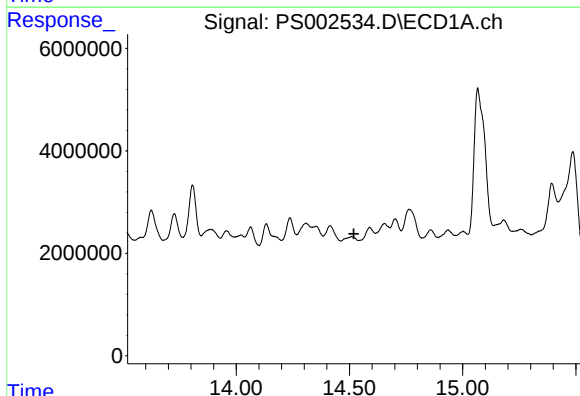


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.519 min
Response: 0
Conc: N.D.

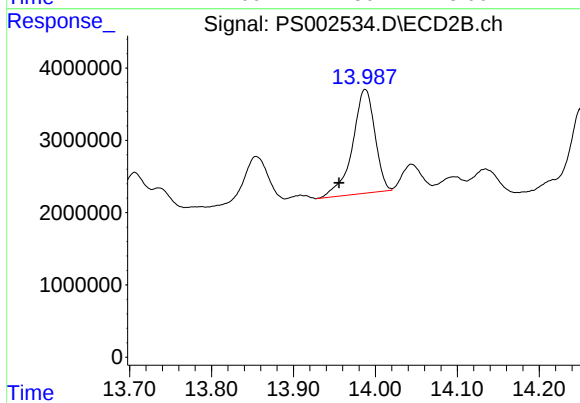

#11 2,4,5-TP (SILVEX)


R.T.: 13.988 min
Delta R.T.: 0.032 min
Response: 27346713
Conc: 13.03 ng/ml

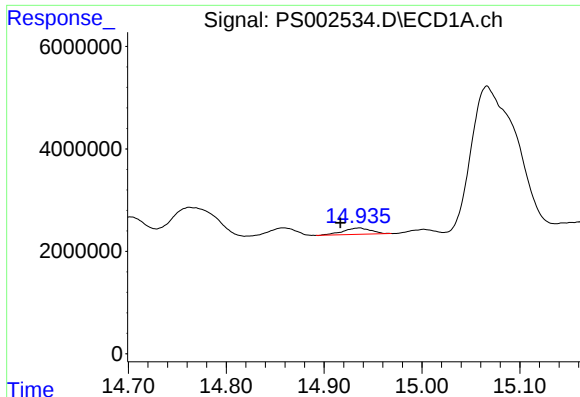

#12 2,4,5-T


R.T.: 14.935 min
Delta R.T.: 0.019 min
Response: 2435405
Conc: 1.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

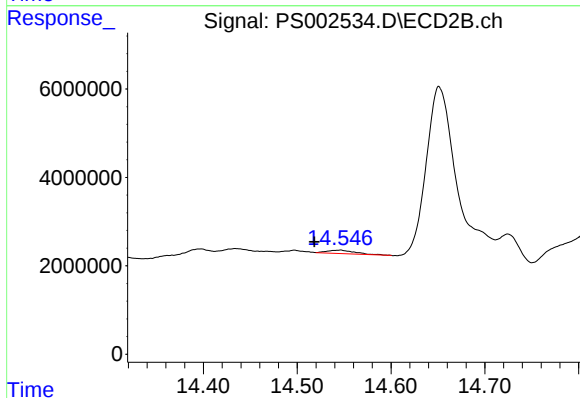


#12 2,4,5-T

R.T.: 14.545 min
Delta R.T.: 0.026 min
Response: 1541697
Conc: 0.90 ng/ml

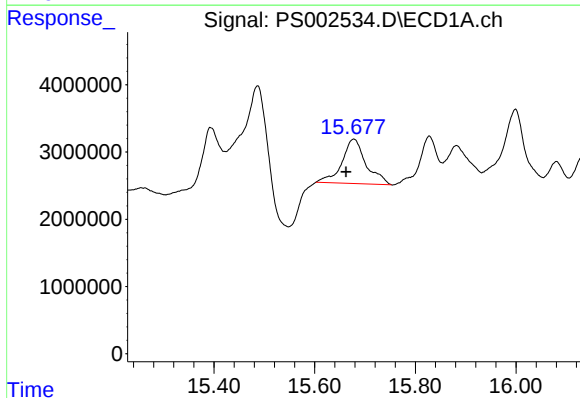


#13 2,4-DB

R.T.: 15.677 min
Delta R.T.: 0.015 min
Response: 21787142
Conc: 96.33 ng/ml

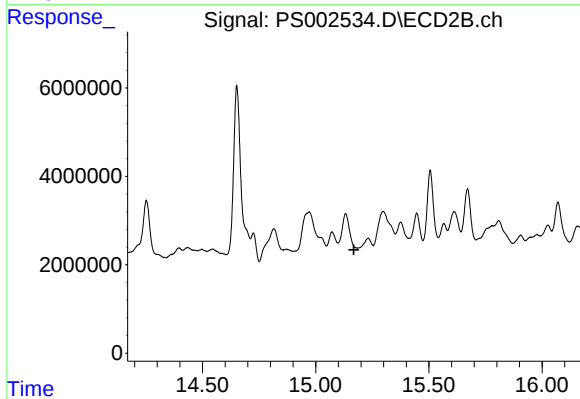

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 15.169 min
Response: 0
Conc: N.D.

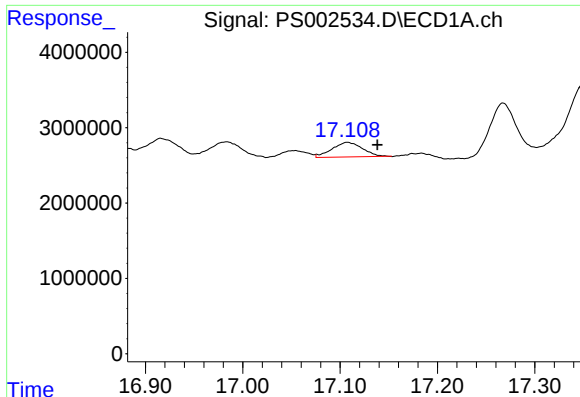

#14 DINOSEB


R.T.: 17.108 min
Delta R.T.: -0.030 min
Response: 4200970
Conc: 2.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

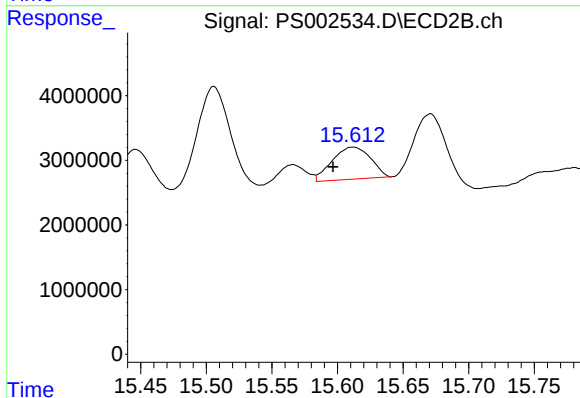


#14 DINOSEB

R.T.: 15.612 min
Delta R.T.: 0.015 min
Response: 10122712
Conc: 6.63 ng/ml

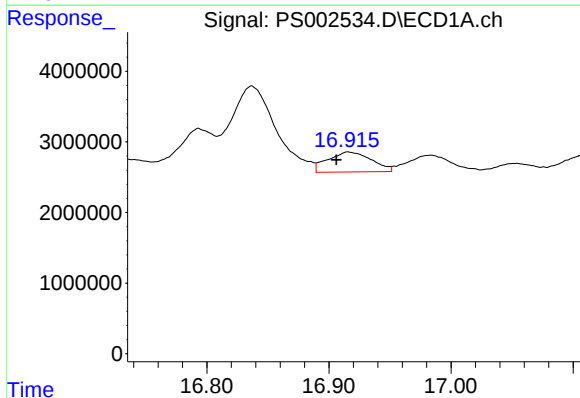


#15 Picloram

R.T.: 16.917 min
Delta R.T.: 0.011 min
Response: 7041040
Conc: 2.77 ng/ml

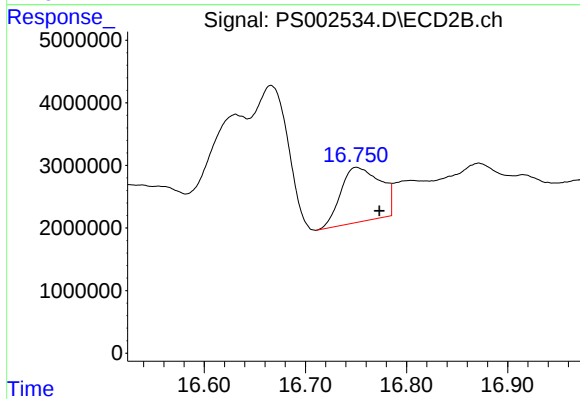

#15 Picloram


R.T.: 16.751 min
Delta R.T.: -0.022 min
Response: 23762137
Conc: 8.64 ng/ml

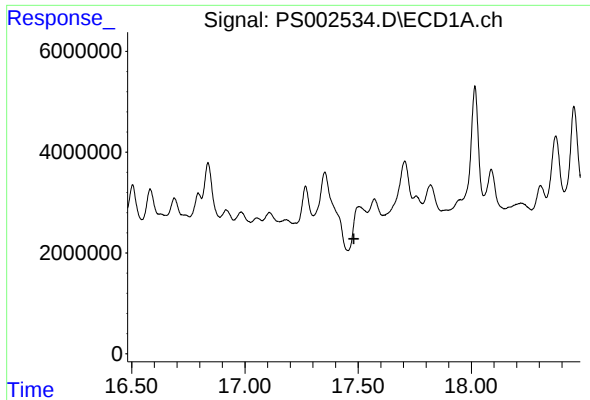

#16 DCPA

R.T.: 17.505 min
Delta R.T.: 0.024 min
Response: -15662899
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

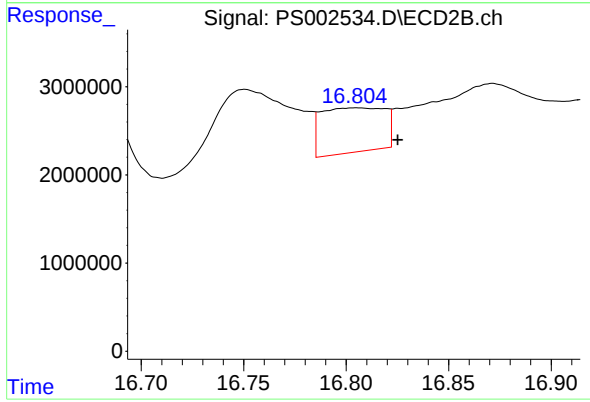

#16 DCPA

R.T.: 16.805 min
Delta R.T.: -0.020 min
Response: 10838214
Conc: 3.73 ng/ml