

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120722\
 Data File : PS021374.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2022 13:32
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 16:02:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.381	6.815	1419.5E6	871.5E6	488.548	505.510
Target Compounds							
1) T	Dalapon	2.529f	0.000	59309	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.765	0.000	2817367	0	<MDL	N.D. #
3) T	4-Nitroph...	6.226	0.000	4997162	0	2.779	N.D. #
5) T	DICAMBA	6.524	6.982	1280125	9545424	<MDL	1.250 #
6) T	MCPD	0.000	7.133f	0	2425985	N.D.	<MDL
7) T	MCPA	6.749f	7.214f	6800298	47117064	<MDL	5.328 #
8) T	DICHLORPROP	7.129	7.627	2108031	3830569	<MDL	1.945 #
9) T	2,4-D	0.000	7.909	0	1926242	N.D.	<MDL
10) T	Pentachlo...	7.553	8.324	8143060	8779679	<MDL	<MDL #
11) T	2,4,5-TP ...	8.087	8.690	8604931	3612418	<MDL	<MDL #
12) T	2,4,5-T	8.361	9.075	21710587	15106006	1.151	1.394
13) T	2,4-DB	8.880	9.590	3173782	2076451	<MDL	1.444 #
14) T	DINOSEB	9.900	9.899	28683376	3641386	1.800	<MDL #
15) T	Picloram	9.721	10.888	199608	169.5E6	<MDL	10.422 #
16) T	DCPA	10.171	10.827	10353342	5343479	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120722\
Data File : PS021374.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2022 13:32
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 16:02:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

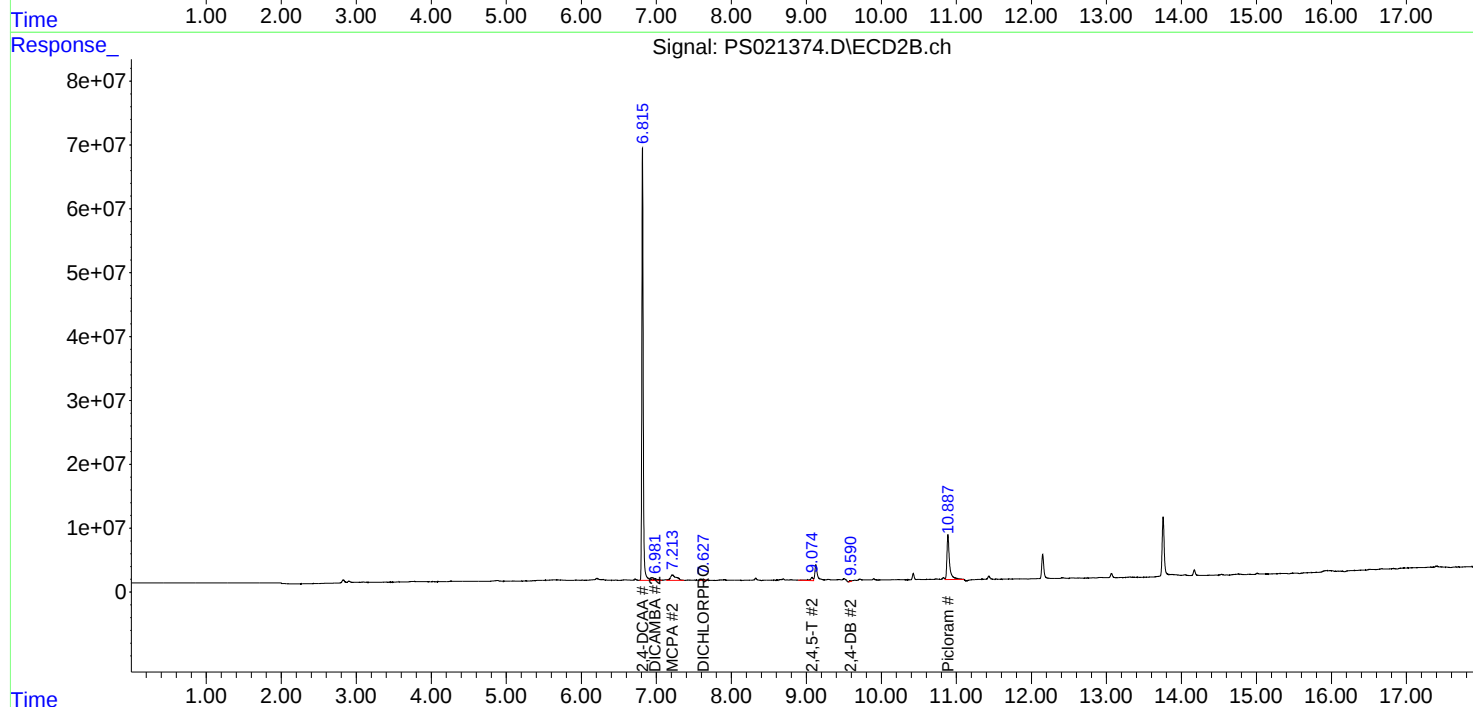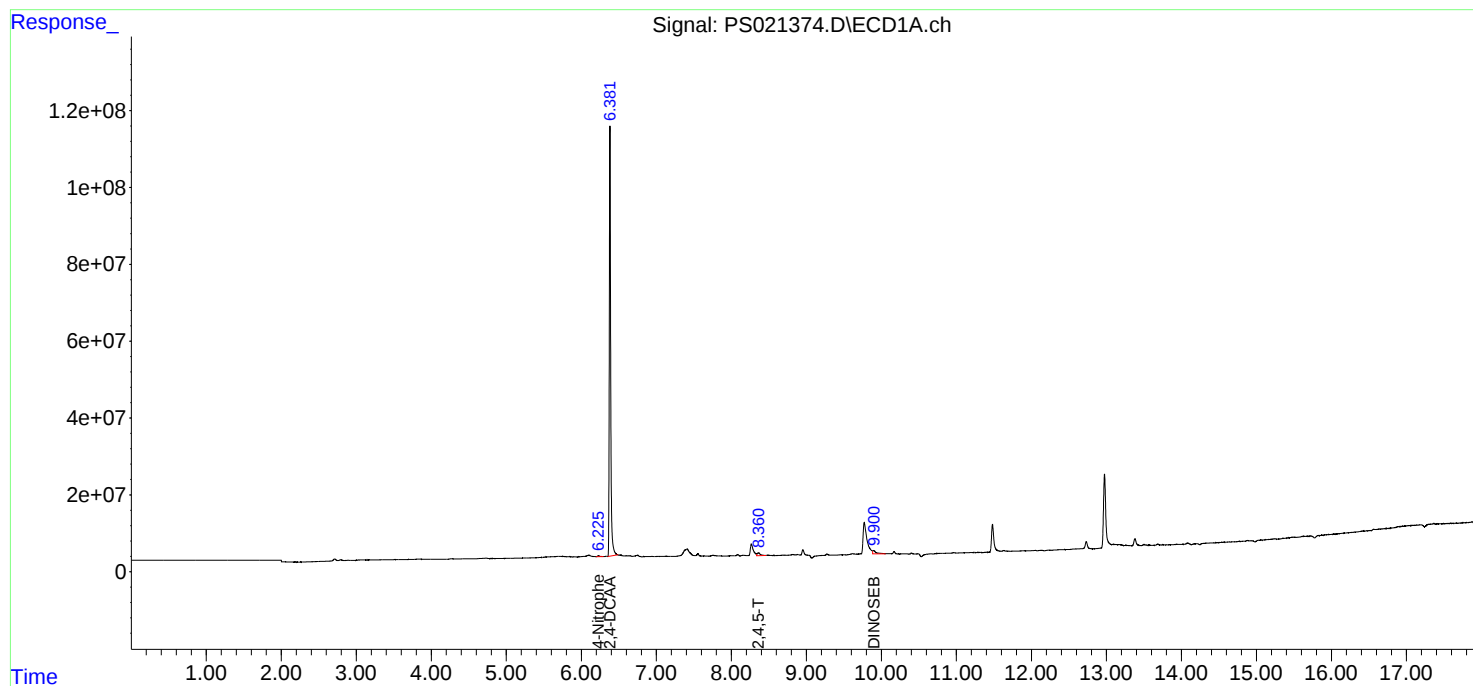


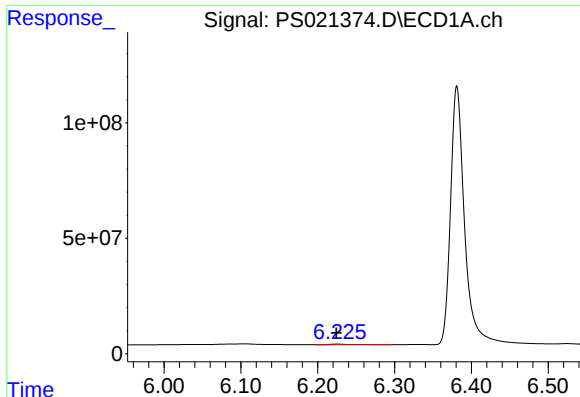

#3 4-Nitrophenol


R.T.: 6.226 min
Delta R.T.: 0.001 min
Response: 4997162
Conc: 2.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

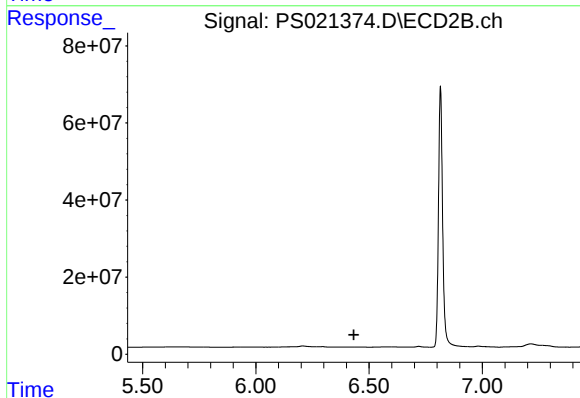


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

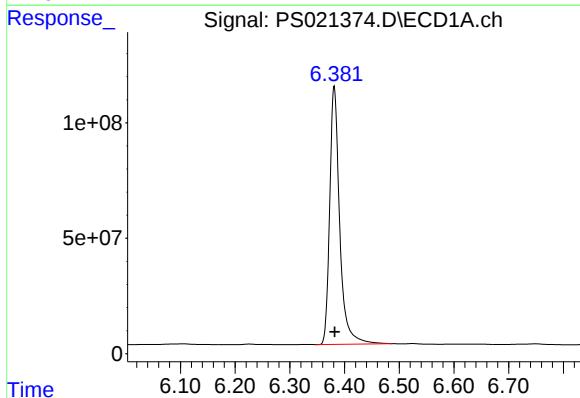


#4 2,4-DCAA

R.T.: 6.381 min
Delta R.T.: 0.000 min
Response: 1419473522
Conc: 488.55 ng/ml

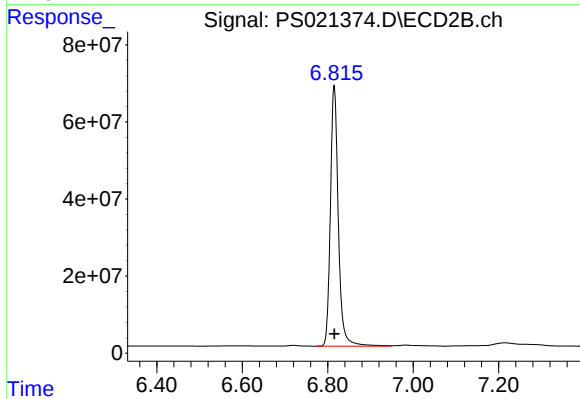

#4 2,4-DCAA


R.T.: 6.815 min
Delta R.T.: 0.000 min
Response: 871496184
Conc: 505.51 ng/ml

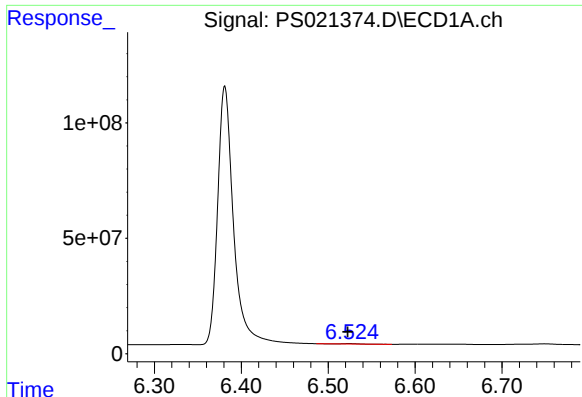

#5 DICAMBA


R.T.: 6.524 min
Delta R.T.: 0.002 min
Response: 1280125
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

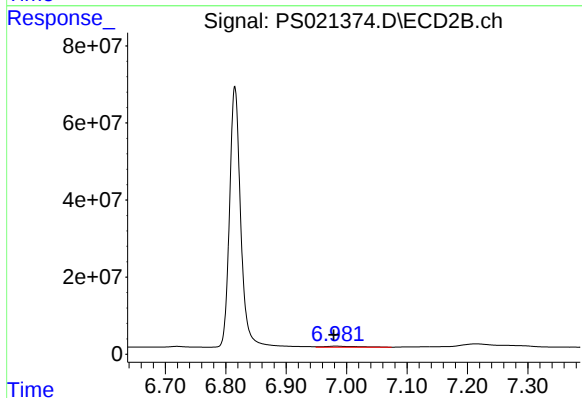


#5 DICAMBA

R.T.: 6.982 min
Delta R.T.: 0.004 min
Response: 9545424
Conc: 1.25 ng/ml

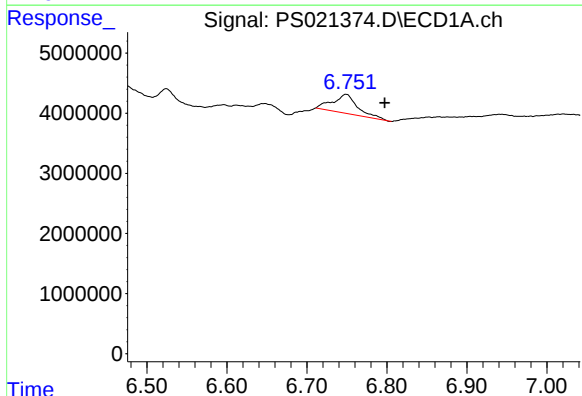


#7 MCPA

R.T.: 6.749 min
Delta R.T.: -0.048 min
Response: 6800298
Conc: N.D.

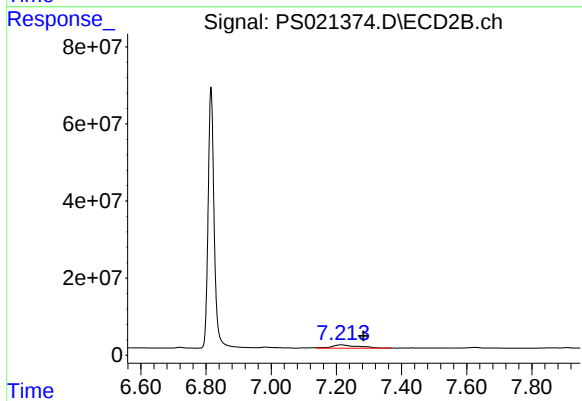

#7 MCPA


R.T.: 7.214 min
Delta R.T.: -0.069 min
Response: 47117064
Conc: 5.33 ug/ml

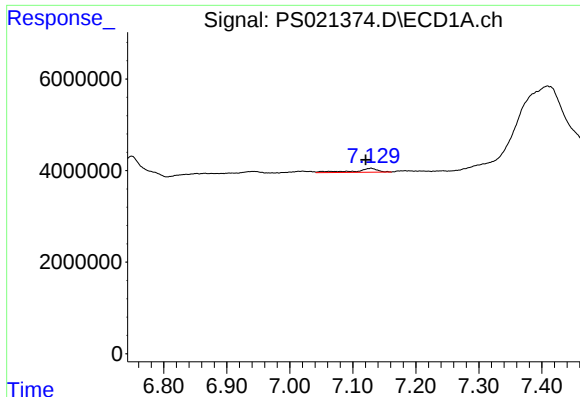

#8 DICHLORPROP


R.T.: 7.129 min
Delta R.T.: 0.008 min
Response: 2108031
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

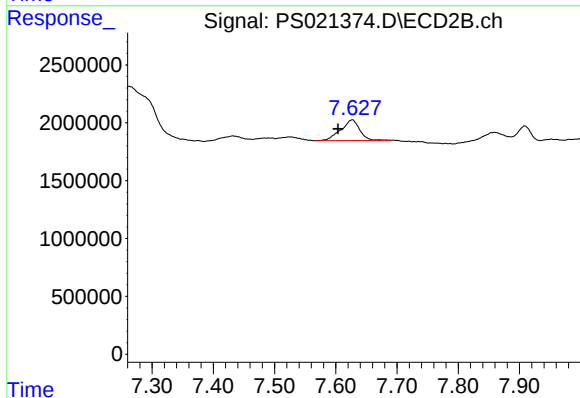


#8 DICHLORPROP

R.T.: 7.627 min
Delta R.T.: 0.023 min
Response: 3830569
Conc: 1.94 ng/ml

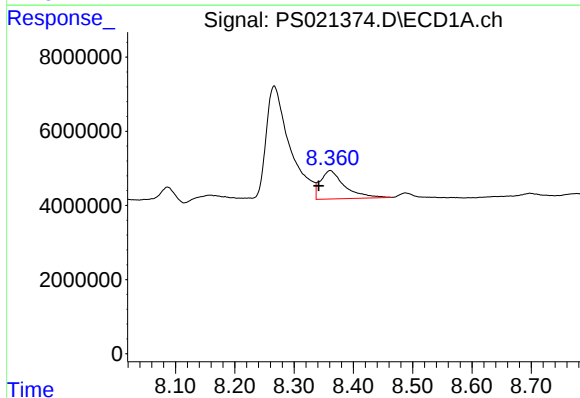


#12 2,4,5-T

R.T.: 8.361 min
Delta R.T.: 0.019 min
Response: 21710587
Conc: 1.15 ng/ml

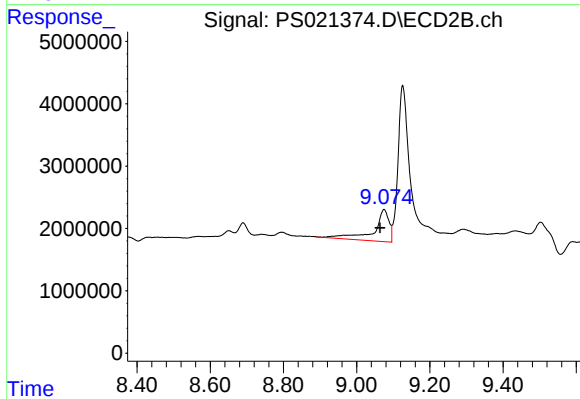

#12 2,4,5-T


R.T.: 9.075 min
Delta R.T.: 0.011 min
Response: 15106006
Conc: 1.39 ng/ml

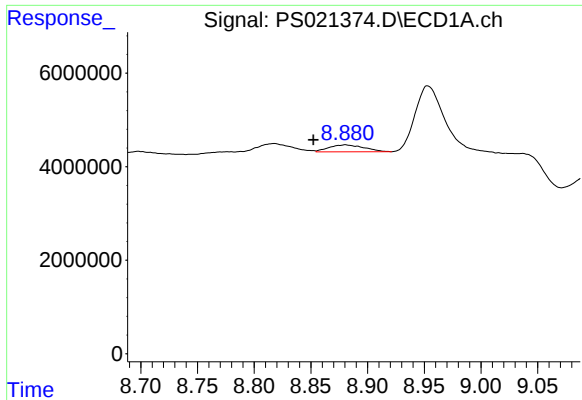

#13 2,4-DB


R.T.: 8.880 min
Delta R.T.: 0.028 min
Response: 3173782
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

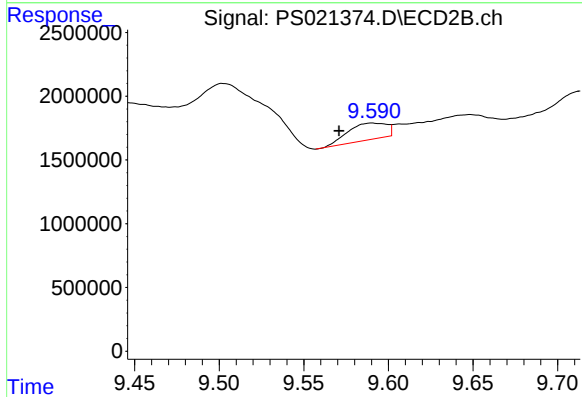


#13 2,4-DB

R.T.: 9.590 min
Delta R.T.: 0.019 min
Response: 2076451
Conc: 1.44 ng/ml

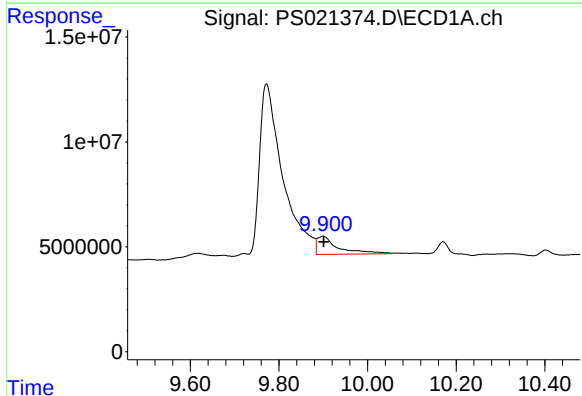


#14 DINOSEB

R.T.: 9.900 min
Delta R.T.: -0.001 min
Response: 28683376
Conc: 1.80 ng/ml

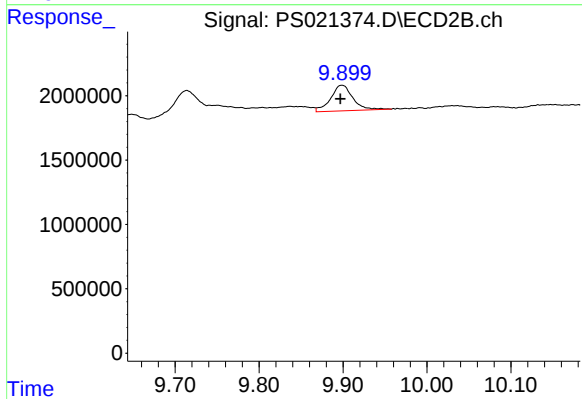

#14 DINOSEB


R.T.: 9.899 min
Delta R.T.: 0.002 min
Response: 3641386
Conc: N.D.

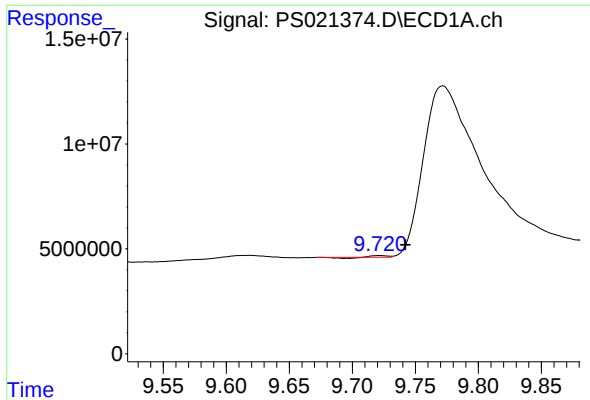

#15 Picloram

R.T.: 9.721 min
Delta R.T.: -0.021 min
Response: 199608
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

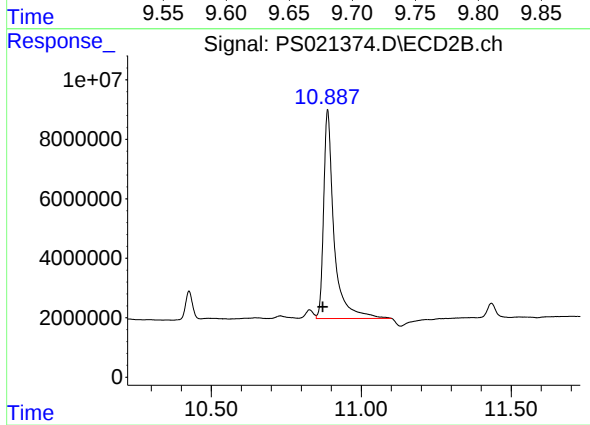

#15 Picloram

R.T.: 10.888 min
Delta R.T.: 0.016 min
Response: 169472242
Conc: 10.42 ng/ml