

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120723\
 Data File : PS025031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2023 10:27
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 23:28:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	2.512	2.561	11609190	4962306	4.026	4.326
2) T	3,5-DICHL...	5.697	0.000	30530984	0	9.033	N.D. #
5) T	DICAMBA	0.000	6.928	0	388655	N.D.	<MDL
6) T	MCPP	6.678	6.972f	9079618	26133149	1.326	12.599 #
7) T	MCPA	0.000	7.239	0	3176926	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.556	0	5137263	N.D.	6.531
9) T	2,4-D	7.244	7.856	204.0E6	363122	67.170	<MDL #
11) T	2,4,5-TP ...	0.000	8.558f	0	1051762	N.D.	<MDL
12) T	2,4,5-T	0.000	8.977	0	670340	N.D.	<MDL
13) T	2,4-DB	0.000	9.471	0	1003500	N.D.	1.813
15) T	Picloram	9.677	10.760	73702883	21944826	3.782	3.353
16) T	DCPA	0.000	10.760	0	21944826	N.D.	4.049



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120723\
Data File : PS025031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2023 10:27
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 23:28:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

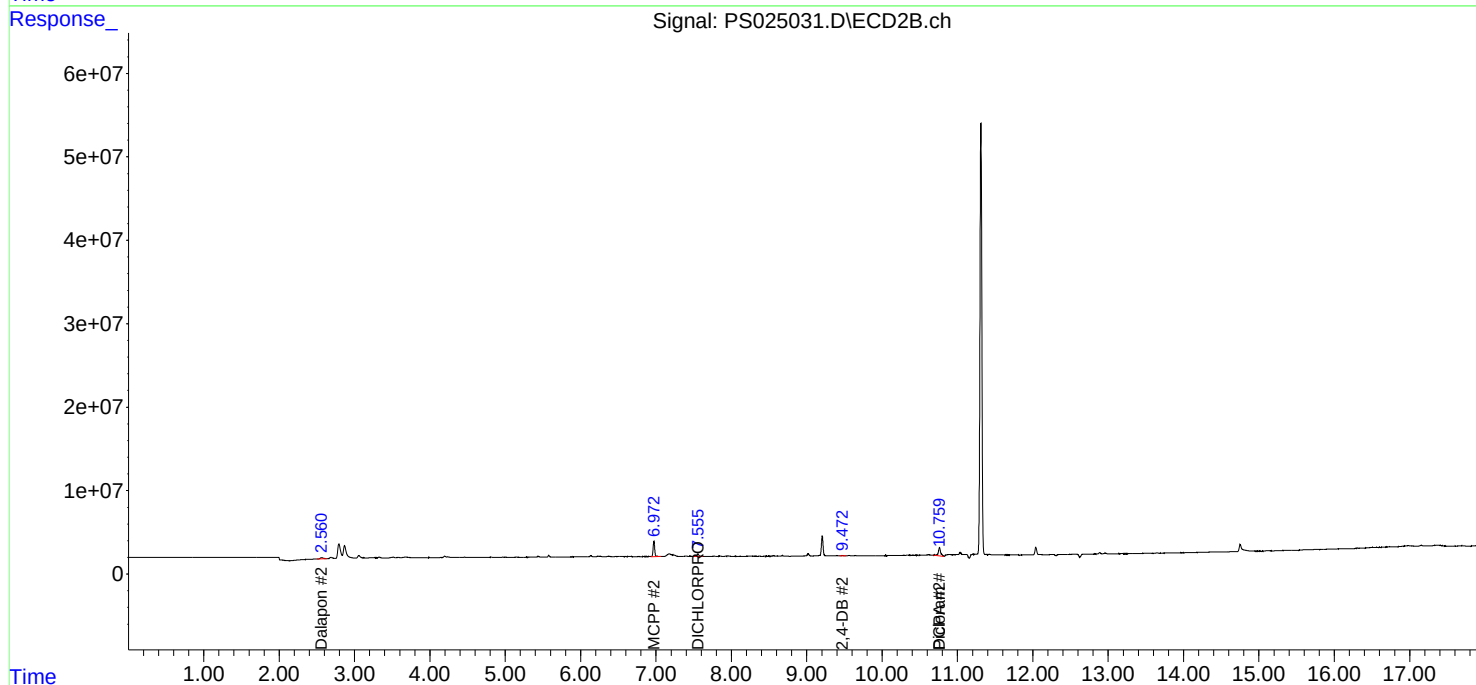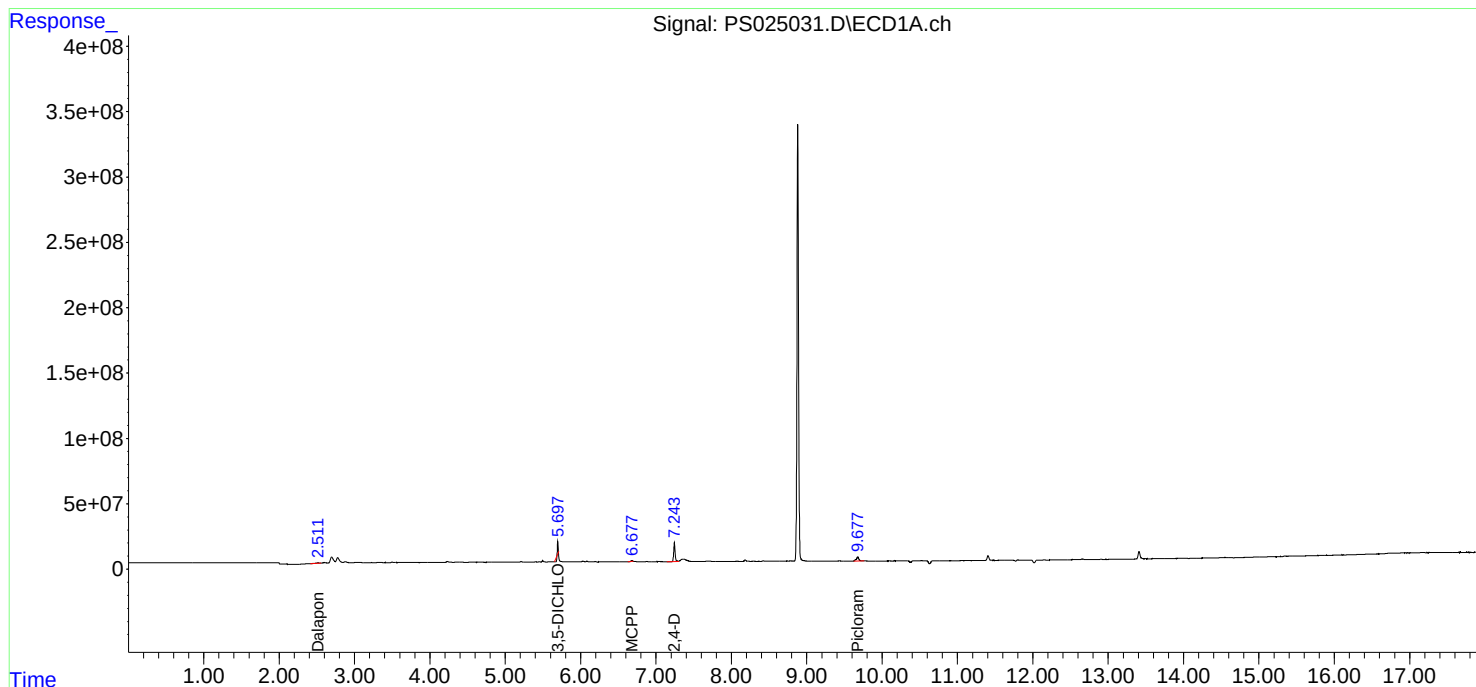


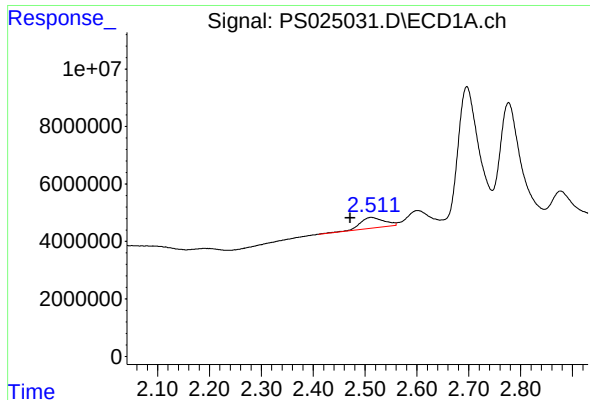

#1 Dalapon


R.T.: 2.512 min
Delta R.T.: 0.040 min
Response: 11609190
Conc: 4.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

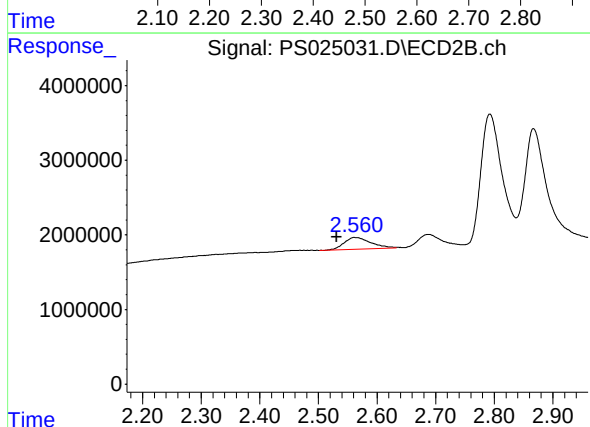


#1 Dalapon

R.T.: 2.561 min
Delta R.T.: 0.029 min
Response: 4962306
Conc: 4.33 ng/ml

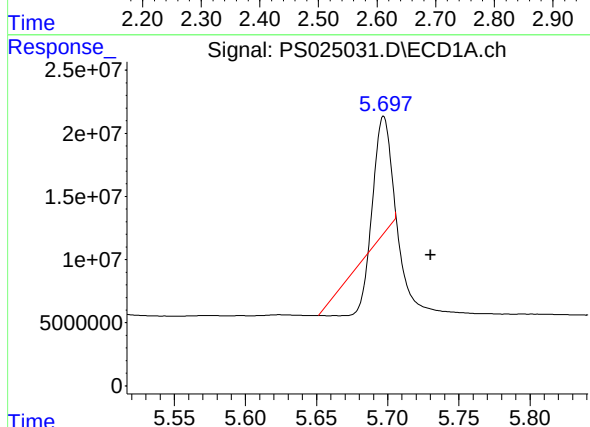


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.697 min
Delta R.T.: -0.033 min
Response: 30530984
Conc: 9.03 ng/ml

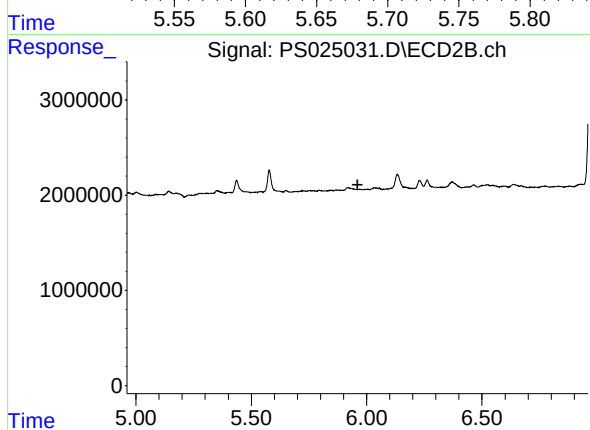

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

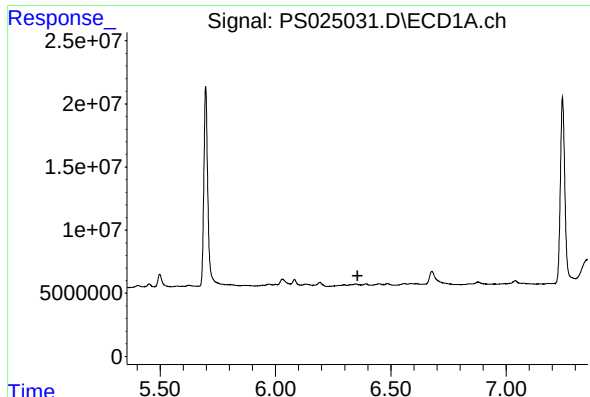

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.355 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

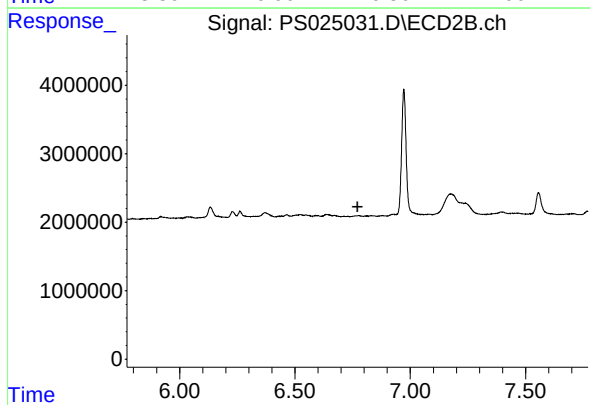


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

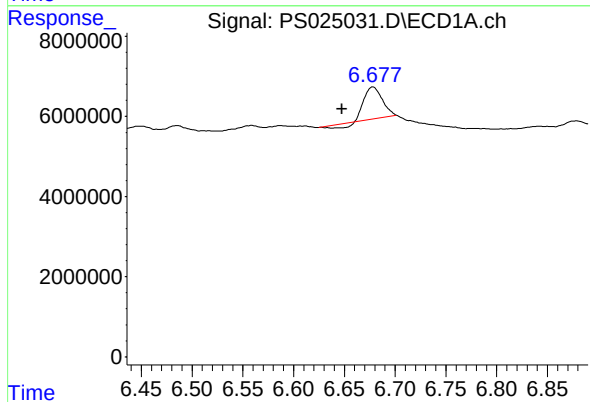


#6 MCPP

R.T.: 6.678 min
Delta R.T.: 0.030 min
Response: 9079618
Conc: 1.33 ug/ml

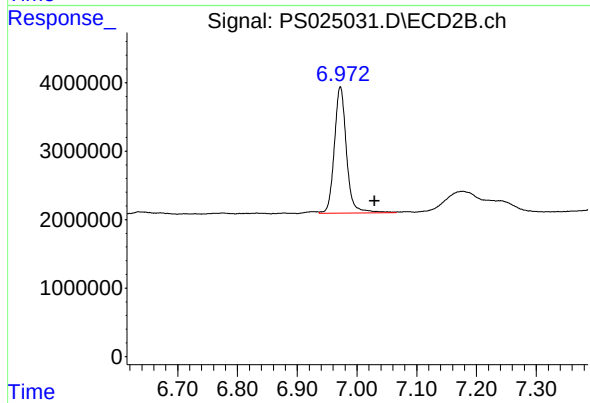

#6 MCPP


R.T.: 6.972 min
Delta R.T.: -0.057 min
Response: 26133149
Conc: 12.60 ug/ml

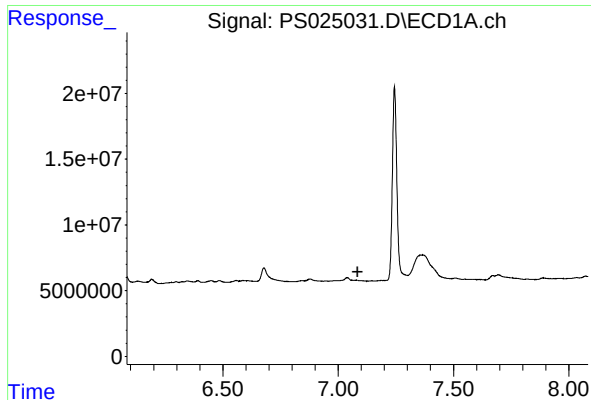

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

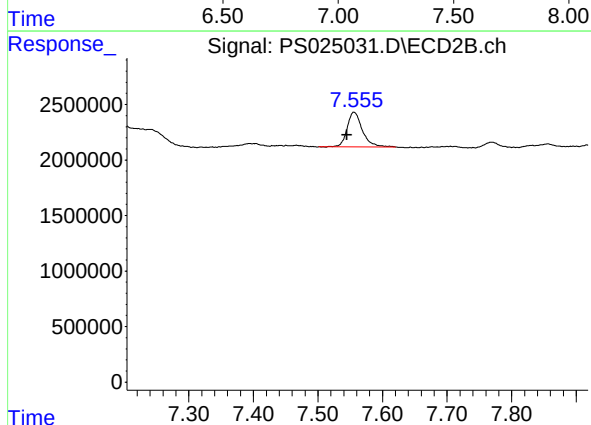


#8 DICHLORPROP

R.T.: 7.556 min
Delta R.T.: 0.011 min
Response: 5137263
Conc: 6.53 ng/ml

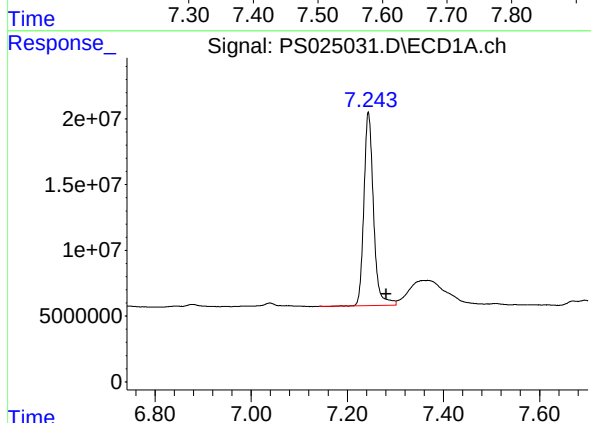


#9 2,4-D

R.T.: 7.244 min
Delta R.T.: -0.037 min
Response: 204017435
Conc: 67.17 ng/ml

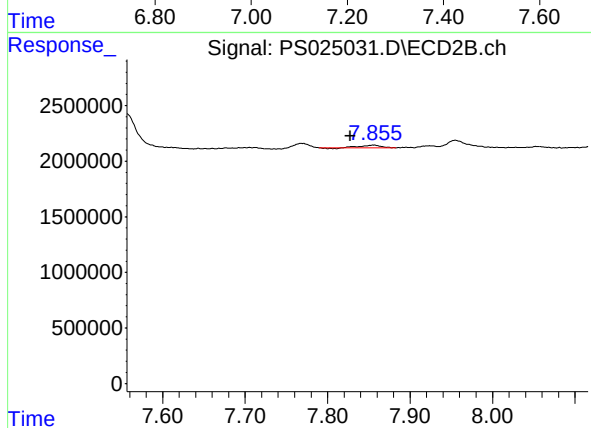

#9 2,4-D


R.T.: 7.856 min
Delta R.T.: 0.028 min
Response: 363122
Conc: N.D.

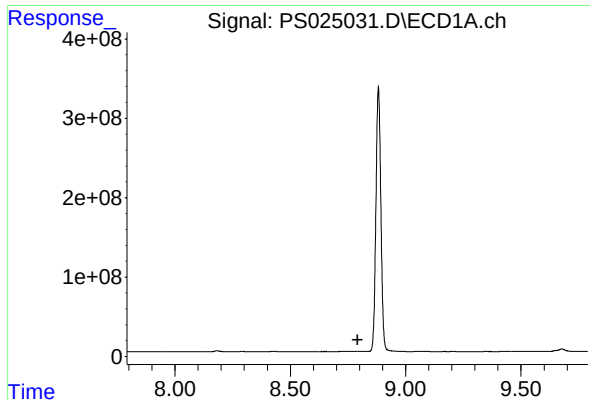

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

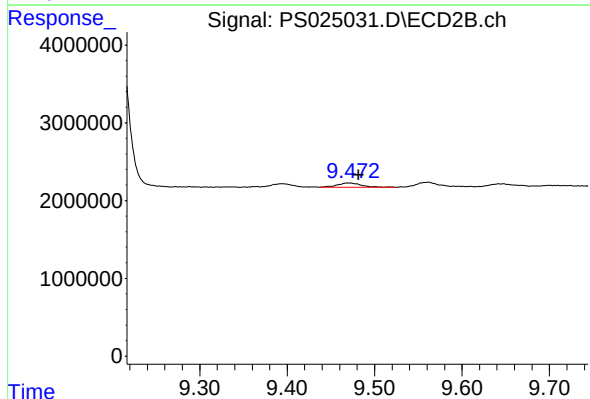


#13 2,4-DB

R.T.: 9.471 min
Delta R.T.: -0.010 min
Response: 1003500
Conc: 1.81 ng/ml

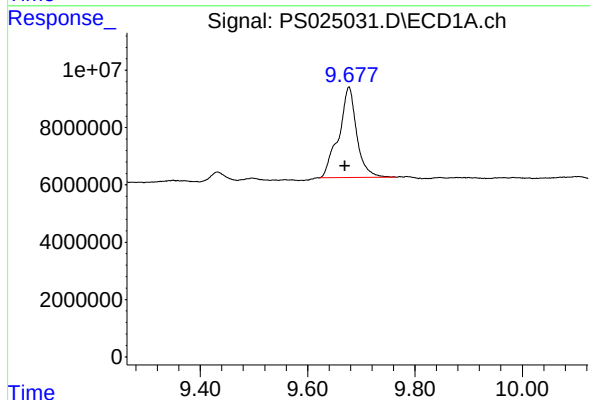


#15 Picloram

R.T.: 9.677 min
Delta R.T.: 0.007 min
Response: 73702883
Conc: 3.78 ng/ml

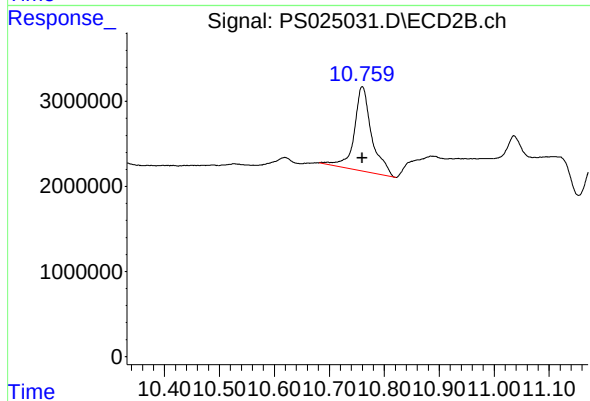

#15 Picloram


R.T.: 10.760 min
Delta R.T.: 0.000 min
Response: 21944826
Conc: 3.35 ng/ml

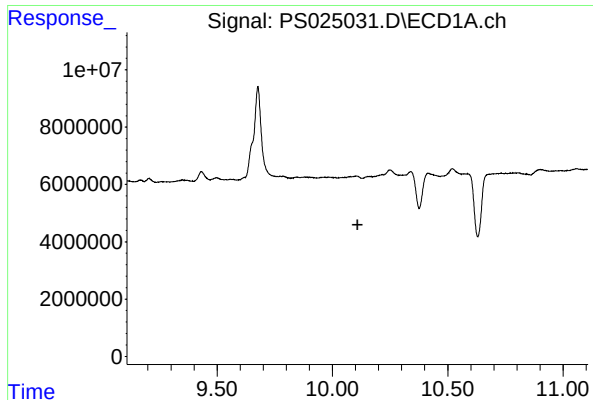

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

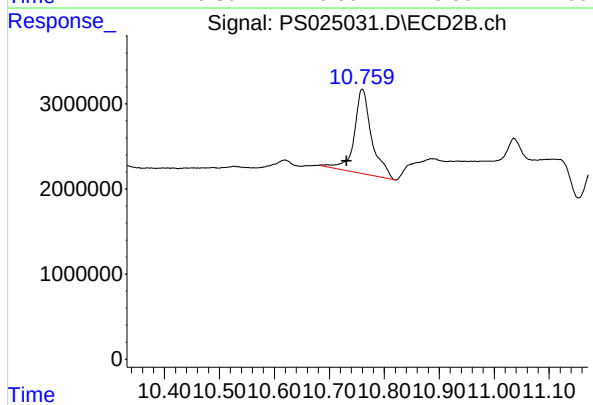

#16 DCPA

R.T.: 10.760 min
Delta R.T.: 0.028 min
Response: 21944826
Conc: 4.05 ng/ml